

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 00:28
 Operator : AR\AJ
 Sample : M2674-10
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TMR-DS-04-060921

Manual Integrations
 APPROVED

Ankita
 6/15/2021 2:40:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:26:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	8702459	15240048	15.829	16.166
28)	SA Decachlor...	10.221	11.427	14155123	22203950	19.974	22.292
Target Compounds							
2)	A alpha-BHC	5.188	6.112	2058524	90496192	2.799	73.189m#
13)	MA Dieldrin	7.594	8.689	26765102	8090365	38.181	8.908 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 00:28
Operator : AR\AJ
Sample : M2674-10
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TMR-DS-04-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:26:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

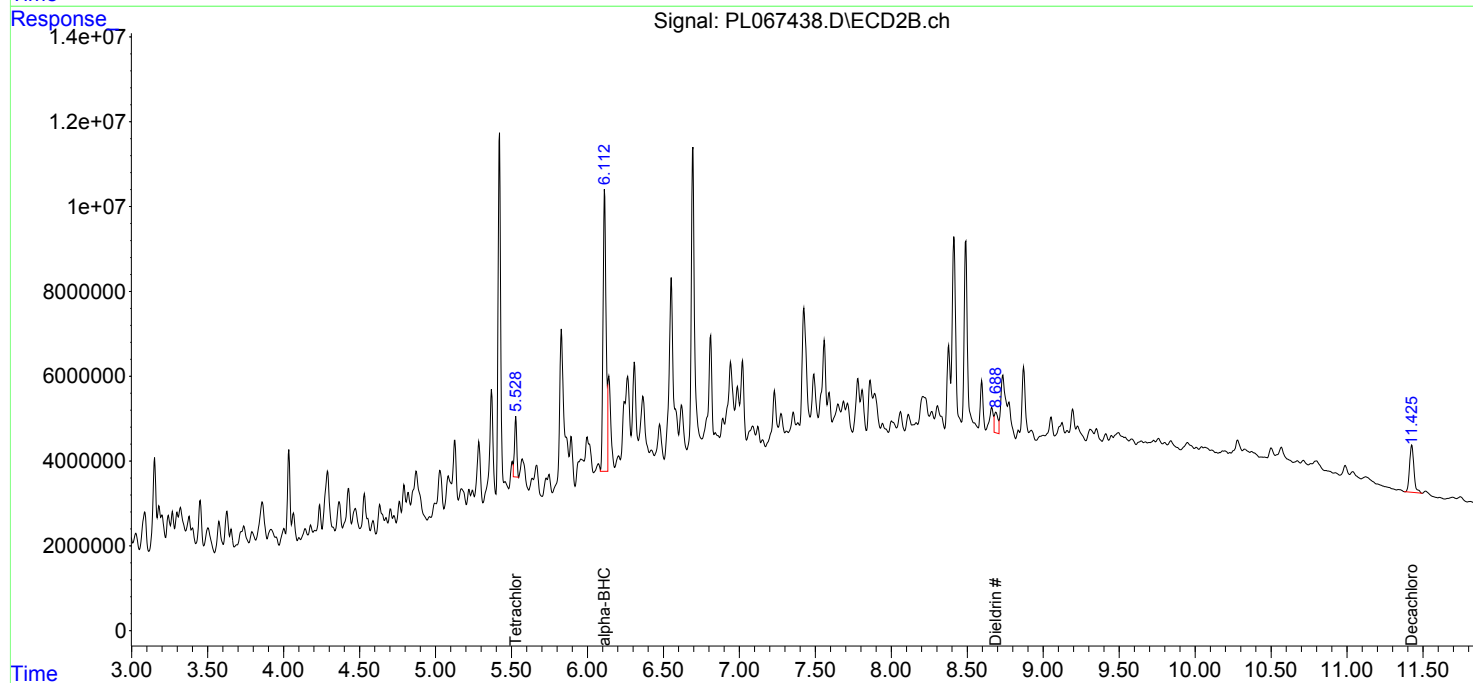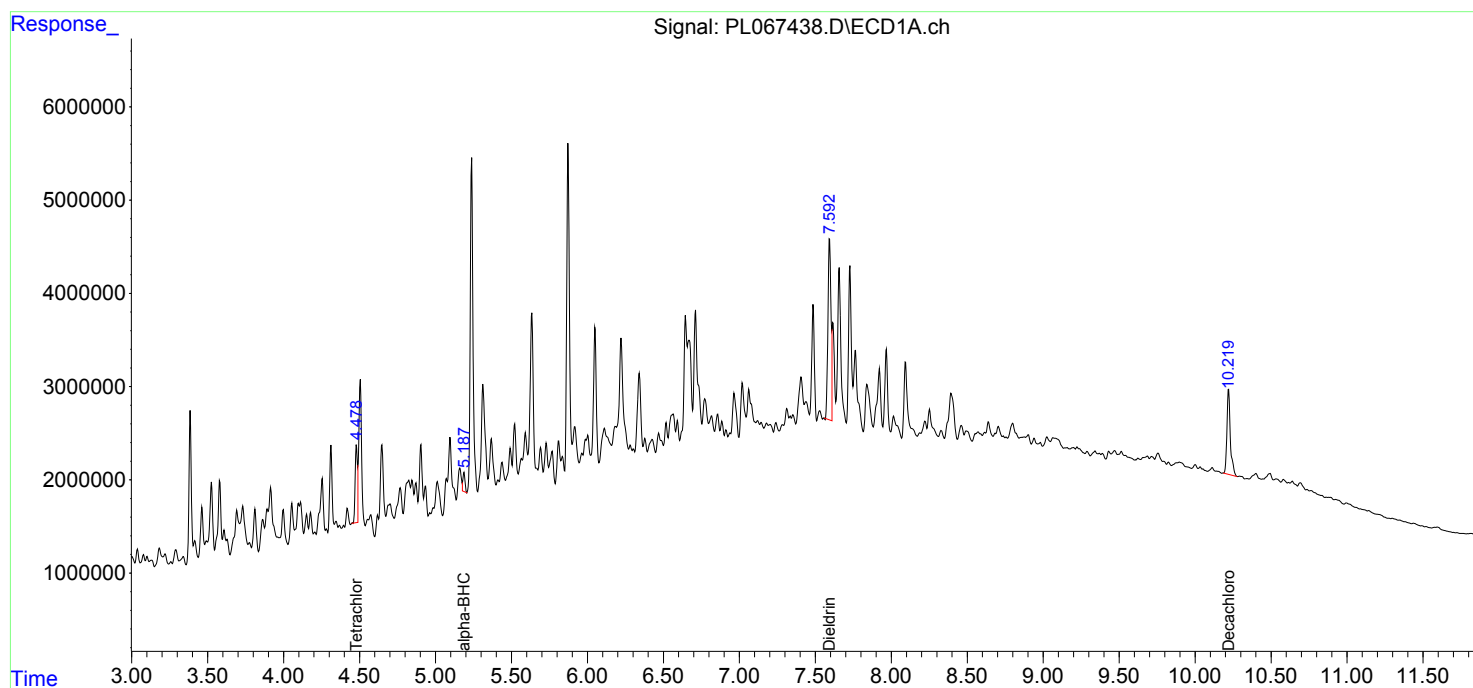

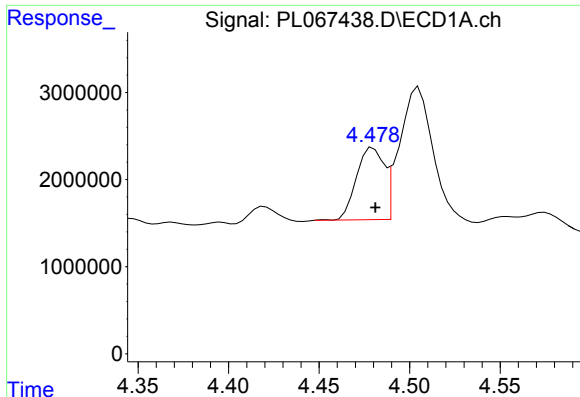


#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 8702459
Conc: 15.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TMR-DS-04-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:40 PM

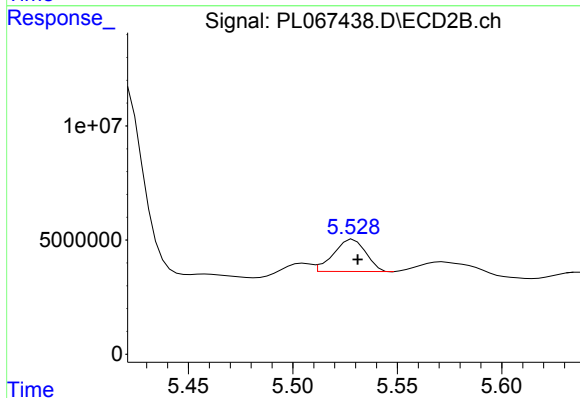


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 15240048
Conc: 16.17 ng/ml

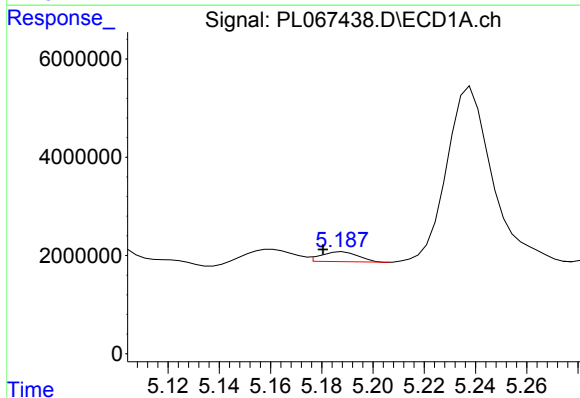


#2 alpha-BHC

R.T.: 5.188 min
Delta R.T.: 0.008 min
Response: 2058524
Conc: 2.80 ng/ml

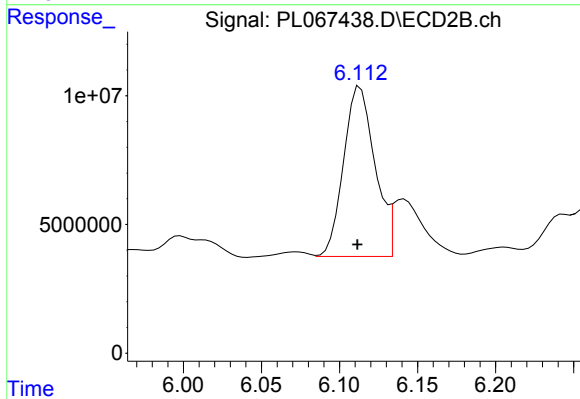

#2 alpha-BHC

R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 90496192
Conc: 73.19 ng/ml m

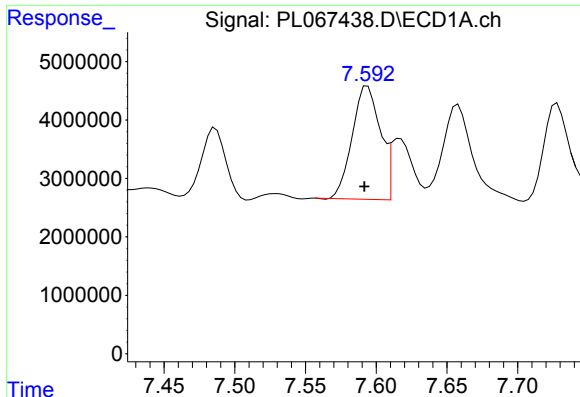


#13 Dieldrin

R.T.: 7.594 min
Delta R.T.: 0.002 min
Response: 26765102
Conc: 38.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TMR-DS-04-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:40 PM

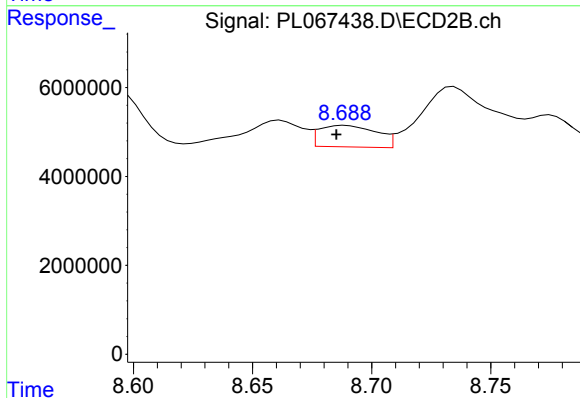


#13 Dieldrin

R.T.: 8.689 min
Delta R.T.: 0.004 min
Response: 8090365
Conc: 8.91 ng/ml

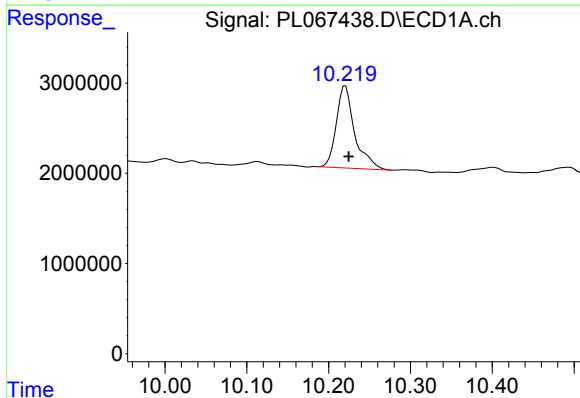

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 14155123
Conc: 19.97 ng/ml

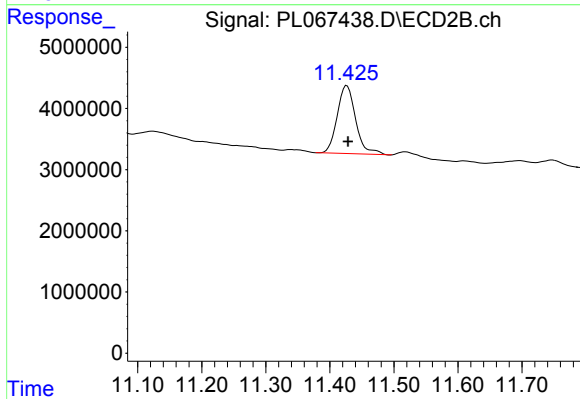

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 22203950
Conc: 22.29 ng/ml