

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
 Data File : PL075753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 10:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:42:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	5.345	0	176780	N.D. 0.078 #
5) MB	Aldrin	7.632f	0.000	3957614	0	4.820 N.D. #
7) B	delta-BHC	0.000	6.404	0	388575	N.D. 0.182 #
8) B	Heptachlo...	8.113	0.000	5564200	0	7.198 N.D. #
9) A	Endosulfan I	0.000	7.492f	0	57897	N.D. 0.035 #
10) B	gamma-Chl...	8.379	0.000	4637774	0	5.972 N.D. #
11) B	alpha-Chl...	8.494f	7.388f	1059832	908168	1.390 0.497 #
15) B	Endosulfa...	9.301	0.000	517757	0	0.832 N.D. #
19) B	Endosulfa...	0.000	8.766	0	230126	N.D. 0.157 #
21) B	Endrin ke...	10.182	0.000	489555	0	0.696 N.D. #
24)	Chlordane-2	7.632	6.633	3957614	1826924	128.677 27.320 #
25)	Chlordane-3	8.379	0.000	4637774	0	44.917 N.D. #
26)	Chlordane-4	8.494f	7.388f	1059832	908168	8.368 4.934 #
27)	Chlordane-5	0.000	8.112	0	429293	N.D. 9.042 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
Data File : PL075753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 10:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:42:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

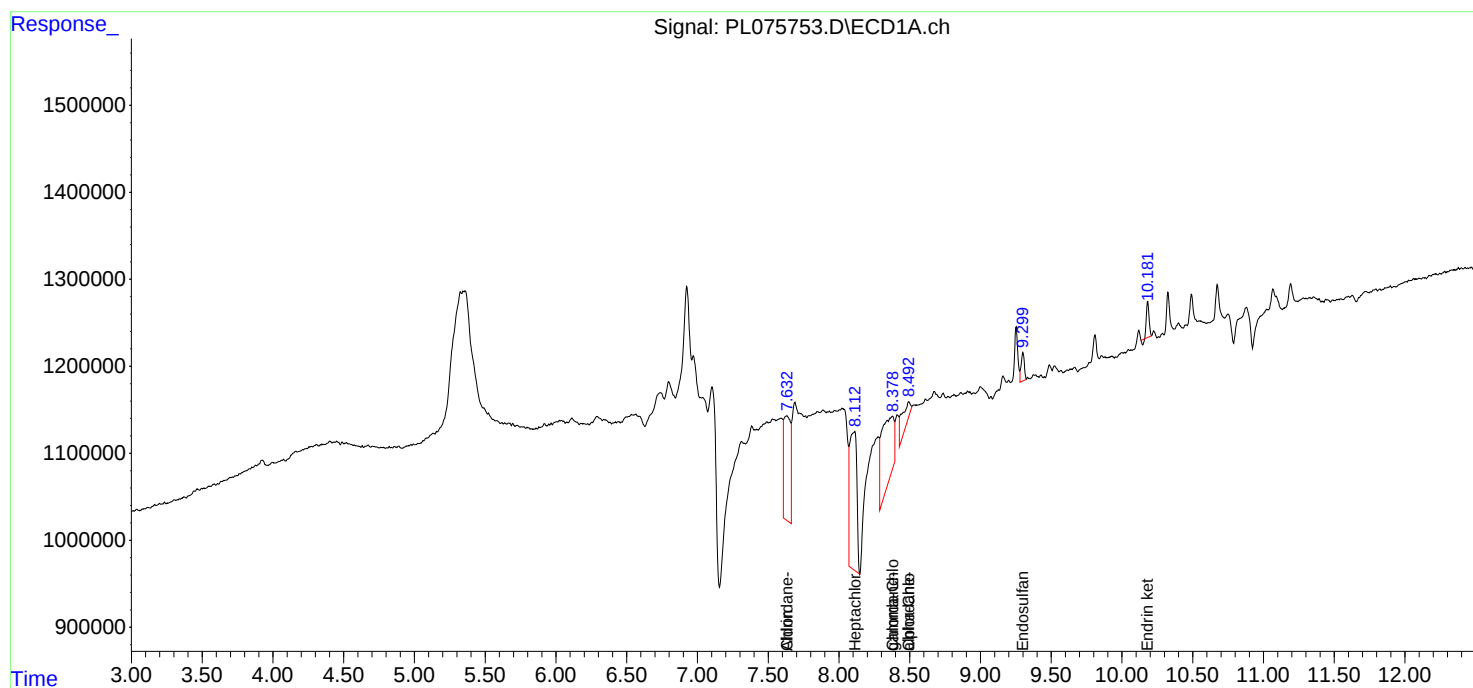


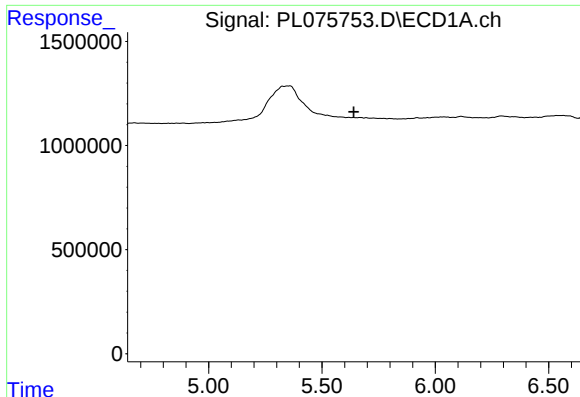

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.641 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

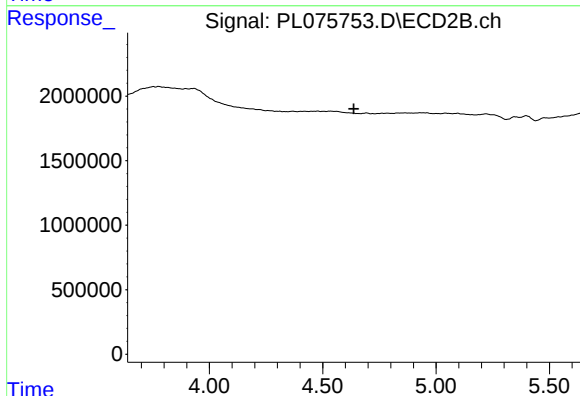


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

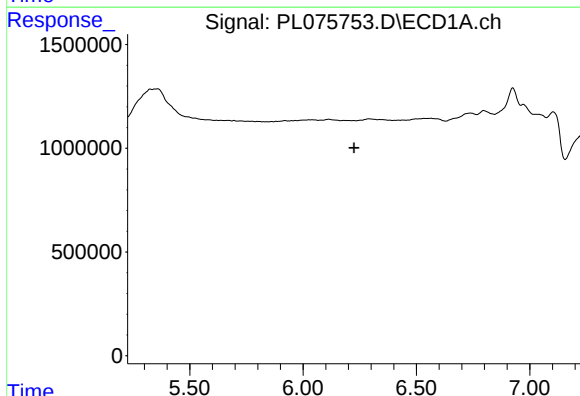


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

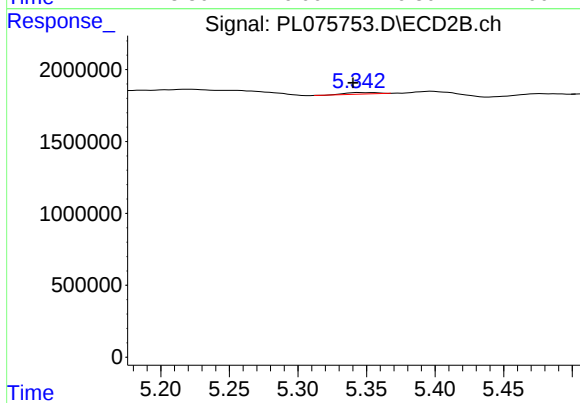

#2 alpha-BHC


R.T.: 5.345 min
Delta R.T.: 0.005 min
Response: 176780
Conc: 0.08 ng/ml

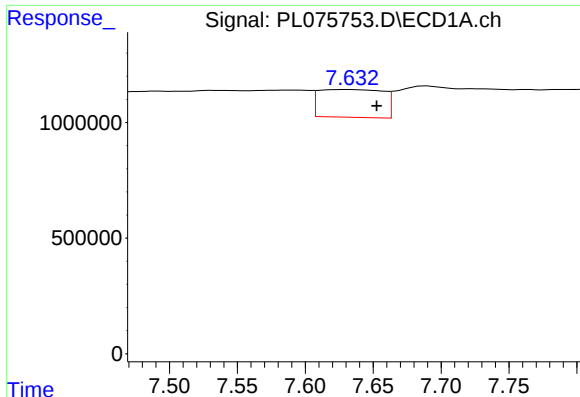

#5 Aldrin


R.T.: 7.632 min
Delta R.T.: -0.020 min
Response: 3957614
Conc: 4.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

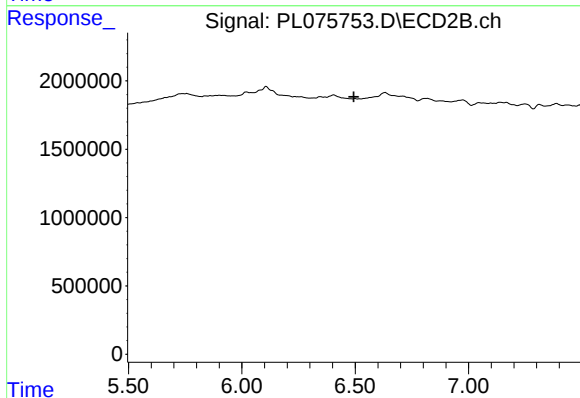


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.493 min
Response: 0
Conc: N.D.

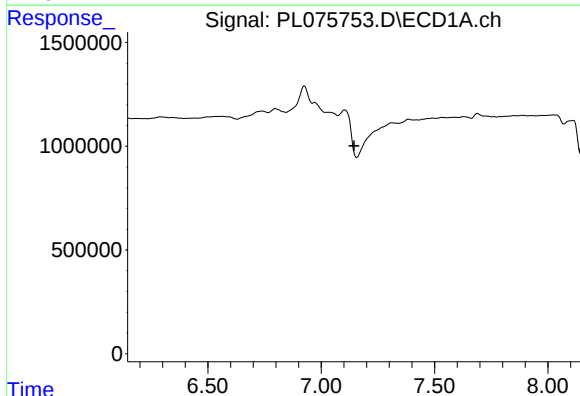


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

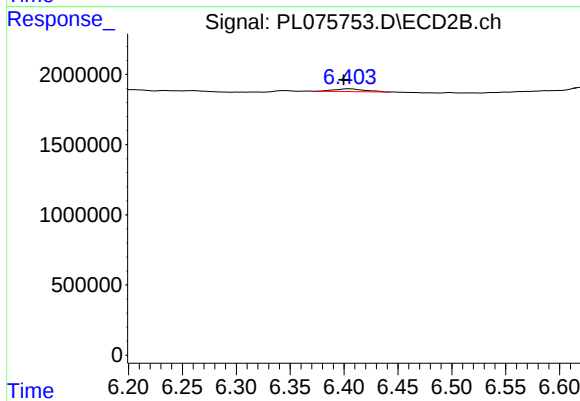

#7 delta-BHC


R.T.: 6.404 min
Delta R.T.: 0.005 min
Response: 388575
Conc: 0.18 ng/ml

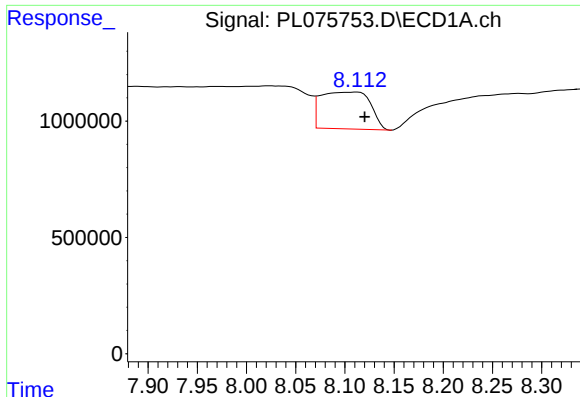

#8 Heptachlor epoxide


R.T.: 8.113 min
Delta R.T.: -0.007 min
Response: 5564200
Conc: 7.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

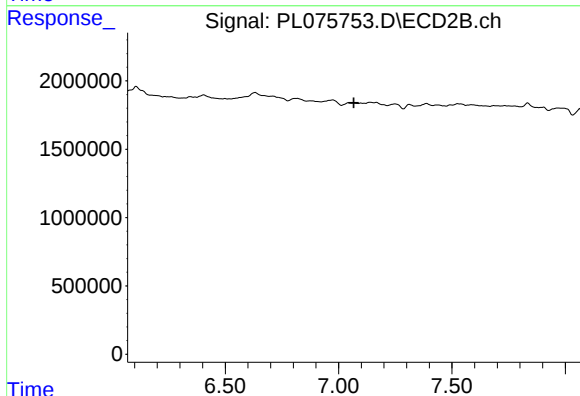


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

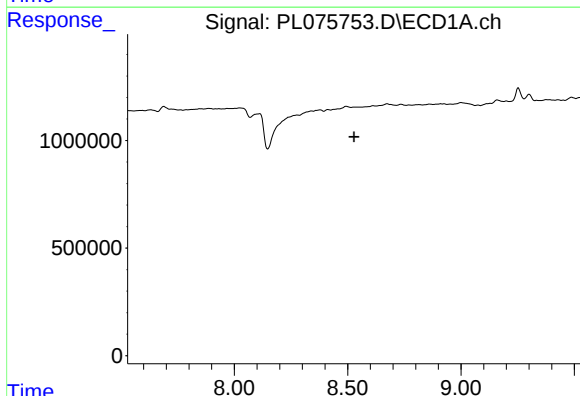


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.528 min
Response: 0
Conc: N.D.

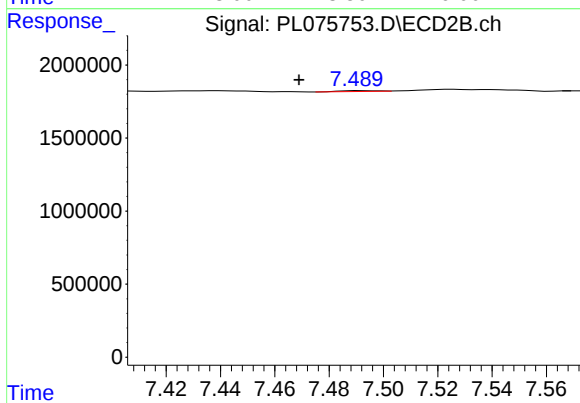

#9 Endosulfan I


R.T.: 7.492 min
Delta R.T.: 0.023 min
Response: 57897
Conc: 0.03 ng/ml

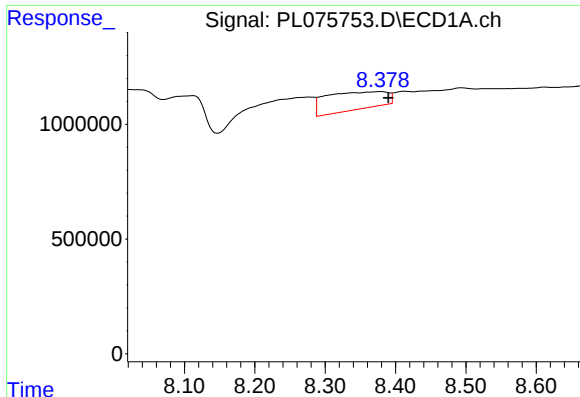

#10 gamma-Chlordane


R.T.: 8.379 min
Delta R.T.: -0.011 min
Response: 4637774
Conc: 5.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

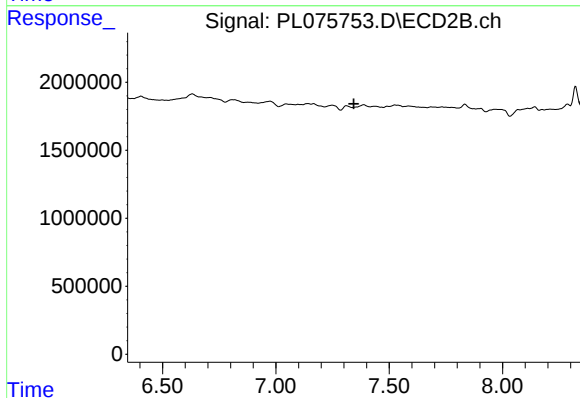


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

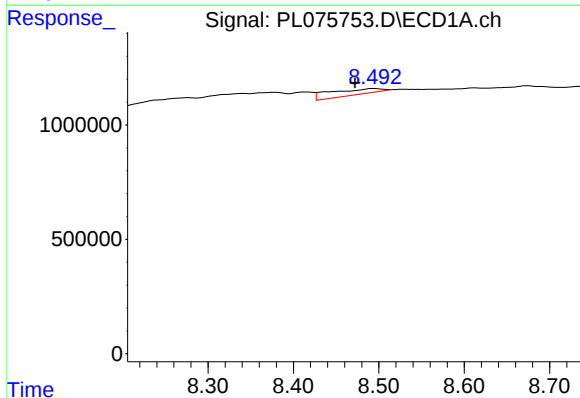


#11 alpha-Chlordane

R.T.: 8.494 min
Delta R.T.: 0.022 min
Response: 1059832
Conc: 1.39 ng/ml

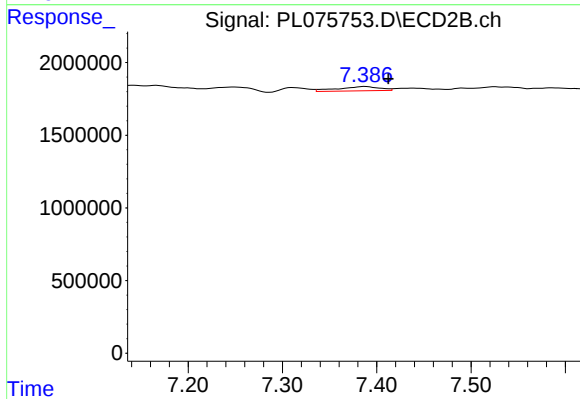

#11 alpha-Chlordane


R.T.: 7.388 min
Delta R.T.: -0.025 min
Response: 908168
Conc: 0.50 ng/ml

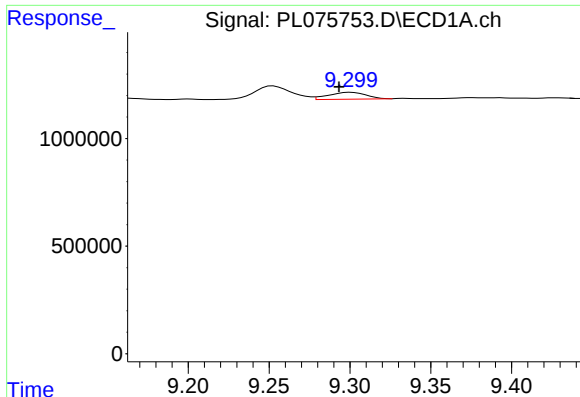

#15 Endosulfan II


R.T.: 9.301 min
Delta R.T.: 0.007 min
Response: 517757
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

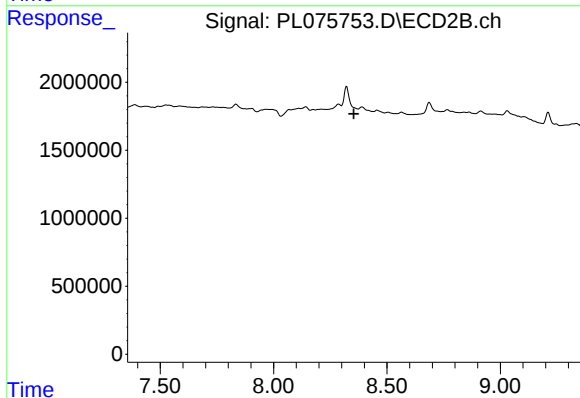


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

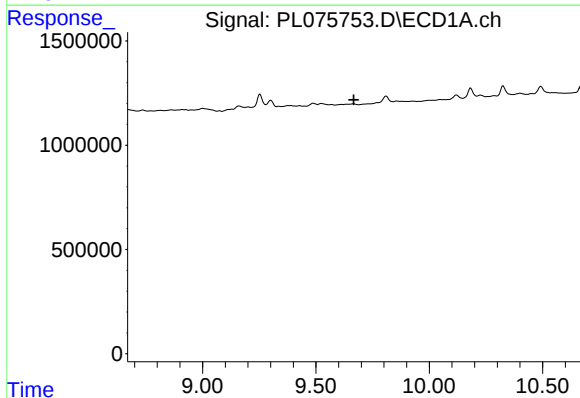


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.666 min
Response: 0
Conc: N.D.

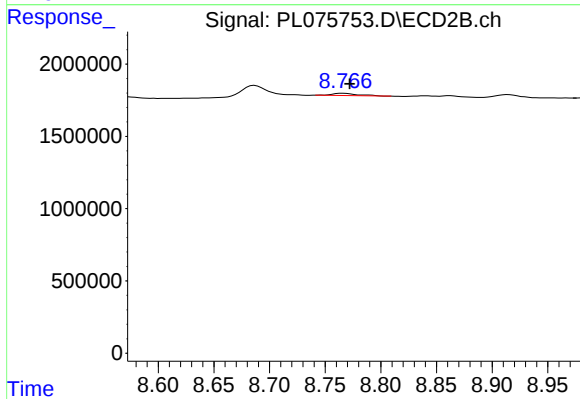

#19 Endosulfan Sulfate


R.T.: 8.766 min
Delta R.T.: -0.006 min
Response: 230126
Conc: 0.16 ng/ml

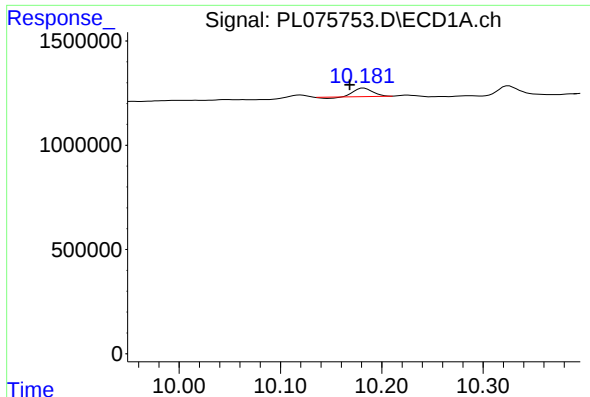

#21 Endrin ketone


R.T.: 10.182 min
Delta R.T.: 0.014 min
Response: 489555
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

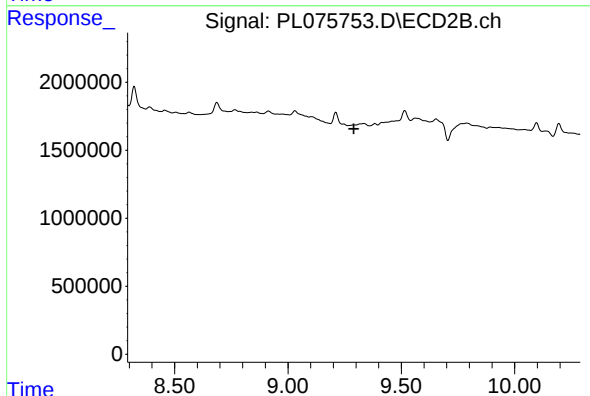


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

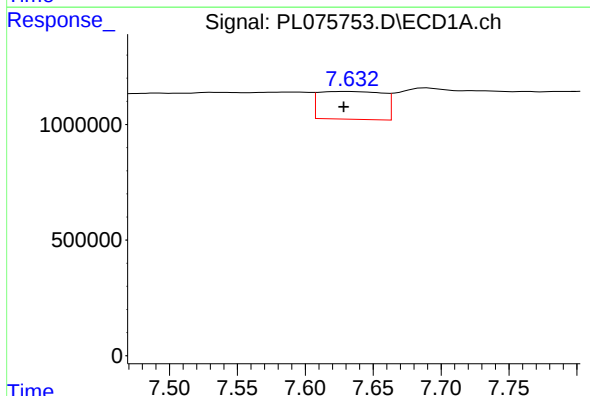


#24 Chlordane-2

R.T.: 7.632 min
Delta R.T.: 0.004 min
Response: 3957614
Conc: 128.68 ng/ml

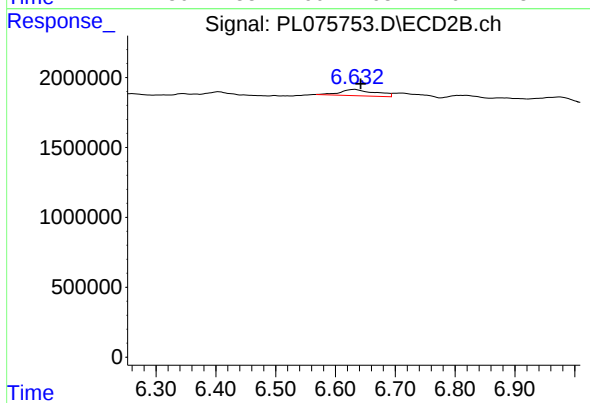

#24 Chlordane-2


R.T.: 6.633 min
Delta R.T.: -0.010 min
Response: 1826924
Conc: 27.32 ng/ml

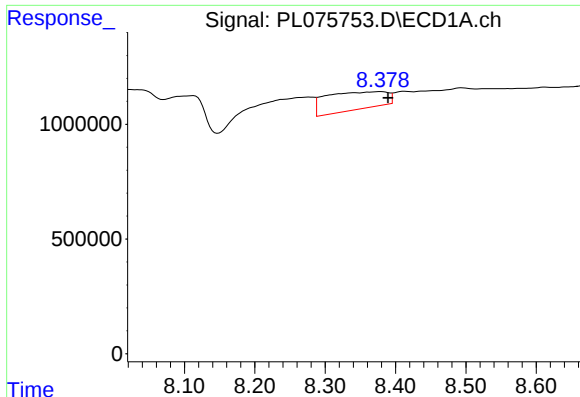

#25 Chlordane-3


R.T.: 8.379 min
Delta R.T.: -0.010 min
Response: 4637774
Conc: 44.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

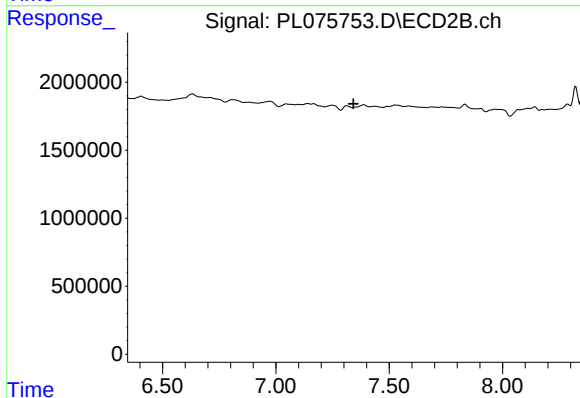


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

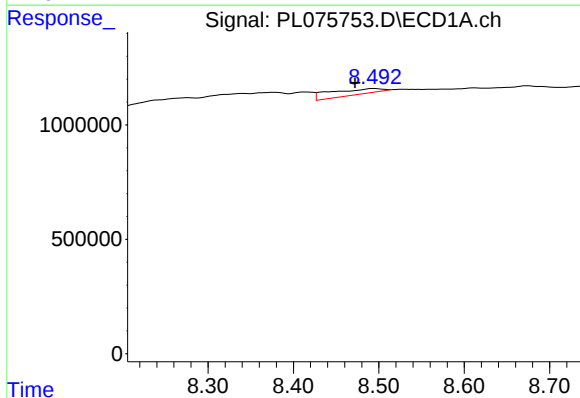


#26 Chlordane-4

R.T.: 8.494 min
Delta R.T.: 0.022 min
Response: 1059832
Conc: 8.37 ng/ml

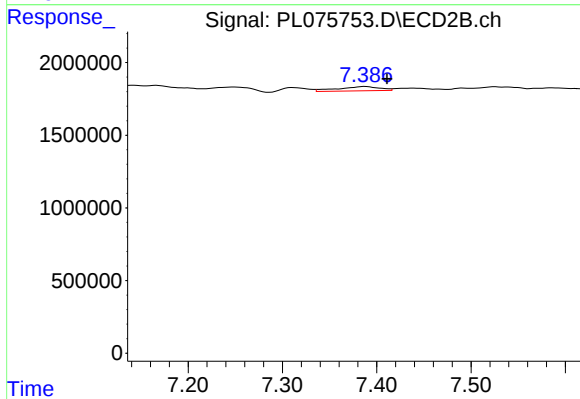

#26 Chlordane-4


R.T.: 7.388 min
Delta R.T.: -0.023 min
Response: 908168
Conc: 4.93 ng/ml

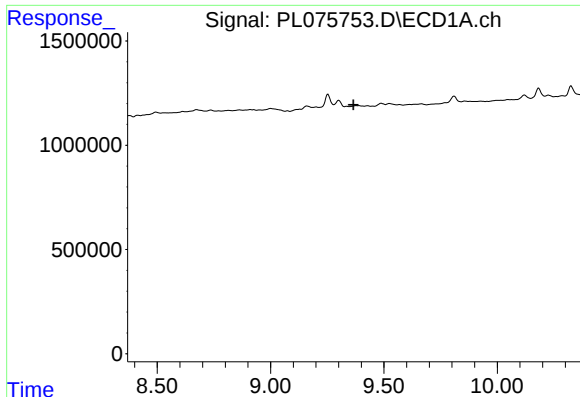

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

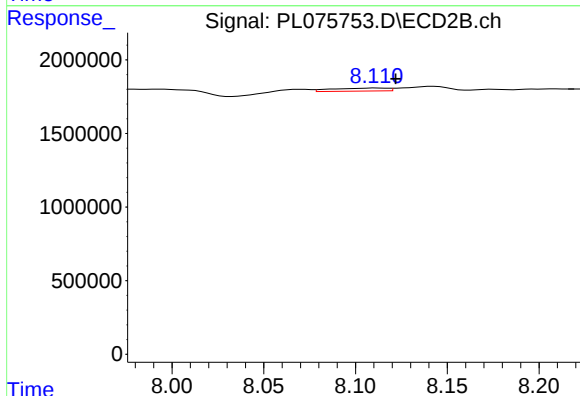


#27 Chlordane-5

R.T.: 8.112 min
Delta R.T.: -0.010 min
Response: 429293
Conc: 9.04 ng/ml

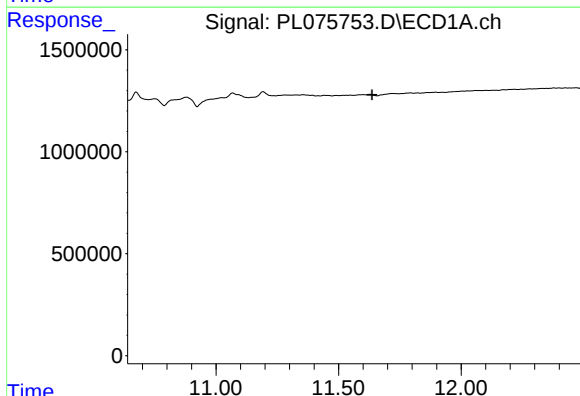

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.636 min
Response: 0
Conc: N.D.

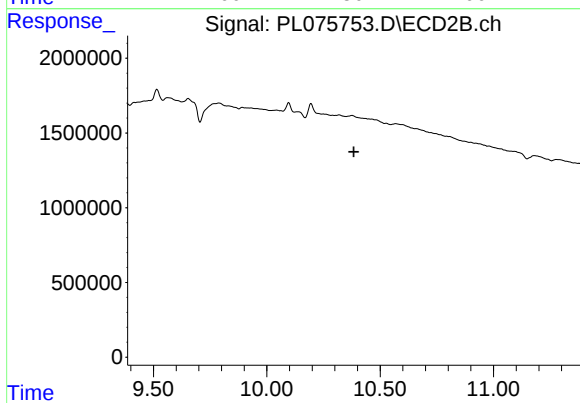

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.383 min
Response: 0
Conc: N.D.