

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
 Data File : PL075770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 16:40
 Operator : AR\AJ
 Sample : N3329-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:46:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	14396105	35135882	21.331	20.937
28)	SA Decachlor...	11.637	10.379	12188595	24728578	19.909	17.551
Target Compounds							
5)	MB Aldrin	0.000	6.485	0	202775	N.D.	0.103 #
7)	B delta-BHC	0.000	6.403	0	533155	N.D.	0.249 #
9)	A Endosulfan I	8.533	0.000	276897	0	0.396	N.D. #
10)	B gamma-Chl...	8.378	7.332	1531217	256409	1.972	0.140 #
11)	B alpha-Chl...	8.500f	7.415	756866	205736	0.992	0.113 #
15)	B Endosulfa...	9.304	8.366	450046	366614	0.723	0.256 #
19)	B Endosulfa...	9.656	8.763	732160	552466	1.169	0.376 #
21)	B Endrin ke...	10.185f	0.000	628677	0	0.894	N.D. #
25)	Chlordane-3	8.378	7.332	1531217	256409	14.830	1.491 #
26)	Chlordane-4	8.500f	7.415	756866	205736	5.976	1.118 #
27)	Chlordane-5	0.000	8.108	0	86732	N.D.	1.827 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
Data File : PL075770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 16:40
Operator : AR\AJ
Sample : N3329-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:46:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

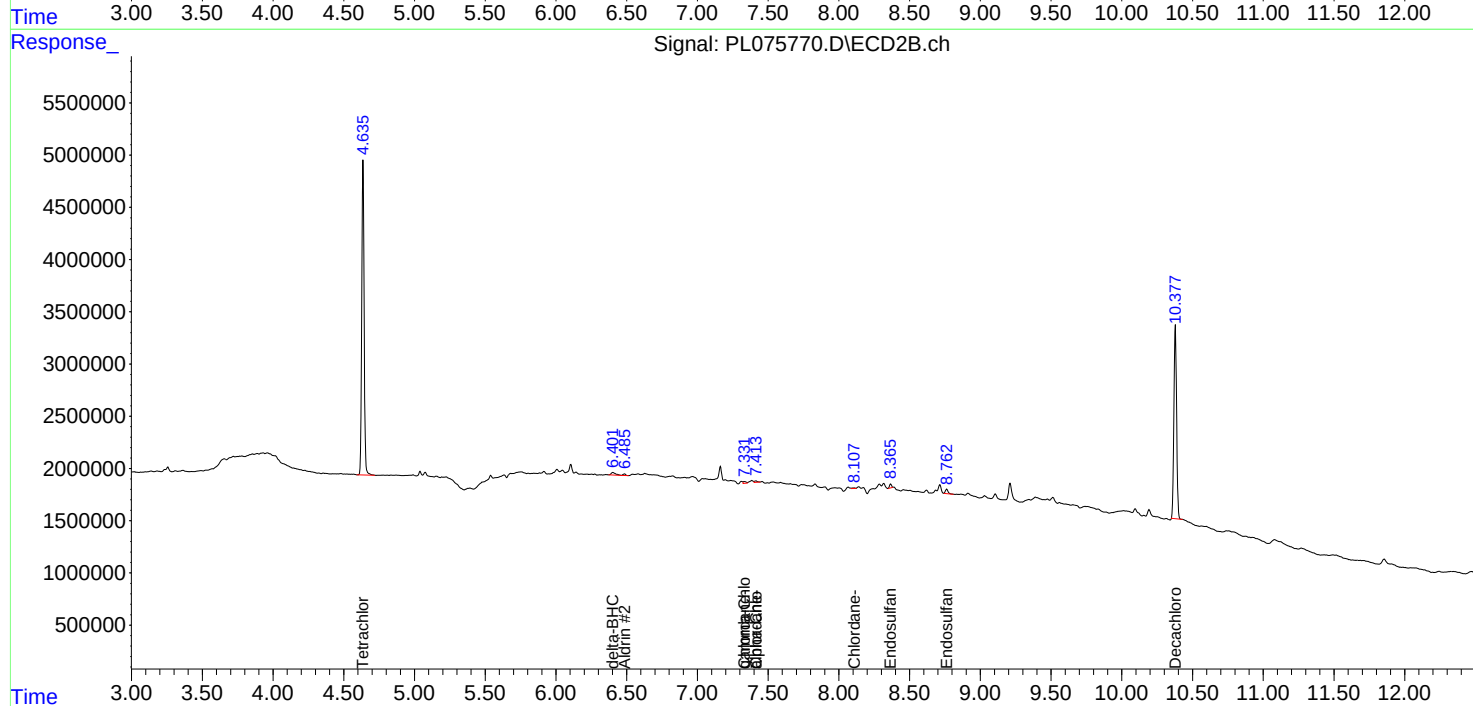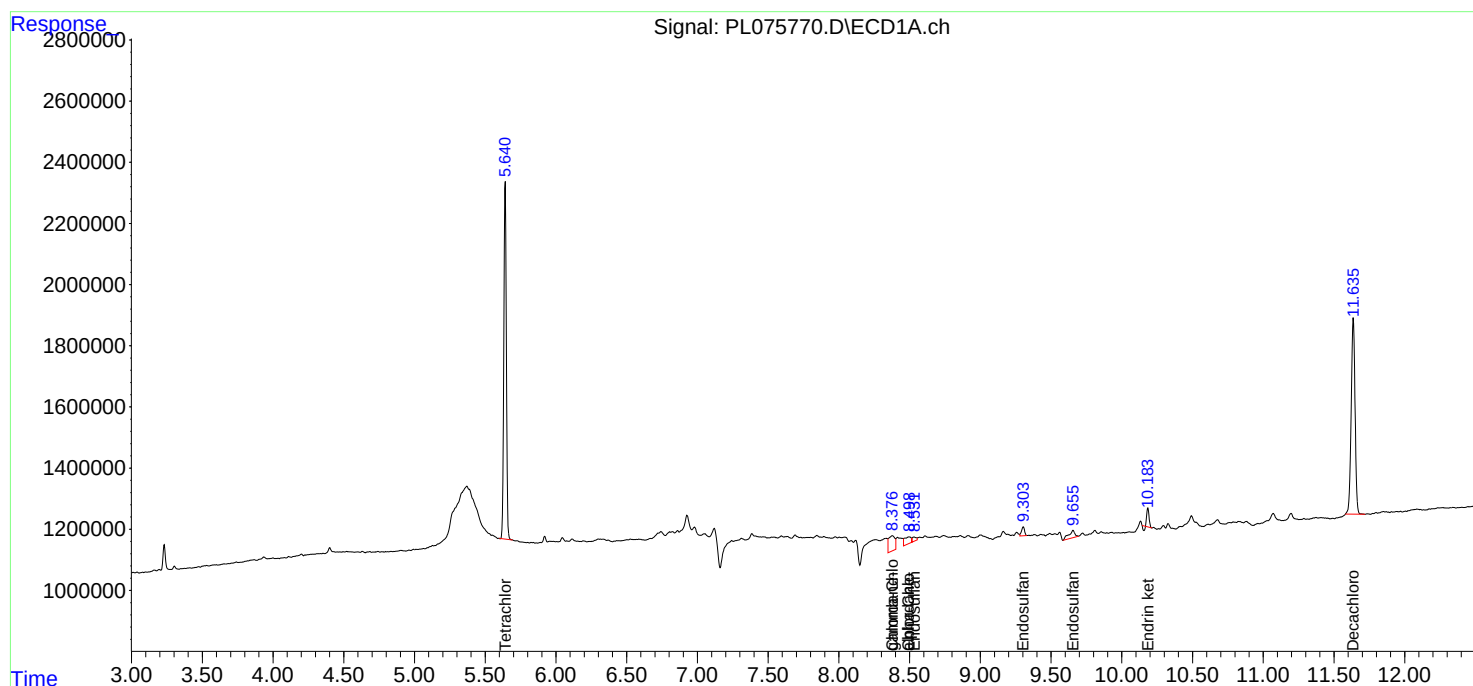


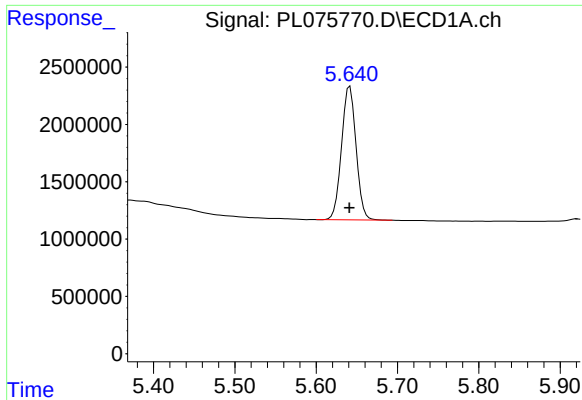

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 14396105
Conc: 21.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

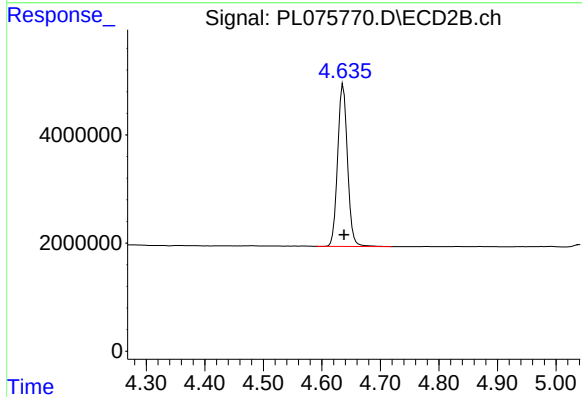


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.001 min
Response: 35135882
Conc: 20.94 ng/ml

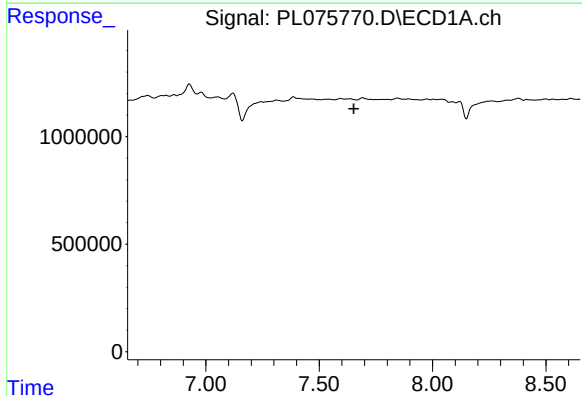


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.652 min
Response: 0
Conc: N.D.

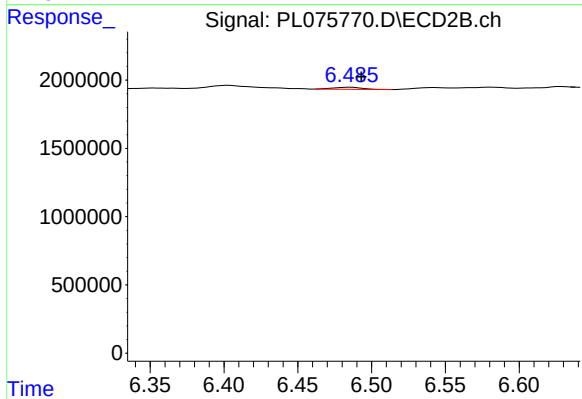

#5 Aldrin


R.T.: 6.485 min
Delta R.T.: -0.008 min
Response: 202775
Conc: 0.10 ng/ml

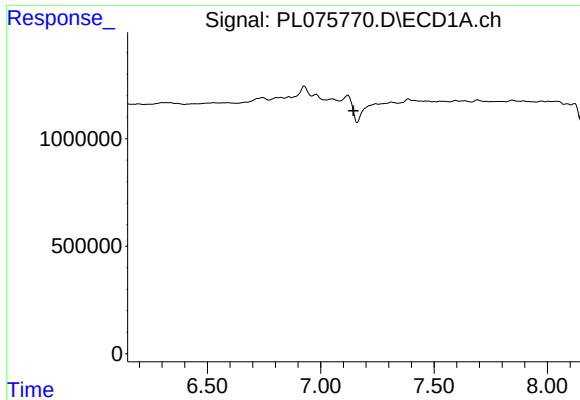

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

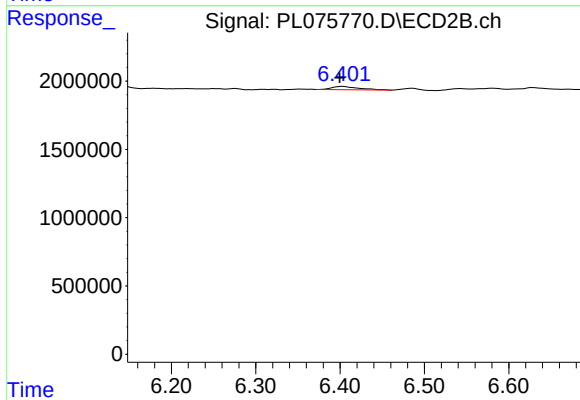


#7 delta-BHC

R.T.: 6.403 min
Delta R.T.: 0.003 min
Response: 533155
Conc: 0.25 ng/ml

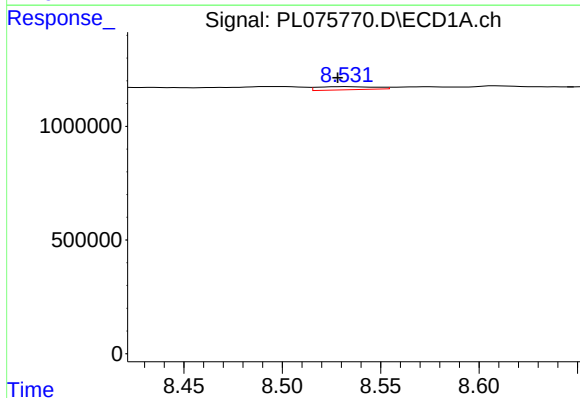


#9 Endosulfan I

R.T.: 8.533 min
Delta R.T.: 0.005 min
Response: 276897
Conc: 0.40 ng/ml

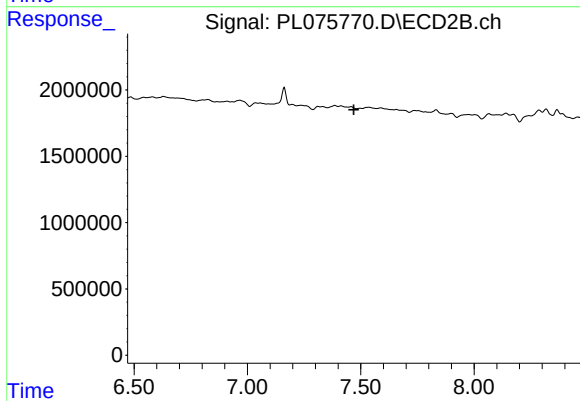

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.469 min
Response: 0
Conc: N.D.

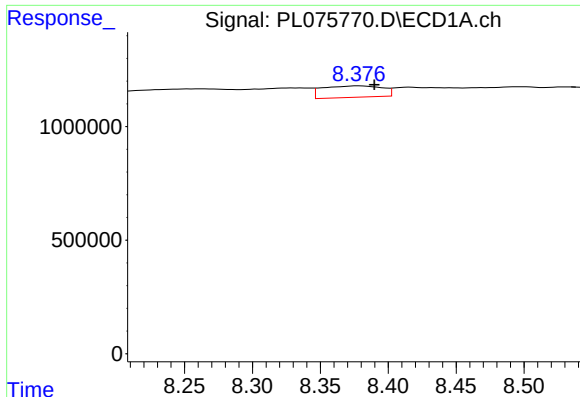

#10 gamma-Chlordane


R.T.: 8.378 min
Delta R.T.: -0.012 min
Response: 1531217
Conc: 1.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

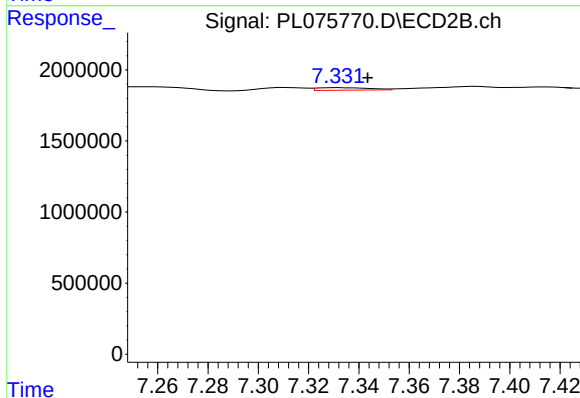


#10 gamma-Chlordane

R.T.: 7.332 min
Delta R.T.: -0.012 min
Response: 256409
Conc: 0.14 ng/ml

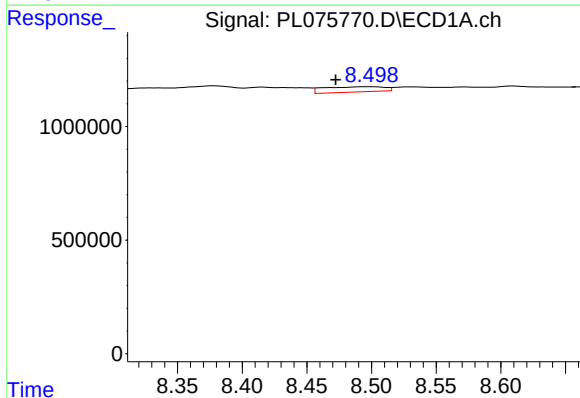


#11 alpha-Chlordane

R.T.: 8.500 min
Delta R.T.: 0.028 min
Response: 756866
Conc: 0.99 ng/ml

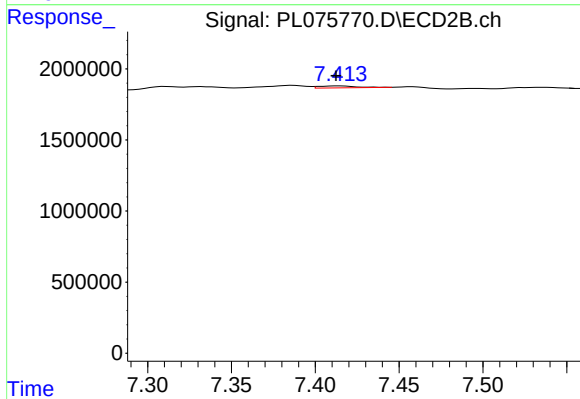

#11 alpha-Chlordane


R.T.: 7.415 min
Delta R.T.: 0.002 min
Response: 205736
Conc: 0.11 ng/ml

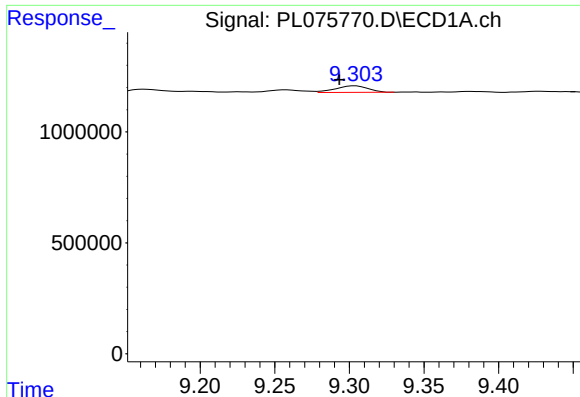

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 450046
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

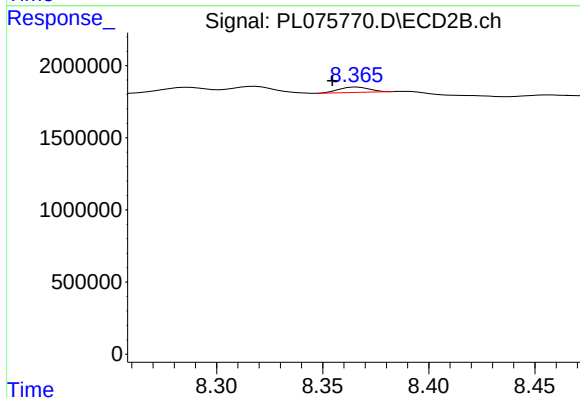


#15 Endosulfan II

R.T.: 8.366 min
Delta R.T.: 0.012 min
Response: 366614
Conc: 0.26 ng/ml

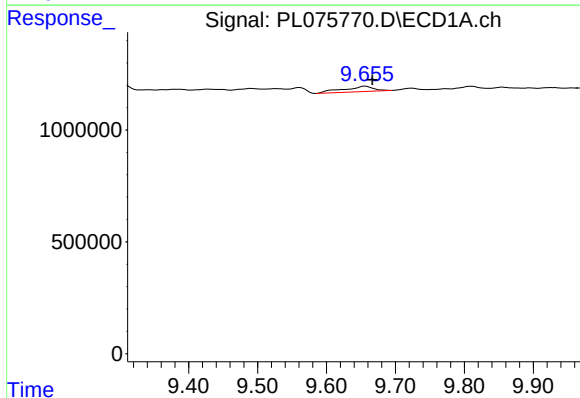


#19 Endosulfan Sulfate

R.T.: 9.656 min
Delta R.T.: -0.010 min
Response: 732160
Conc: 1.17 ng/ml

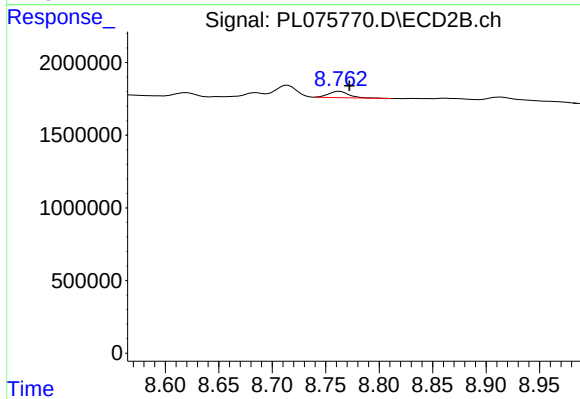

#19 Endosulfan Sulfate


R.T.: 8.763 min
Delta R.T.: -0.009 min
Response: 552466
Conc: 0.38 ng/ml

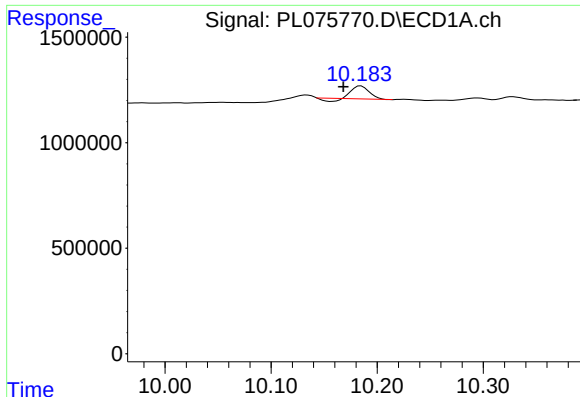

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.016 min
Response: 628677
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

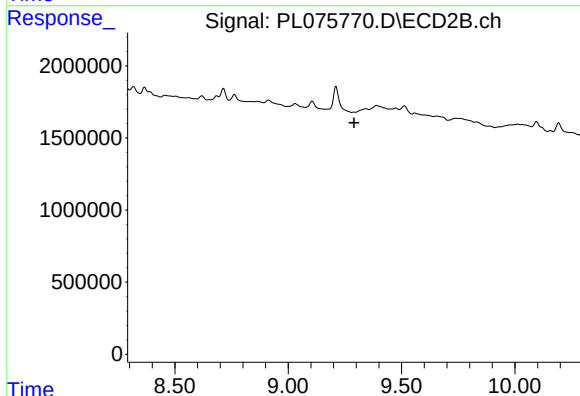


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

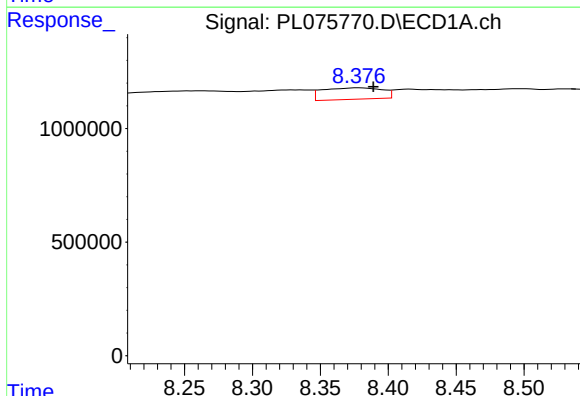


#25 Chlordane-3

R.T.: 8.378 min
Delta R.T.: -0.011 min
Response: 1531217
Conc: 14.83 ng/ml

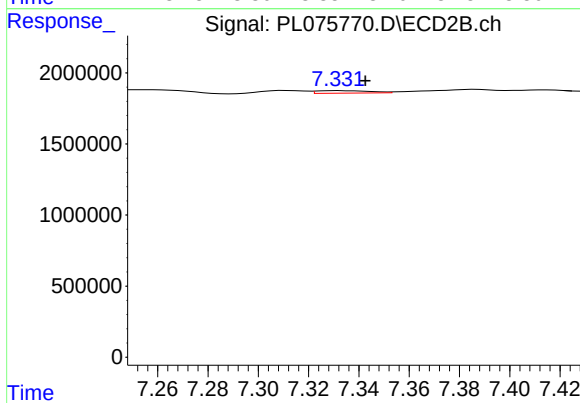

#25 Chlordane-3


R.T.: 7.332 min
Delta R.T.: -0.011 min
Response: 256409
Conc: 1.49 ng/ml

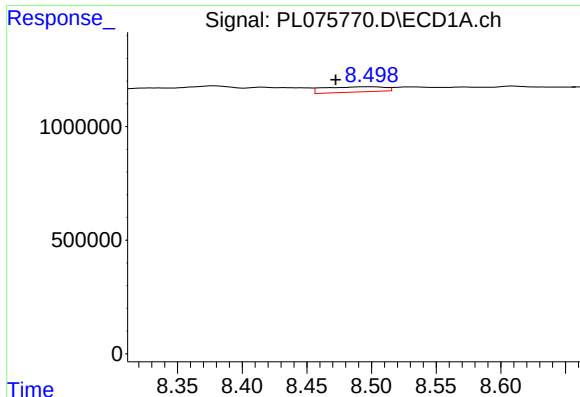

#26 Chlordane-4


R.T.: 8.500 min
Delta R.T.: 0.028 min
Response: 756866
Conc: 5.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

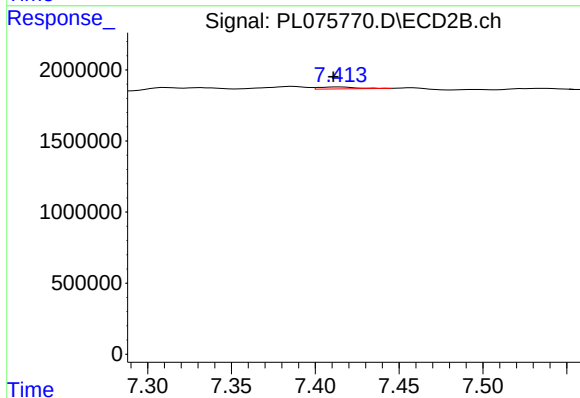


#26 Chlordane-4

R.T.: 7.415 min
Delta R.T.: 0.004 min
Response: 205736
Conc: 1.12 ng/ml

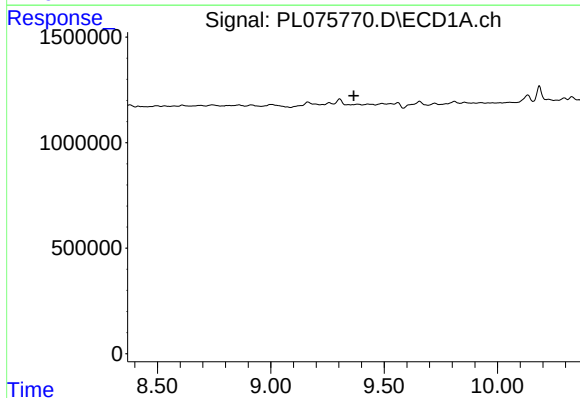


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

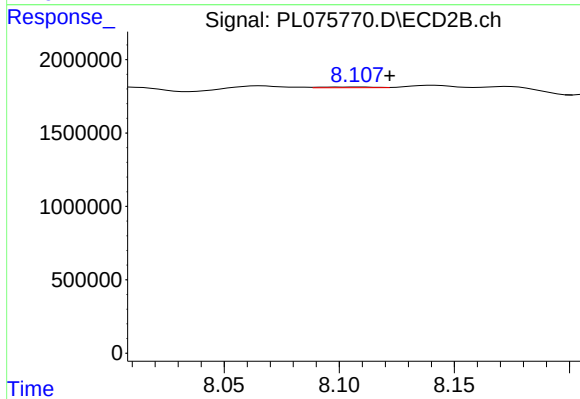

#27 Chlordane-5


R.T.: 8.108 min
Delta R.T.: -0.013 min
Response: 86732
Conc: 1.83 ng/ml

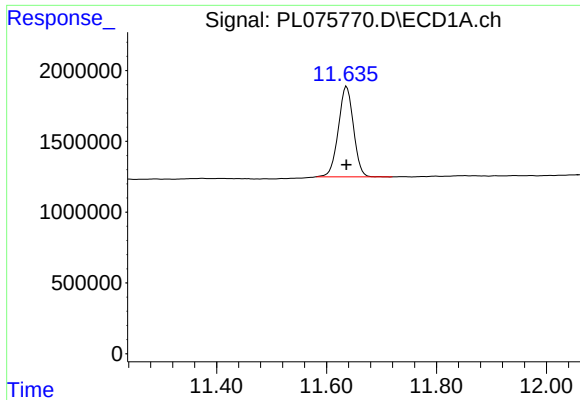

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: 0.000 min
Response: 12188595
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

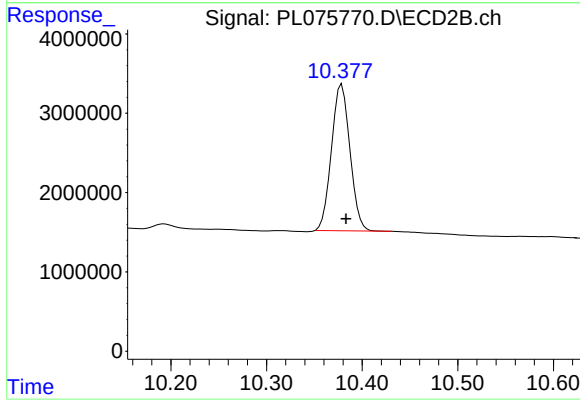

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 24728578
Conc: 17.55 ng/ml