

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
 Data File : PL075773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 17:29
 Operator : AR\AJ
 Sample : N3336-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:47:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	8756226	22294215	12.974	13.285
28)	SA Decachlor...	11.636	10.378	7946934	16472650	12.980	11.691
Target Compounds							
7)	B delta-BHC	0.000	6.400	0	437802	N.D.	0.204 #
9)	A Endosulfan I	8.534	0.000	291133	0	0.416	N.D. #
10)	B gamma-Chl...	8.383	7.324f	2843014	380990	3.661	0.208 #
11)	B alpha-Chl...	8.474	0.000	927889	0	1.217	N.D. #
12)	B 4,4'-DDE	8.657	7.620	664305	1798776	1.004	1.125
15)	B Endosulfa...	9.304	0.000	316841	0	0.509	N.D. #
17)	MA 4,4'-DDT	9.519	8.463	307730	898231	0.480	0.639 #
21)	B Endrin ke...	10.184f	0.000	1001653	0	1.424	N.D. #
25)	Chlordane-3	8.383	7.324f	2843014	380990	27.535	2.215 #
26)	Chlordane-4	8.474	0.000	927889	0	7.326	N.D. #
27)	Chlordane-5	0.000	8.110	0	59457	N.D.	1.252 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
Data File : PL075773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 17:29
Operator : AR\AJ
Sample : N3336-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:47:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

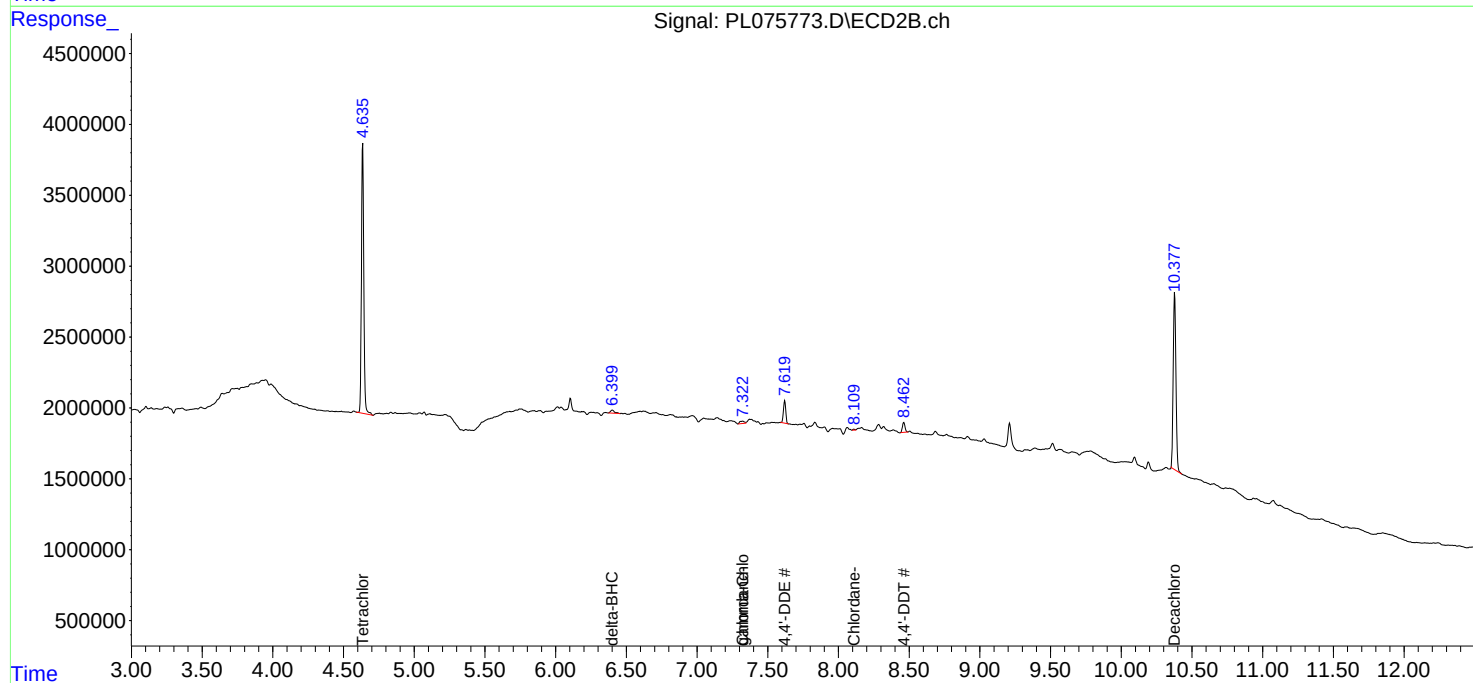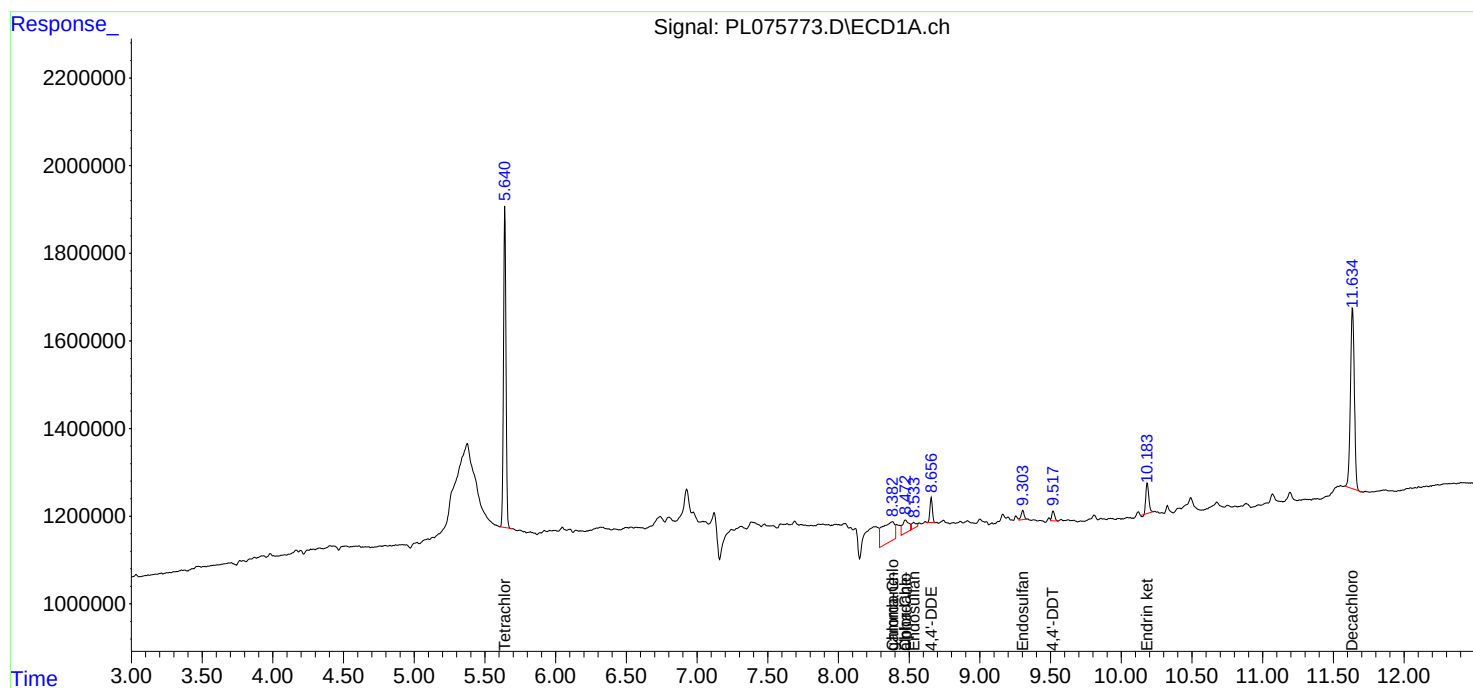


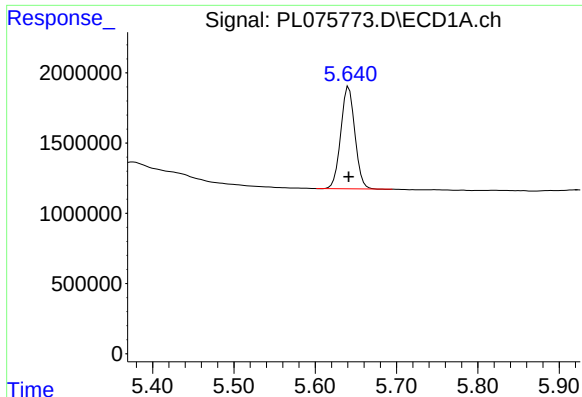

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 8756226
Conc: 12.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

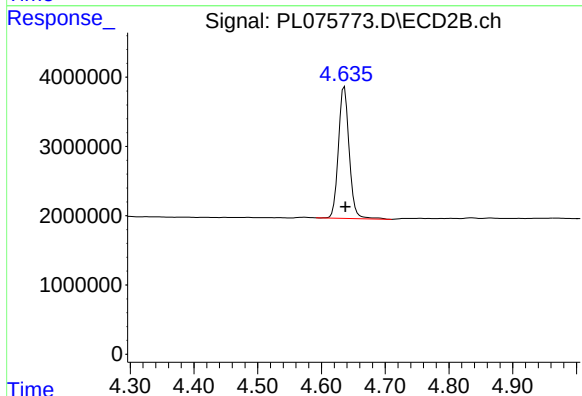


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 22294215
Conc: 13.28 ng/ml

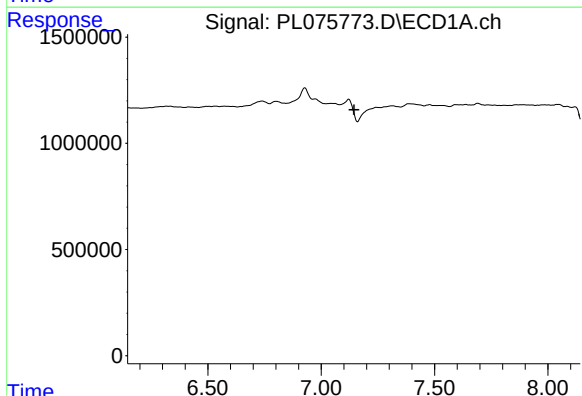


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

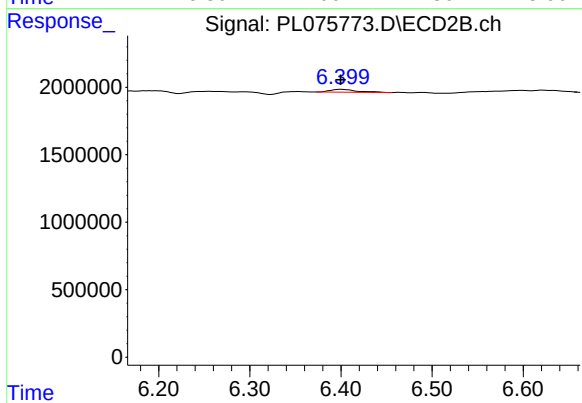

#7 delta-BHC


R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 437802
Conc: 0.20 ng/ml

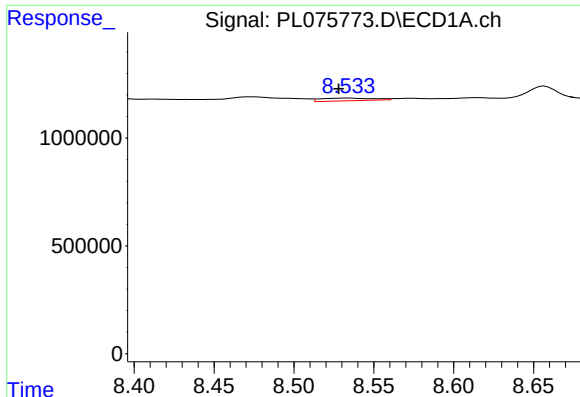

#9 Endosulfan I


R.T.: 8.534 min
Delta R.T.: 0.006 min
Response: 291133
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

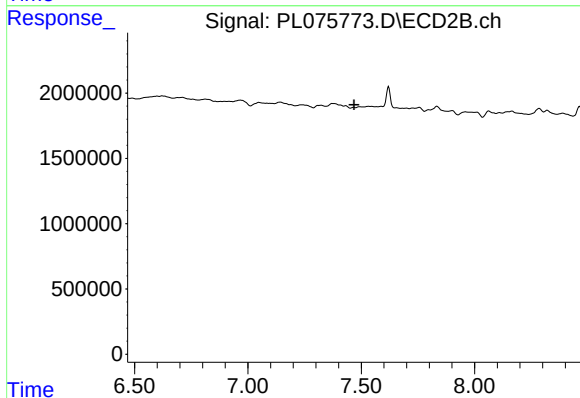


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

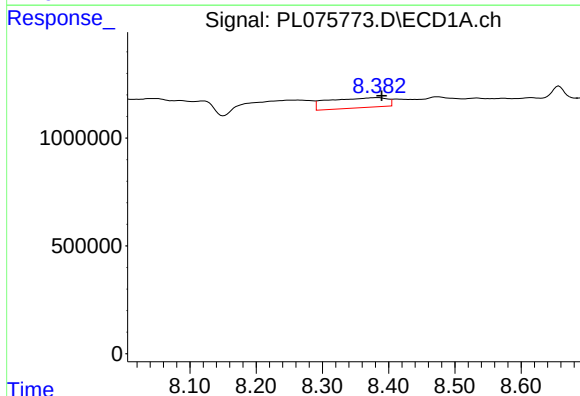


#10 gamma-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 2843014
Conc: 3.66 ng/ml

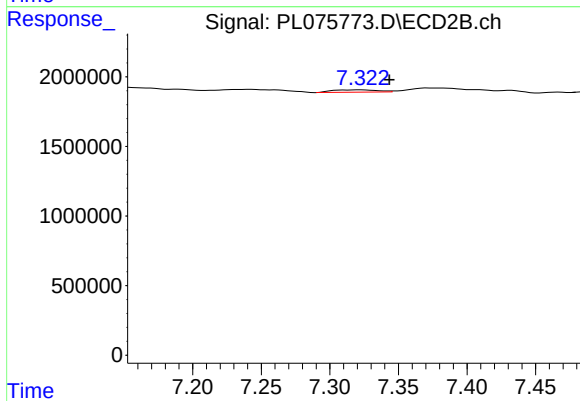

#10 gamma-Chlordane


R.T.: 7.324 min
Delta R.T.: -0.020 min
Response: 380990
Conc: 0.21 ng/ml

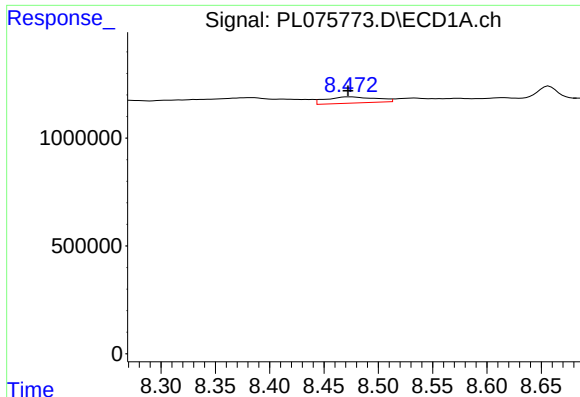

#11 alpha-Chlordane


R.T.: 8.474 min
Delta R.T.: 0.002 min
Response: 927889
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

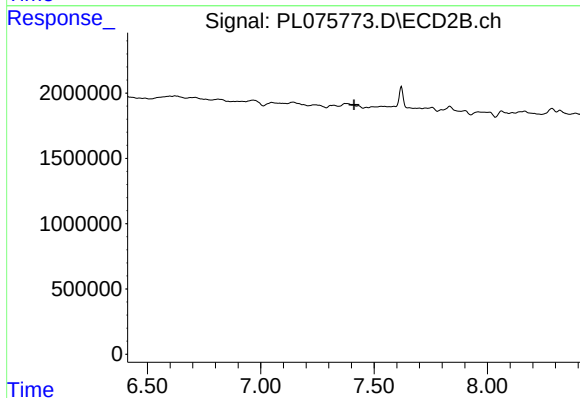


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

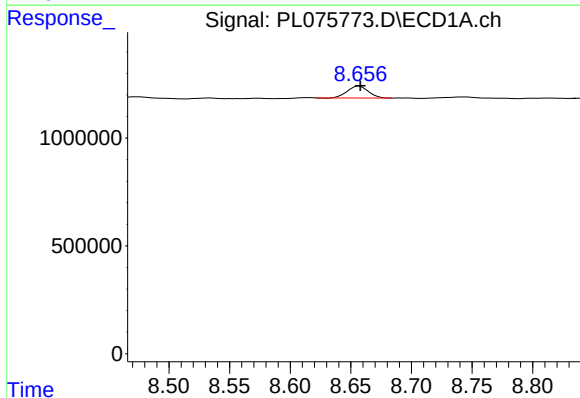


#12 4,4'-DDE

R.T.: 8.657 min
Delta R.T.: 0.000 min
Response: 664305
Conc: 1.00 ng/ml

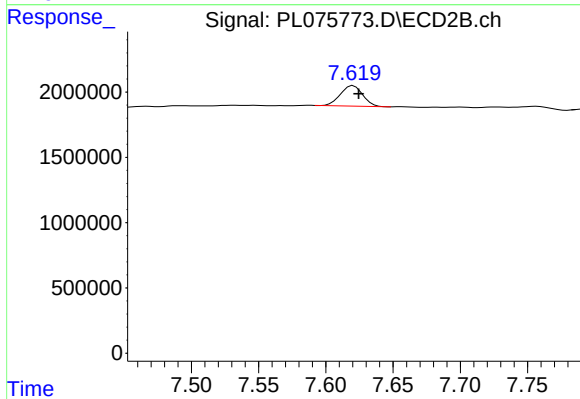

#12 4,4'-DDE


R.T.: 7.620 min
Delta R.T.: -0.004 min
Response: 1798776
Conc: 1.13 ng/ml

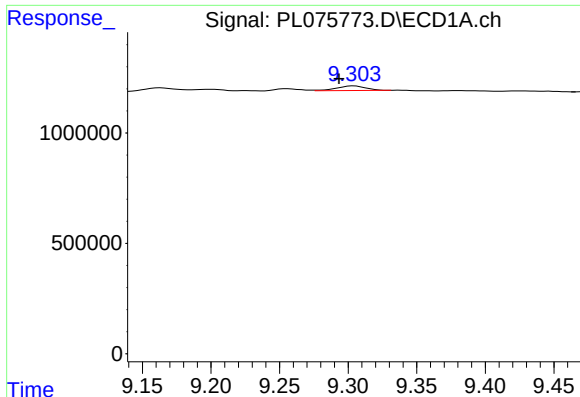

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 316841
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

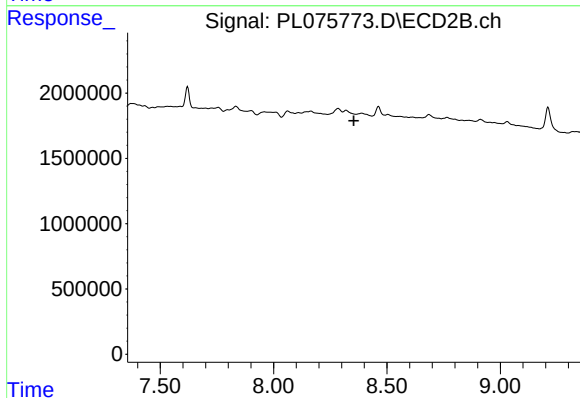


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

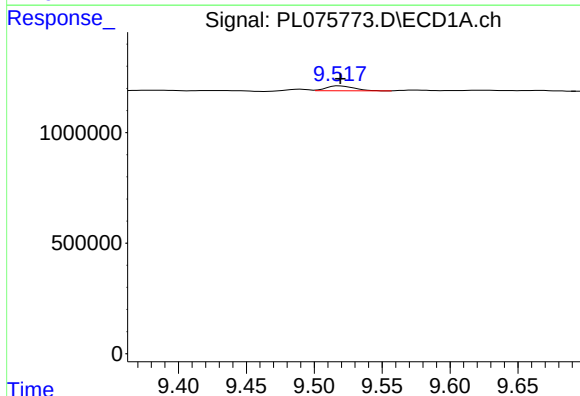


#17 4,4'-DDT

R.T.: 9.519 min
Delta R.T.: 0.000 min
Response: 307730
Conc: 0.48 ng/ml

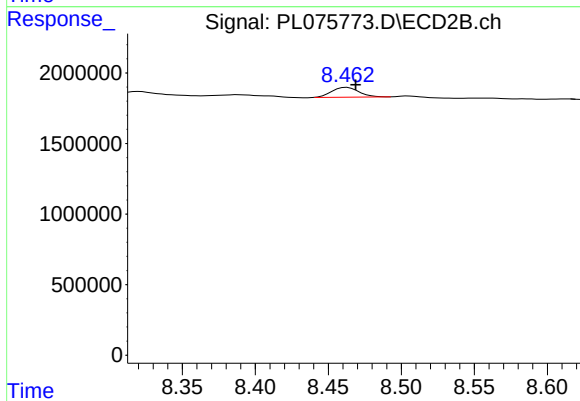

#17 4,4'-DDT


R.T.: 8.463 min
Delta R.T.: -0.006 min
Response: 898231
Conc: 0.64 ng/ml

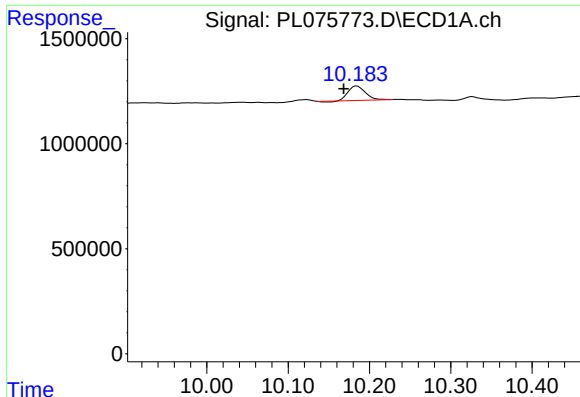

#21 Endrin ketone


R.T.: 10.184 min
Delta R.T.: 0.016 min
Response: 1001653
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

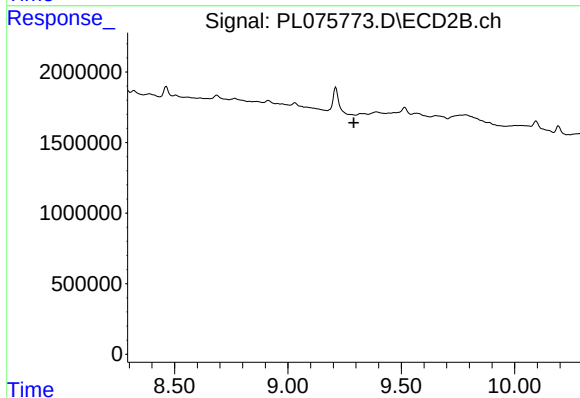


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

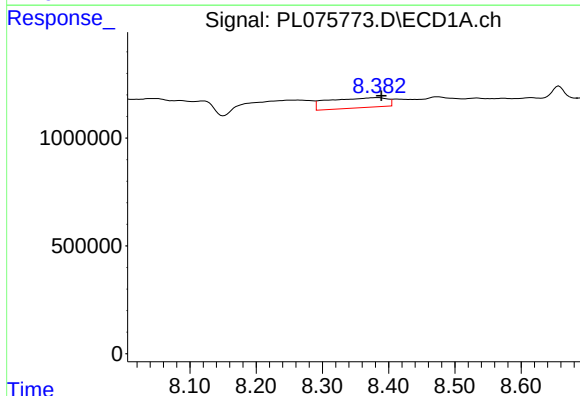


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 2843014
Conc: 27.53 ng/ml

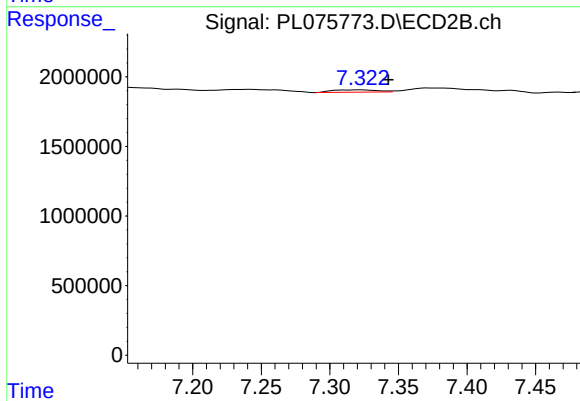

#25 Chlordane-3


R.T.: 7.324 min
Delta R.T.: -0.019 min
Response: 380990
Conc: 2.22 ng/ml

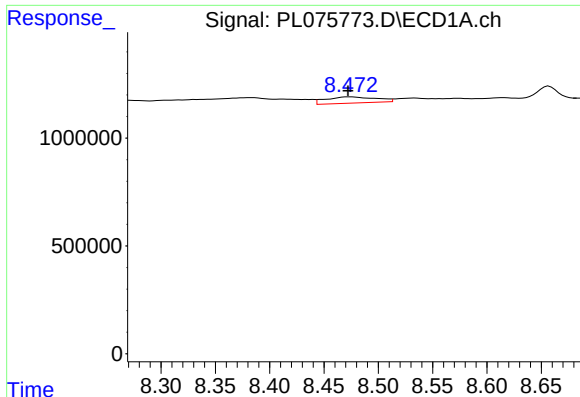

#26 Chlordane-4


R.T.: 8.474 min
Delta R.T.: 0.002 min
Response: 927889
Conc: 7.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

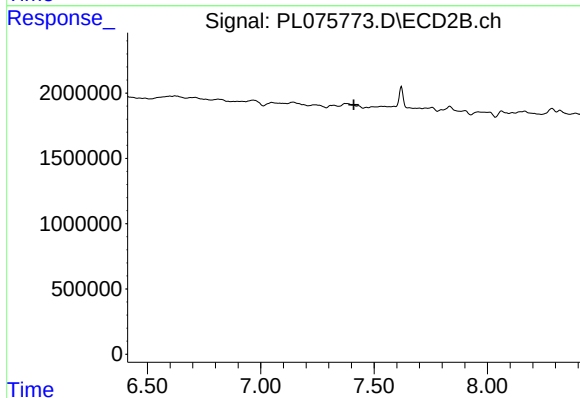


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

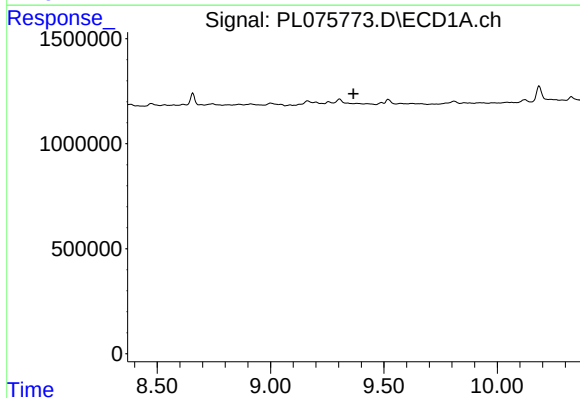


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

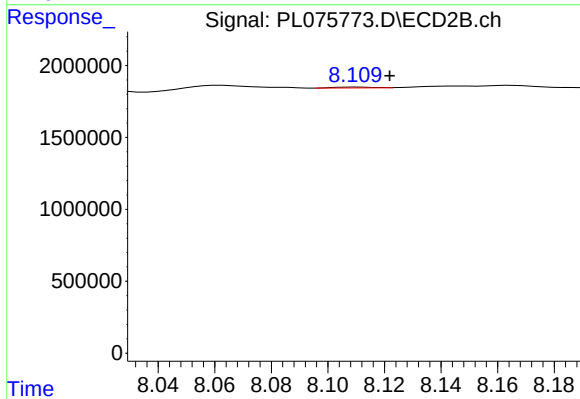

#27 Chlordane-5


R.T.: 8.110 min
Delta R.T.: -0.012 min
Response: 59457
Conc: 1.25 ng/ml

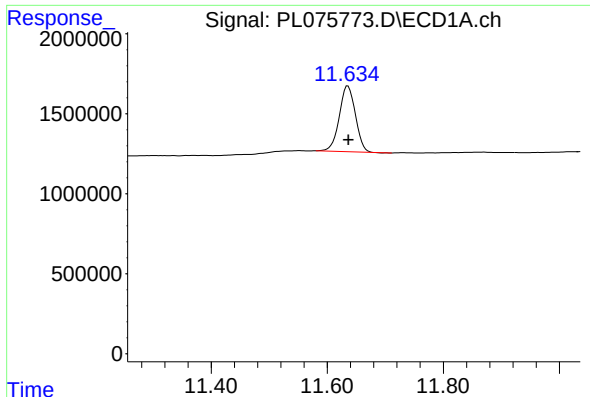

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 7946934
Conc: 12.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

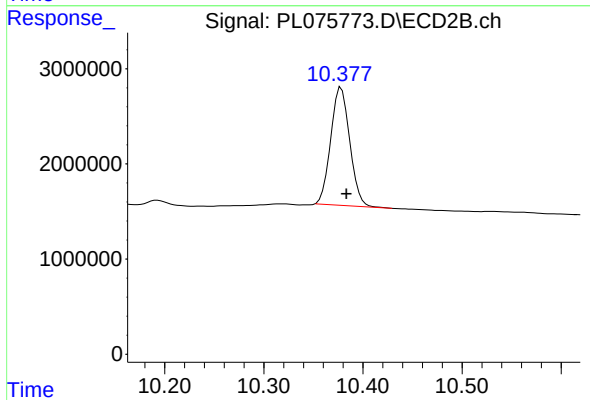

#28 Decachlorobiphenyl

R.T.: 10.378 min
Delta R.T.: -0.005 min
Response: 16472650
Conc: 11.69 ng/ml