

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
 Data File : PL075780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 19:37
 Operator : AR\AJ
 Sample : PB145458TB
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:49:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.637	13565564	32235109	20.101	19.208
28)	SA Decachlor...	11.637	10.379	12896118	27235105	21.064	19.330
Target Compounds							
7)	B delta-BHC	0.000	6.403	0	558471	N.D.	0.261 #
9)	A Endosulfan I	8.532	0.000	213658	0	0.305	N.D. #
10)	B gamma-Chl...	8.379	0.000	1372881	0	1.768	N.D. #
11)	B alpha-Chl...	8.492f	7.387f	876972	321071	1.150	0.176 #
15)	B Endosulfa...	9.304	0.000	343310	0	0.552	N.D. #
21)	B Endrin ke...	10.185f	0.000	1087736	0	1.547	N.D. #
25)	Chlordane-3	8.379	0.000	1372881	0	13.296	N.D. #
26)	Chlordane-4	8.492f	7.387f	876972	321071	6.924	1.744 #
27)	Chlordane-5	0.000	8.105f	0	85127	N.D.	1.793 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
Data File : PL075780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 19:37
Operator : AR\AJ
Sample : PB145458TB
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:49:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

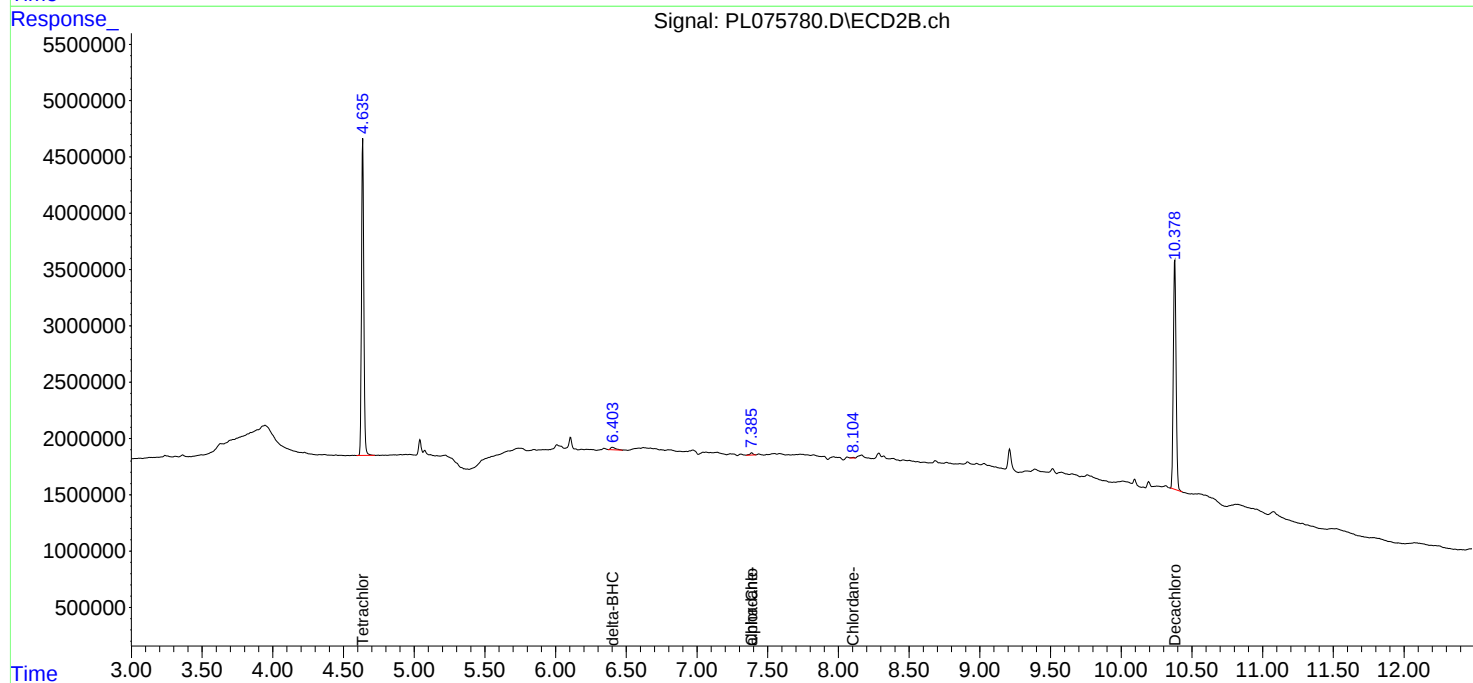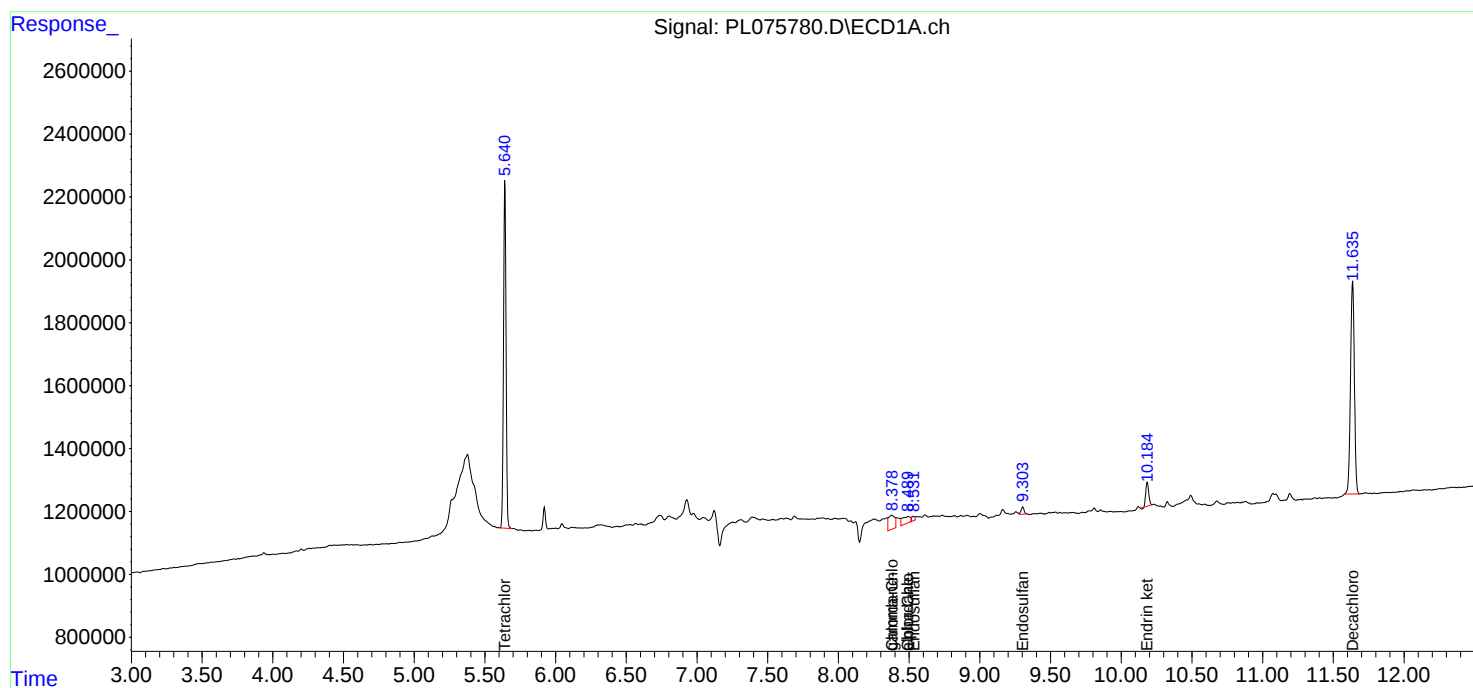


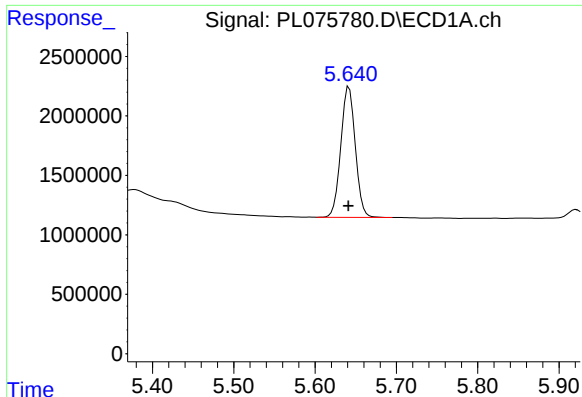

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 13565564
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

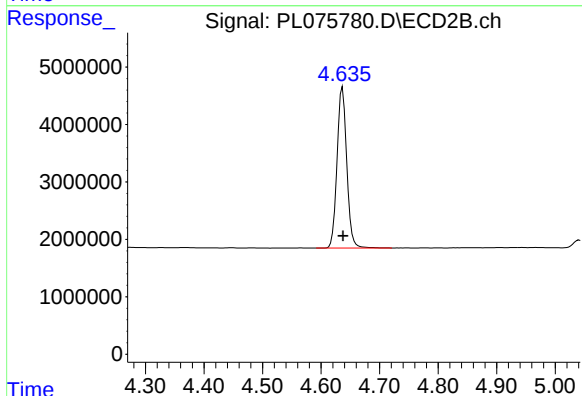


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.001 min
Response: 32235109
Conc: 19.21 ng/ml

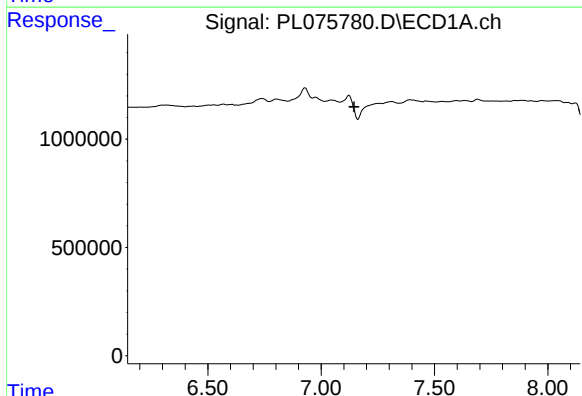


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

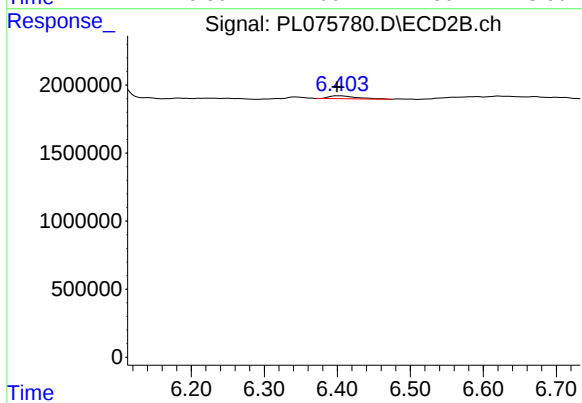

#7 delta-BHC


R.T.: 6.403 min
Delta R.T.: 0.003 min
Response: 558471
Conc: 0.26 ng/ml

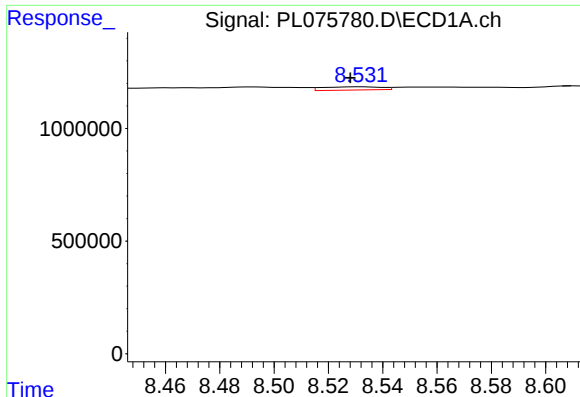

#9 Endosulfan I


R.T.: 8.532 min
Delta R.T.: 0.004 min
Response: 213658
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

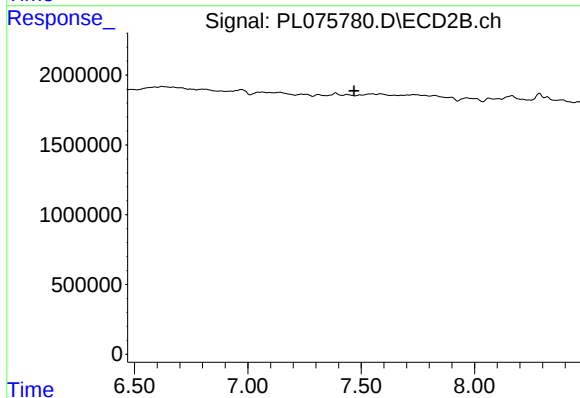


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

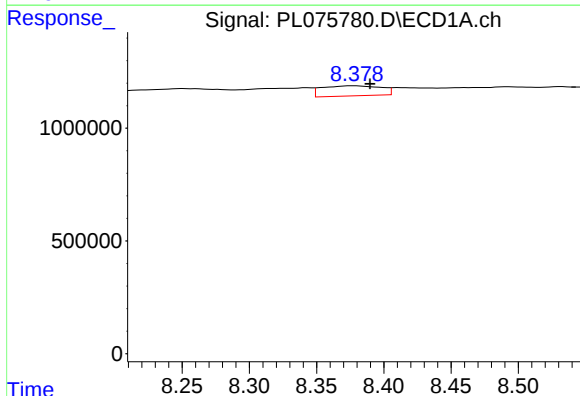


#10 gamma-Chlordane

R.T.: 8.379 min
Delta R.T.: -0.011 min
Response: 1372881
Conc: 1.77 ng/ml

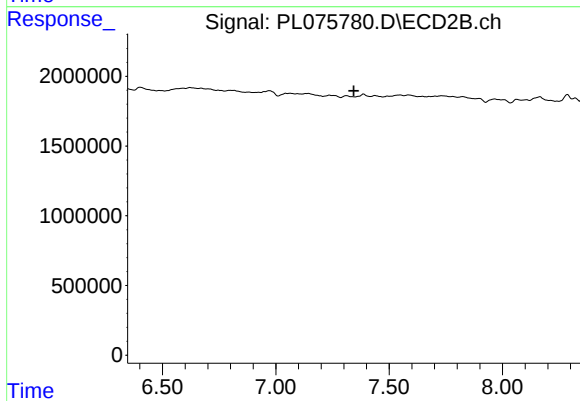

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

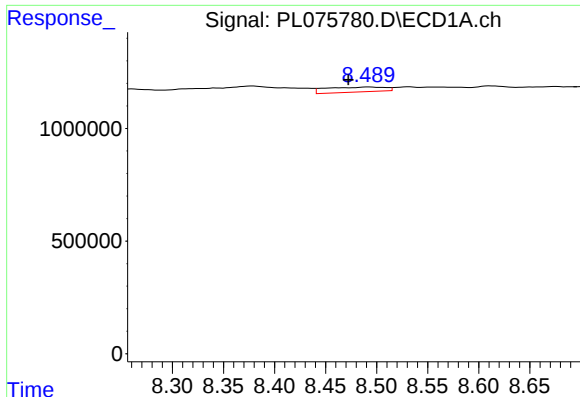

#11 alpha-Chlordane


R.T.: 8.492 min
Delta R.T.: 0.020 min
Response: 876972
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

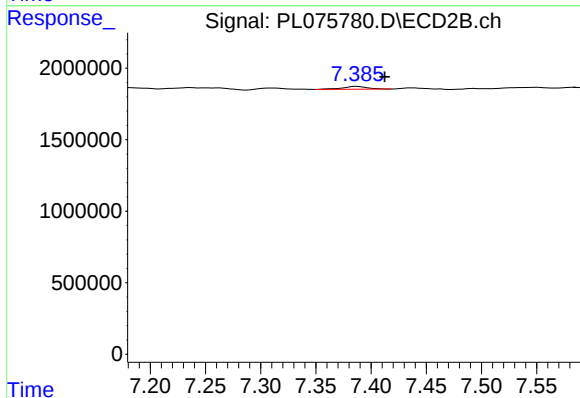


#11 alpha-Chlordane

R.T.: 7.387 min
Delta R.T.: -0.026 min
Response: 321071
Conc: 0.18 ng/ml

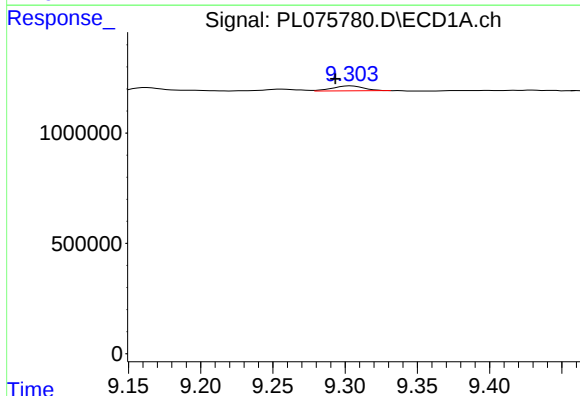


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 343310
Conc: 0.55 ng/ml

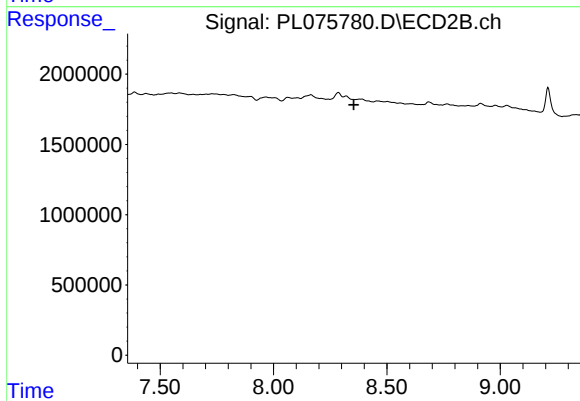

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

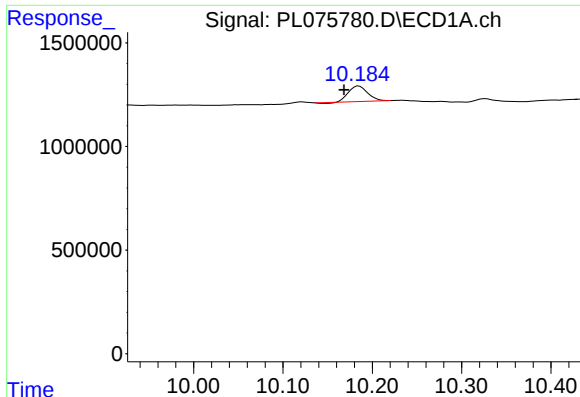

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 1087736
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

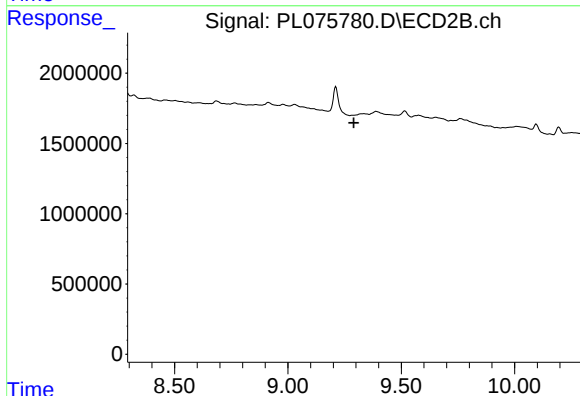


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

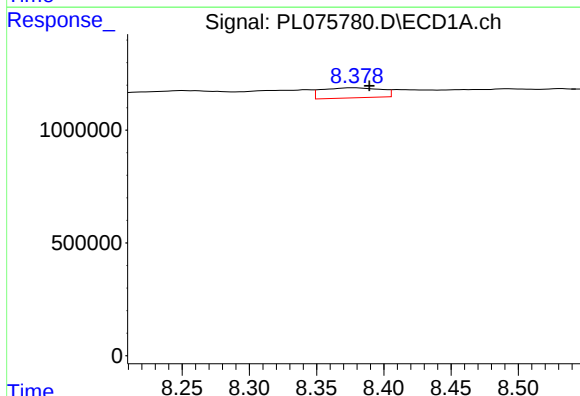


#25 Chlordane-3

R.T.: 8.379 min
Delta R.T.: -0.011 min
Response: 1372881
Conc: 13.30 ng/ml

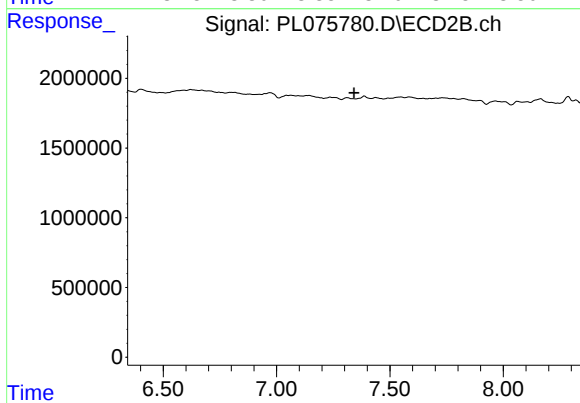

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

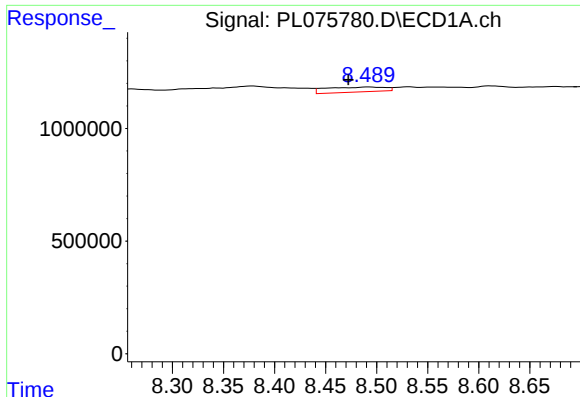

#26 Chlordane-4


R.T.: 8.492 min
Delta R.T.: 0.020 min
Response: 876972
Conc: 6.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

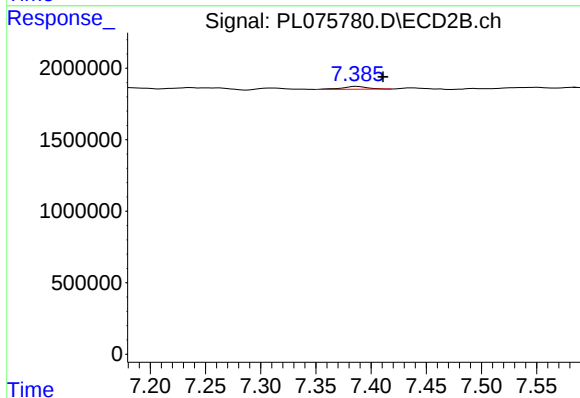


#26 Chlordane-4

R.T.: 7.387 min
Delta R.T.: -0.024 min
Response: 321071
Conc: 1.74 ng/ml

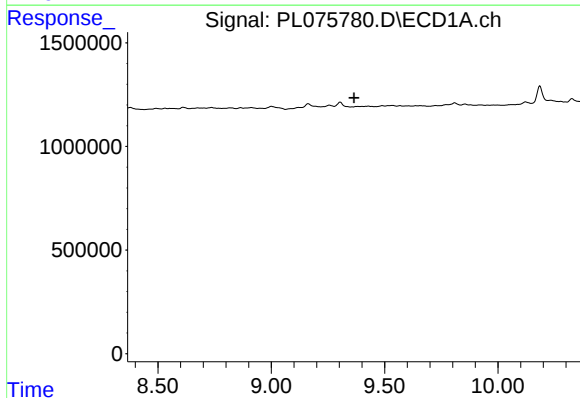


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

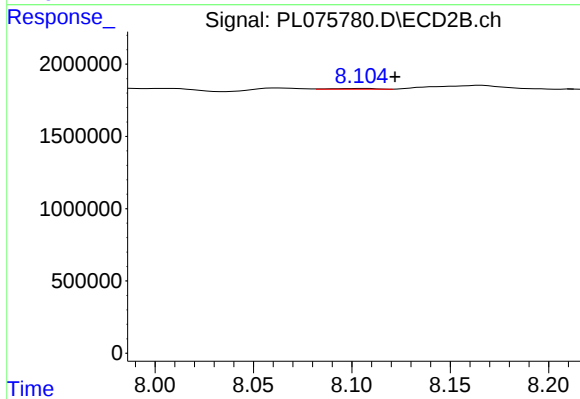

#27 Chlordane-5


R.T.: 8.105 min
Delta R.T.: -0.017 min
Response: 85127
Conc: 1.79 ng/ml

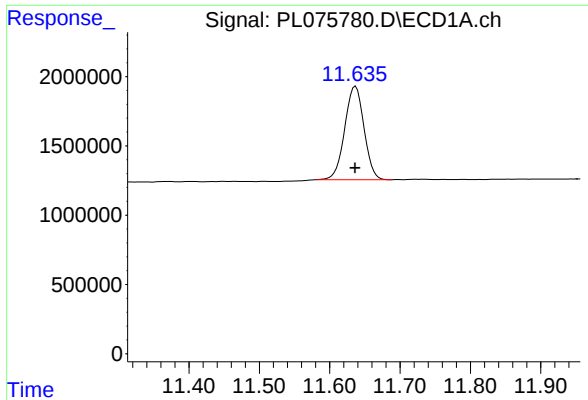

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: 0.000 min
Response: 12896118
Conc: 21.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

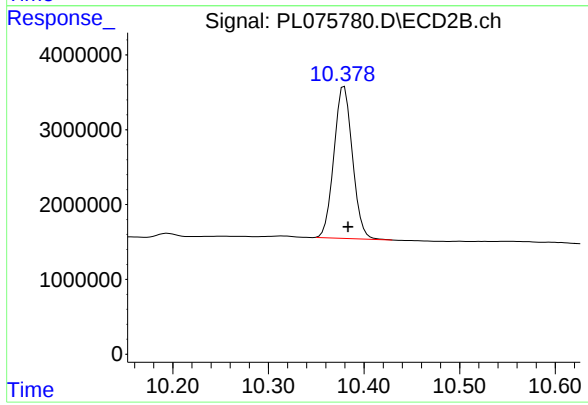

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 27235105
Conc: 19.33 ng/ml