

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
 Data File : PL075781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 19:54
 Operator : AR\AJ
 Sample : PB145493TB
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:49:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	13745447	32686841	20.367	19.477
28)	SA Decachlor...	11.637	10.379	13259993	28005194	21.659	19.877
Target Compounds							
7)	B delta-BHC	0.000	6.402	0	331972	N.D.	0.155 #
9)	A Endosulfan I	8.536	0.000	146804	0	0.210	N.D. #
10)	B gamma-Chl...	8.383	0.000	1252170	0	1.612	N.D. #
11)	B alpha-Chl...	8.494f	7.387f	471952	291412	0.619	0.160 #
15)	B Endosulfa...	9.304	0.000	352840	0	0.567	N.D. #
21)	B Endrin ke...	10.185f	0.000	1156172	0	1.644	N.D. #
25)	Chlordane-3	8.383	0.000	1252170	0	12.127	N.D. #
26)	Chlordane-4	8.494f	7.387f	471952	291412	3.726	1.583 #
27)	Chlordane-5	0.000	8.100f	0	43819	N.D.	0.923 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
Data File : PL075781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 19:54
Operator : AR\AJ
Sample : PB145493TB
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:49:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

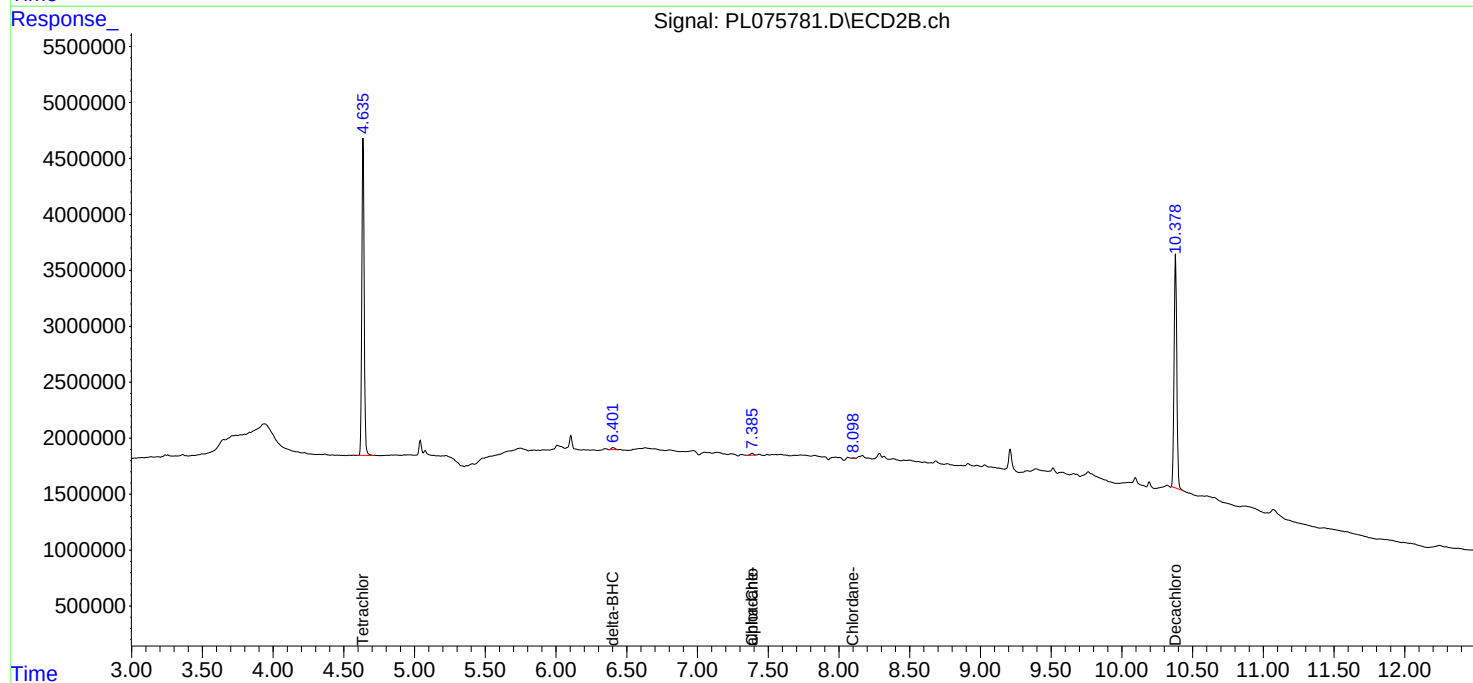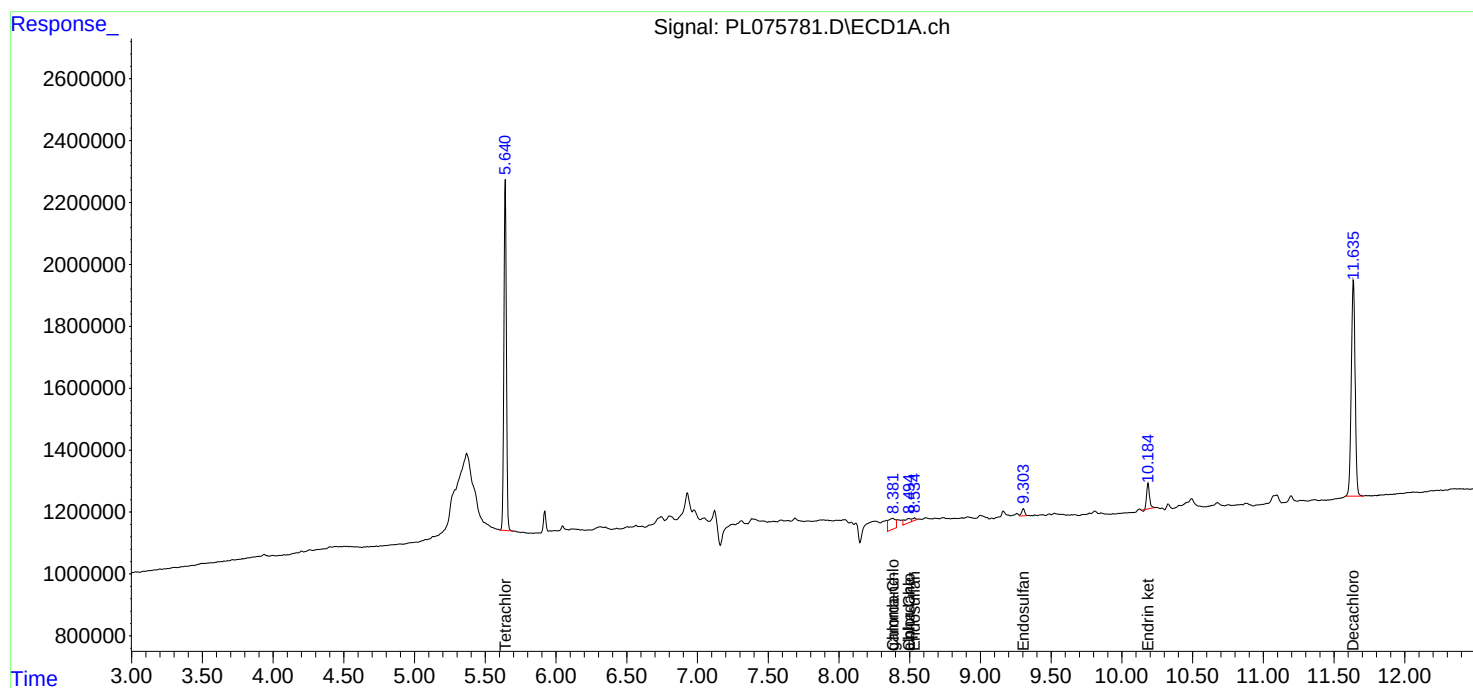


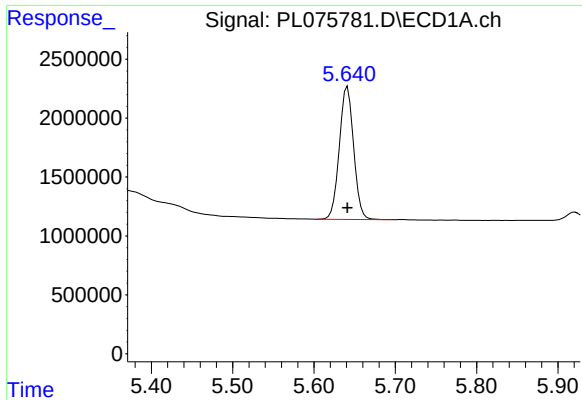

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 13745447
Conc: 20.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

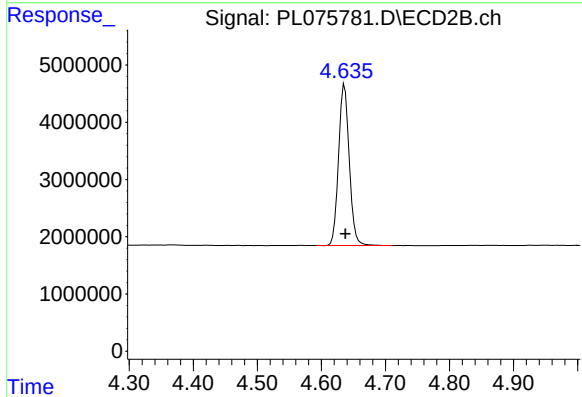


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 32686841
Conc: 19.48 ng/ml

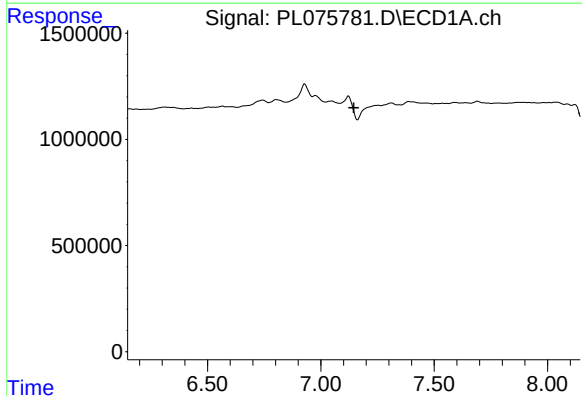


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

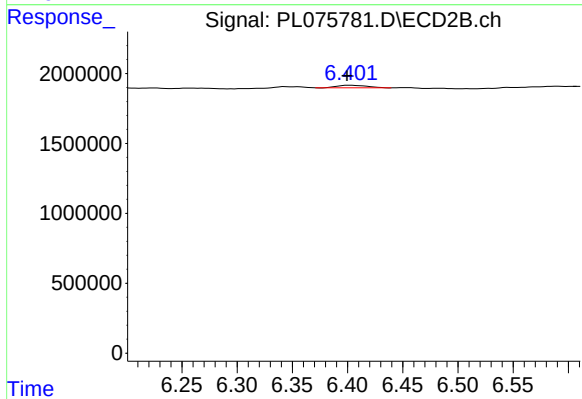

#7 delta-BHC


R.T.: 6.402 min
Delta R.T.: 0.003 min
Response: 331972
Conc: 0.16 ng/ml

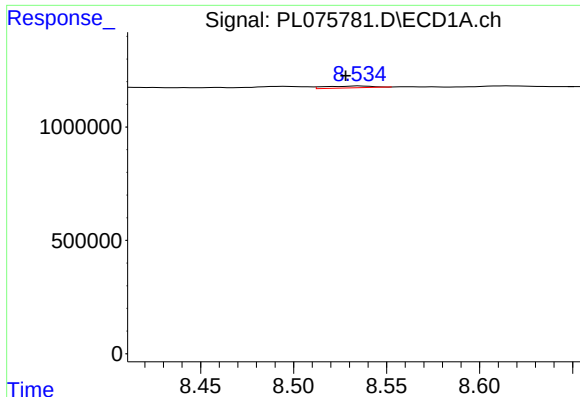

#9 Endosulfan I


R.T.: 8.536 min
Delta R.T.: 0.008 min
Response: 146804
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

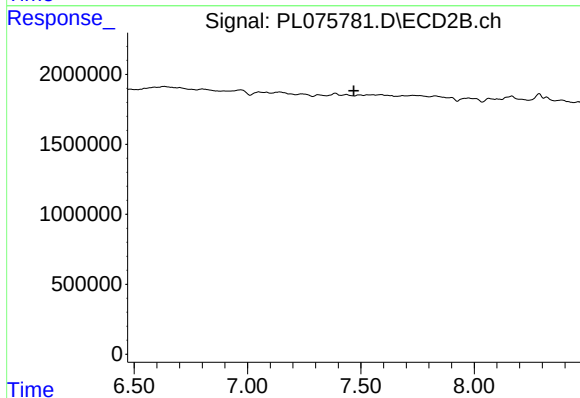


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

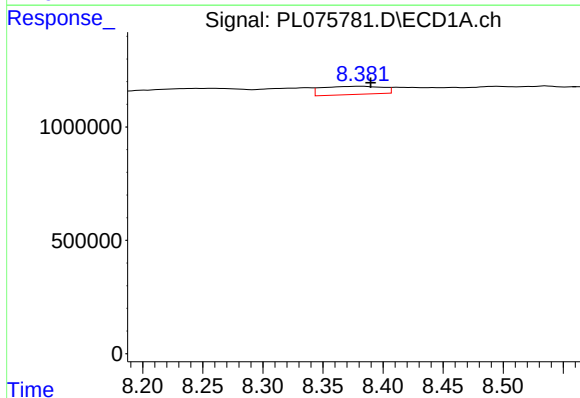


#10 gamma-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1252170
Conc: 1.61 ng/ml

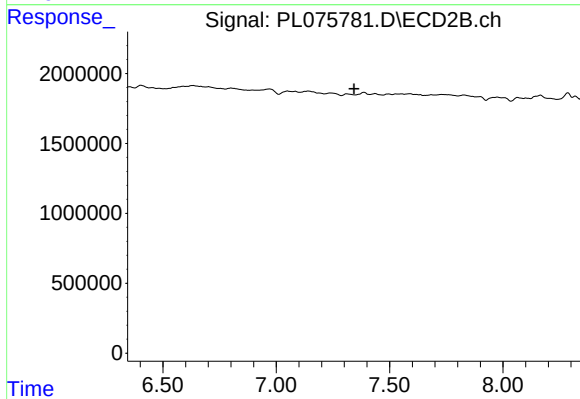

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

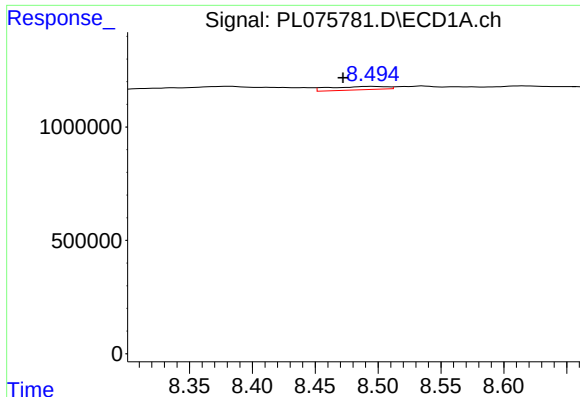

#11 alpha-Chlordane


R.T.: 8.494 min
Delta R.T.: 0.022 min
Response: 471952
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

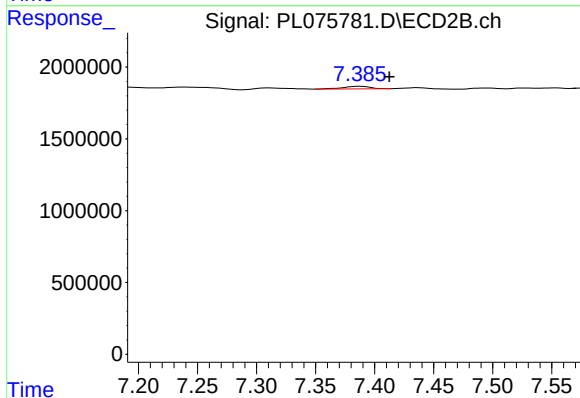


#11 alpha-Chlordane

R.T.: 7.387 min
Delta R.T.: -0.025 min
Response: 291412
Conc: 0.16 ng/ml

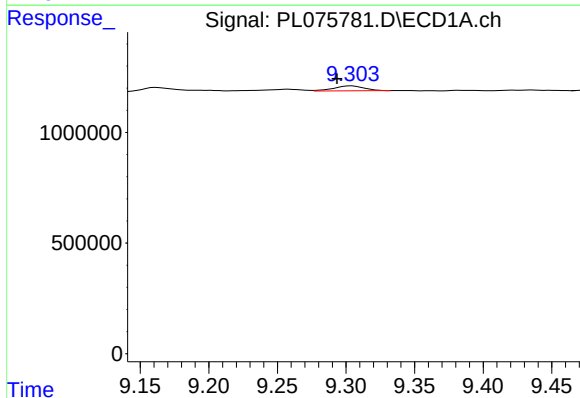


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 352840
Conc: 0.57 ng/ml

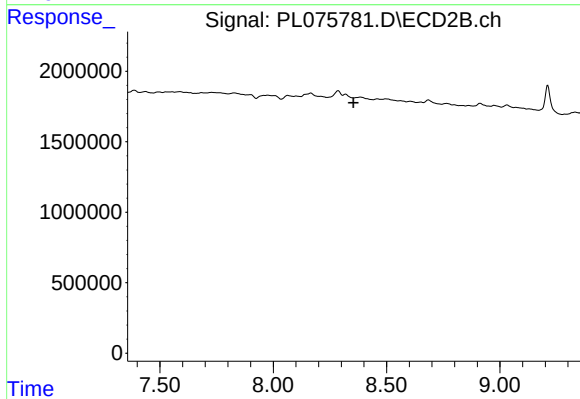

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

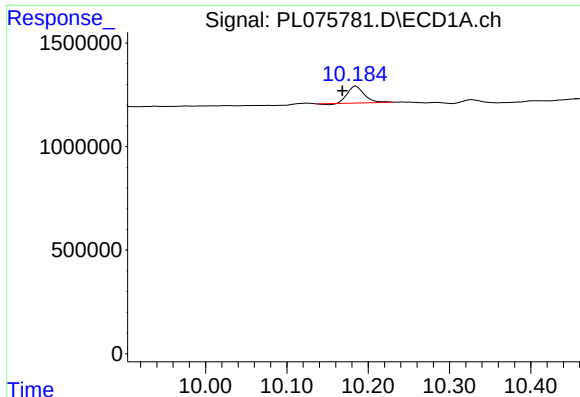

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 1156172
Conc: 1.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

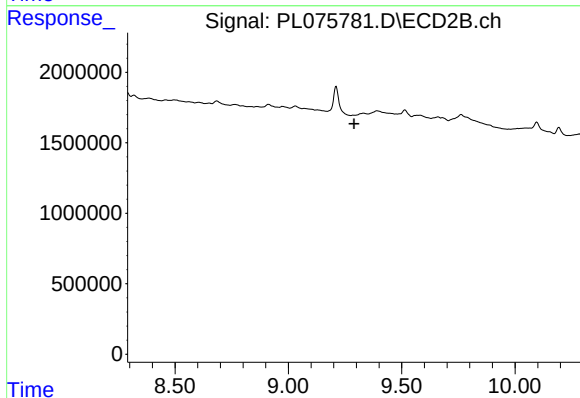


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

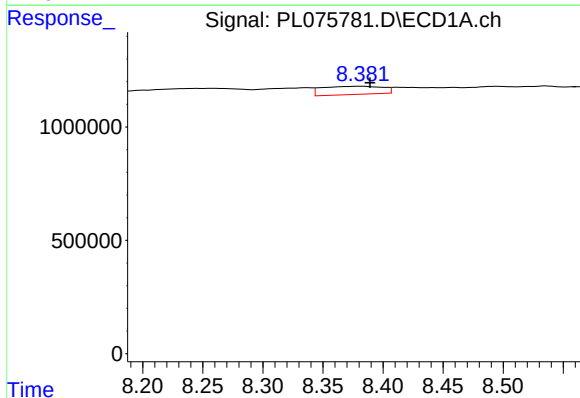


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1252170
Conc: 12.13 ng/ml

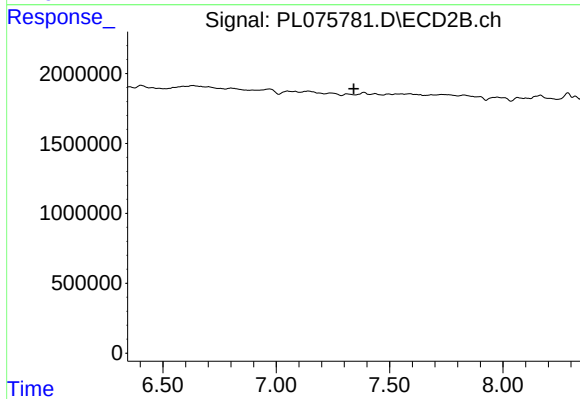

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

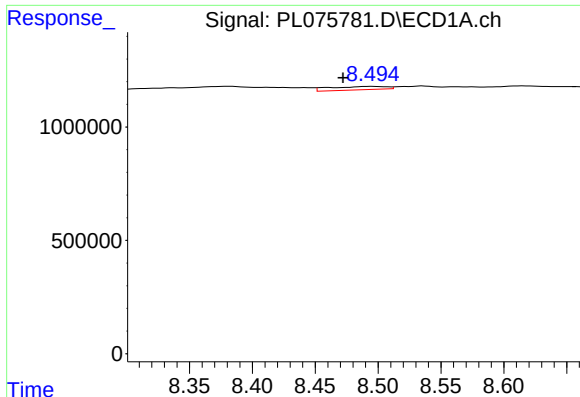

#26 Chlordane-4


R.T.: 8.494 min
Delta R.T.: 0.022 min
Response: 471952
Conc: 3.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

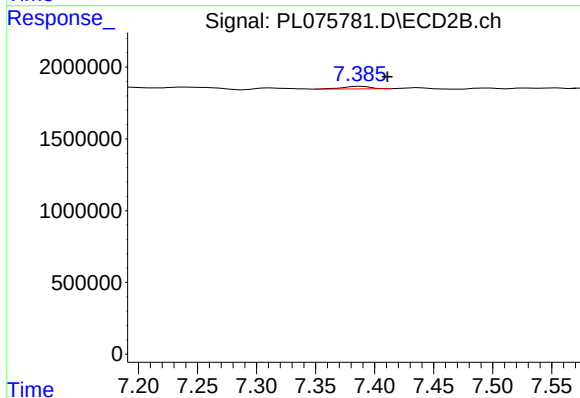


#26 Chlordane-4

R.T.: 7.387 min
Delta R.T.: -0.024 min
Response: 291412
Conc: 1.58 ng/ml

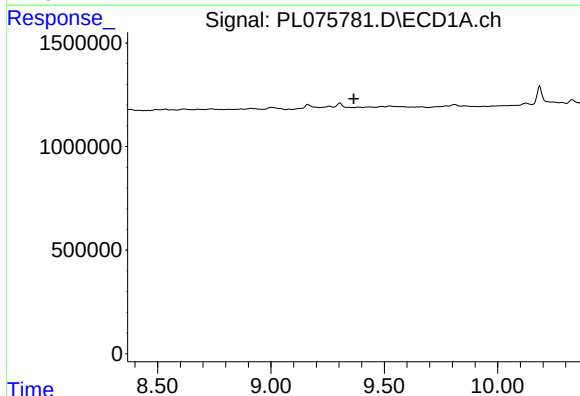


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

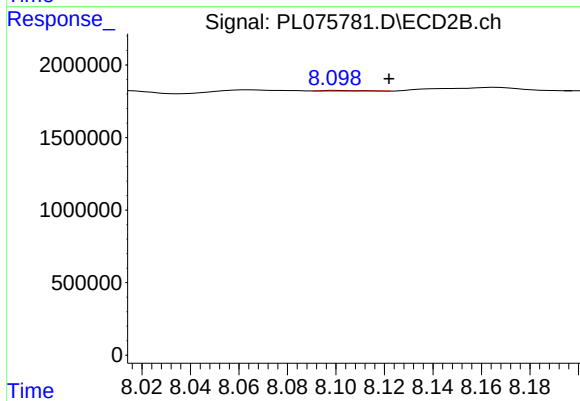

#27 Chlordane-5


R.T.: 8.100 min
Delta R.T.: -0.022 min
Response: 43819
Conc: 0.92 ng/ml

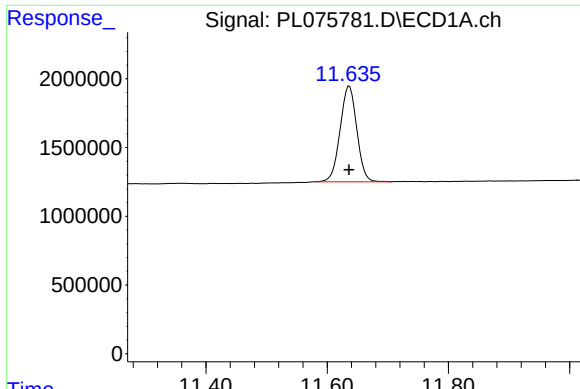

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: 0.000 min
Response: 13259993
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

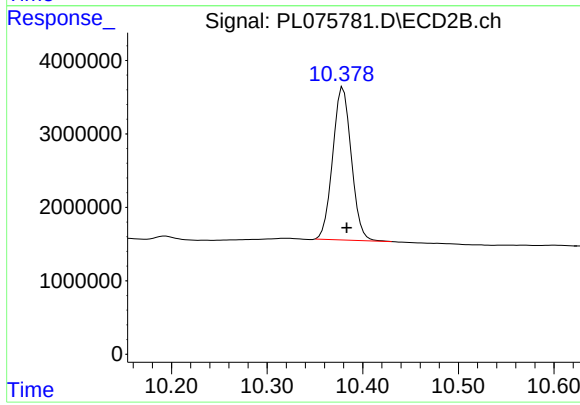

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 28005194
Conc: 19.88 ng/ml