

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
 Data File : PL075782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 20:10
 Operator : AR\AJ
 Sample : N3299-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:49:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.637	15440395	36139805	22.879	21.535
28)	SA Decachlor...	11.636	10.379	14698238	31054235	24.008	22.041
Target Compounds							
3)	MA gamma-BHC...	0.000	5.754	0	477513	N.D.	0.220 #
4)	MA Heptachlor	0.000	6.177	0	302498	N.D.	0.142 #
9)	A Endosulfan I	8.530	7.492f	284097	398022	0.406	0.238 #
10)	B gamma-Chl...	8.381	0.000	1659762	0	2.137	N.D. #
11)	B alpha-Chl...	8.501f	7.387f	729514	595517	0.957	0.326 #
13)	MA Dieldrin	0.000	7.761	0	713769	N.D.	0.422 #
15)	B Endosulfa...	9.303	0.000	339518	0	0.546	N.D. #
21)	B Endrin ke...	10.185f	0.000	994015	0	1.413	N.D. #
25)	Chlordane-3	8.381	0.000	1659762	0	16.075	N.D. #
26)	Chlordane-4	8.501f	7.387f	729514	595517	5.760	3.235 #
27)	Chlordane-5	0.000	8.143f	0	238005	N.D.	5.013 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061422\
Data File : PL075782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 20:10
Operator : AR\AJ
Sample : N3299-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:49:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

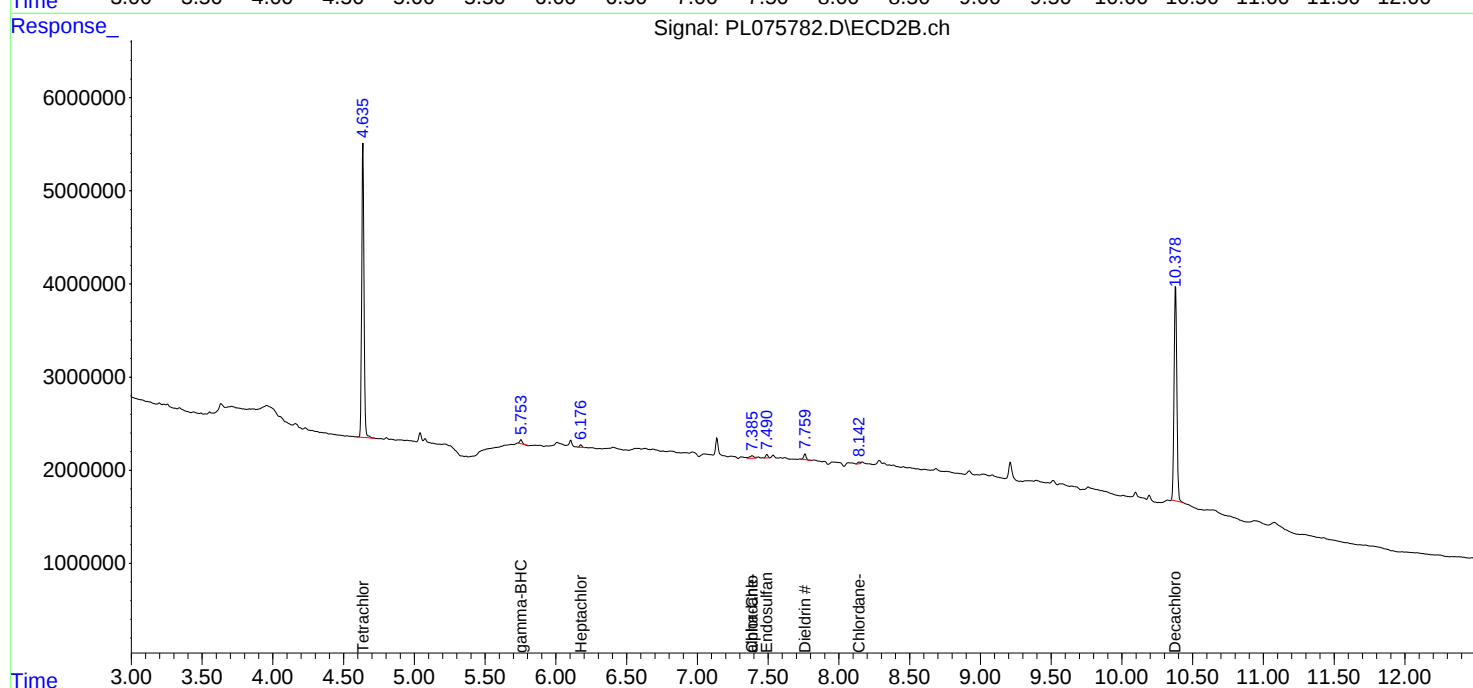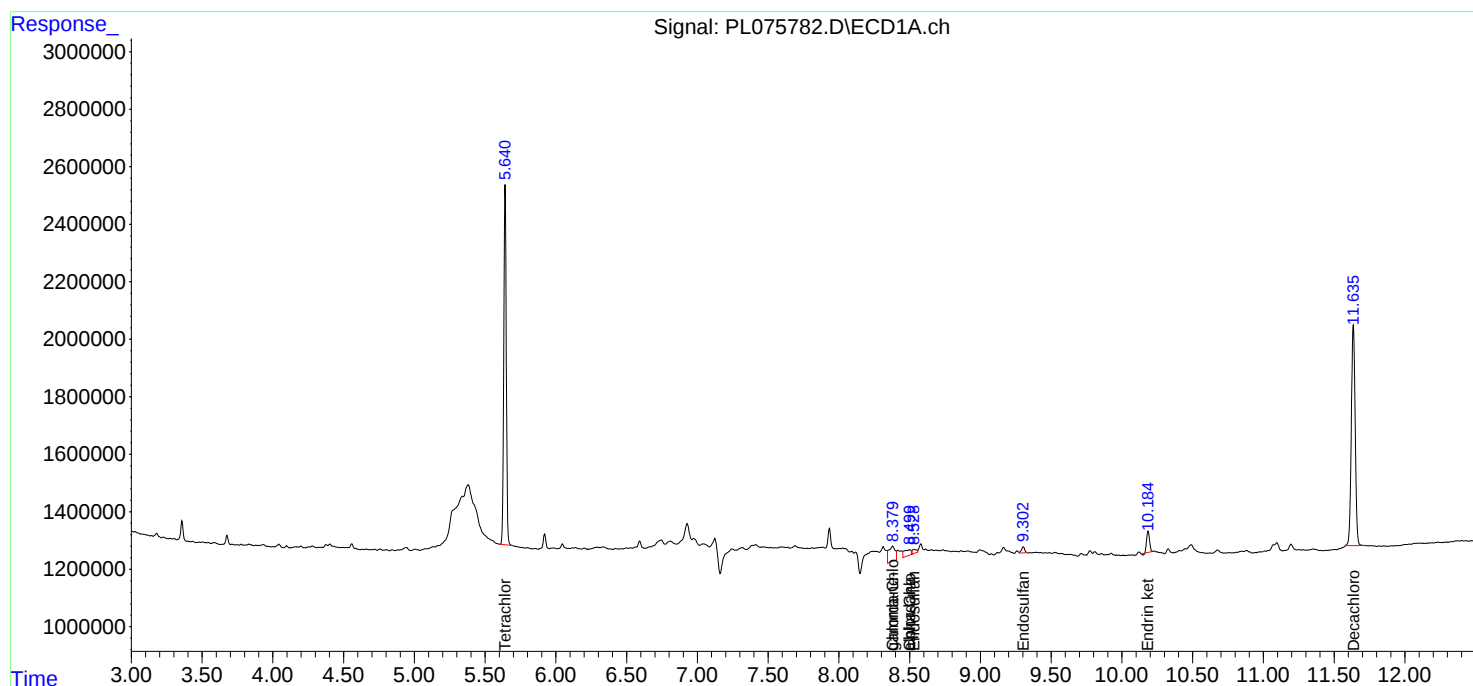


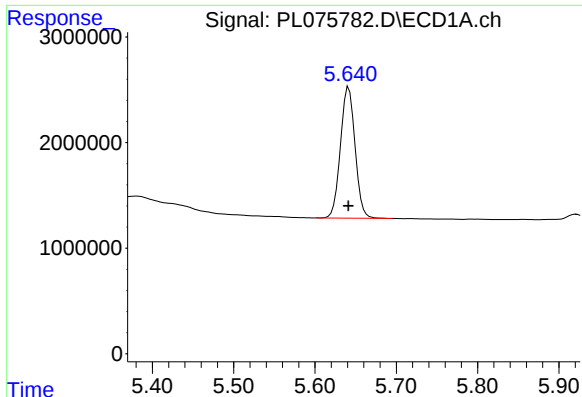

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 15440395
Conc: 22.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

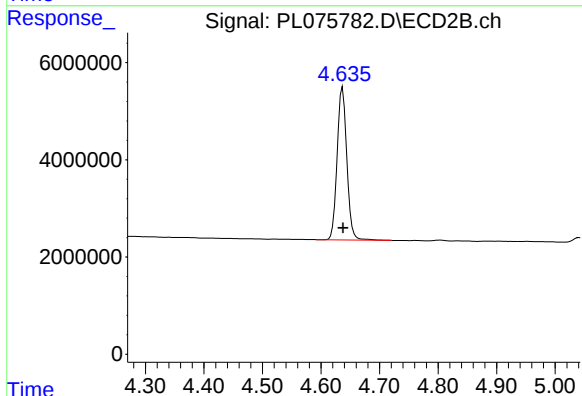


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.001 min
Response: 36139805
Conc: 21.53 ng/ml

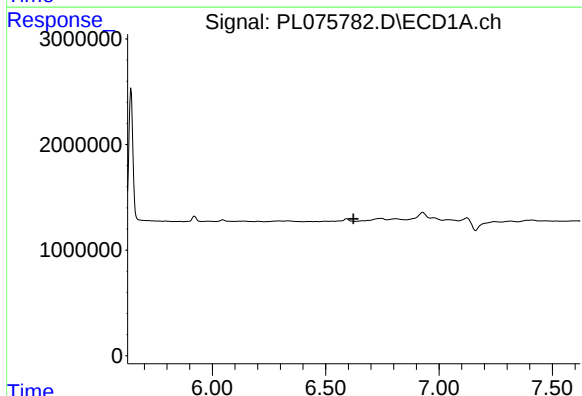


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.623 min
Response: 0
Conc: N.D.

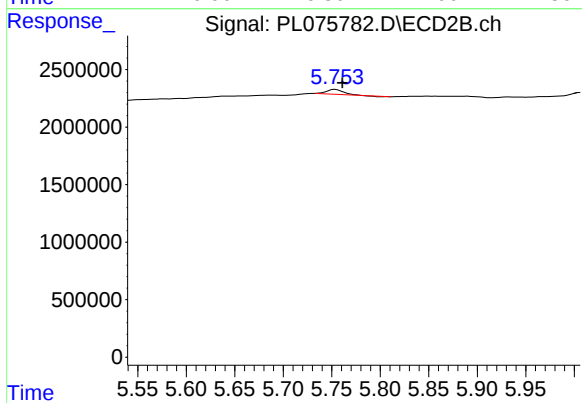

#3 gamma-BHC (Lindane)


R.T.: 5.754 min
Delta R.T.: -0.007 min
Response: 477513
Conc: 0.22 ng/ml

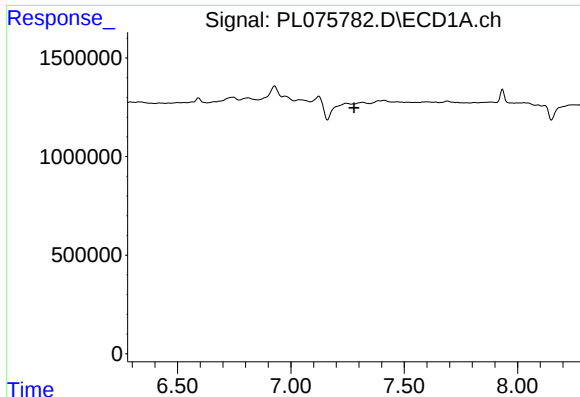

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

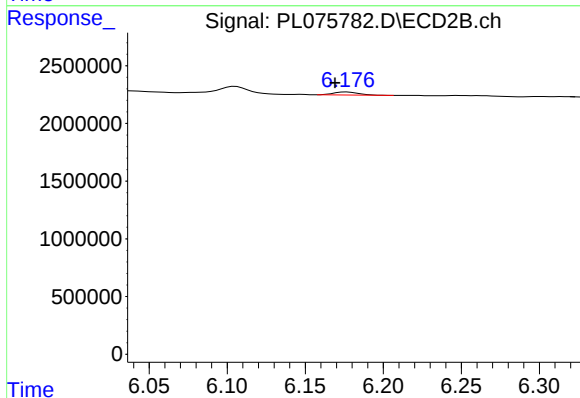


#4 Heptachlor

R.T.: 6.177 min
Delta R.T.: 0.008 min
Response: 302498
Conc: 0.14 ng/ml

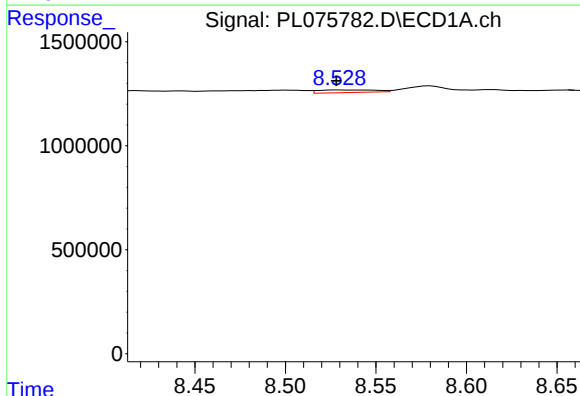


#9 Endosulfan I

R.T.: 8.530 min
Delta R.T.: 0.002 min
Response: 284097
Conc: 0.41 ng/ml

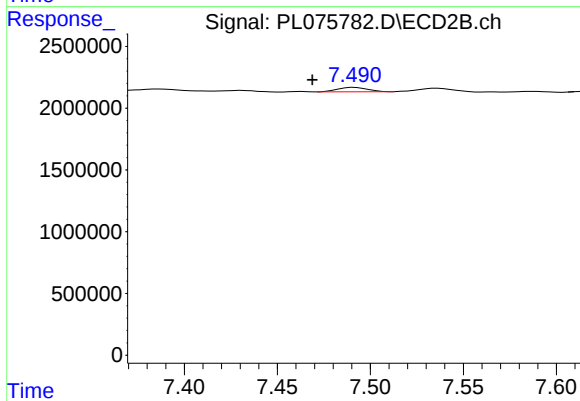

#9 Endosulfan I


R.T.: 7.492 min
Delta R.T.: 0.023 min
Response: 398022
Conc: 0.24 ng/ml

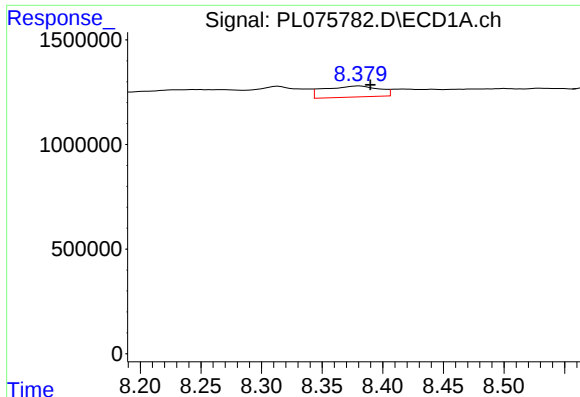

#10 gamma-Chlordane


R.T.: 8.381 min
Delta R.T.: -0.009 min
Response: 1659762
Conc: 2.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

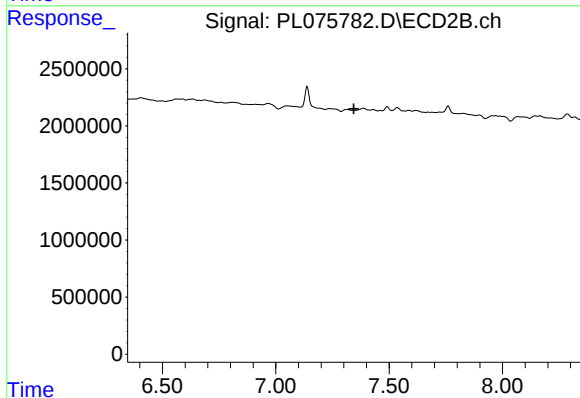


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

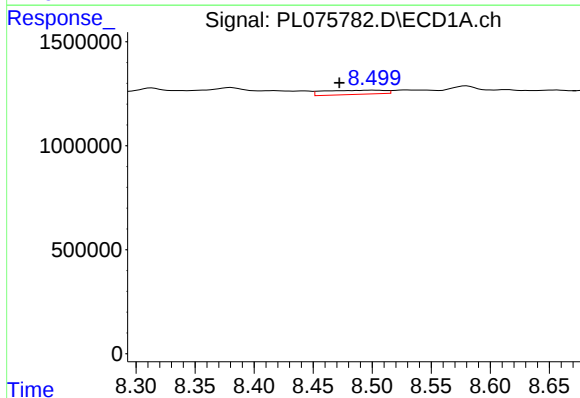


#11 alpha-Chlordane

R.T.: 8.501 min
Delta R.T.: 0.029 min
Response: 729514
Conc: 0.96 ng/ml

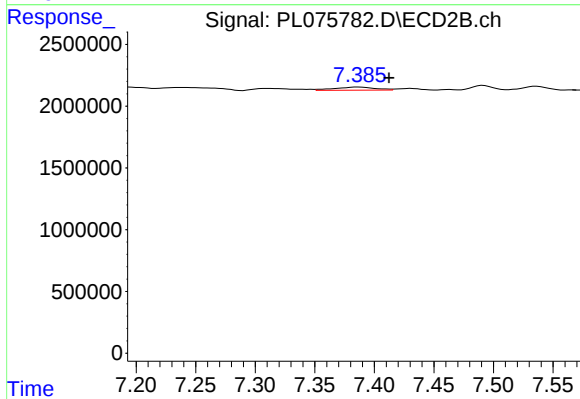

#11 alpha-Chlordane


R.T.: 7.387 min
Delta R.T.: -0.026 min
Response: 595517
Conc: 0.33 ng/ml

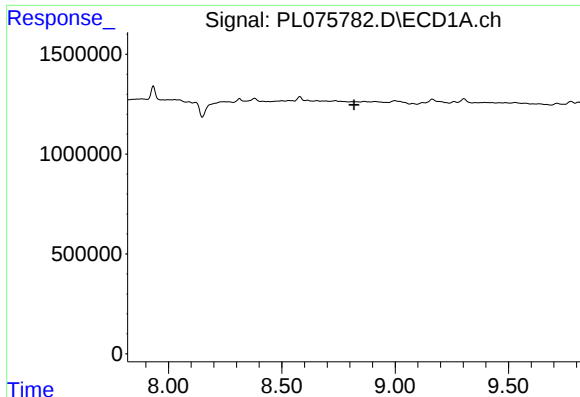

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

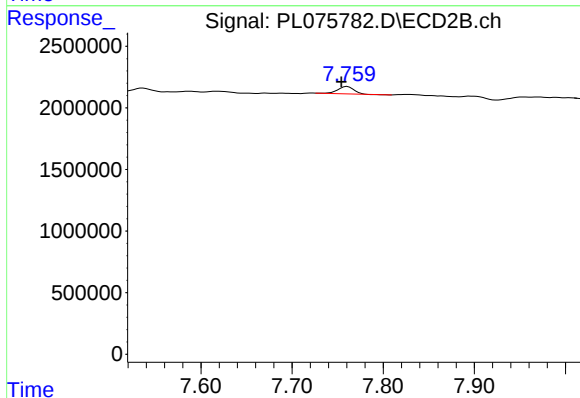


#13 Dieldrin

R.T.: 7.761 min
Delta R.T.: 0.007 min
Response: 713769
Conc: 0.42 ng/ml

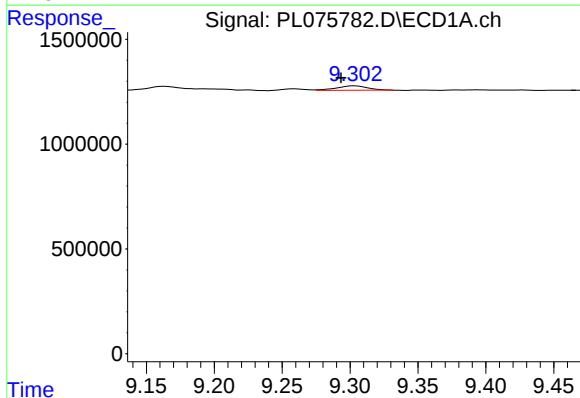


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.010 min
Response: 339518
Conc: 0.55 ng/ml

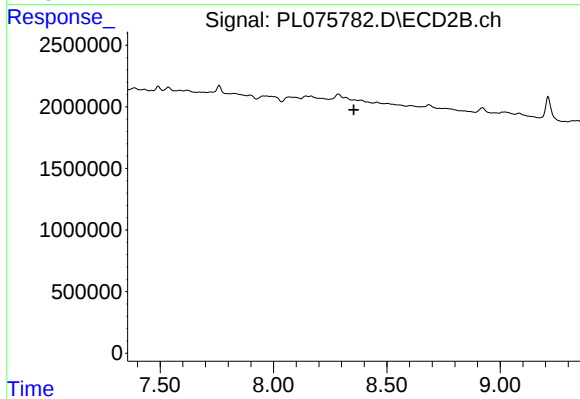

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

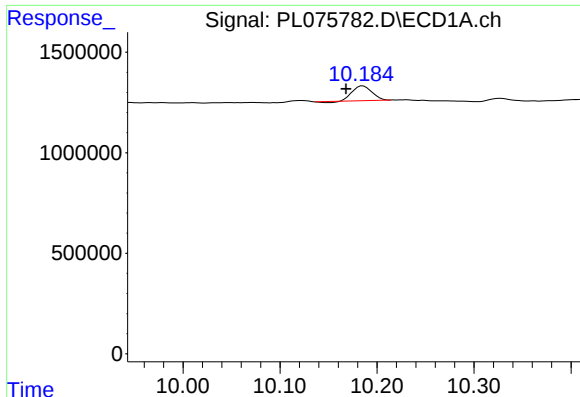

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 994015
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

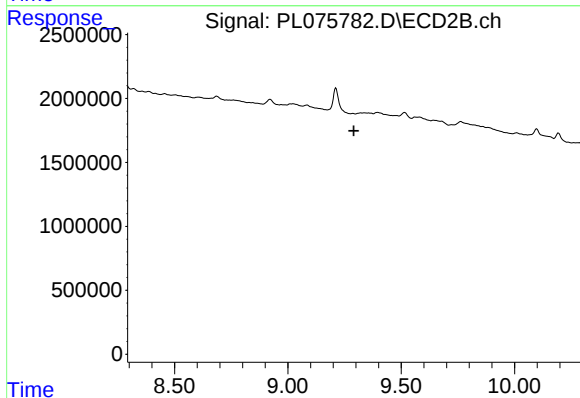


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

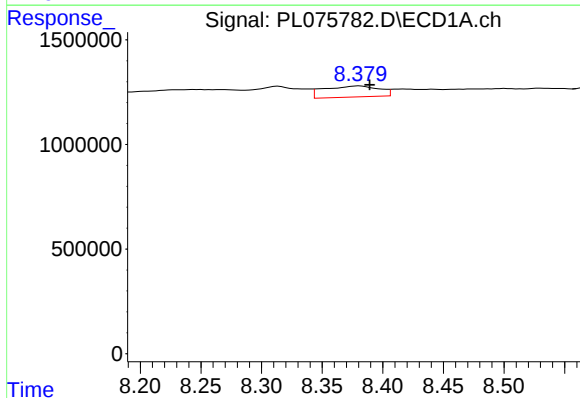


#25 Chlordane-3

R.T.: 8.381 min
Delta R.T.: -0.009 min
Response: 1659762
Conc: 16.07 ng/ml

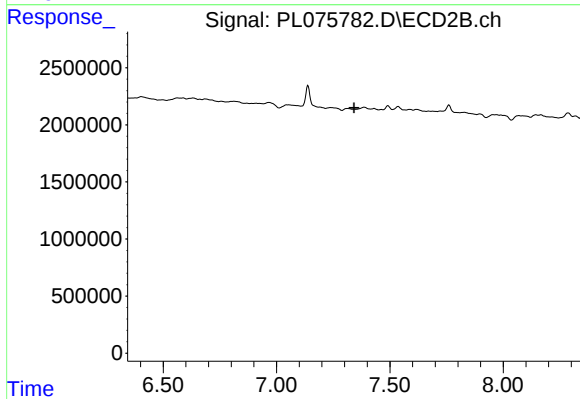

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

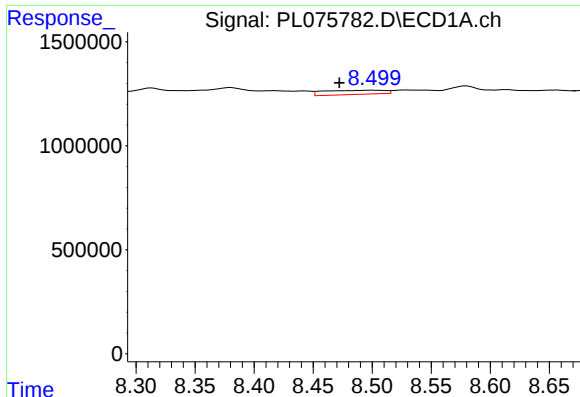

#26 Chlordane-4


R.T.: 8.501 min
Delta R.T.: 0.029 min
Response: 729514
Conc: 5.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

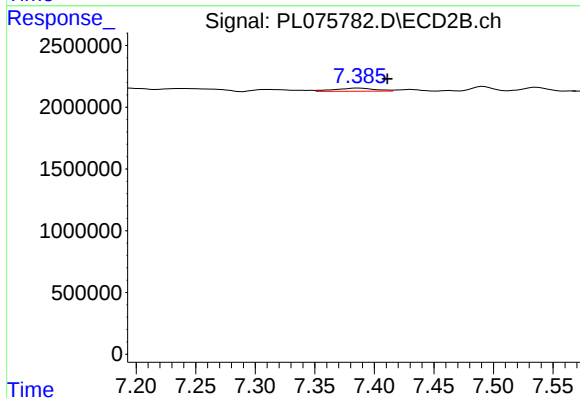


#26 Chlordane-4

R.T.: 7.387 min
Delta R.T.: -0.024 min
Response: 595517
Conc: 3.24 ng/ml

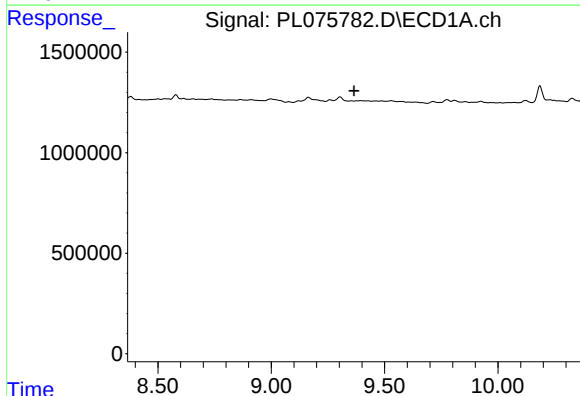


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

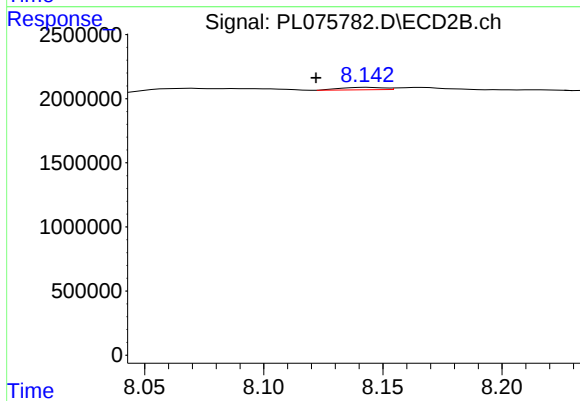

#27 Chlordane-5


R.T.: 8.143 min
Delta R.T.: 0.022 min
Response: 238005
Conc: 5.01 ng/ml

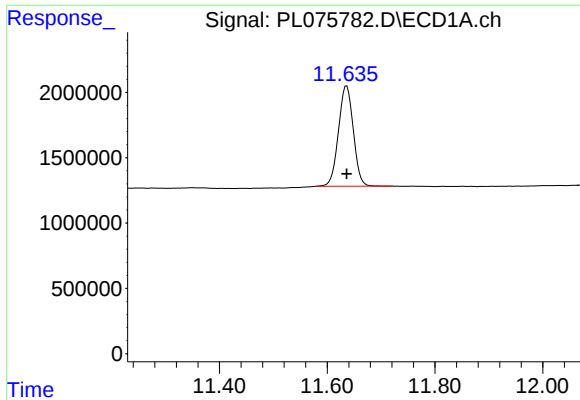

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 14698238
Conc: 24.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

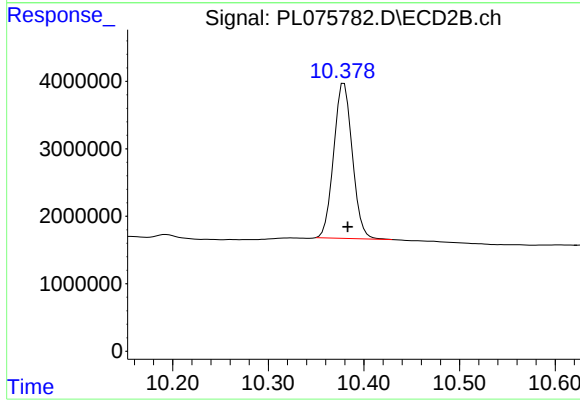

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 31054235
Conc: 22.04 ng/ml