

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061423\
 Data File : PL083426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2023 15:16
 Operator : AR\AJ
 Sample : 03214-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HYATT-PIPE-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 22:30:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	2.632	27734059	25245352	9.437	9.724
28)	SA Decachlor...	8.730	7.733	17216141	20912836	8.209	8.410
Target Compounds							
12)	B 4,4'-DDE	5.954	5.080	13502295	16342332	4.898	6.729 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061423\
Data File : PL083426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2023 15:16
Operator : AR\AJ
Sample : 03214-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HYATT-PIPE-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 22:30:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

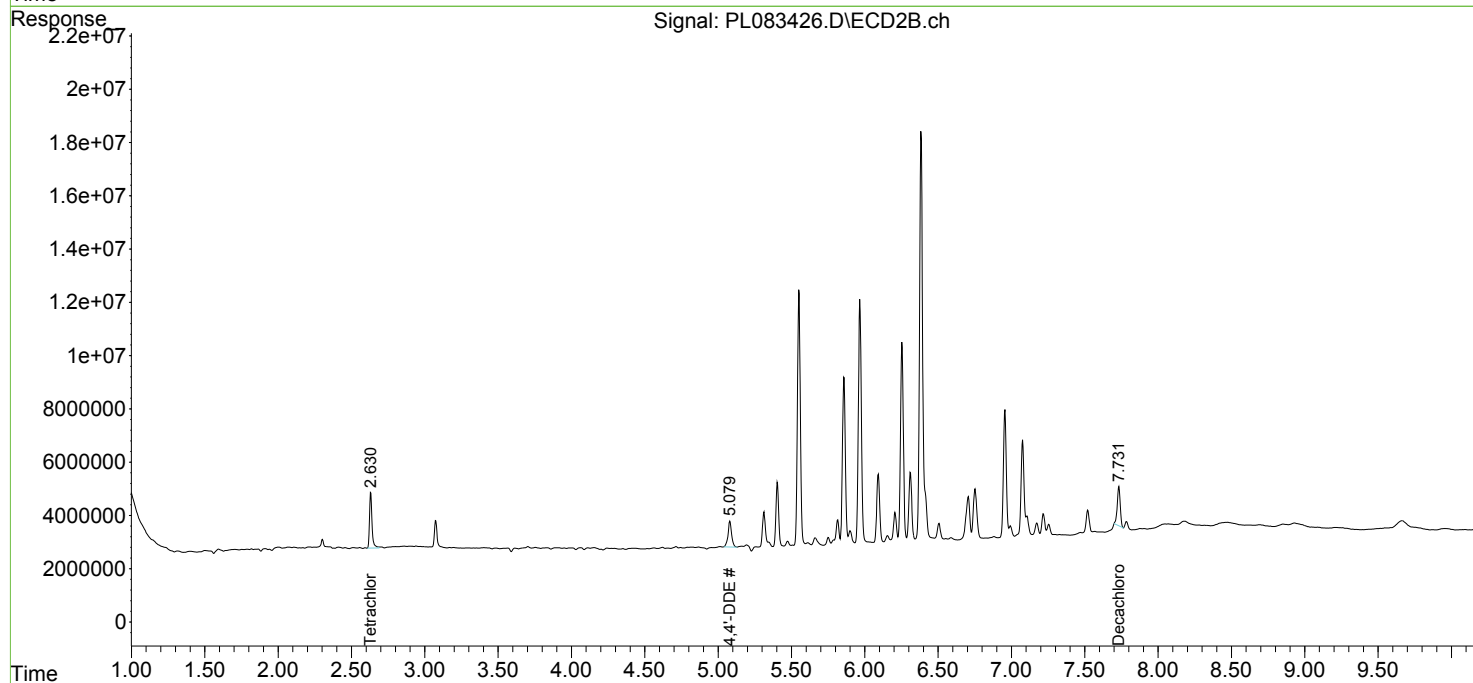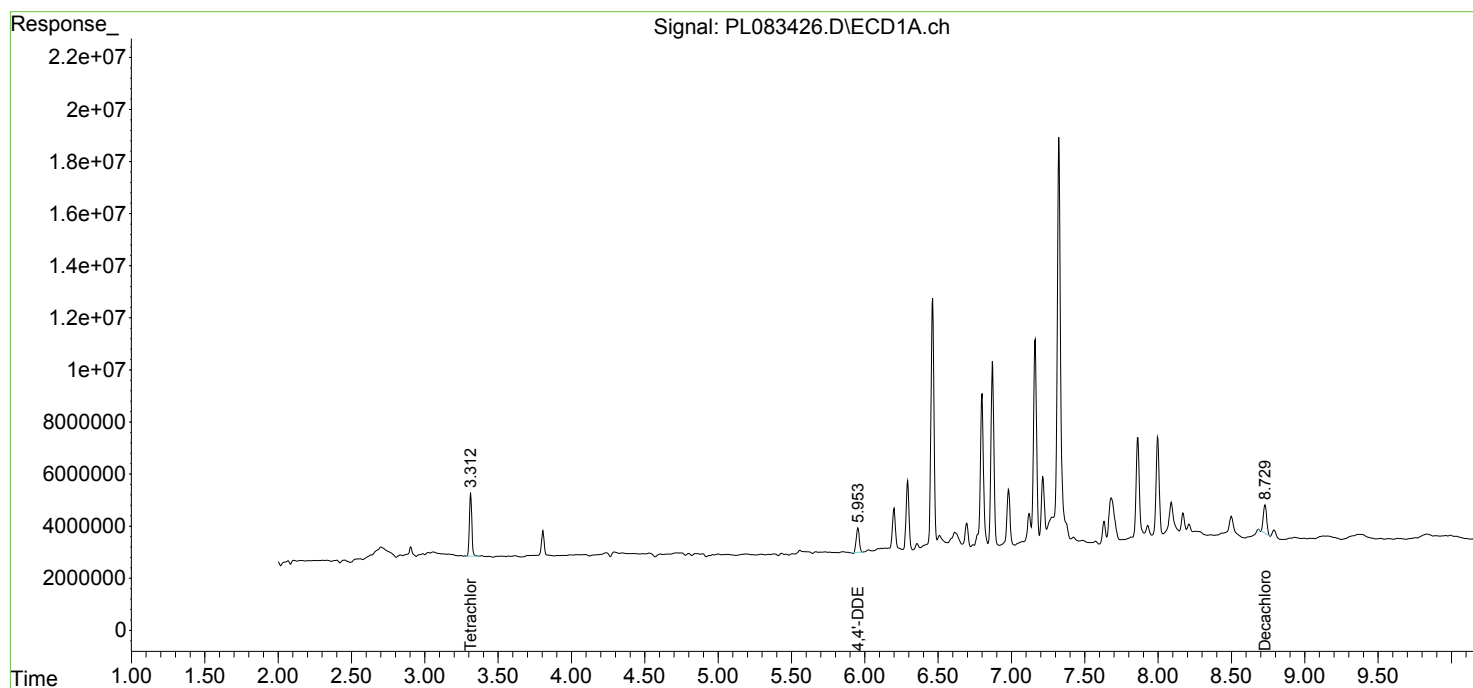


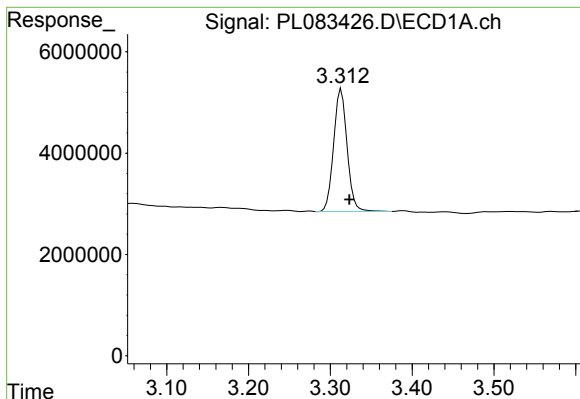

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.010 min
Response: 27734059
Conc: 9.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
HYATT-PIPE-TP

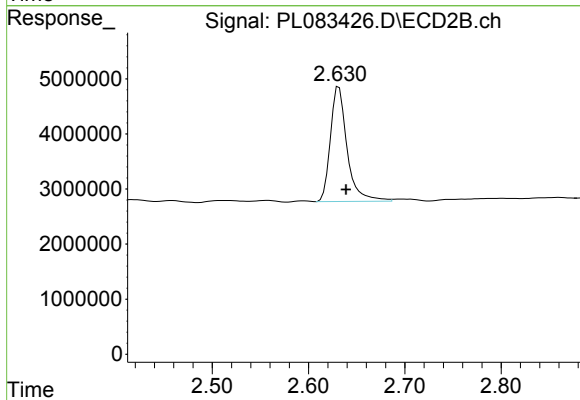


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: -0.007 min
Response: 25245352
Conc: 9.72 ng/ml

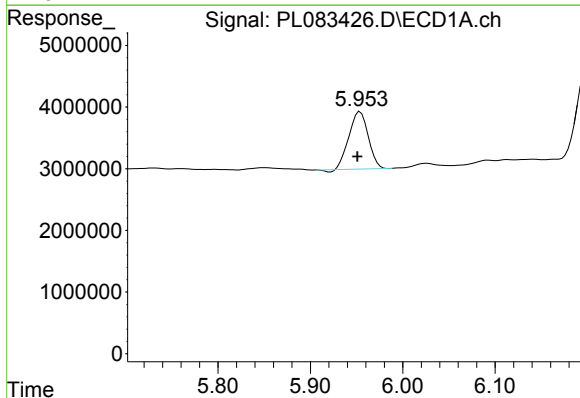


#12 4,4'-DDE

R.T.: 5.954 min
Delta R.T.: 0.003 min
Response: 13502295
Conc: 4.90 ng/ml

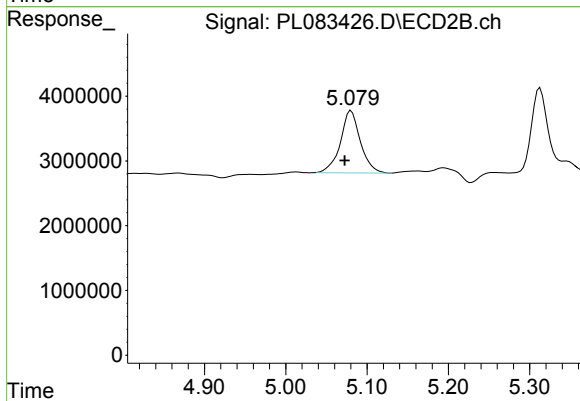

#12 4,4'-DDE


R.T.: 5.080 min
Delta R.T.: 0.008 min
Response: 16342332
Conc: 6.73 ng/ml

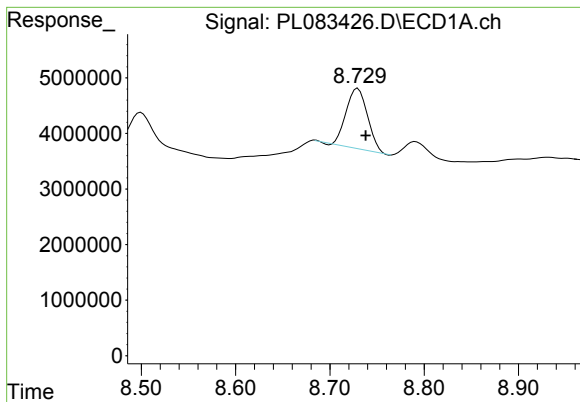

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.008 min
Response: 17216141
Conc: 8.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
HYATT-PIPE-TP

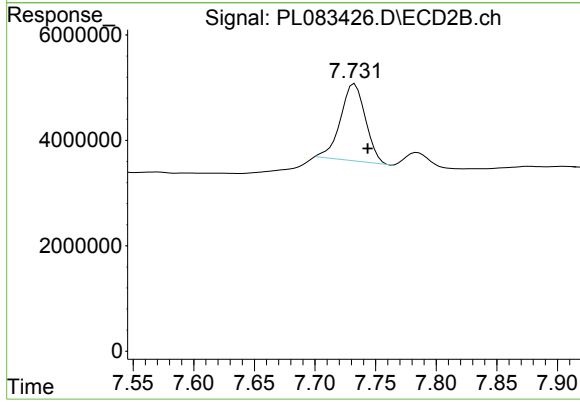

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: -0.011 min
Response: 20912836
Conc: 8.41 ng/ml