

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 05:24
 Operator : UA\AJ
 Sample : J3241-09 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 07:38:46 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.340	3.937	41373037	10543143	5.818	4.124 #
2) SA Decachlor...	8.023	8.949	26843389	12615236	4.126	4.945
Target Compounds						
6) B beta-BHC	4.260f	0.000	14260482	0	3.339	N.D. #
10) B gamma-Chl...	5.168f	0.000	10496891	0	1.248	N.D. #
12) B 4,4'-DDE	5.461	0.000	9572827	0	1.217	N.D. #
17) MA 4,4'-DDT	6.203	0.000	22720421	0	3.870	N.D. #
18) B Endrin al...	0.000	6.957	0	17860052	N.D.	9.184 #
23) Chlordane-1	4.189	0.000	6615030	0	22.958	N.D. #
24) Chlordane-2	4.688	0.000	4183135	0	13.618	N.D. #
25) Chlordane-3	5.168	0.000	10496891	0	11.167	N.D. #
27) Chlordane-5	0.000	6.957	0	17860052	N.D.	211.837 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 05:24
Operator : UA\AJ
Sample : J3241-09 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 07:38:46 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

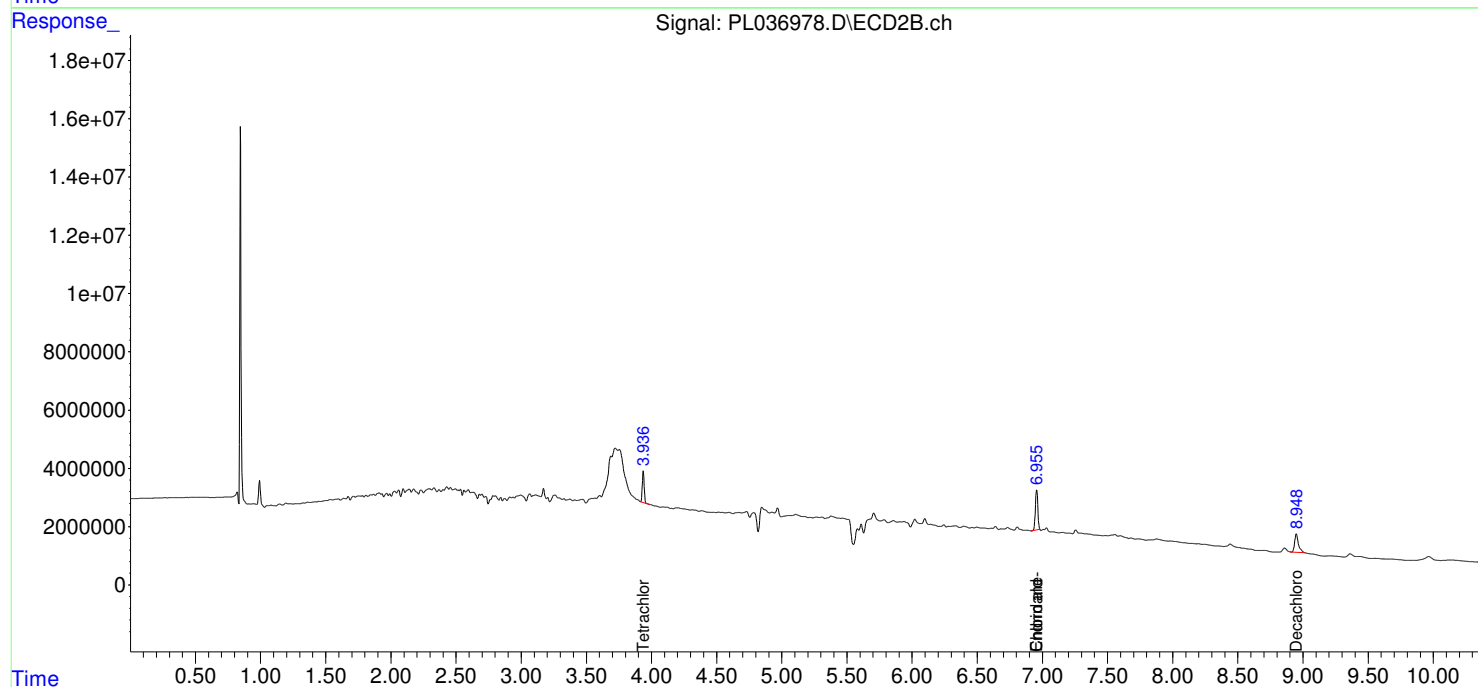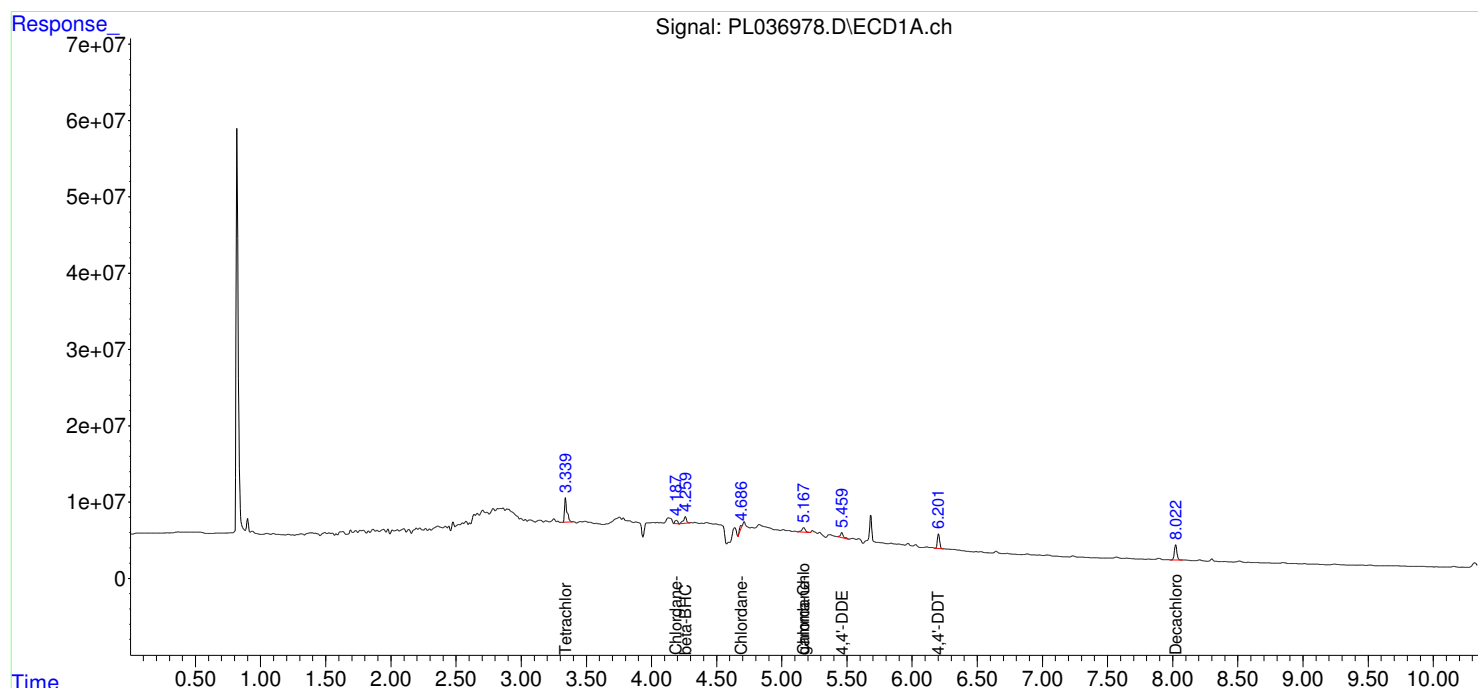


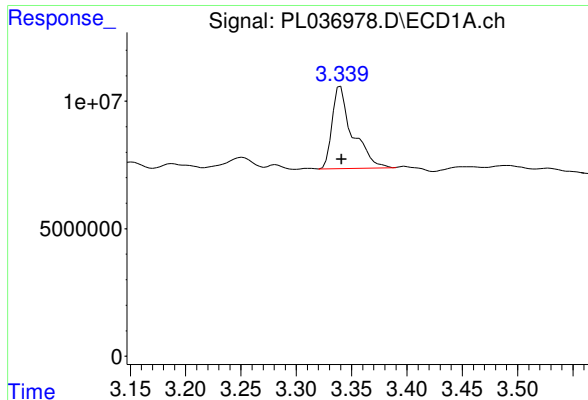

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.000 min
Response: 41373037
Conc: 5.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

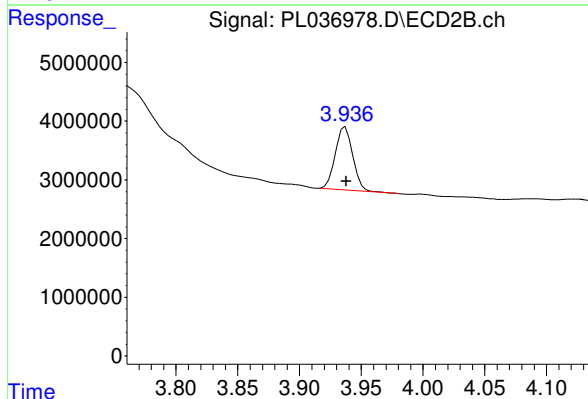


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 10543143
Conc: 4.12 ng/ml

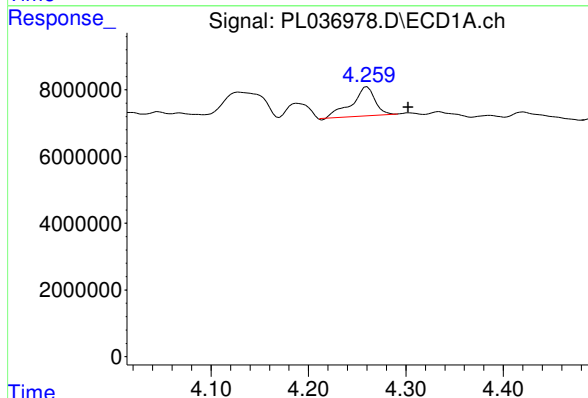


#6 beta-BHC

R.T.: 4.260 min
Delta R.T.: -0.042 min
Response: 14260482
Conc: 3.34 ng/ml

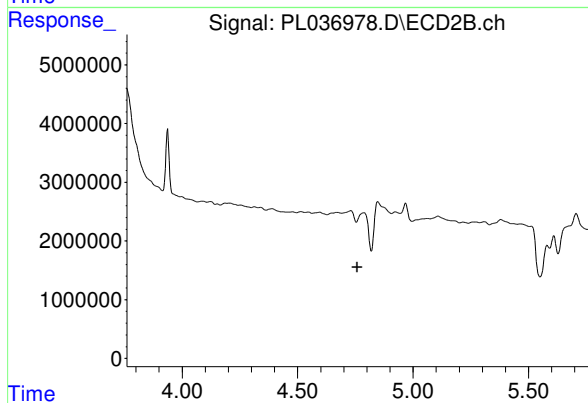

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

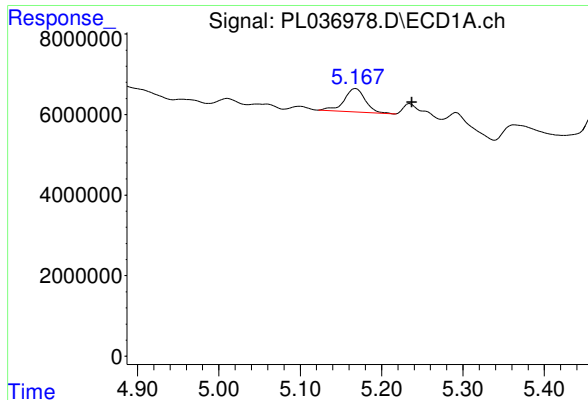

#10 gamma-Chlordane


R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 10496891
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

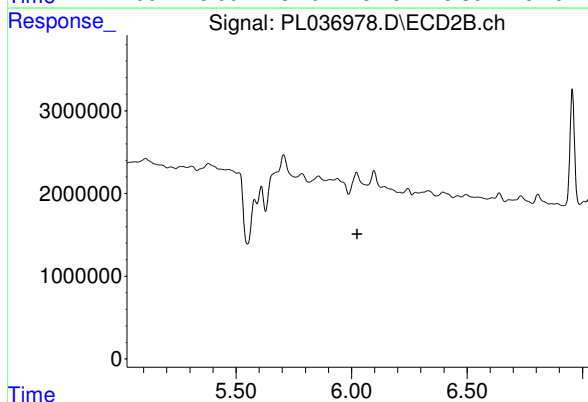


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

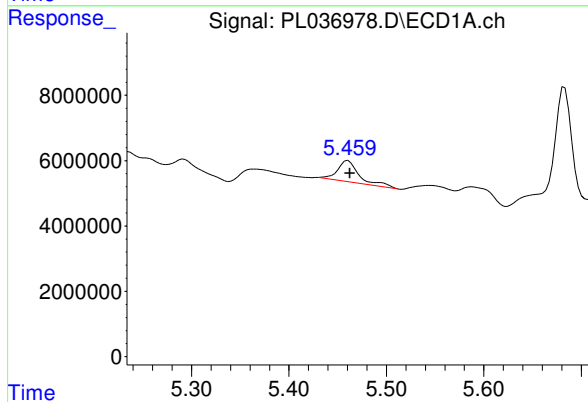


#12 4,4'-DDE

R.T.: 5.461 min
Delta R.T.: -0.002 min
Response: 9572827
Conc: 1.22 ng/ml

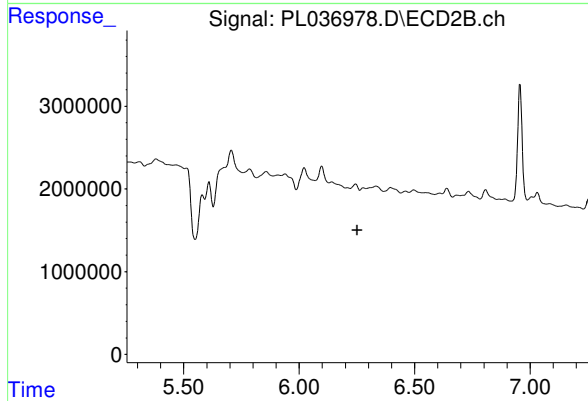

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

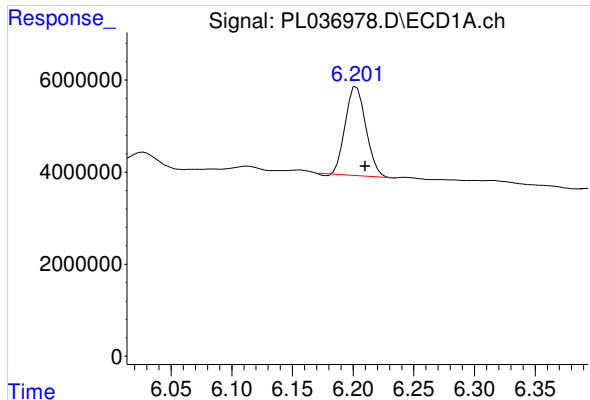

#17 4,4'-DDT


R.T.: 6.203 min
Delta R.T.: -0.007 min
Response: 22720421
Conc: 3.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

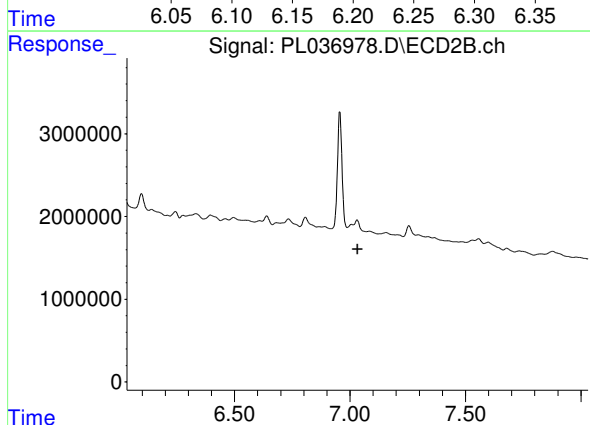


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.033 min
Response: 0
Conc: N.D.

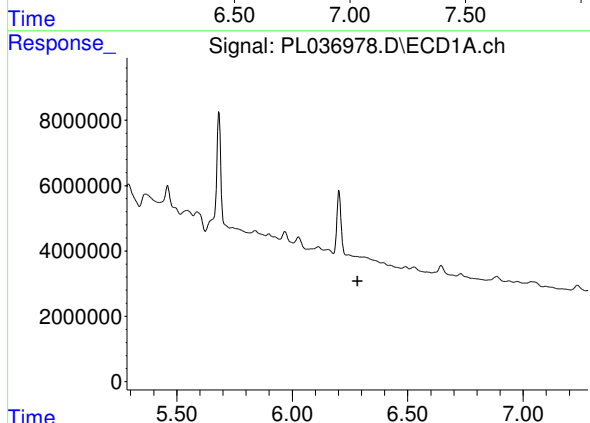


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.283 min
Response: 0
Conc: N.D.

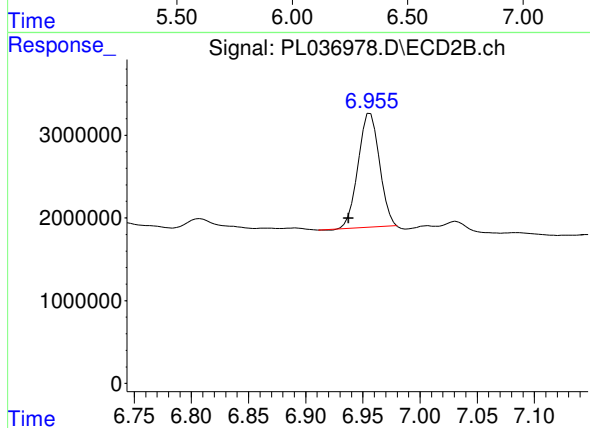

#18 Endrin aldehyde


R.T.: 6.957 min
Delta R.T.: 0.019 min
Response: 17860052
Conc: 9.18 ng/ml

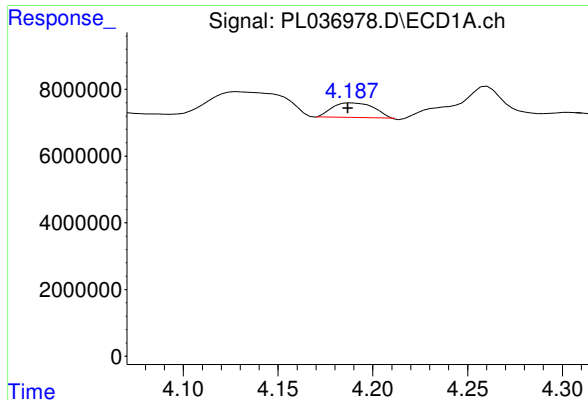

#23 Chlordane-1


R.T.: 4.189 min
Delta R.T.: 0.002 min
Response: 6615030
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

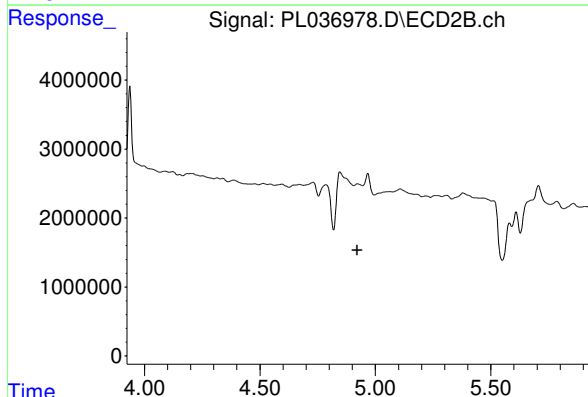


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

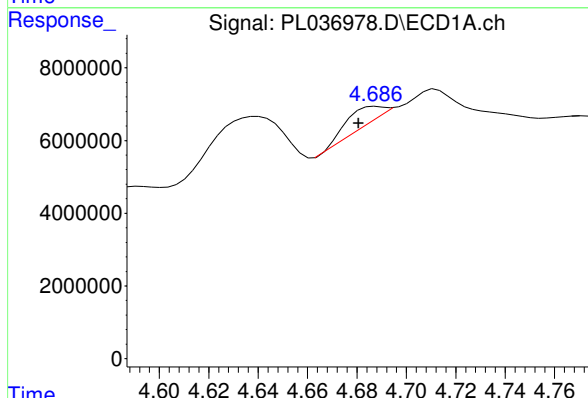


#24 Chlordane-2

R.T.: 4.688 min
Delta R.T.: 0.007 min
Response: 4183135
Conc: 13.62 ng/ml

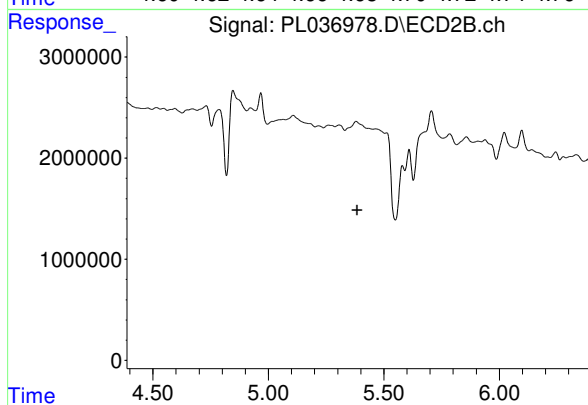

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.385 min
Response: 0
Conc: N.D.

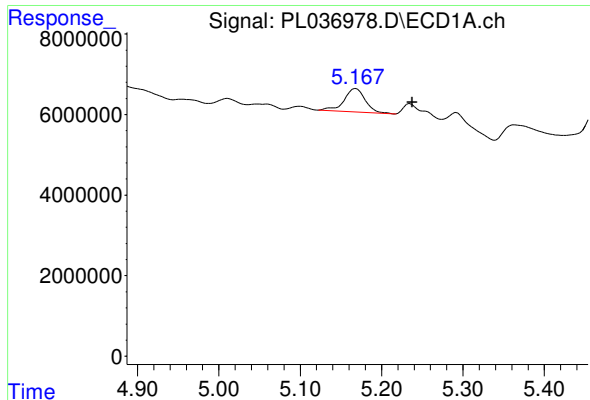

#25 Chlordane-3


R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 10496891
Conc: 11.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

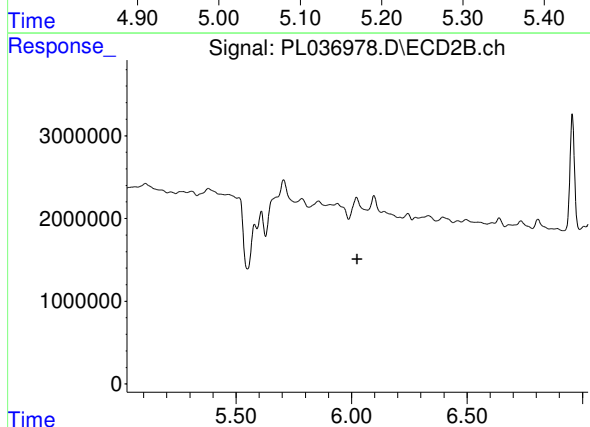


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

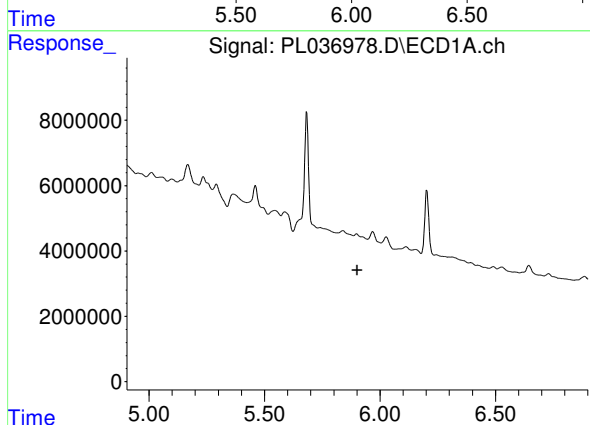


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.902 min
Response: 0
Conc: N.D.

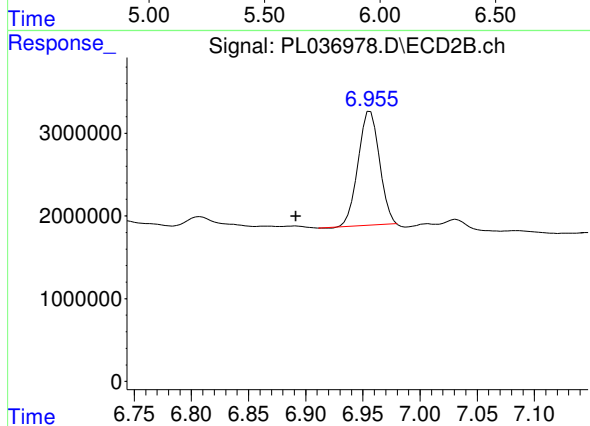

#27 Chlordane-5


R.T.: 6.957 min
Delta R.T.: 0.065 min
Response: 17860052
Conc: 211.84 ng/ml

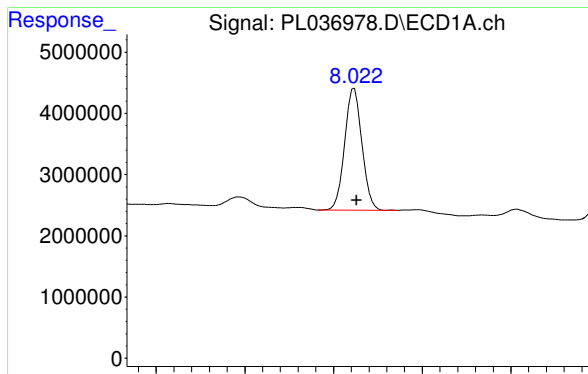

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.002 min
Response: 26843389
Conc: 4.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

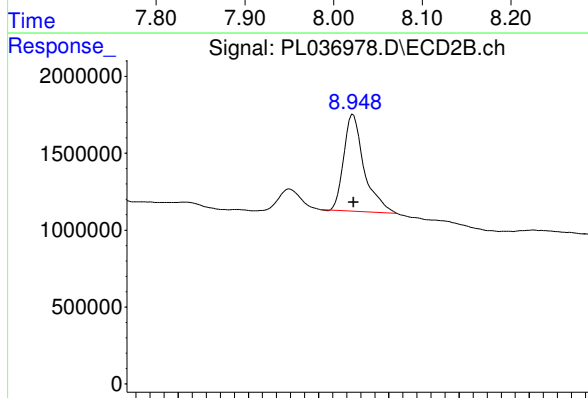

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 12615236
Conc: 4.95 ng/ml