

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 05:38
 Operator : UA\AJ
 Sample : J3241-11 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 07:38:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.340	3.937	28622620	9699564	4.025	3.794
28) SA Decachlor...	8.023	8.949	25061911	11643717	3.852	4.564
Target Compounds						
6) B beta-BHC	4.260f	0.000	20594565	0	4.822	N.D. #
10) B gamma-Chl...	5.168f	0.000	9342331	0	1.111	N.D. #
17) MA 4,4'-DDT	6.204	0.000	7021094	0	1.196	N.D. #
23) Chlordane-1	4.192	0.000	8662888	0	30.065	N.D. #
24) Chlordane-2	4.640	0.000	8010550	0	26.078	N.D. #
25) Chlordane-3	5.168	0.000	9342331	0	9.938	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 05:38
Operator : UA\AJ
Sample : J3241-11 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 07:38:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

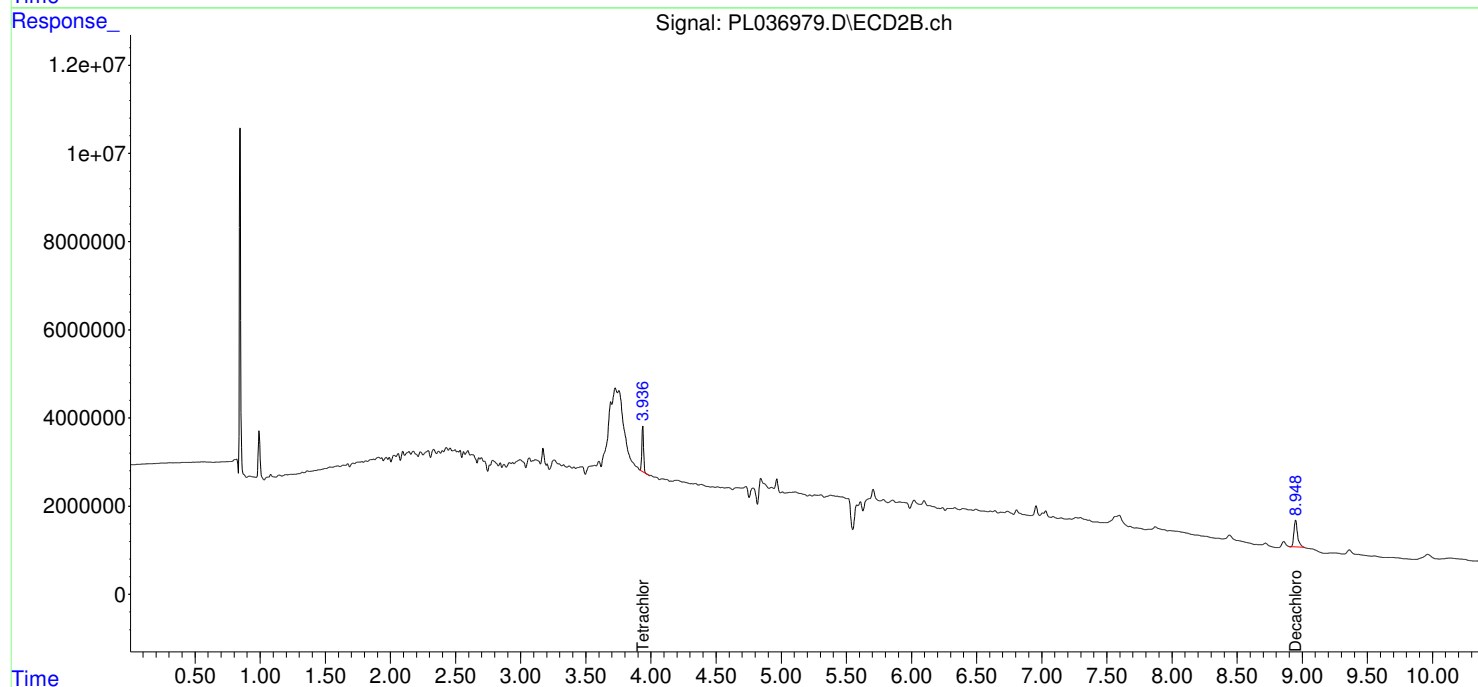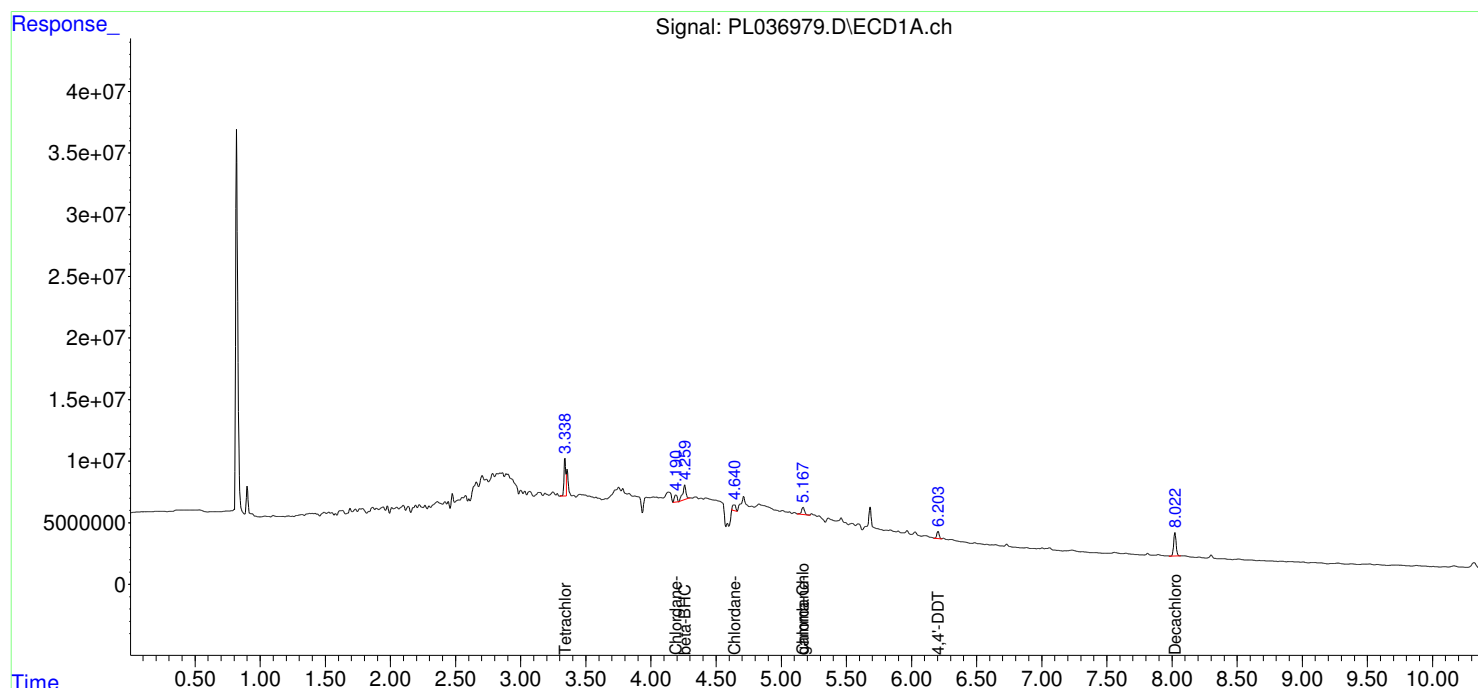


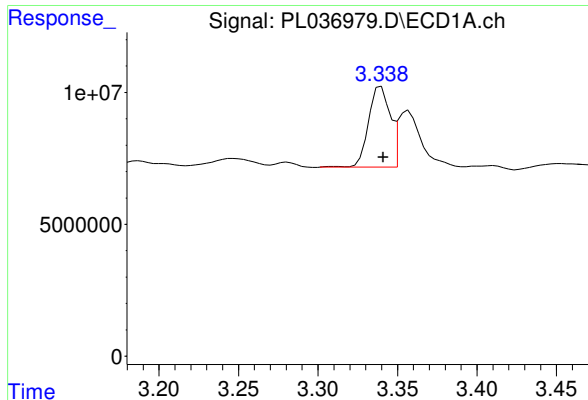

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 28622620
Conc: 4.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

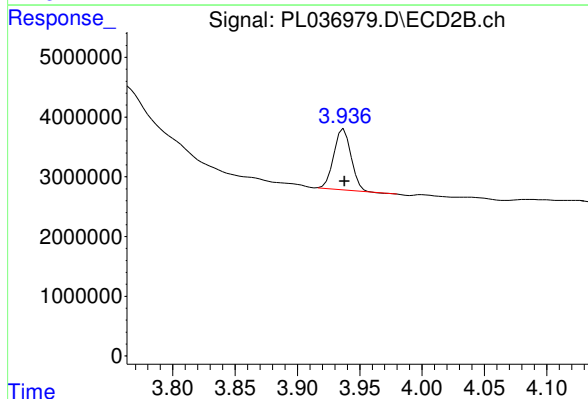


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 9699564
Conc: 3.79 ng/ml

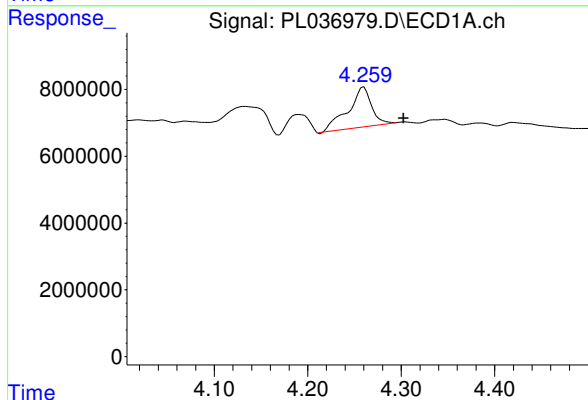


#6 beta-BHC

R.T.: 4.260 min
Delta R.T.: -0.042 min
Response: 20594565
Conc: 4.82 ng/ml

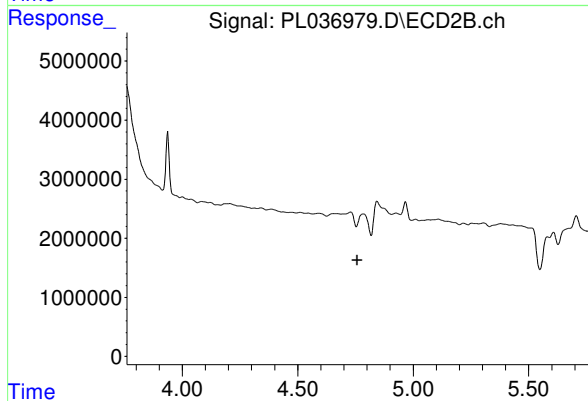

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

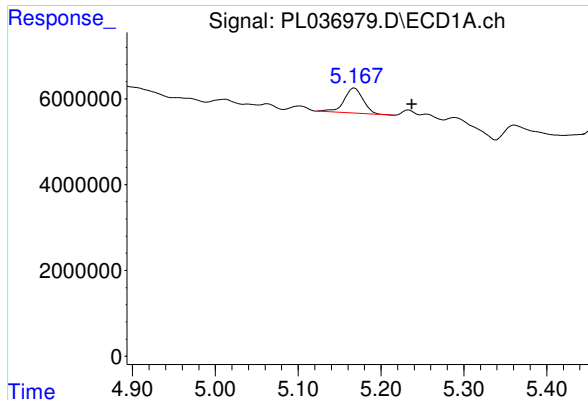

#10 gamma-Chlordane


R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 9342331
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

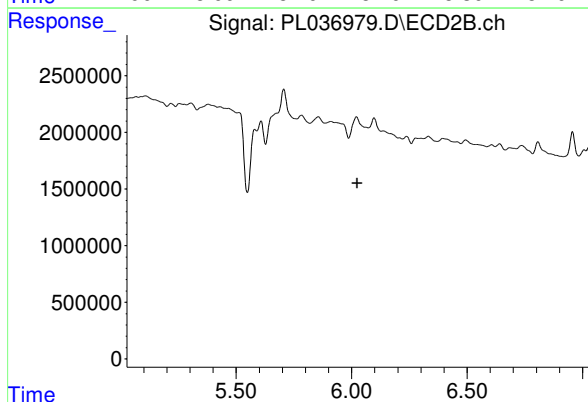


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

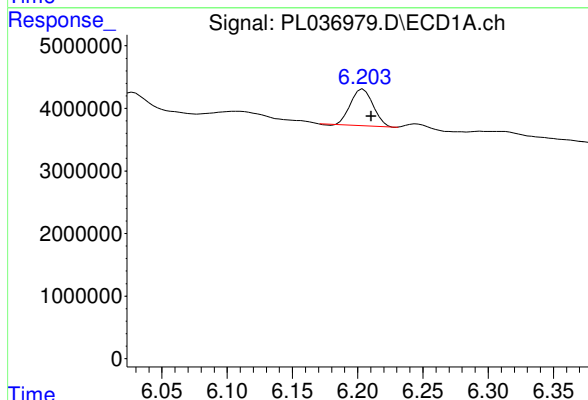


#17 4,4'-DDT

R.T.: 6.204 min
Delta R.T.: -0.006 min
Response: 7021094
Conc: 1.20 ng/ml

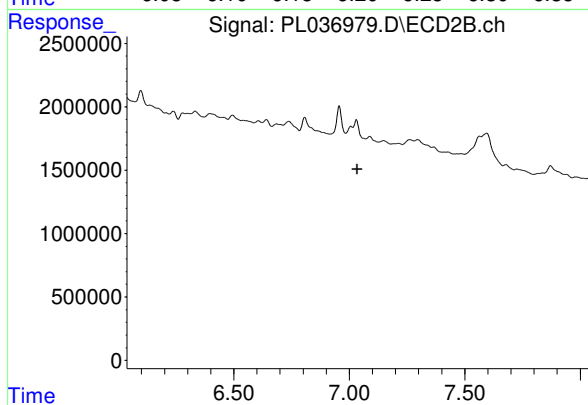

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

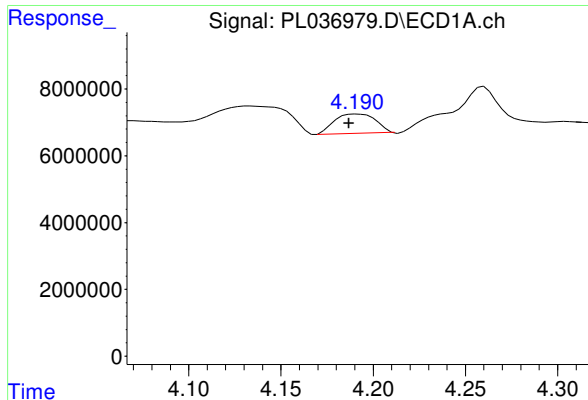

#23 Chlordane-1


R.T.: 4.192 min
Delta R.T.: 0.005 min
Response: 8662888
Conc: 30.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

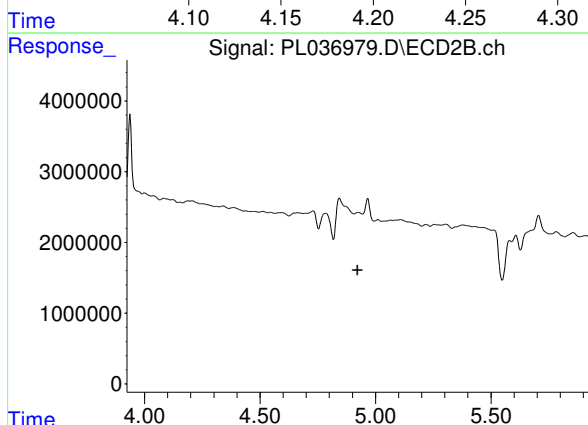


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

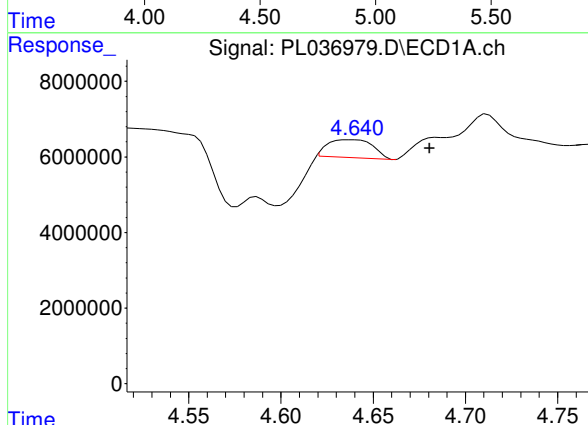


#24 Chlordane-2

R.T.: 4.640 min
Delta R.T.: -0.041 min
Response: 8010550
Conc: 26.08 ng/ml

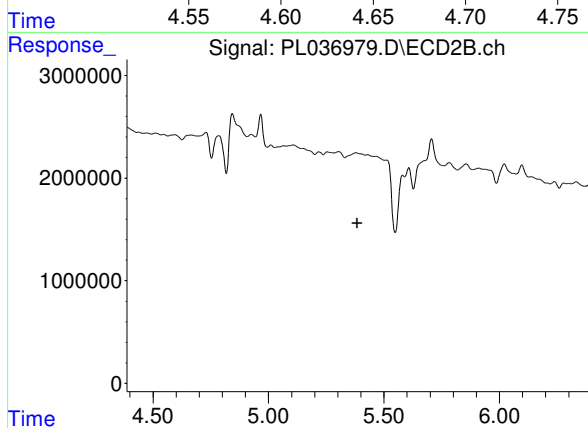

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.385 min
Response: 0
Conc: N.D.

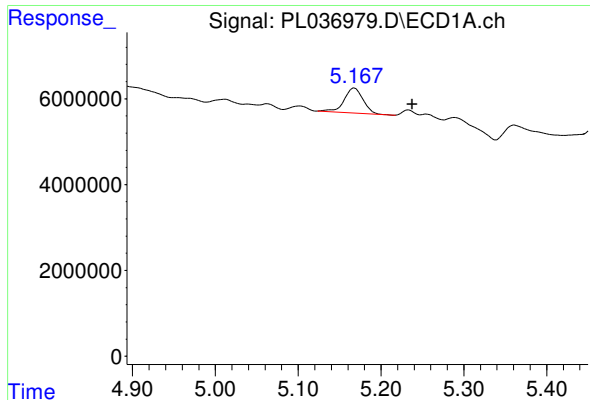

#25 Chlordane-3


R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 9342331
Conc: 9.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

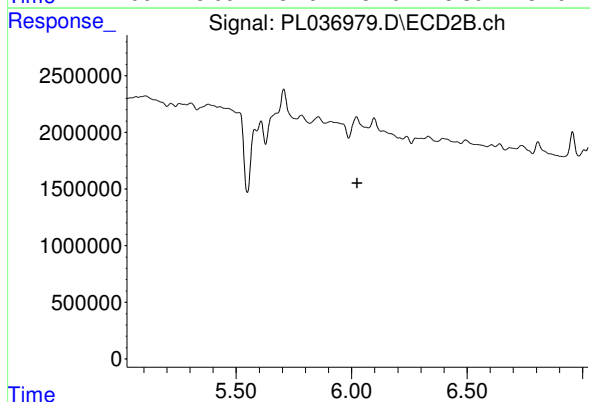


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

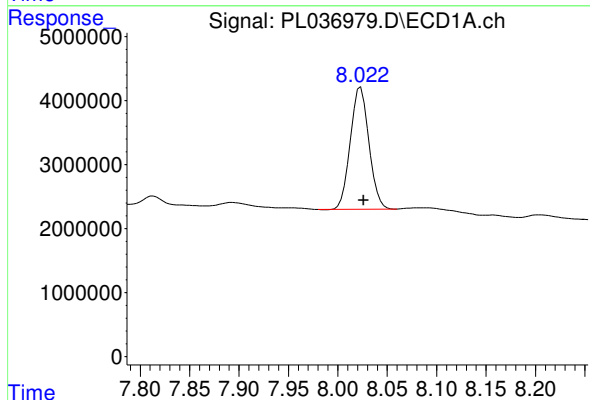

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.003 min
Response: 25061911
Conc: 3.85 ng/ml

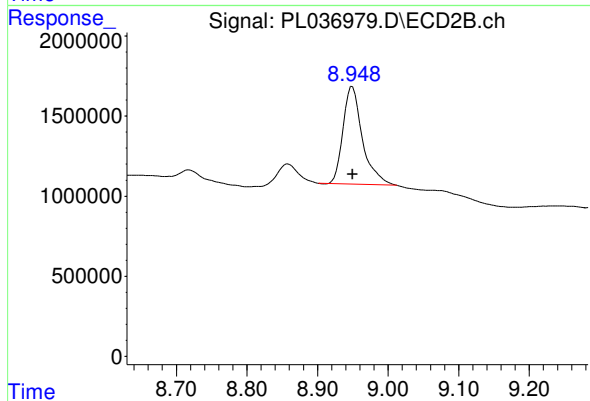

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 11643717
Conc: 4.56 ng/ml