

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 05:52
 Operator : UA\AJ
 Sample : J3239-09
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 07:38:55 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	83691558	30192923	11.769	11.810
28)	SA Decachlor...	8.025	8.950	49109879	20738629	7.548	8.130
Target Compounds							
4)	MA Heptachlor	4.340	0.000	22479470	0	2.435	N.D. #
5)	MB Aldrin	4.552	0.000	11097706	0	1.201	N.D. #
6)	B beta-BHC	4.340f	0.000	22479470	0	5.264	N.D. #
7)	B delta-BHC	4.512	0.000	4309205	0	0.449	N.D. #
10)	B gamma-Chl...	5.169f	0.000	8431383	0	1.003	N.D. #
12)	B 4,4'-DDE	5.461	0.000	9214814	0	1.172	N.D. #
23)	Chlordane-1	4.137	0.000	17899498	0	62.121	N.D. #
25)	Chlordane-3	5.169	0.000	8431383	0	8.969	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 05:52
Operator : UA\AJ
Sample : J3239-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 07:38:55 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

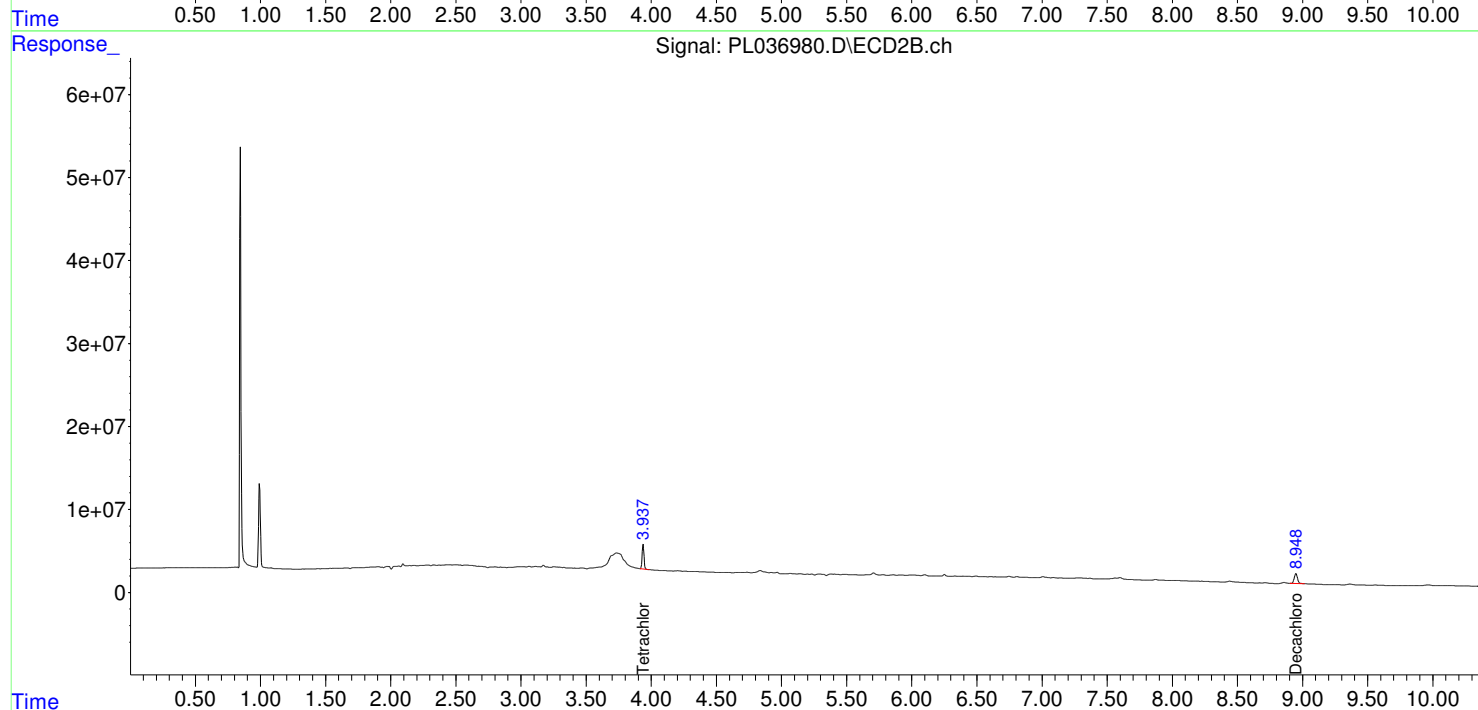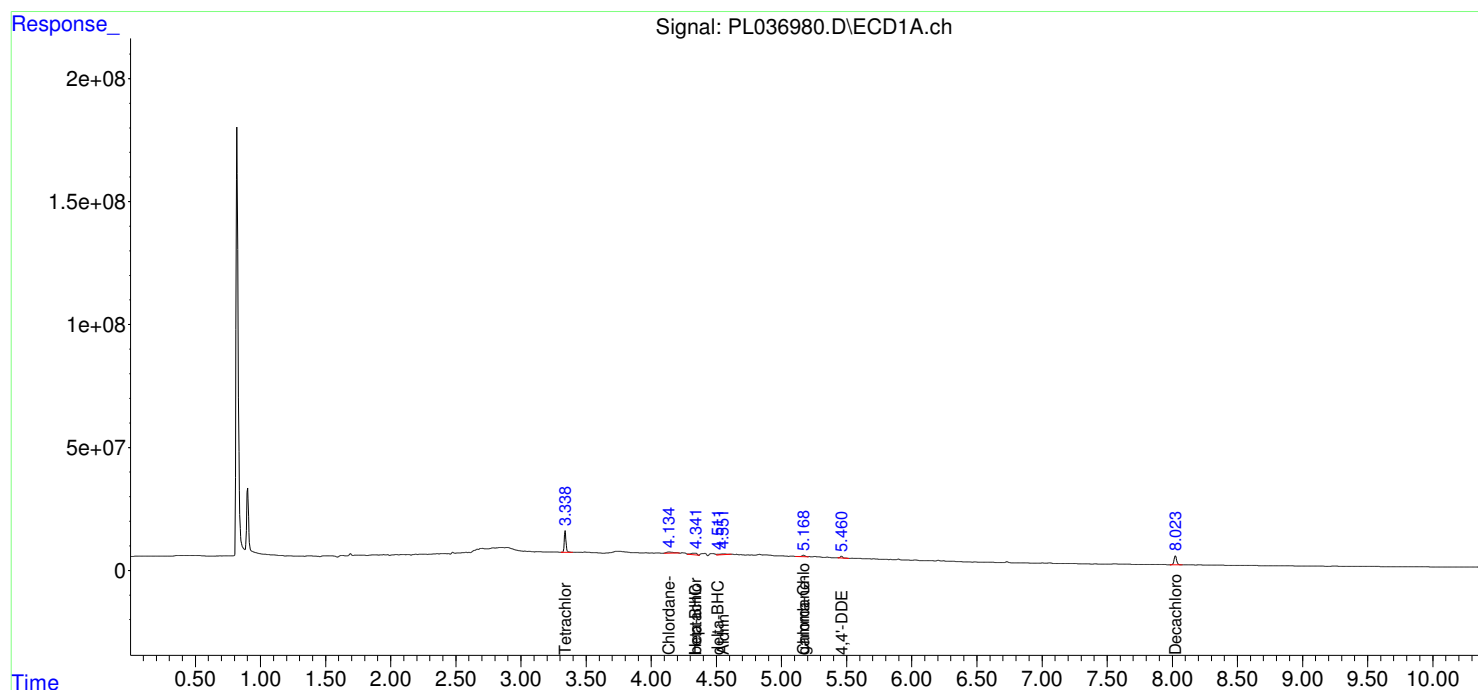


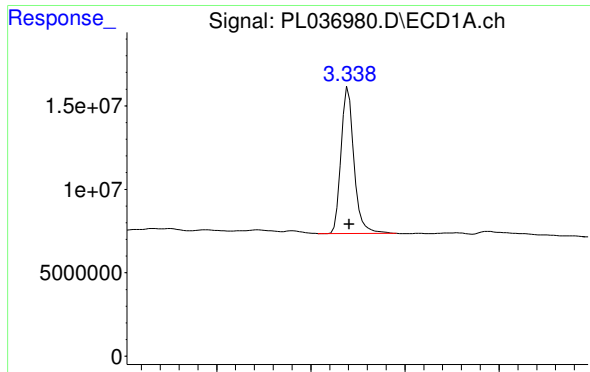

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 83691558
Conc: 11.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

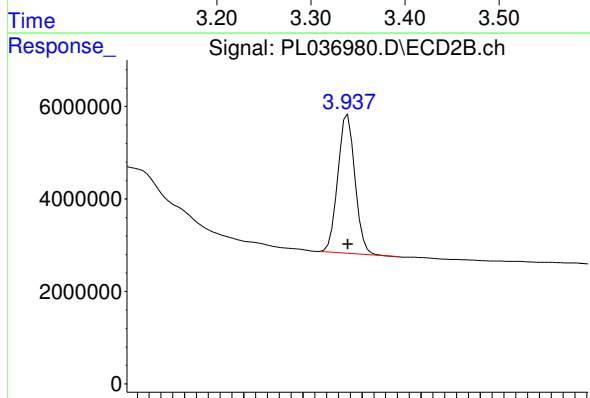


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 30192923
Conc: 11.81 ng/ml

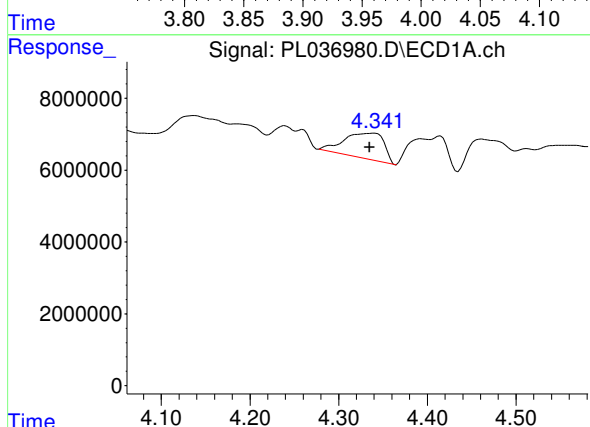


#4 Heptachlor

R.T.: 4.340 min
Delta R.T.: 0.005 min
Response: 22479470
Conc: 2.43 ng/ml

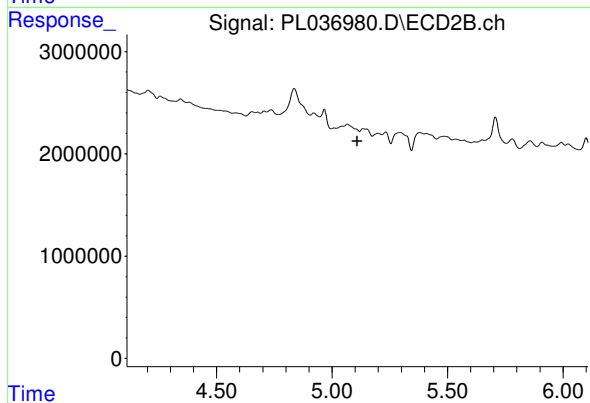

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.109 min
Response: 0
Conc: N.D.

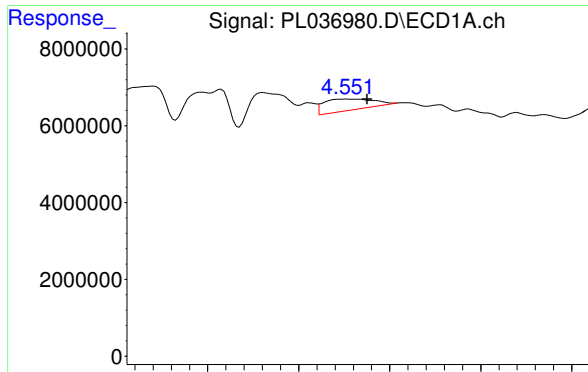

#5 Aldrin


R.T.: 4.552 min
Delta R.T.: -0.024 min
Response: 11097706
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

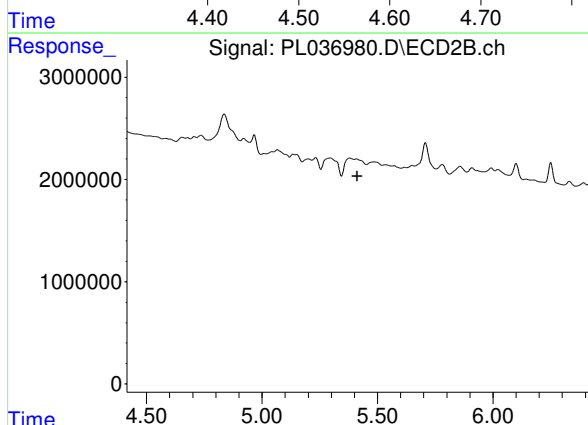


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

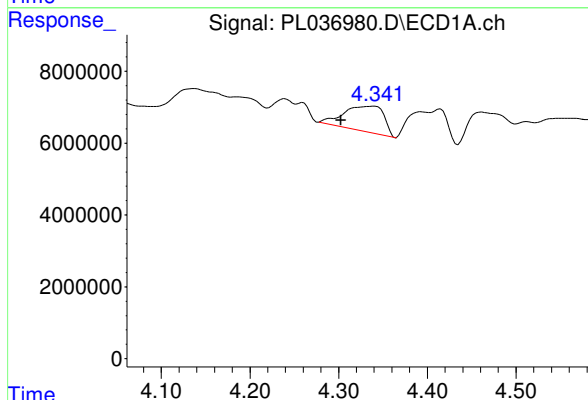


#6 beta-BHC

R.T.: 4.340 min
Delta R.T.: 0.037 min
Response: 22479470
Conc: 5.26 ng/ml

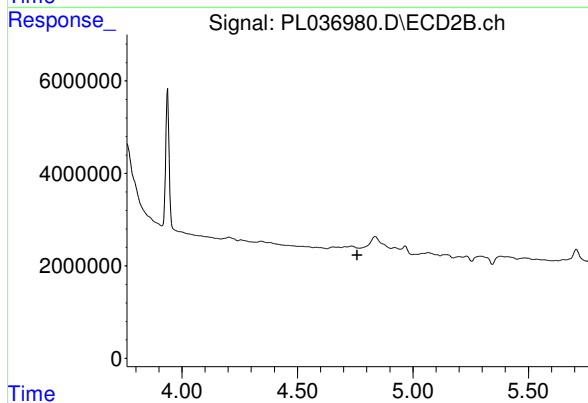

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

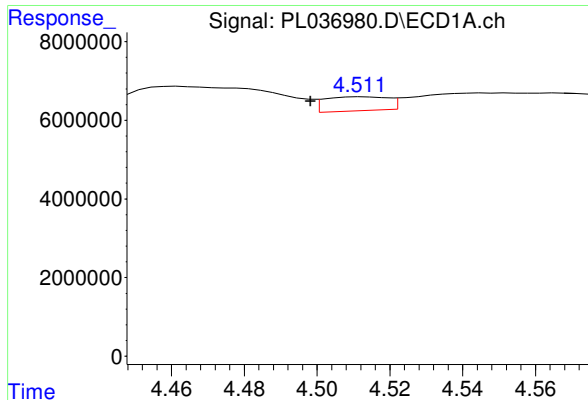

#7 delta-BHC


R.T.: 4.512 min
Delta R.T.: 0.014 min
Response: 4309205
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

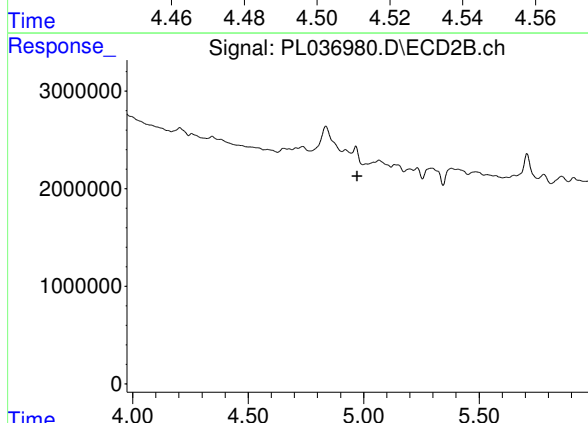


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

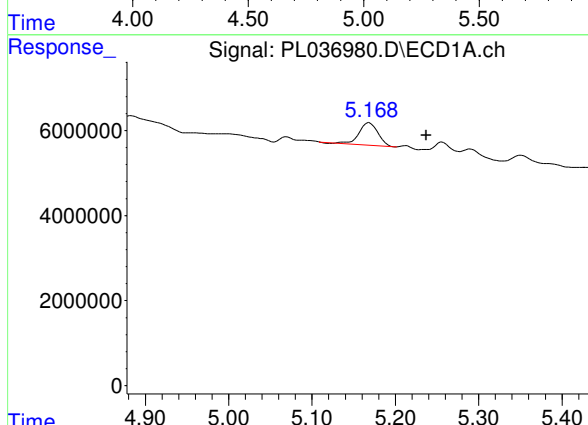


#10 gamma-Chlordane

R.T.: 5.169 min
Delta R.T.: -0.068 min
Response: 8431383
Conc: 1.00 ng/ml

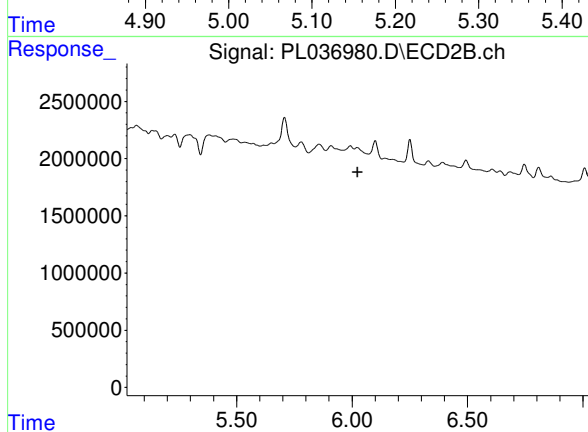

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

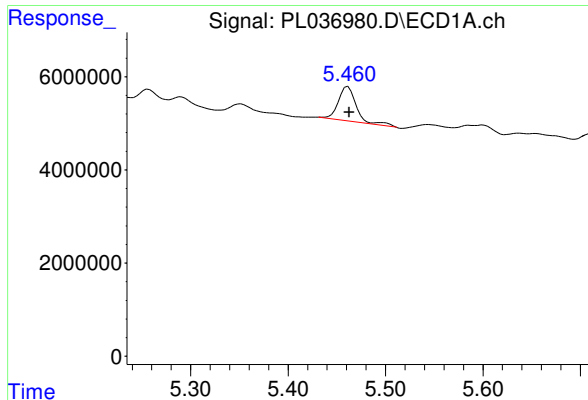

#12 4,4'-DDE


R.T.: 5.461 min
Delta R.T.: -0.001 min
Response: 9214814
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

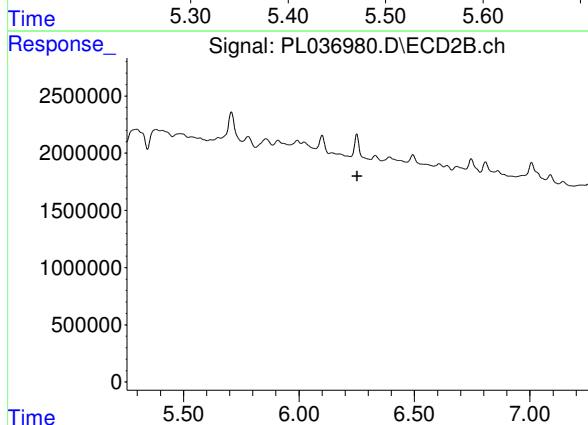


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

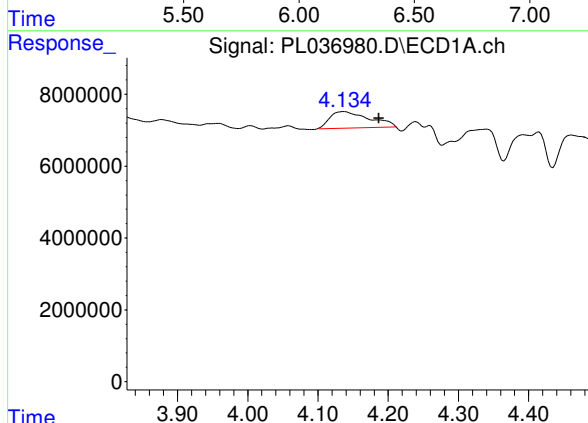


#23 Chlordane-1

R.T.: 4.137 min
Delta R.T.: -0.050 min
Response: 17899498
Conc: 62.12 ng/ml

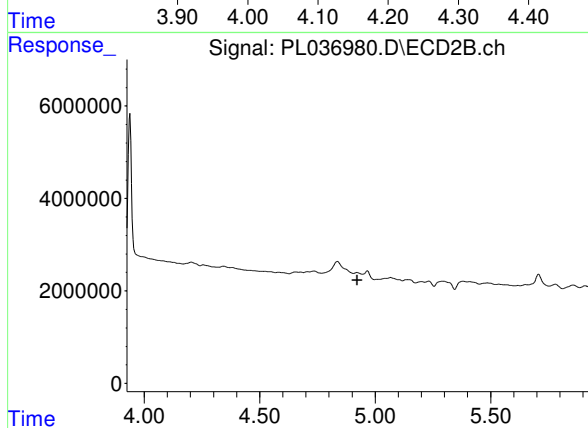

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

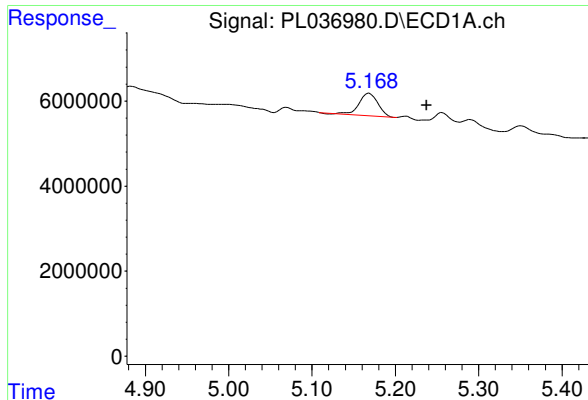

#25 Chlordane-3


R.T.: 5.169 min
Delta R.T.: -0.069 min
Response: 8431383
Conc: 8.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

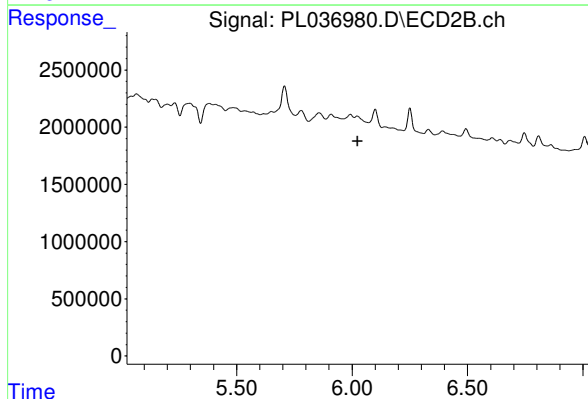


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

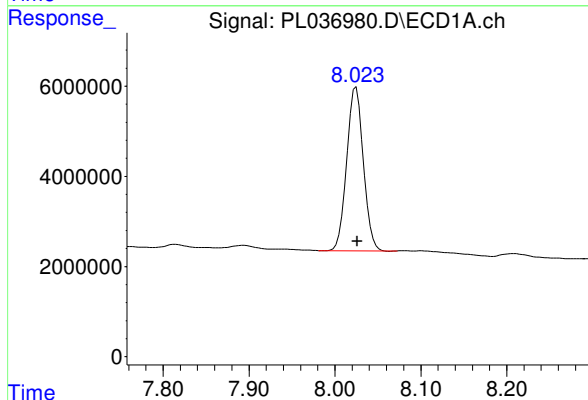

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: -0.001 min
Response: 49109879
Conc: 7.55 ng/ml

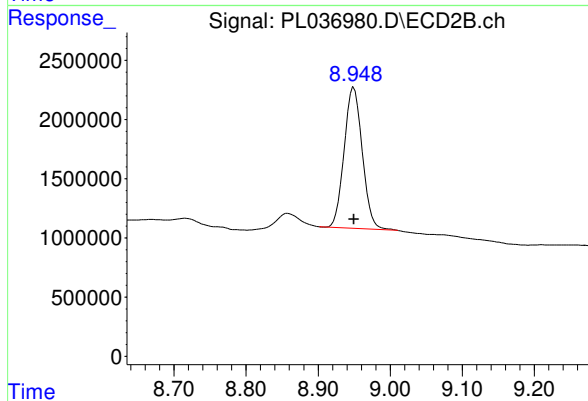

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 20738629
Conc: 8.13 ng/ml