

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 08:12
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:08:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.339	3.938	123.5E6	43859477	17.361	17.156
28)	SA Decachlor...	8.023	8.949	117.2E6	44519111	18.017	17.452
Target Compounds							
6)	B beta-BHC	4.260f	0.000	5114315	0	1.198	N.D. #
8)	B Heptachlo...	0.000	5.782	0	28241620	N.D.	10.235 #
10)	B gamma-Chl...	5.168f	0.000	14106759	0	1.677	N.D. #
14)	MA Endrin	5.857	0.000	27014324	0	3.877	N.D. #
23)	Chlordane-1	4.126	0.000	24763011	0	85.942	N.D. #
24)	Chlordane-2	0.000	5.319	0	34502749	N.D.	297.244 #
25)	Chlordane-3	5.168	0.000	14106759	0	15.007	N.D. #
27)	Chlordane-5	5.857	0.000	27014324	0	216.577	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 08:12
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:08:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

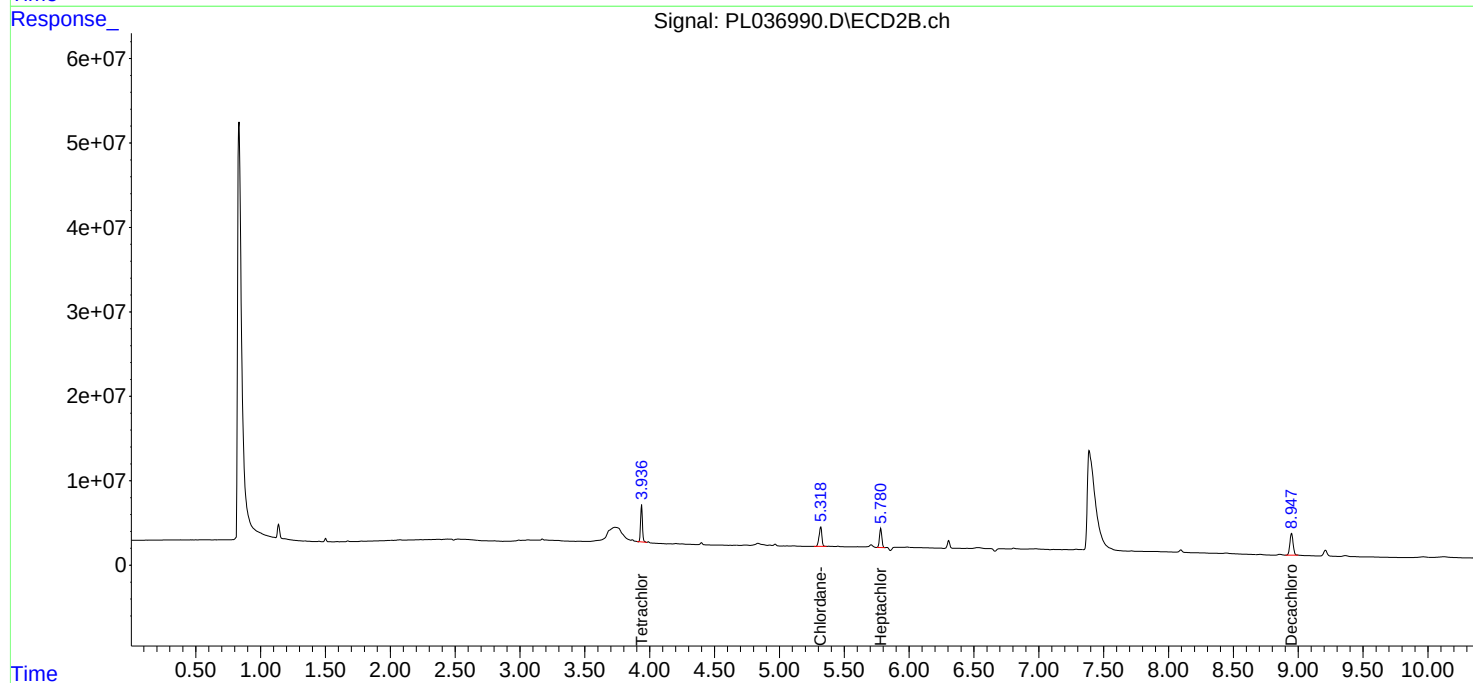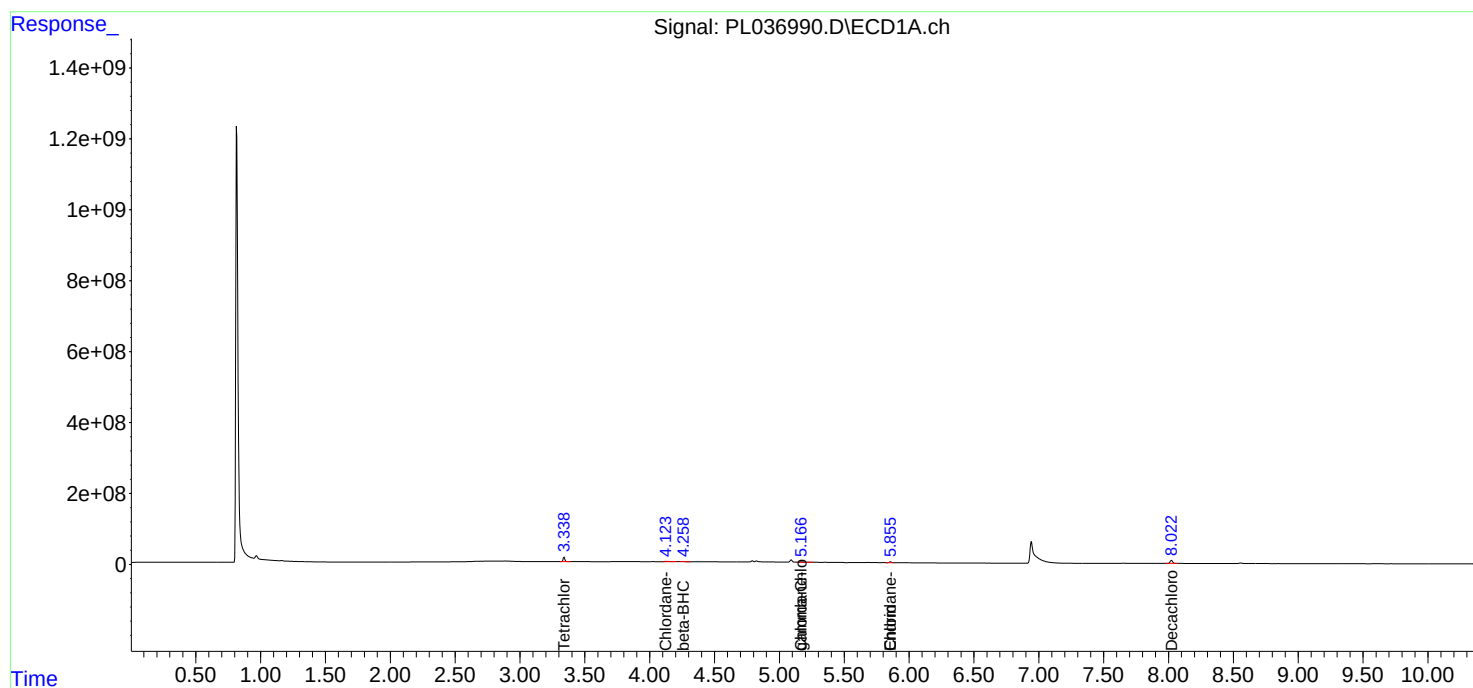


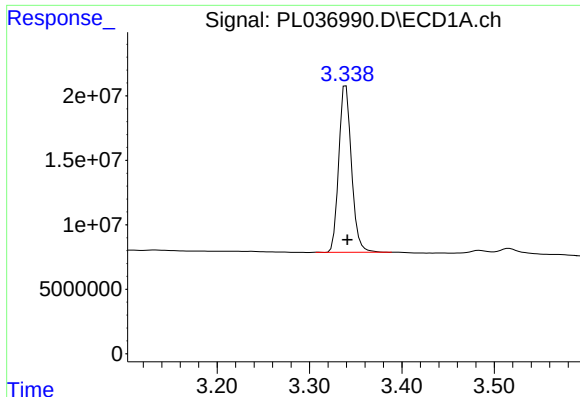

#1 Tetrachloro-m-xylene


R.T.: 3.339 min
Delta R.T.: -0.002 min
Response: 123458191
Conc: 17.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

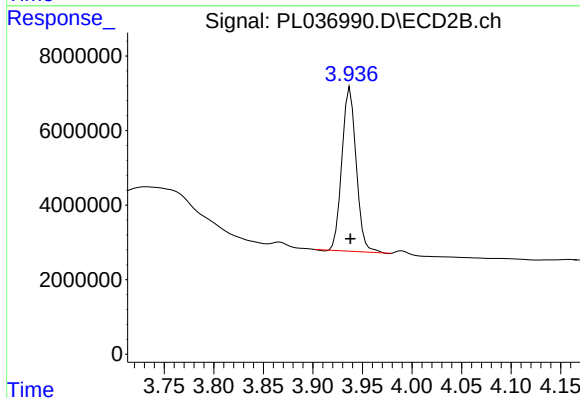


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 43859477
Conc: 17.16 ng/ml

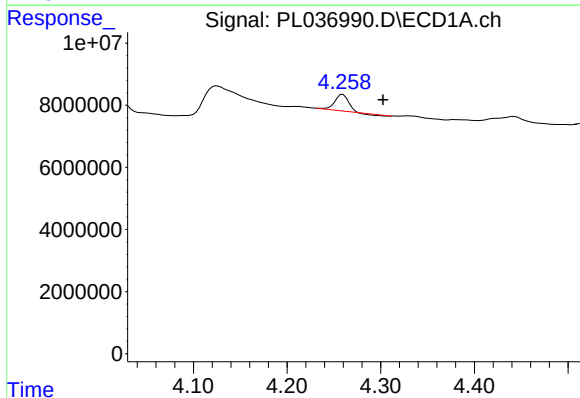


#6 beta-BHC

R.T.: 4.260 min
Delta R.T.: -0.043 min
Response: 5114315
Conc: 1.20 ng/ml

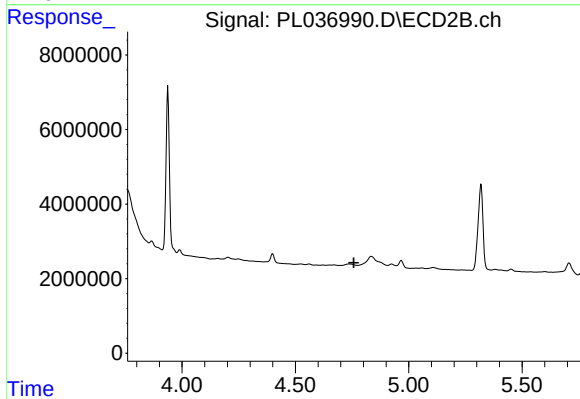

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

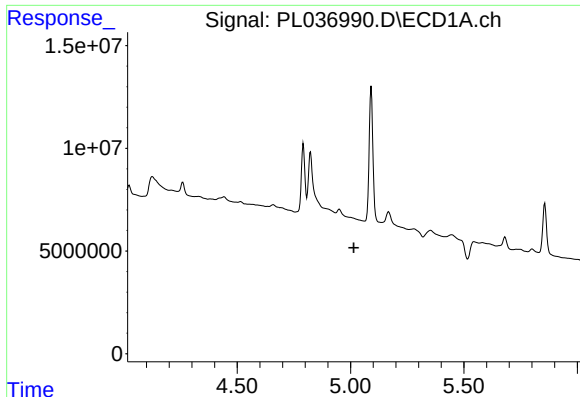

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

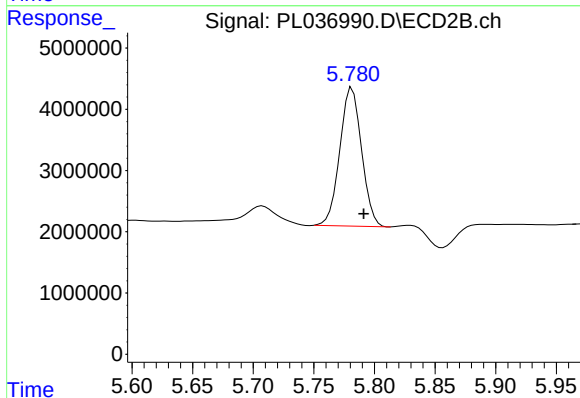


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.010 min
Response: 28241620
Conc: 10.24 ng/ml

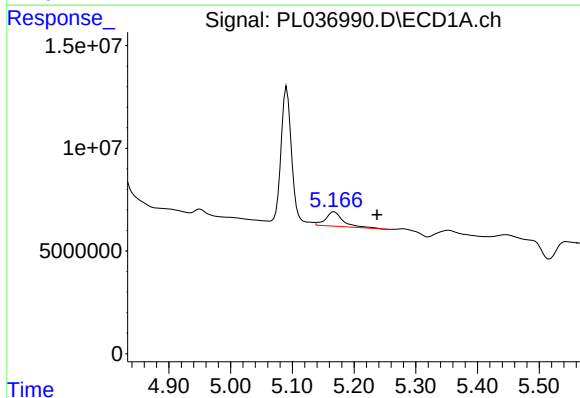


#10 gamma-Chlordane

R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 14106759
Conc: 1.68 ng/ml

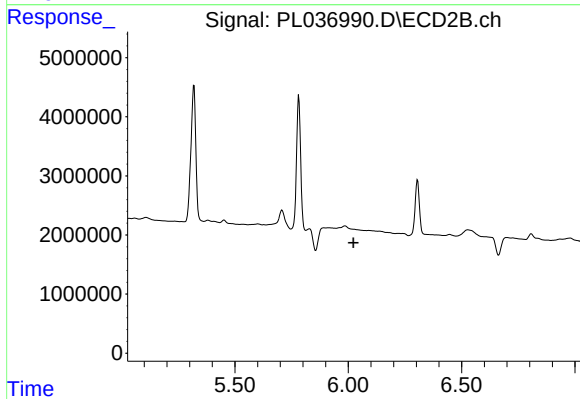

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

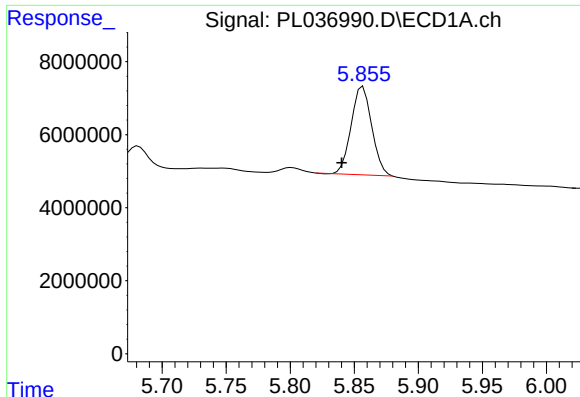

#14 Endrin


R.T.: 5.857 min
Delta R.T.: 0.016 min
Response: 27014324
Conc: 3.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

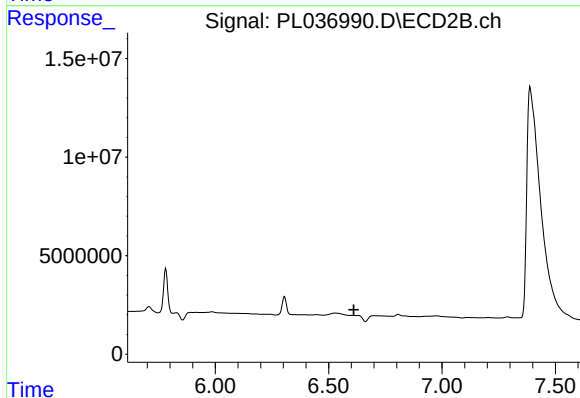


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

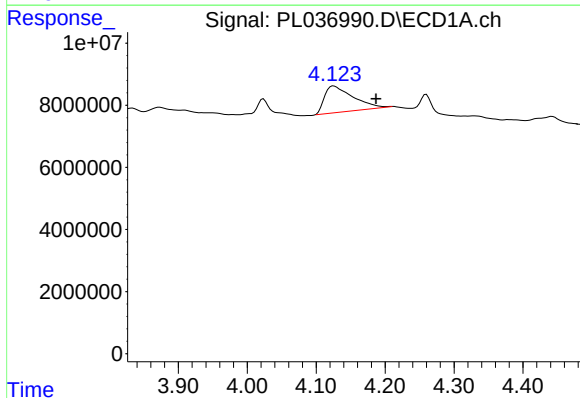


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: -0.061 min
Response: 24763011
Conc: 85.94 ng/ml

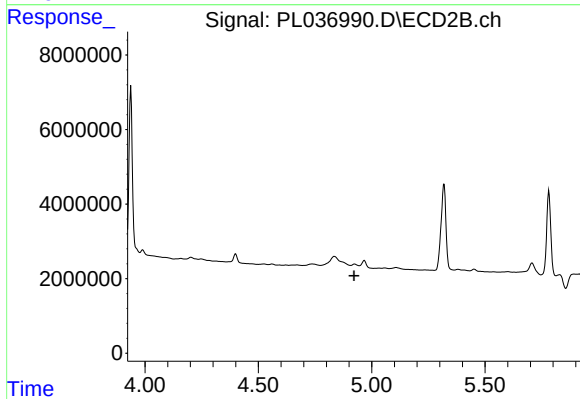

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

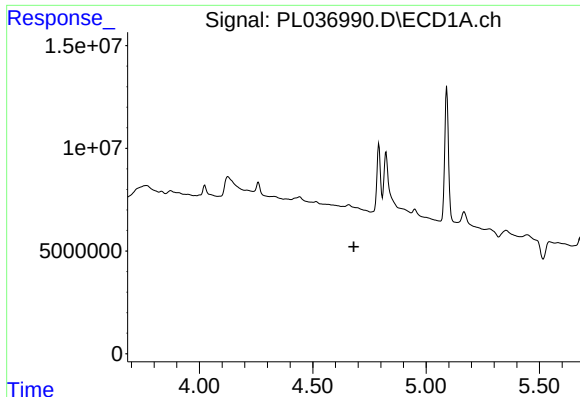

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

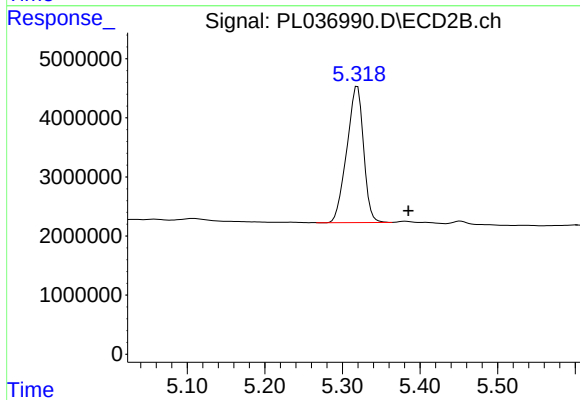


#24 Chlordane-2

R.T.: 5.319 min
Delta R.T.: -0.066 min
Response: 34502749
Conc: 297.24 ng/ml

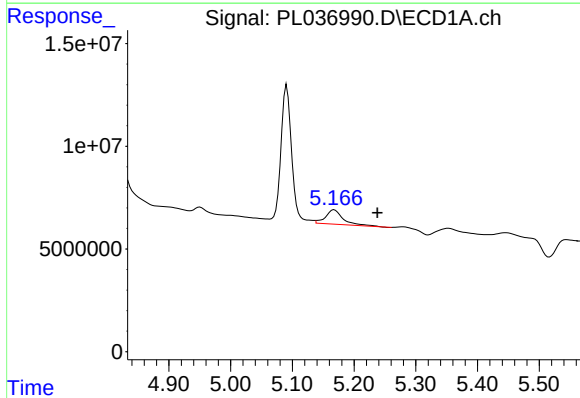


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: -0.070 min
Response: 14106759
Conc: 15.01 ng/ml

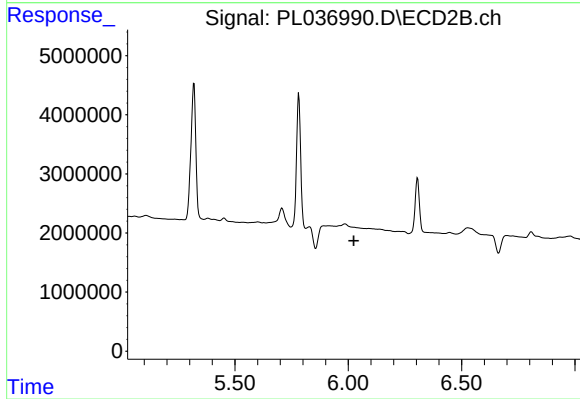

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

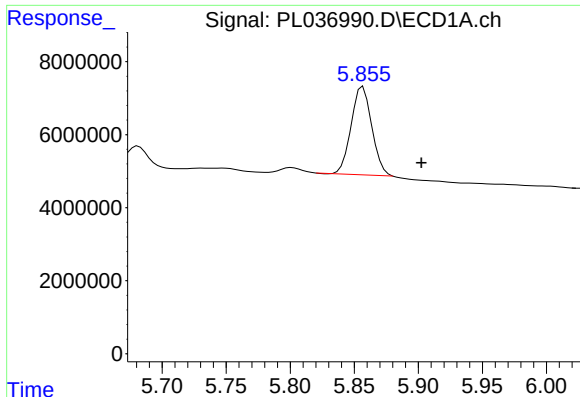

#27 Chlordane-5


R.T.: 5.857 min
Delta R.T.: -0.046 min
Response: 27014324
Conc: 216.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

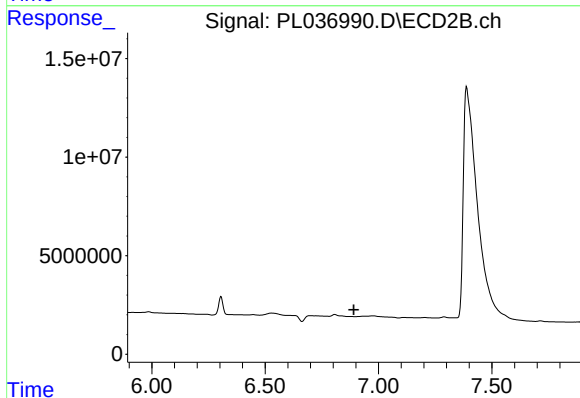


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.892 min
Response: 0
Conc: N.D.

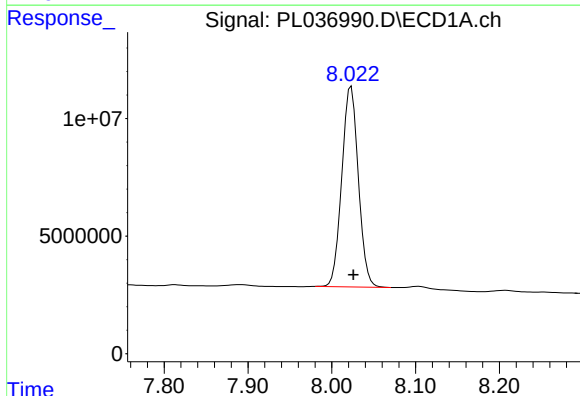

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.003 min
Response: 117215563
Conc: 18.02 ng/ml

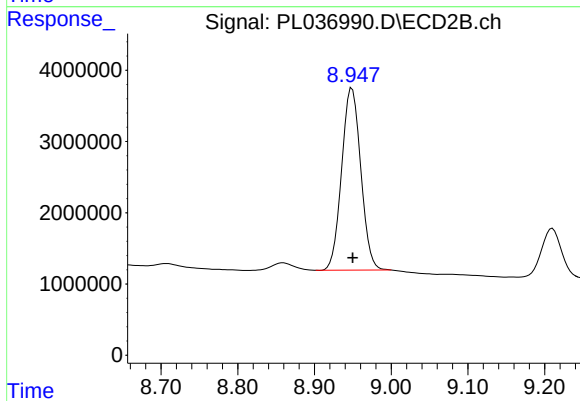

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 44519111
Conc: 17.45 ng/ml