

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 10:05
 Operator : UA\AJ
 Sample : J3488-01
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:09:36 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	84415658	31502821	11.871	12.323
28)	SA Decachlor...	8.023	8.949	48008861	18993651	7.379	7.446
Target Compounds							
2)	A alpha-BHC	3.723f	0.000	338804	0	0.030	N.D. #
6)	B beta-BHC	4.260f	0.000	9042118	0	2.117	N.D. #
10)	B gamma-Chl...	5.256	0.000	12769501	0	1.518	N.D. #
11)	B alpha-Chl...	5.256f	0.000	12769501	0	1.567	N.D. #
12)	B 4,4'-DDE	5.461	0.000	11503634	0	1.463	N.D. #
14)	MA Endrin	5.899f	0.000	4371931	0	0.628	N.D. #
17)	MA 4,4'-DDT	6.205	0.000	12685499	0	2.161	N.D. #
23)	Chlordane-1	4.136	0.000	2799231	0	9.715	N.D. #
25)	Chlordane-3	5.256	0.000	12769501	0	13.584	N.D. #
26)	Chlordane-4	5.256	0.000	12769501	0	15.028	N.D. #
27)	Chlordane-5	5.899	0.000	4371931	0	35.050	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 10:05
Operator : UA\AJ
Sample : J3488-01
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:09:36 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

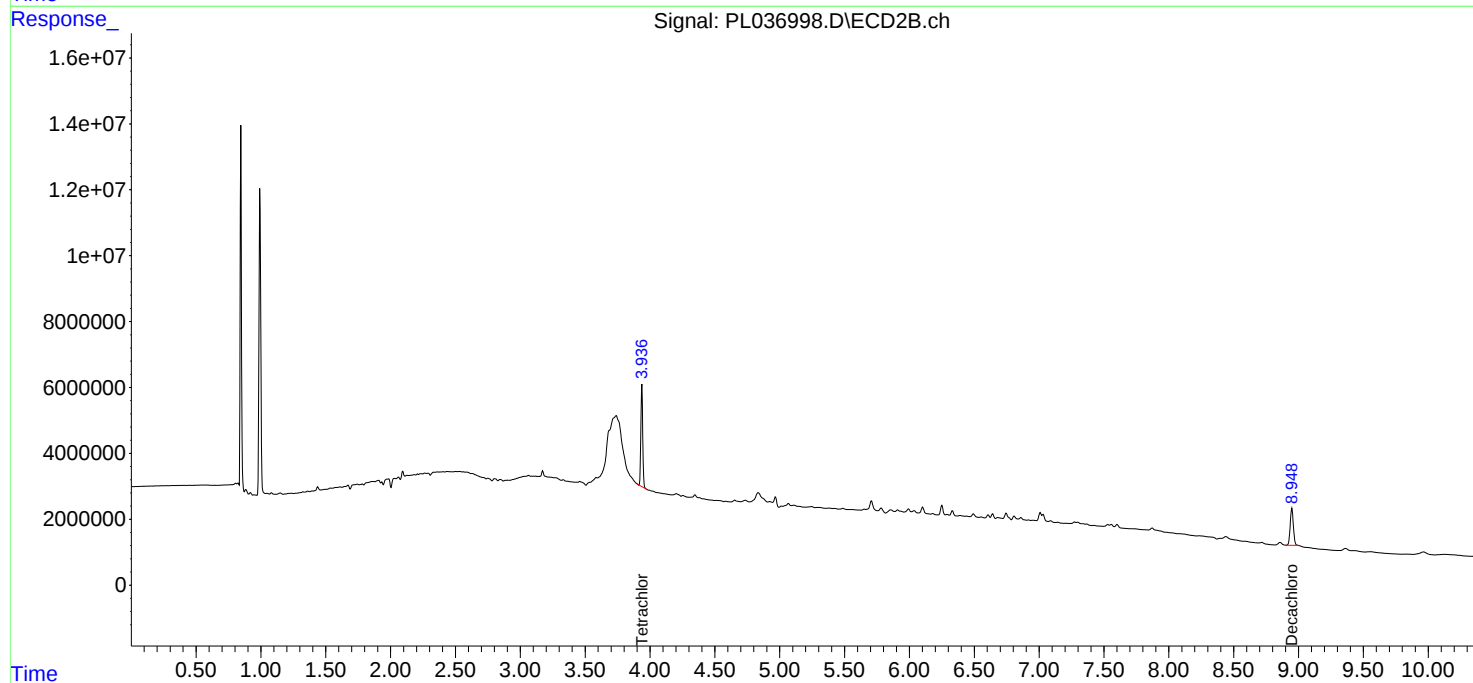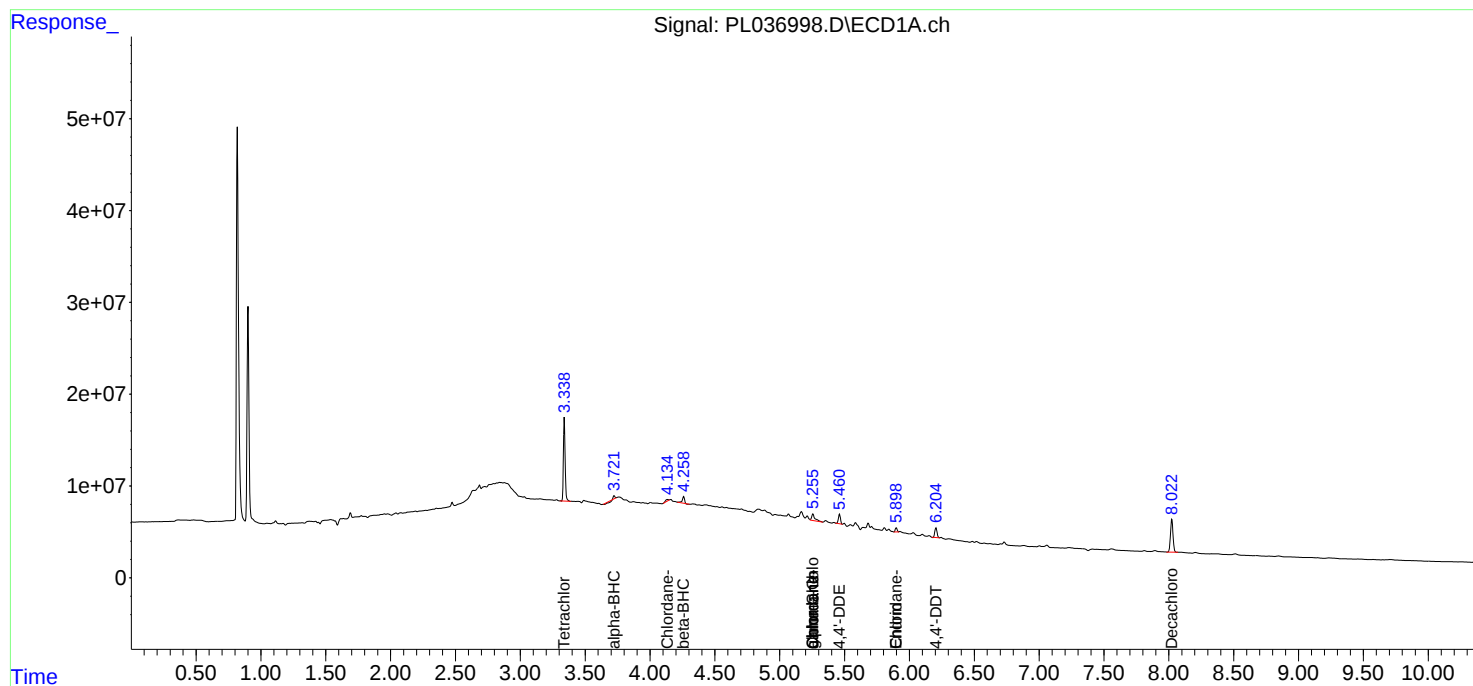


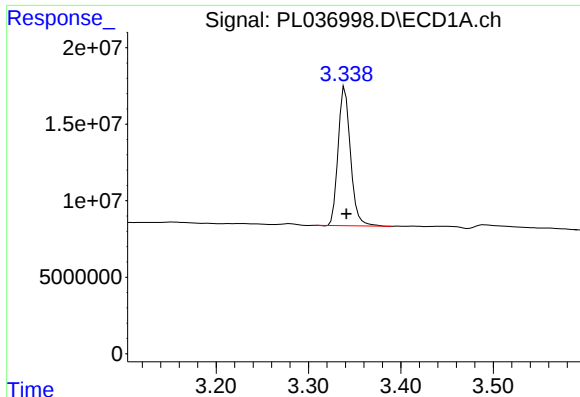

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 84415658
Conc: 11.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

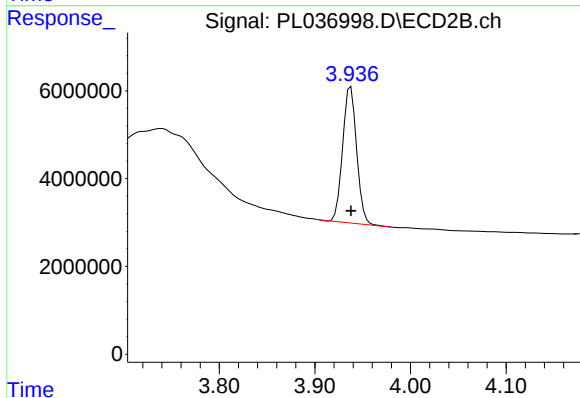


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 31502821
Conc: 12.32 ng/ml

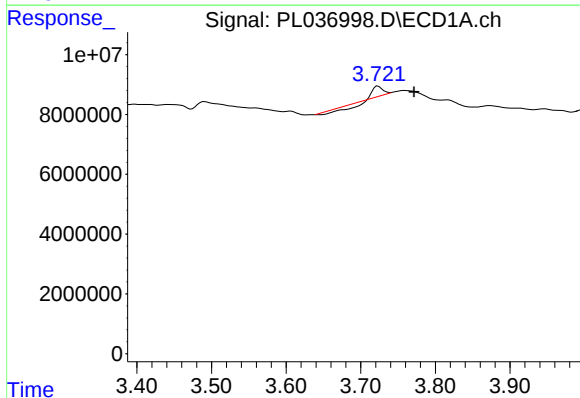


#2 alpha-BHC

R.T.: 3.723 min
Delta R.T.: -0.048 min
Response: 338804
Conc: 0.03 ng/ml

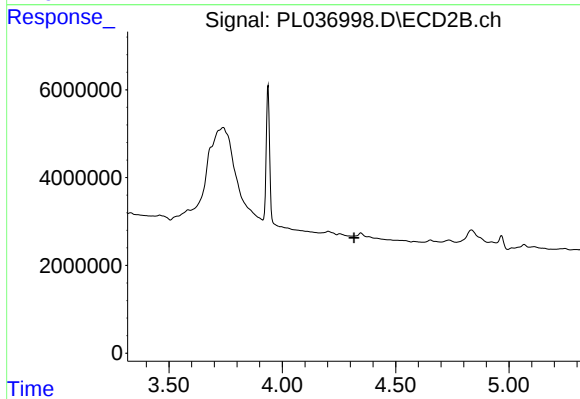

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

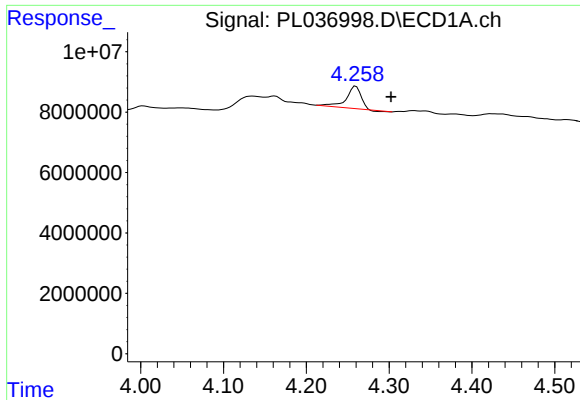

#6 beta-BHC


R.T.: 4.260 min
Delta R.T.: -0.043 min
Response: 9042118
Conc: 2.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

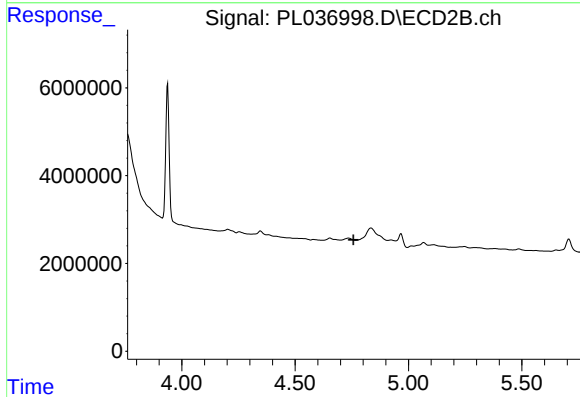


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

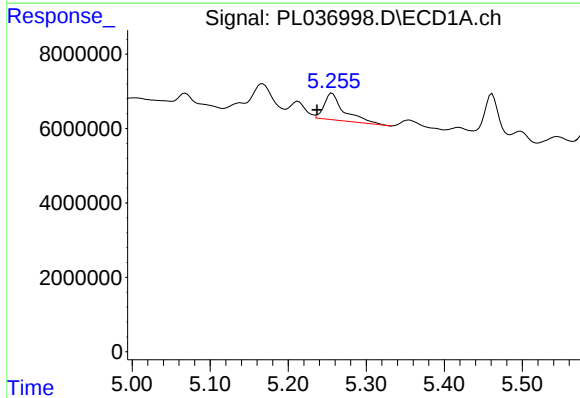


#10 gamma-Chlordane

R.T.: 5.256 min
Delta R.T.: 0.019 min
Response: 12769501
Conc: 1.52 ng/ml

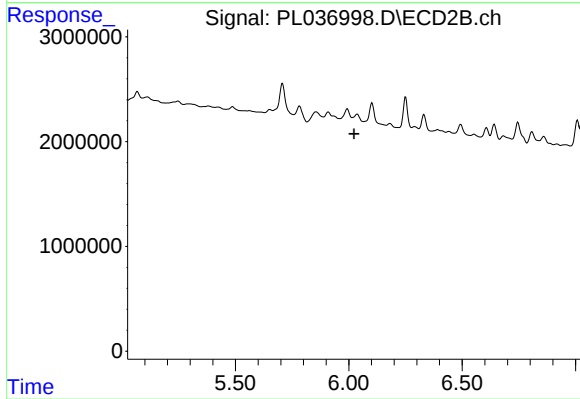

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

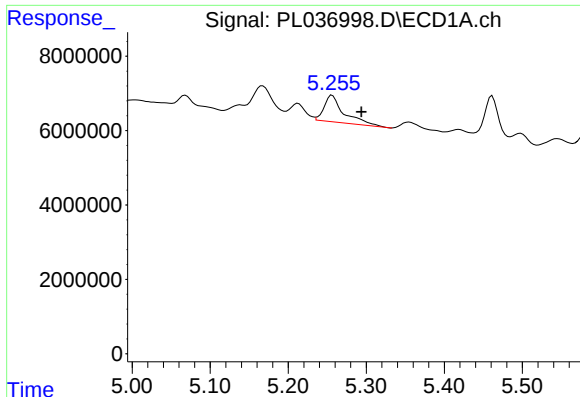

#11 alpha-Chlordane


R.T.: 5.256 min
Delta R.T.: -0.038 min
Response: 12769501
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

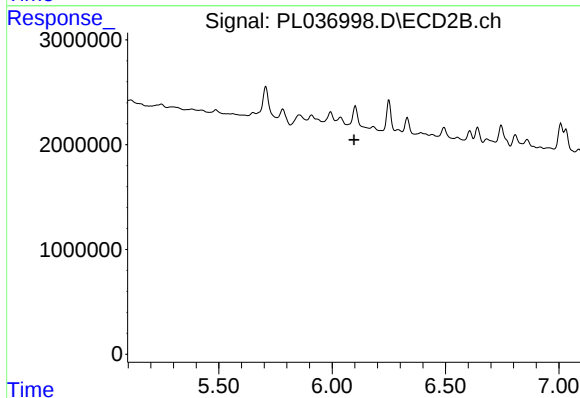


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

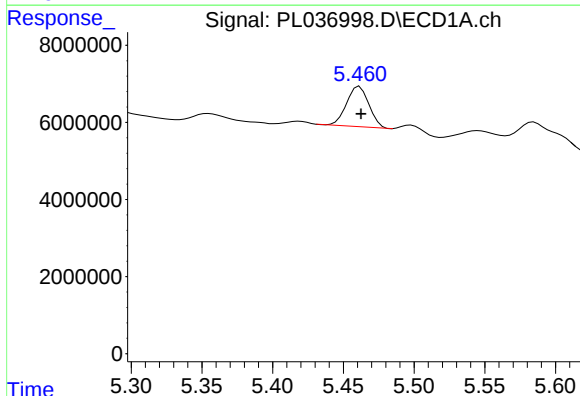


#12 4,4'-DDE

R.T.: 5.461 min
Delta R.T.: -0.001 min
Response: 11503634
Conc: 1.46 ng/ml

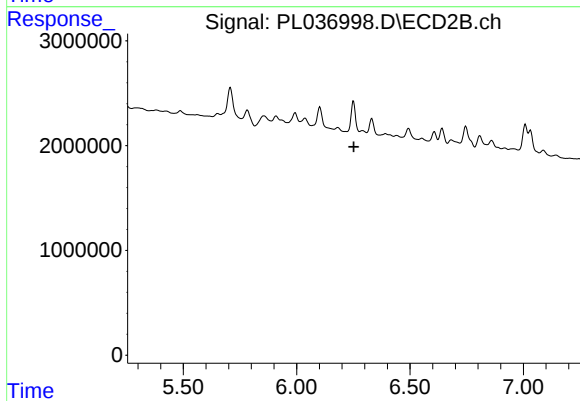

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

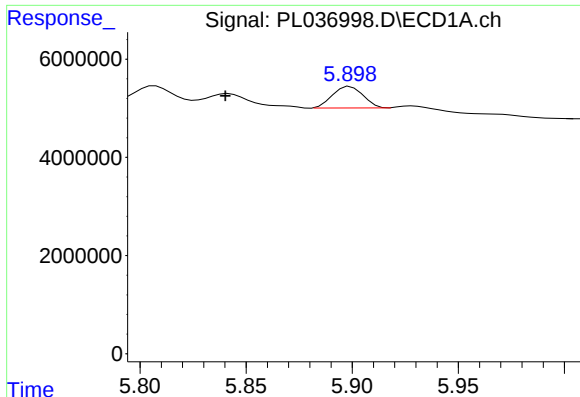

#14 Endrin


R.T.: 5.899 min
Delta R.T.: 0.059 min
Response: 4371931
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

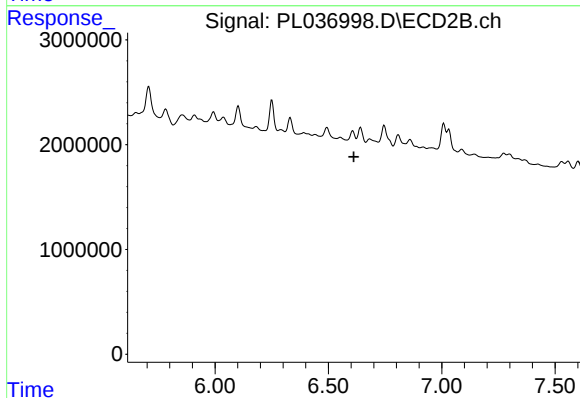


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

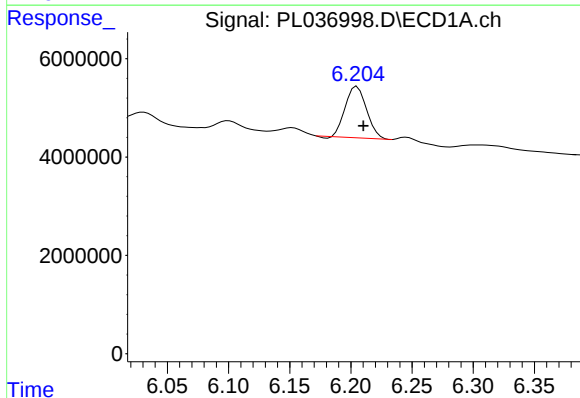


#17 4,4'-DDT

R.T.: 6.205 min
Delta R.T.: -0.005 min
Response: 12685499
Conc: 2.16 ng/ml

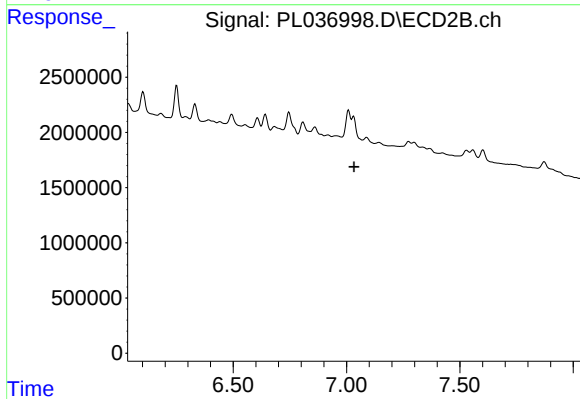

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

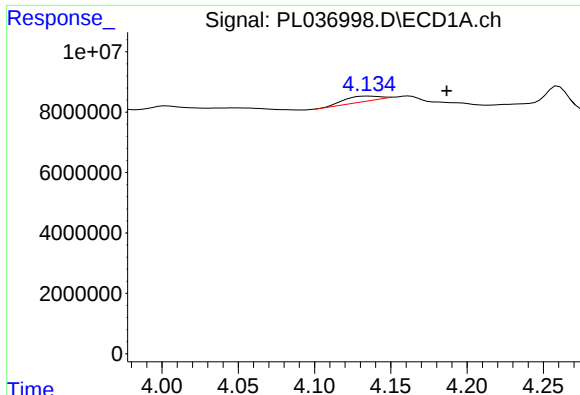

#23 Chlordane-1


R.T.: 4.136 min
Delta R.T.: -0.051 min
Response: 2799231
Conc: 9.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

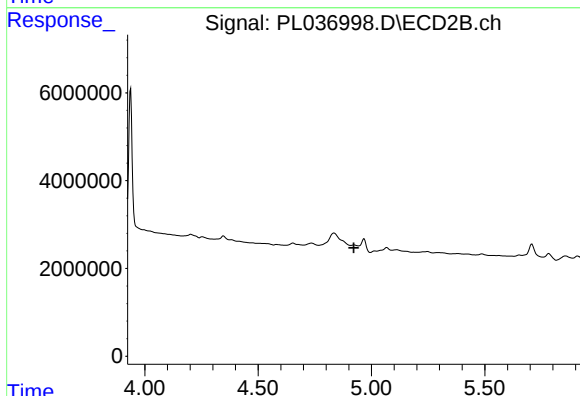


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

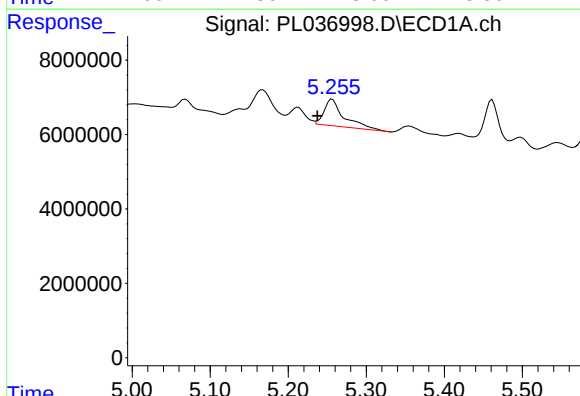


#25 Chlordane-3

R.T.: 5.256 min
Delta R.T.: 0.019 min
Response: 12769501
Conc: 13.58 ng/ml

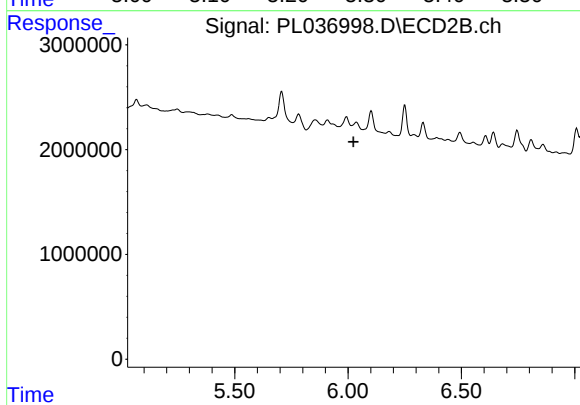

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

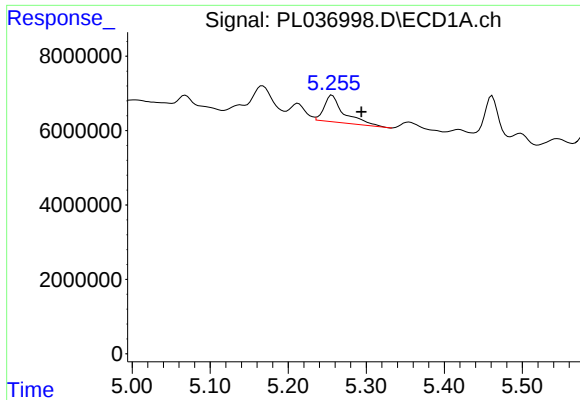

#26 Chlordane-4


R.T.: 5.256 min
Delta R.T.: -0.037 min
Response: 12769501
Conc: 15.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

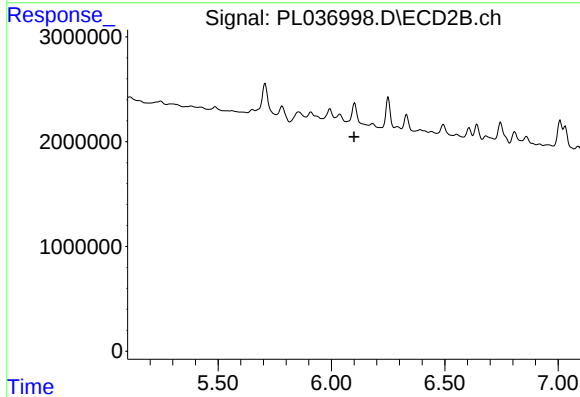


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

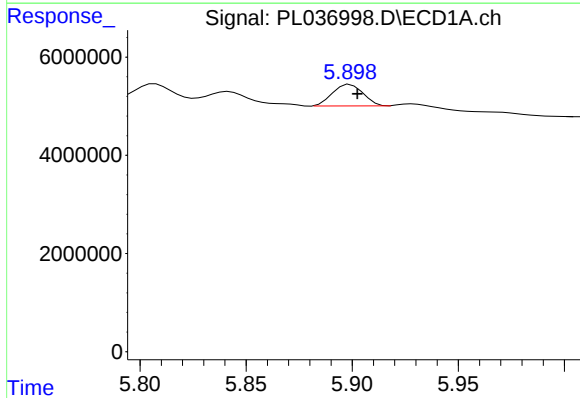


#27 Chlordane-5

R.T.: 5.899 min
Delta R.T.: -0.003 min
Response: 4371931
Conc: 35.05 ng/ml

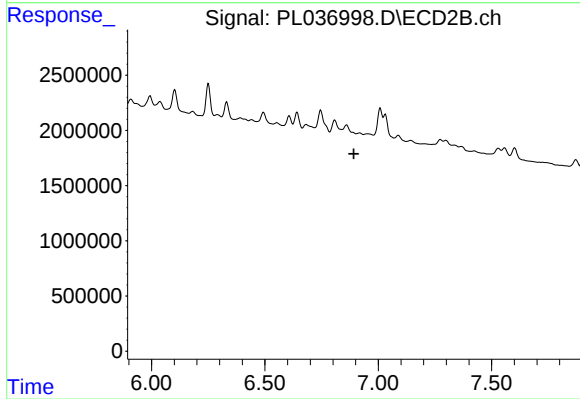

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.892 min
Response: 0
Conc: N.D.

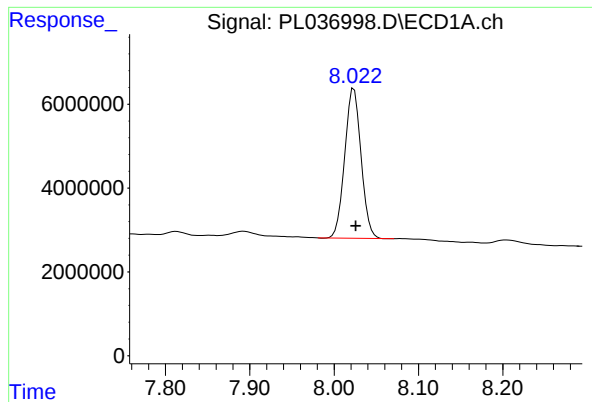

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.002 min
Response: 48008861
Conc: 7.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

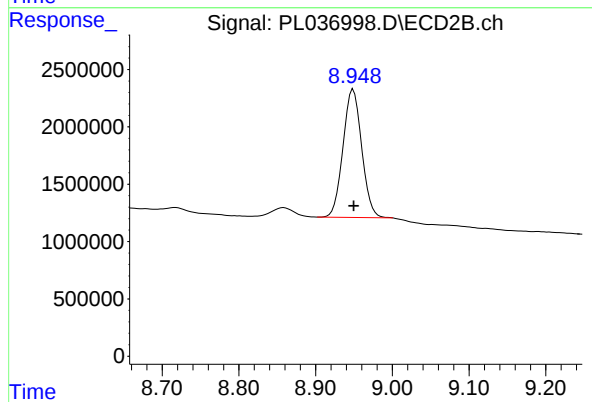

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 18993651
Conc: 7.45 ng/ml