

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 05:10
 Operator : UA\AJ
 Sample : J3241-07 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-05-061318-A

Manual Integrations
 APPROVED

UGO
 6/15/2018 1:38:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 07:38:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.338	3.936	19555805	7181127	2.750m	2.809m
28)	SA Decachlor...	8.024	0.000	17142318	0	2.635	N.D. #
Target Compounds							
12)	B 4,4'-DDE	5.460	6.248	5486075	1115320	0.698m	0.455m#
17)	MA 4,4'-DDT	6.207	7.031	8135780	3978934	1.386	1.891m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 05:10
Operator : UA\AJ
Sample : J3241-07 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-05-061318-A


Manual Integrations
APPROVED

UGO
6/15/2018 1:38:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 07:38:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

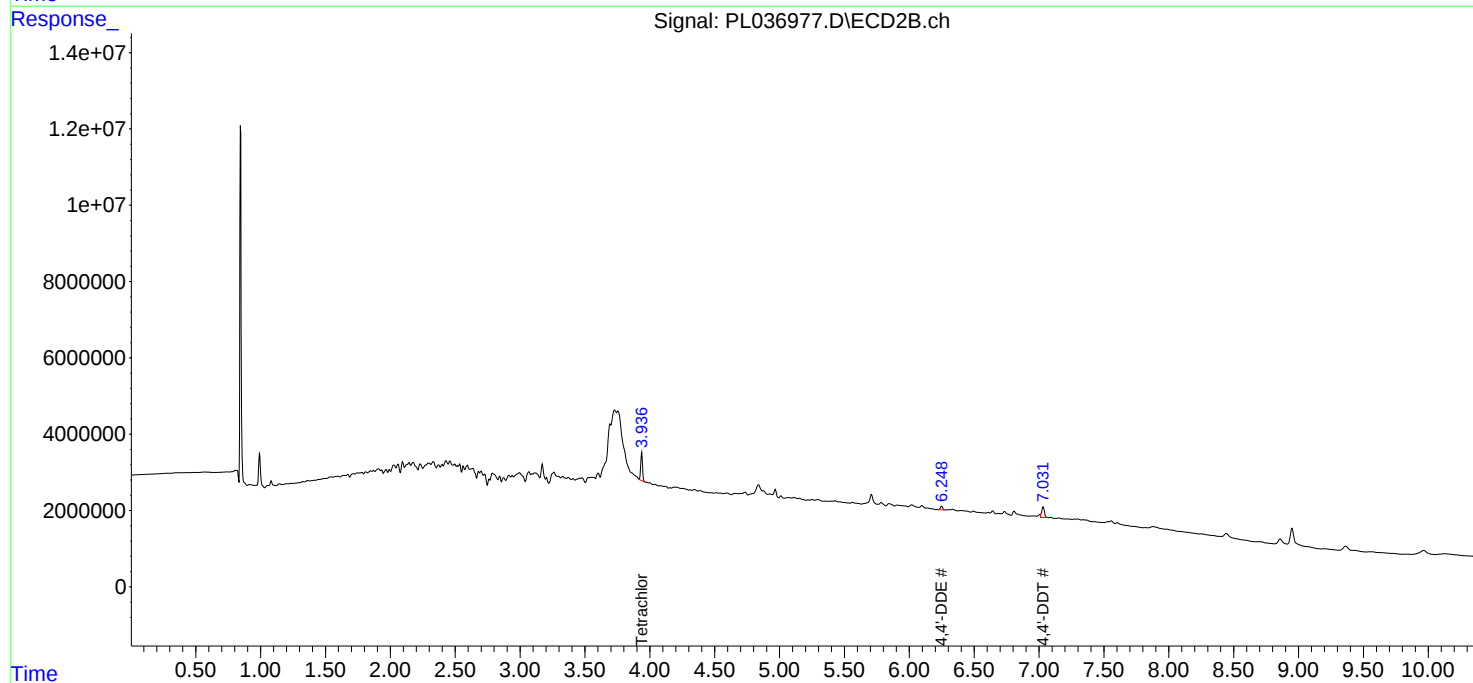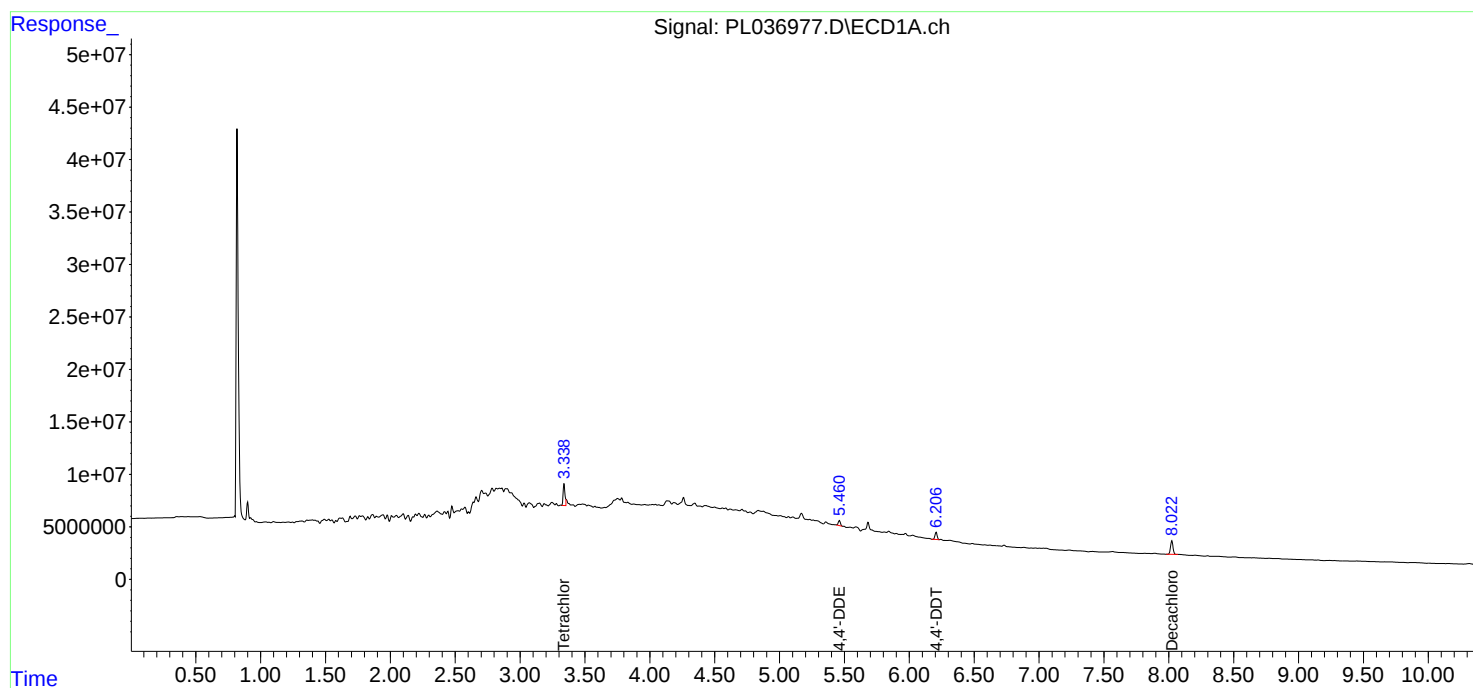

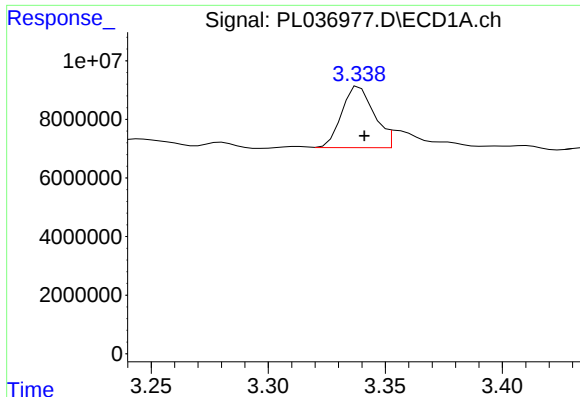


#1 Tetrachloro-m-xylene

R.T.: 3.338 min
Delta R.T.: -0.003 min
Response: 19555805
Conc: 2.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HR-05-061318-A


Manual Integrations
APPROVED

UGO
6/15/2018 1:38:09 PM

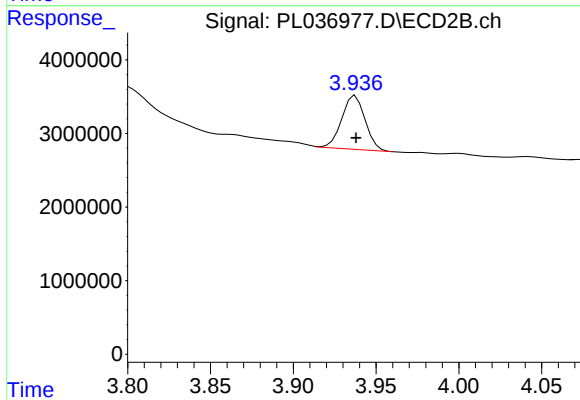


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 7181127
Conc: 2.81 ng/ml m

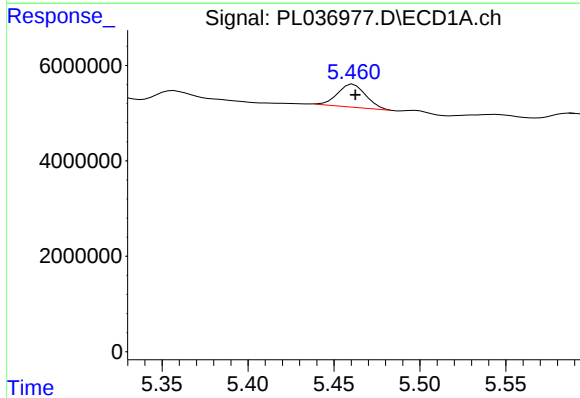


#12 4,4'-DDE

R.T.: 5.460 min
Delta R.T.: -0.003 min
Response: 5486075
Conc: 0.70 ng/ml m

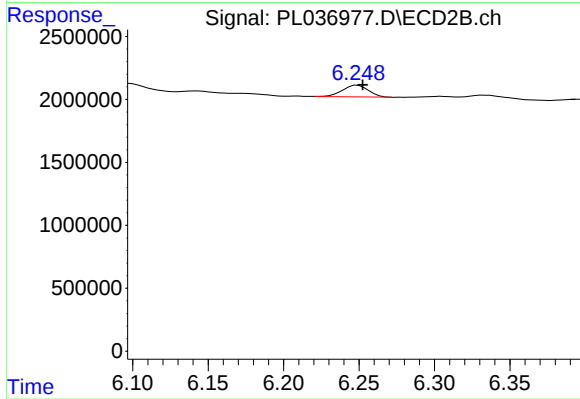

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.005 min
Response: 1115320
Conc: 0.45 ng/ml m

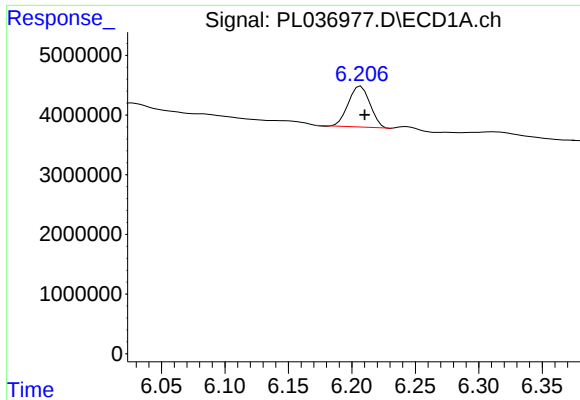


#17 4,4'-DDT

R.T.: 6.207 min
Delta R.T.: -0.003 min
Response: 8135780
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-061318-A


Manual Integrations
APPROVED

UGO
6/15/2018 1:38:09 PM

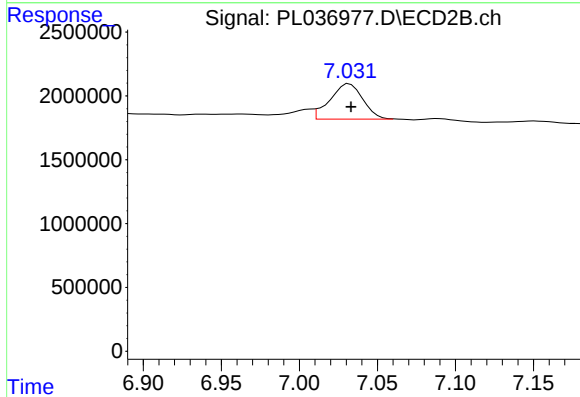


#17 4,4'-DDT

R.T.: 7.031 min
Delta R.T.: -0.002 min
Response: 3978934
Conc: 1.89 ng/ml m

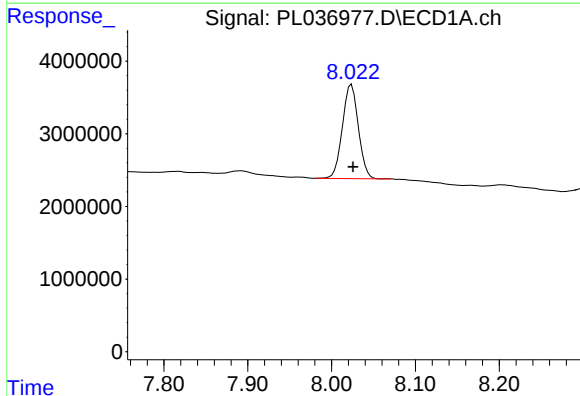

#28 Decachlorobiphenyl

R.T.: 8.024 min
Delta R.T.: -0.002 min
Response: 17142318
Conc: 2.63 ng/ml

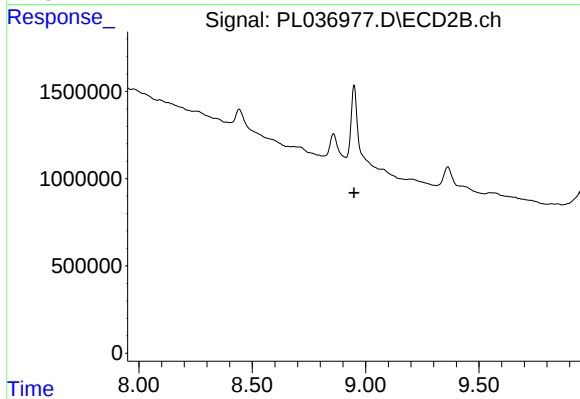

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.950 min
Response: 0
Conc: N.D.