

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 05:38
 Operator : UA\AJ
 Sample : J3241-11 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-05-061318-C

Manual Integrations
 APPROVED

UGO
 6/15/2018 1:38:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 07:38:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.937	28622620	9699564	4.025	3.794
28)	SA Decachlor...	8.023	8.949	25061911	11643717	3.852	4.564
Target Compounds							
17)	MA 4,4'-DDT	6.203	7.030	7326281	2196214	1.248m	1.044m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 05:38
Operator : UA\AJ
Sample : J3241-11 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-05-061318-C


Manual Integrations
APPROVED

UGO
6/15/2018 1:38:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 07:38:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

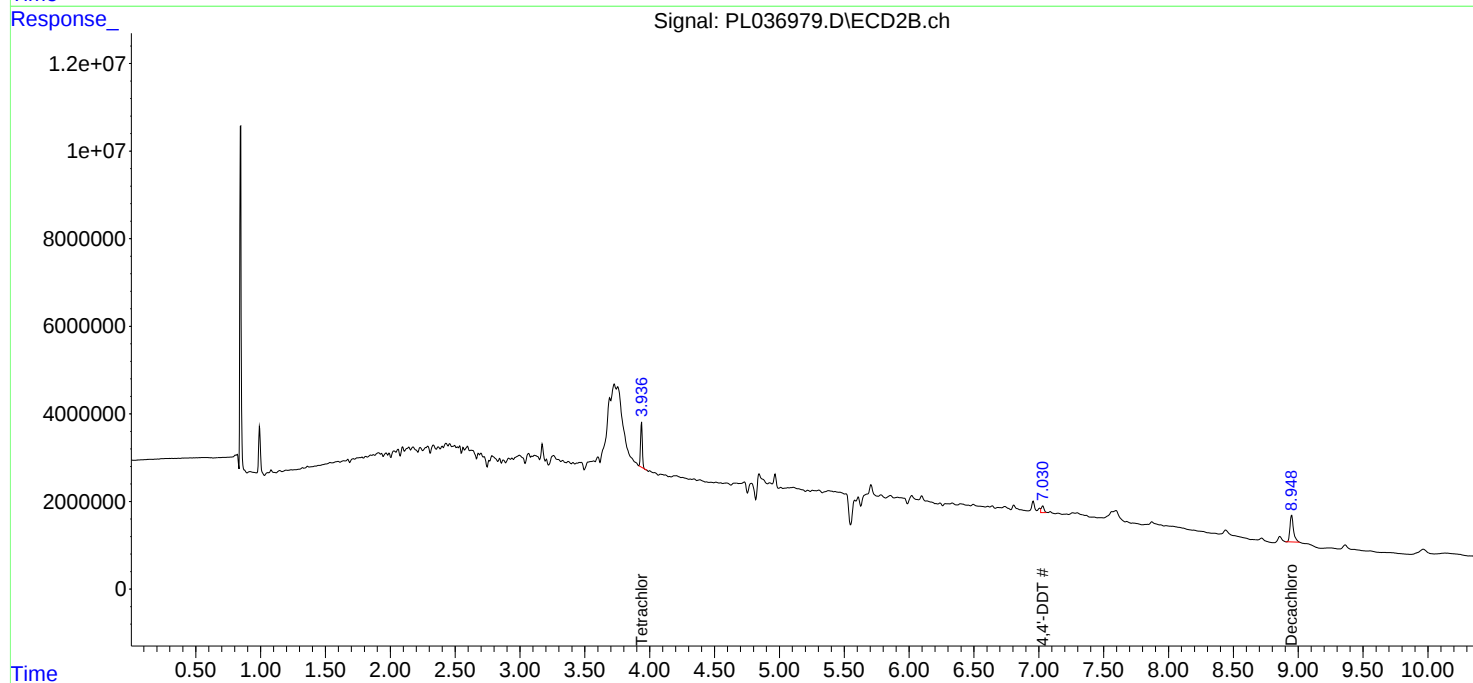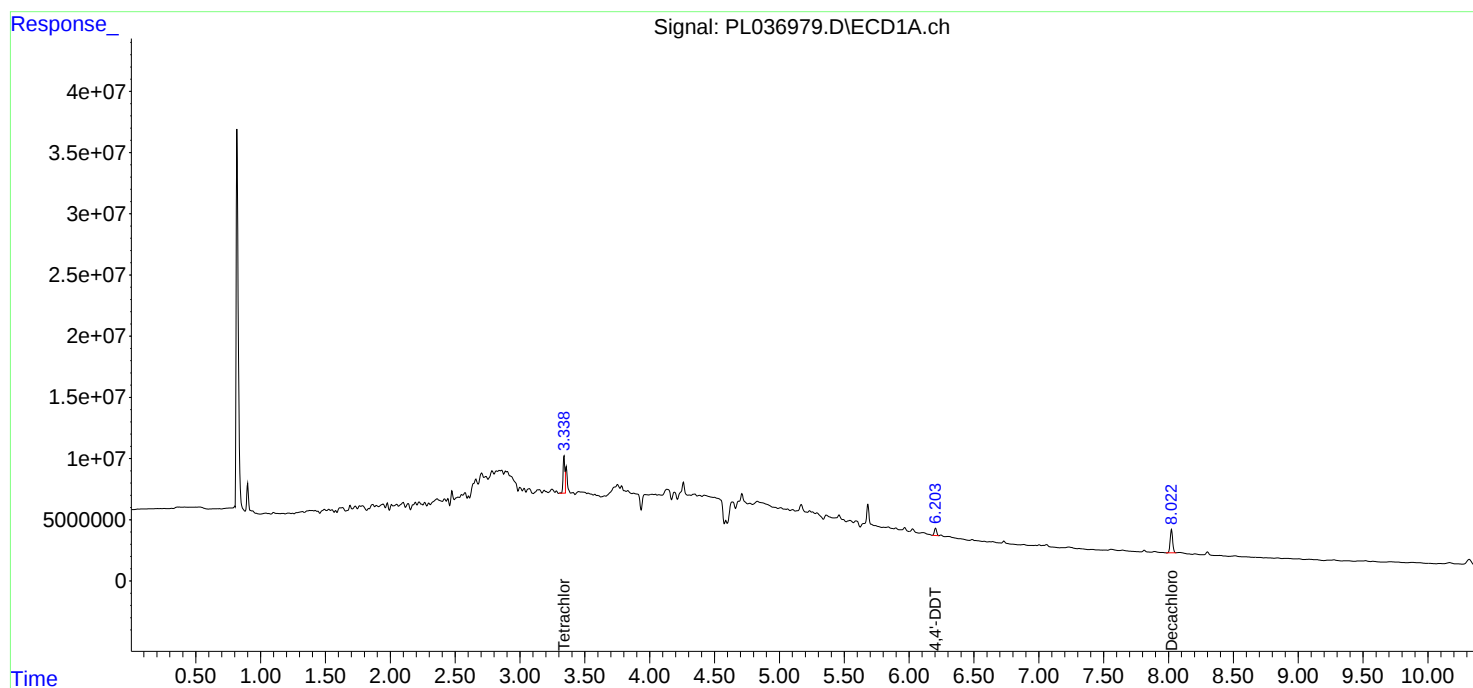

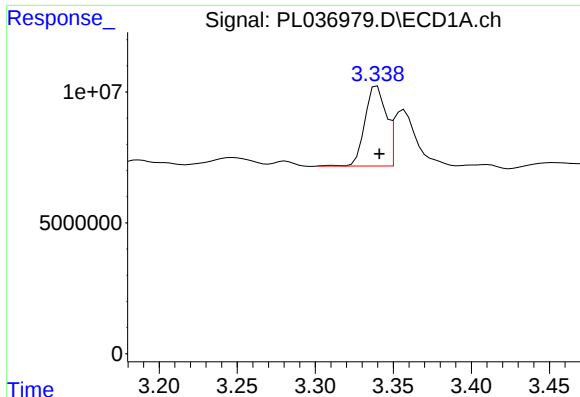


#1 Tetrachloro-m-xylene

R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 28622620
Conc: 4.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-061318-C


Manual Integrations
APPROVED

UGO
6/15/2018 1:38:16 PM

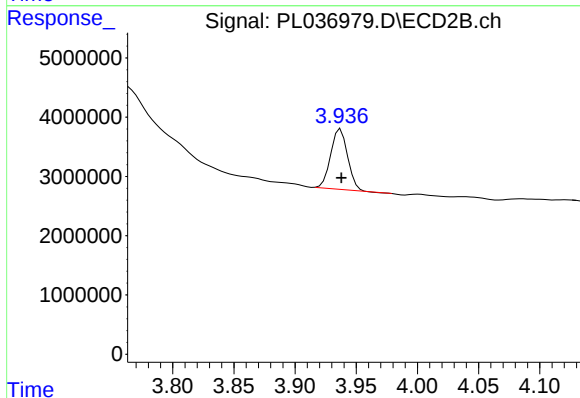


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 9699564
Conc: 3.79 ng/ml

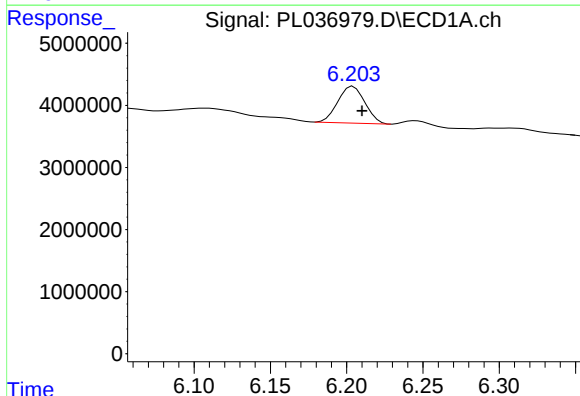


#17 4,4'-DDT

R.T.: 6.203 min
Delta R.T.: -0.007 min
Response: 7326281
Conc: 1.25 ng/ml m

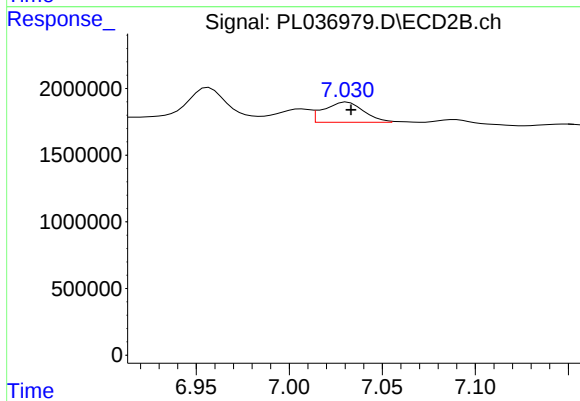

#17 4,4'-DDT

R.T.: 7.030 min
Delta R.T.: -0.003 min
Response: 2196214
Conc: 1.04 ng/ml m

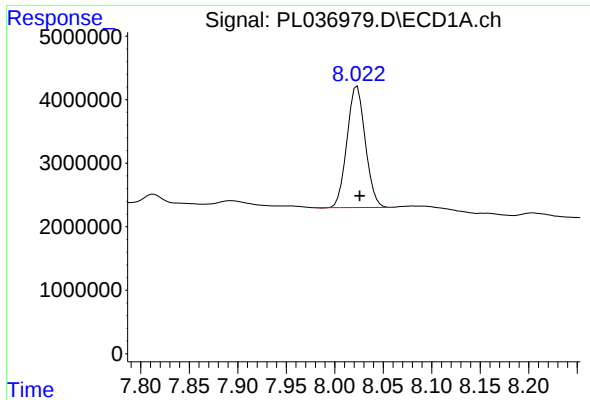


#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.003 min
Response: 25061911
Conc: 3.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-061318-C

Manual Integrations
APPROVED

UGO
6/15/2018 1:38:16 PM

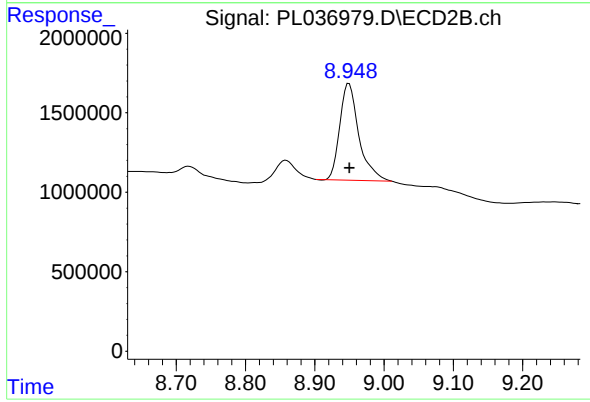

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 11643717
Conc: 4.56 ng/ml