

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
 Data File : PL036998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 10:05
 Operator : UA\AJ
 Sample : J3488-01
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-RO-3091

Manual Integrations
 APPROVED

UGO
 6/15/2018 1:40:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:09:36 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	84415658	31502821	11.871	12.323
28)	SA Decachlor...	8.023	8.949	48008861	18993651	7.379	7.446
Target Compounds							
12)	B 4,4'-DDE	5.461	6.249	11503634	3702122	1.463	1.509m
17)	MA 4,4'-DDT	6.205	7.030	12685499	2876273	2.161	1.367m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061518\
Data File : PL036998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 10:05
Operator : UA\AJ
Sample : J3488-01
Misc :
ALS Vial : 79 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FS-RO-3091


Manual Integrations
APPROVED

UGO
6/15/2018 1:40:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:09:36 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

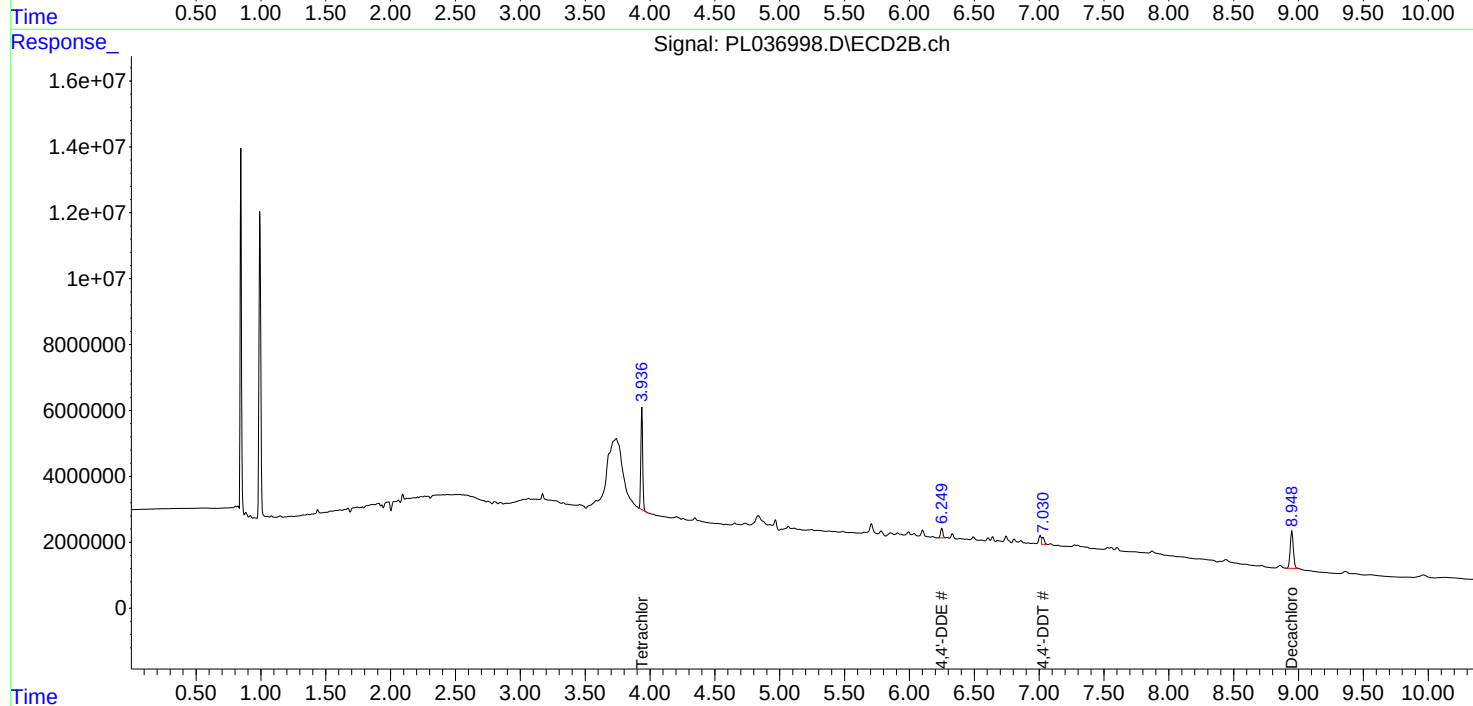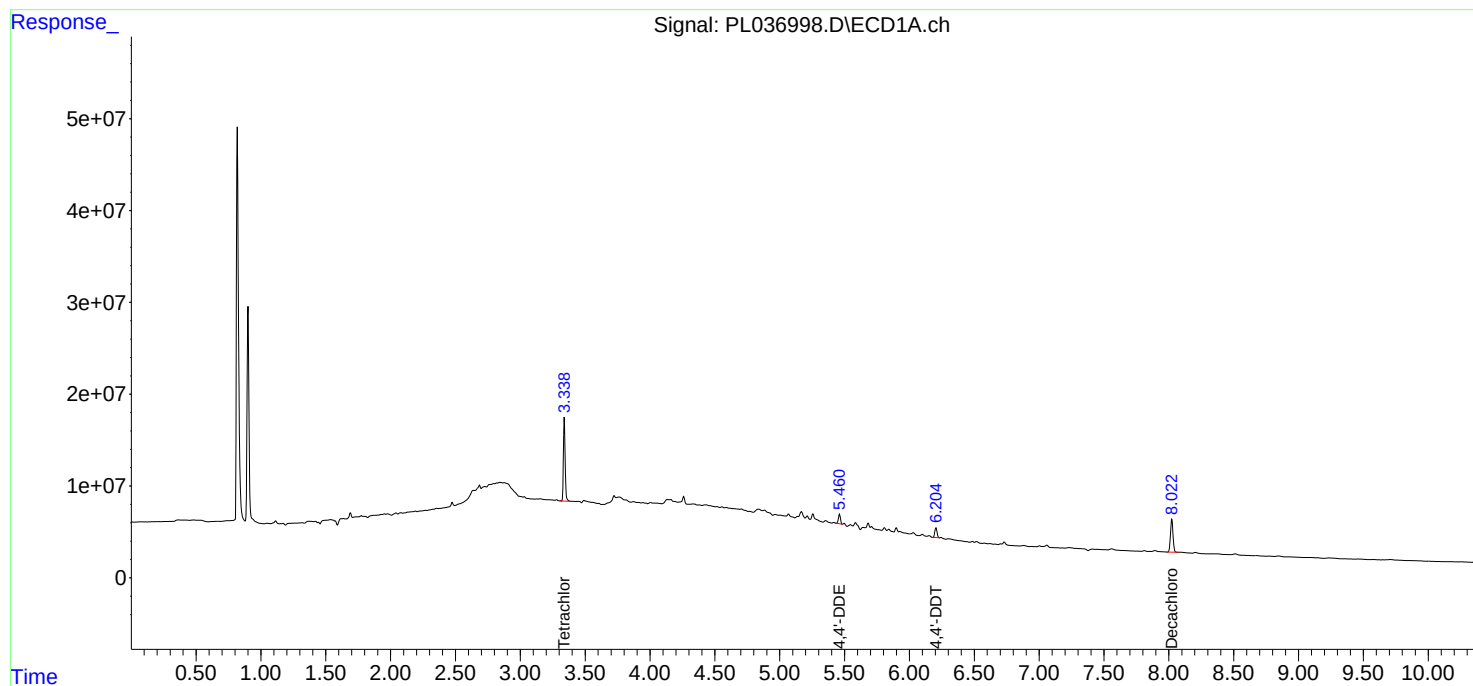

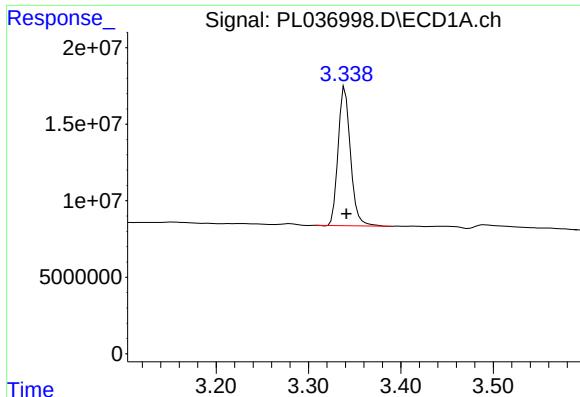


#1 Tetrachloro-m-xylene

R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 84415658
Conc: 11.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-RO-3091


Manual Integrations
APPROVED

UGO
6/15/2018 1:40:01 PM

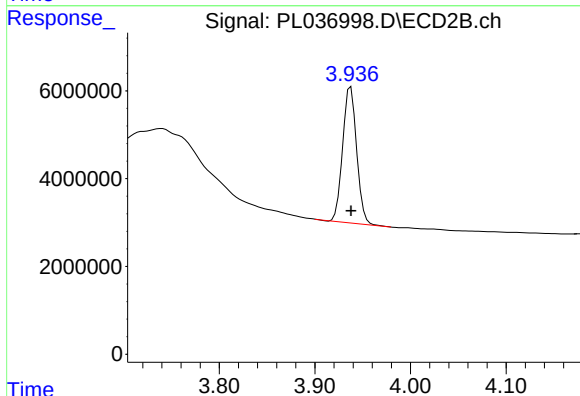


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 31502821
Conc: 12.32 ng/ml

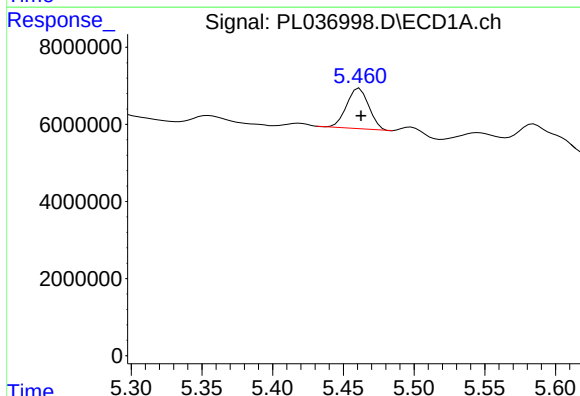


#12 4,4'-DDE

R.T.: 5.461 min
Delta R.T.: -0.001 min
Response: 11503634
Conc: 1.46 ng/ml

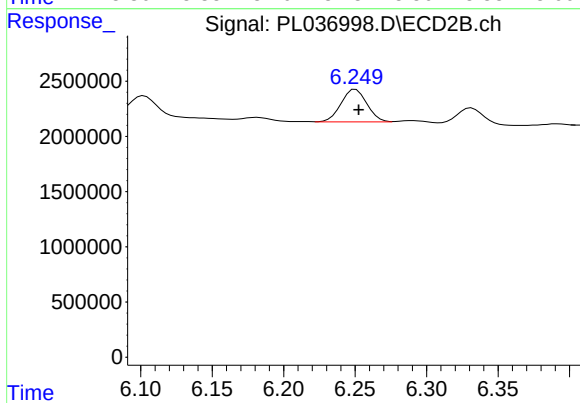

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.003 min
Response: 3702122
Conc: 1.51 ng/ml m

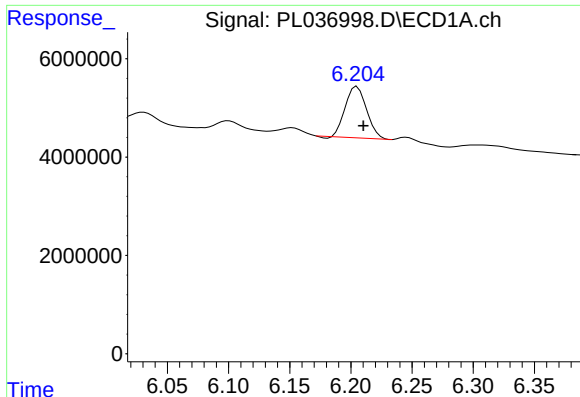


#17 4,4'-DDT

R.T.: 6.205 min
Delta R.T.: -0.005 min
Response: 12685499
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-RO-3091


Manual Integrations
APPROVED

UGO
6/15/2018 1:40:01 PM

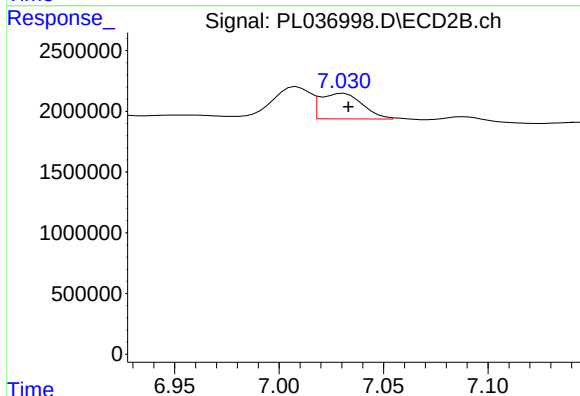


#17 4,4'-DDT

R.T.: 7.030 min
Delta R.T.: -0.003 min
Response: 2876273
Conc: 1.37 ng/ml m

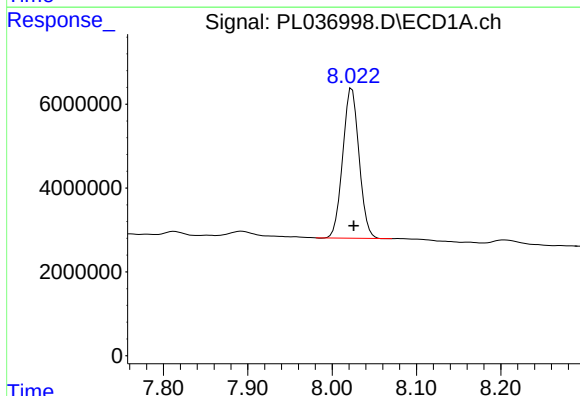

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.002 min
Response: 48008861
Conc: 7.38 ng/ml

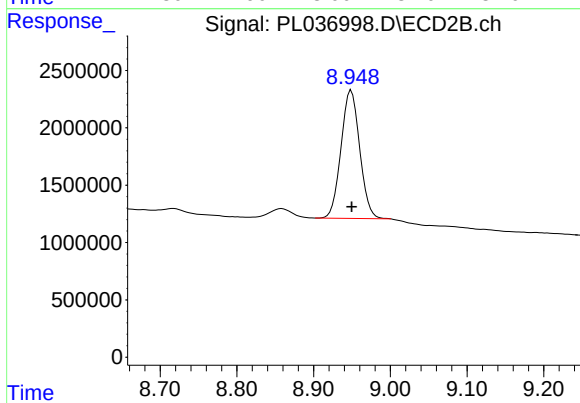

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 18993651
Conc: 7.45 ng/ml