

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061521\
 Data File : PL067472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 15:41
 Operator : AR\AJ
 Sample : M2672-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 17-B6(8-12)

Manual Integrations
 APPROVED

Ankita
 6/16/2021 3:34:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 18:24:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	11812594	22129089	21.486	23.473
28)	SA Decachlor...	10.227	11.435	16010848	25534972	22.592	25.636
Target Compounds							
12)	B 4,4'-DDE	7.483	8.524	2806874	400519	4.219m	0.442m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061521\
Data File : PL067472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 15:41
Operator : AR\AJ
Sample : M2672-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
17-B6(8-12)


Manual Integrations
APPROVED

Ankita
6/16/2021 3:34:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 18:24:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

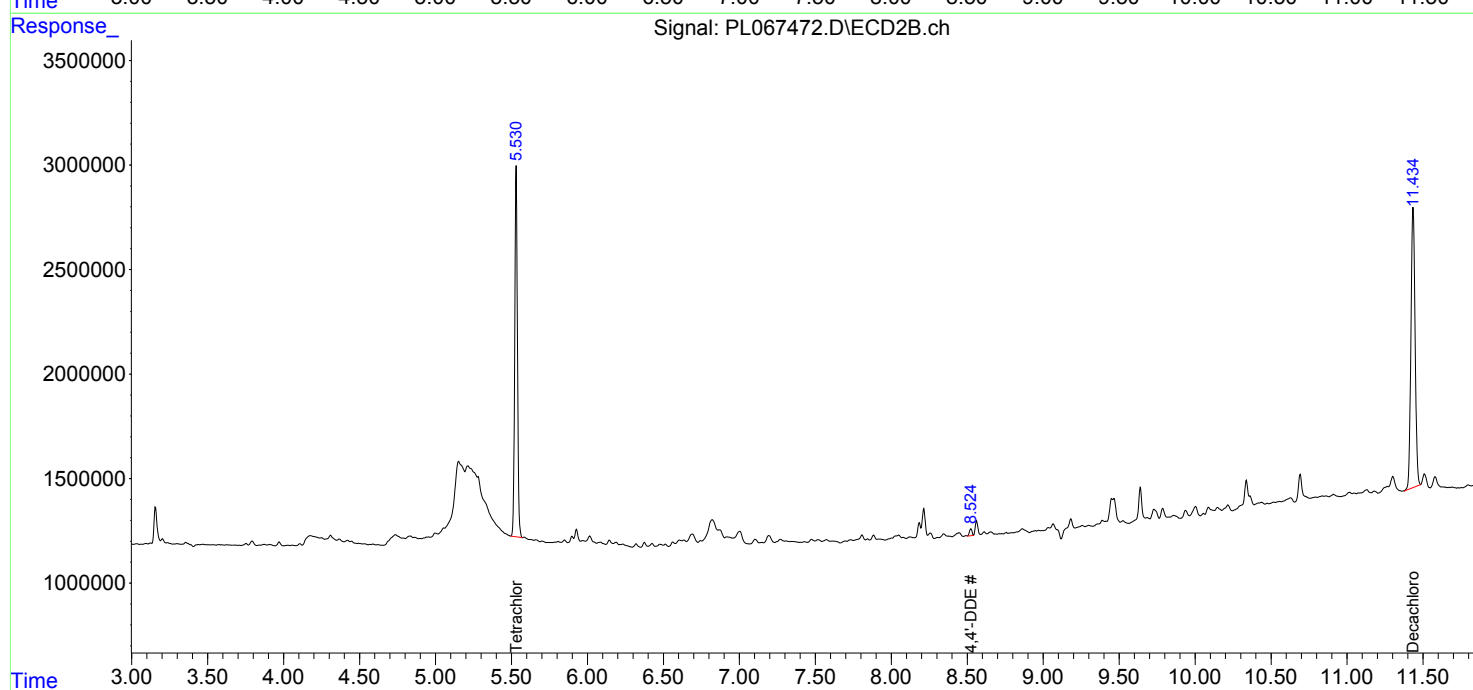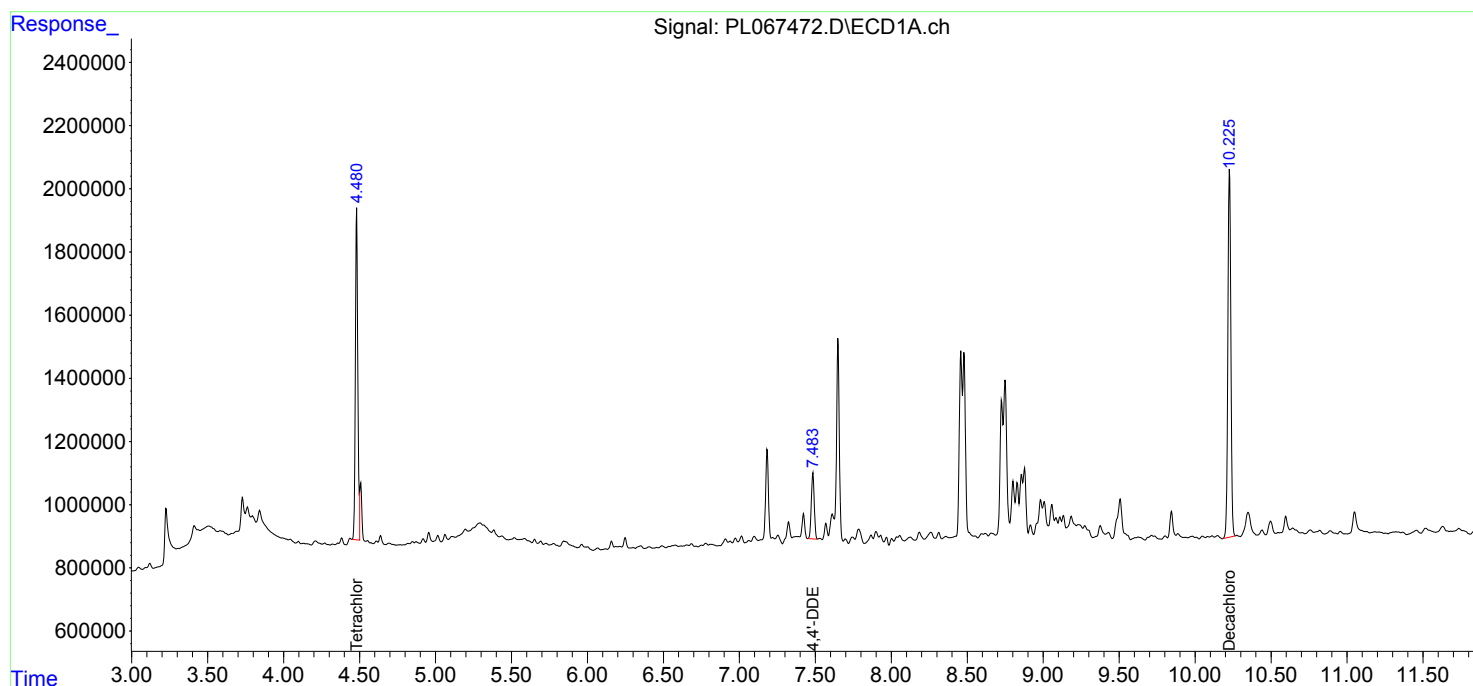

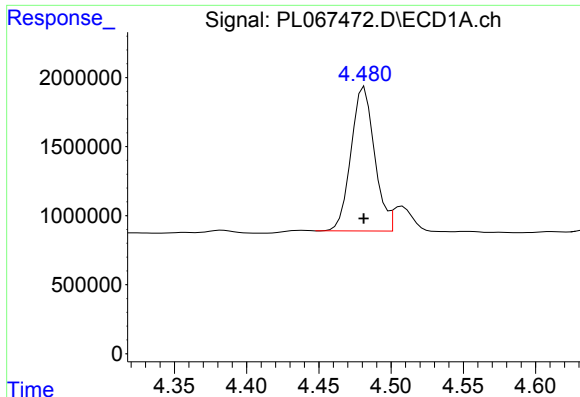


#1 Tetrachloro-m-xylene

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 11812594
Conc: 21.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
17-B6(8-12)


Manual Integrations
APPROVED

Ankita
6/16/2021 3:34:55 PM

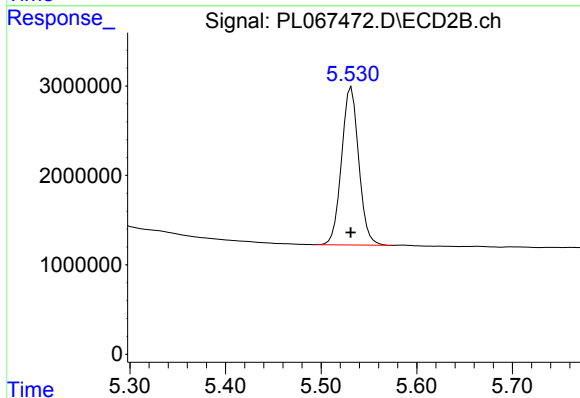


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 22129089
Conc: 23.47 ng/ml

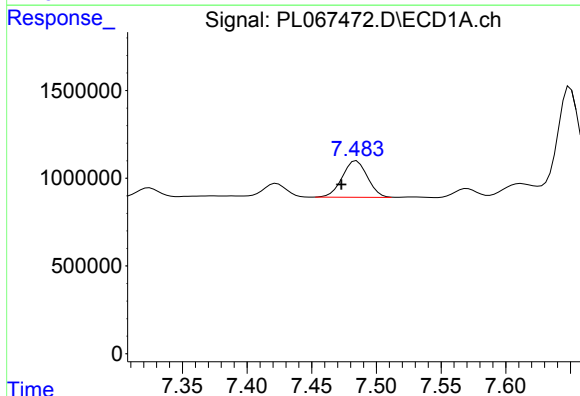


#12 4,4'-DDE

R.T.: 7.483 min
Delta R.T.: 0.010 min
Response: 2806874
Conc: 4.22 ng/ml m

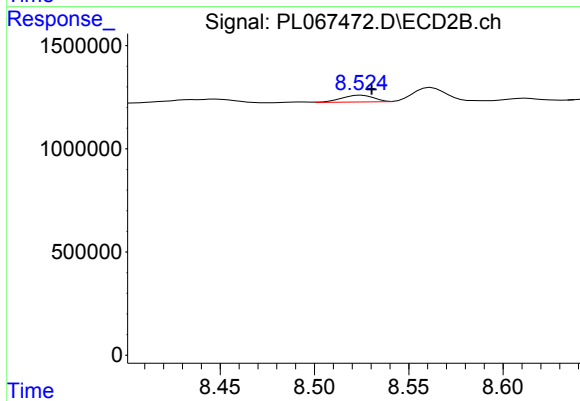

#12 4,4'-DDE

R.T.: 8.524 min
Delta R.T.: -0.007 min
Response: 400519
Conc: 0.44 ng/ml m

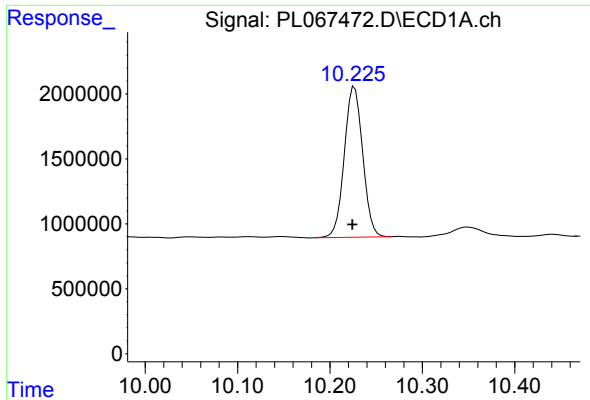


#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: 0.002 min
Response: 16010848
Conc: 22.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
17-B6(8-12)

Manual Integrations
APPROVED

Ankita
6/16/2021 3:34:55 PM

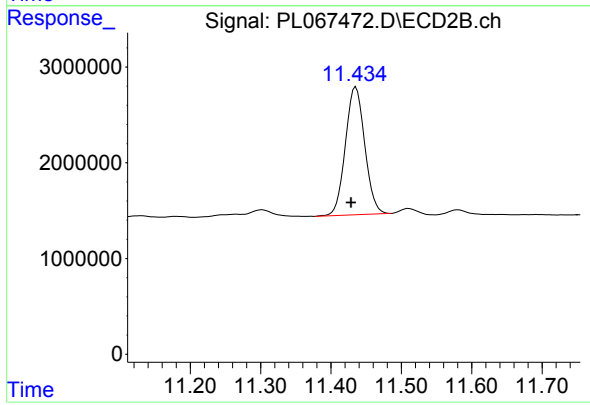

#28 Decachlorobiphenyl

R.T.: 11.435 min
Delta R.T.: 0.007 min
Response: 25534972
Conc: 25.64 ng/ml