

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061522\
 Data File : PL075807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2022 08:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 14:05:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.637	11731077	28170762	17.382	16.786
28)	SA Decachlor...	11.637	10.379	12323213	22510447	20.129	15.977
Target Compounds							
7)	B delta-BHC	0.000	6.399	0	983401	N.D.	0.459 #
10)	B gamma-Chl...	8.382	0.000	871252	0	1.122	N.D. #
11)	B alpha-Chl...	0.000	7.387f	0	319243	N.D.	0.175 #
14)	MA Endrin	0.000	8.065f	0	753040	N.D.	0.551 #
15)	B Endosulfa...	9.304	0.000	340859	0	0.548	N.D. #
19)	B Endosulfa...	0.000	8.767	0	259734	N.D.	0.177 #
21)	B Endrin ke...	10.186f	0.000	1188343	0	1.690	N.D. #
25)	Chlordane-3	8.382	0.000	871252	0	8.438	N.D. #
26)	Chlordane-4	0.000	7.387f	0	319243	N.D.	1.734 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061522\
Data File : PL075807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2022 08:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 14:05:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

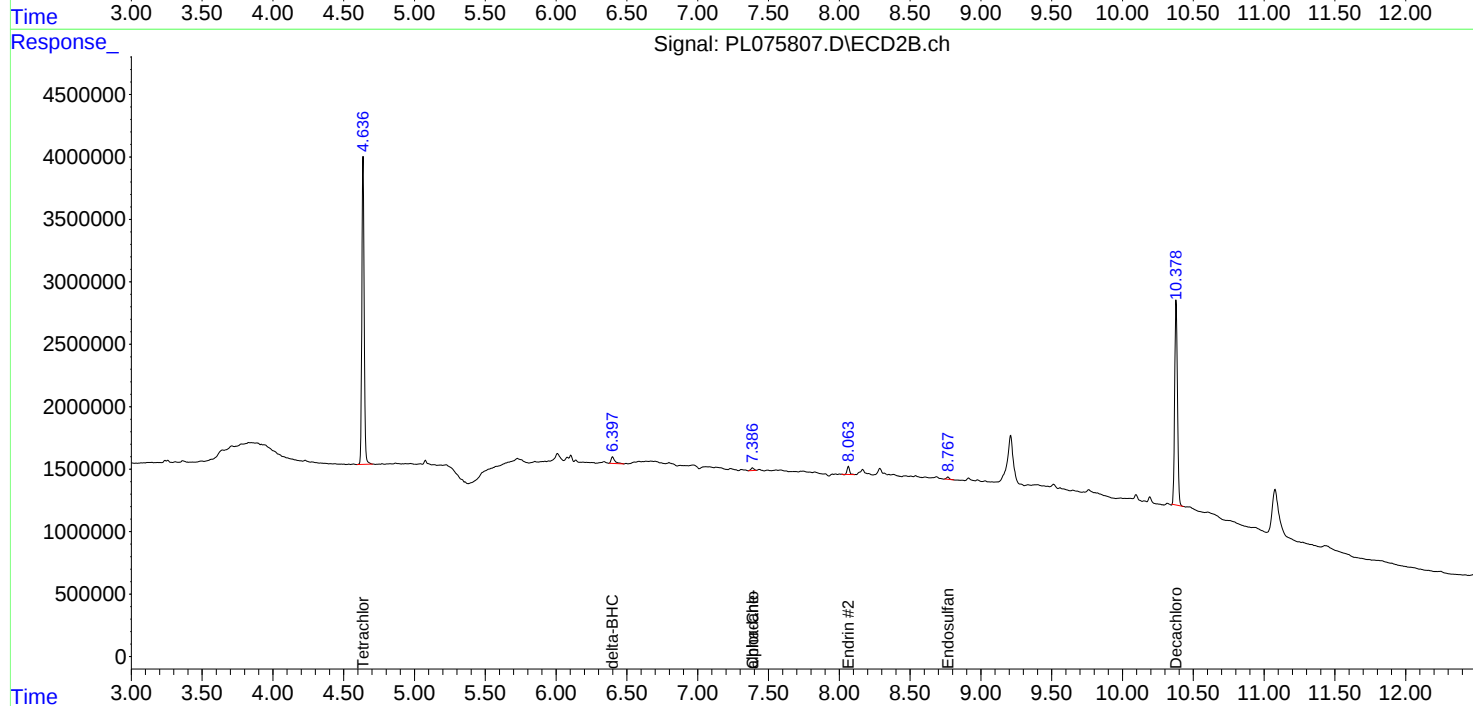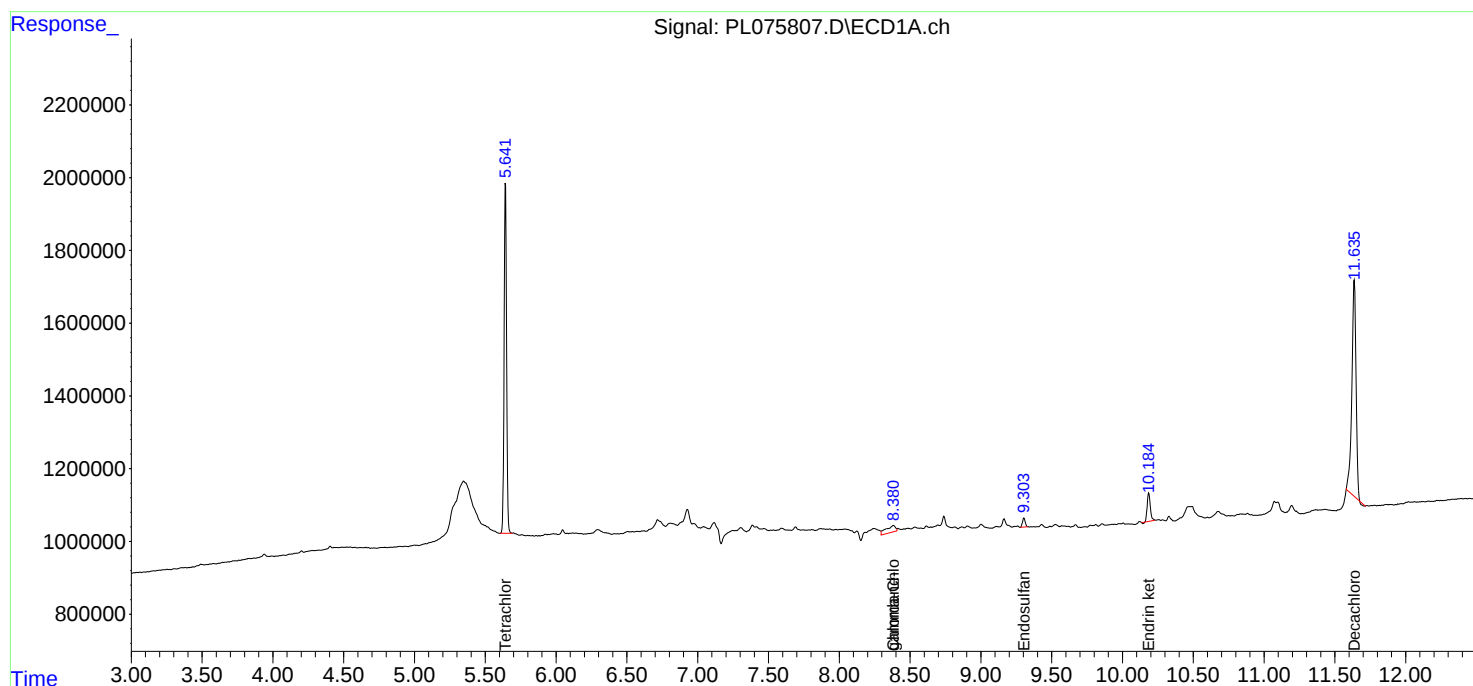


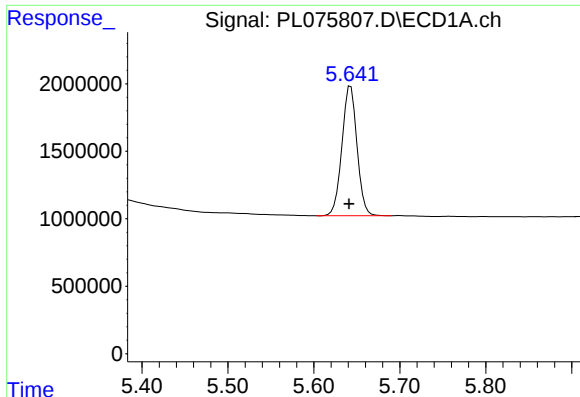

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 11731077
Conc: 17.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

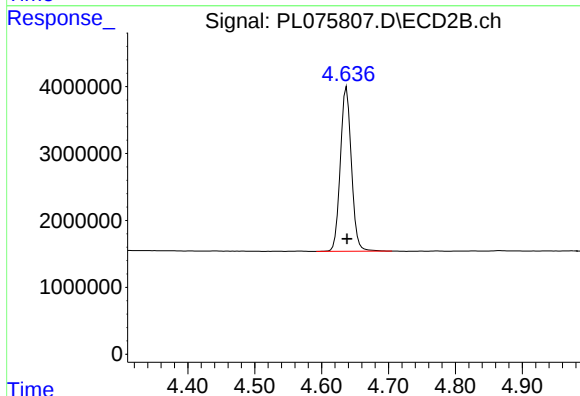


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 28170762
Conc: 16.79 ng/ml

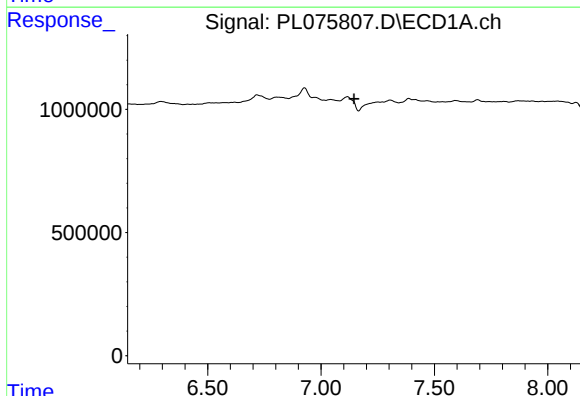


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

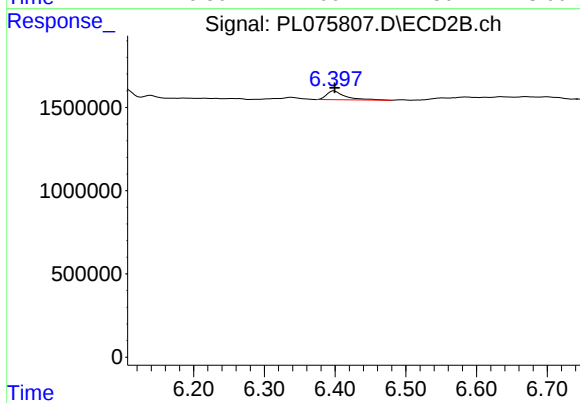

#7 delta-BHC


R.T.: 6.399 min
Delta R.T.: -0.001 min
Response: 983401
Conc: 0.46 ng/ml

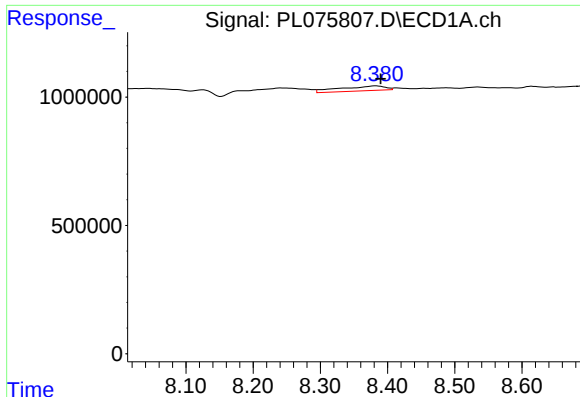

#10 gamma-Chlordane


R.T.: 8.382 min
Delta R.T.: -0.007 min
Response: 871252
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

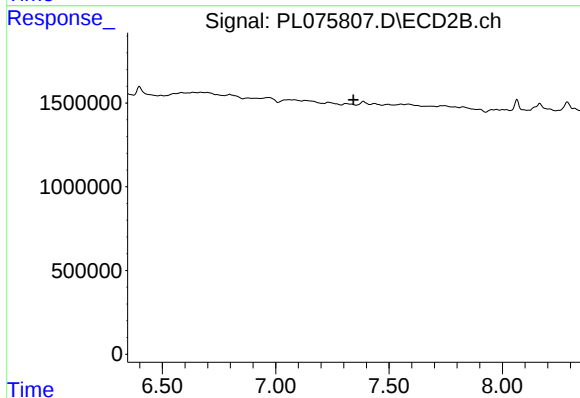


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

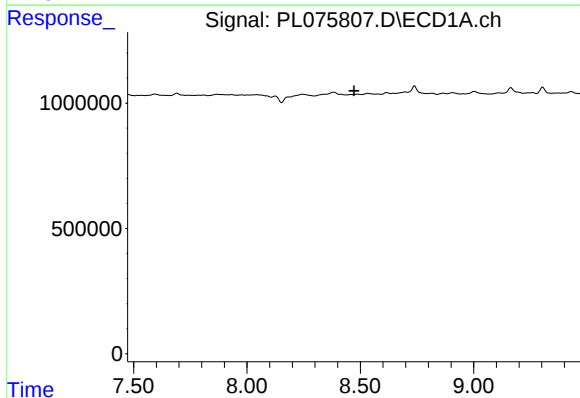


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

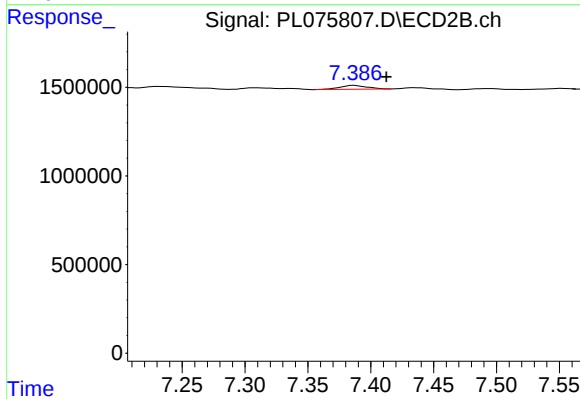

#11 alpha-Chlordane


R.T.: 7.387 min
Delta R.T.: -0.025 min
Response: 319243
Conc: 0.17 ng/ml

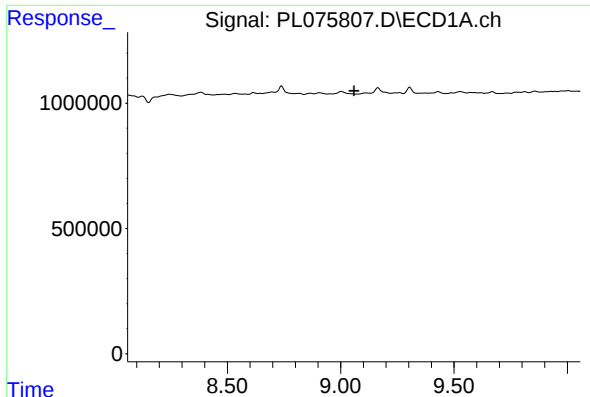

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

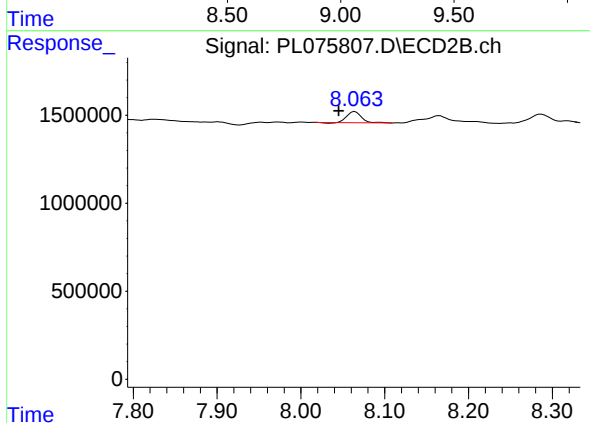


#14 Endrin

R.T.: 8.065 min
Delta R.T.: 0.020 min
Response: 753040
Conc: 0.55 ng/ml

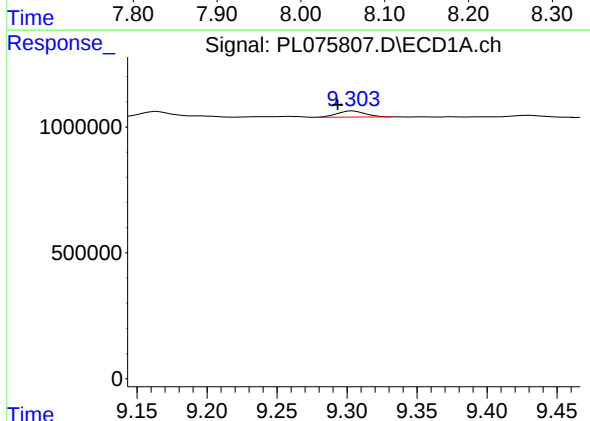


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 340859
Conc: 0.55 ng/ml

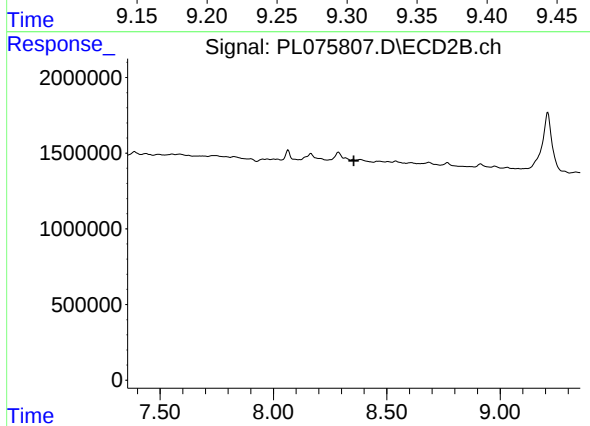

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

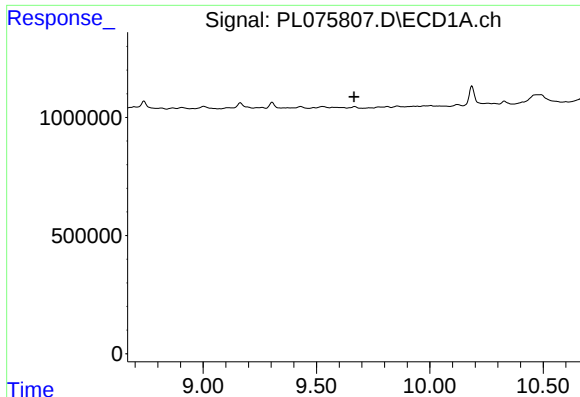

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

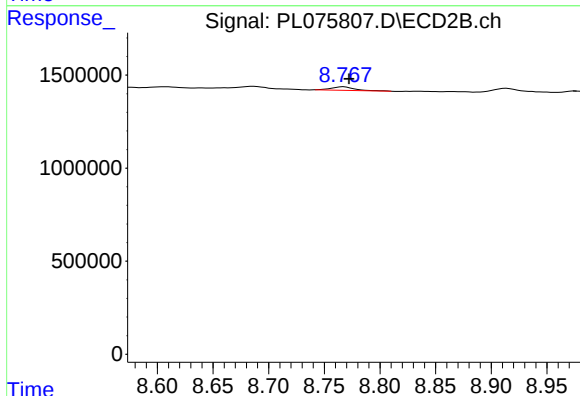


#19 Endosulfan Sulfate

R.T.: 8.767 min
Delta R.T.: -0.005 min
Response: 259734
Conc: 0.18 ng/ml

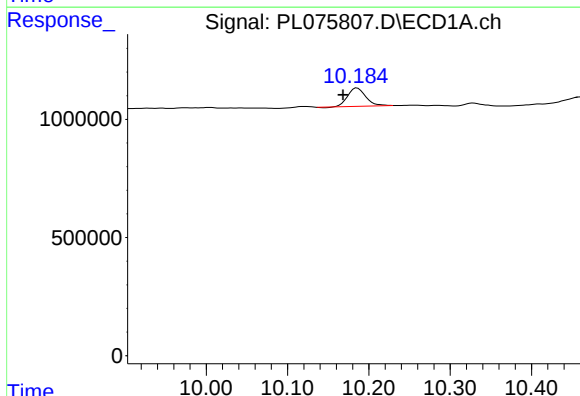


#21 Endrin ketone

R.T.: 10.186 min
Delta R.T.: 0.017 min
Response: 1188343
Conc: 1.69 ng/ml

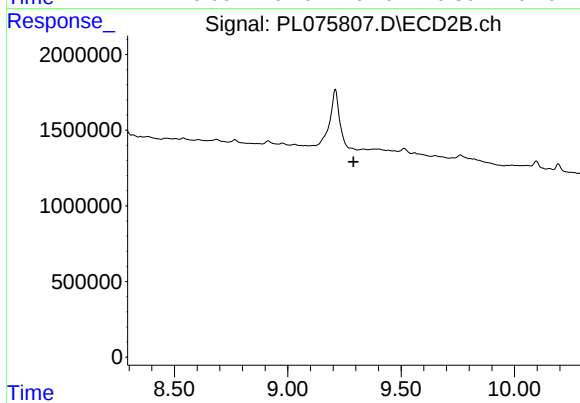

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.290 min
Response: 0
Conc: N.D.

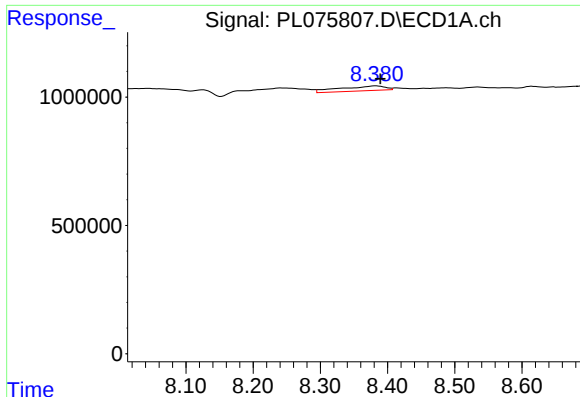

#25 Chlordane-3


R.T.: 8.382 min
Delta R.T.: -0.007 min
Response: 871252
Conc: 8.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

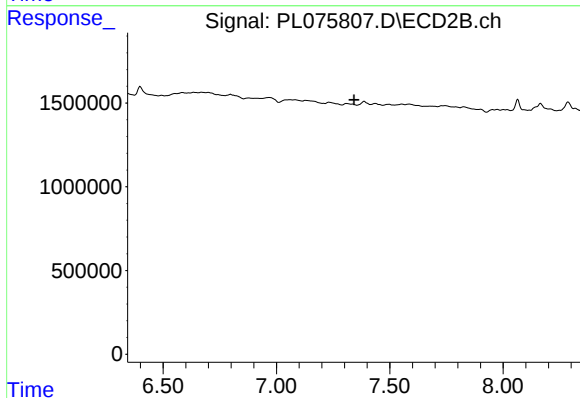


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

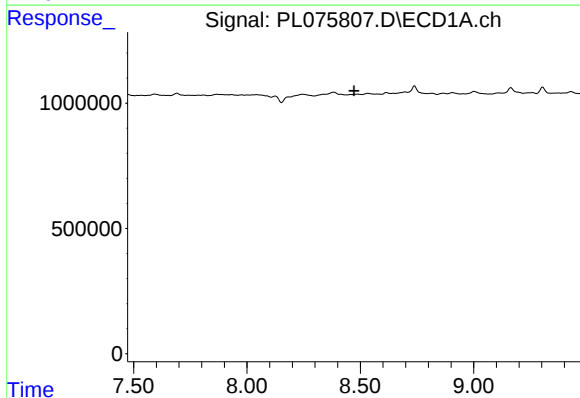


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

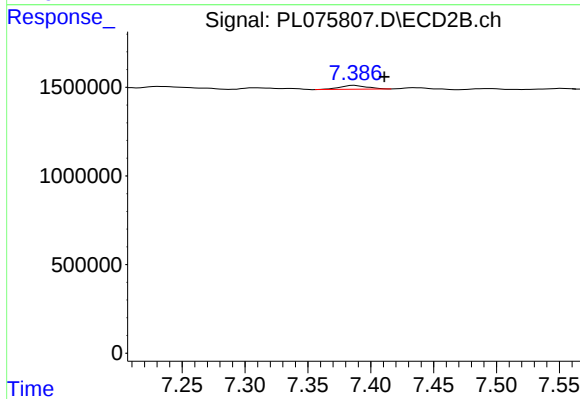

#26 Chlordane-4


R.T.: 7.387 min
Delta R.T.: -0.024 min
Response: 319243
Conc: 1.73 ng/ml

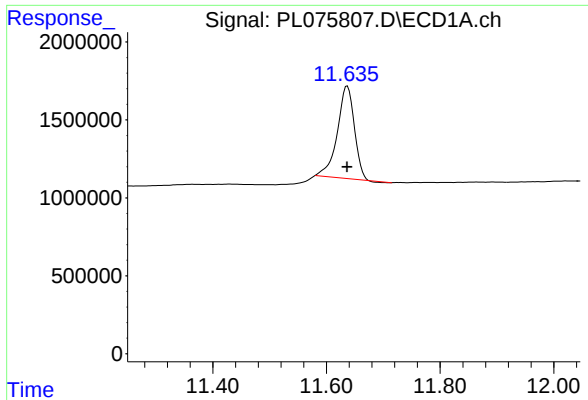

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: 0.000 min
Response: 12323213
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

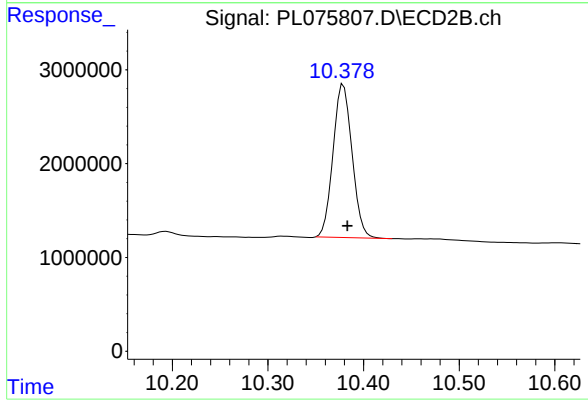

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 22510447
Conc: 15.98 ng/ml