

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061622\
 Data File : PL075825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2022 09:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 23:26:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.636	12449593	30348753	18.447	18.084
28)	SA Decachlor...	11.631	10.378	10692652	21353768	17.465	15.156
Target Compounds							
7)	B delta-BHC	0.000	6.398	0	414767	N.D.	0.194 #
9)	A Endosulfan I	8.538	0.000	513920	0	0.735	N.D. #
10)	B gamma-Chl...	8.385	0.000	328004	0	0.422	N.D. #
11)	B alpha-Chl...	8.501f	7.386f	667896	169732	0.876	0.093 #
14)	MA Endrin	0.000	8.063f	0	293704	N.D.	0.215 #
15)	B Endosulfa...	9.303	0.000	300580	0	0.483	N.D. #
19)	B Endosulfa...	0.000	8.767	0	227494	N.D.	0.155 #
21)	B Endrin ke...	10.185f	0.000	464805	0	0.661	N.D. #
25)	Chlordane-3	8.385	0.000	328004	0	3.177	N.D. #
26)	Chlordane-4	8.501f	7.386f	667896	169732	5.273	0.922 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061622\
Data File : PL075825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2022 09:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 23:26:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

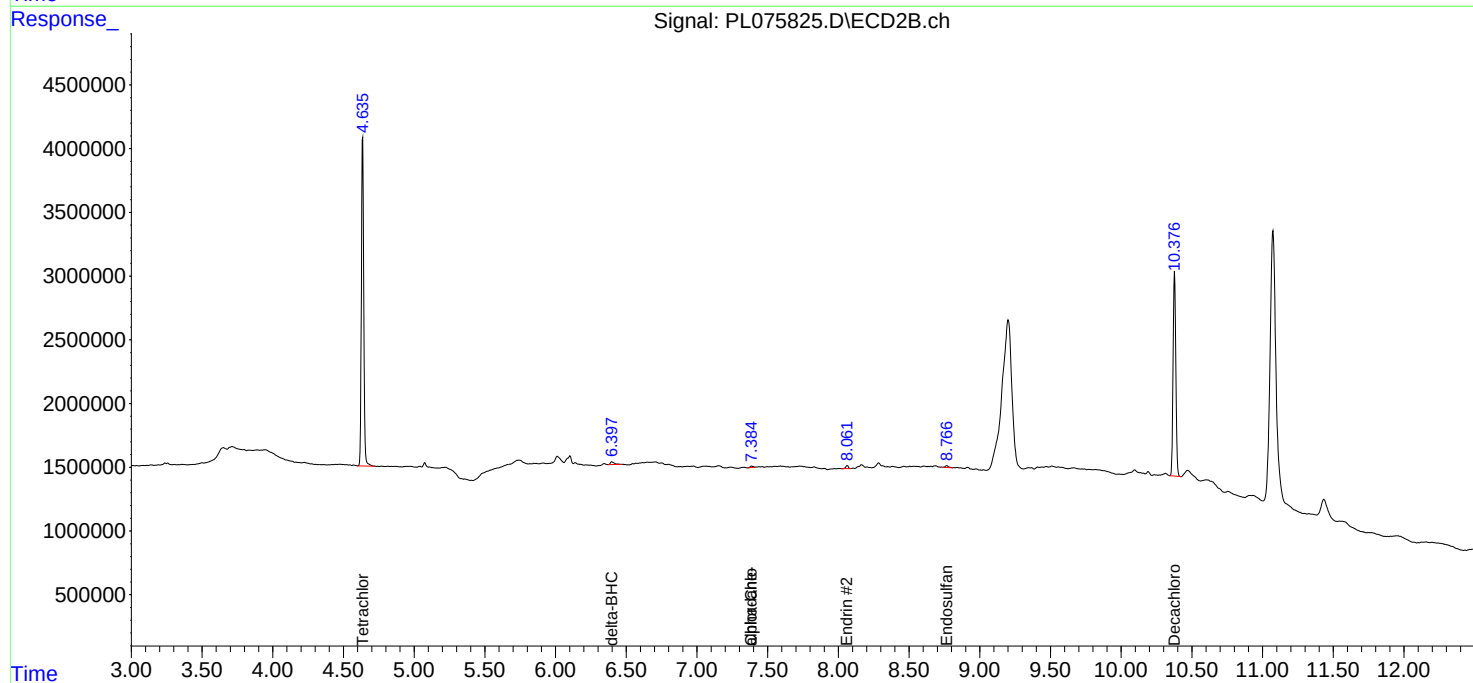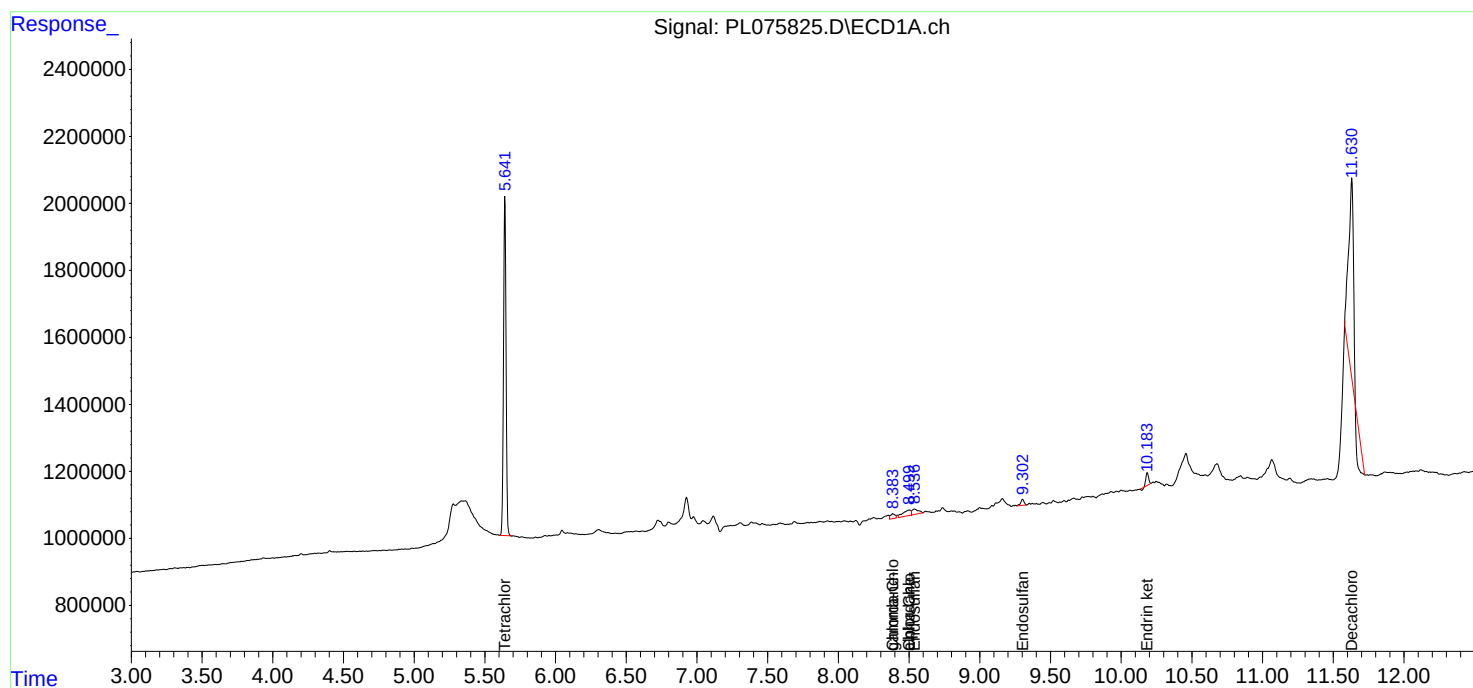


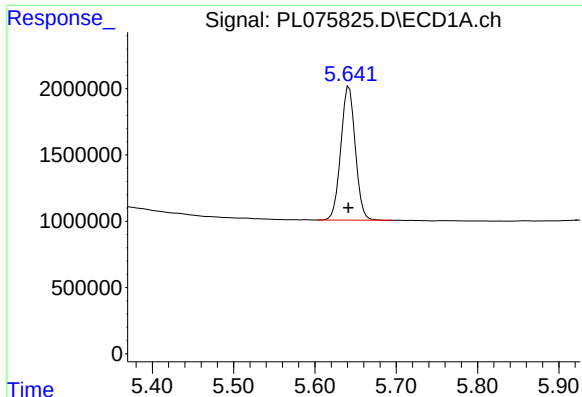

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.001 min
Response: 12449593
Conc: 18.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

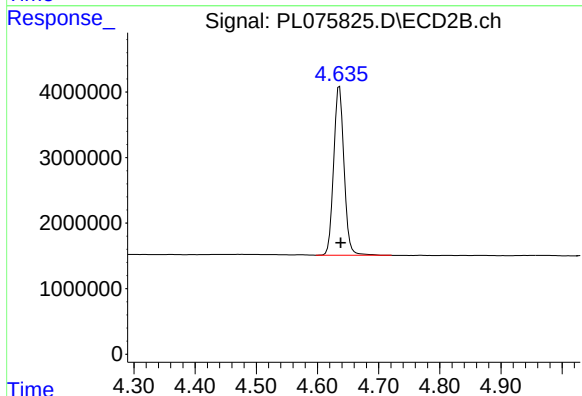


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 30348753
Conc: 18.08 ng/ml

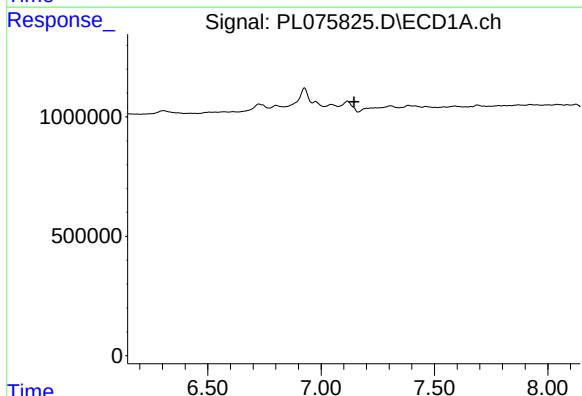


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

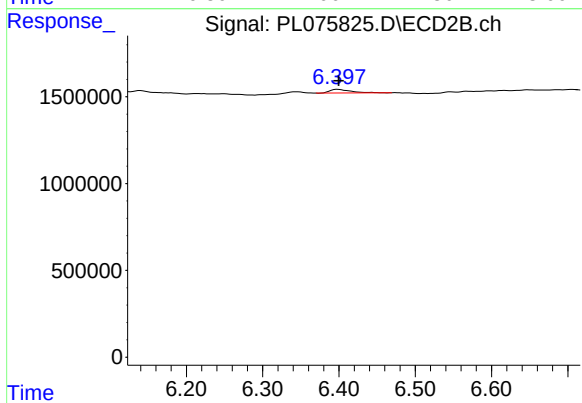

#7 delta-BHC


R.T.: 6.398 min
Delta R.T.: -0.001 min
Response: 414767
Conc: 0.19 ng/ml

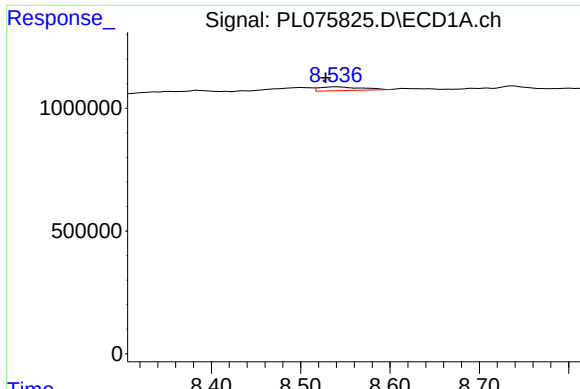

#9 Endosulfan I


R.T.: 8.538 min
Delta R.T.: 0.010 min
Response: 513920
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

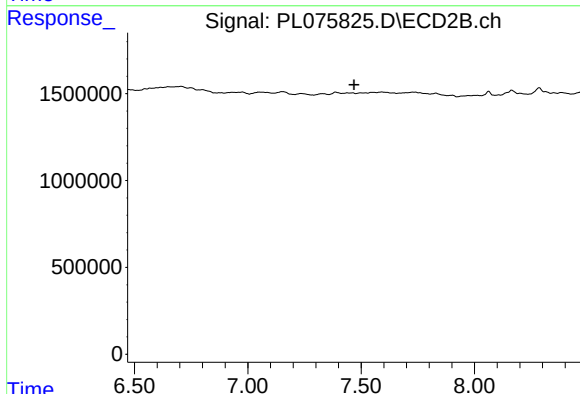


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

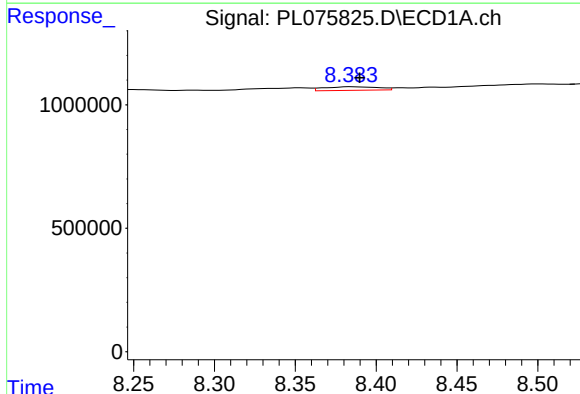


#10 gamma-Chlordane

R.T.: 8.385 min
Delta R.T.: -0.005 min
Response: 328004
Conc: 0.42 ng/ml

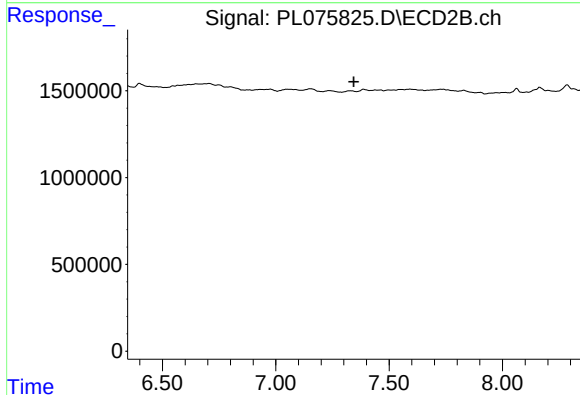

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

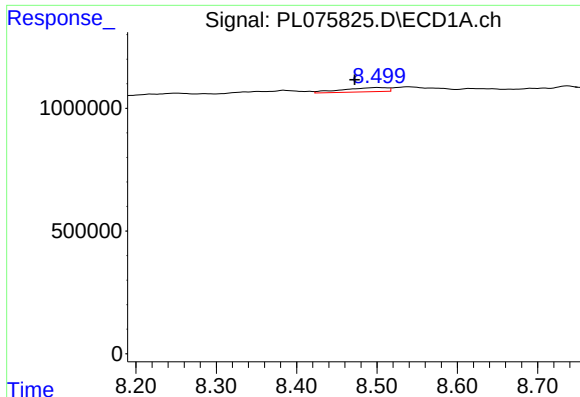

#11 alpha-Chlordane


R.T.: 8.501 min
Delta R.T.: 0.028 min
Response: 667896
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

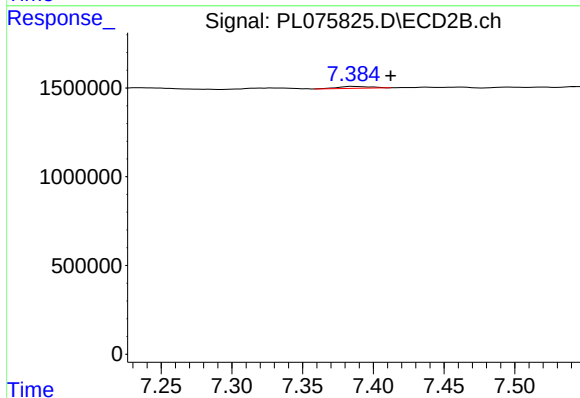


#11 alpha-Chlordane

R.T.: 7.386 min
Delta R.T.: -0.026 min
Response: 169732
Conc: 0.09 ng/ml

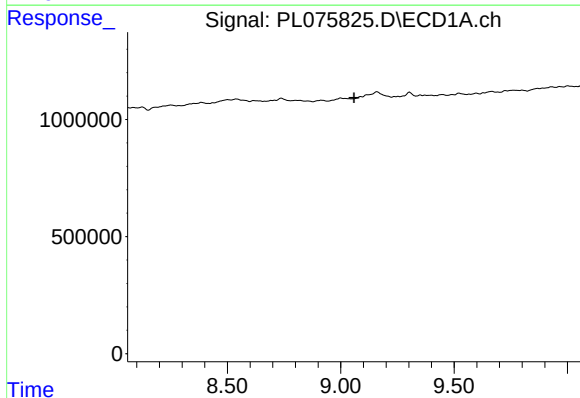


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

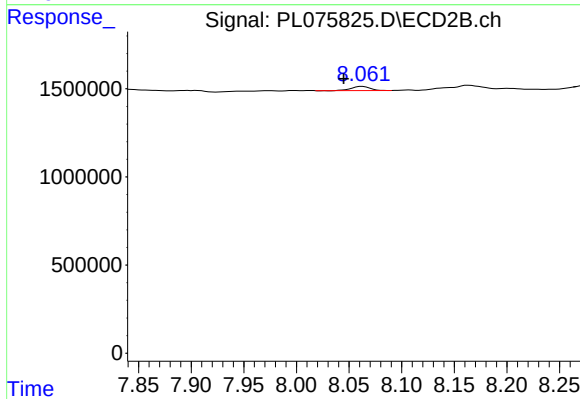

#14 Endrin


R.T.: 8.063 min
Delta R.T.: 0.018 min
Response: 293704
Conc: 0.21 ng/ml

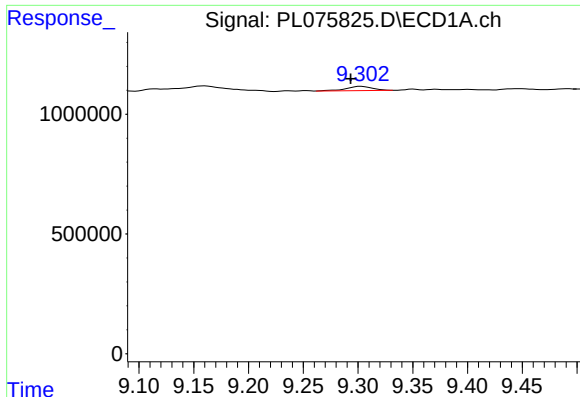

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.010 min
Response: 300580
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

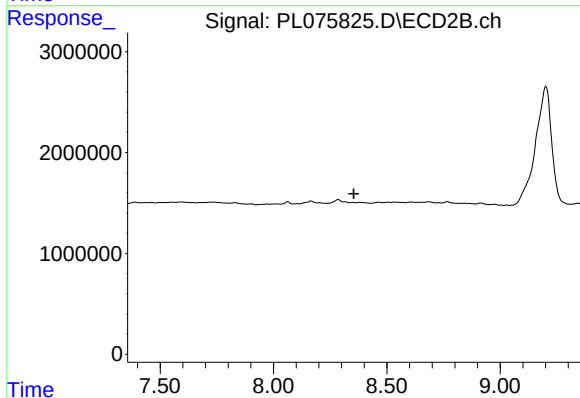


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

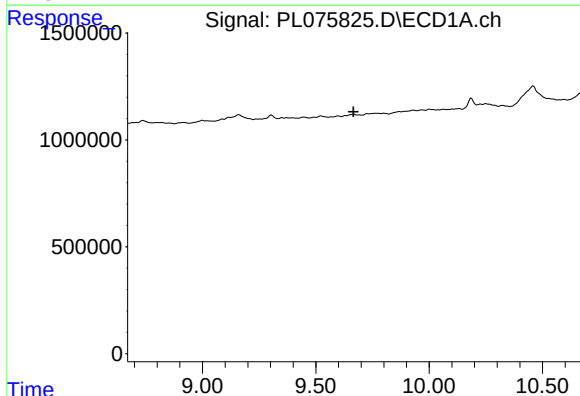


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.666 min
Response: 0
Conc: N.D.

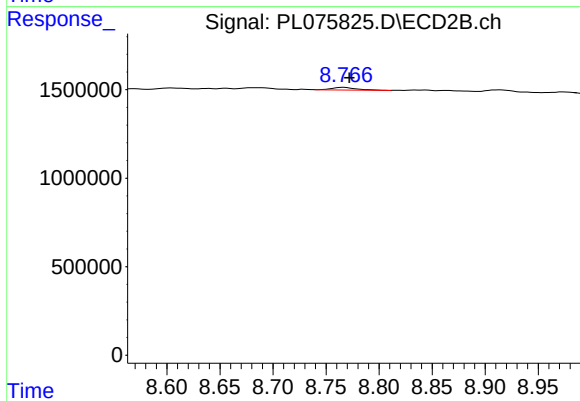

#19 Endosulfan Sulfate


R.T.: 8.767 min
Delta R.T.: -0.005 min
Response: 227494
Conc: 0.15 ng/ml

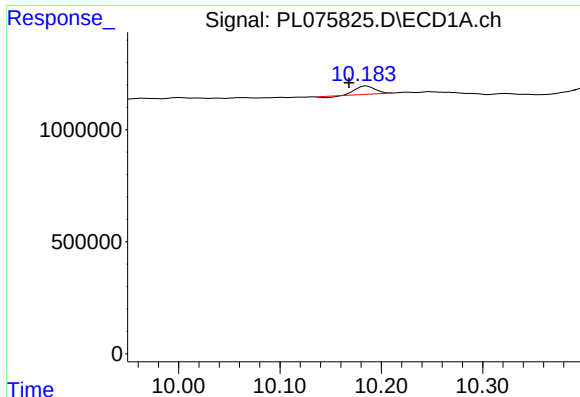

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 464805
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

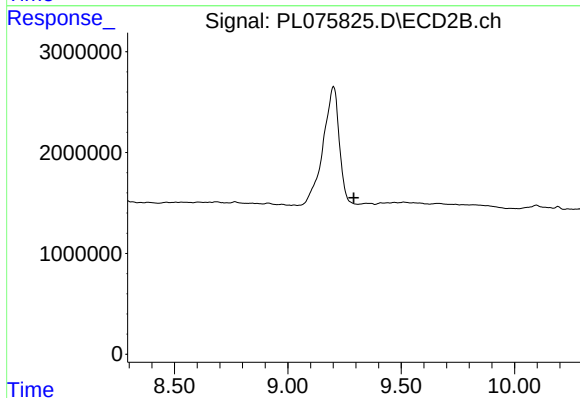


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

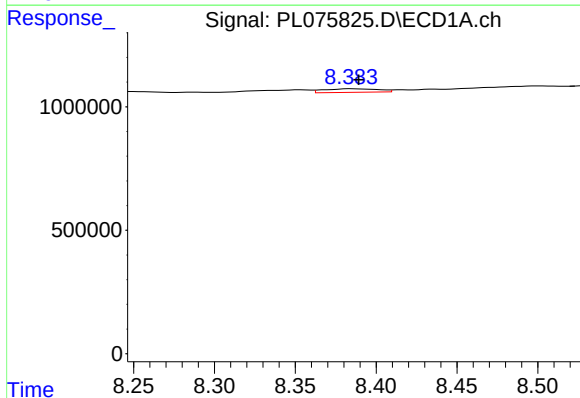


#25 Chlordane-3

R.T.: 8.385 min
Delta R.T.: -0.004 min
Response: 328004
Conc: 3.18 ng/ml

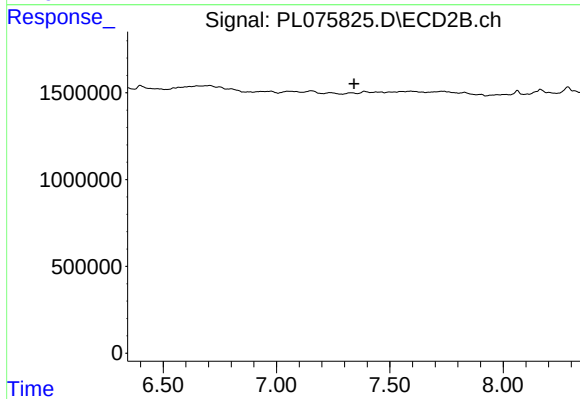

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

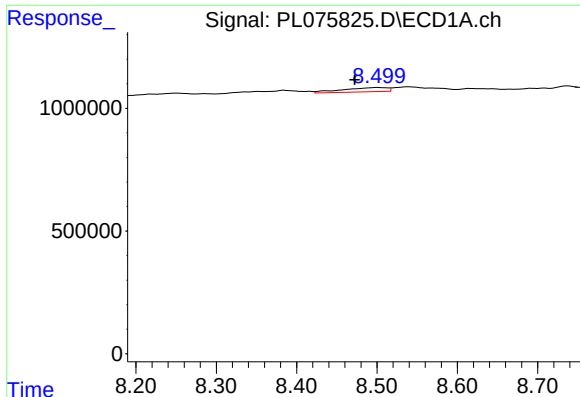

#26 Chlordane-4


R.T.: 8.501 min
Delta R.T.: 0.028 min
Response: 667896
Conc: 5.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

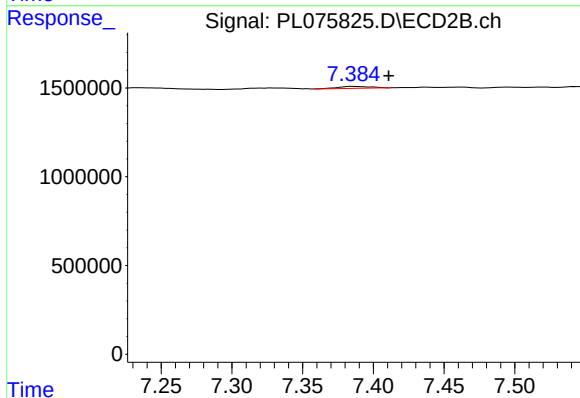


#26 Chlordane-4

R.T.: 7.386 min
Delta R.T.: -0.025 min
Response: 169732
Conc: 0.92 ng/ml

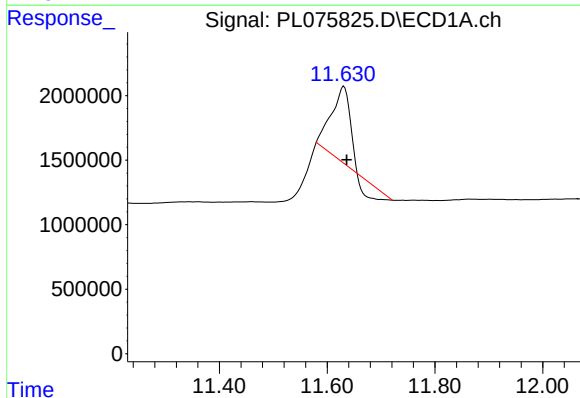

#28 Decachlorobiphenyl

R.T.: 11.631 min
Delta R.T.: -0.005 min
Response: 10692652
Conc: 17.47 ng/ml

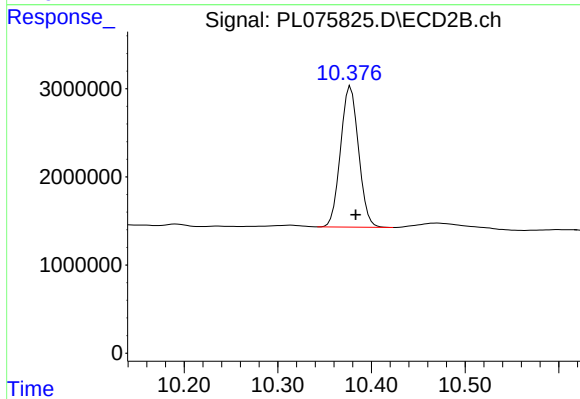

#28 Decachlorobiphenyl

R.T.: 10.378 min
Delta R.T.: -0.005 min
Response: 21353768
Conc: 15.16 ng/ml