

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061622\
 Data File : PL075828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2022 12:44
 Operator : AR\AJ
 Sample : N3189-05RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 23:29:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.635	2857682	7092794	4.234	4.226
28)	SA Decachlor...	11.633	10.376	5423228	8616703	8.858	6.116 #
Target Compounds							
7)	B delta-BHC	0.000	6.400	0	377531	N.D.	0.176 #
8)	B Heptachlo...	8.124	0.000	950195	0	1.229	N.D. #
10)	B gamma-Chl...	8.381	0.000	411800	0	0.530	N.D. #
13)	MA Dieldrin	0.000	7.737f	0	80951	N.D.	0.048 #
14)	MA Endrin	0.000	8.061f	0	453502	N.D.	0.332 #
15)	B Endosulfa...	9.304	0.000	284531	0	0.457	N.D. #
21)	B Endrin ke...	10.184f	0.000	573907	0	0.816	N.D. #
25)	Chlordane-3	8.381	0.000	411800	0	3.988	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061622\
Data File : PL075828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2022 12:44
Operator : AR\AJ
Sample : N3189-05RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 23:29:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

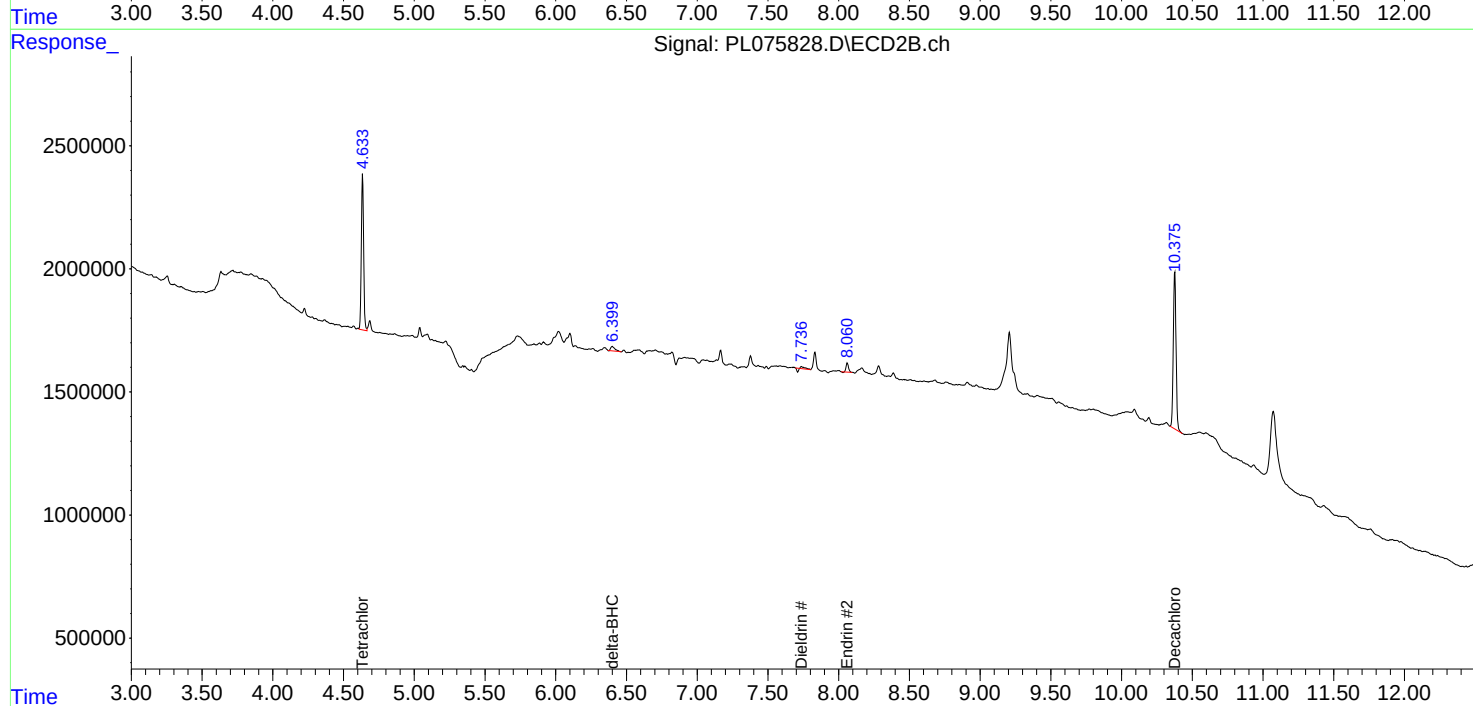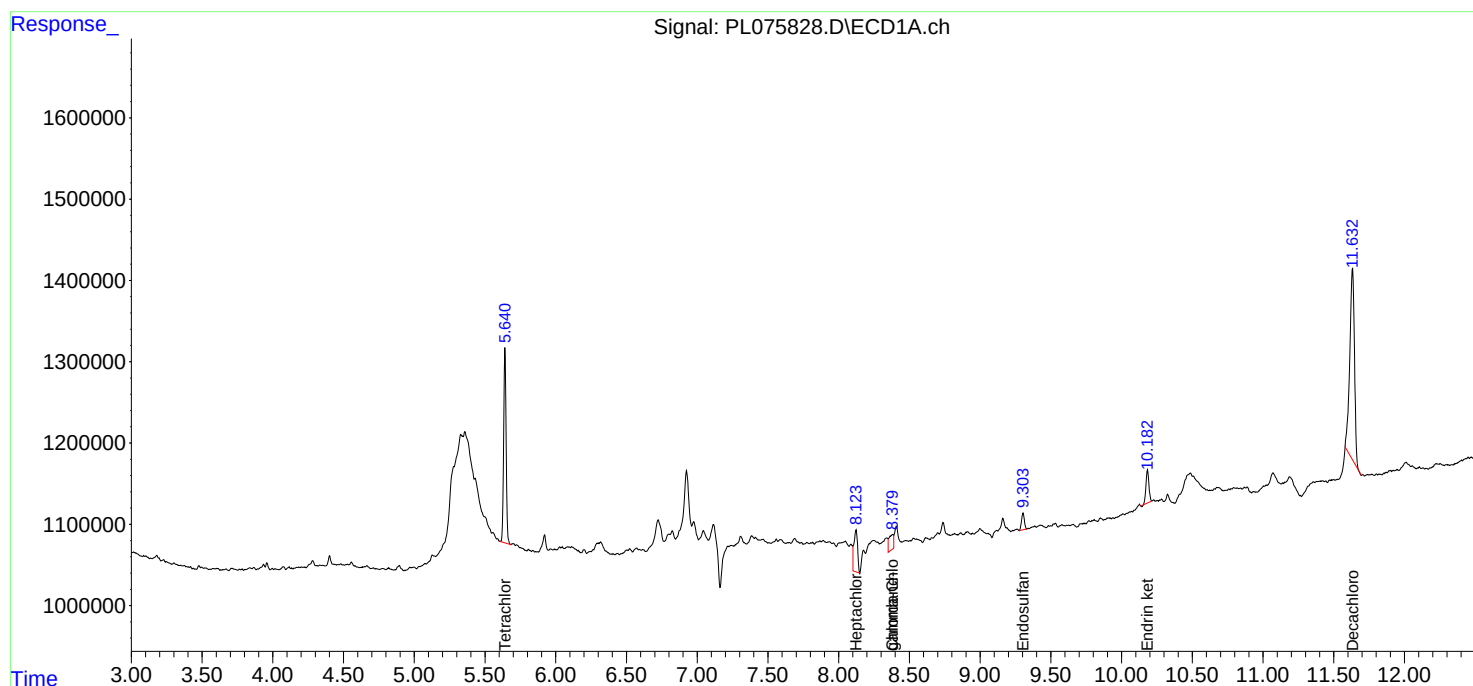


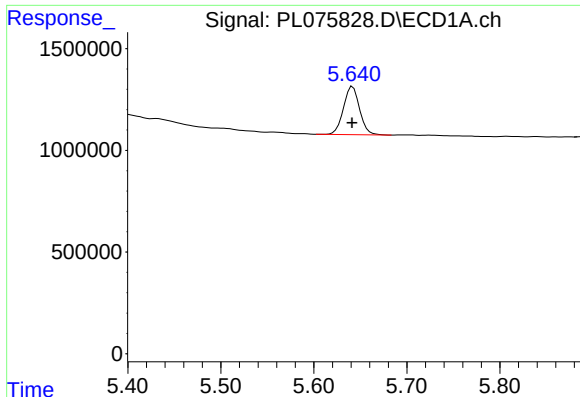

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 2857682
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

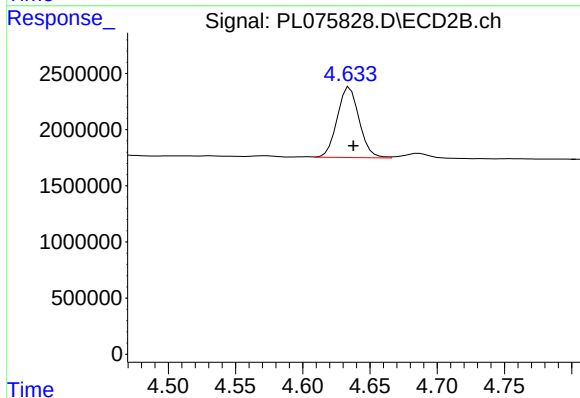


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 7092794
Conc: 4.23 ng/ml

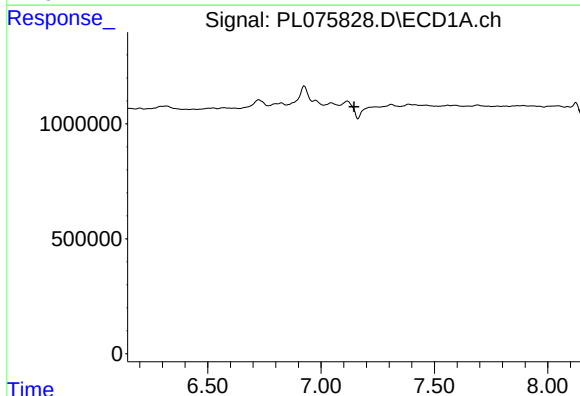


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

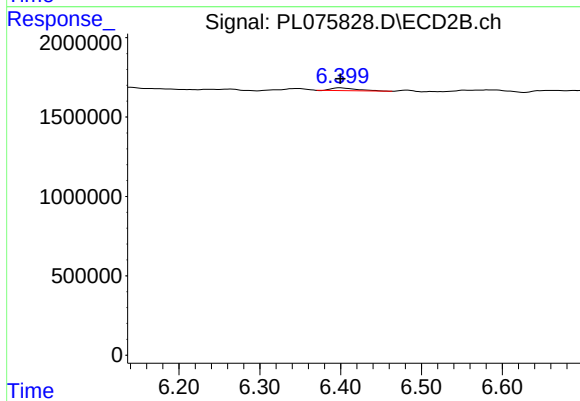

#7 delta-BHC


R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 377531
Conc: 0.18 ng/ml

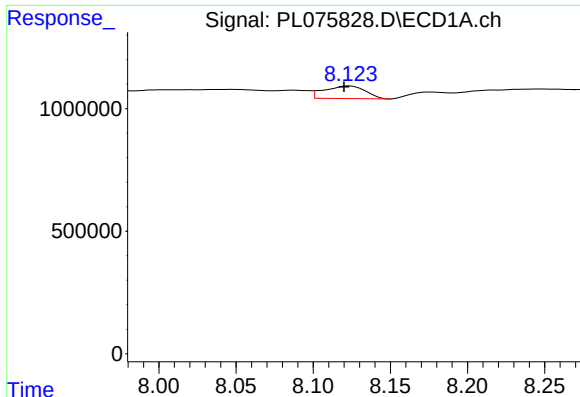

#8 Heptachlor epoxide


R.T.: 8.124 min
Delta R.T.: 0.004 min
Response: 950195
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

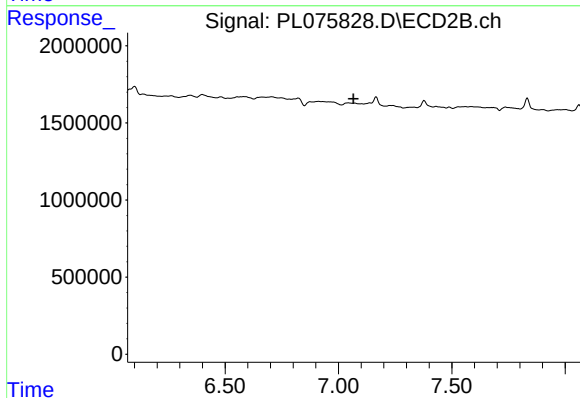


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

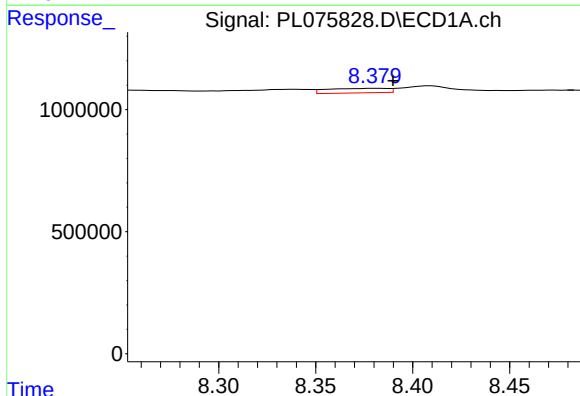


#10 gamma-Chlordane

R.T.: 8.381 min
Delta R.T.: -0.009 min
Response: 411800
Conc: 0.53 ng/ml

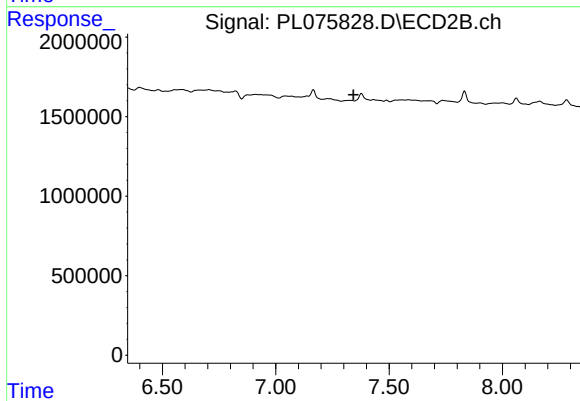

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

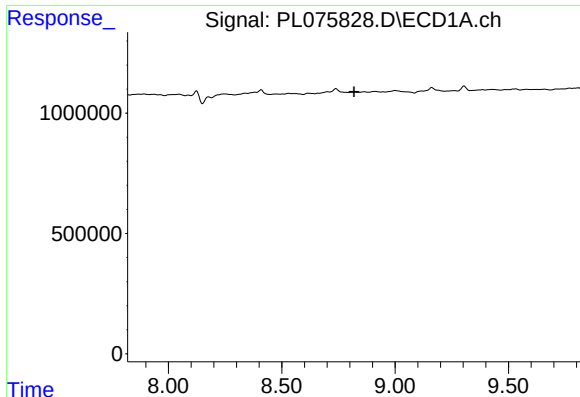

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

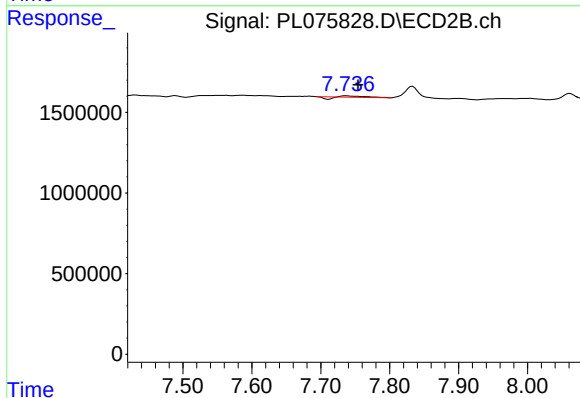


#13 Dieldrin

R.T.: 7.737 min
Delta R.T.: -0.017 min
Response: 80951
Conc: 0.05 ng/ml

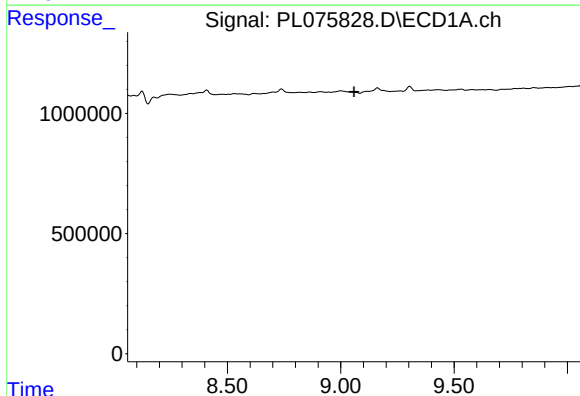


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

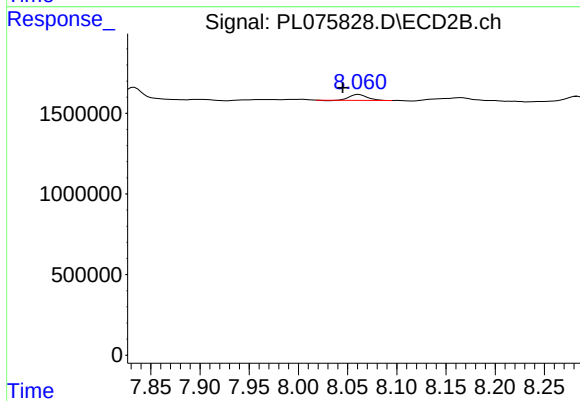

#14 Endrin


R.T.: 8.061 min
Delta R.T.: 0.016 min
Response: 453502
Conc: 0.33 ng/ml

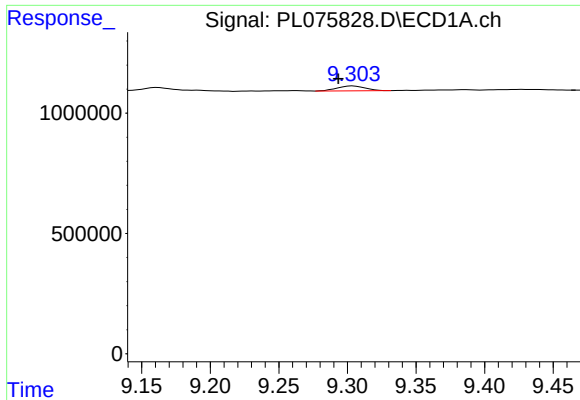

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 284531
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

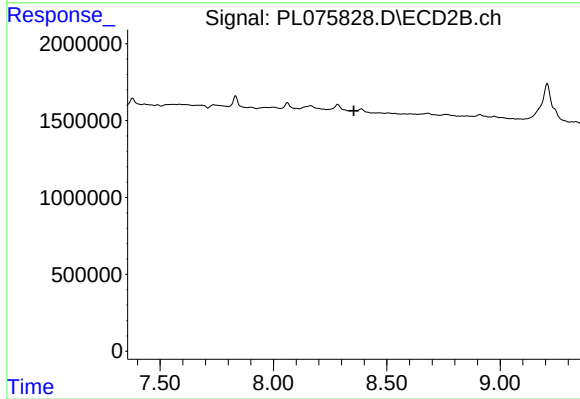


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

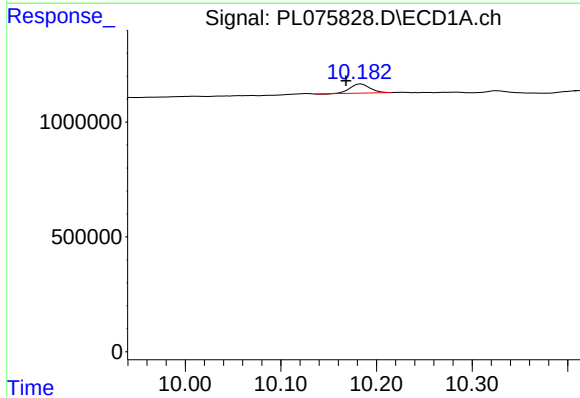


#21 Endrin ketone

R.T.: 10.184 min
Delta R.T.: 0.015 min
Response: 573907
Conc: 0.82 ng/ml

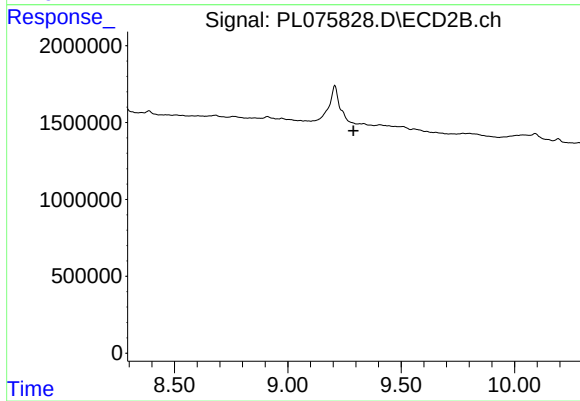

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

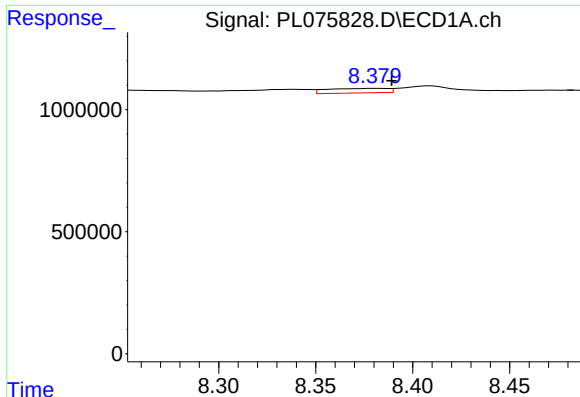

#25 Chlordane-3


R.T.: 8.381 min
Delta R.T.: -0.009 min
Response: 411800
Conc: 3.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

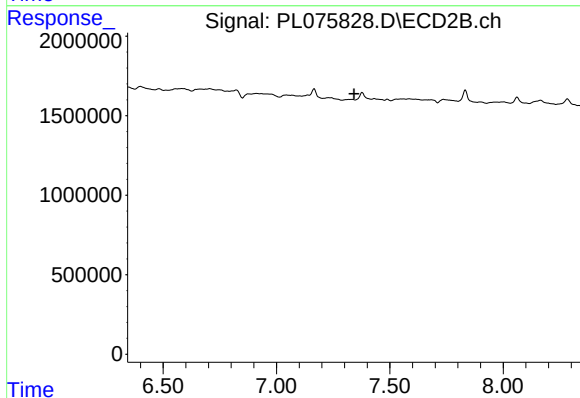


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

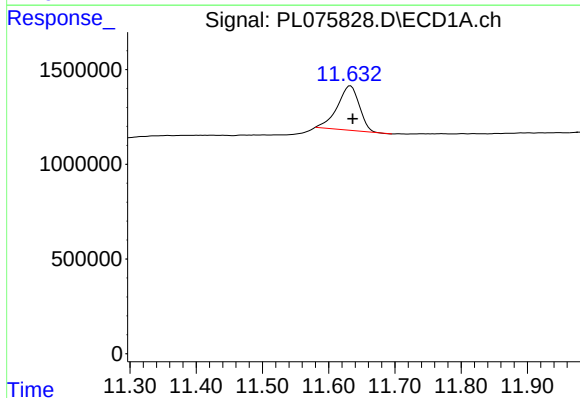

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: -0.003 min
Response: 5423228
Conc: 8.86 ng/ml

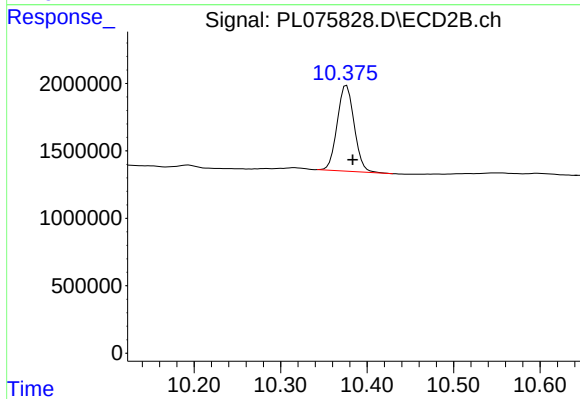

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: -0.007 min
Response: 8616703
Conc: 6.12 ng/ml