

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061622\
 Data File : PL075828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2022 12:44
 Operator : AR\AJ
 Sample : N3189-05RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220423-SPLP-AMENDED-COMPOSITE-CRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/20/2022
 Supervised By :Ankita Jodhani 06/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 23:29:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.642	4.635	2857682	7092794	4.234	4.226
28) SA Decachlor...	11.632	10.376	5358704	8616703	8.753m	6.116 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061622\
Data File : PL075828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2022 12:44
Operator : AR\AJ
Sample : N3189-05RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20220423-SPLP-AMENDED-COMPOSITE-CRE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/20/2022
Supervised By : Ankita Jodhani 06/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 23:29:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

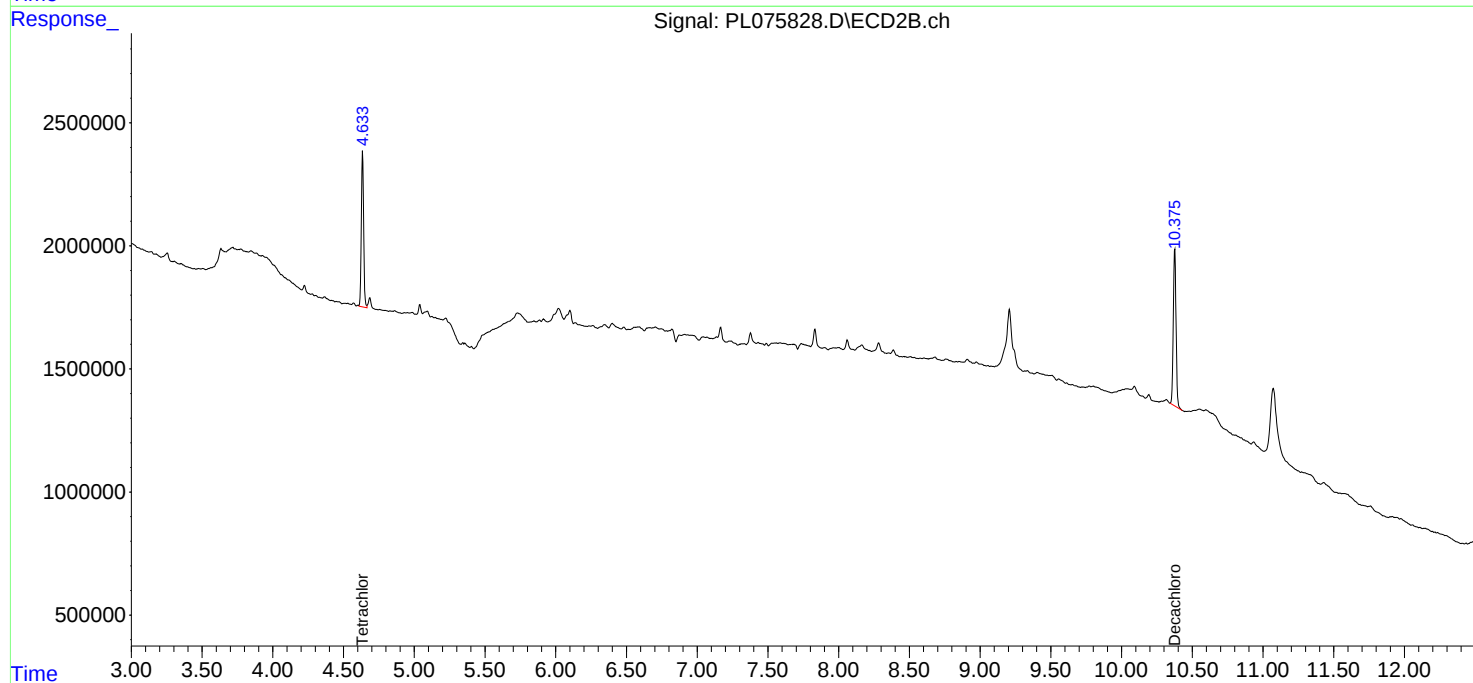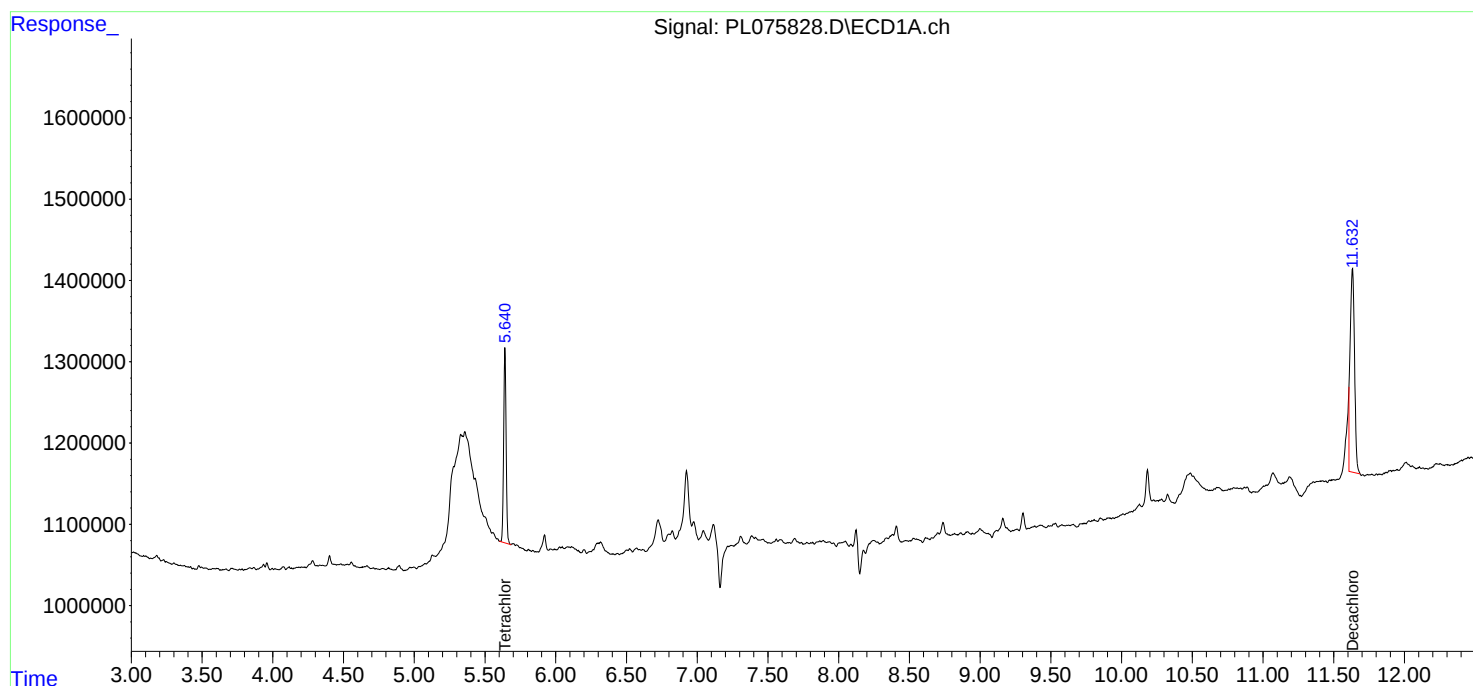

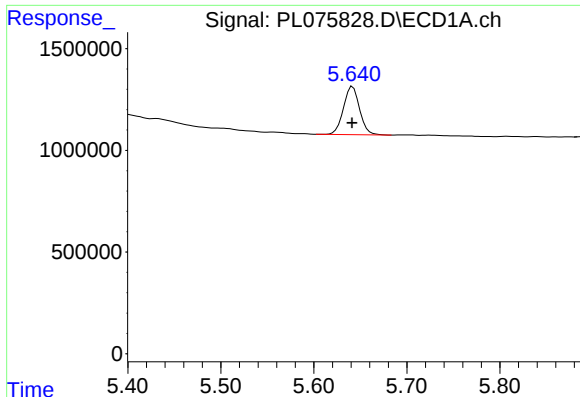


#1 Tetrachloro-m-xylene

R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 2857682
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220423-SPLP-AMENDED-COMPOSITE-CRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/20/2022
Supervised By :Ankita Jodhani 06/20/2022

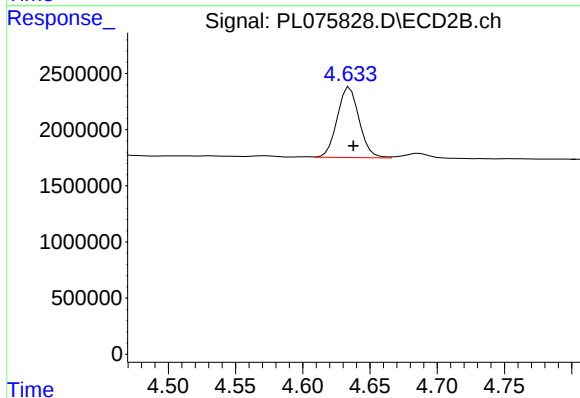


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 7092794
Conc: 4.23 ng/ml

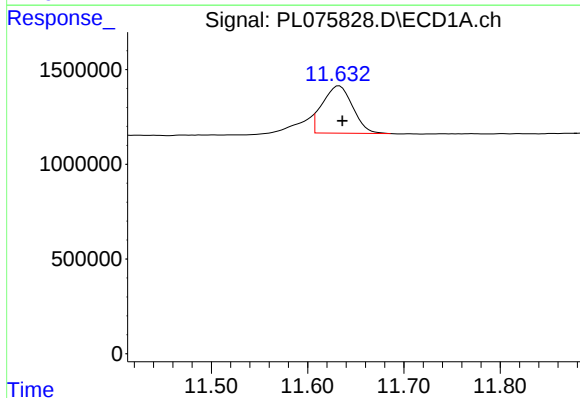

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: -0.005 min
Response: 5358704
Conc: 8.75 ng/ml m

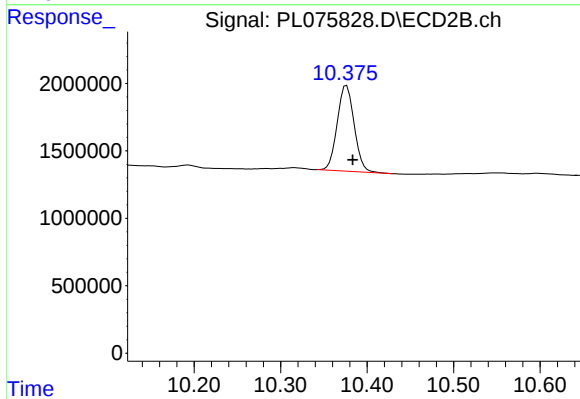

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: -0.007 min
Response: 8616703
Conc: 6.12 ng/ml