

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
 Data File : PL049535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 08:44
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:08:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	4.305	0.000	26038096	0	1.470	N.D.	#
6) B	beta-BHC	4.305f	0.000	26038096	0	3.747	N.D.	#
7) B	delta-BHC	4.500f	0.000	1641454	0	0.102	N.D.	#
17) MA	4,4'-DDT	6.166	0.000	279.7E6	0	22.718	N.D.	#
18) B	Endrin al...	6.251	0.000	245.0E6	0	22.386	N.D.	#
20) A	Methoxychlor	6.736	0.000	354.2E6	0	55.218	N.D.	#
21) B	Endrin ke...	6.944	0.000	95799922	0	6.731	N.D.	#
22)	Mirex	7.106	0.000	31702863	0	3.009	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
Data File : PL049535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 08:44
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:08:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

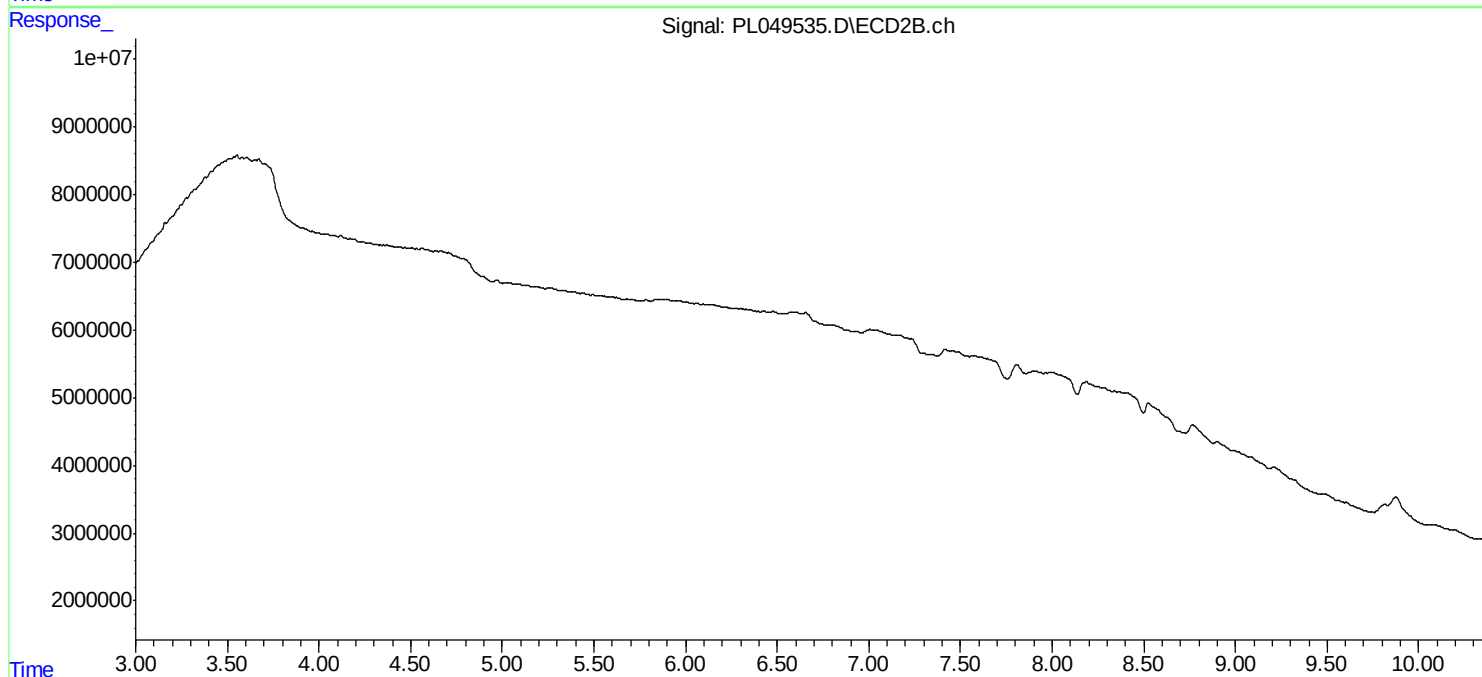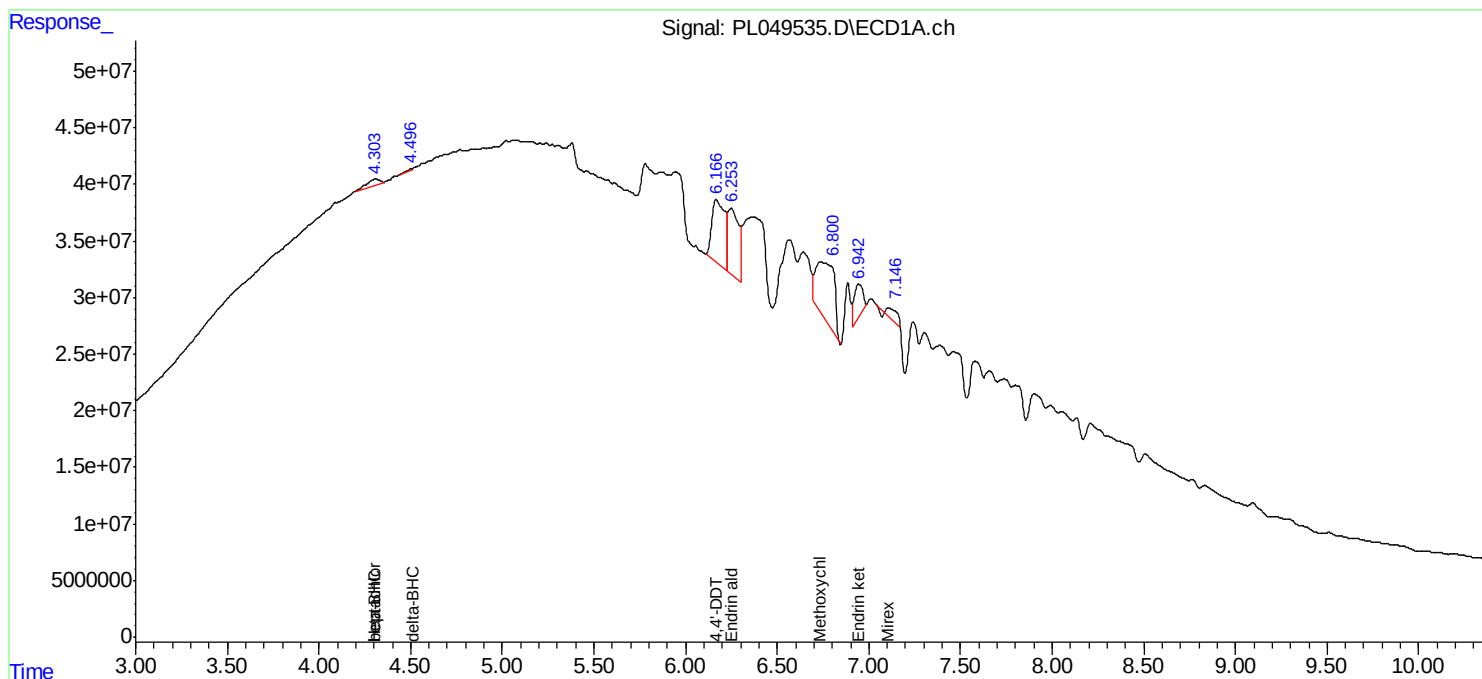


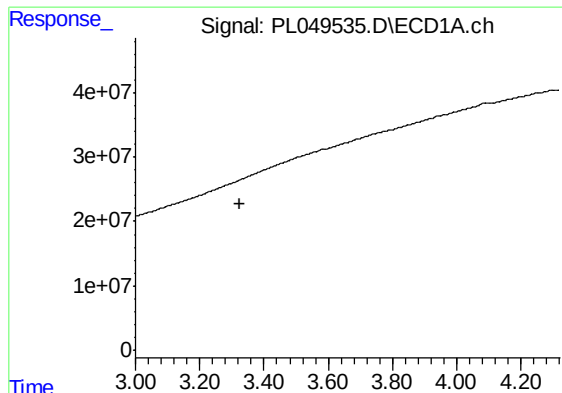

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

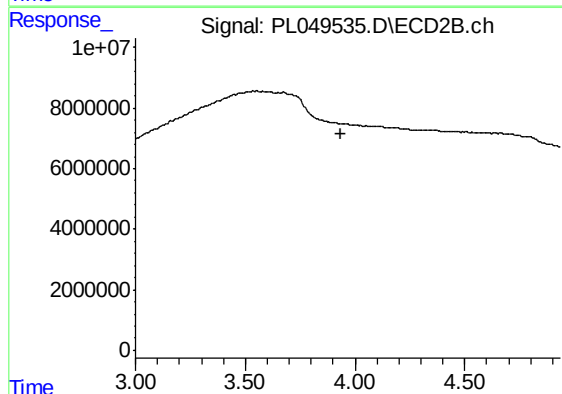


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

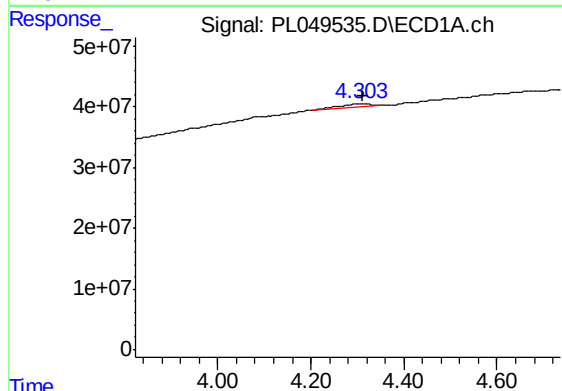


#4 Heptachlor

R.T.: 4.305 min
Delta R.T.: -0.007 min
Response: 26038096
Conc: 1.47 ng/ml

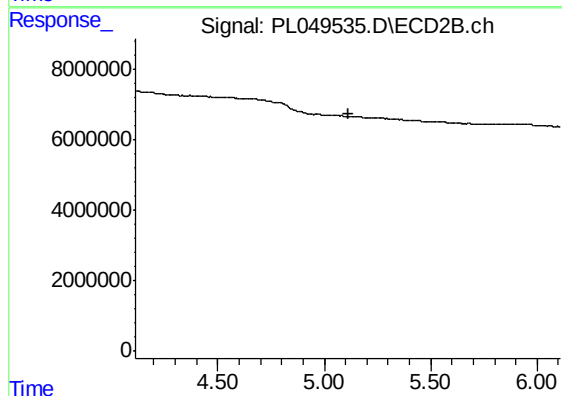

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

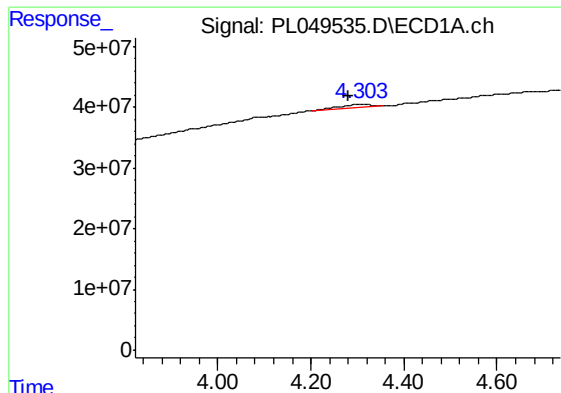

#6 beta-BHC


R.T.: 4.305 min
Delta R.T.: 0.023 min
Response: 26038096
Conc: 3.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

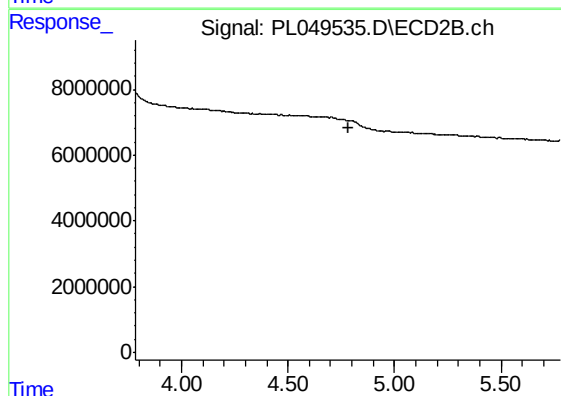


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

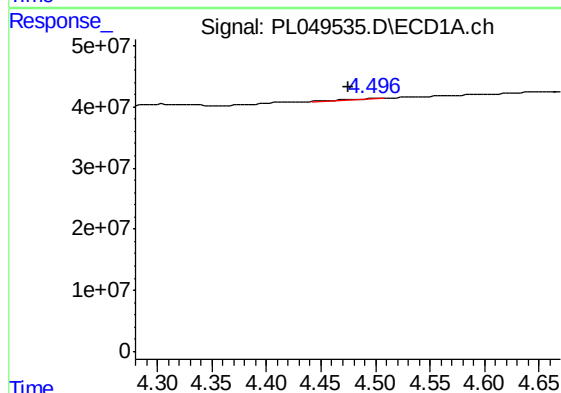


#7 delta-BHC

R.T.: 4.500 min
Delta R.T.: 0.025 min
Response: 1641454
Conc: 0.10 ng/ml

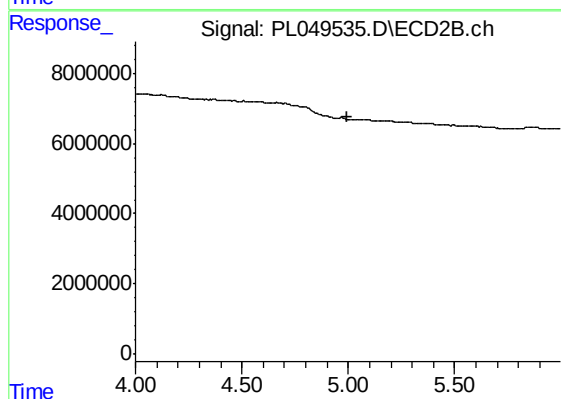

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

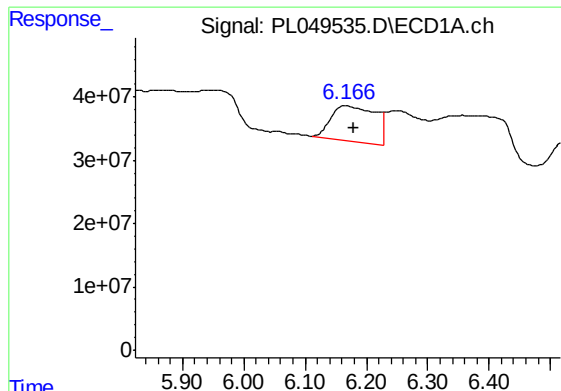

#17 4,4'-DDT


R.T.: 6.166 min
Delta R.T.: -0.013 min
Response: 279715560
Conc: 22.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

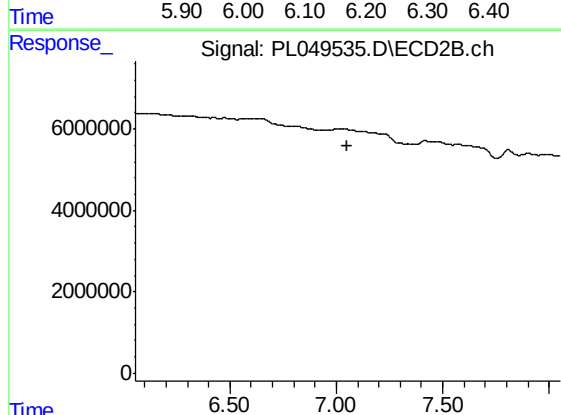


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

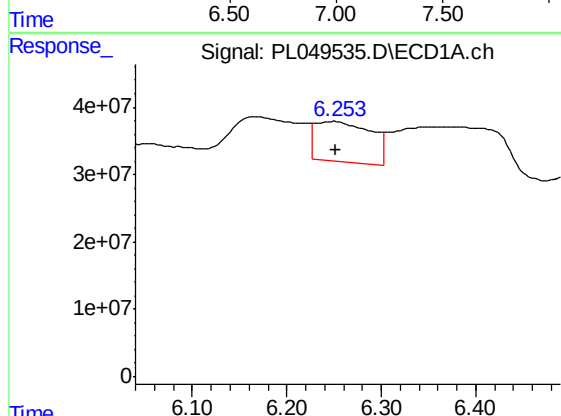


#18 Endrin aldehyde

R.T.: 6.251 min
Delta R.T.: -0.001 min
Response: 244988681
Conc: 22.39 ng/ml

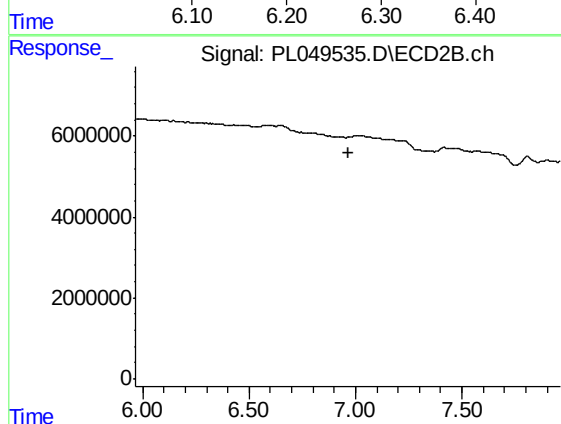

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.965 min
Response: 0
Conc: N.D.

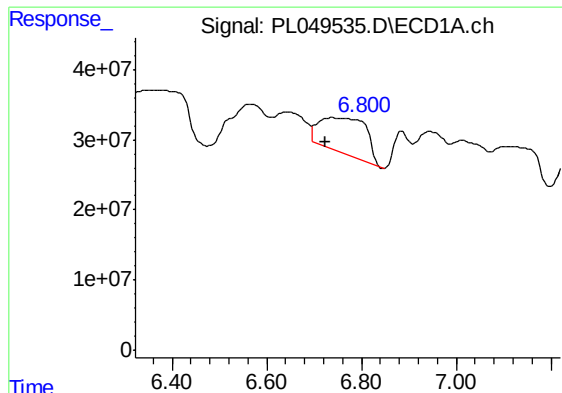

#20 Methoxychlor


R.T.: 6.736 min
Delta R.T.: 0.011 min
Response: 354152793
Conc: 55.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

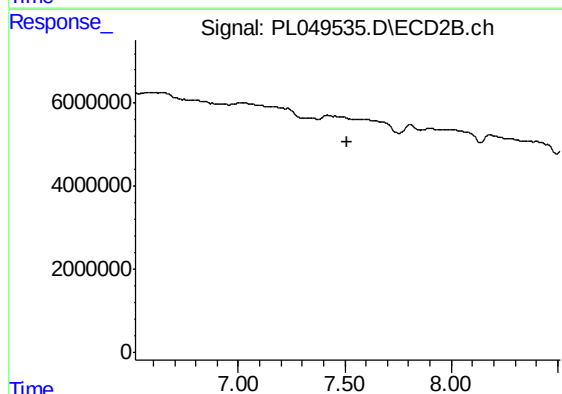


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

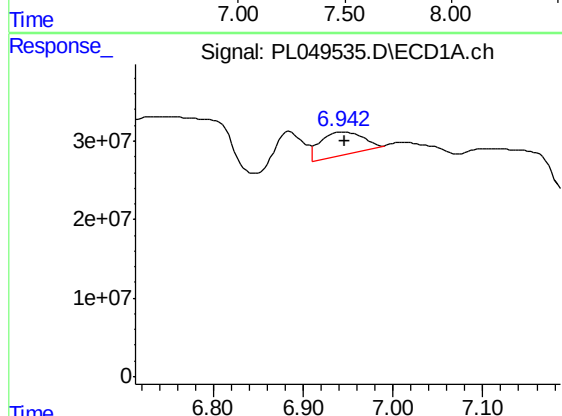


#21 Endrin ketone

R.T.: 6.944 min
Delta R.T.: -0.002 min
Response: 95799922
Conc: 6.73 ng/ml

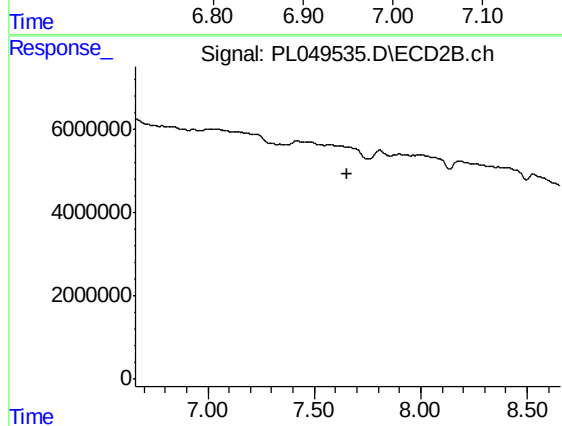

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

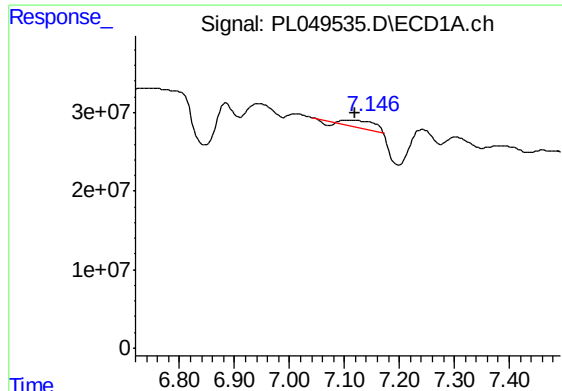

#22 Mirex


R.T.: 7.106 min
Delta R.T.: -0.014 min
Response: 31702863
Conc: 3.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

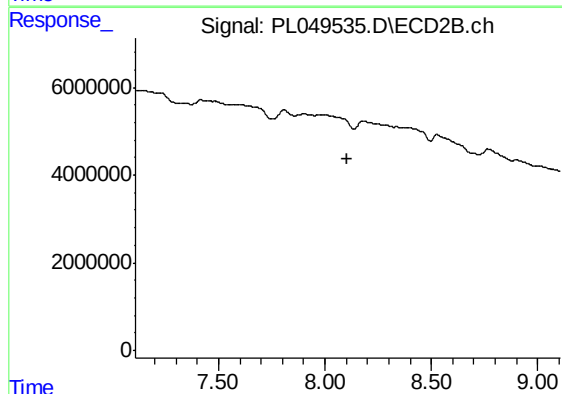


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.107 min
Response: 0
Conc: N.D.

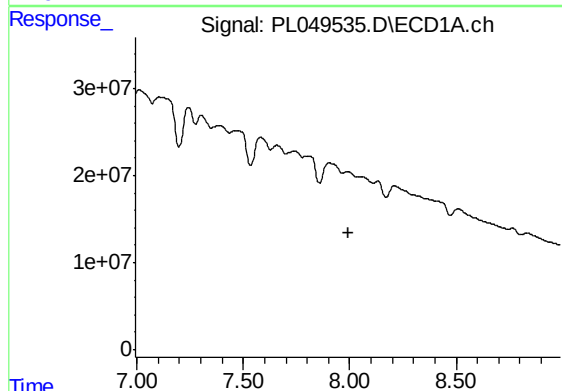

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

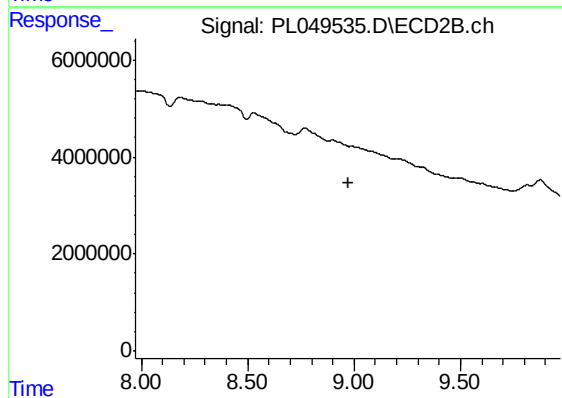

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.972 min
Response: 0
Conc: N.D.