

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
 Data File : PL049545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 11:14
 Operator : SM\AJ
 Sample : K3154-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-02-061419-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:10:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	83555071	24599709	7.583	8.515
28)	SA Decachlor...	7.990	8.970	82672826	29144795	6.502	8.727 #
Target Compounds							
4)	MA Heptachlor	0.000	5.109	0	2665256	N.D.	0.663 #
6)	B beta-BHC	0.000	4.803f	0	2114520	N.D.	1.228 #
7)	B delta-BHC	0.000	4.971f	0	1912789	N.D.	0.624 #
10)	B gamma-Chl...	5.229f	0.000	5843635	0	0.366	N.D. #
11)	B alpha-Chl...	0.000	6.106	0	4284524	N.D.	1.235 #
12)	B 4,4'-DDE	5.433	6.264	11364582	4129793	0.727	1.258 #
16)	A 4,4'-DDD	0.000	6.758	0	3527976	N.D.	1.341 #
17)	MA 4,4'-DDT	6.175	7.052	10209539	1820362	0.829	0.649
20)	A Methoxychlor	6.702f	0.000	8271817	0	1.290	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
Data File : PL049545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 11:14
Operator : SM\AJ
Sample : K3154-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:10:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

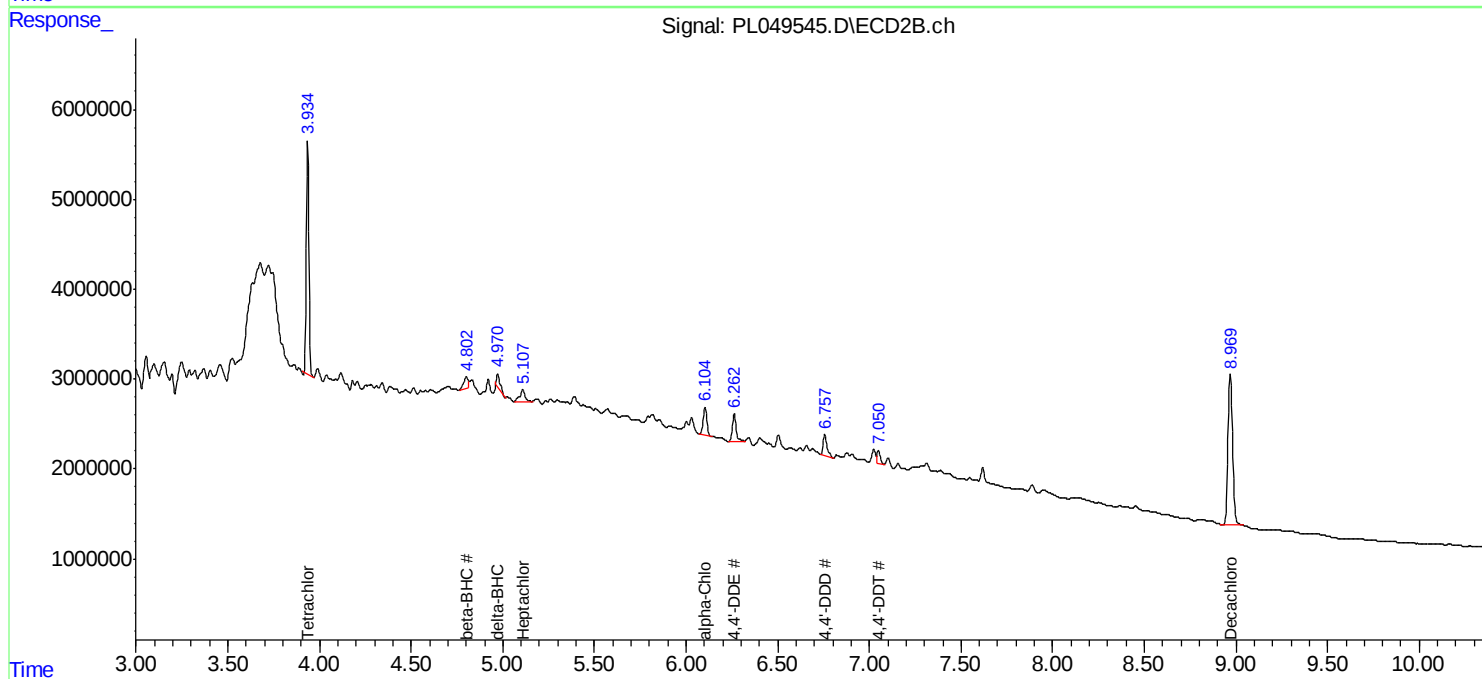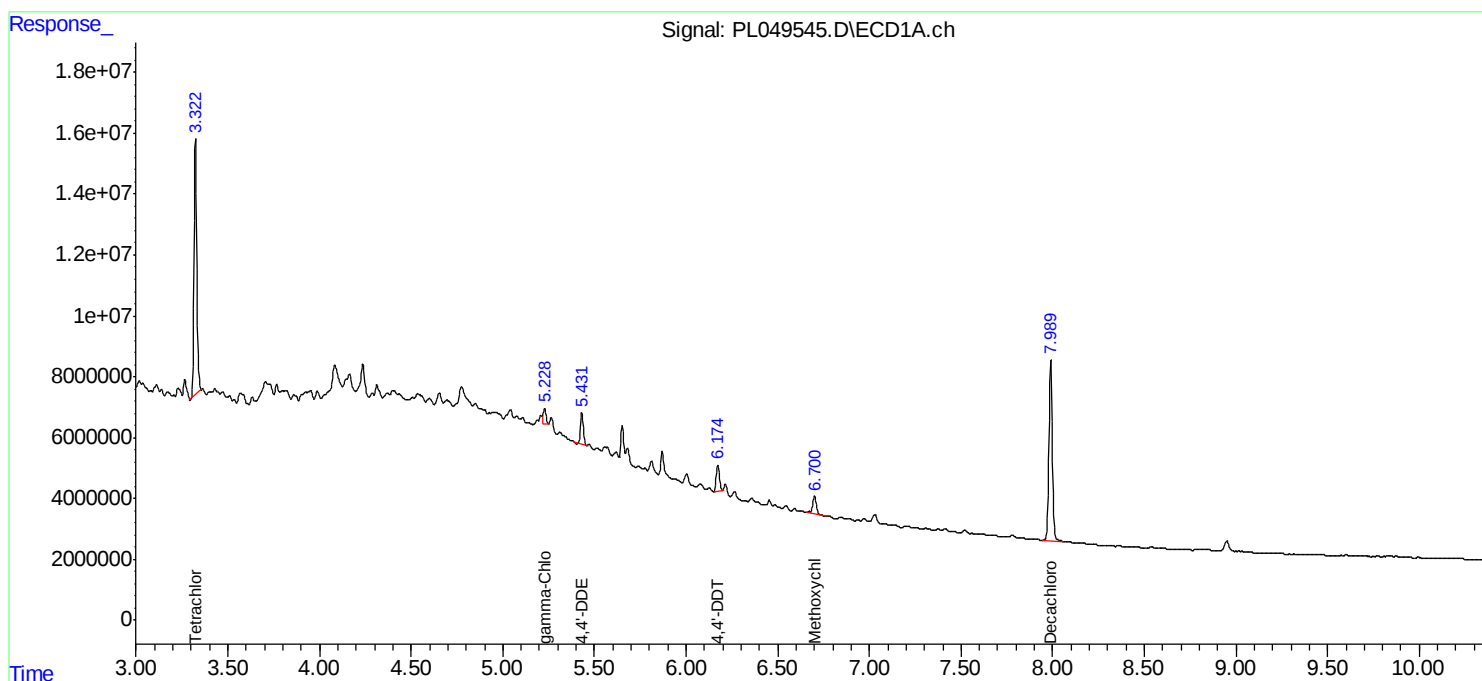


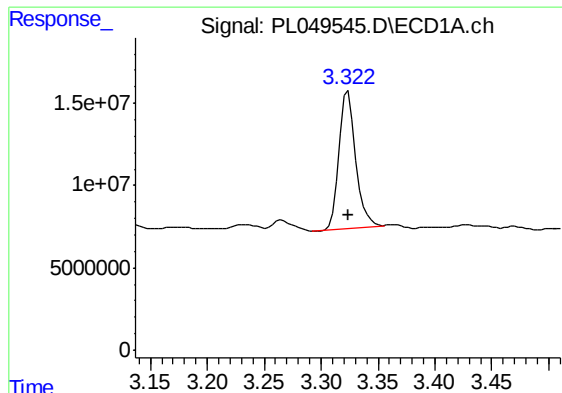

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 83555071
Conc: 7.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

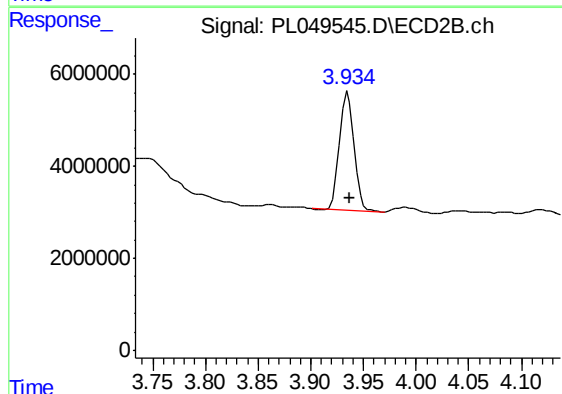


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 24599709
Conc: 8.51 ng/ml

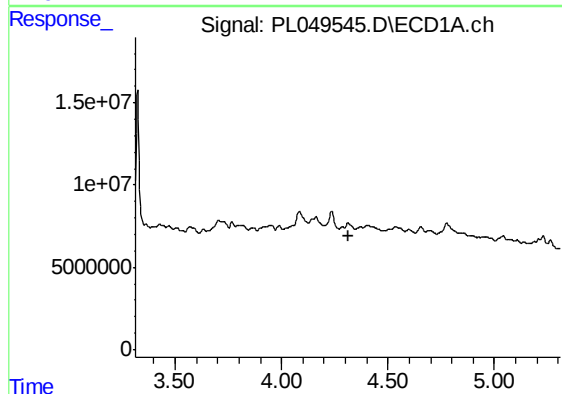


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.312 min
Response: 0
Conc: N.D.

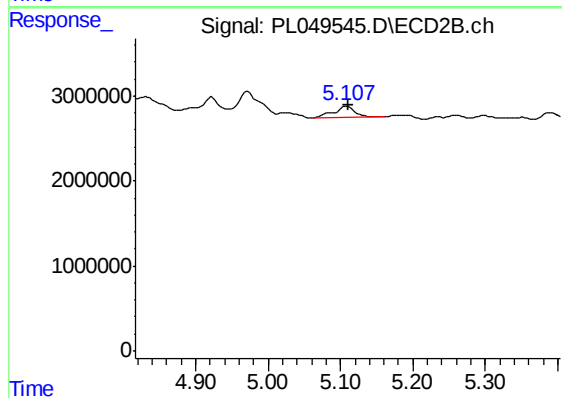

#4 Heptachlor


R.T.: 5.109 min
Delta R.T.: -0.003 min
Response: 2665256
Conc: 0.66 ng/ml

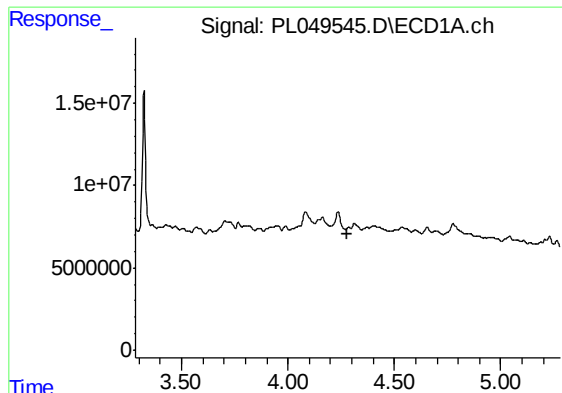

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

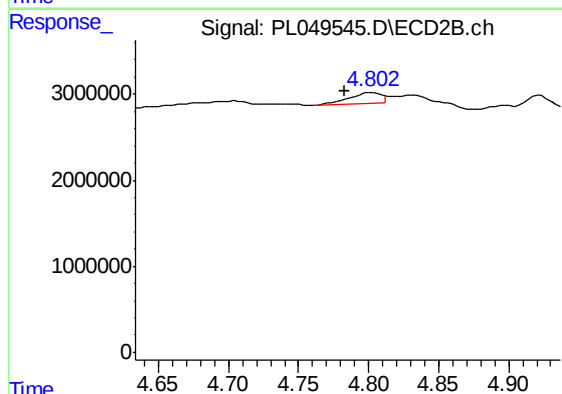


#6 beta-BHC

R.T.: 4.803 min
Delta R.T.: 0.020 min
Response: 2114520
Conc: 1.23 ng/ml

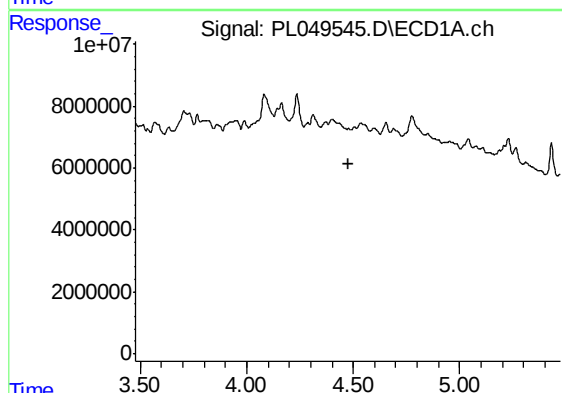


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.475 min
Response: 0
Conc: N.D.

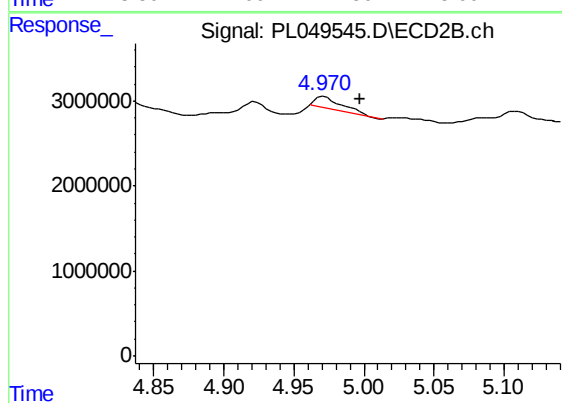

#7 delta-BHC


R.T.: 4.971 min
Delta R.T.: -0.026 min
Response: 1912789
Conc: 0.62 ng/ml

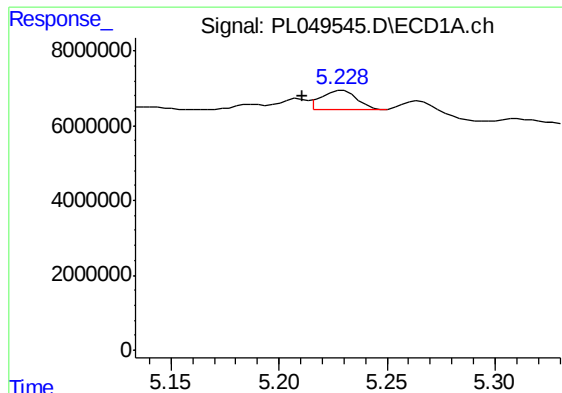

#10 gamma-Chlordane


R.T.: 5.229 min
Delta R.T.: 0.019 min
Response: 5843635
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

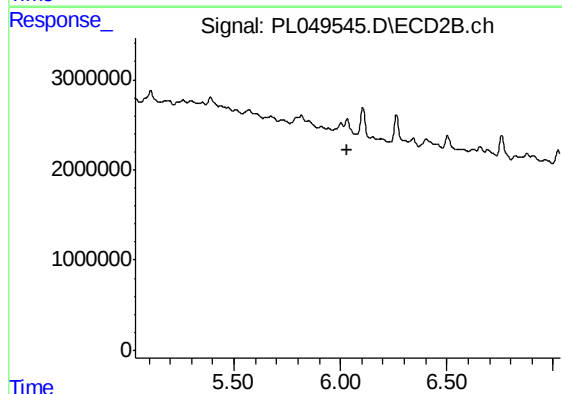


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

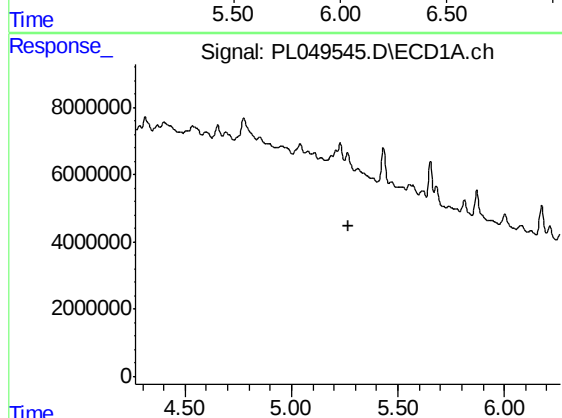


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

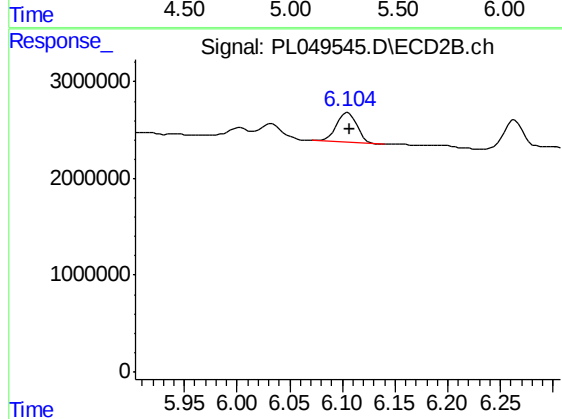

#11 alpha-Chlordane


R.T.: 6.106 min
Delta R.T.: -0.001 min
Response: 4284524
Conc: 1.24 ng/ml

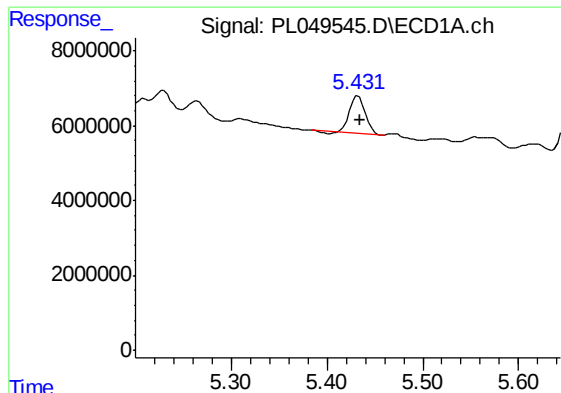

#12 4,4'-DDE


R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 11364582
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

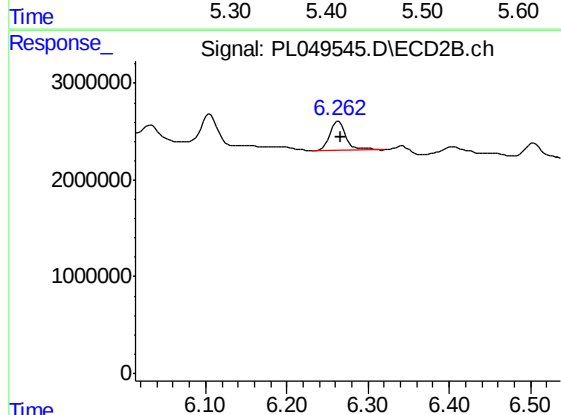


#12 4,4'-DDE

R.T.: 6.264 min
Delta R.T.: -0.003 min
Response: 4129793
Conc: 1.26 ng/ml

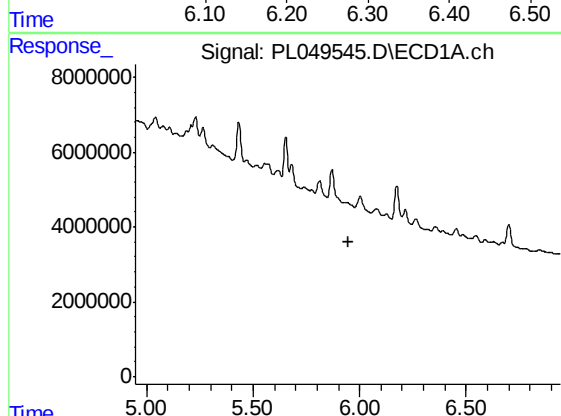


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.945 min
Response: 0
Conc: N.D.

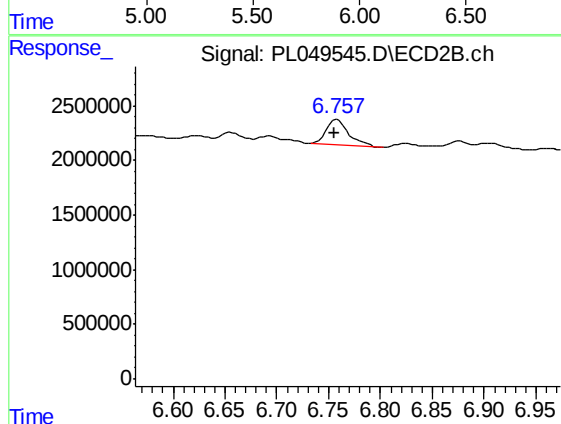

#16 4,4'-DDD


R.T.: 6.758 min
Delta R.T.: 0.002 min
Response: 3527976
Conc: 1.34 ng/ml

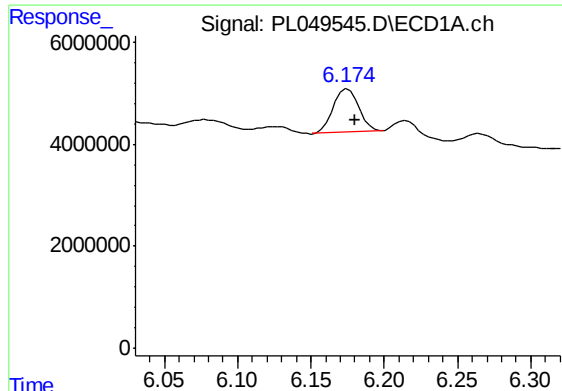

#17 4,4'-DDT


R.T.: 6.175 min
Delta R.T.: -0.005 min
Response: 10209539
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

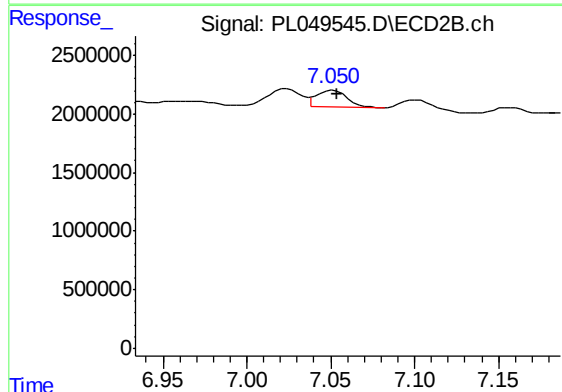


#17 4,4'-DDT

R.T.: 7.052 min
Delta R.T.: -0.002 min
Response: 1820362
Conc: 0.65 ng/ml

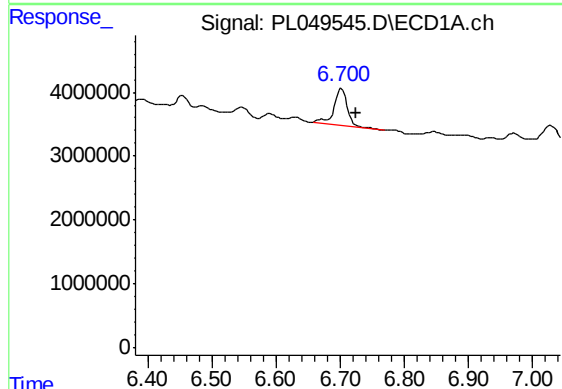


#20 Methoxychlor

R.T.: 6.702 min
Delta R.T.: -0.023 min
Response: 8271817
Conc: 1.29 ng/ml

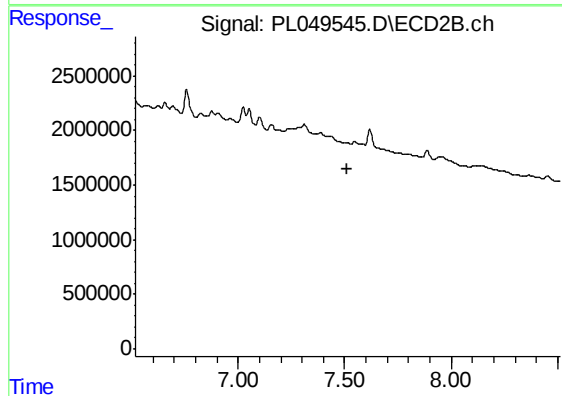

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

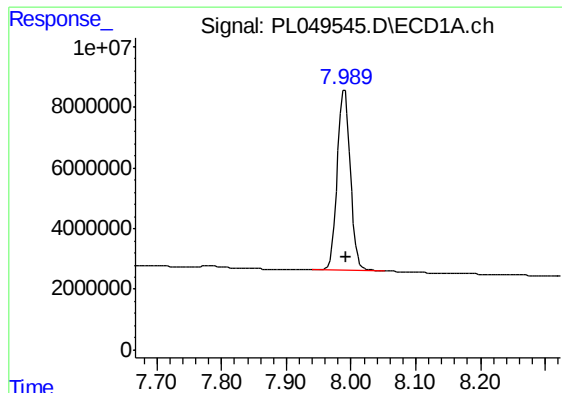

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.003 min
Response: 82672826
Conc: 6.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-061419-E

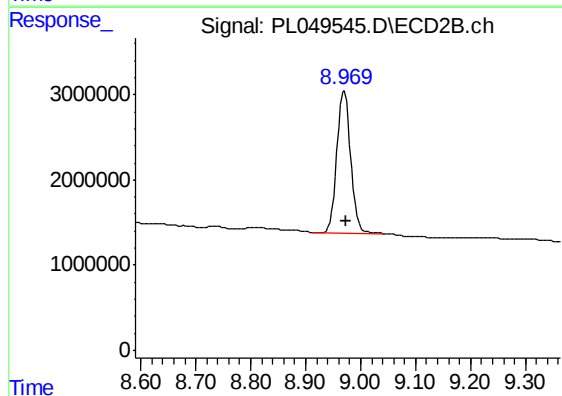

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.002 min
Response: 29144795
Conc: 8.73 ng/ml