

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
 Data File : PL049560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 15:58
 Operator : SM\AJ
 Sample : K3406-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAT-B14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:13:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	124.1E6	30594408	11.266	10.590
28)	SA Decachlor...	7.990	8.970	113.7E6	35633010	8.942	10.670
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	8659075	N.D.	5.027 #
7)	B delta-BHC	0.000	4.973f	0	1369683	N.D.	0.447 #
8)	B Heptachlo...	0.000	5.793	0	3336318	N.D.	1.021 #
10)	B gamma-Chl...	5.187f	0.000	22111030	0	1.385	N.D. #
12)	B 4,4'-DDE	5.433	6.263	16640848	3426325	1.064	1.044
13)	MA Dieldrin	5.573f	6.404	20364999	3658276	1.332	1.091
15)	B Endosulfa...	0.000	6.824f	0	1064140	N.D.	0.351 #
16)	A 4,4'-DDD	0.000	6.759	0	9372509	N.D.	3.563 #
17)	MA 4,4'-DDT	6.173	7.024f	27704735	4404453	2.250	1.571 #
18)	B Endrin al...	6.265	0.000	11033890	0	1.008	N.D. #
19)	B Endosulfa...	6.455	0.000	16357822	0	1.260	N.D. #
20)	A Methoxychlor	6.702f	0.000	44099168	0	6.876	N.D. #
21)	B Endrin ke...	6.971f	0.000	7010270	0	0.493	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
Data File : PL049560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 15:58
Operator : SM\AJ
Sample : K3406-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
BAT-B14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:13:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

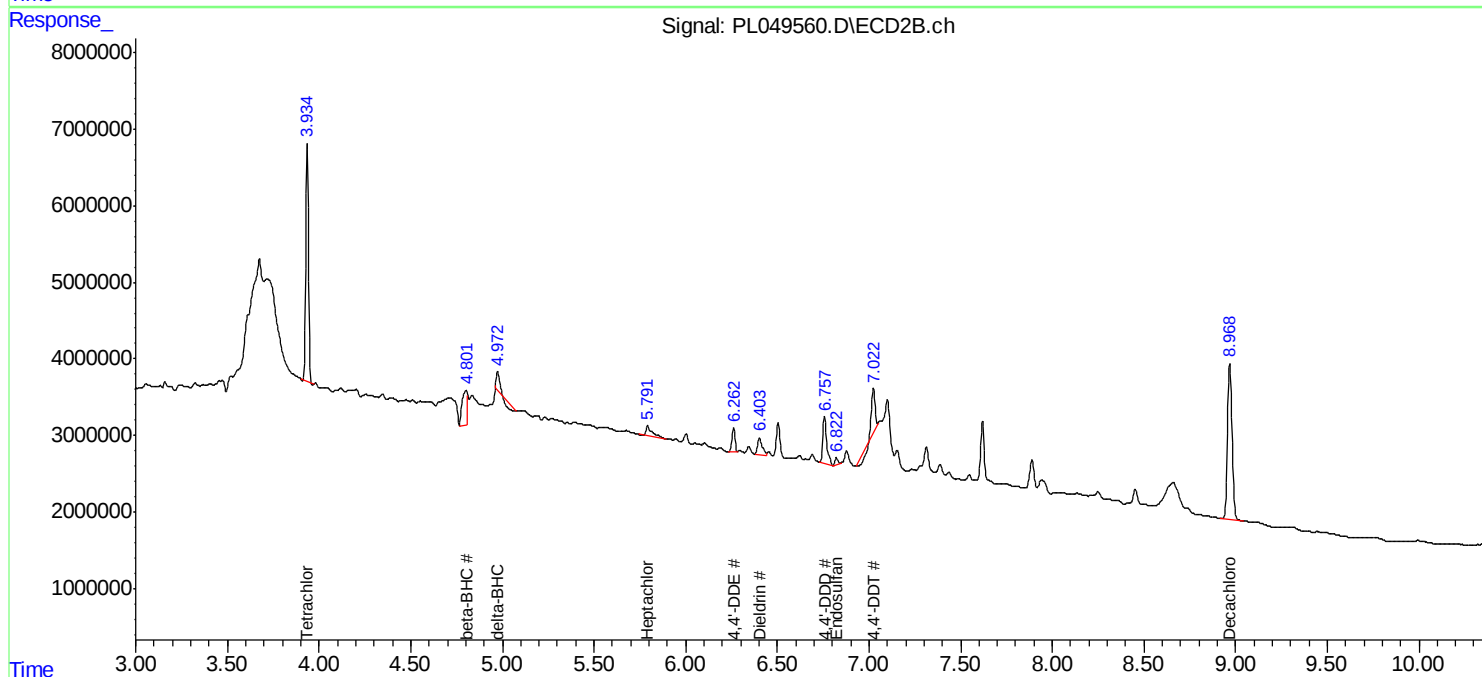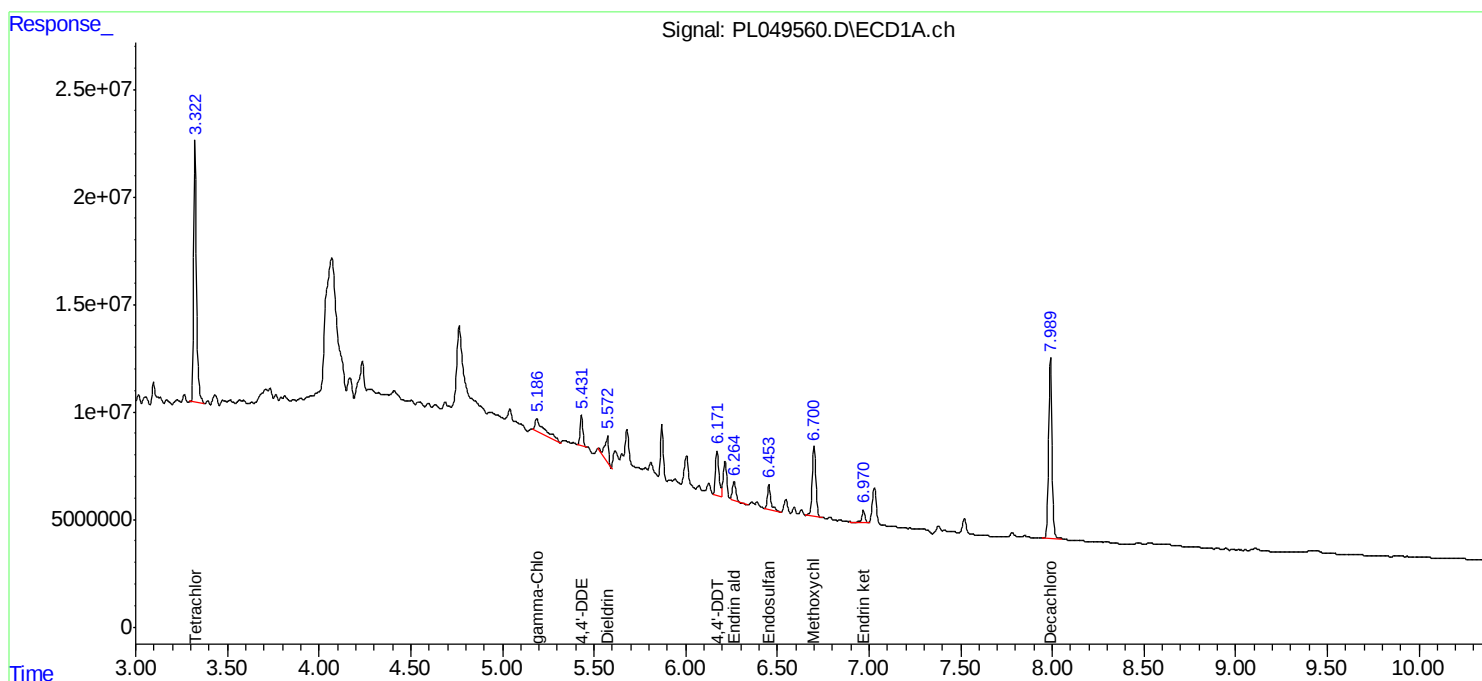


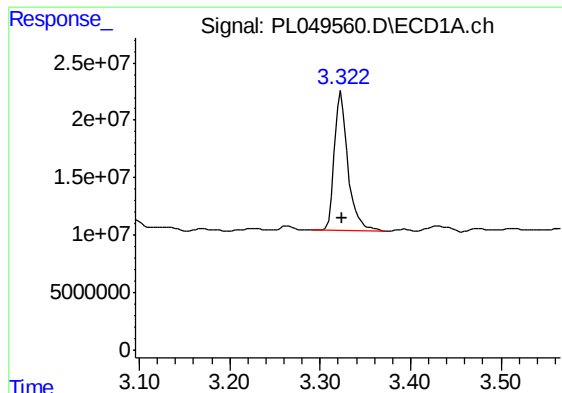

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 124142043
Conc: 11.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

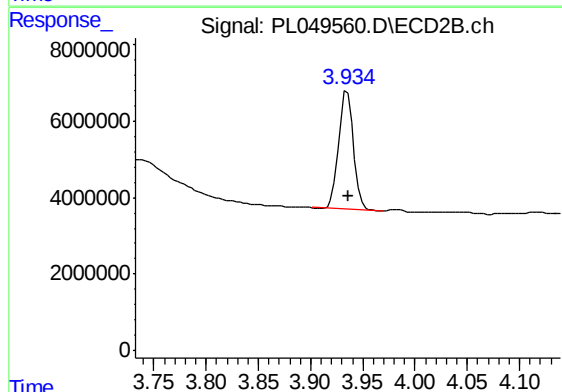


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 30594408
Conc: 10.59 ng/ml

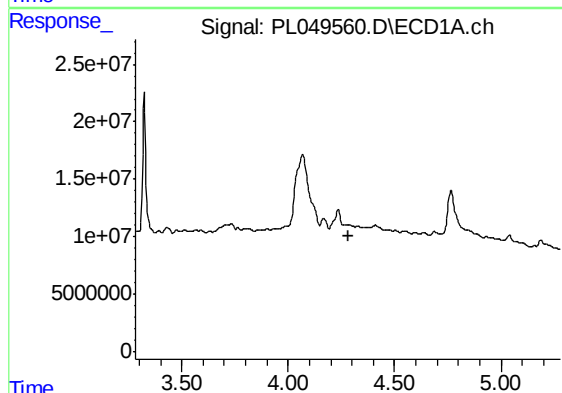


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

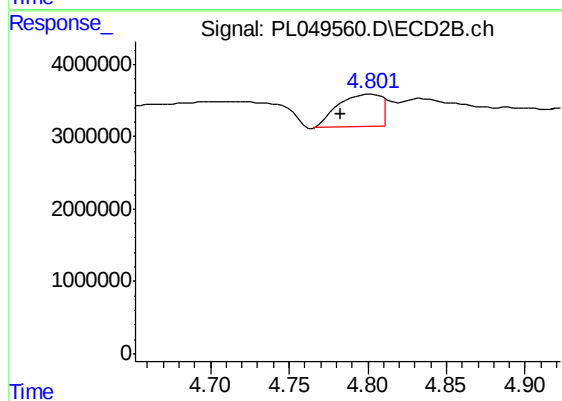

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.020 min
Response: 8659075
Conc: 5.03 ng/ml

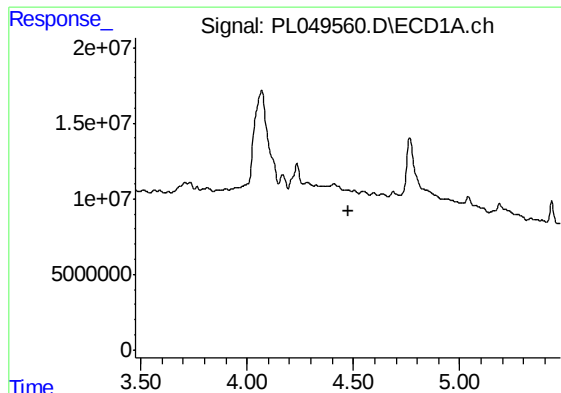

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BAT-B14

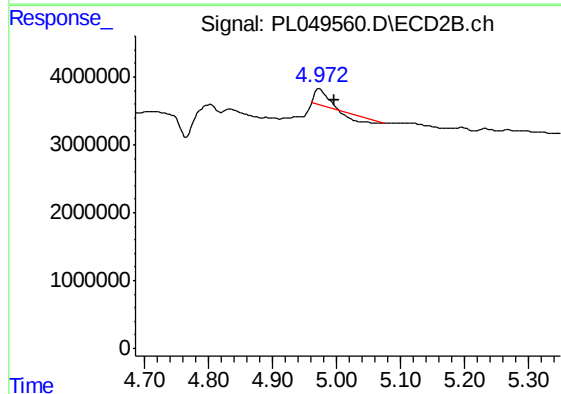


#7 delta-BHC

R.T.: 4.973 min
Delta R.T.: -0.024 min
Response: 1369683
Conc: 0.45 ng/ml

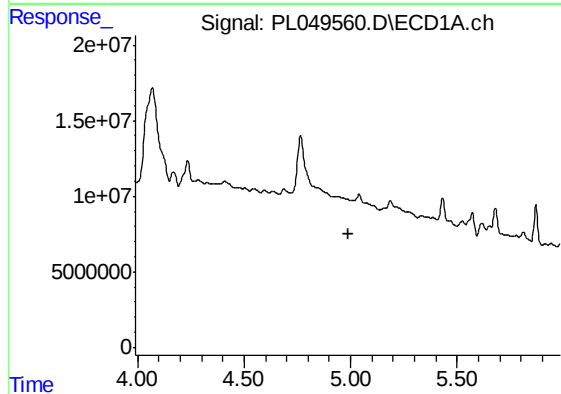


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

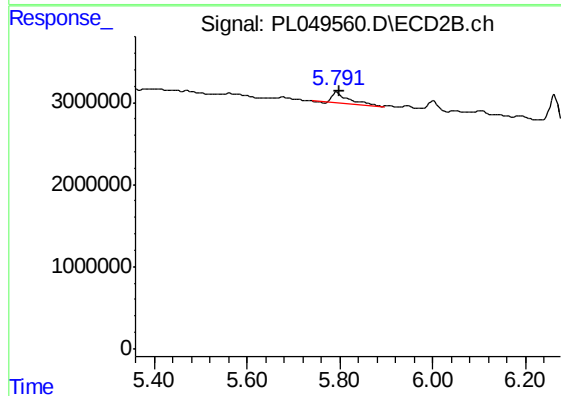

#8 Heptachlor epoxide


R.T.: 5.793 min
Delta R.T.: -0.008 min
Response: 3336318
Conc: 1.02 ng/ml

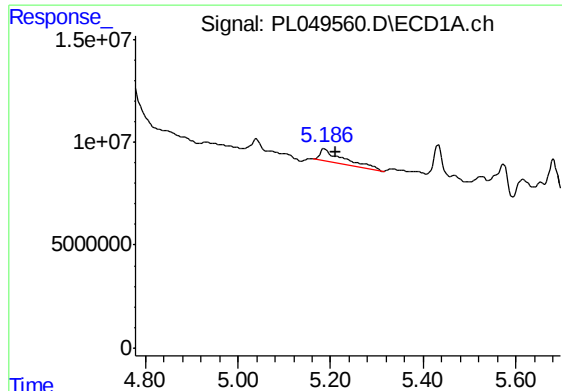

#10 gamma-Chlordane


R.T.: 5.187 min
Delta R.T.: -0.024 min
Response: 22111030
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

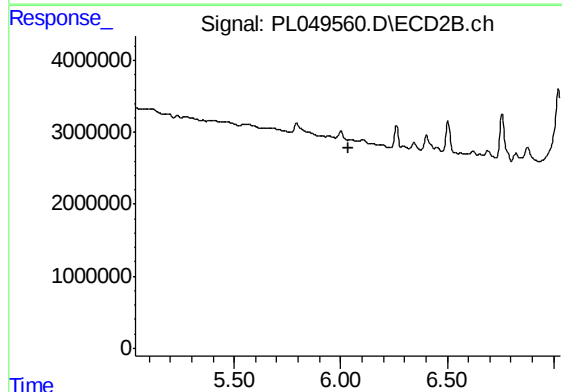


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

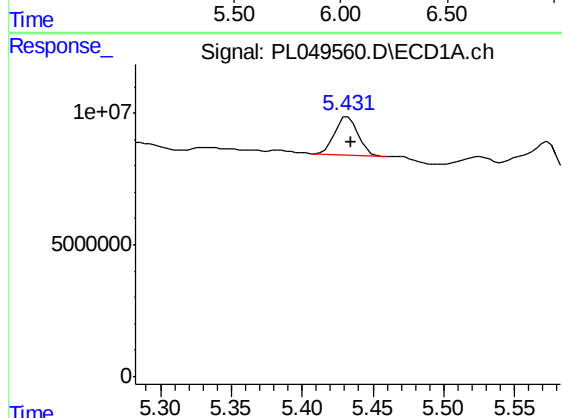


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 16640848
Conc: 1.06 ng/ml

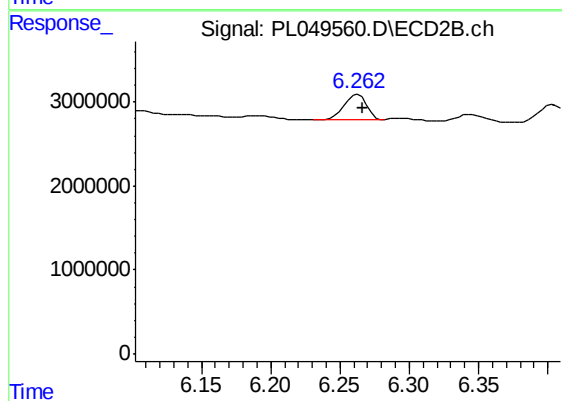

#12 4,4'-DDE


R.T.: 6.263 min
Delta R.T.: -0.004 min
Response: 3426325
Conc: 1.04 ng/ml

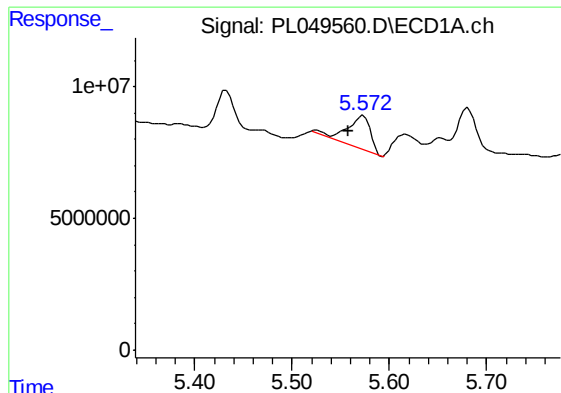

#13 Diieldrin


R.T.: 5.573 min
Delta R.T.: 0.015 min
Response: 20364999
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

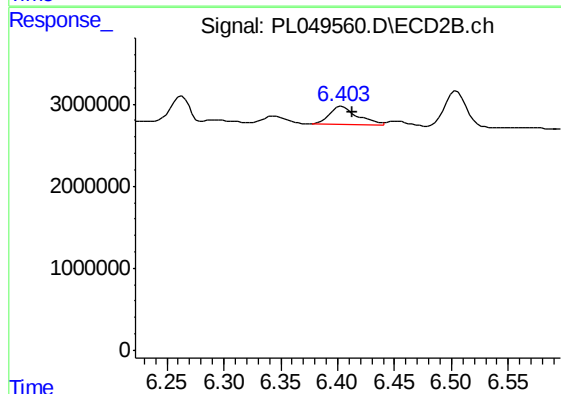


#13 Diieldrin

R.T.: 6.404 min
Delta R.T.: -0.009 min
Response: 3658276
Conc: 1.09 ng/ml

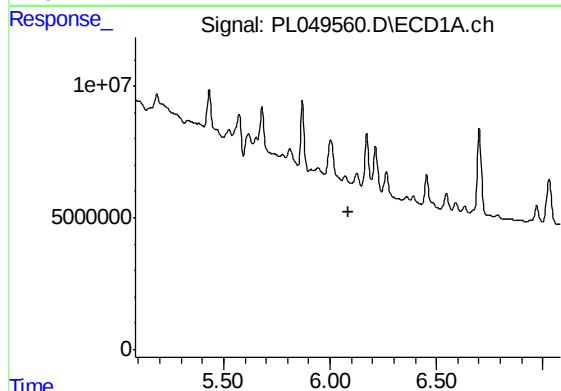


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.085 min
Response: 0
Conc: N.D.

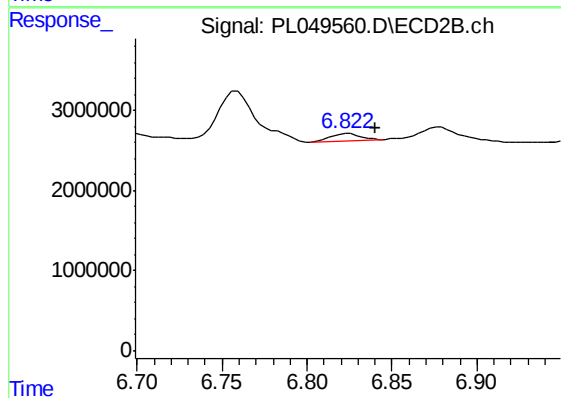

#15 Endosulfan II


R.T.: 6.824 min
Delta R.T.: -0.017 min
Response: 1064140
Conc: 0.35 ng/ml

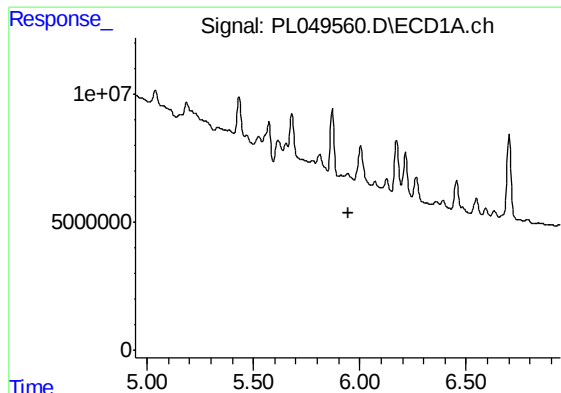

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BAT-B14

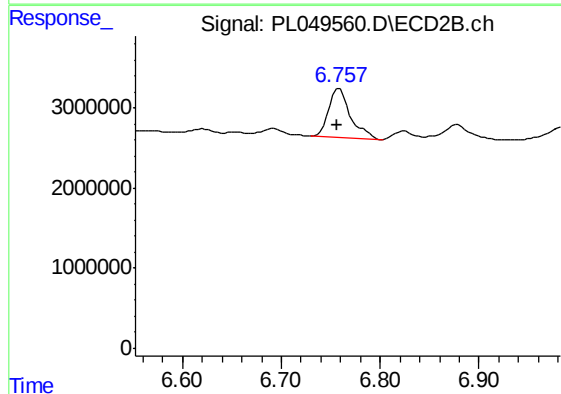


#16 4,4'-DDD

R.T.: 6.759 min
Delta R.T.: 0.003 min
Response: 9372509
Conc: 3.56 ng/ml

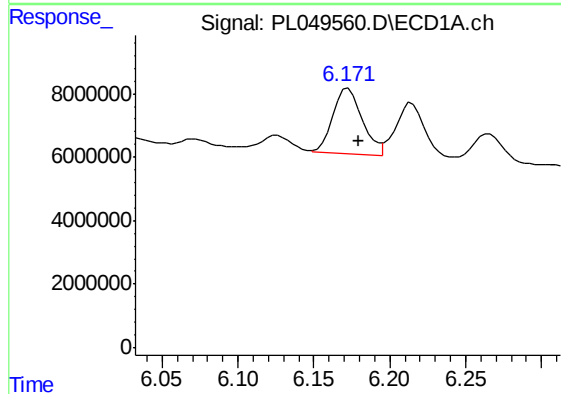


#17 4,4'-DDT

R.T.: 6.173 min
Delta R.T.: -0.007 min
Response: 27704735
Conc: 2.25 ng/ml

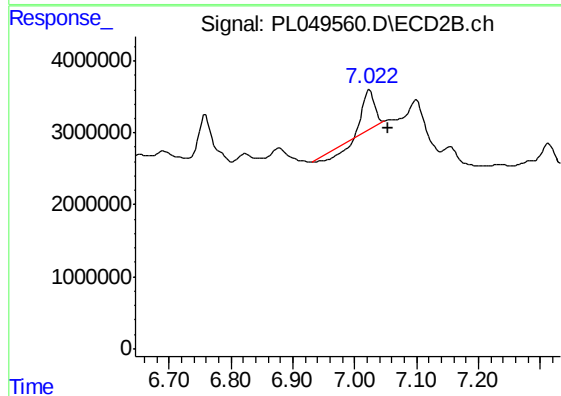

#17 4,4'-DDT


R.T.: 7.024 min
Delta R.T.: -0.030 min
Response: 4404453
Conc: 1.57 ng/ml

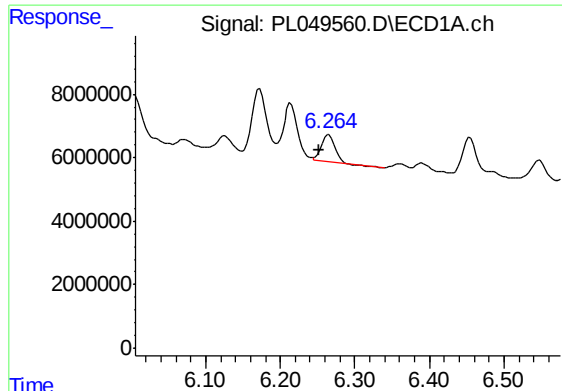

#18 Endrin aldehyde


R.T.: 6.265 min
Delta R.T.: 0.013 min
Response: 11033890
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

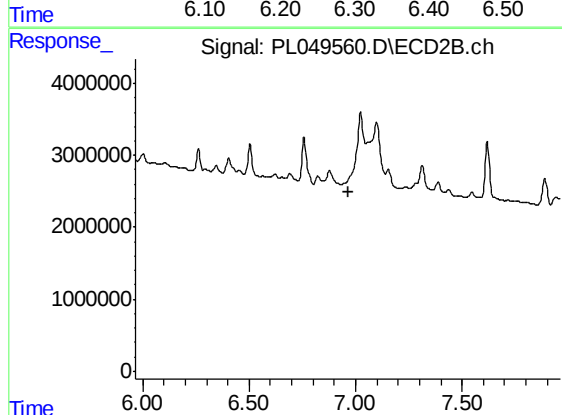


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.965 min
Response: 0
Conc: N.D.

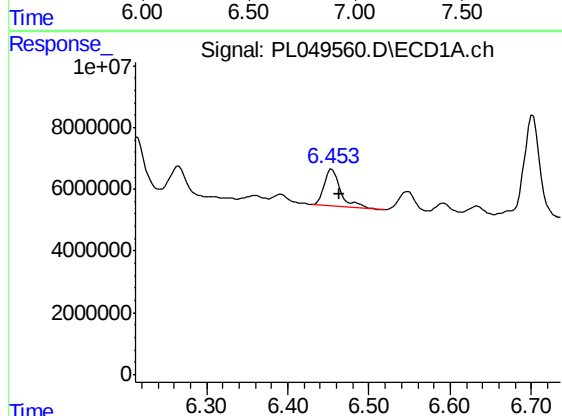


#19 Endosulfan Sulfate

R.T.: 6.455 min
Delta R.T.: -0.009 min
Response: 16357822
Conc: 1.26 ng/ml

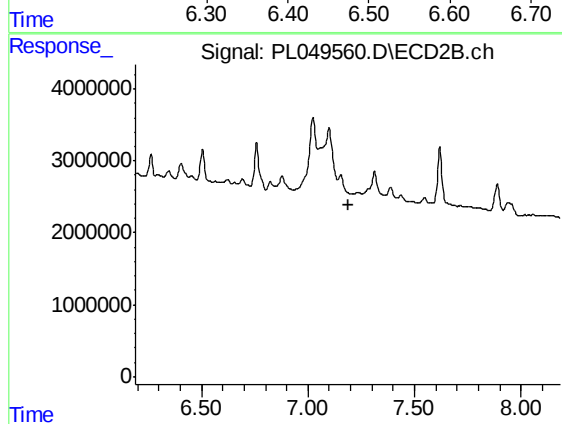

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

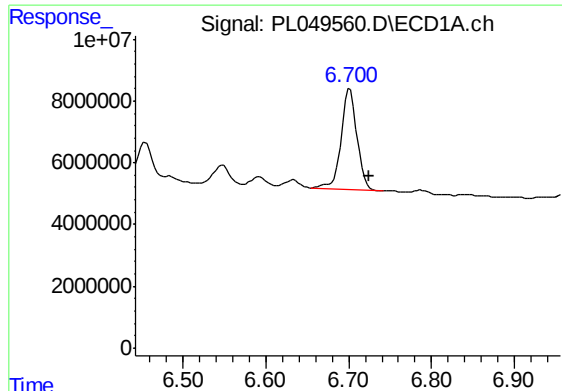

#20 Methoxychlor


R.T.: 6.702 min
Delta R.T.: -0.023 min
Response: 44099168
Conc: 6.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

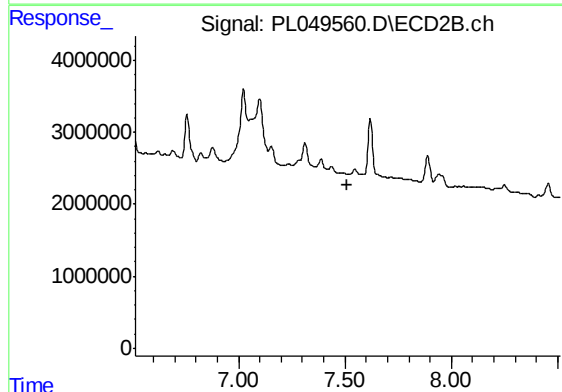


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

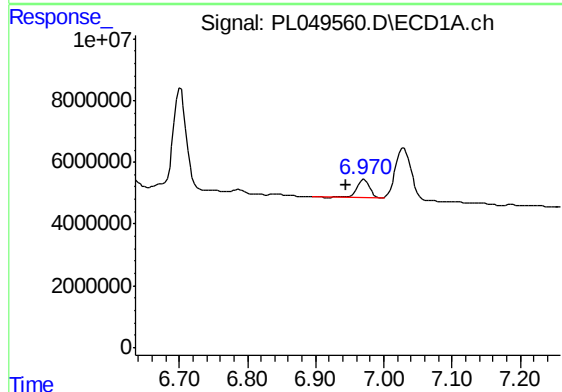


#21 Endrin ketone

R.T.: 6.971 min
Delta R.T.: 0.026 min
Response: 7010270
Conc: 0.49 ng/ml

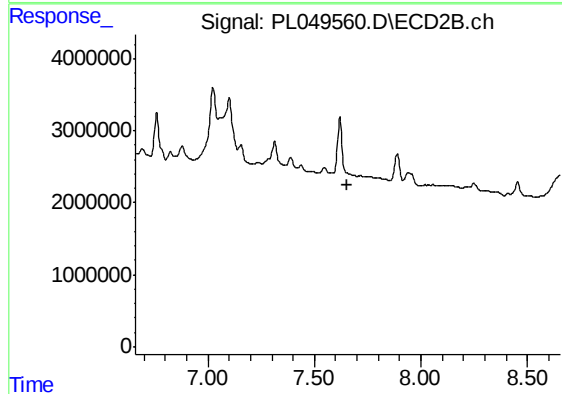

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

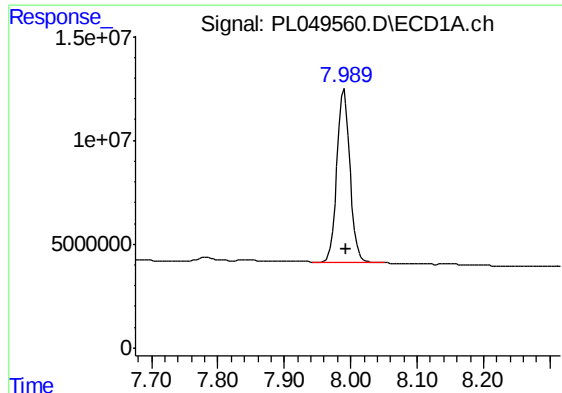

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.003 min
Response: 113703820
Conc: 8.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

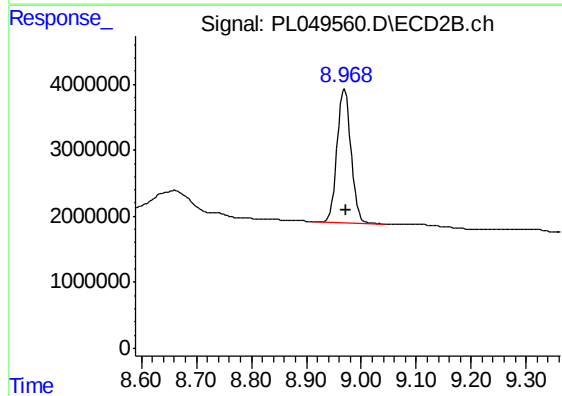

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.003 min
Response: 35633010
Conc: 10.67 ng/ml