

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
 Data File : PL049560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 15:58
 Operator : SM\AJ
 Sample : K3406-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAT-B14

Manual Integrations
 APPROVED

Ankita
 6/18/2019 11:25:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:13:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.934	124.1E6	31205135	11.266	10.801m
28)	SA Decachlor...	7.990	8.970	113.7E6	35633010	8.942	10.670
Target Compounds							
12)	B 4,4'-DDE	5.433	6.263	16640848	3426325	1.064	1.044

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061719\
Data File : PL049560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 15:58
Operator : SM\AJ
Sample : K3406-02
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BAT-B14


Manual Integrations
APPROVED

Ankita
6/18/2019 11:25:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:13:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

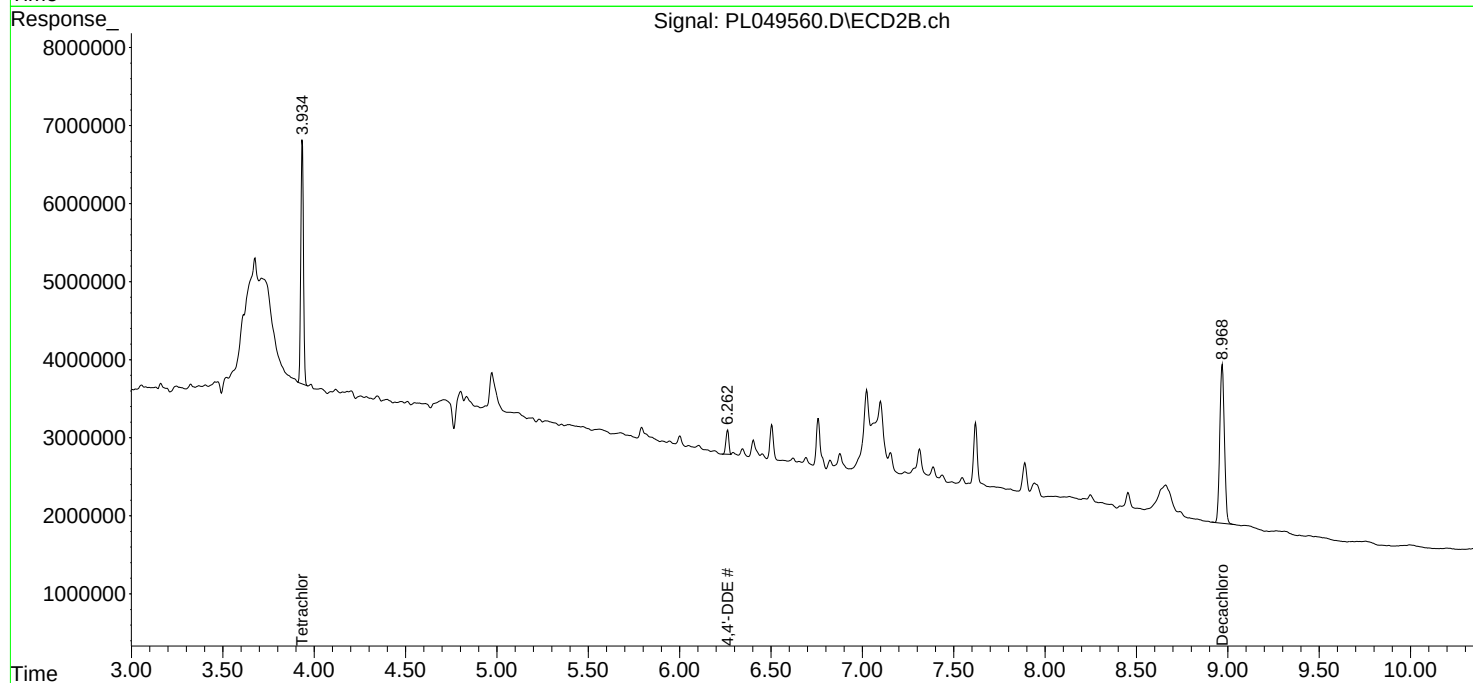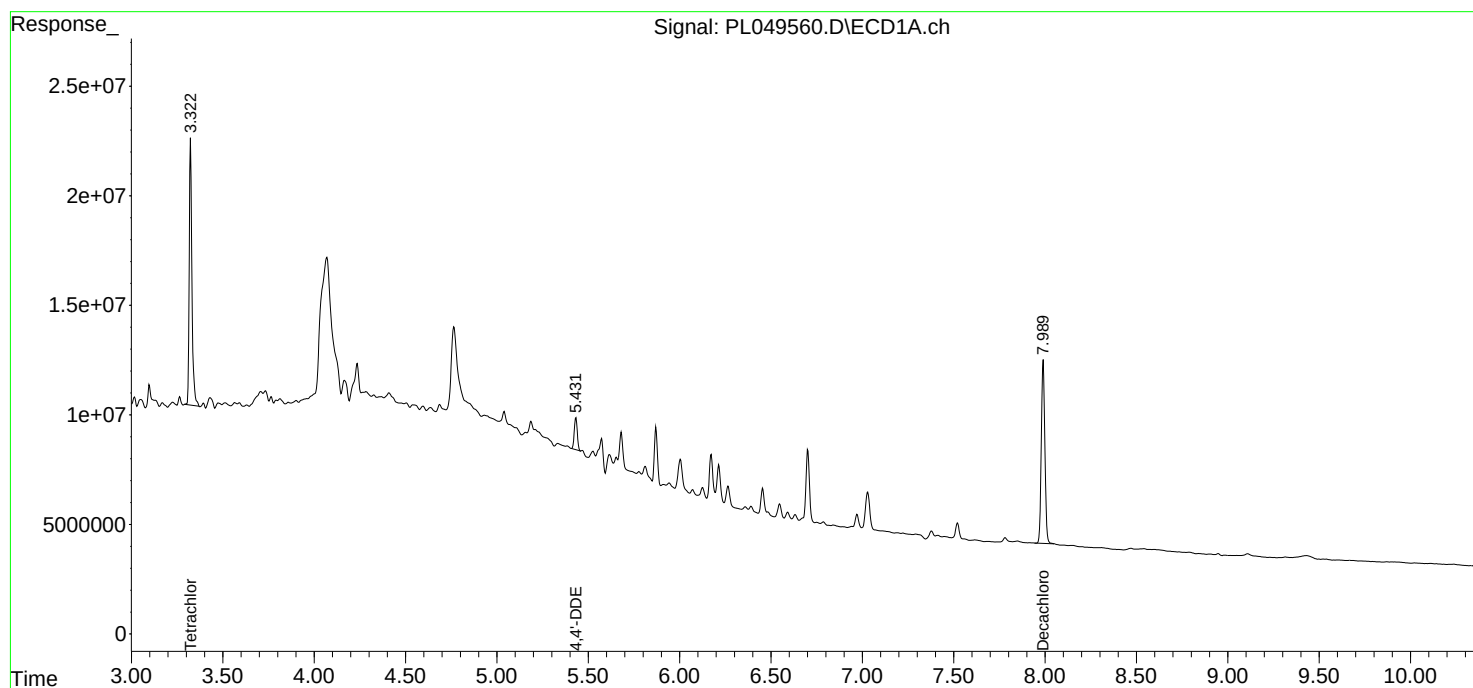

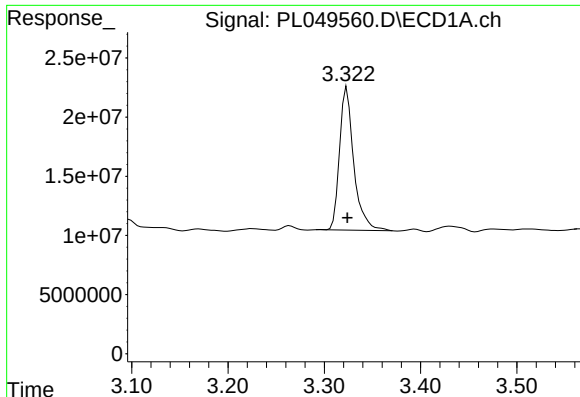


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 124142043
Conc: 11.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14


Manual Integrations
APPROVED

Ankita
6/18/2019 11:25:43 AM

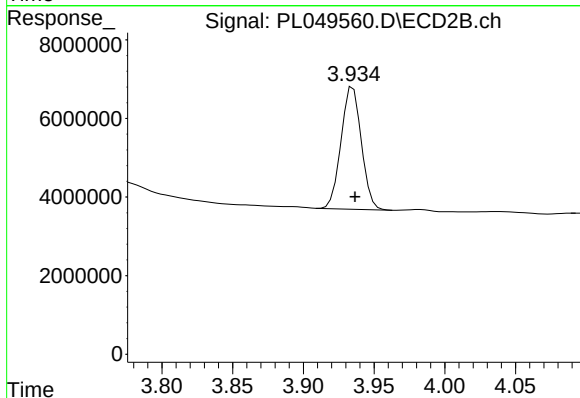


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.003 min
Response: 31205135
Conc: 10.80 ng/ml m

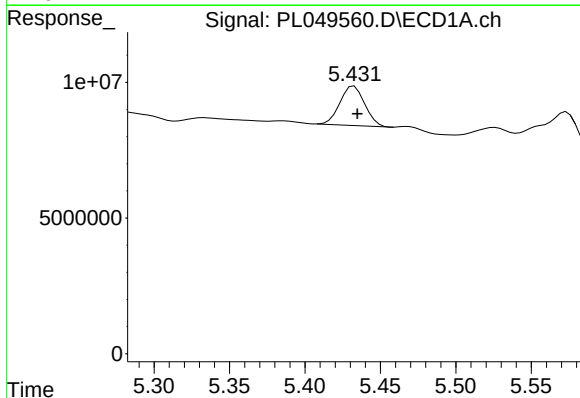


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 16640848
Conc: 1.06 ng/ml

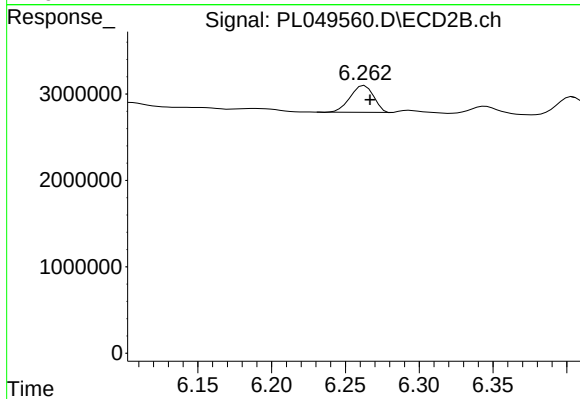

#12 4,4'-DDE

R.T.: 6.263 min
Delta R.T.: -0.004 min
Response: 3426325
Conc: 1.04 ng/ml

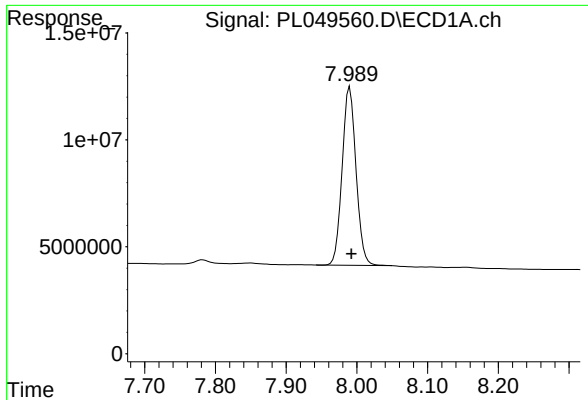

#28 Decachlorobiphenyl

R.T.: 7.990 min

Delta R.T.: -0.003 min


Response: 113703820

Conc: 8.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B14

Manual Integrations
APPROVED

Ankita
6/18/2019 11:25:43 AM

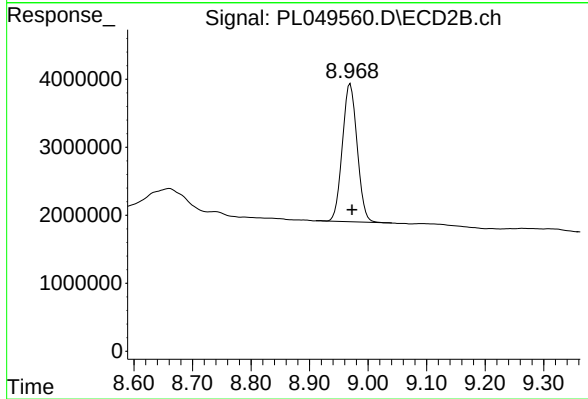

#28 Decachlorobiphenyl

R.T.: 8.970 min

Delta R.T.: -0.003 min

Response: 35633010

Conc: 10.67 ng/ml