

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 11:34
 Operator : AR\AJ
 Sample : M2678-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 15:10:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.487	5.528	10157506	17703640	18.475	18.779
28)	SA Decachlor...	10.227	11.430	14360668	21790725	20.264	21.877
Target Compounds							
4)	MA Heptachlor	5.983f	0.000	288305	0	0.382	N.D. #
6)	B beta-BHC	5.983	0.000	288305	0	0.806	N.D. #
10)	B gamma-Chl...	0.000	8.280f	0	397140	N.D.	0.393 #
11)	B alpha-Chl...	7.228f	0.000	147460	0	0.201	N.D. #
15)	B Endosulfa...	0.000	9.176f	0	561276	N.D.	0.704 #
24)	Chlordane-2	6.462f	0.000	207711	0	7.757	N.D. #
25)	Chlordane-3	0.000	8.280f	0	397140	N.D.	2.967 #
26)	Chlordane-4	7.228f	0.000	147460	0	2.018	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 11:34
Operator : AR\AJ
Sample : M2678-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 15:10:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

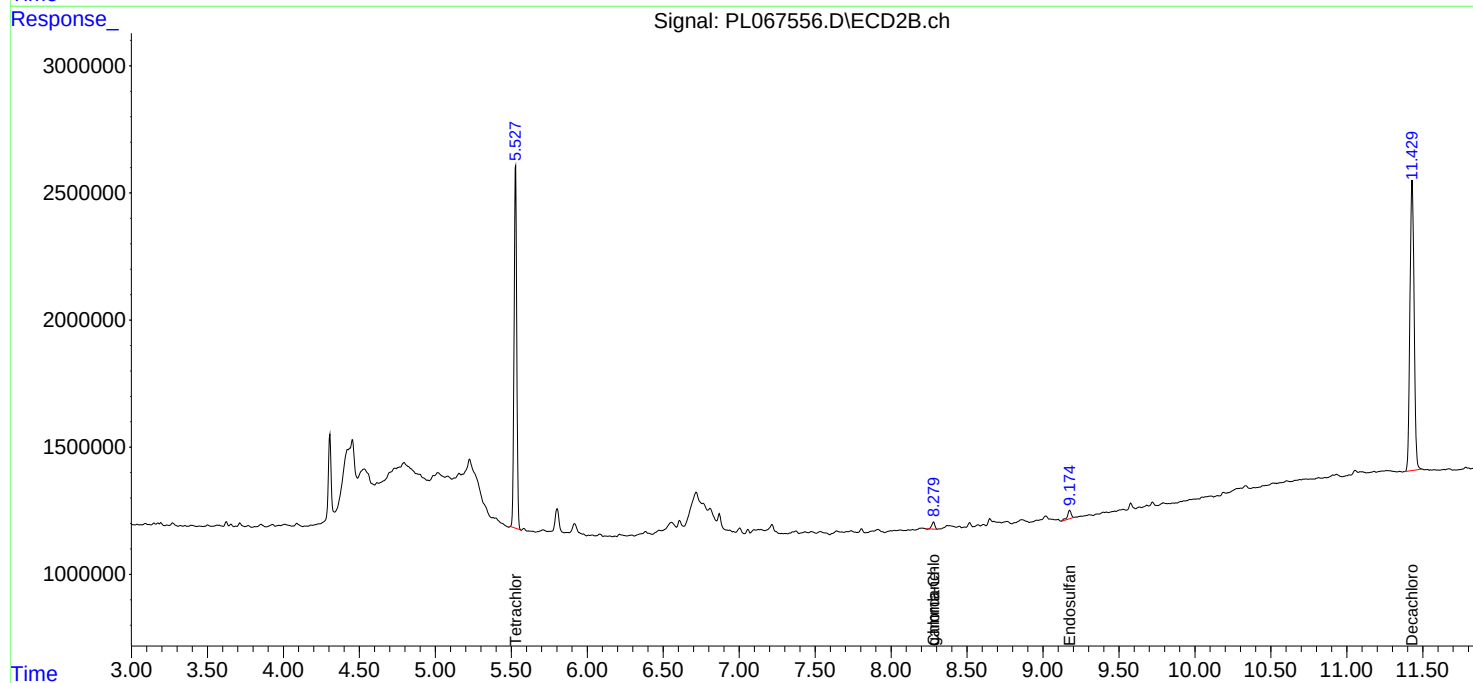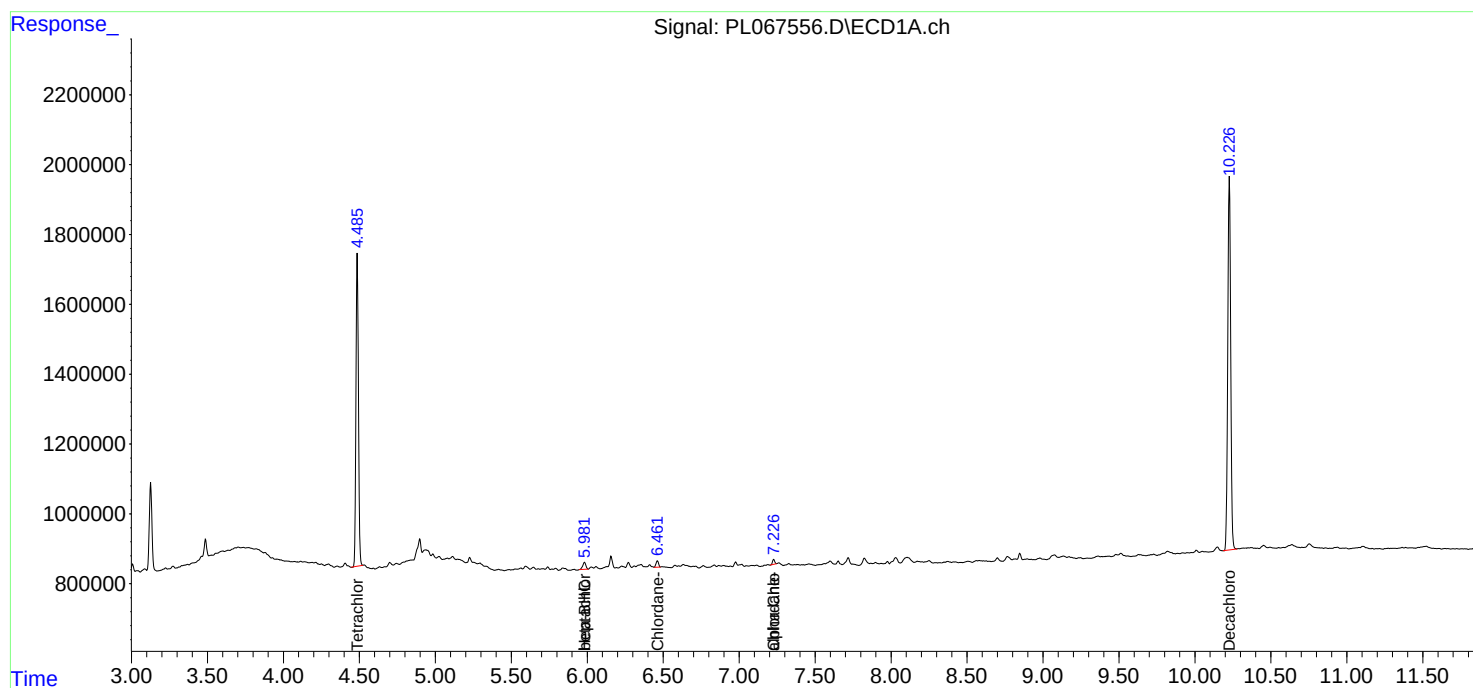


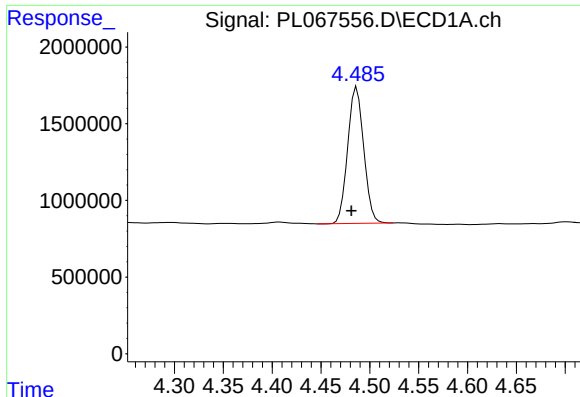

#1 Tetrachloro-m-xylene


R.T.: 4.487 min
Delta R.T.: 0.006 min
Response: 10157506
Conc: 18.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

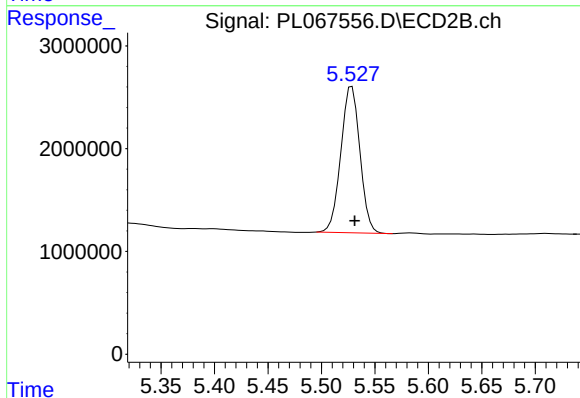


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 17703640
Conc: 18.78 ng/ml

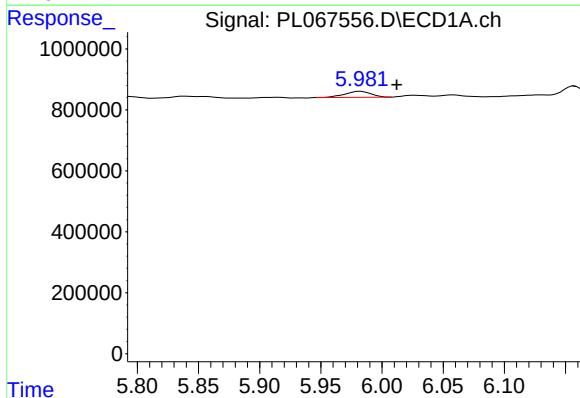


#4 Heptachlor

R.T.: 5.983 min
Delta R.T.: -0.029 min
Response: 288305
Conc: 0.38 ng/ml

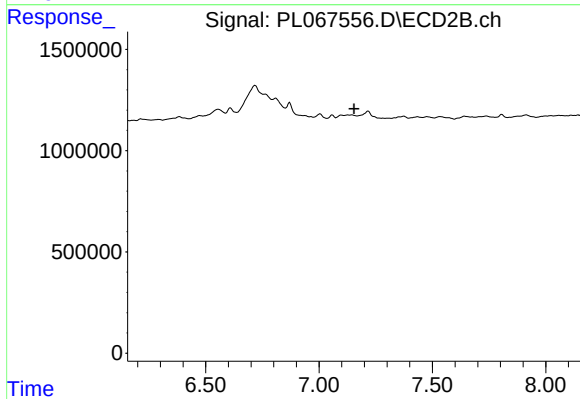

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

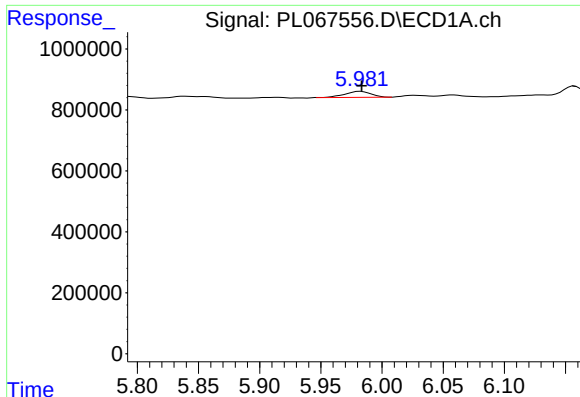

#6 beta-BHC


R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 288305
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

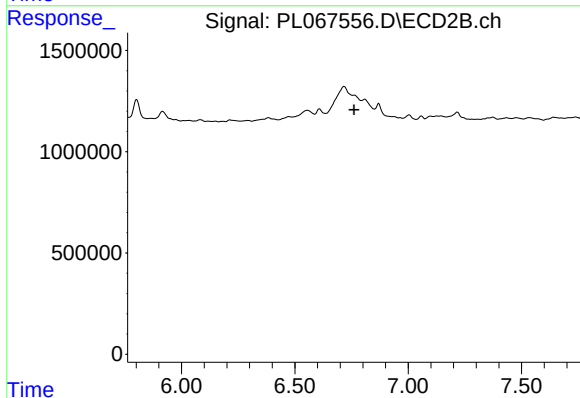


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

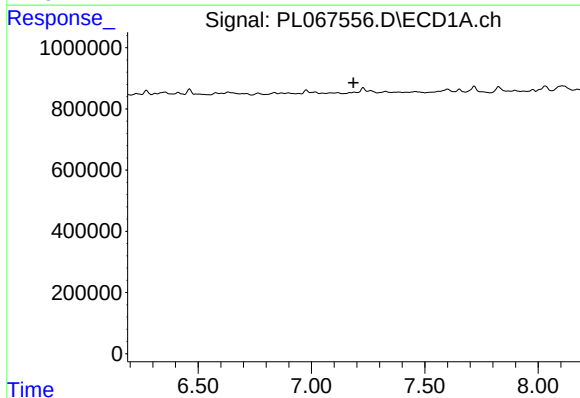


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

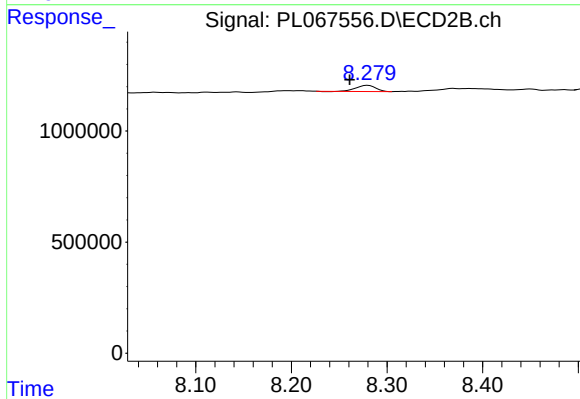

#10 gamma-Chlordane


R.T.: 8.280 min
Delta R.T.: 0.019 min
Response: 397140
Conc: 0.39 ng/ml

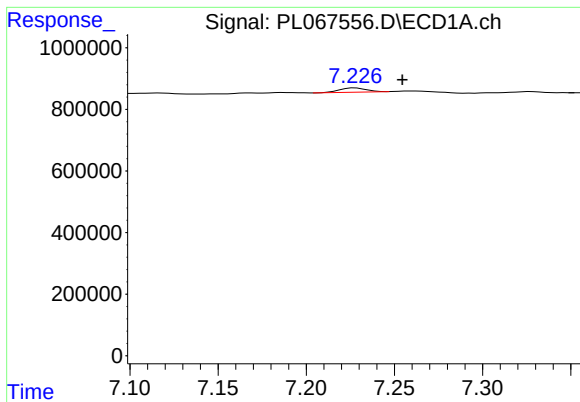

#11 alpha-Chlordane


R.T.: 7.228 min
Delta R.T.: -0.027 min
Response: 147460
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

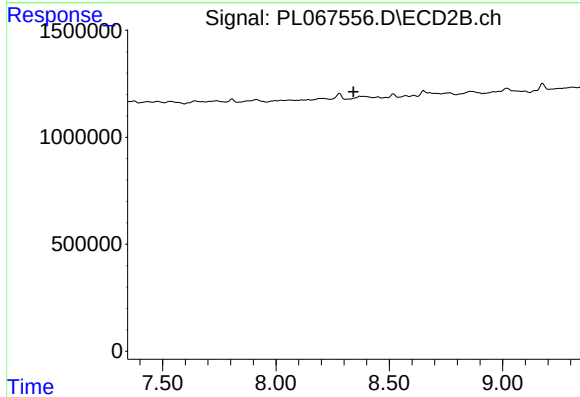

#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

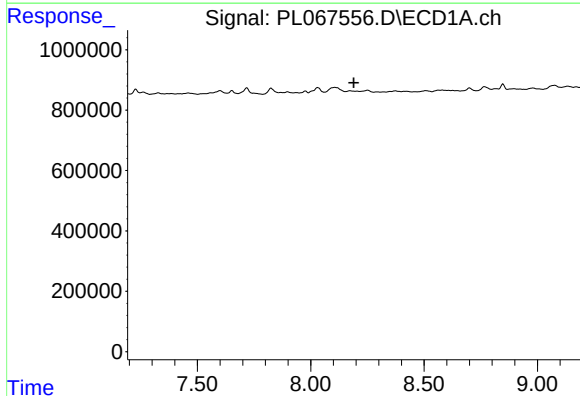


#15 Endosulfan II

```

      R.T.:      0.000 min
Exp R.T.  :      8.190 min
  Response:           0
    Conc:    N.D.

```

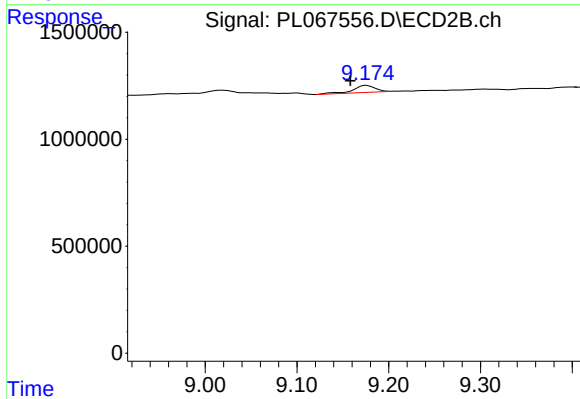


#15 Endosulfan II

```

      R.T.:    9.176 min
Delta R.T.:   0.017 min
  Response:   561276
      Conc:    0.70 ng/ml


```

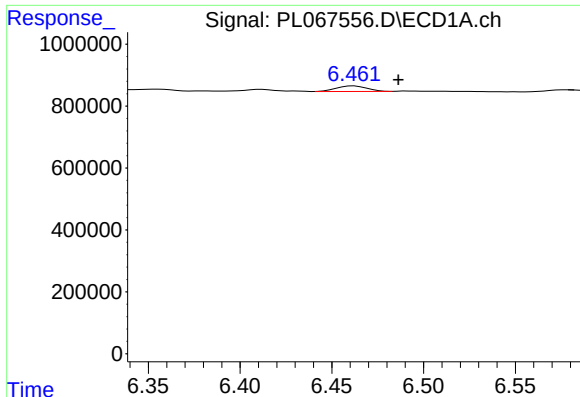

#24 Chlordane-2


R.T.: 6.462 min
Delta R.T.: -0.024 min
Response: 207711
Conc: 7.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

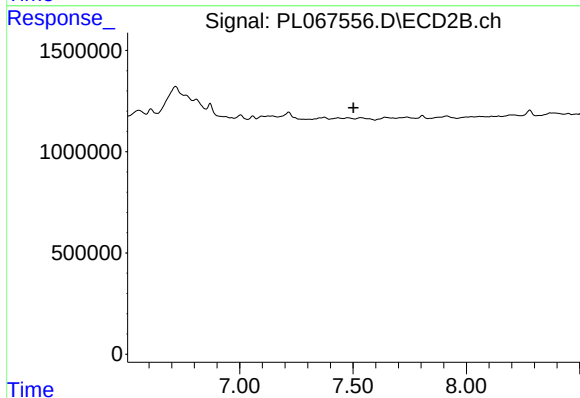


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

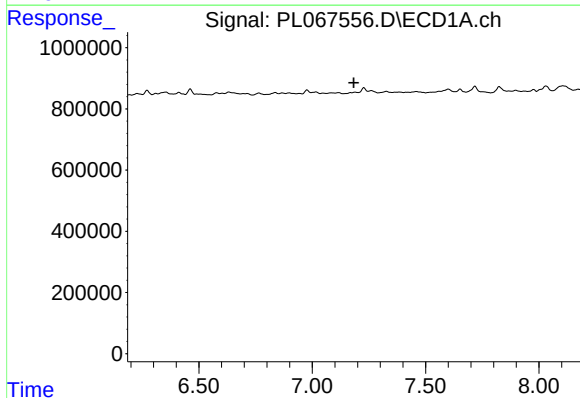


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.184 min
Response: 0
Conc: N.D.

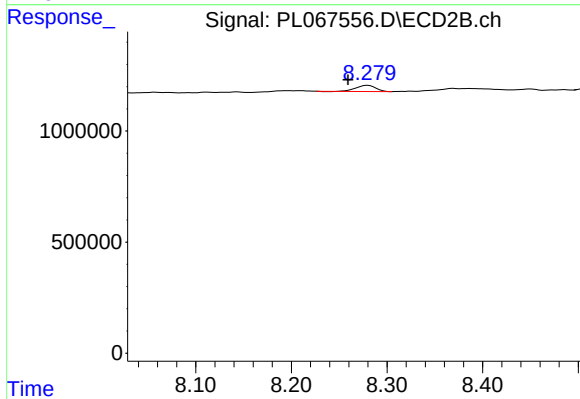

#25 Chlordane-3


R.T.: 8.280 min
Delta R.T.: 0.021 min
Response: 397140
Conc: 2.97 ng/ml

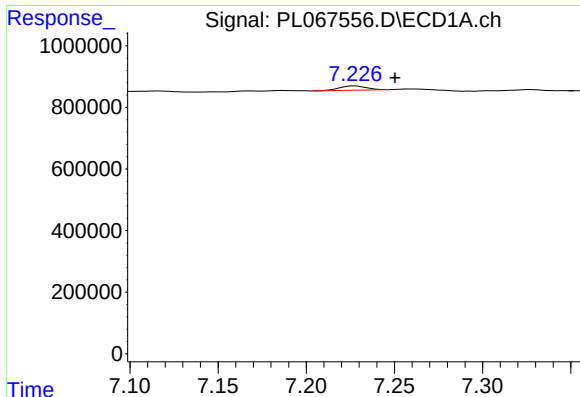

#26 Chlordane-4


R.T.: 7.228 min
Delta R.T.: -0.023 min
Response: 147460
Conc: 2.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

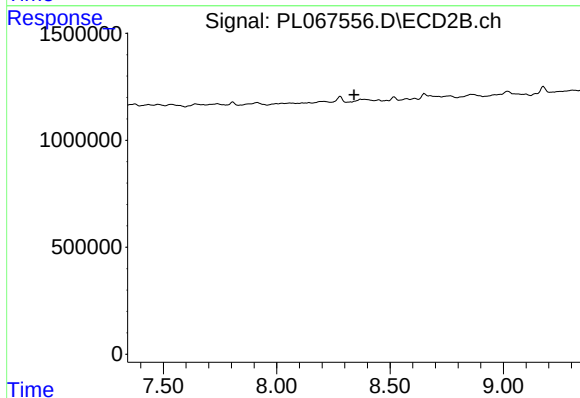


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

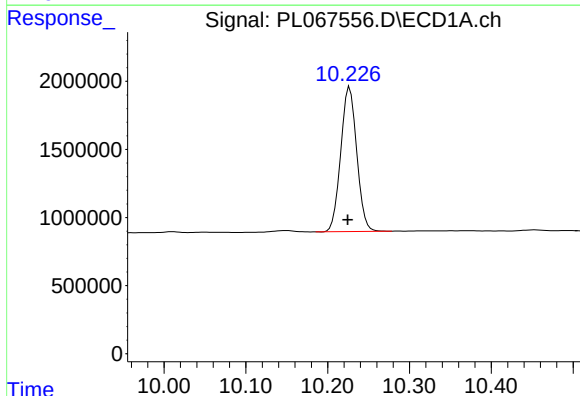

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: 0.003 min
Response: 14360668
Conc: 20.26 ng/ml

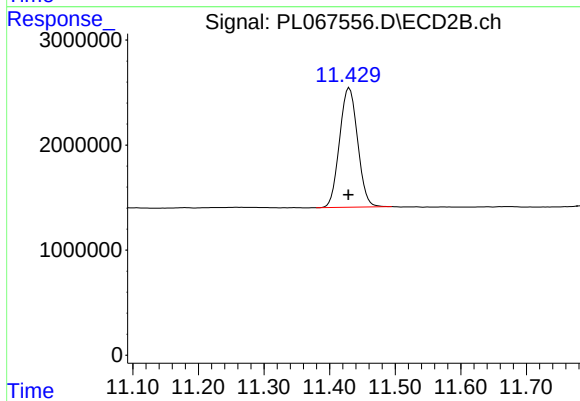

#28 Decachlorobiphenyl

R.T.: 11.430 min
Delta R.T.: 0.002 min
Response: 21790725
Conc: 21.88 ng/ml