

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 14:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 15:12:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	10092768	17853368	18.358	18.938
28)	SA Decachlor...	10.219	11.427	13542193	21248814	19.109	21.333
Target Compounds							
3)	MA gamma-BHC...	5.598	0.000	825802	0	1.102	N.D. #
4)	MA Heptachlor	5.987f	0.000	457147	0	0.606	N.D. #
6)	B beta-BHC	5.987	0.000	457147	0	1.278	N.D. #
15)	B Endosulfa...	0.000	9.180f	0	838503	N.D.	1.052 #
23)	Chlordane-1	0.000	6.940f	0	611671	N.D.	21.661 #
24)	Chlordane-2	6.486	0.000	257048	0	9.599	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 14:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 15:12:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

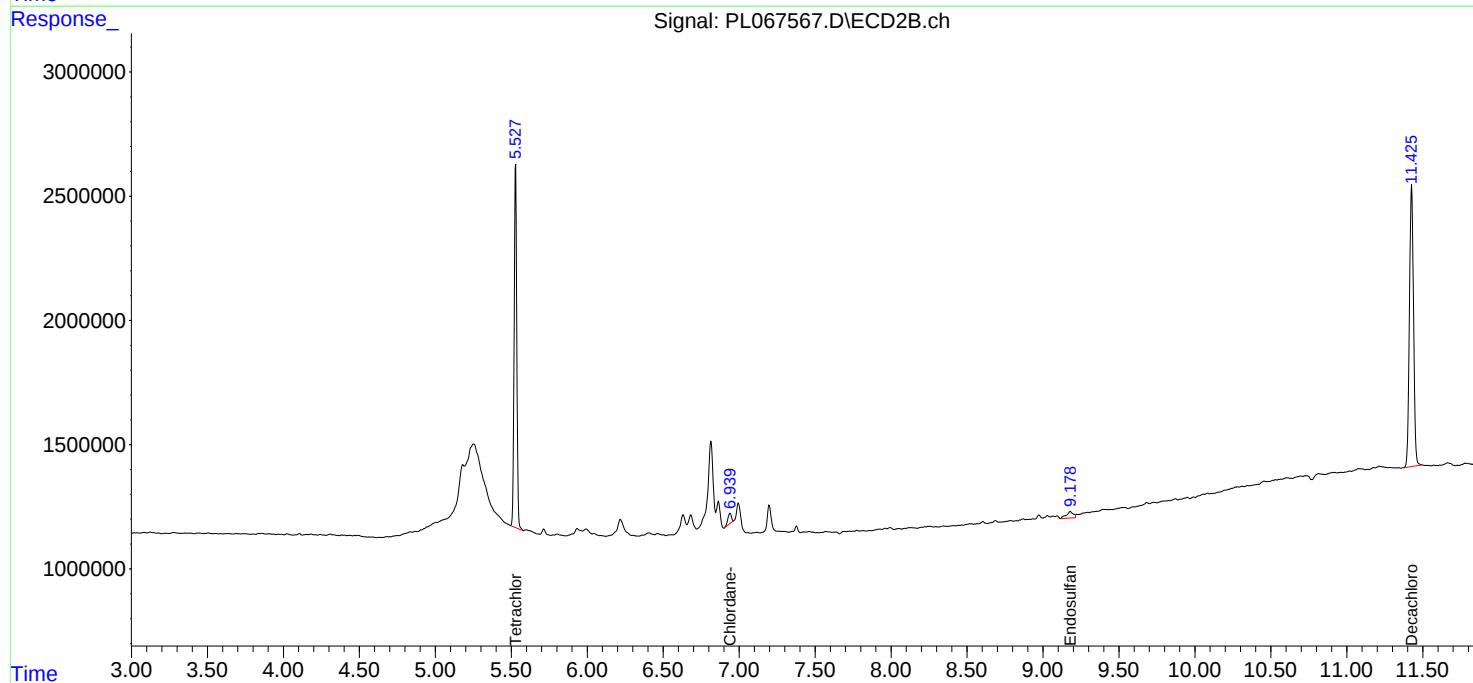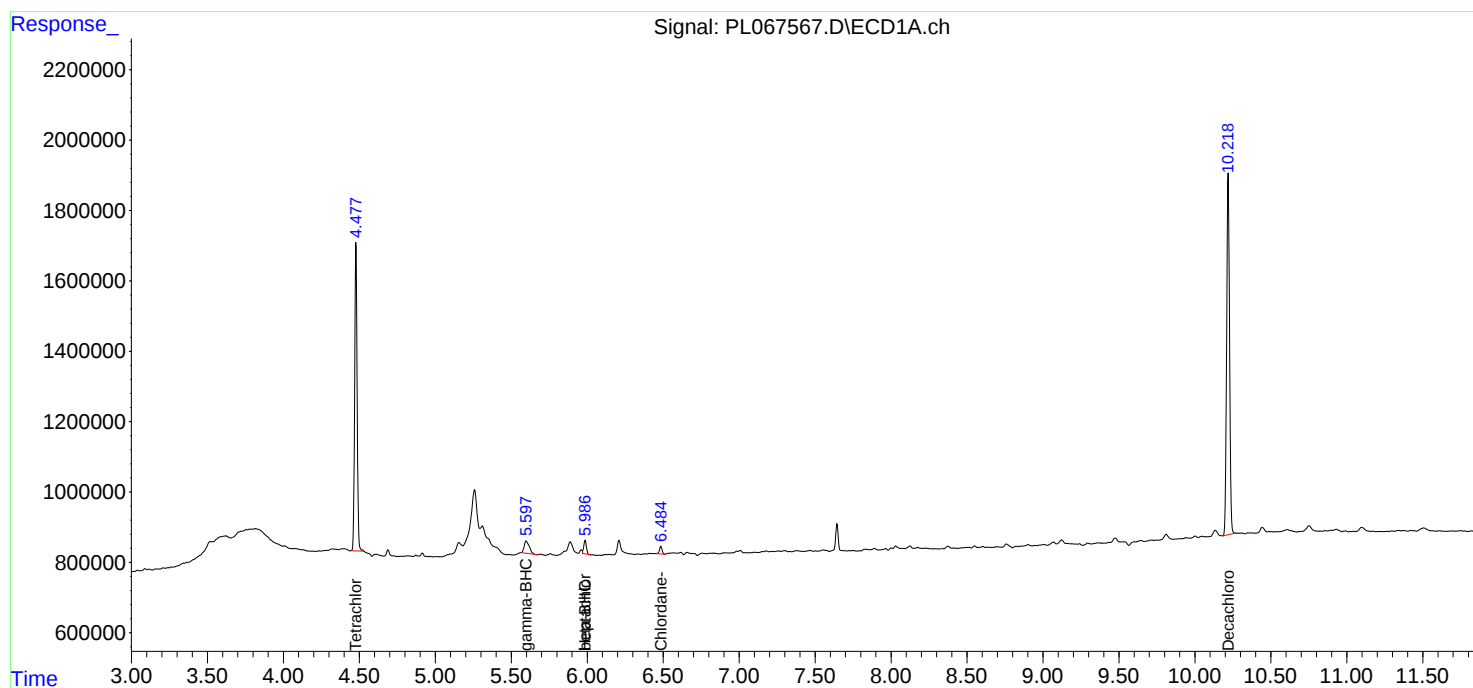


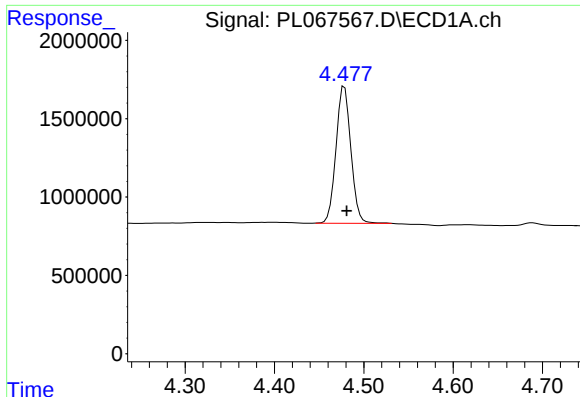

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10092768
Conc: 18.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

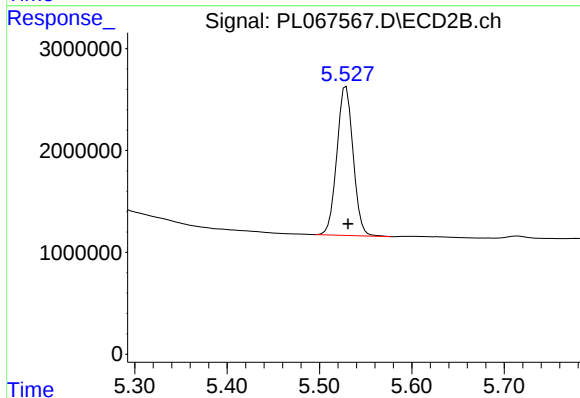


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 17853368
Conc: 18.94 ng/ml

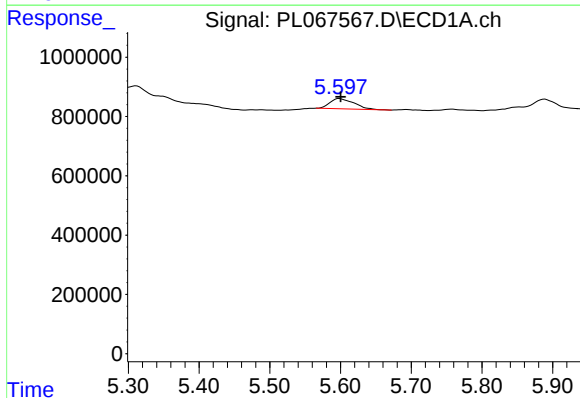


#3 gamma-BHC (Lindane)

R.T.: 5.598 min
Delta R.T.: -0.002 min
Response: 825802
Conc: 1.10 ng/ml

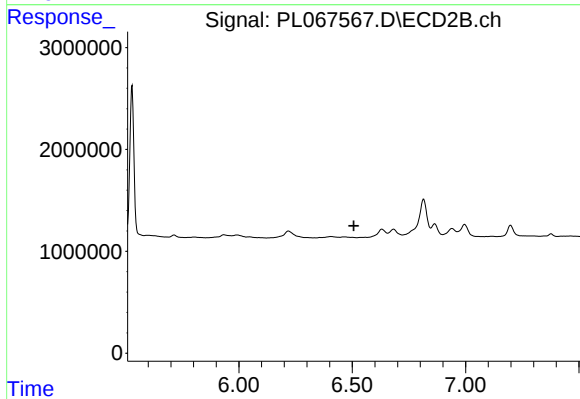

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

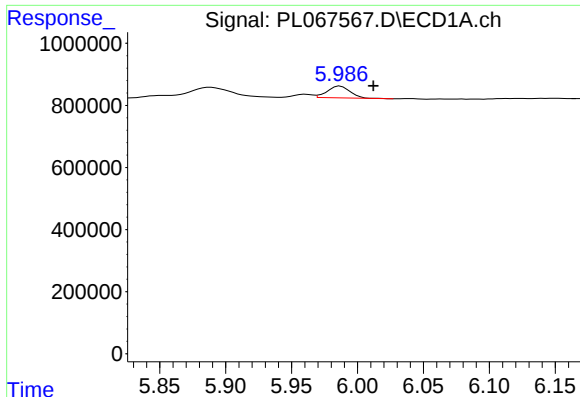

#4 Heptachlor


R.T.: 5.987 min
Delta R.T.: -0.025 min
Response: 457147
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

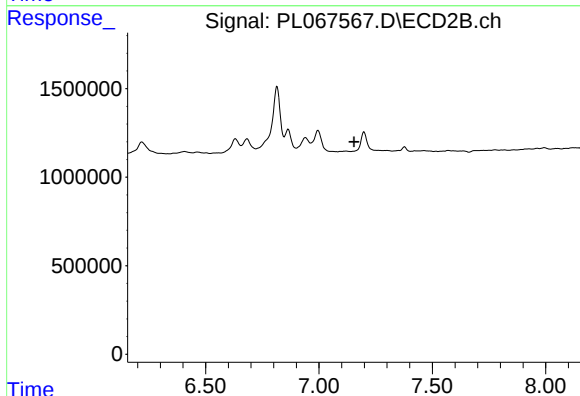


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

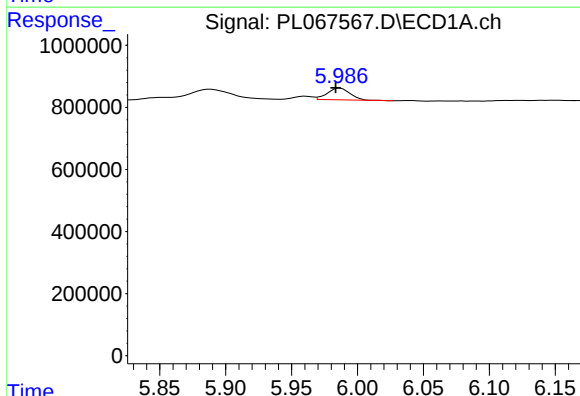


#6 beta-BHC

R.T.: 5.987 min
Delta R.T.: 0.004 min
Response: 457147
Conc: 1.28 ng/ml

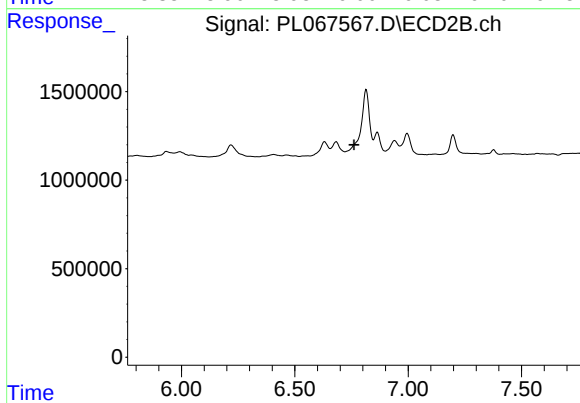

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

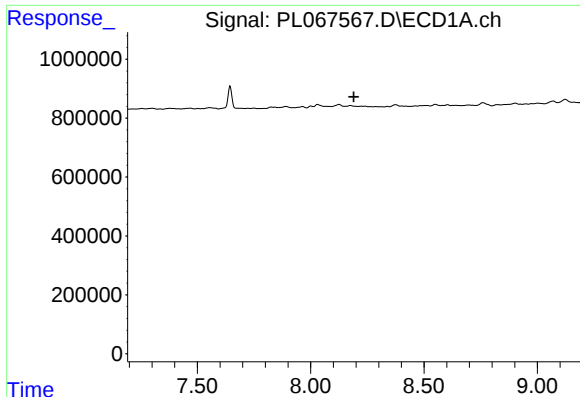

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

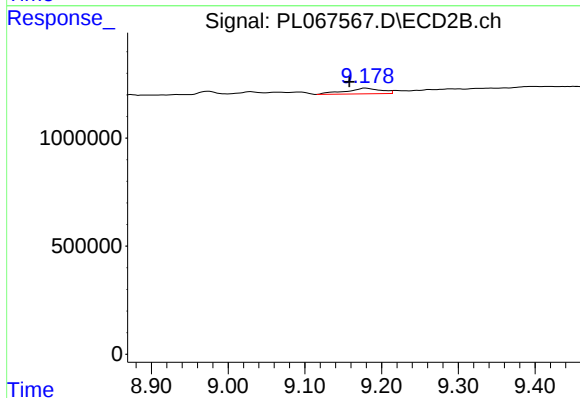


#15 Endosulfan II

R.T.: 9.180 min
Delta R.T.: 0.021 min
Response: 838503
Conc: 1.05 ng/ml

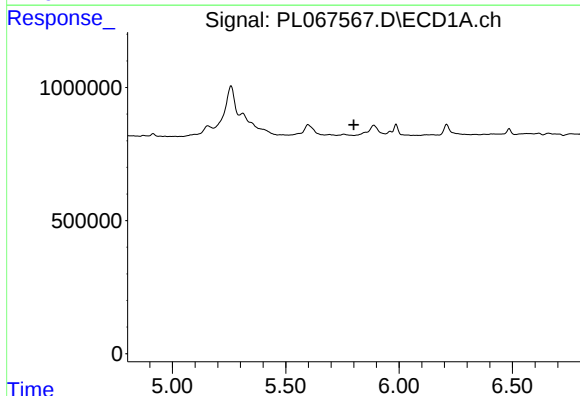


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

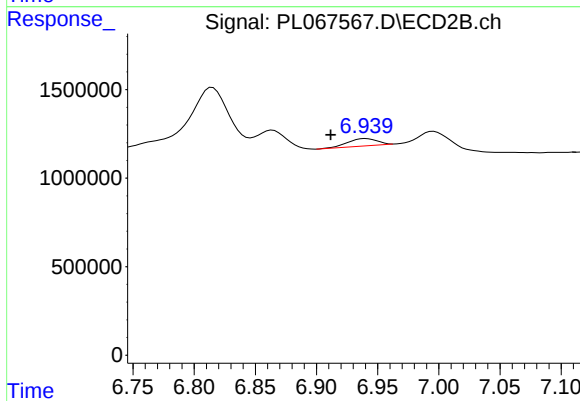

#23 Chlordane-1


R.T.: 6.940 min
Delta R.T.: 0.028 min
Response: 611671
Conc: 21.66 ng/ml

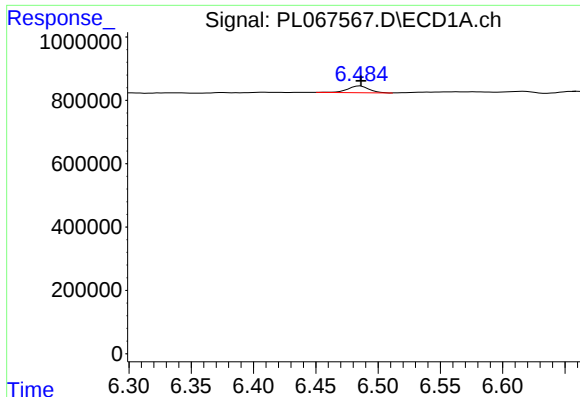

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 257048
Conc: 9.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

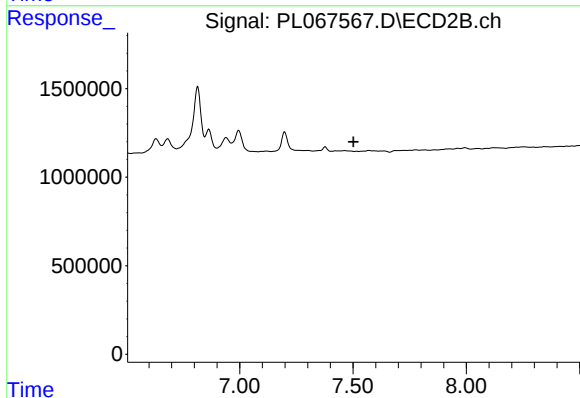


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

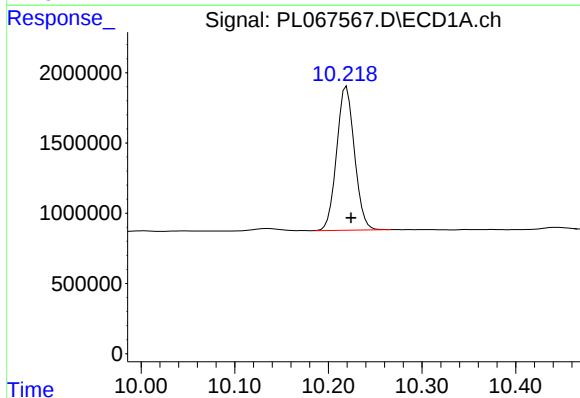

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 13542193
Conc: 19.11 ng/ml

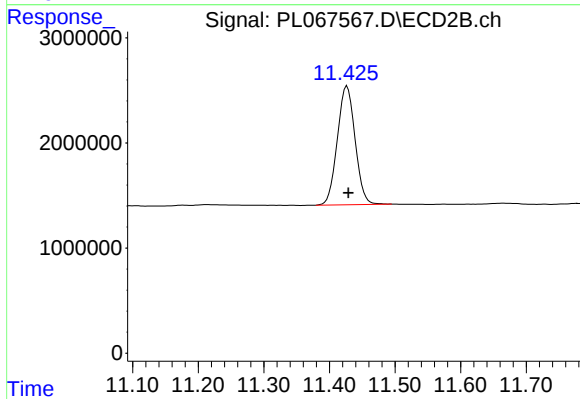

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 21248814
Conc: 21.33 ng/ml