

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 15:10
 Operator : AR\AJ
 Sample : M2708-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-06-061421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 02:09:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	6170577	10974224	11.224	11.641
28)	SA Decachlor...	10.219	11.426	8947300	14760974	12.625	14.819
Target Compounds							
7)	B delta-BHC	0.000	7.000f	0	927296	N.D.	0.789 #
10)	B gamma-Chl...	7.180	8.258	268837	569591	0.371	0.564 #
11)	B alpha-Chl...	7.248	8.340	539645	1104682	0.737	1.094 #
12)	B 4,4'-DDE	7.468	8.526	1666692	2096741	2.505	2.314
14)	MA Endrin	7.897f	0.000	216453	0	0.330	N.D. #
17)	MA 4,4'-DDT	8.305	0.000	355878	0	0.612	N.D. #
23)	Chlordane-1	5.797	0.000	105302	0	5.691	N.D. #
25)	Chlordane-3	7.180	8.258	268837	569591	4.001	4.256
26)	Chlordane-4	7.248	8.340	539645	1104682	7.384	6.815



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 15:10
Operator : AR\AJ
Sample : M2708-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
AU-06-061421

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 02:09:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

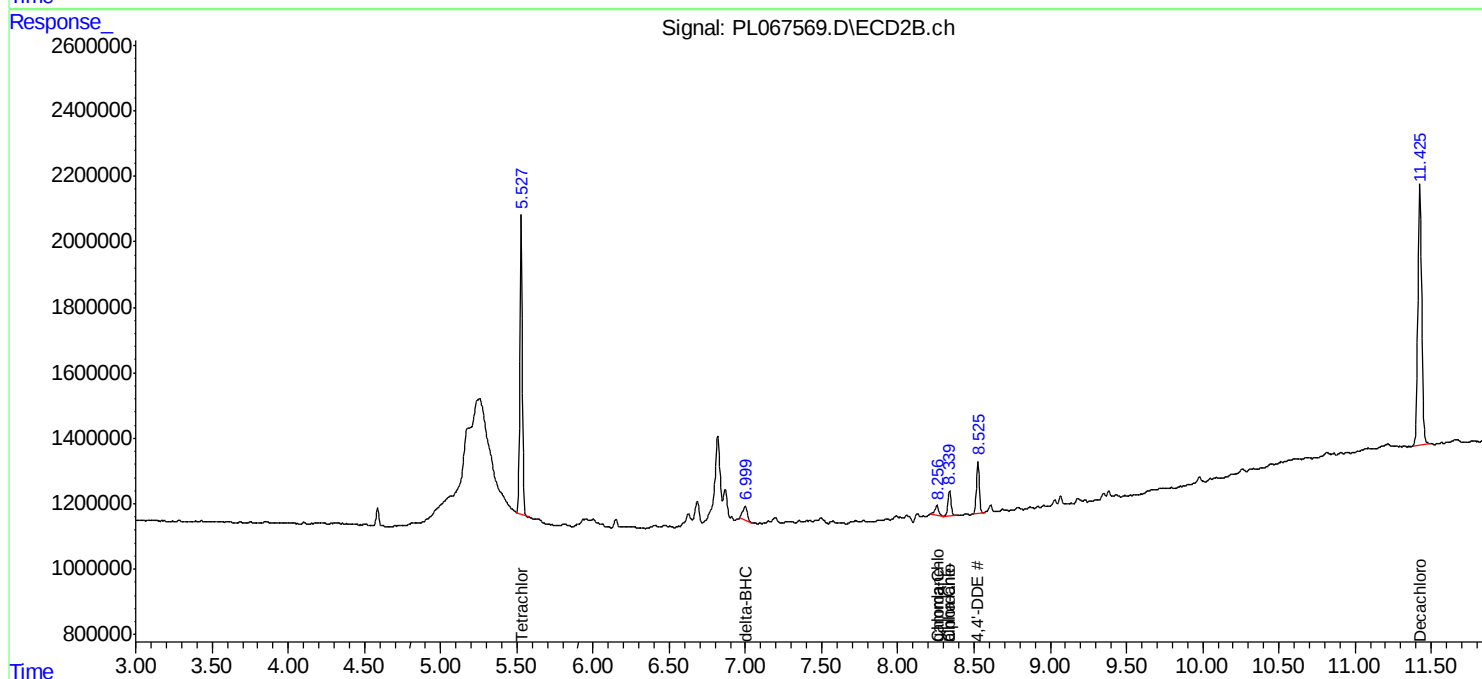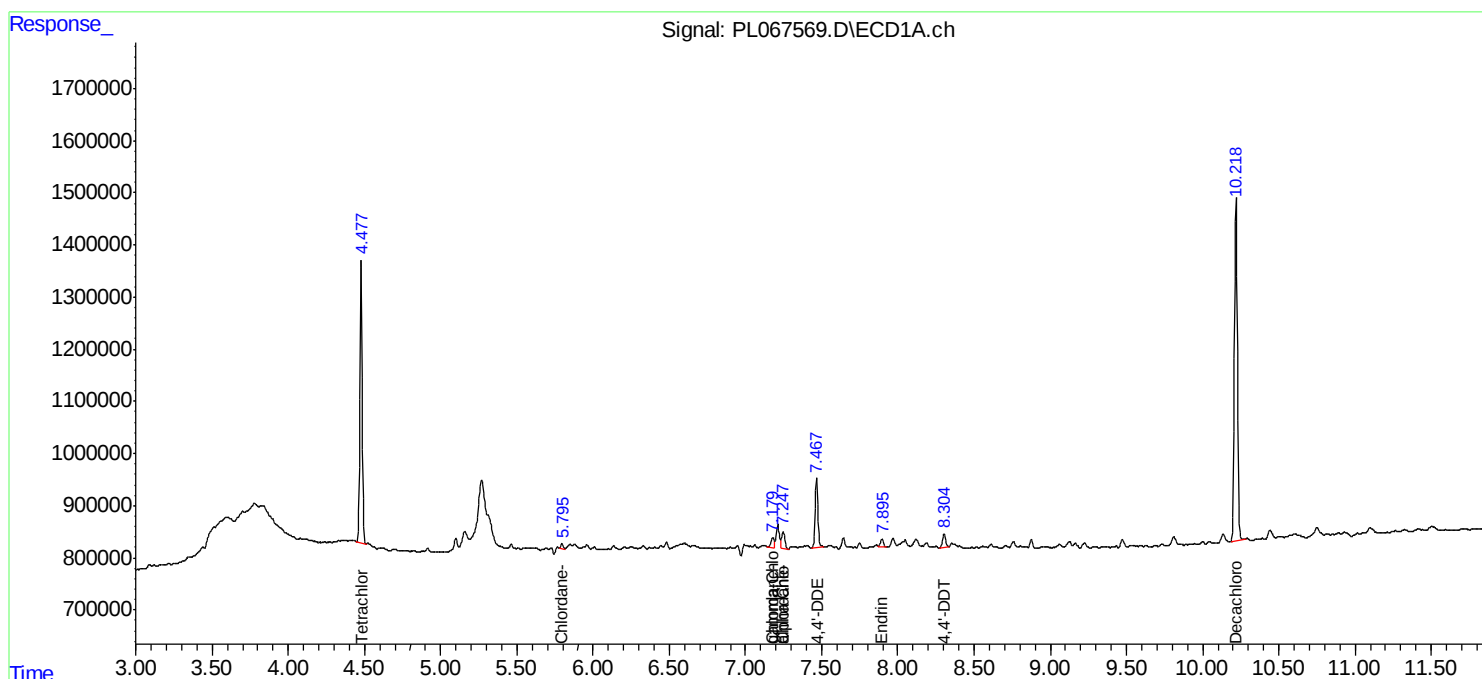


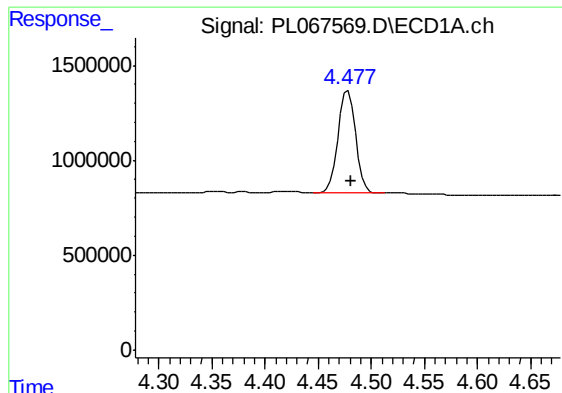

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 6170577
Conc: 11.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-061421

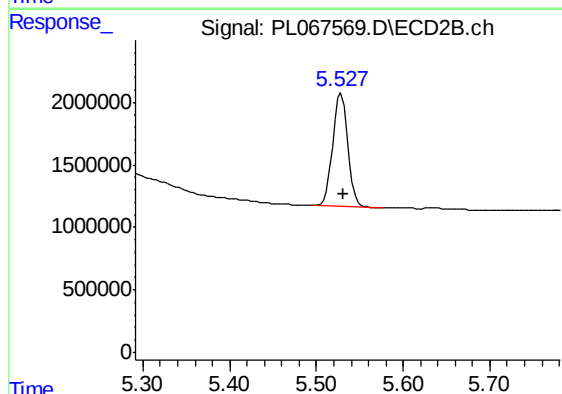


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 10974224
Conc: 11.64 ng/ml

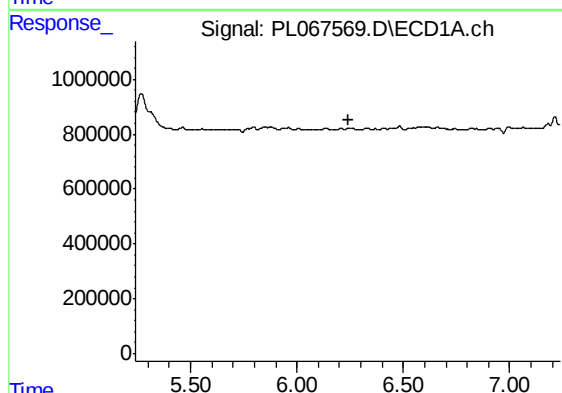


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

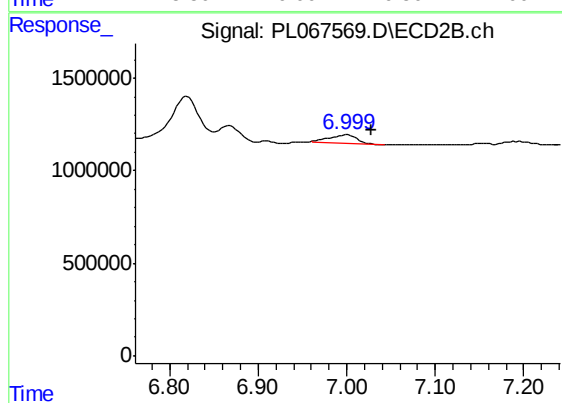

#7 delta-BHC


R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 927296
Conc: 0.79 ng/ml

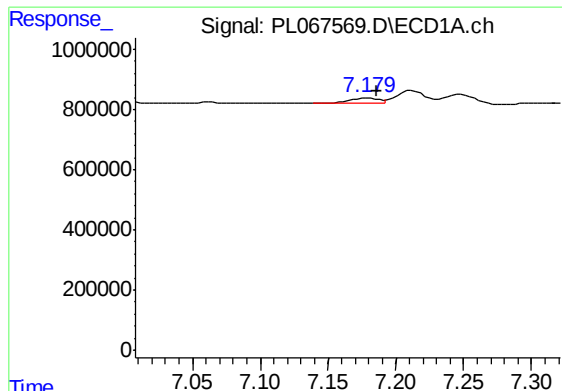

#10 gamma-Chlordane


R.T.: 7.180 min
Delta R.T.: -0.006 min
Response: 268837
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-061421

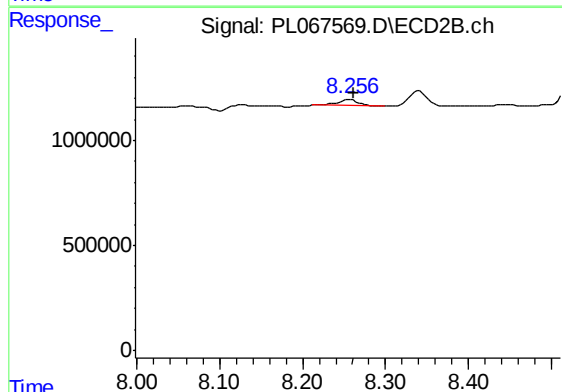


#10 gamma-Chlordane

R.T.: 8.258 min
Delta R.T.: -0.003 min
Response: 569591
Conc: 0.56 ng/ml

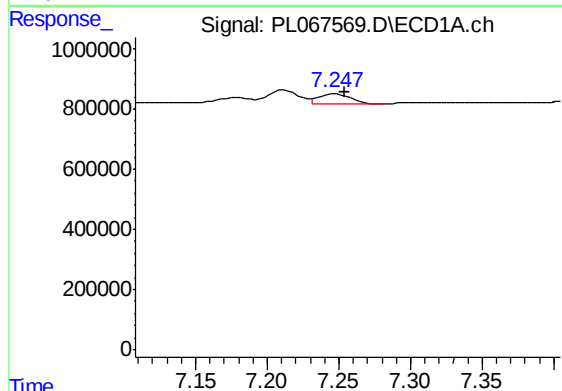


#11 alpha-Chlordane

R.T.: 7.248 min
Delta R.T.: -0.006 min
Response: 539645
Conc: 0.74 ng/ml

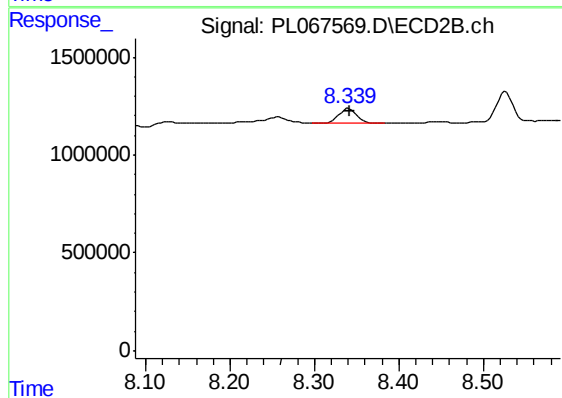

#11 alpha-Chlordane


R.T.: 8.340 min
Delta R.T.: -0.002 min
Response: 1104682
Conc: 1.09 ng/ml

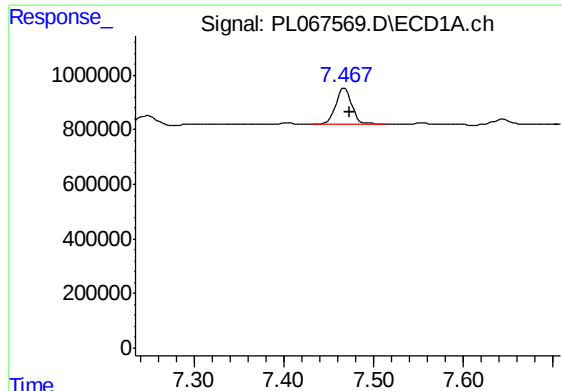

#12 4,4'-DDE


R.T.: 7.468 min
Delta R.T.: -0.005 min
Response: 1666692
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-061421

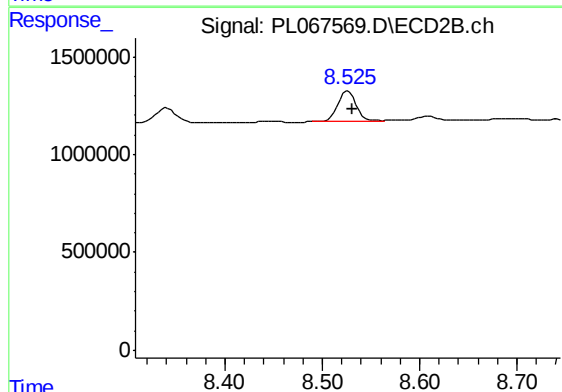


#12 4,4'-DDE

R.T.: 8.526 min
Delta R.T.: -0.004 min
Response: 2096741
Conc: 2.31 ng/ml

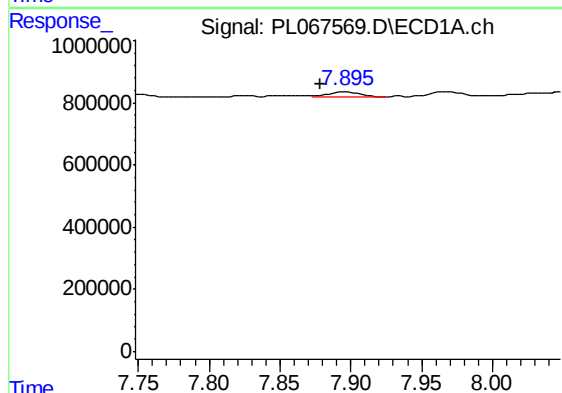


#14 Endrin

R.T.: 7.897 min
Delta R.T.: 0.018 min
Response: 216453
Conc: 0.33 ng/ml

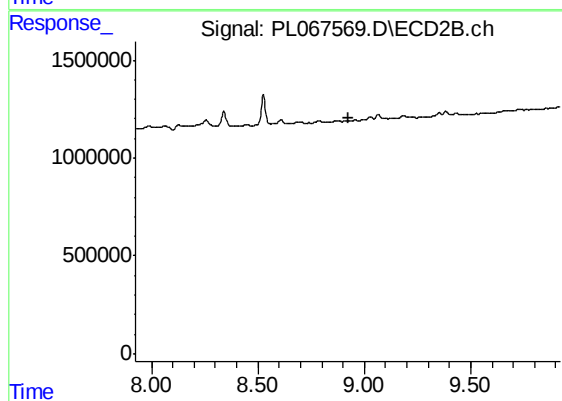

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

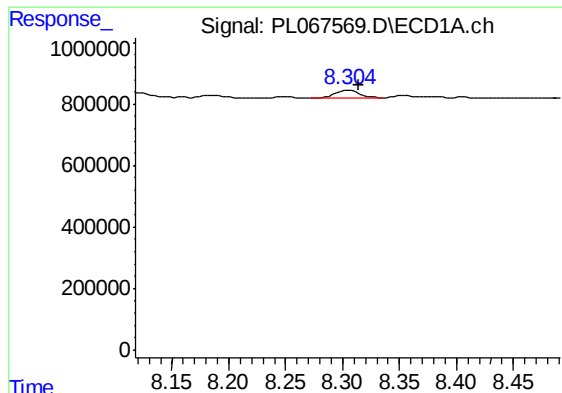

#17 4,4'-DDT


R.T.: 8.305 min
Delta R.T.: -0.009 min
Response: 355878
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-061421

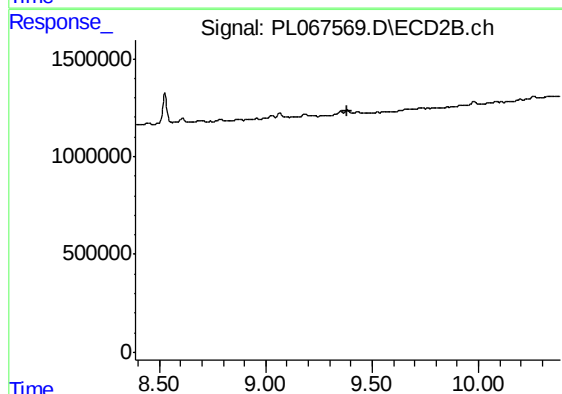


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.386 min
Response: 0
Conc: N.D.

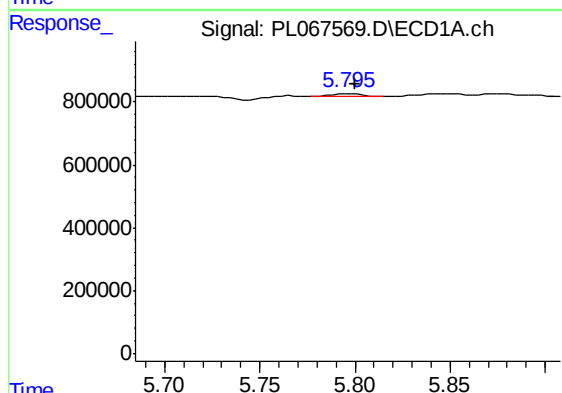


#23 Chlordane-1

R.T.: 5.797 min
Delta R.T.: -0.003 min
Response: 105302
Conc: 5.69 ng/ml

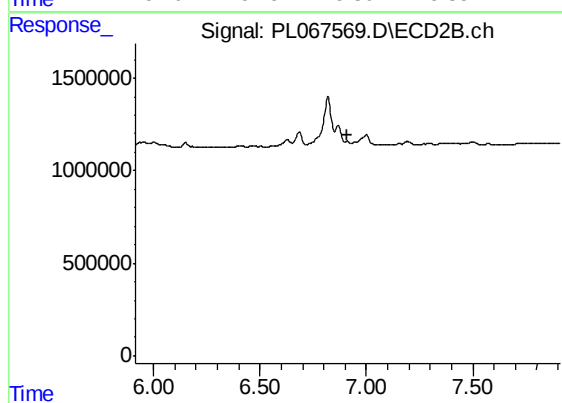

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

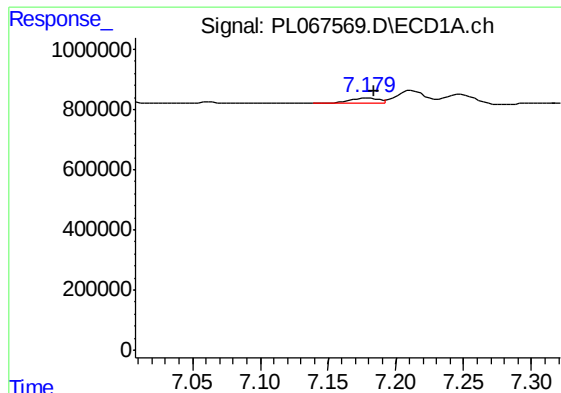

#25 Chlordane-3


R.T.: 7.180 min
Delta R.T.: -0.004 min
Response: 268837
Conc: 4.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-061421

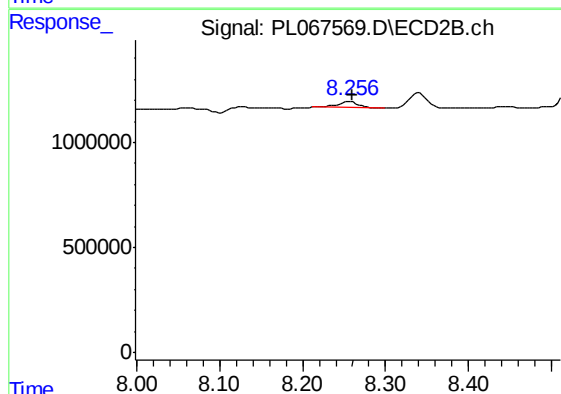


#25 Chlordane-3

R.T.: 8.258 min
Delta R.T.: -0.002 min
Response: 569591
Conc: 4.26 ng/ml

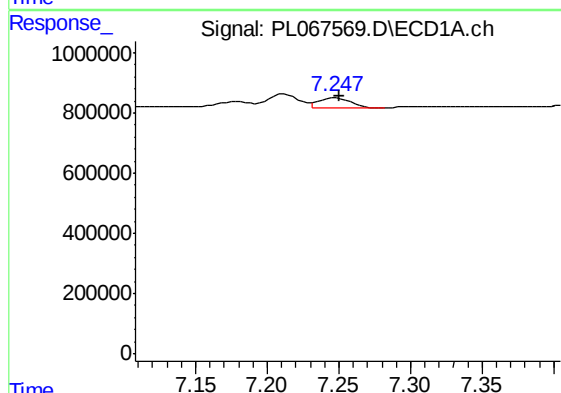


#26 Chlordane-4

R.T.: 7.248 min
Delta R.T.: -0.002 min
Response: 539645
Conc: 7.38 ng/ml

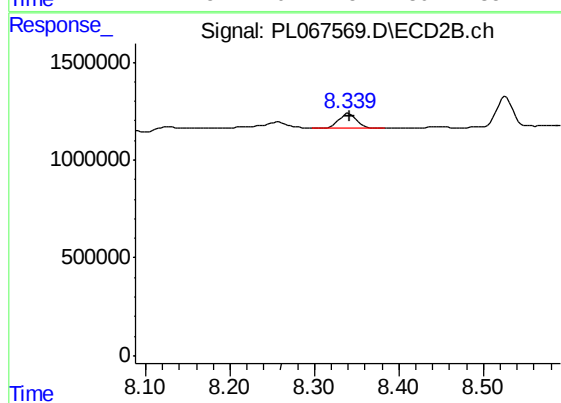

#26 Chlordane-4


R.T.: 8.340 min
Delta R.T.: 0.000 min
Response: 1104682
Conc: 6.81 ng/ml

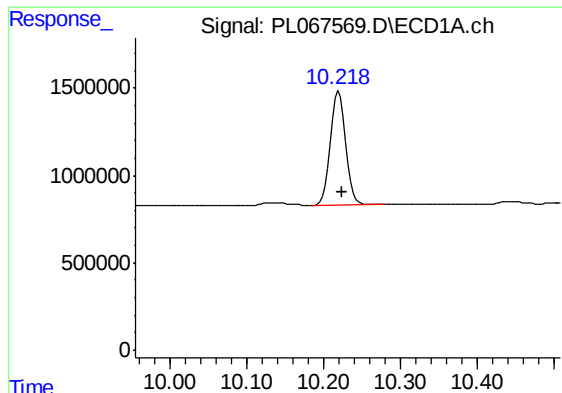

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 8947300
Conc: 12.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-061421

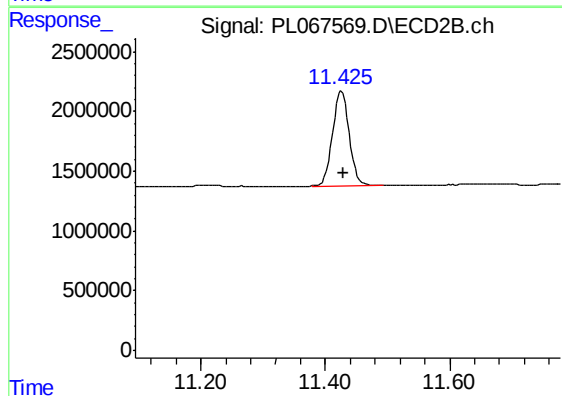

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 14760974
Conc: 14.82 ng/ml