

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 19:53
 Operator : AR\AJ
 Sample : M2687-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 17-B6(108-112)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:37:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	9931089	17683372	18.064	18.758
28)	SA Decachlor...	10.219	11.426	13729261	22244031	19.373	22.332
Target Compounds							
6)	B beta-BHC	5.961f	0.000	212766	0	0.595	N.D. #
7)	B delta-BHC	0.000	7.004f	0	1467762	N.D.	1.249 #
11)	B alpha-Chl...	7.253	0.000	333797	0	0.456	N.D. #
26)	Chlordane-4	7.253	0.000	333797	0	4.568	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067584.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 19:53
Operator : AR\AJ
Sample : M2687-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
17-B6(108-112)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:37:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

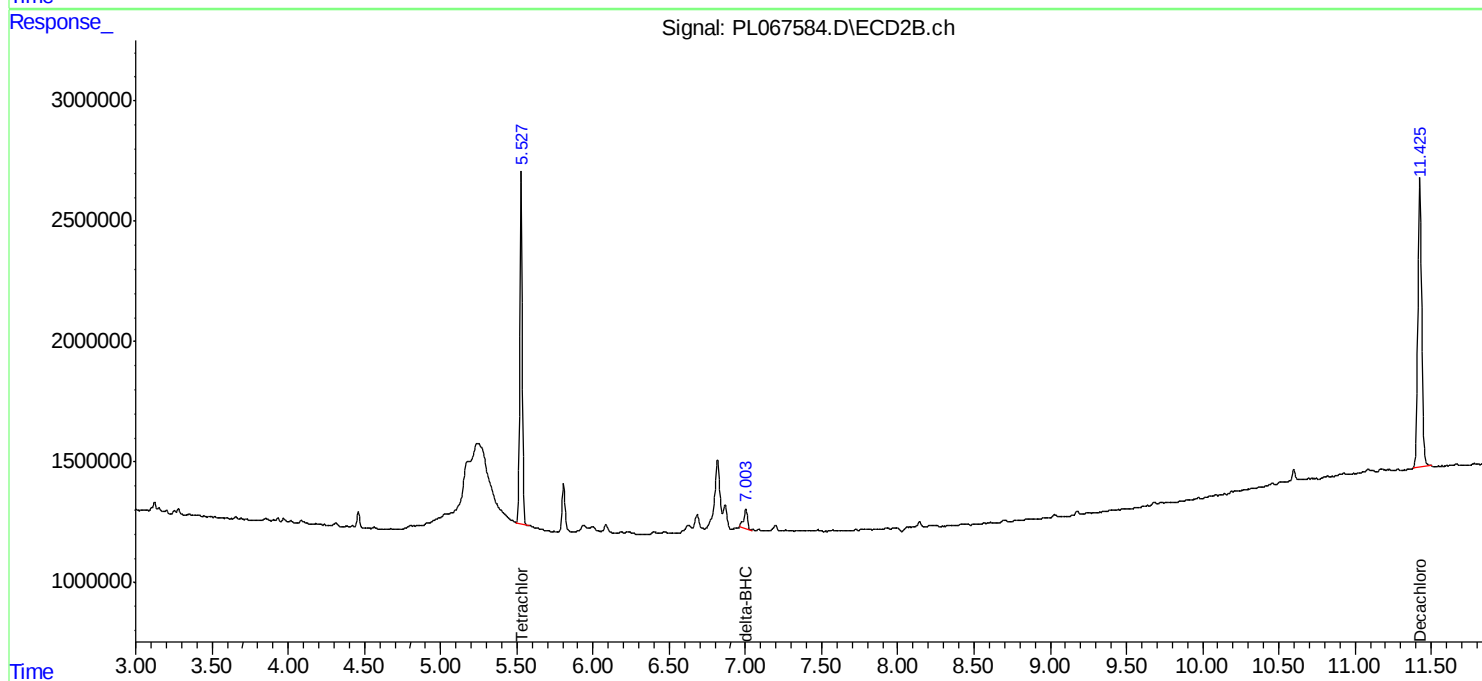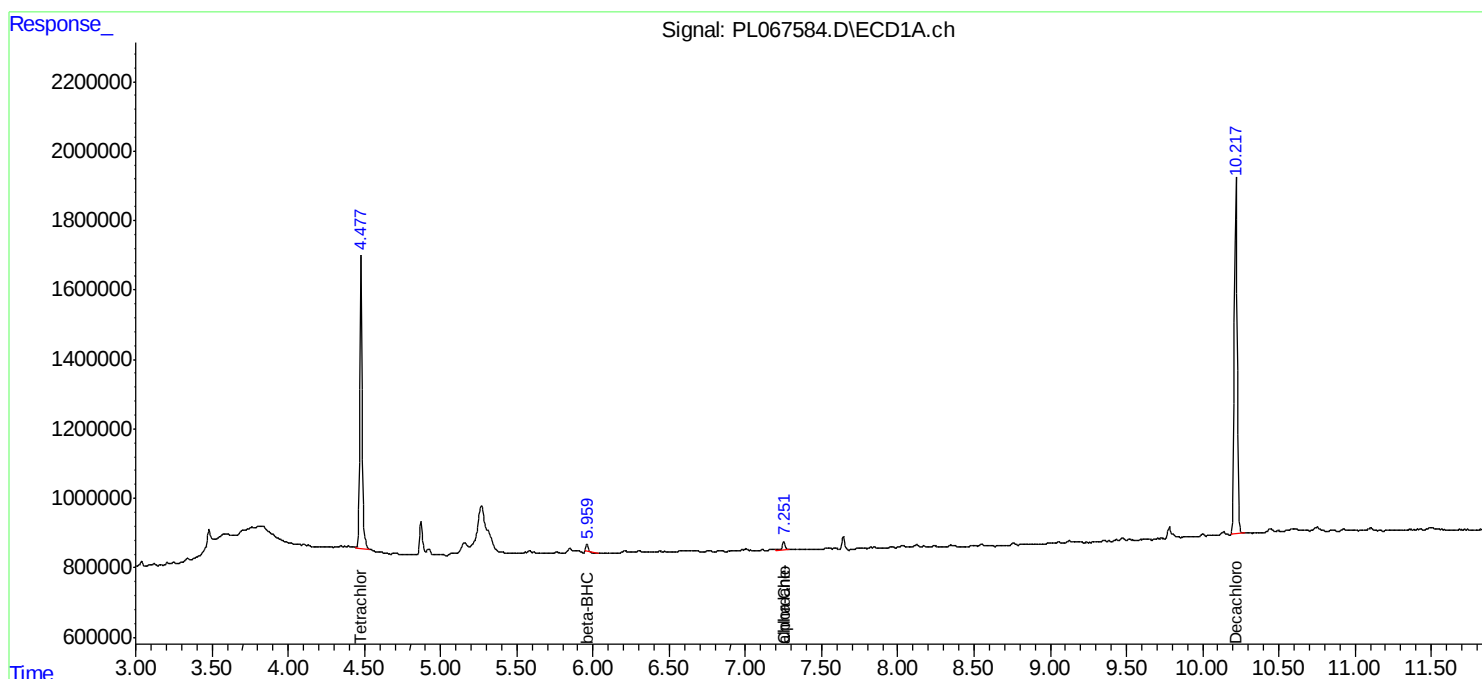


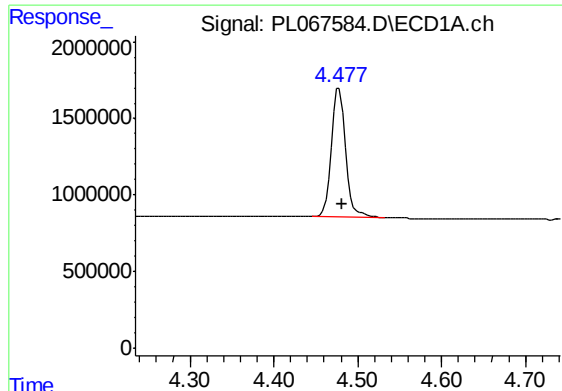

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 9931089
Conc: 18.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
17-B6(108-112)

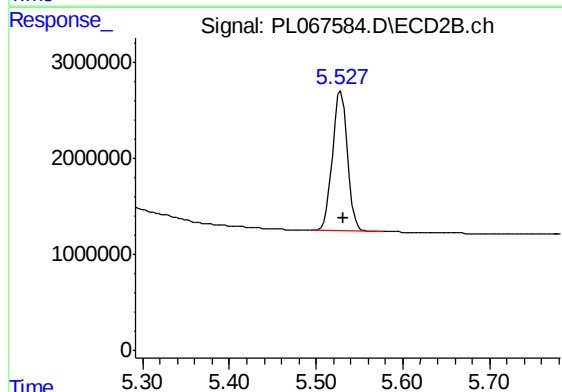


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 17683372
Conc: 18.76 ng/ml

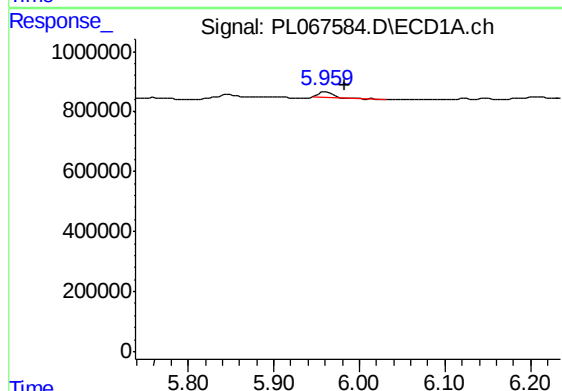


#6 beta-BHC

R.T.: 5.961 min
Delta R.T.: -0.023 min
Response: 212766
Conc: 0.59 ng/ml

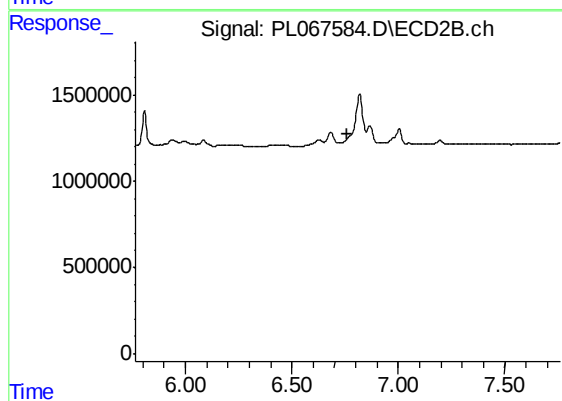

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

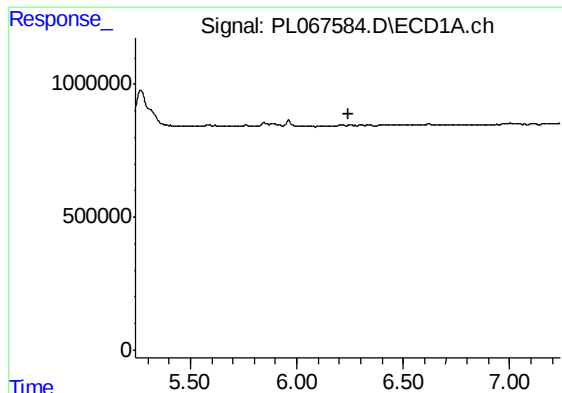

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
17-B6(108-112)

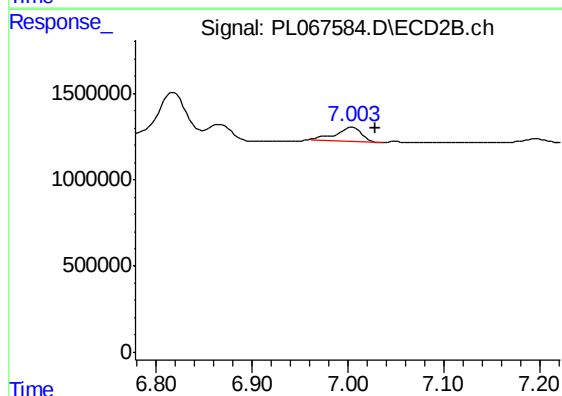


#7 delta-BHC

R.T.: 7.004 min
Delta R.T.: -0.024 min
Response: 1467762
Conc: 1.25 ng/ml

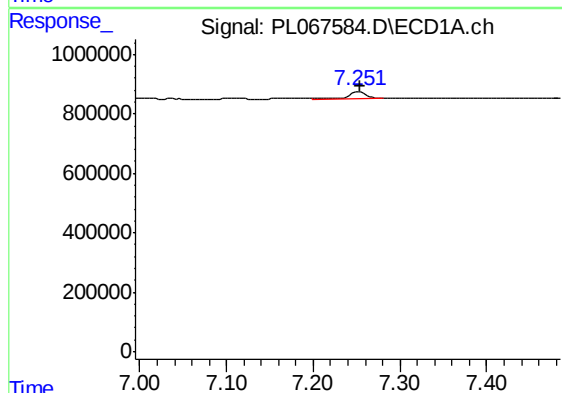


#11 alpha-Chlordane

R.T.: 7.253 min
Delta R.T.: -0.002 min
Response: 333797
Conc: 0.46 ng/ml

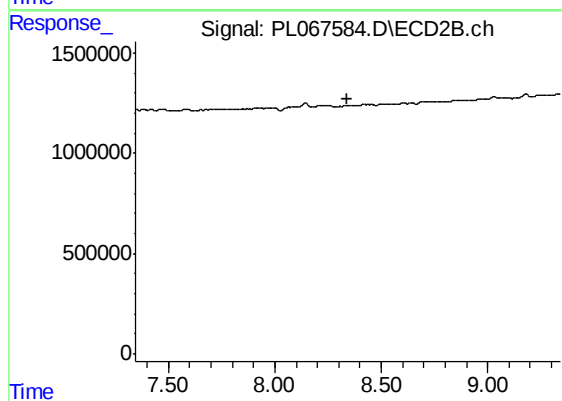

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

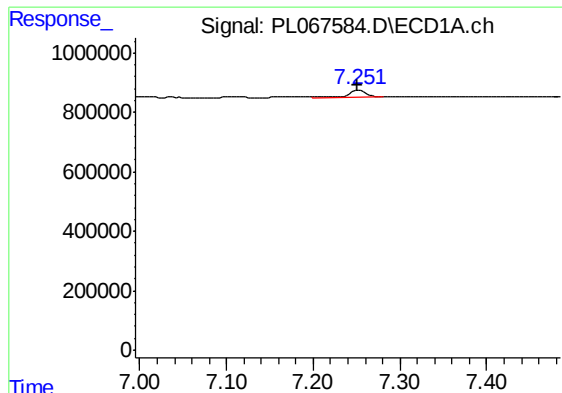

#26 Chlordane-4


R.T.: 7.253 min
Delta R.T.: 0.002 min
Response: 333797
Conc: 4.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
17-B6(108-112)

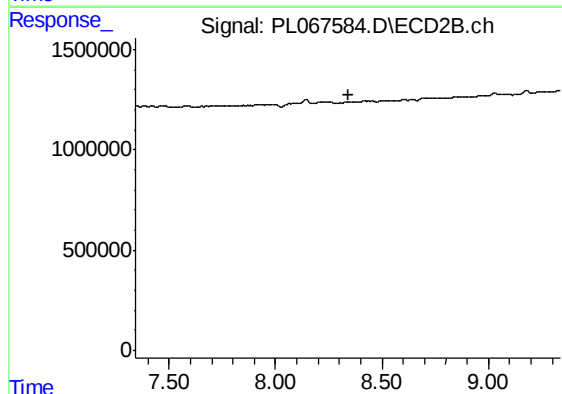


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

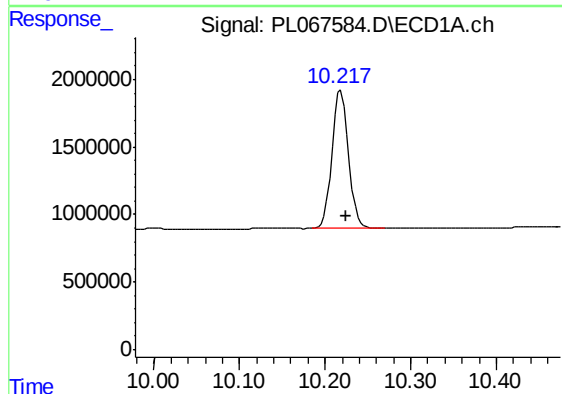

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 13729261
Conc: 19.37 ng/ml

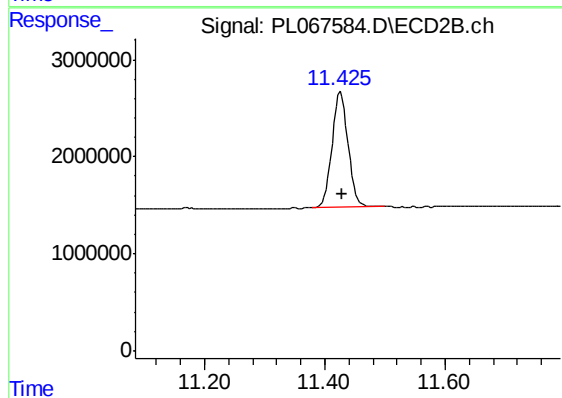

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.002 min
Response: 22244031
Conc: 22.33 ng/ml