

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 21:32
 Operator : AR\AJ
 Sample : M2687-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUP-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:39:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	4.480	5.531	10927310	18745443	19.876	19.884
28) SA	Decachlor...	10.223	11.432	14749936	23568547	20.813	23.662
Target Compounds							
6) B	beta-BHC	5.963f	0.000	294365	0	0.823	N.D. #
7) B	delta-BHC	0.000	7.007f	0	1684546	N.D.	1.433 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 21:32
Operator : AR\AJ
Sample : M2687-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DUP-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:39:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

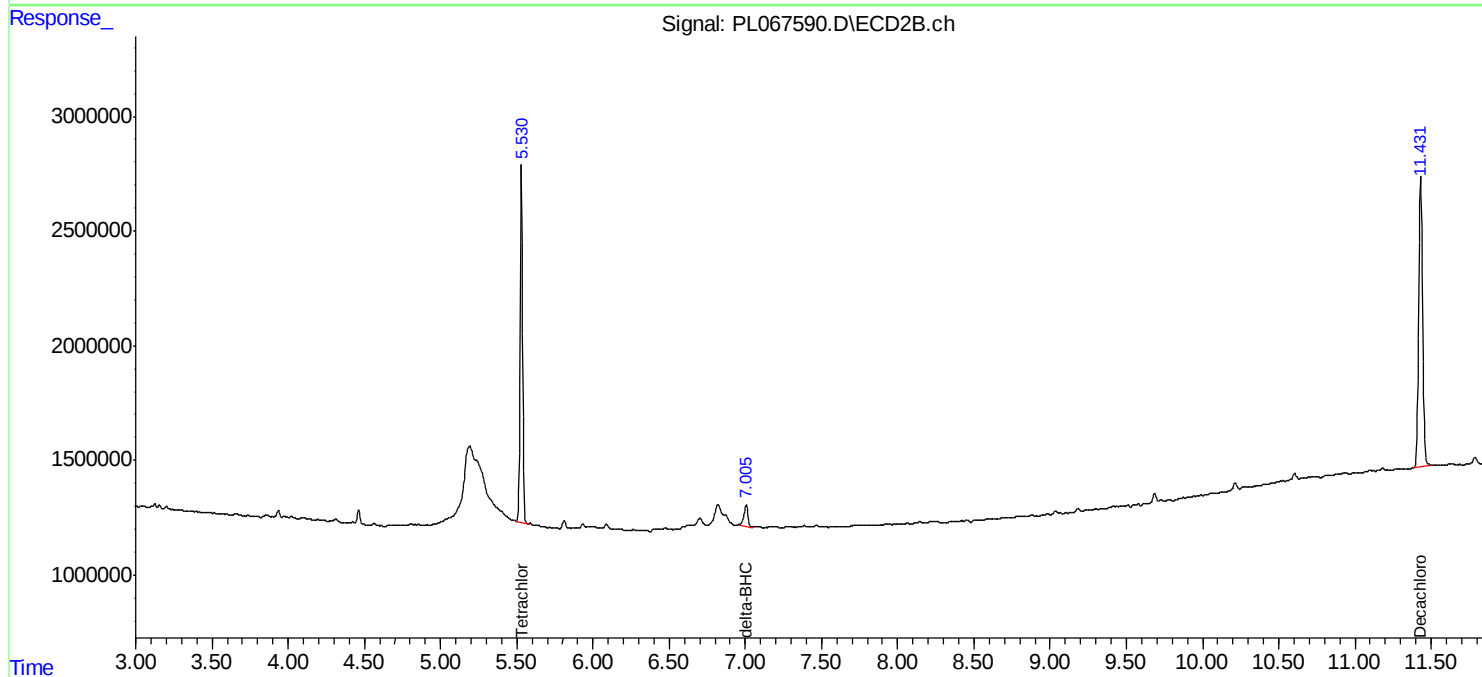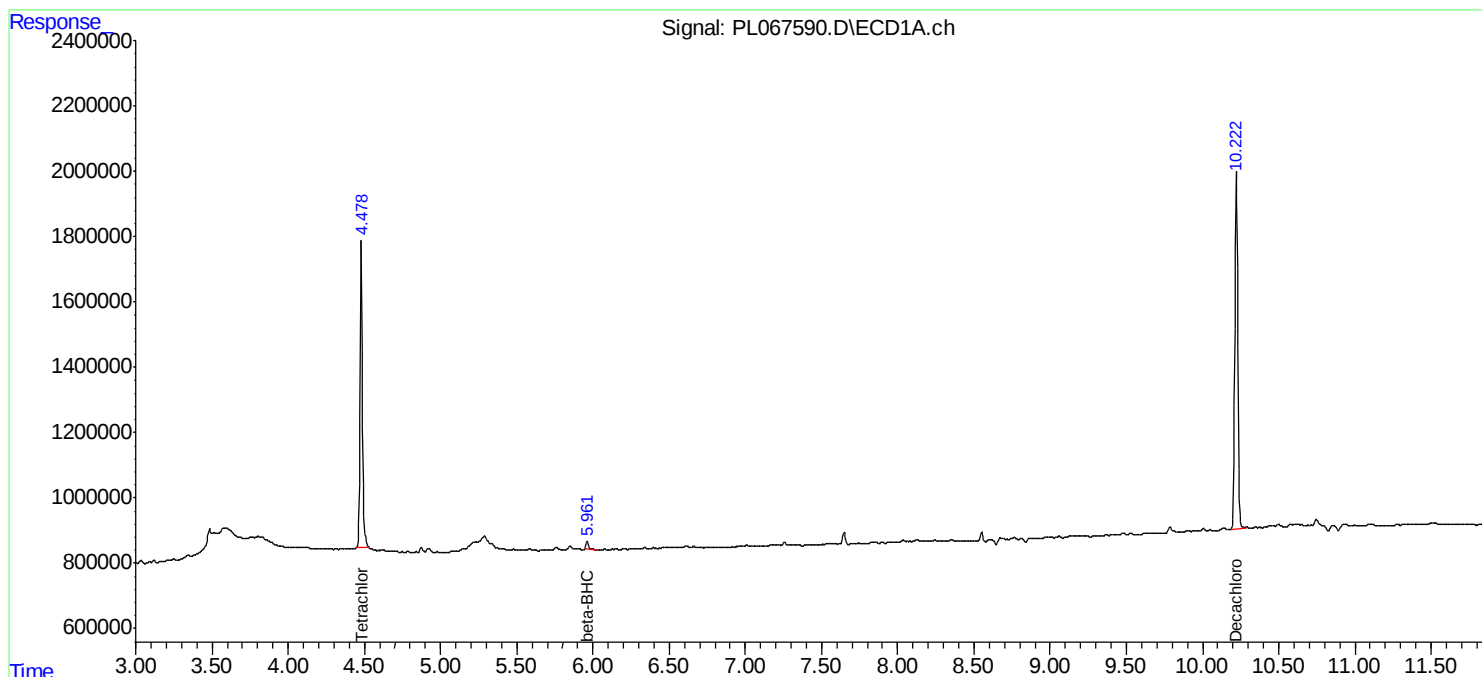


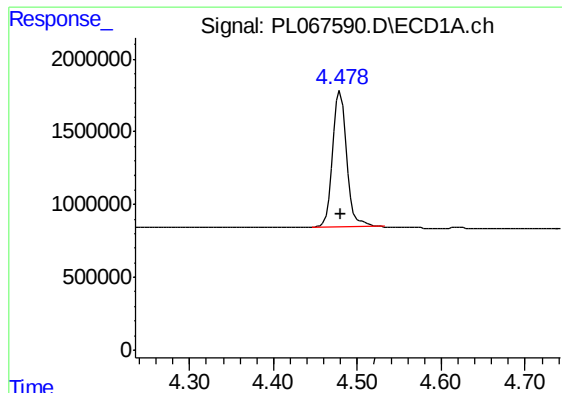

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 10927310
Conc: 19.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-02

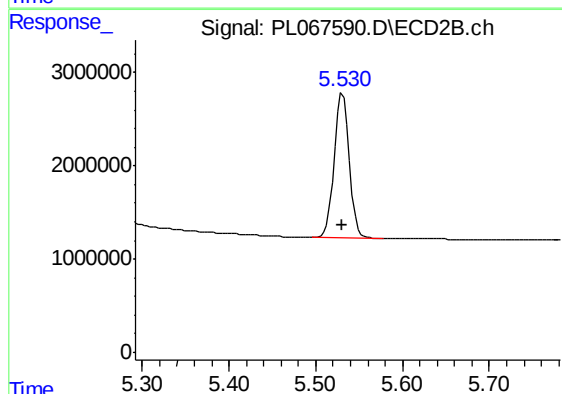


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 18745443
Conc: 19.88 ng/ml

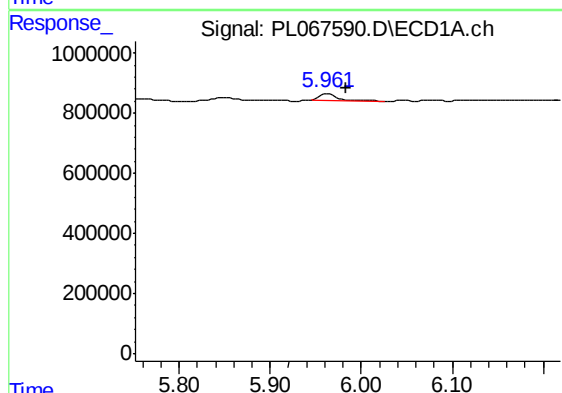


#6 beta-BHC

R.T.: 5.963 min
Delta R.T.: -0.021 min
Response: 294365
Conc: 0.82 ng/ml

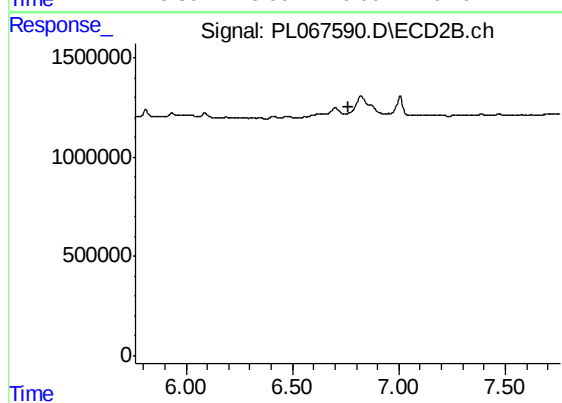

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

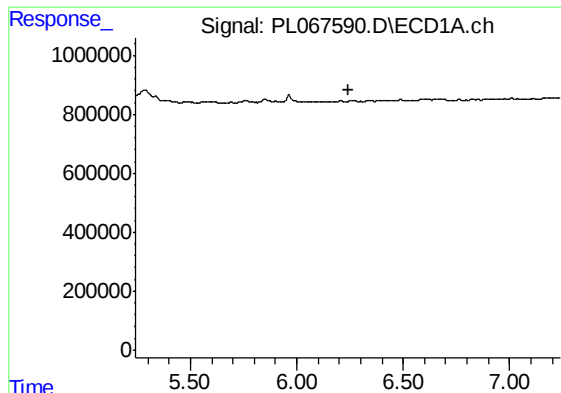

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DUP-02

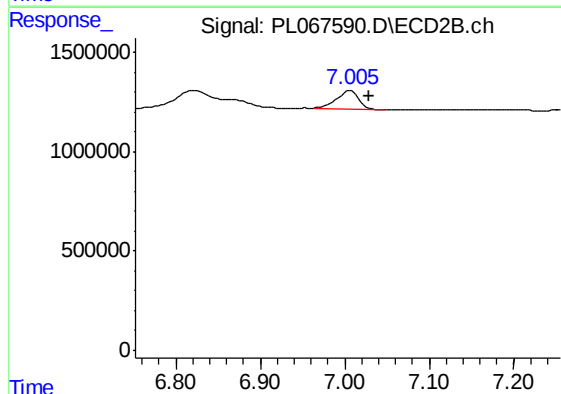


#7 delta-BHC

R.T.: 7.007 min
Delta R.T.: -0.021 min
Response: 1684546
Conc: 1.43 ng/ml

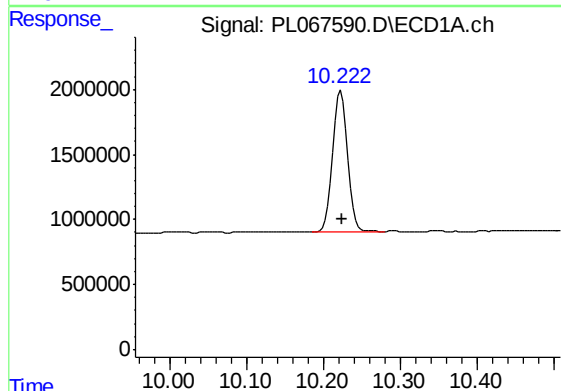

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.001 min
Response: 14749936
Conc: 20.81 ng/ml

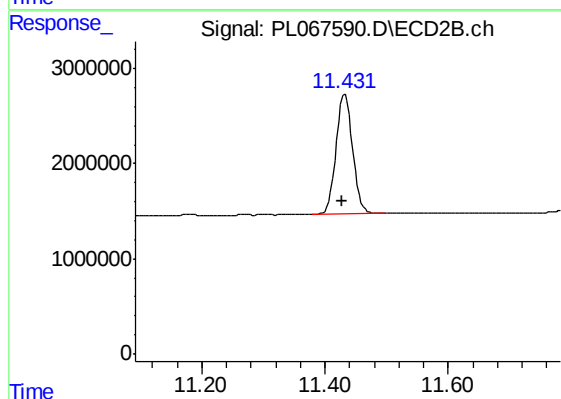

#28 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: 0.004 min
Response: 23568547
Conc: 23.66 ng/ml