

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 21:49
 Operator : AR\AJ
 Sample : M2687-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUP-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:39:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.531	11342500	19361288	20.631	20.537
28)	SA Decachlor...	10.223	11.431	15140111	24218028	21.364	24.314
Target Compounds							
2)	A alpha-BHC	0.000	6.089f	0	429089	N.D.	0.347 #
6)	B beta-BHC	5.963f	0.000	528447	0	1.477	N.D. #
7)	B delta-BHC	0.000	7.008f	0	2310213	N.D.	1.965 #
11)	B alpha-Chl...	7.256	0.000	193353	0	0.264	N.D. #
26)	Chlordane-4	7.256	0.000	193353	0	2.646	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 21:49
Operator : AR\AJ
Sample : M2687-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DUP-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:39:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

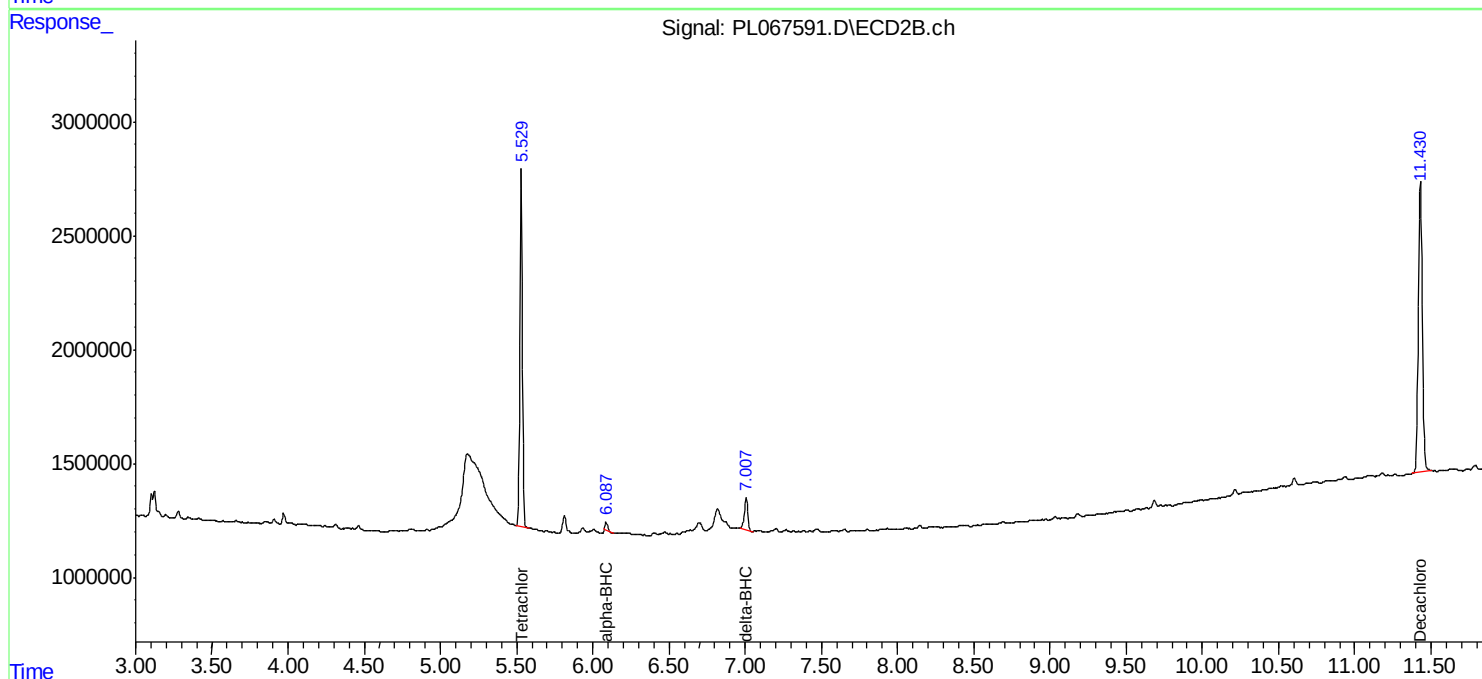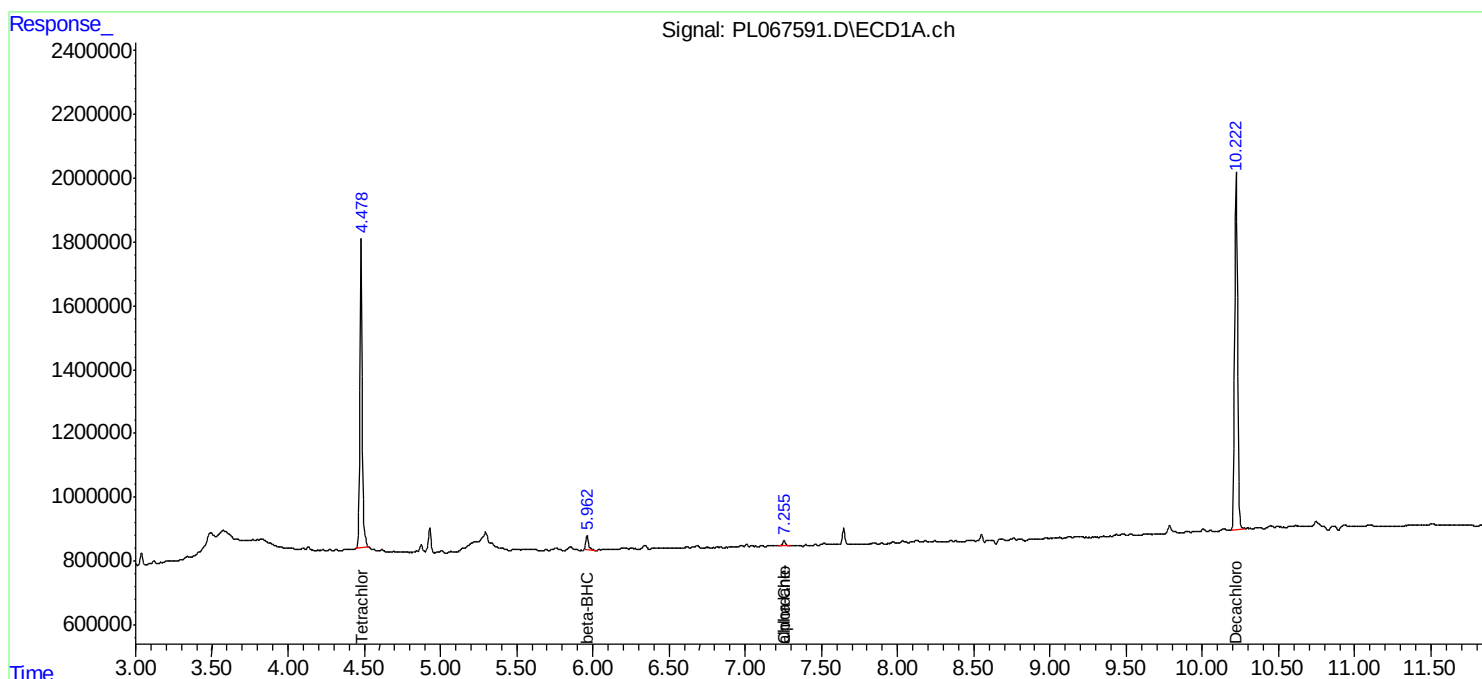


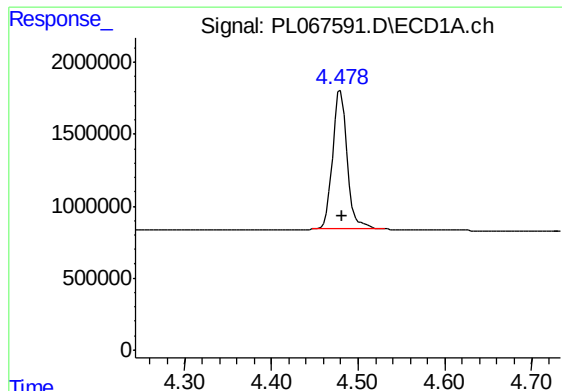

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 11342500
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-03

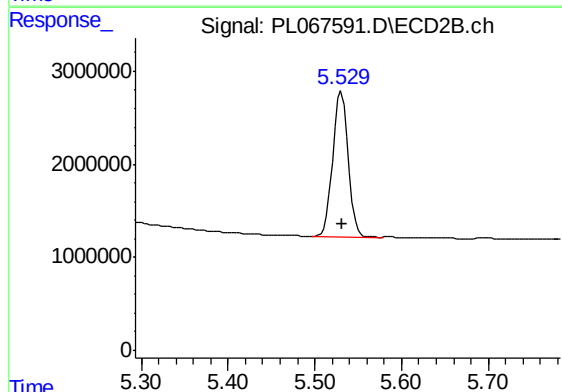


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 19361288
Conc: 20.54 ng/ml

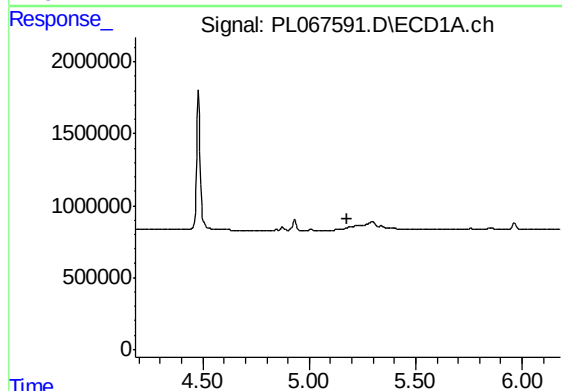


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.181 min
Response: 0
Conc: N.D.

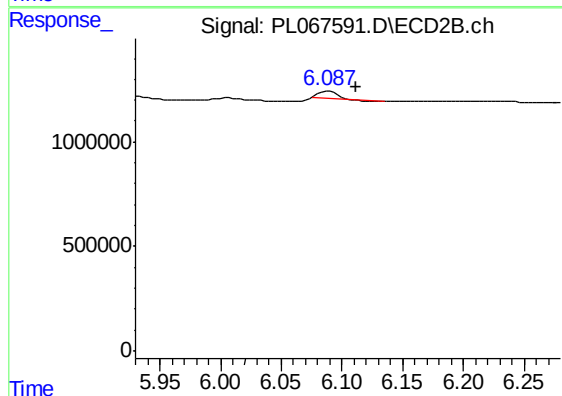

#2 alpha-BHC


R.T.: 6.089 min
Delta R.T.: -0.023 min
Response: 429089
Conc: 0.35 ng/ml

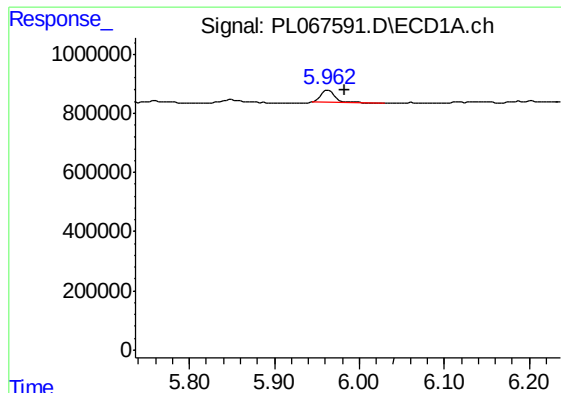

#6 beta-BHC


R.T.: 5.963 min
Delta R.T.: -0.020 min
Response: 528447
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-03

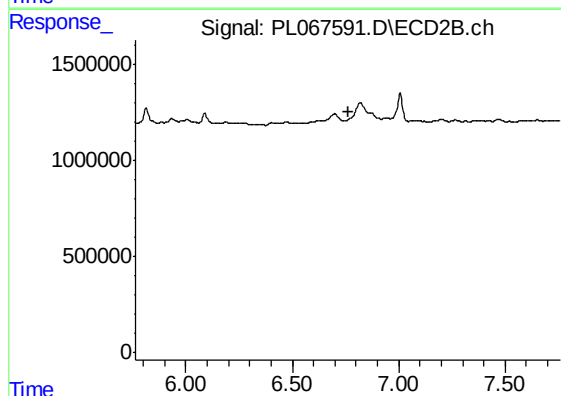


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

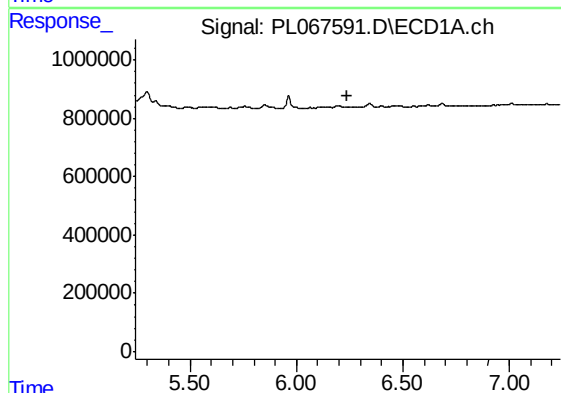


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

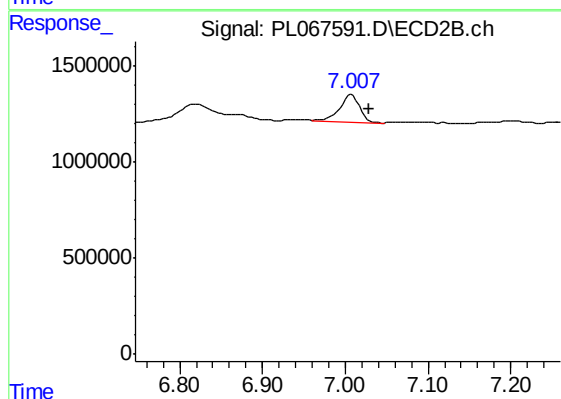

#7 delta-BHC


R.T.: 7.008 min
Delta R.T.: -0.020 min
Response: 2310213
Conc: 1.97 ng/ml

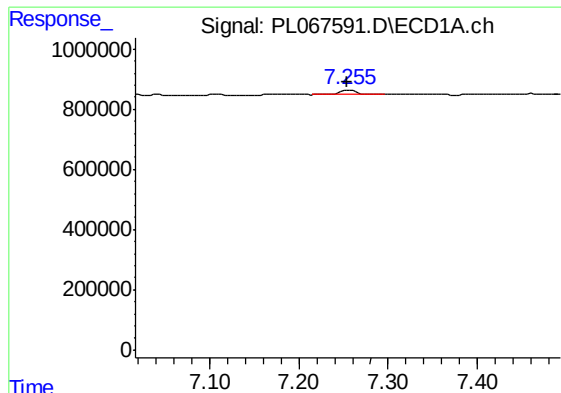

#11 alpha-Chlordane


R.T.: 7.256 min
Delta R.T.: 0.002 min
Response: 193353
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-03

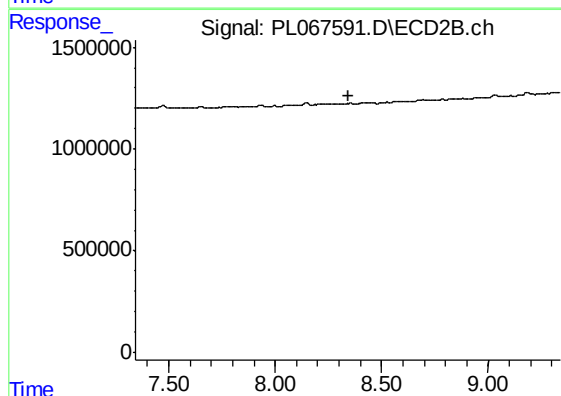


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

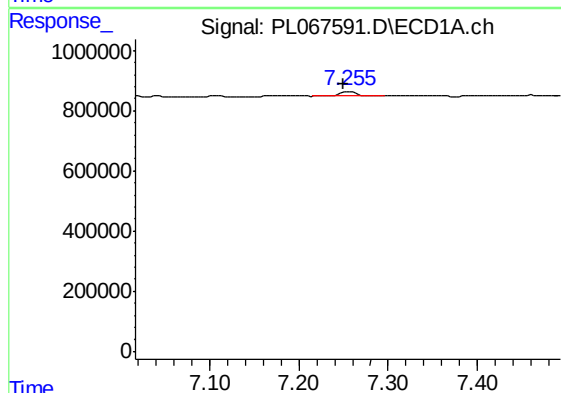


#26 Chlordane-4

R.T.: 7.256 min
Delta R.T.: 0.006 min
Response: 193353
Conc: 2.65 ng/ml

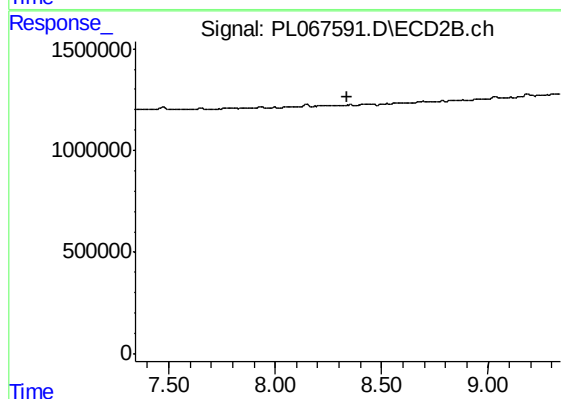

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

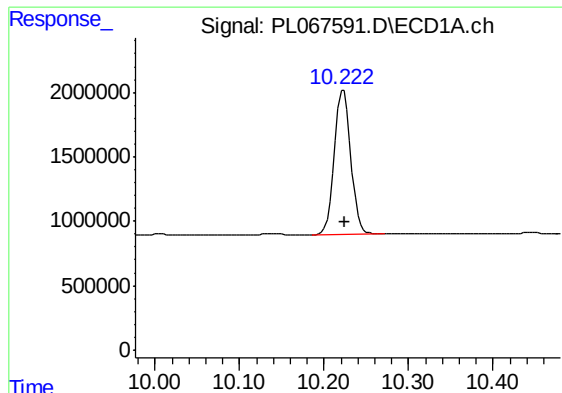

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.001 min
Response: 15140111
Conc: 21.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-03

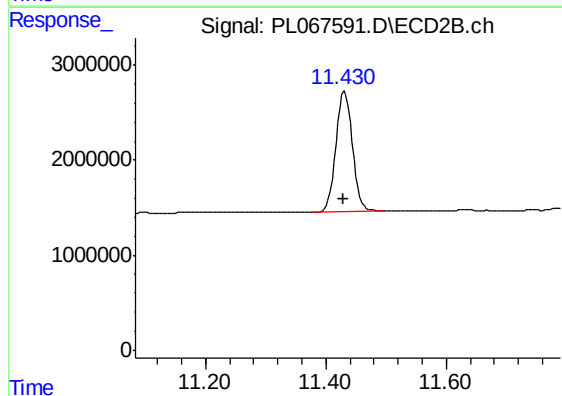

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: 0.003 min
Response: 24218028
Conc: 24.31 ng/ml