

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 01:42
 Operator : AR\AJ
 Sample : M2748-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-10-AOC-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:43:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.528	11490940	20195357	20.901	21.422
28)	SA Decachlor...	10.218	11.425	13506700	21295296	19.059	21.380
Target Compounds							
2)	A alpha-BHC	5.179	0.000	376562	0	0.512	N.D. #
7)	B delta-BHC	0.000	7.001f	0	791570	N.D.	0.673 #
22)	Mirex	9.304	0.000	253565	0	0.403	N.D. #
24)	Chlordane-2	6.467f	0.000	709130	0	26.482	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 01:42
Operator : AR\AJ
Sample : M2748-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-10-AOC-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:43:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

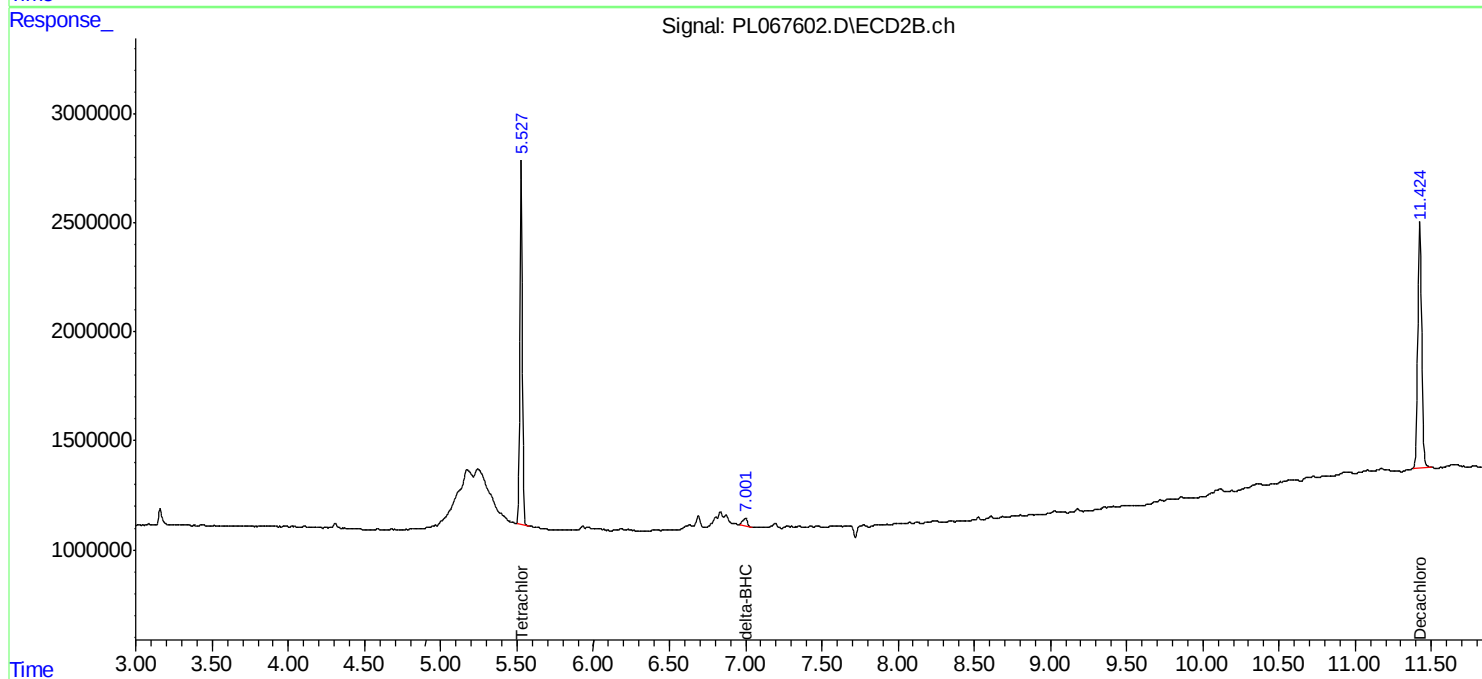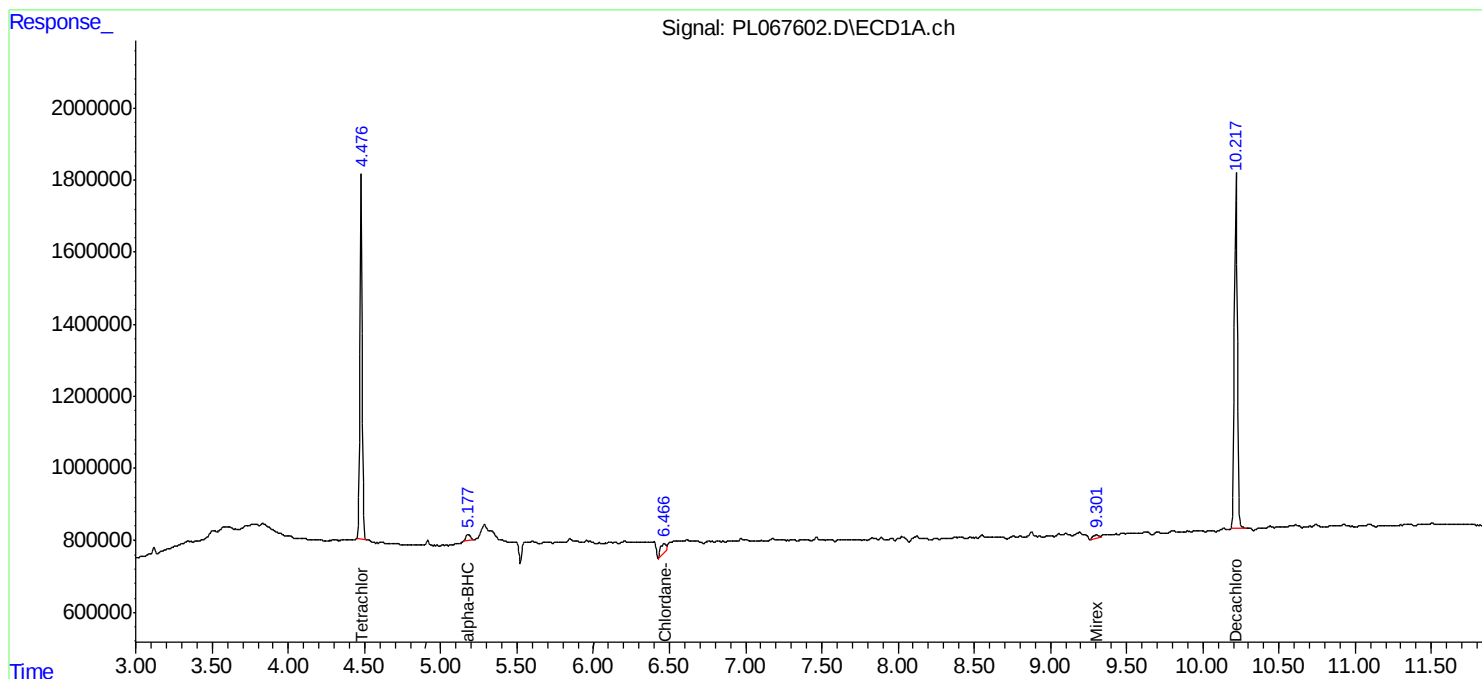


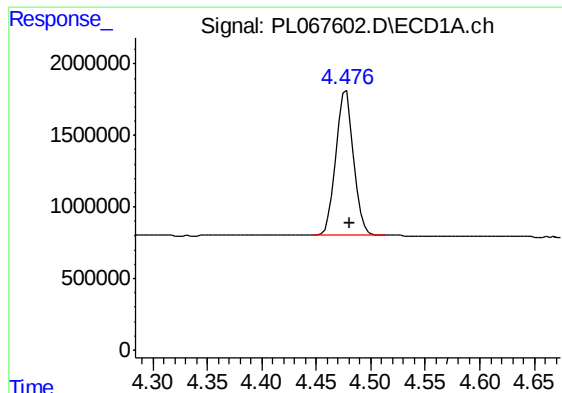

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 11490940
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10-AOC-2

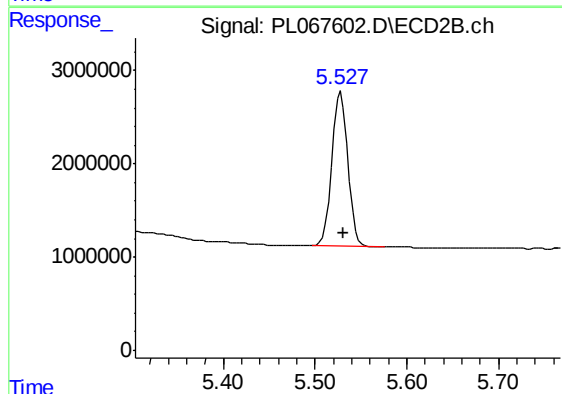


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 20195357
Conc: 21.42 ng/ml

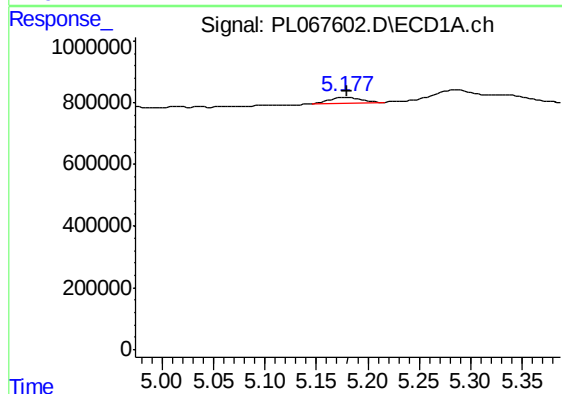


#2 alpha-BHC

R.T.: 5.179 min
Delta R.T.: -0.002 min
Response: 376562
Conc: 0.51 ng/ml

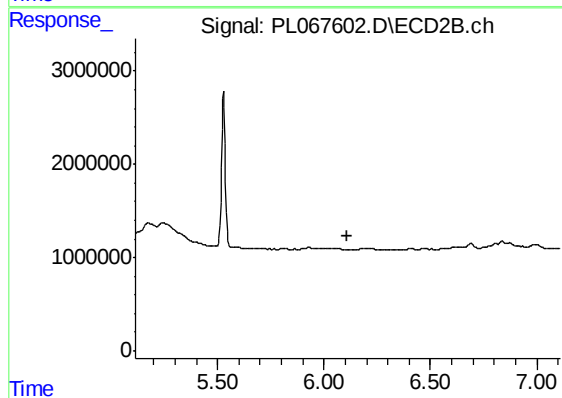

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

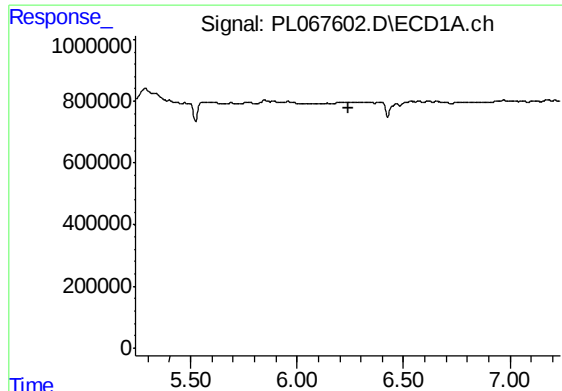

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-10-AOC-2

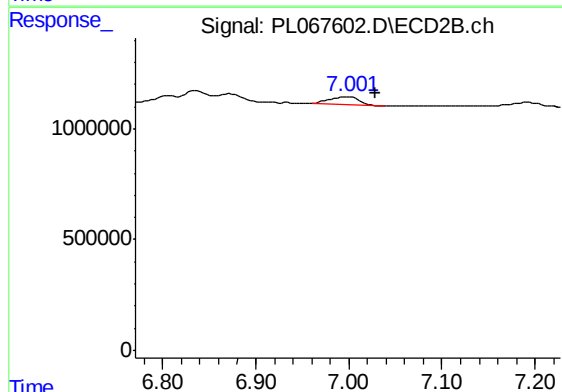


#7 delta-BHC

R.T.: 7.001 min
Delta R.T.: -0.027 min
Response: 791570
Conc: 0.67 ng/ml

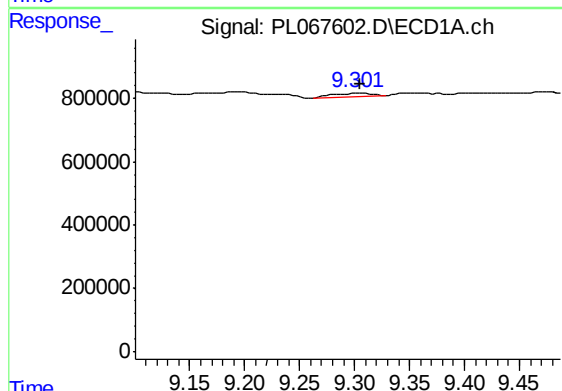


#22 Mirex

R.T.: 9.304 min
Delta R.T.: -0.002 min
Response: 253565
Conc: 0.40 ng/ml

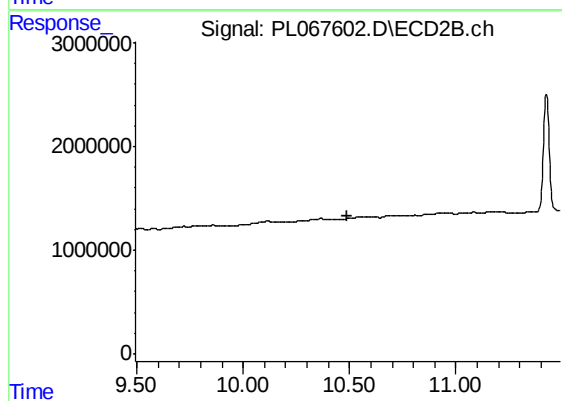

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

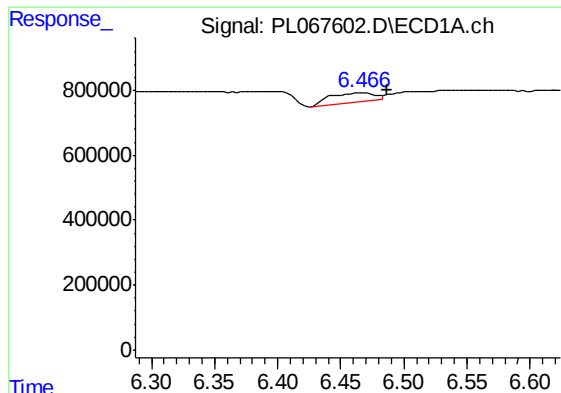

#24 Chlordane-2


R.T.: 6.467 min
Delta R.T.: -0.019 min
Response: 709130
Conc: 26.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10-AOC-2

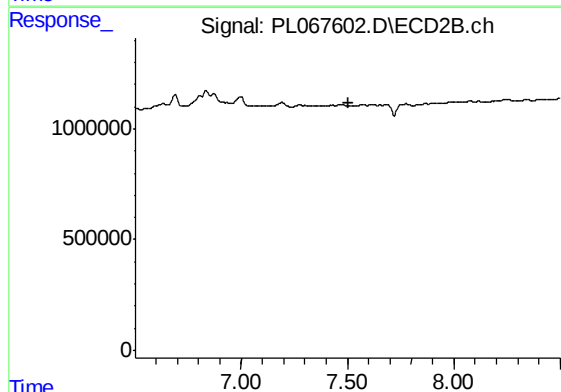


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

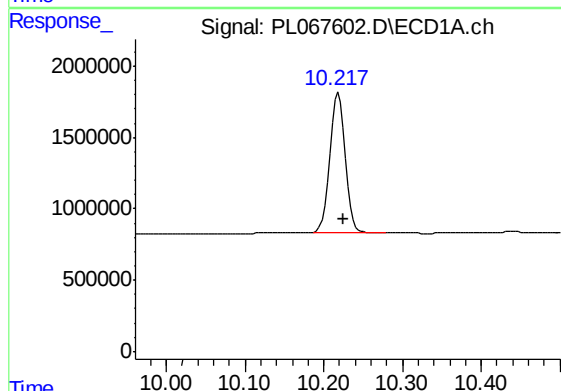

#28 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.006 min
Response: 13506700
Conc: 19.06 ng/ml

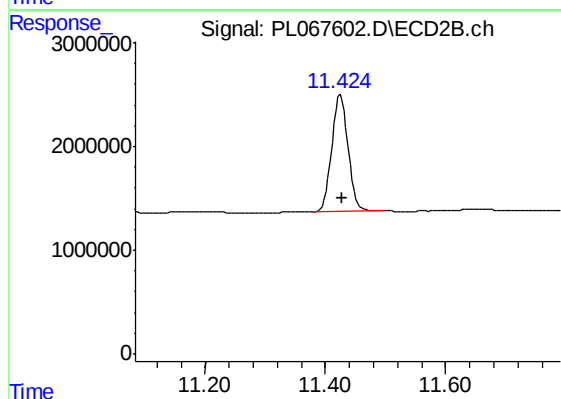

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 21295296
Conc: 21.38 ng/ml