

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 00:19
 Operator : AR\AJ
 Sample : M2736-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-01-061621

Manual Integrations
 APPROVED

Ankita
 6/18/2021 12:13:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:41:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	6992390	12404381	12.718	13.158
28)	SA Decachlor...	10.219	11.425	9233107	15872651	13.029	15.935
Target Compounds							
17)	MA 4,4'-DDT	8.302	9.382	580106	373090	0.997	0.509m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 00:19
Operator : AR\AJ
Sample : M2736-01
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PL-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 12:13:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:41:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

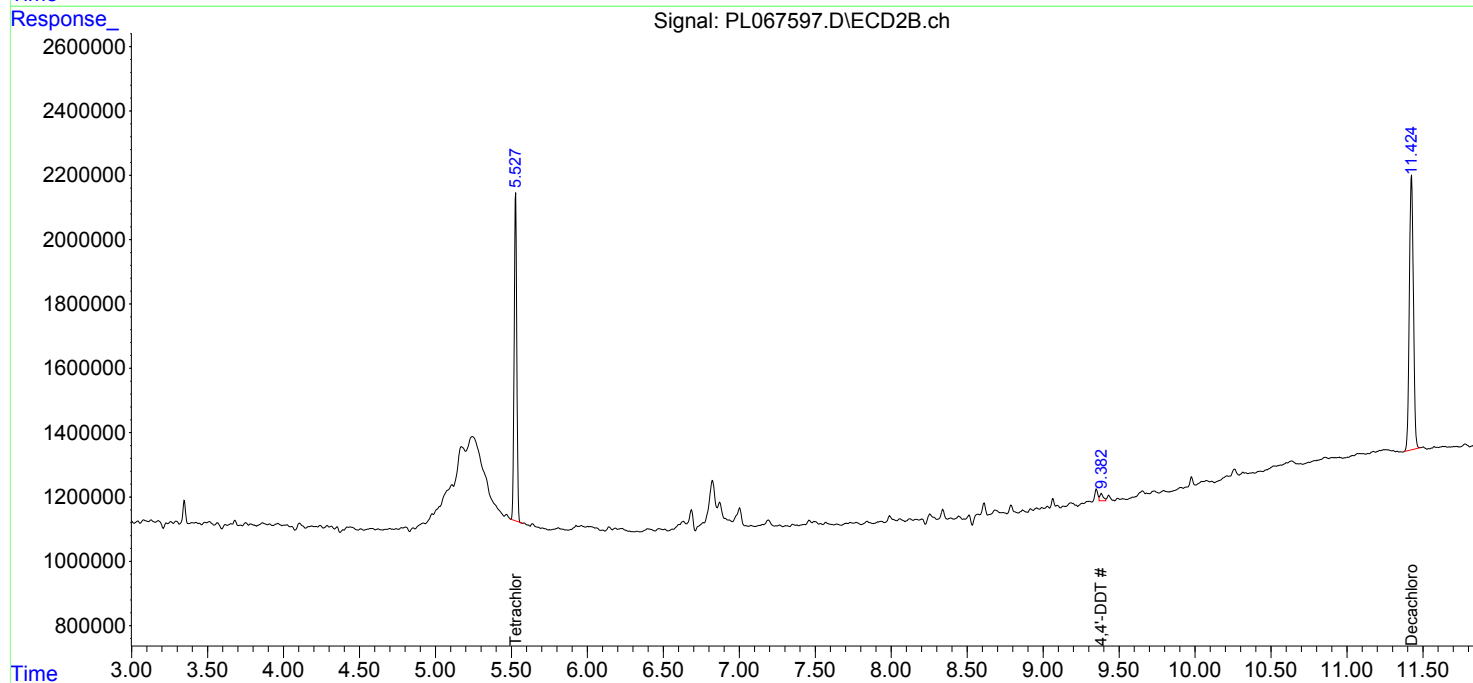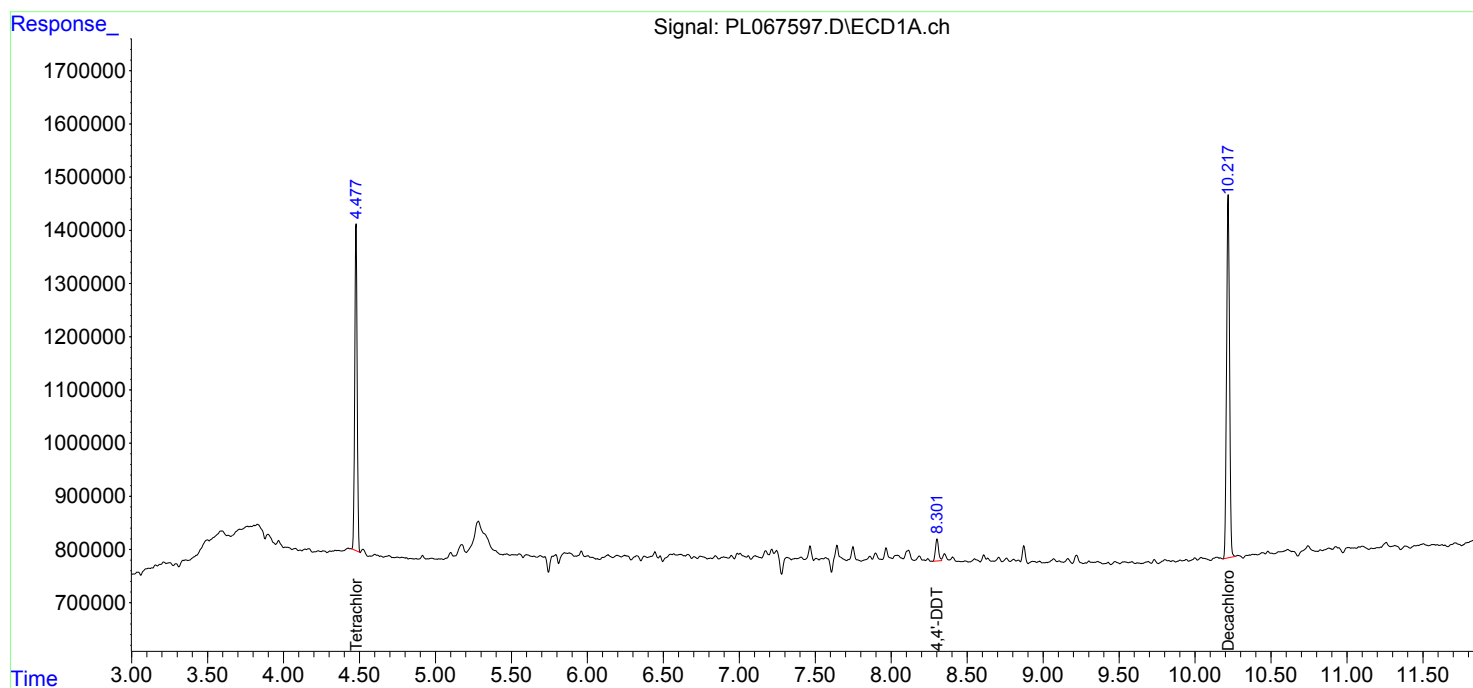

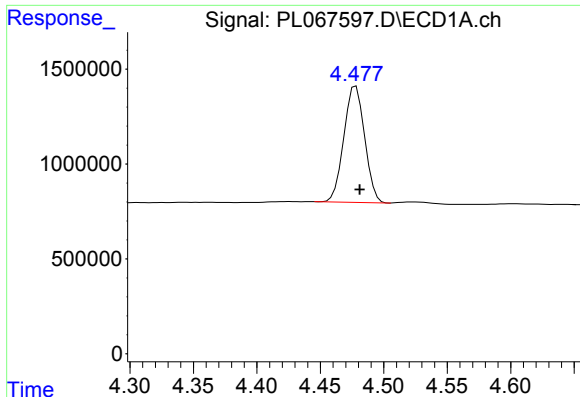


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 6992390
Conc: 12.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 12:13:34 PM

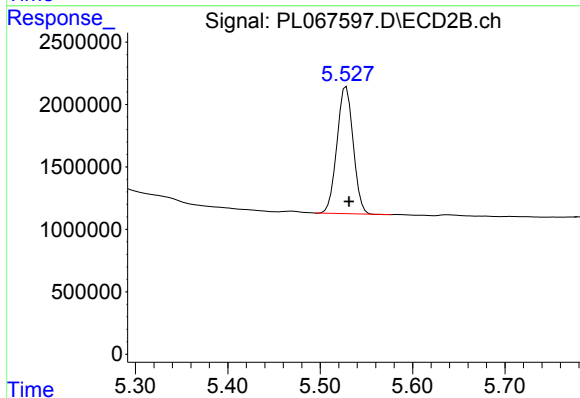


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 12404381
Conc: 13.16 ng/ml

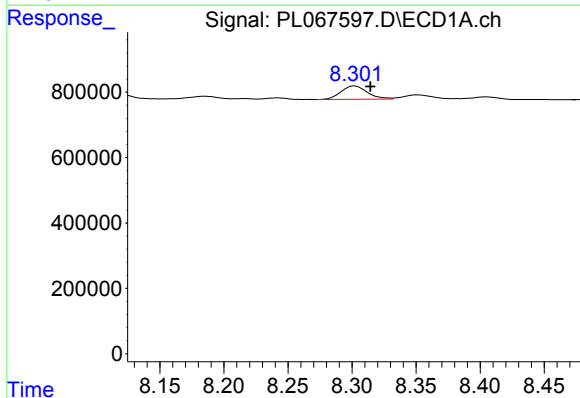


#17 4,4'-DDT

R.T.: 8.302 min
Delta R.T.: -0.012 min
Response: 580106
Conc: 1.00 ng/ml

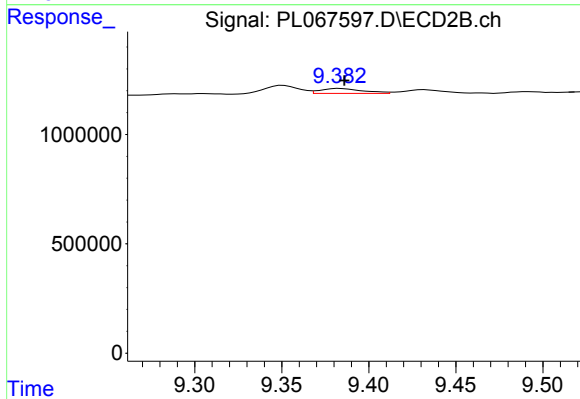

#17 4,4'-DDT

R.T.: 9.382 min
Delta R.T.: -0.004 min
Response: 373090
Conc: 0.51 ng/ml m

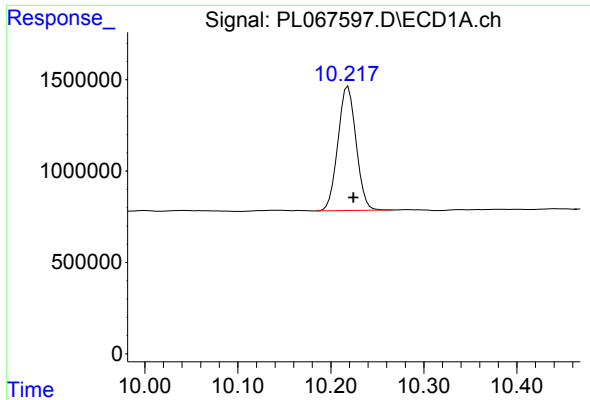


#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 9233107
Conc: 13.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-061621

Manual Integrations
APPROVED

Ankita
6/18/2021 12:13:34 PM

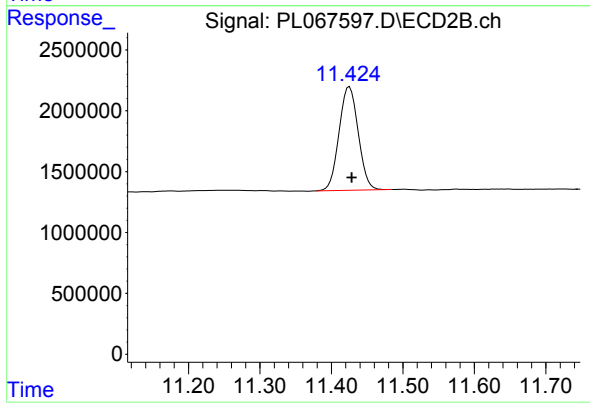

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 15872651
Conc: 15.94 ng/ml