

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 03:38
 Operator : AR\AJ
 Sample : M2719-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-061521

Manual Integrations
 APPROVED

Ankita
 6/18/2021 4:25:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:44:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	6578139	11166431	11.965	11.845
28)	SA Decachlor...	10.219	11.426	8066062	13419400	11.382	13.473
Target Compounds							
10)	B gamma-Chl...	7.177	8.255	253446	452584	0.350m	0.448m#
11)	B alpha-Chl...	7.246	8.339	325744	640423	0.445m	0.634 #
12)	B 4,4'-DDE	7.467	8.522	495905	355113	0.745	0.392 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 03:38
Operator : AR\AJ
Sample : M2719-01
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
OK-03-061521


Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:44:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

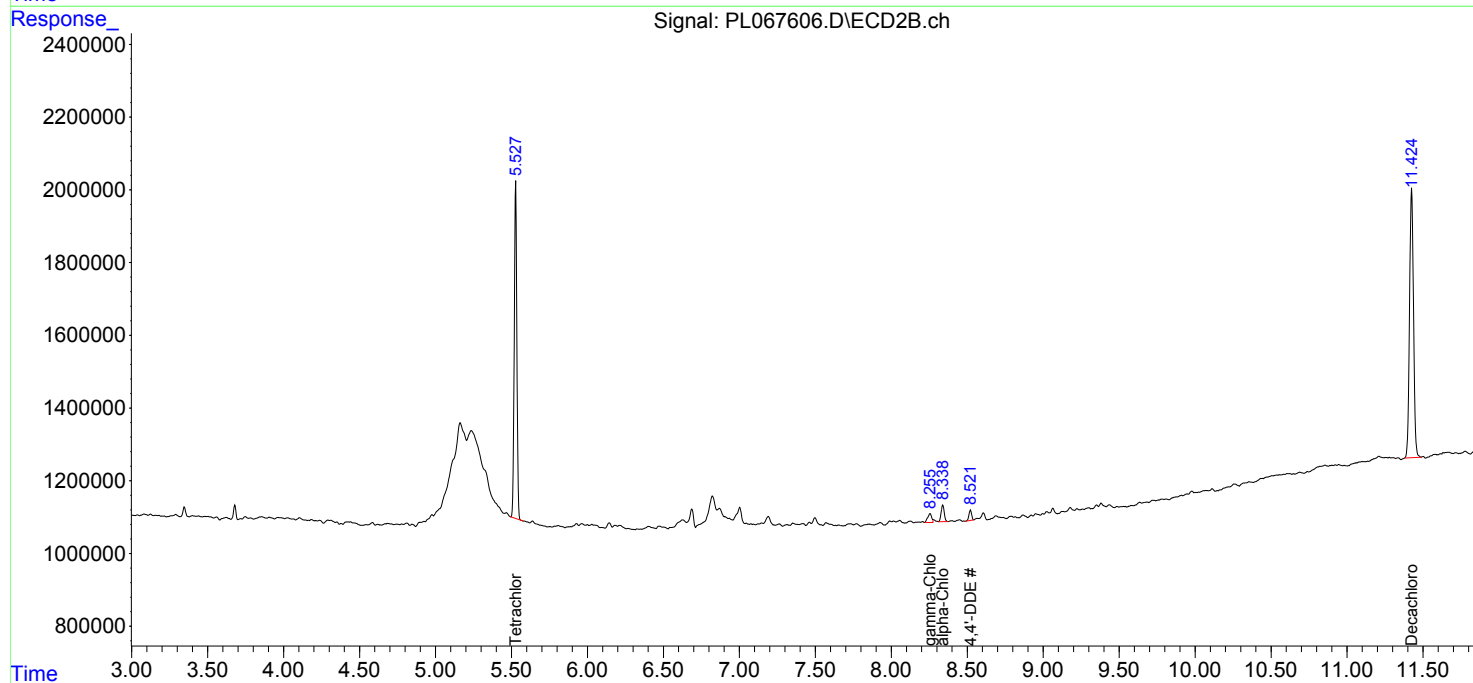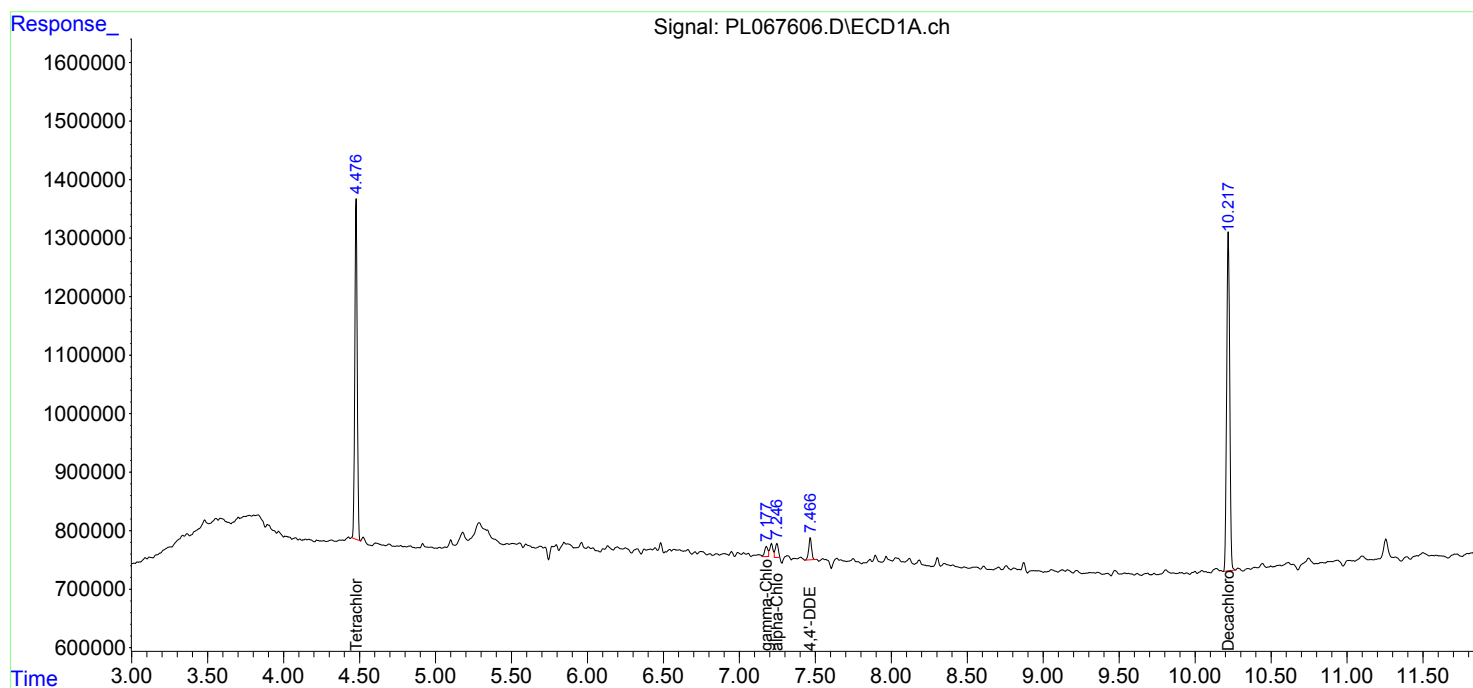

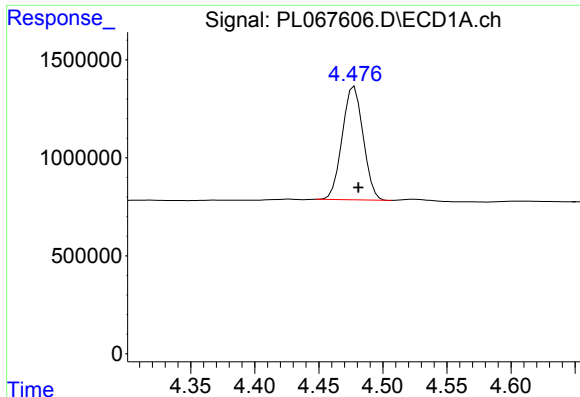


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 6578139
Conc: 11.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061521


Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:05 PM

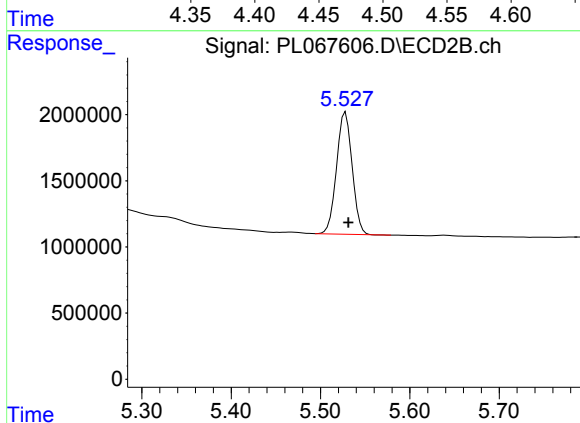


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 11166431
Conc: 11.84 ng/ml

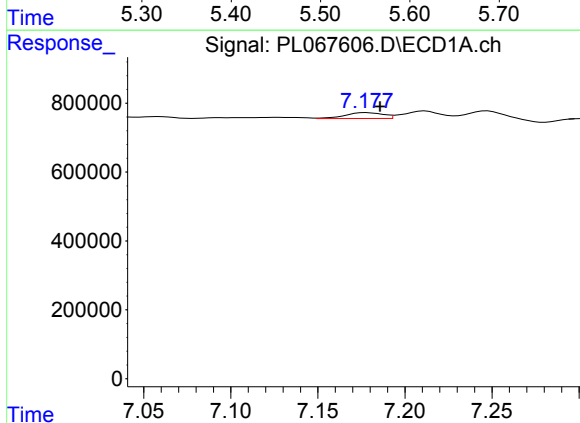


#10 gamma-Chlordane

R.T.: 7.177 min
Delta R.T.: -0.009 min
Response: 253446
Conc: 0.35 ng/ml m

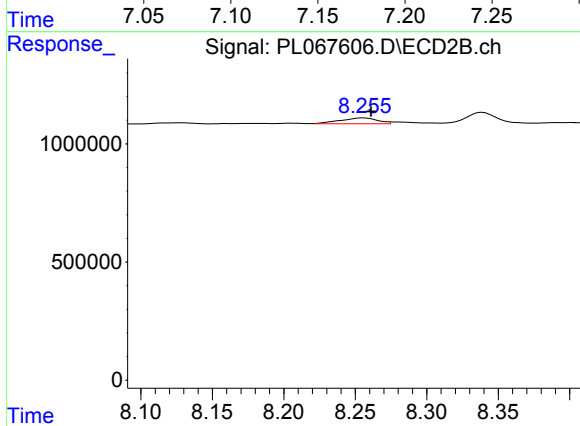

#10 gamma-Chlordane

R.T.: 8.255 min
Delta R.T.: -0.006 min
Response: 452584
Conc: 0.45 ng/ml m

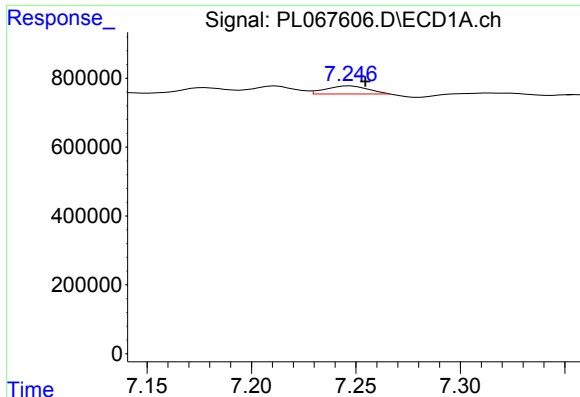


#11 alpha-Chlordane

R.T.: 7.246 min
Delta R.T.: -0.008 min
Response: 325744
Conc: 0.44 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-03-061521


Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:05 PM

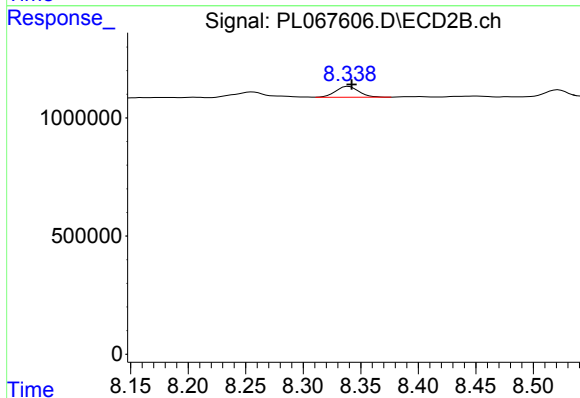


#11 alpha-Chlordane

R.T.: 8.339 min
Delta R.T.: -0.003 min
Response: 640423
Conc: 0.63 ng/ml

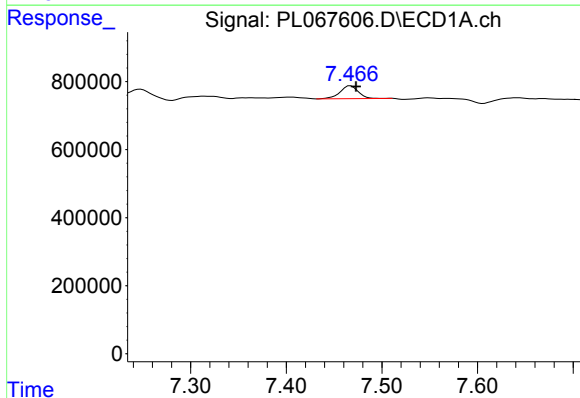


#12 4,4'-DDE

R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 495905
Conc: 0.75 ng/ml

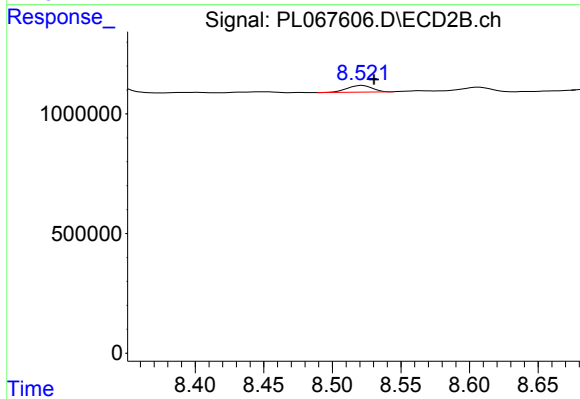

#12 4,4'-DDE

R.T.: 8.522 min
Delta R.T.: -0.008 min
Response: 355113
Conc: 0.39 ng/ml

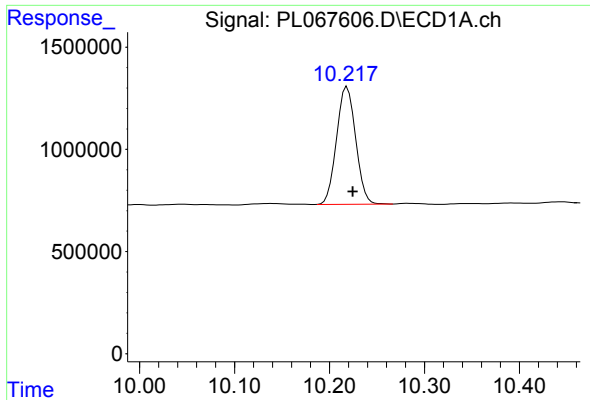


#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 8066062
Conc: 11.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061521

Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:05 PM

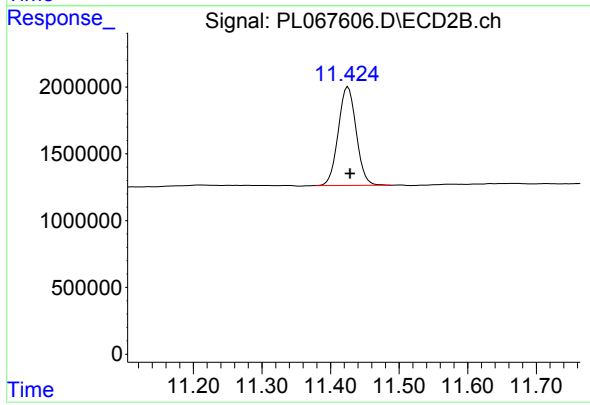

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 13419400
Conc: 13.47 ng/ml