

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
 Data File : PL067607.D
 Signal(s) : ECD2B.ch
 Acq On : 18 Jun 21 03:55 am
 Operator : AR\AJ
 Sample : M2738-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-061621

Manual Integrations
 APPROVED

Ankita
 6/18/2021 4:25:07 PM

Integration File: autoint1.e
 Quant Time: Jun 18 04:44:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	5419855	8764589	9.858	9.297
28)	SA Decachlor...	10.219	11.426	6973196	11100346	9.840	11.144
Target Compounds							
10)	B gamma-Chl...	7.179	8.257	2648585	4116632	3.653m	4.077
11)	B alpha-Chl...	7.248	8.340	2676894	7265153	3.656	7.196 #
12)	B 4,4'-DDE	7.466	8.523	418516	744769	0.629m	0.822 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061721\
Data File : PL067607.D
Signal(s) : ECD2B.ch
Acq On : 18 Jun 21 03:55 am
Operator : AR\AJ
Sample : M2738-01
Misc :
ALS Vial : 47 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
HD-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:07 PM

Integration File: autoint1.e
Quant Time: Jun 18 04:44:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

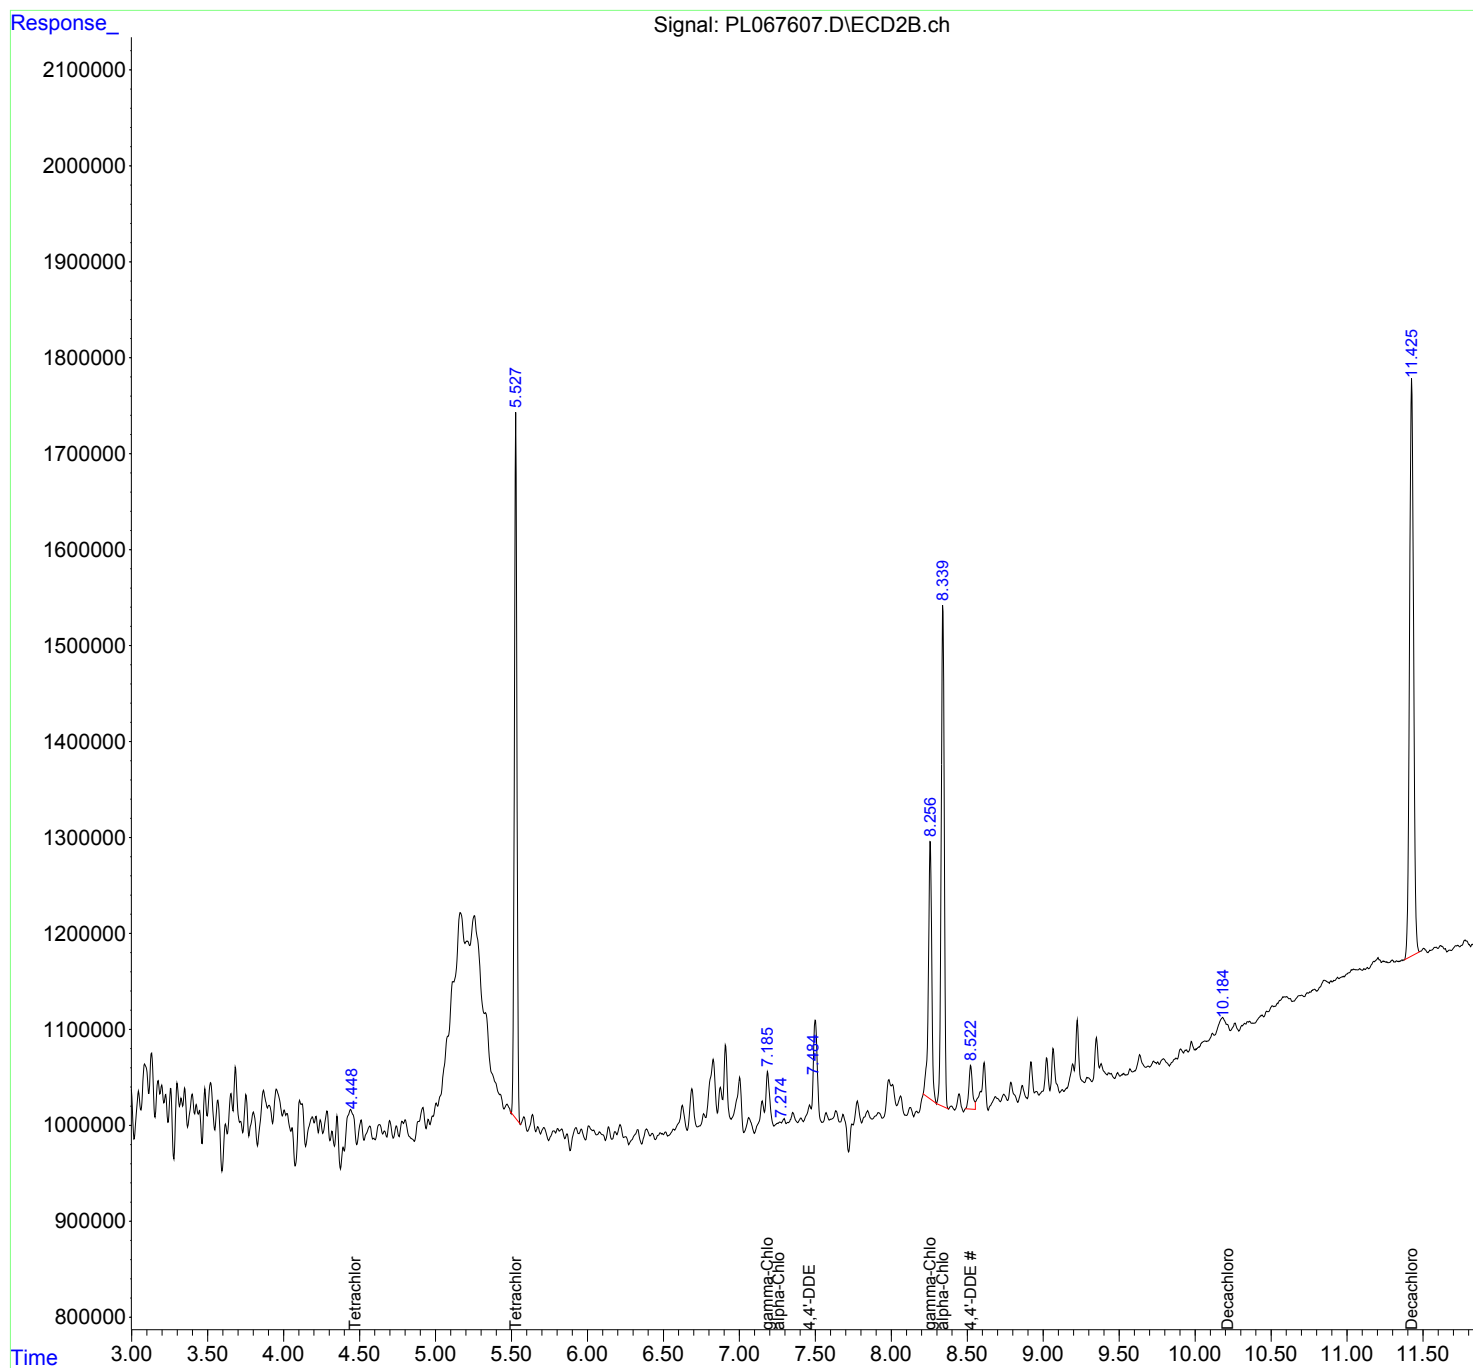

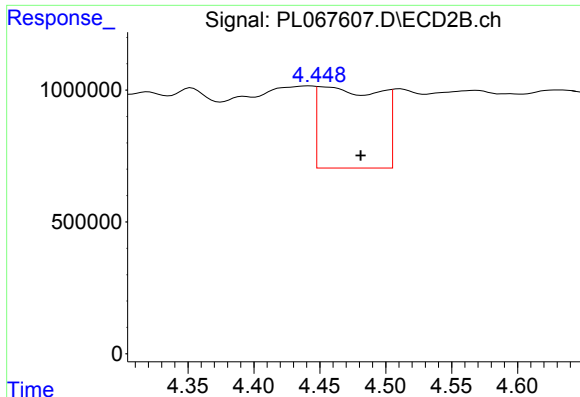


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 5419855
Conc: 9.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:07 PM

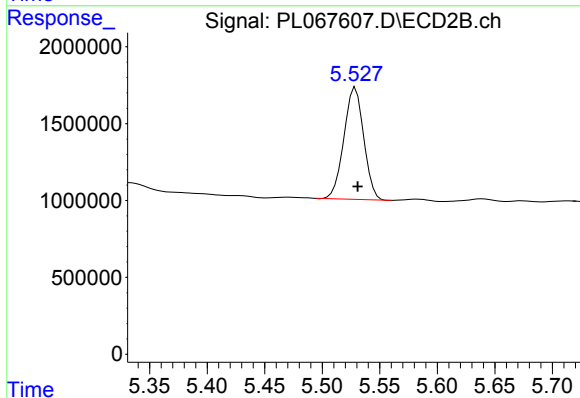


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 8764589
Conc: 9.30 ng/ml

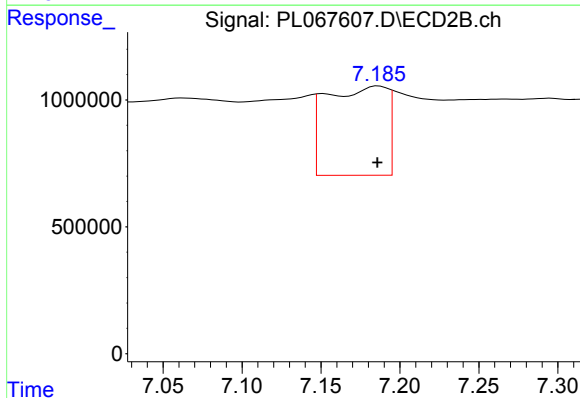


#10 gamma-Chlordane

R.T.: 7.179 min
Delta R.T.: -0.007 min
Response: 2648585
Conc: 3.65 ng/ml m

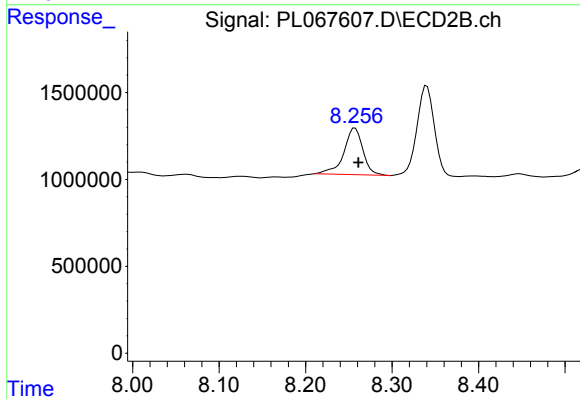

#10 gamma-Chlordane

R.T.: 8.257 min
Delta R.T.: -0.004 min
Response: 4116632
Conc: 4.08 ng/ml

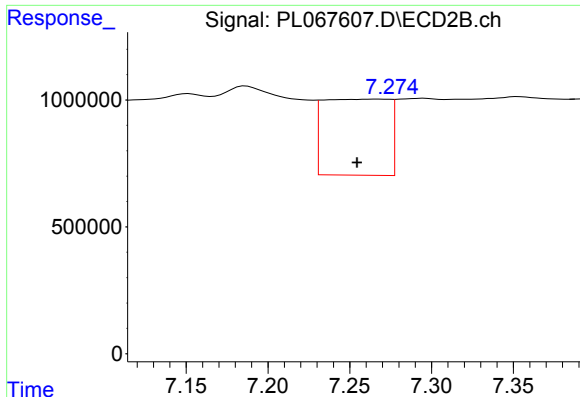


#11 alpha-Chlordane

R.T.: 7.248 min
Delta R.T.: -0.007 min
Response: 2676894
Conc: 3.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:07 PM

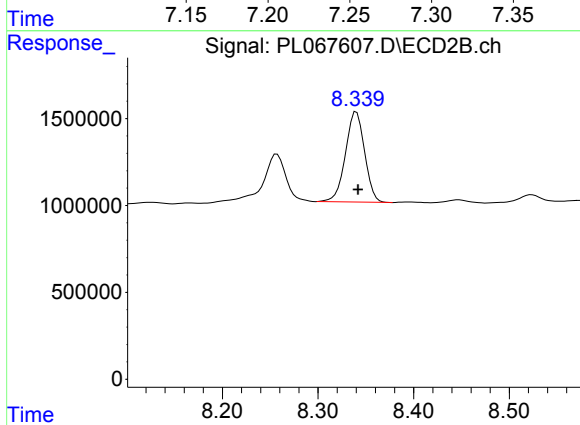


#11 alpha-Chlordane

R.T.: 8.340 min
Delta R.T.: -0.002 min
Response: 7265153
Conc: 7.20 ng/ml

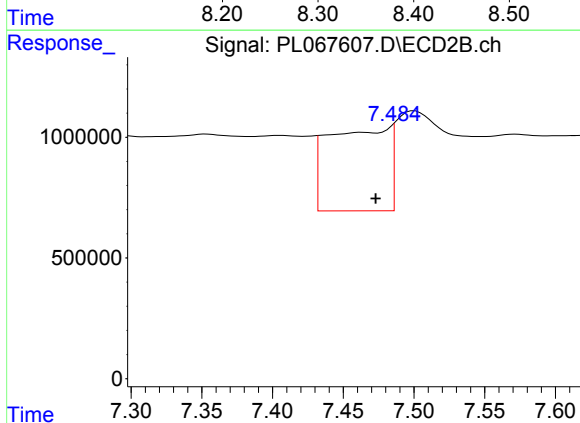


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 418516
Conc: 0.63 ng/ml m

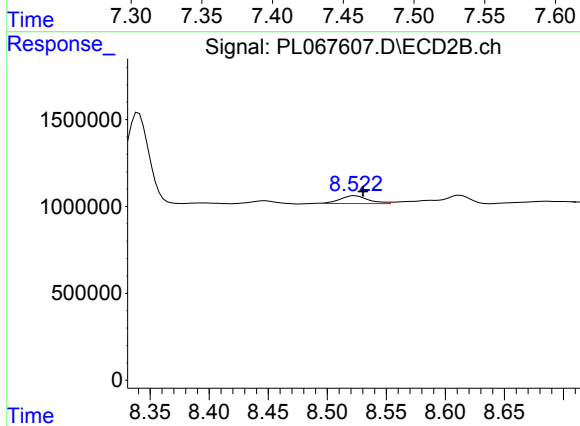

#12 4,4'-DDE

R.T.: 8.523 min
Delta R.T.: -0.007 min
Response: 744769
Conc: 0.82 ng/ml

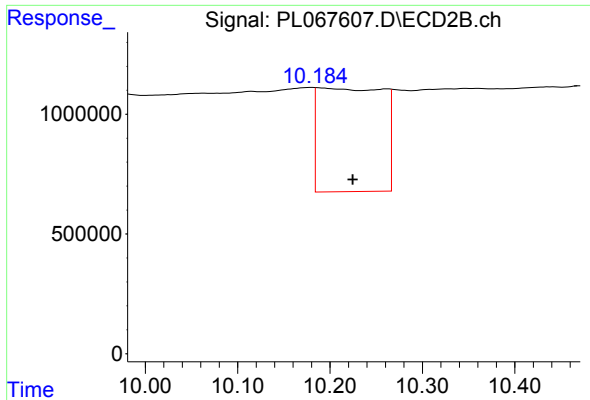


#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 6973196
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-061621

Manual Integrations
APPROVED

Ankita
6/18/2021 4:25:07 PM

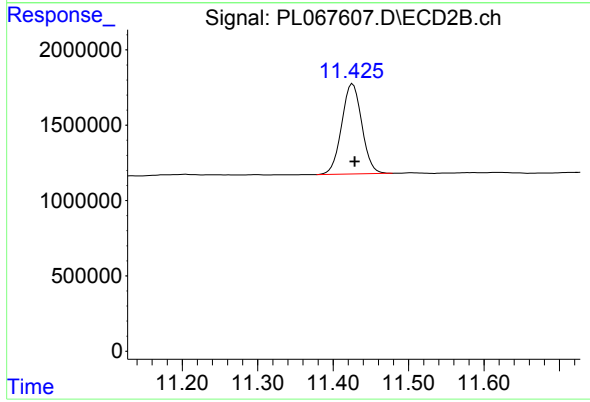

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 11100346
Conc: 11.14 ng/ml