

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
 Data File : PL075832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2022 09:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 22:25:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.637	14882359	36488329	22.052	21.743
28)	SA Decachlor...	11.641	10.380	13292478	28245186	21.712	20.047
Target Compounds							
7)	B delta-BHC	0.000	6.399	0	470917	N.D.	0.220 #
9)	A Endosulfan I	8.534	0.000	97738	0	0.140	N.D. #
10)	B gamma-Chl...	8.385	0.000	960103	0	1.236	N.D. #
11)	B alpha-Chl...	0.000	7.386f	0	344284	N.D.	0.189 #
14)	MA Endrin	0.000	8.063f	0	421724	N.D.	0.308 #
15)	B Endosulfa...	9.305	0.000	399868	0	0.643	N.D. #
21)	B Endrin ke...	10.187f	0.000	813175	0	1.156	N.D. #
23)	Chlordane-1	0.000	5.977f	0	831239	N.D.	15.122 #
25)	Chlordane-3	8.385	0.000	960103	0	9.299	N.D. #
26)	Chlordane-4	0.000	7.386f	0	344284	N.D.	1.870 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
Data File : PL075832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2022 09:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 22:25:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

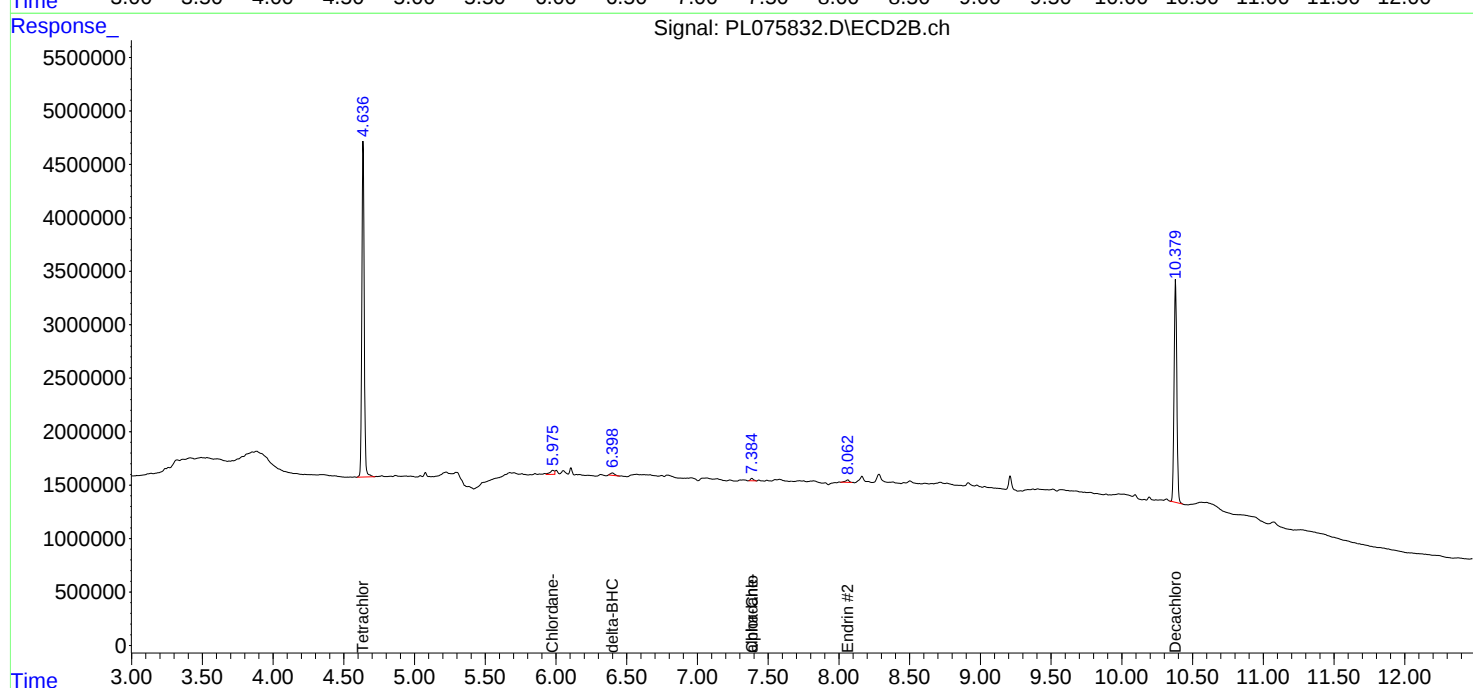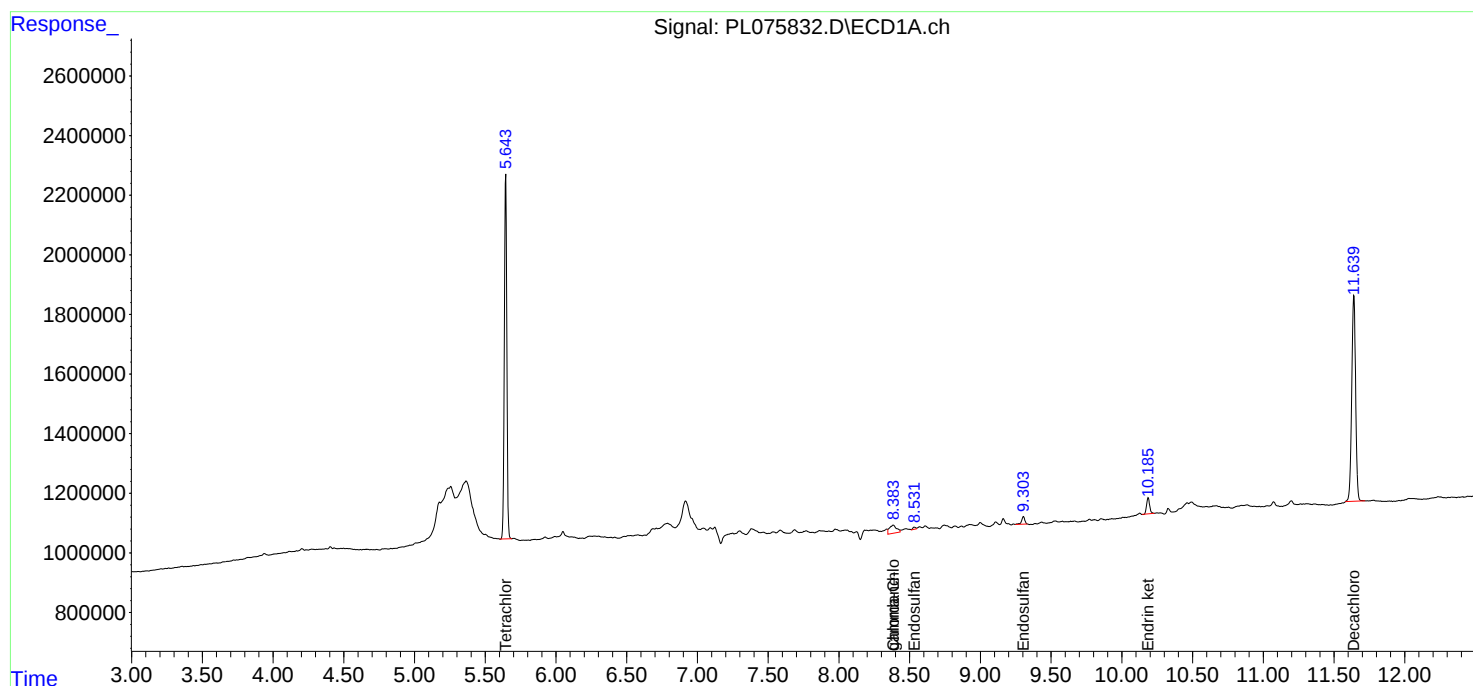


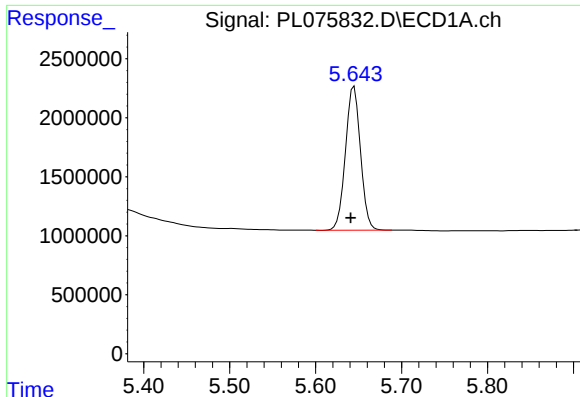

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: 0.004 min
Response: 14882359
Conc: 22.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

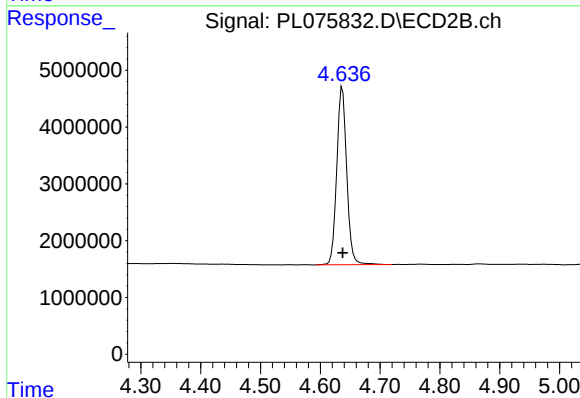


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 36488329
Conc: 21.74 ng/ml

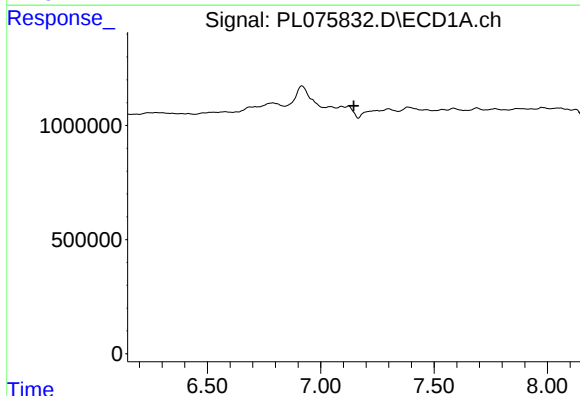


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

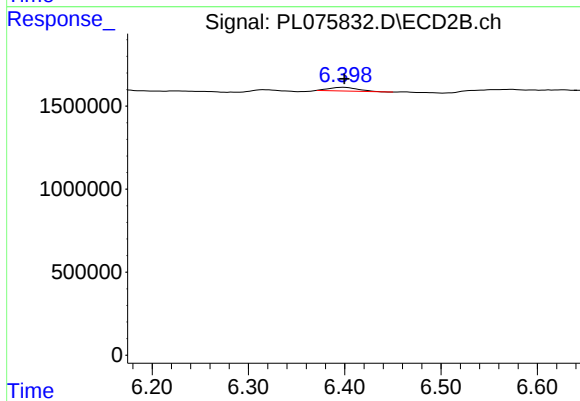

#7 delta-BHC


R.T.: 6.399 min
Delta R.T.: -0.001 min
Response: 470917
Conc: 0.22 ng/ml

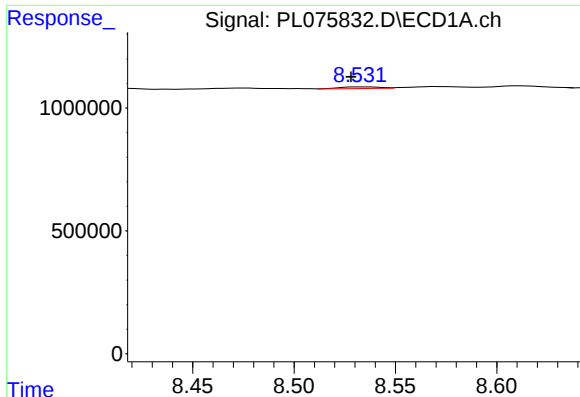

#9 Endosulfan I


R.T.: 8.534 min
Delta R.T.: 0.006 min
Response: 97738
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

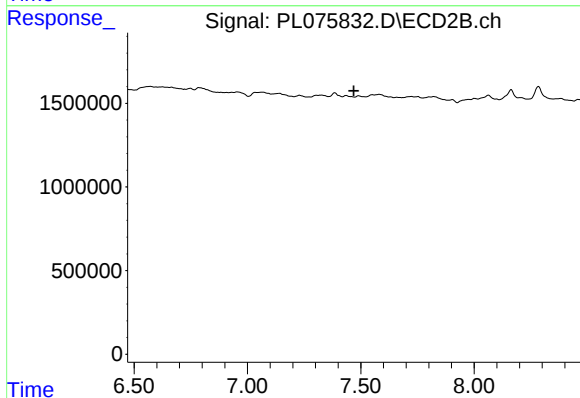


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

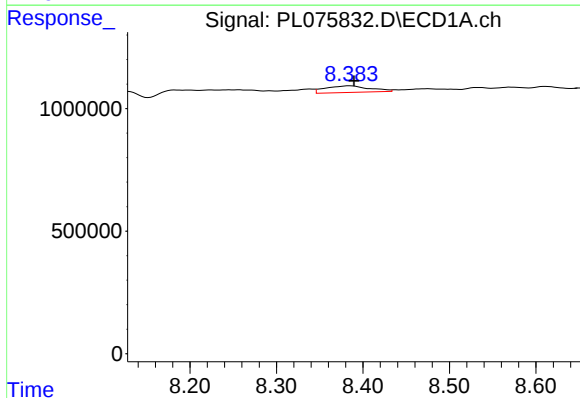


#10 gamma-Chlordane

R.T.: 8.385 min
Delta R.T.: -0.005 min
Response: 960103
Conc: 1.24 ng/ml

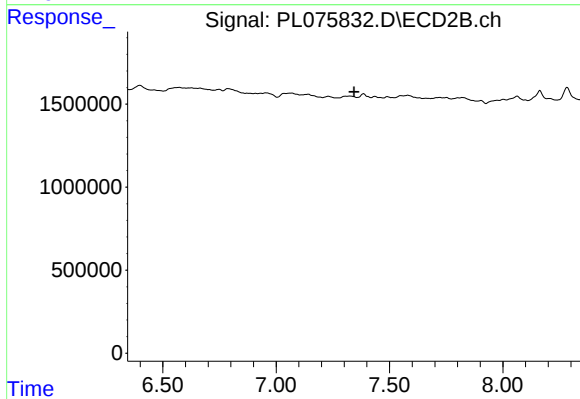

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

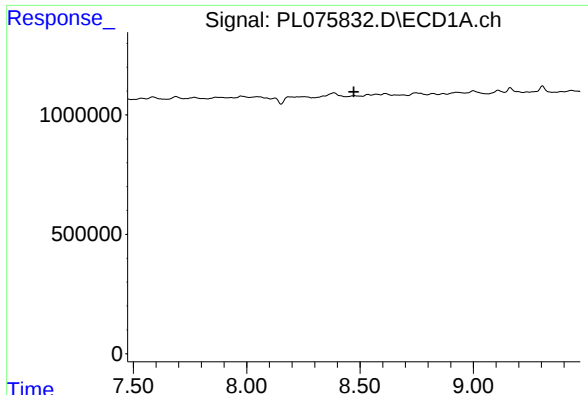

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

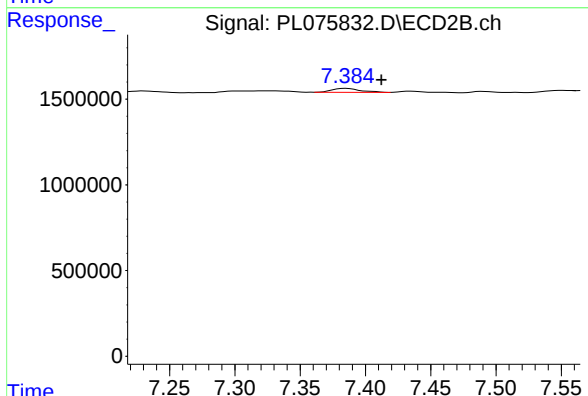


#11 alpha-Chlordane

R.T.: 7.386 min
Delta R.T.: -0.027 min
Response: 344284
Conc: 0.19 ng/ml

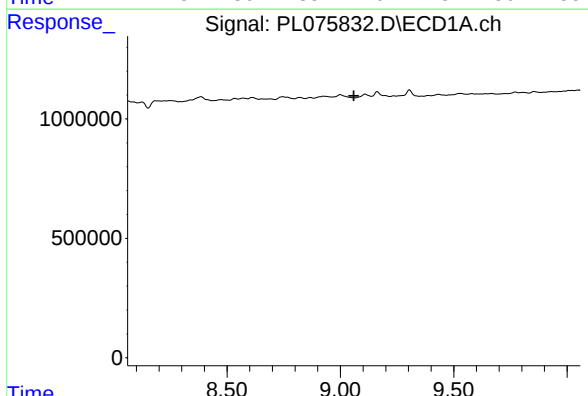


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

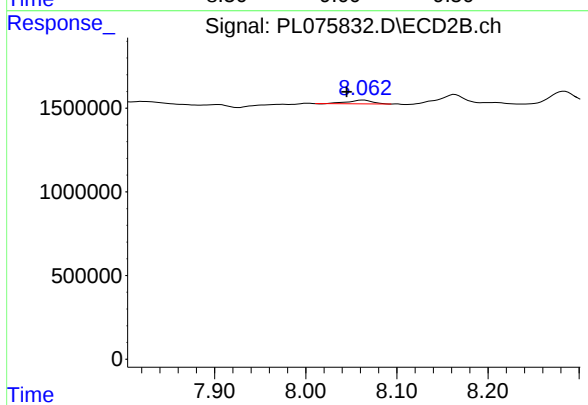

#14 Endrin


R.T.: 8.063 min
Delta R.T.: 0.018 min
Response: 421724
Conc: 0.31 ng/ml

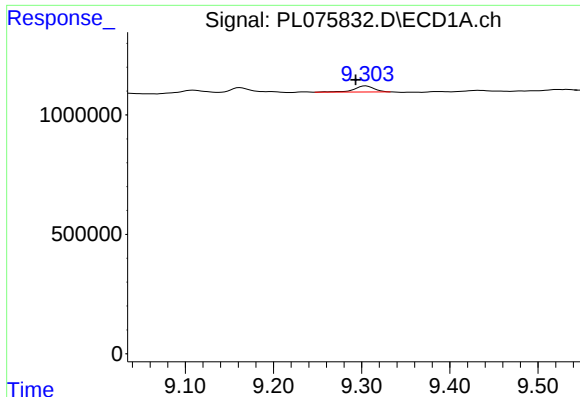

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.011 min
Response: 399868
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

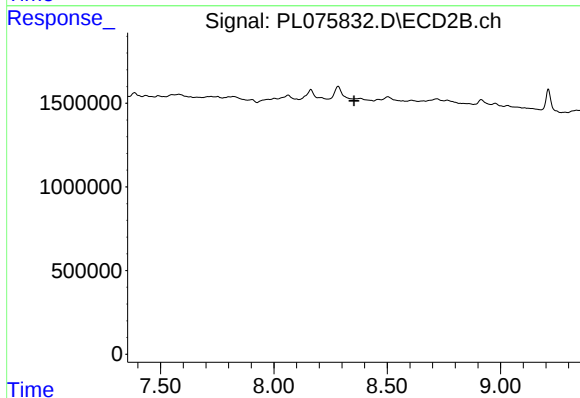


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

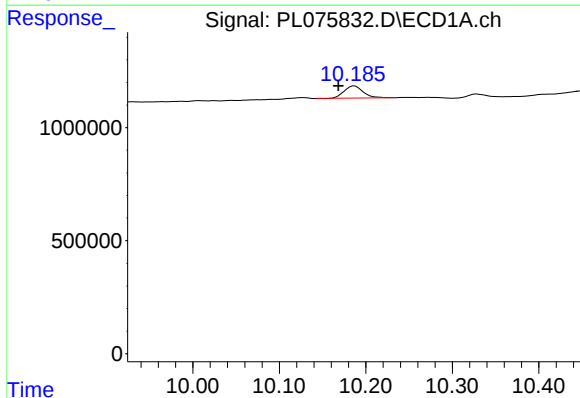


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.019 min
Response: 813175
Conc: 1.16 ng/ml

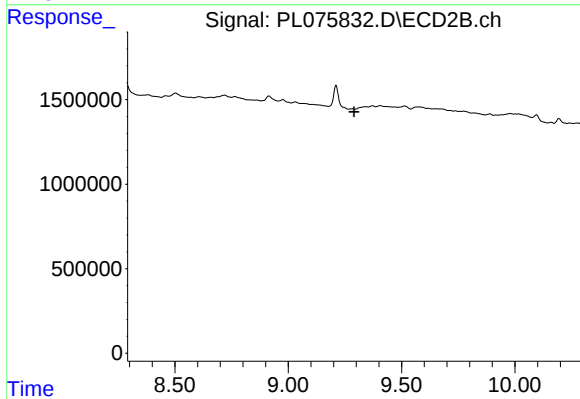

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

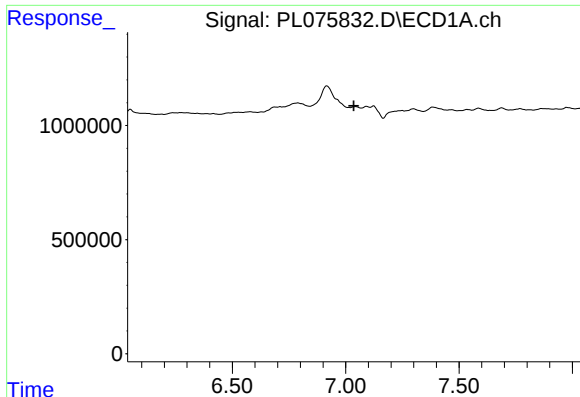

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 7.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

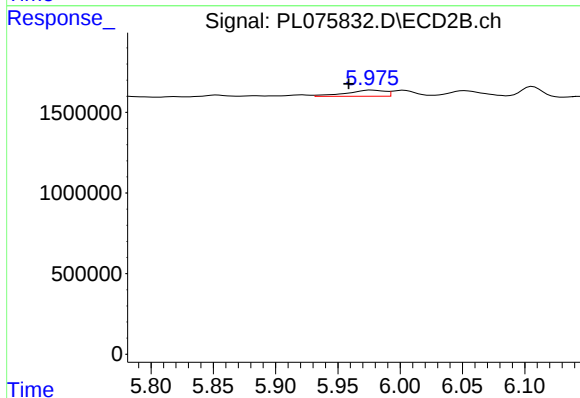


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: 0.018 min
Response: 831239
Conc: 15.12 ng/ml

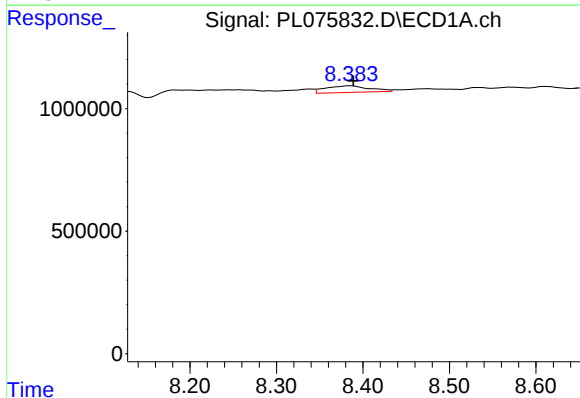


#25 Chlordane-3

R.T.: 8.385 min
Delta R.T.: -0.004 min
Response: 960103
Conc: 9.30 ng/ml

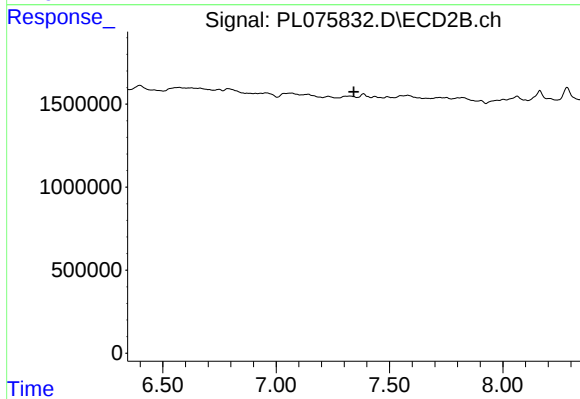

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

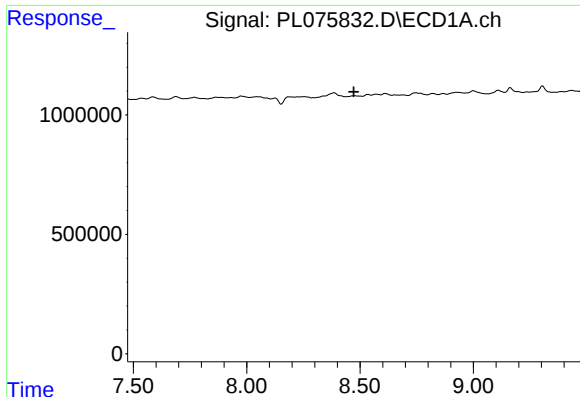

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

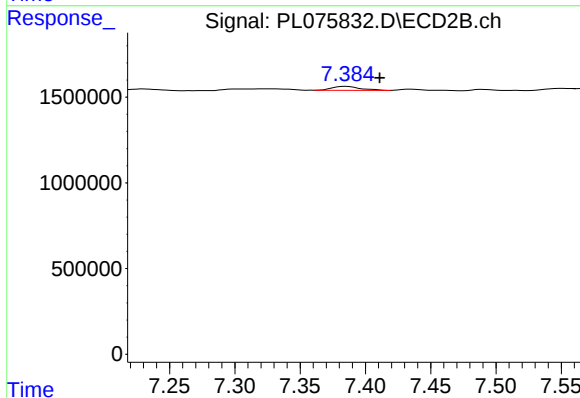


#26 Chlordane-4

R.T.: 7.386 min
Delta R.T.: -0.025 min
Response: 344284
Conc: 1.87 ng/ml

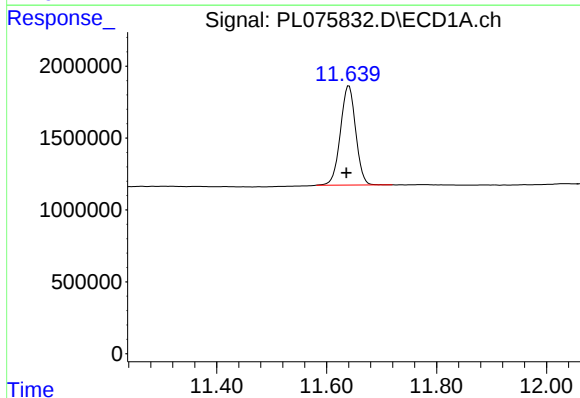

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.004 min
Response: 13292478
Conc: 21.71 ng/ml

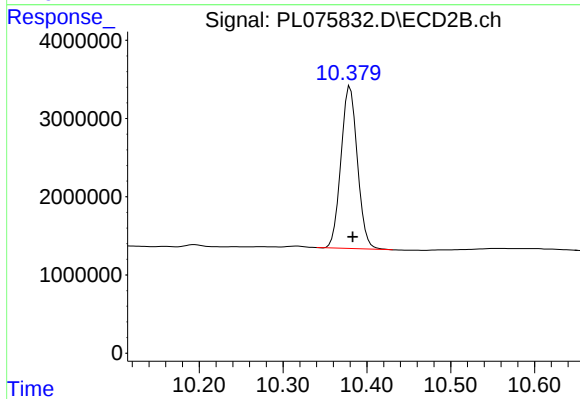

#28 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: -0.003 min
Response: 28245186
Conc: 20.05 ng/ml