

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
 Data File : PL075840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2022 13:25
 Operator : AR\AJ
 Sample : PB145565TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 22:30:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.635	13652172	32892444	20.229	19.600
28)	SA Decachlor...	11.638	10.379	12898979	28115125	21.069	19.955
Target Compounds							
7)	B delta-BHC	0.000	6.401	0	352215	N.D.	0.165 #
9)	A Endosulfan I	8.533	0.000	412308	0	0.589	N.D. #
10)	B gamma-Chl...	8.383	0.000	1084887	0	1.397	N.D. #
11)	B alpha-Chl...	0.000	7.387f	0	242599	N.D.	0.133 #
14)	MA Endrin	0.000	8.062f	0	233939	N.D.	0.171 #
15)	B Endosulfa...	9.305	0.000	228696	0	0.368	N.D. #
21)	B Endrin ke...	10.185f	0.000	548703	0	0.780	N.D. #
25)	Chlordane-3	8.383	0.000	1084887	0	10.507	N.D. #
26)	Chlordane-4	0.000	7.387f	0	242599	N.D.	1.318 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
Data File : PL075840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2022 13:25
Operator : AR\AJ
Sample : PB145565TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 22:30:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

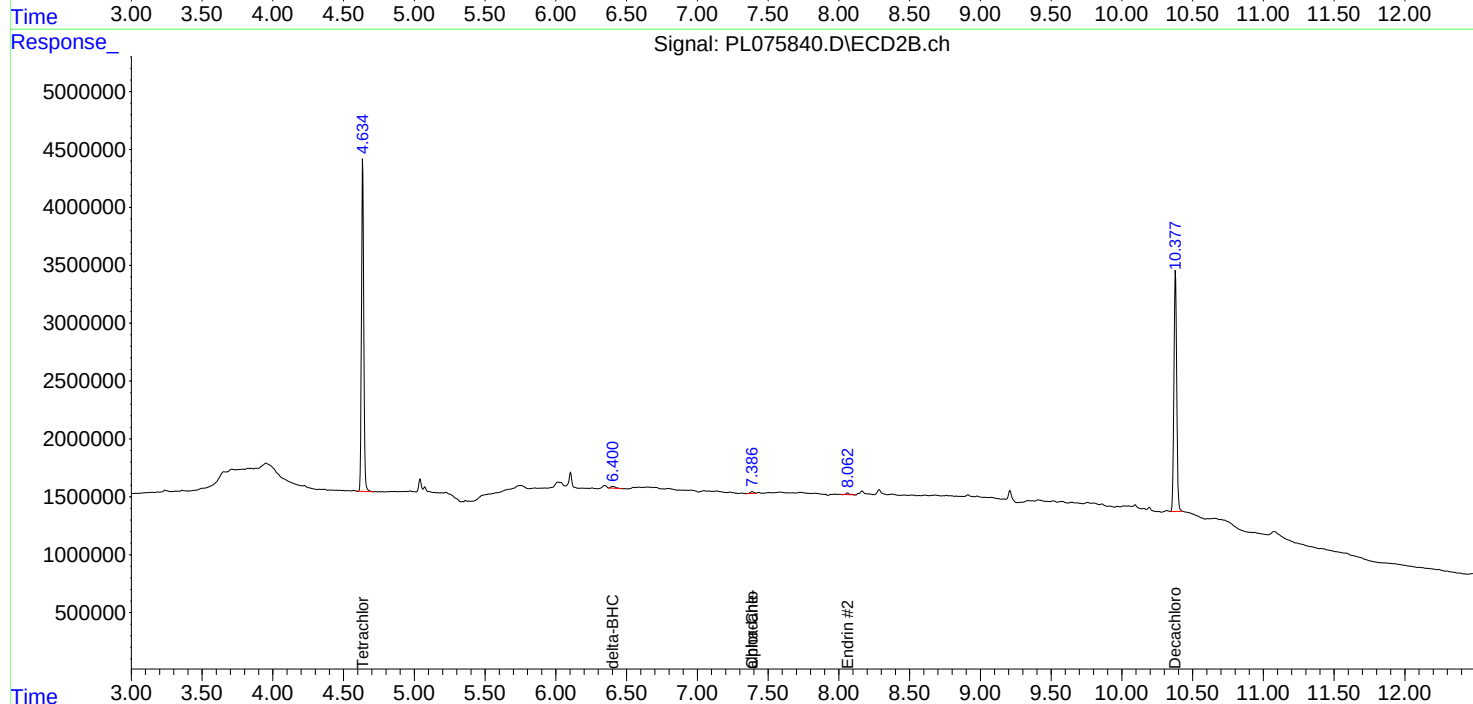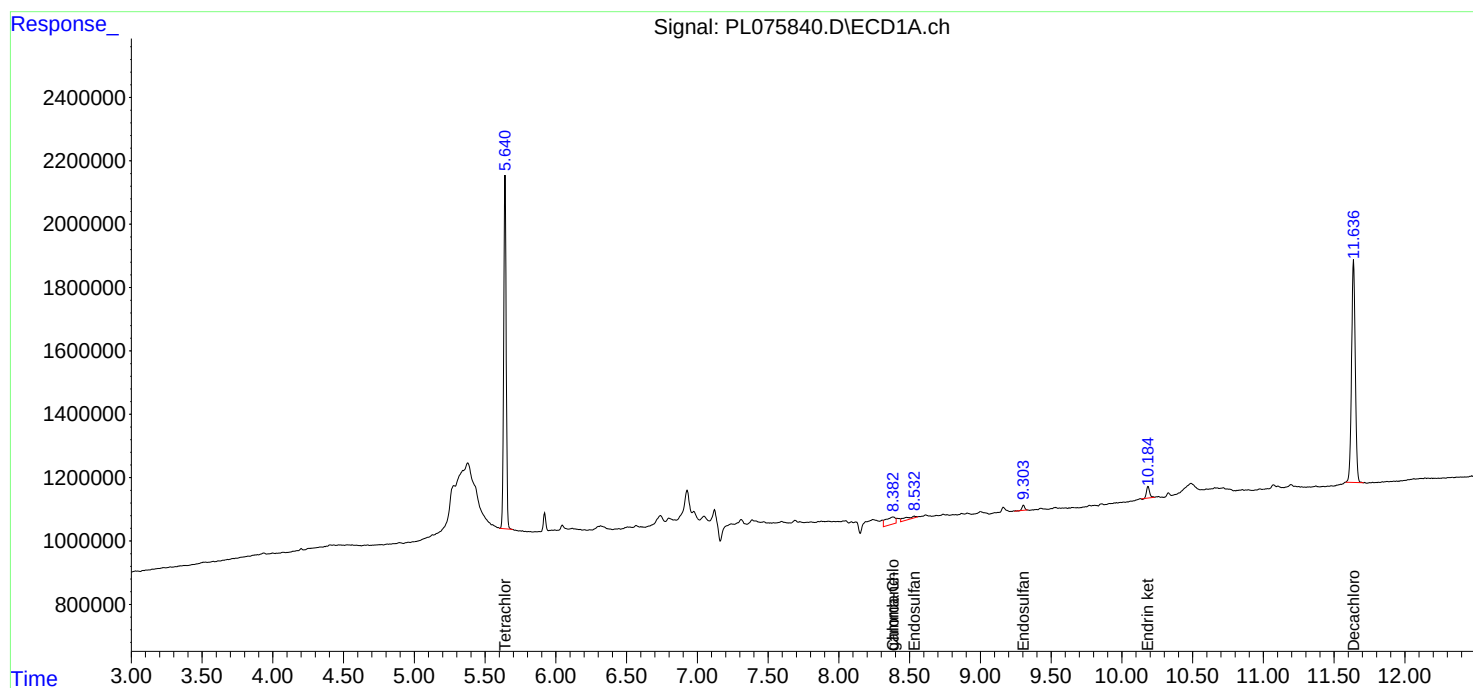


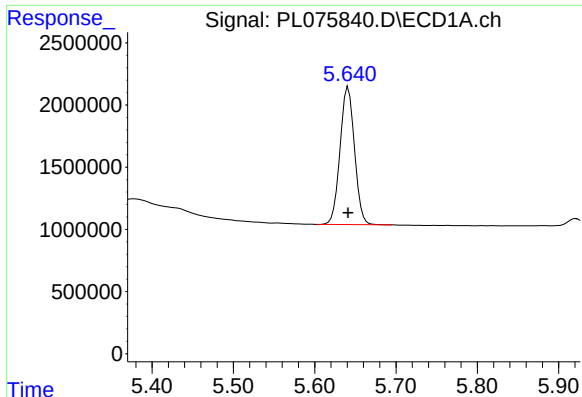

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 13652172
Conc: 20.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

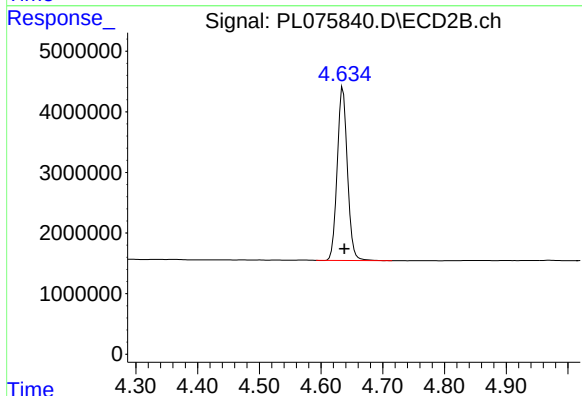


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.002 min
Response: 32892444
Conc: 19.60 ng/ml

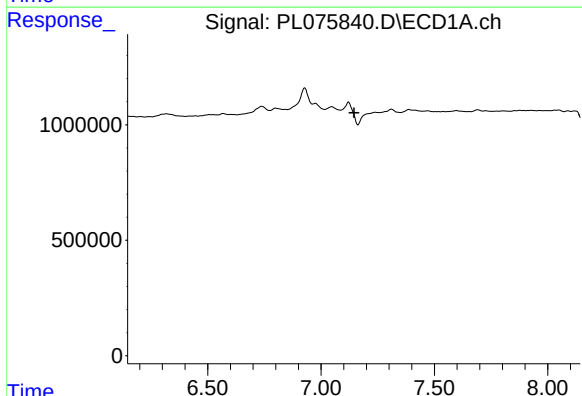


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

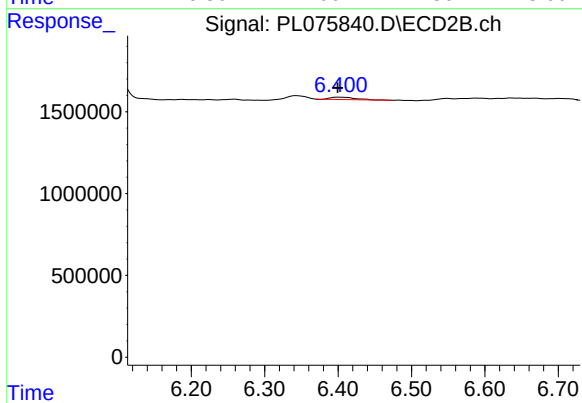

#7 delta-BHC


R.T.: 6.401 min
Delta R.T.: 0.001 min
Response: 352215
Conc: 0.16 ng/ml

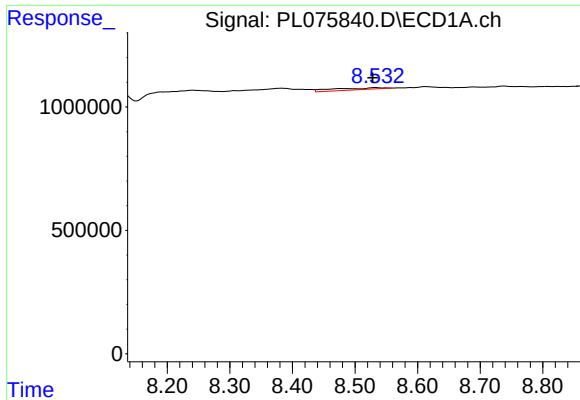

#9 Endosulfan I


R.T.: 8.533 min
Delta R.T.: 0.005 min
Response: 412308
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

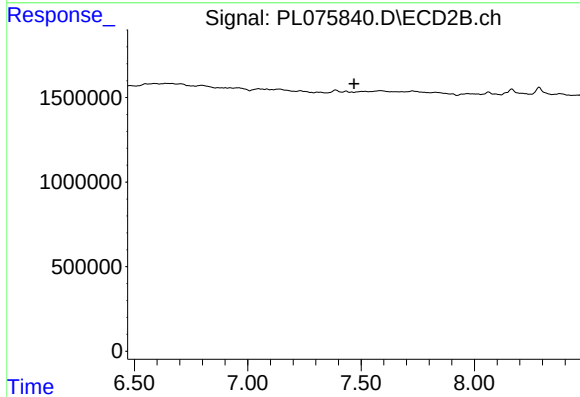


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

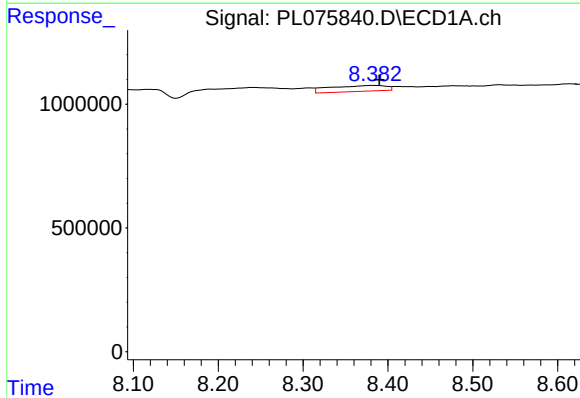


#10 gamma-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1084887
Conc: 1.40 ng/ml

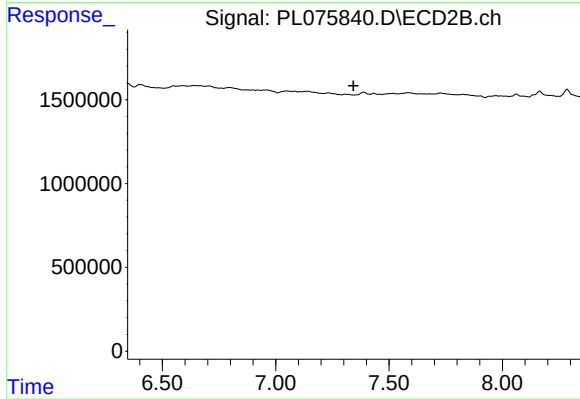

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

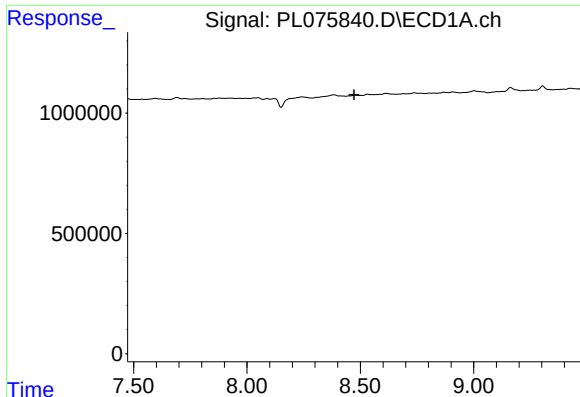

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

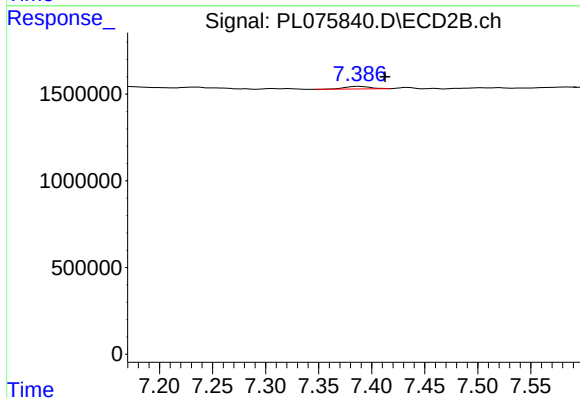


#11 alpha-Chlordane

R.T.: 7.387 min
Delta R.T.: -0.025 min
Response: 242599
Conc: 0.13 ng/ml

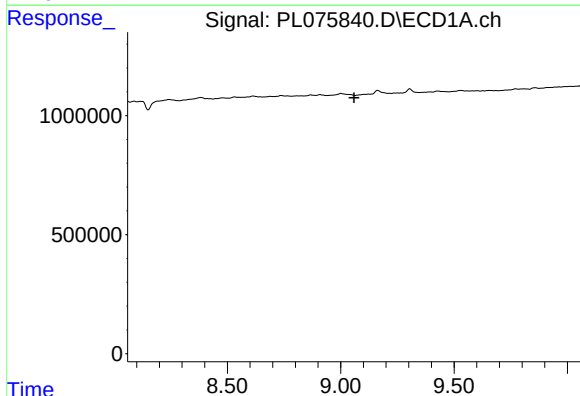


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

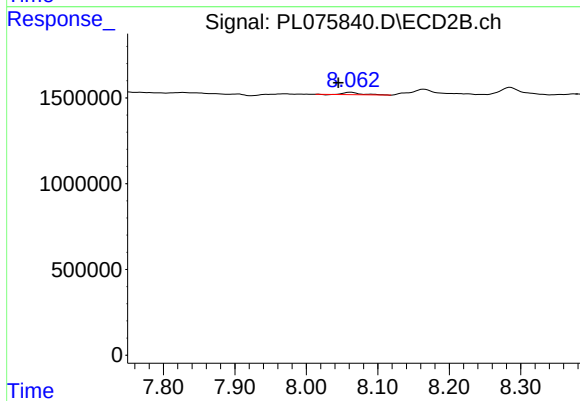

#14 Endrin


R.T.: 8.062 min
Delta R.T.: 0.017 min
Response: 233939
Conc: 0.17 ng/ml

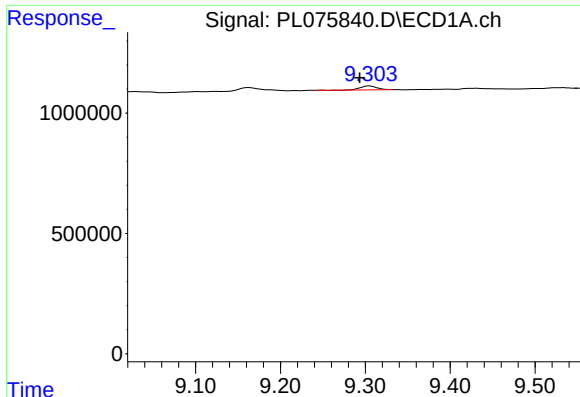

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.011 min
Response: 228696
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

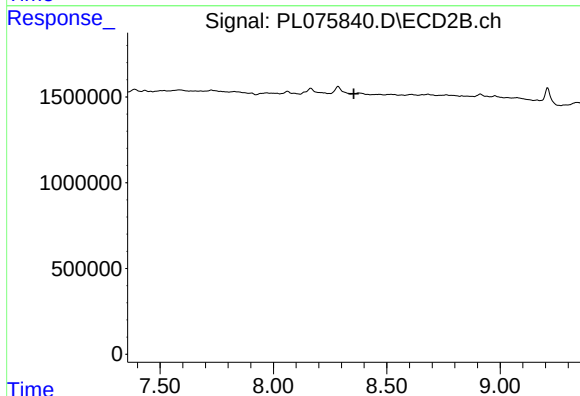


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

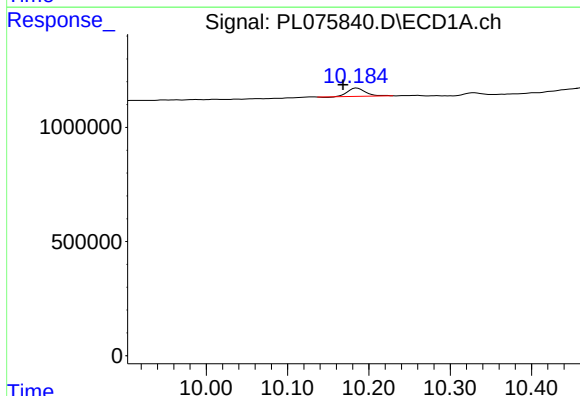


#21 Endrin ketone

R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 548703
Conc: 0.78 ng/ml

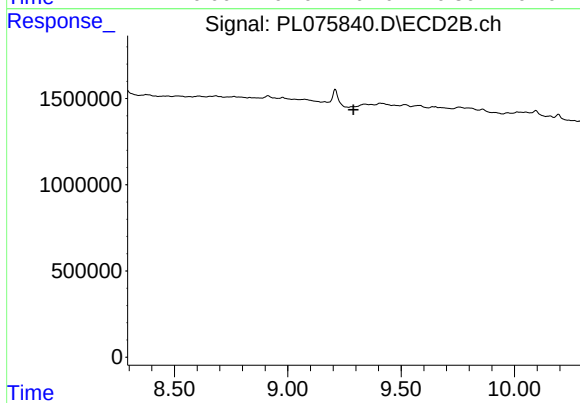

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

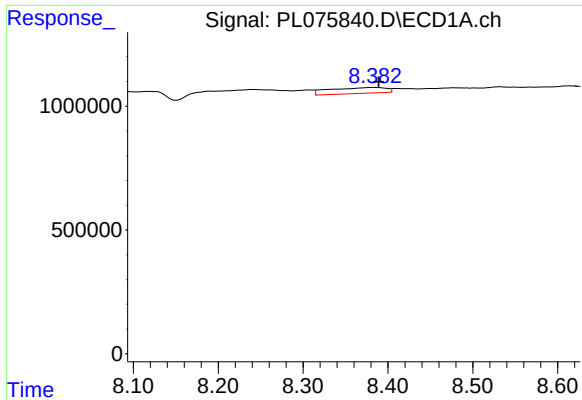

#25 Chlordane-3


R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 1084887
Conc: 10.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

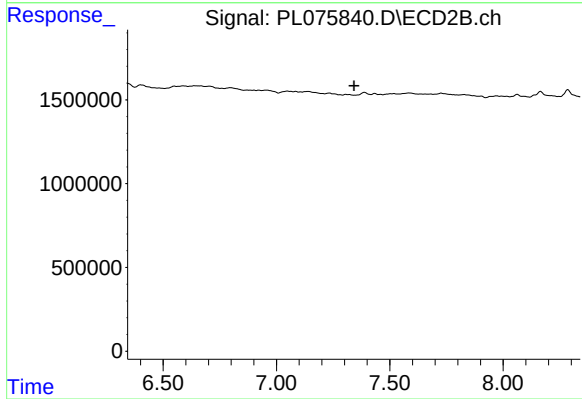


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

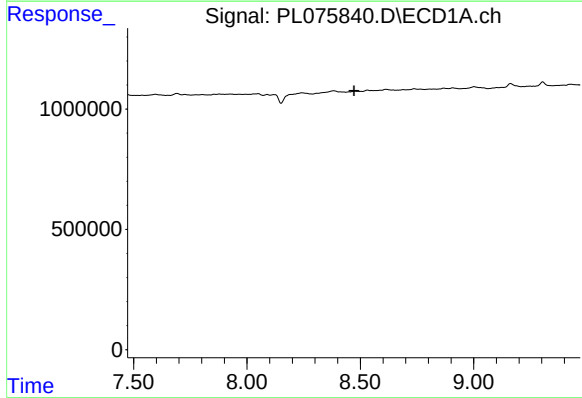


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

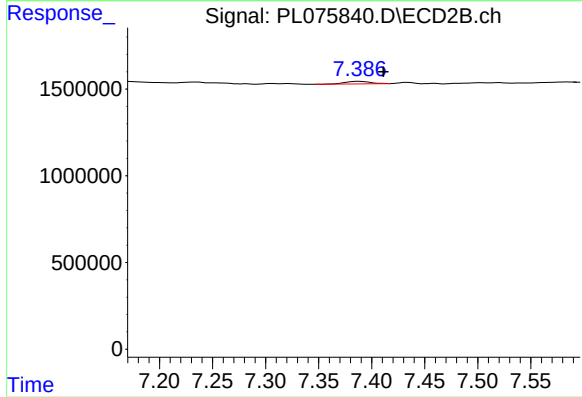

#26 Chlordane-4


R.T.: 7.387 min
Delta R.T.: -0.024 min
Response: 242599
Conc: 1.32 ng/ml

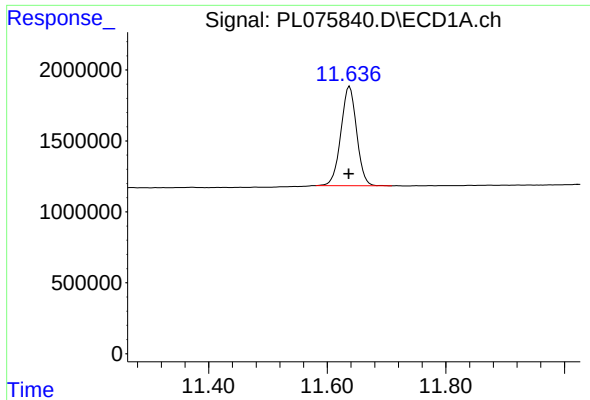

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: 0.002 min
Response: 12898979
Conc: 21.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

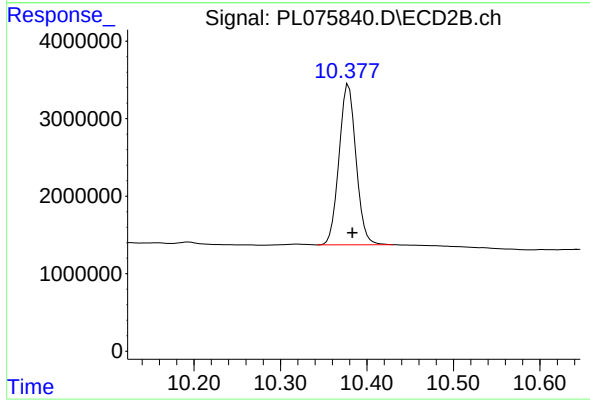

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 28115125
Conc: 19.95 ng/ml