

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
 Data File : PL075844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2022 14:31
 Operator : AR\AJ
 Sample : PB145627BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 22:32:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.636	13115375	32153418	19.433	19.160
28)	SA Decachlor...	11.638	10.379	12443513	26418974	20.325	18.751
Target Compounds							
7)	B delta-BHC	0.000	6.401	0	324061	N.D.	0.151 #
9)	A Endosulfan I	8.538	0.000	67736	0	0.097	N.D. #
11)	B alpha-Chl...	0.000	7.389f	0	202249	N.D.	0.111 #
14)	MA Endrin	0.000	8.063f	0	142557	N.D.	0.104 #
15)	B Endosulfa...	9.306	0.000	193840	0	0.311	N.D. #
19)	B Endosulfa...	9.666	8.763	146873	430234	0.234	0.293
21)	B Endrin ke...	10.186f	9.297	537054	46535	0.764	0.029 #
26)	Chlordane-4	0.000	7.389f	0	202249	N.D.	1.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
Data File : PL075844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2022 14:31
Operator : AR\AJ
Sample : PB145627BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 22:32:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

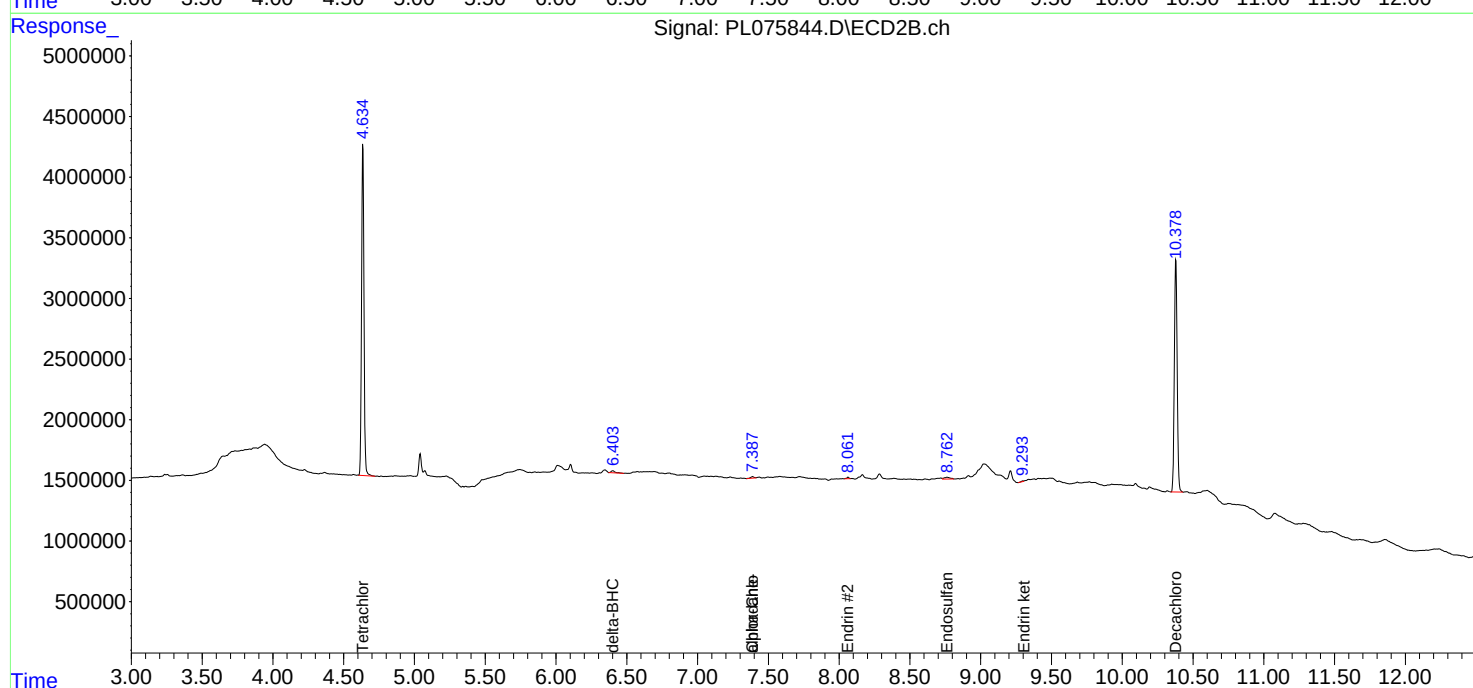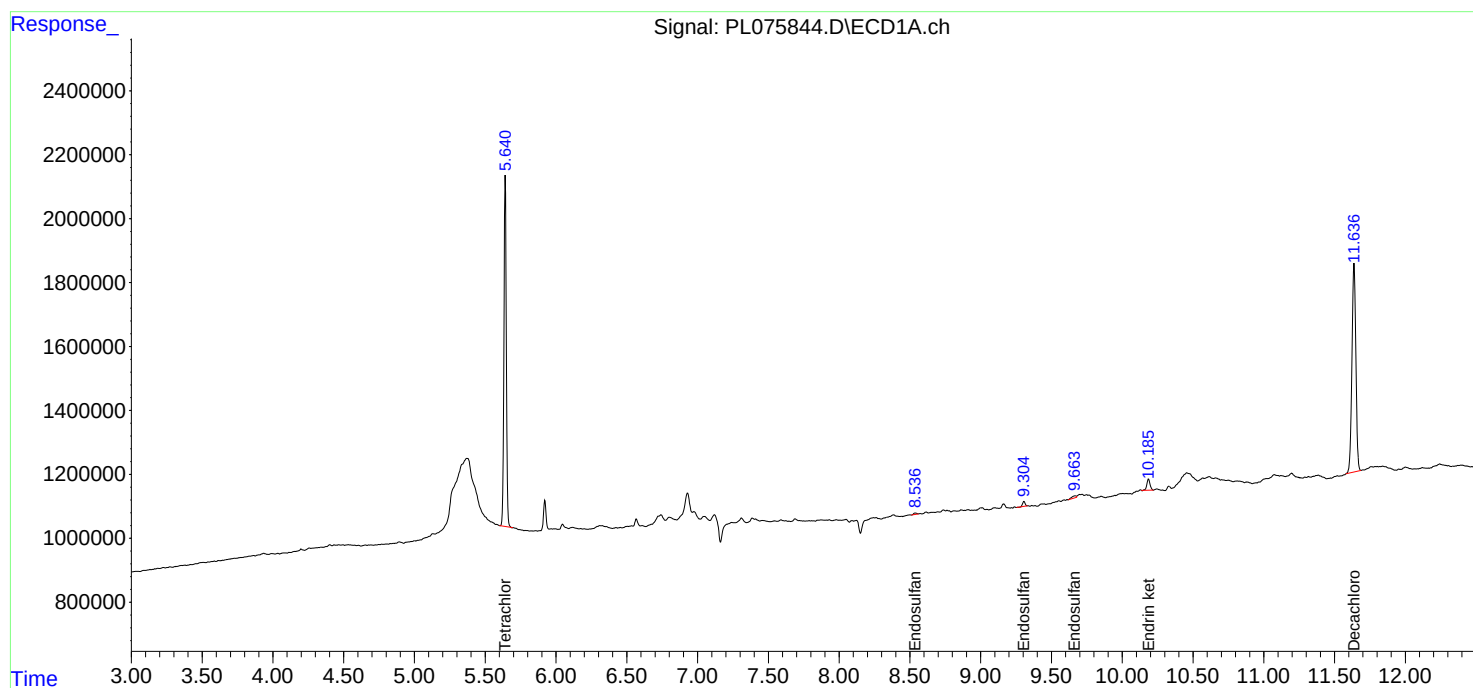


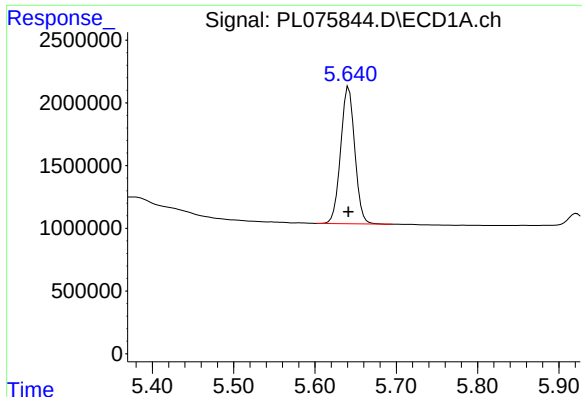

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 13115375
Conc: 19.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

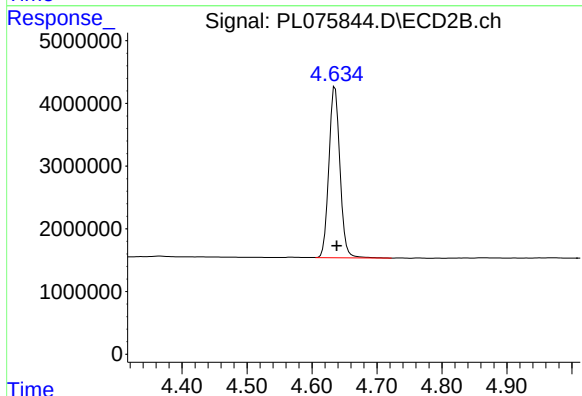


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 32153418
Conc: 19.16 ng/ml

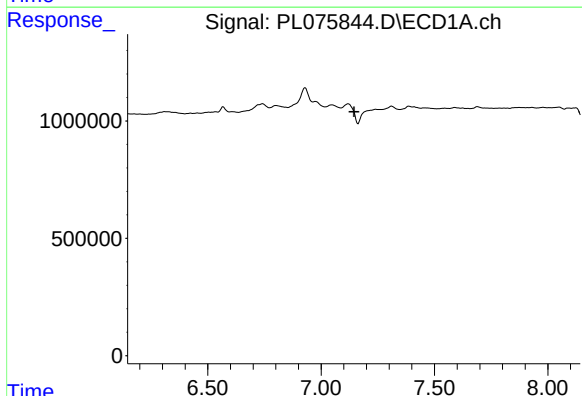


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

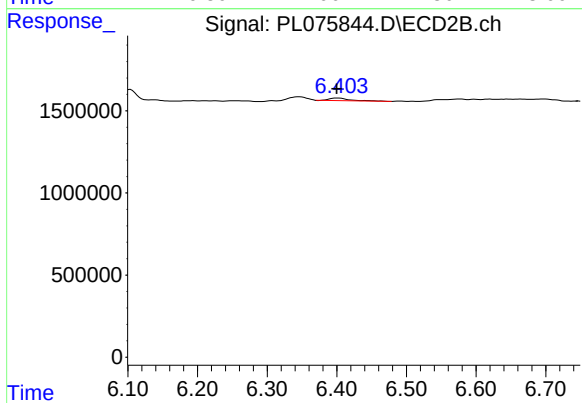

#7 delta-BHC


R.T.: 6.401 min
Delta R.T.: 0.002 min
Response: 324061
Conc: 0.15 ng/ml

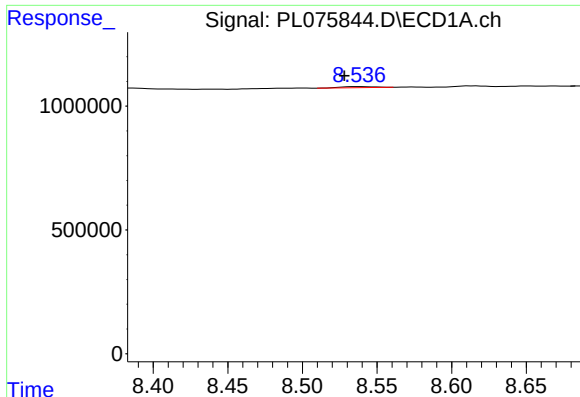

#9 Endosulfan I


R.T.: 8.538 min
Delta R.T.: 0.010 min
Response: 67736
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

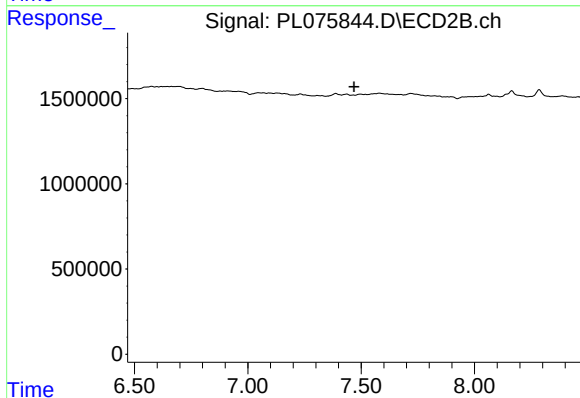


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

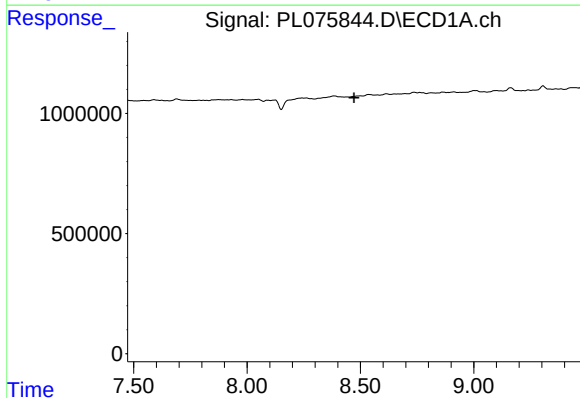


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

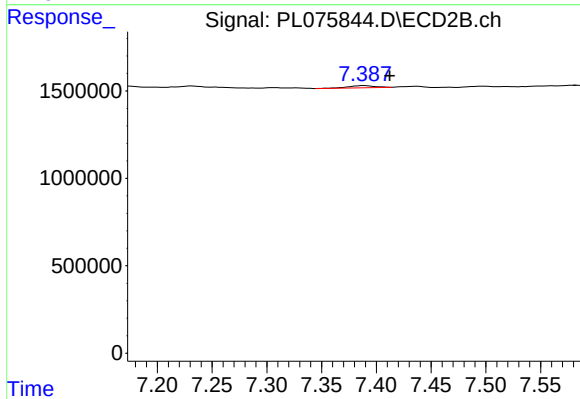

#11 alpha-Chlordane


R.T.: 7.389 min
Delta R.T.: -0.024 min
Response: 202249
Conc: 0.11 ng/ml

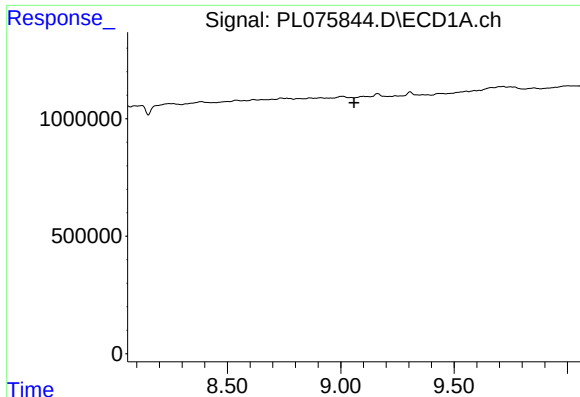

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

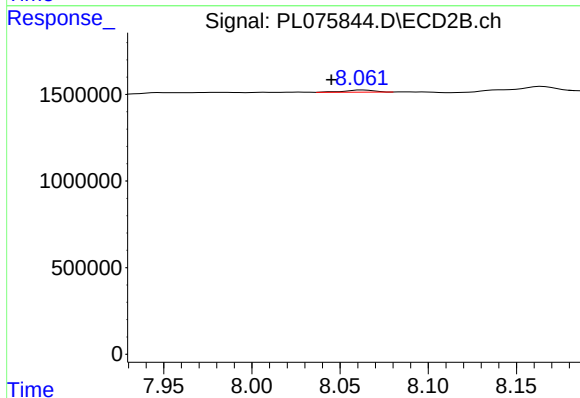


#14 Endrin

R.T.: 8.063 min
Delta R.T.: 0.018 min
Response: 142557
Conc: 0.10 ng/ml

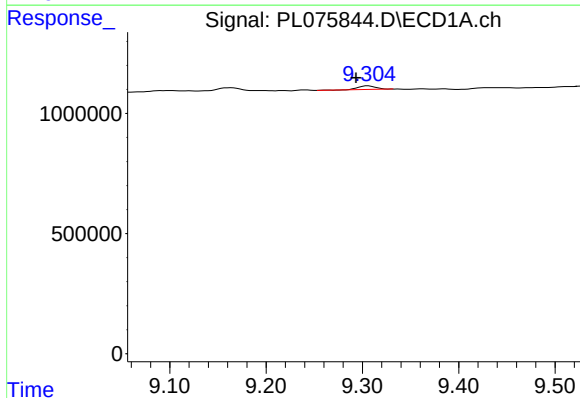


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.012 min
Response: 193840
Conc: 0.31 ng/ml

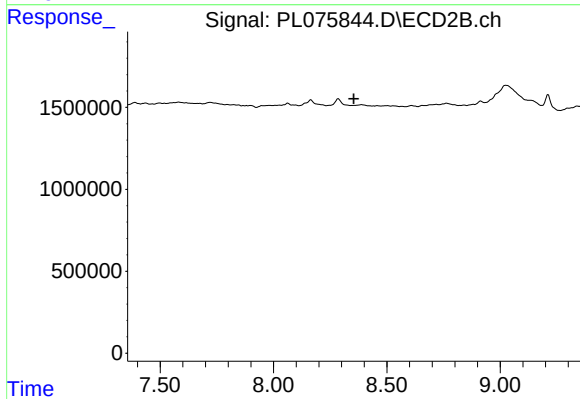

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

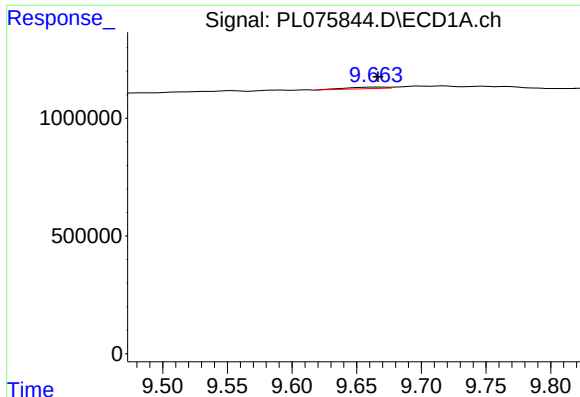

#19 Endosulfan Sulfate


R.T.: 9.666 min
Delta R.T.: 0.000 min
Response: 146873
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

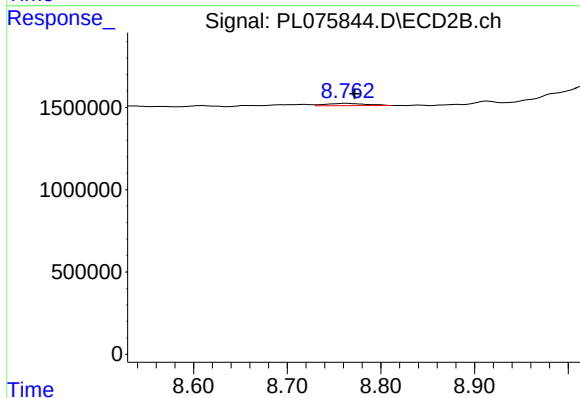


#19 Endosulfan Sulfate

R.T.: 8.763 min
Delta R.T.: -0.009 min
Response: 430234
Conc: 0.29 ng/ml

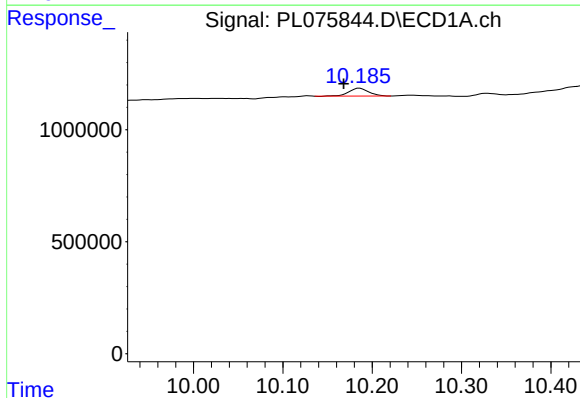


#21 Endrin ketone

R.T.: 10.186 min
Delta R.T.: 0.018 min
Response: 537054
Conc: 0.76 ng/ml

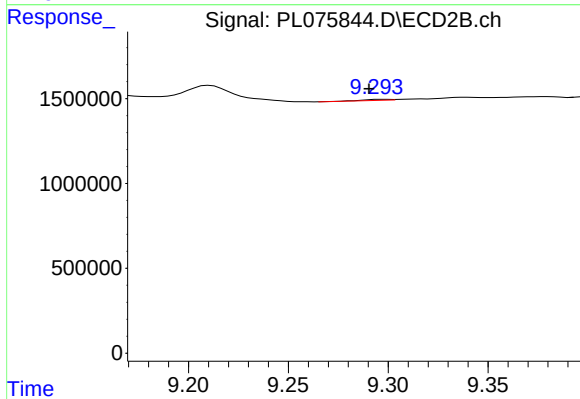

#21 Endrin ketone


R.T.: 9.297 min
Delta R.T.: 0.006 min
Response: 46535
Conc: 0.03 ng/ml

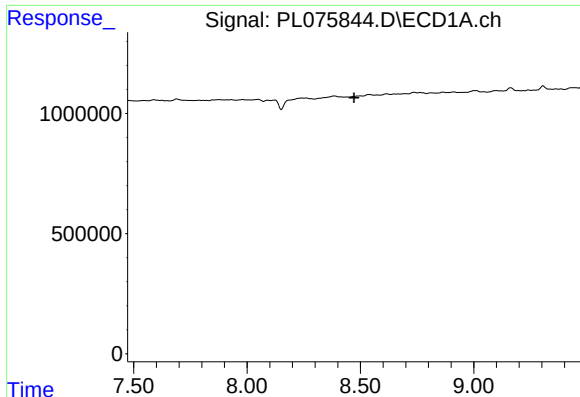

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

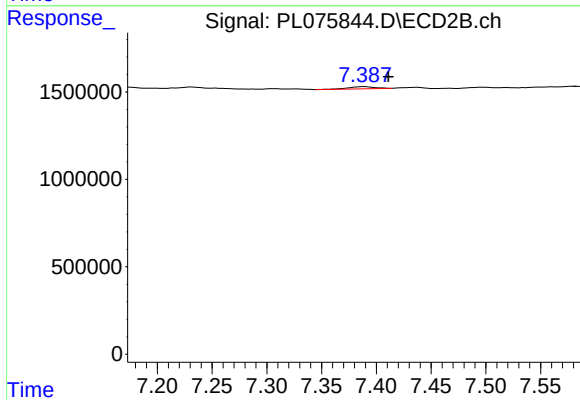


#26 Chlordane-4

R.T.: 7.389 min
Delta R.T.: -0.022 min
Response: 202249
Conc: 1.10 ng/ml

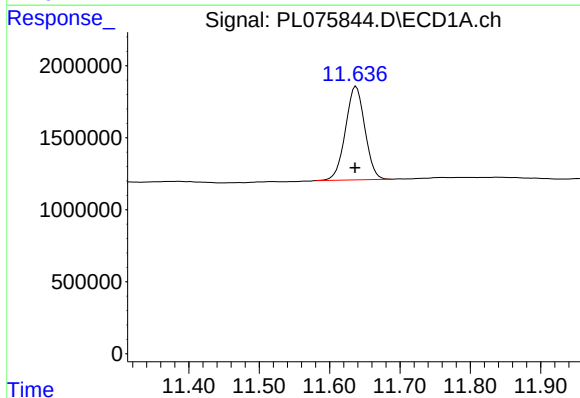

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: 0.001 min
Response: 12443513
Conc: 20.33 ng/ml

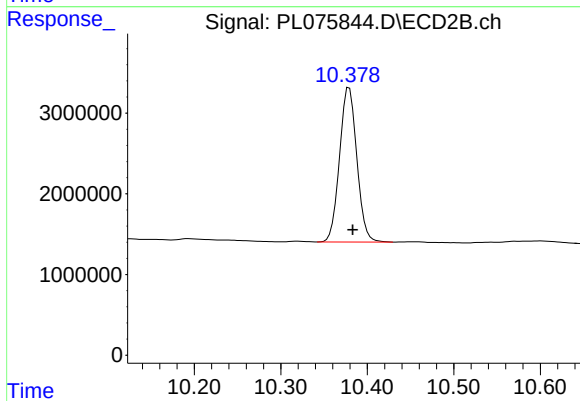

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 26418974
Conc: 18.75 ng/ml