

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
 Data File : PL075854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2022 17:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 22:39:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	14944699	36204920	22.144	21.574
28)	SA Decachlor...	11.639	10.379	14072570	29933195	22.986	21.245
Target Compounds							
4)	MA Heptachlor	7.307f	0.000	362824	0	0.395	N.D. #
7)	B delta-BHC	0.000	6.403	0	383537	N.D.	0.179 #
8)	B Heptachlo...	8.124	0.000	670808	0	0.868	N.D. #
10)	B gamma-Chl...	8.387	7.327f	1682374	572004	2.166	0.312 #
11)	B alpha-Chl...	8.469	7.387f	216597	293764	0.284	0.161 #
13)	MA Dieldrin	8.817	7.752	284269	-170048	0.393	N.D. #
14)	MA Endrin	0.000	8.063f	0	805353	N.D.	0.589 #
15)	B Endosulfa...	9.302	0.000	686979	0	1.104	N.D. #
21)	B Endrin ke...	10.187f	9.279	460000	179036	0.654	0.111 #
24)	Chlordane-2	0.000	6.668f	0	682030	N.D.	10.199 #
25)	Chlordane-3	8.387	7.327f	1682374	572004	16.294	3.326 #
26)	Chlordane-4	8.469	7.387f	216597	293764	1.710	1.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061722\
Data File : PL075854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2022 17:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 22:39:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

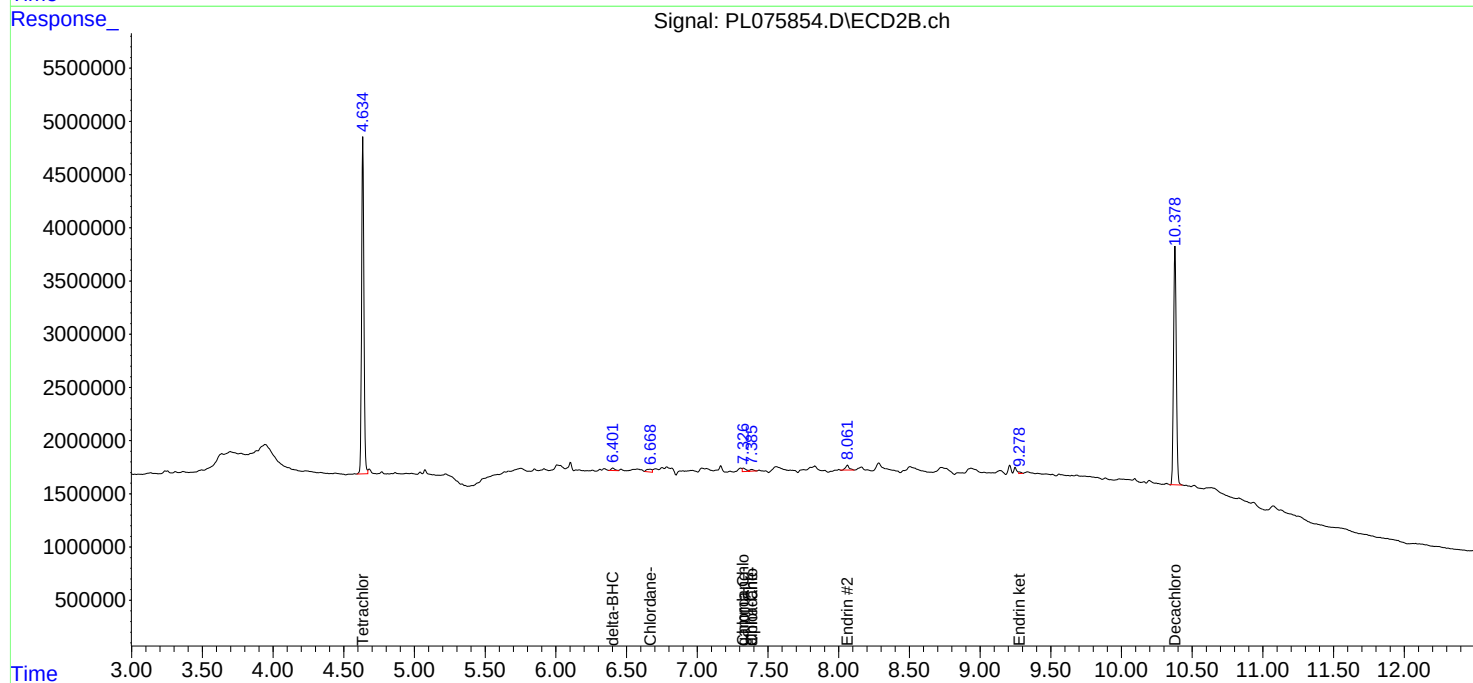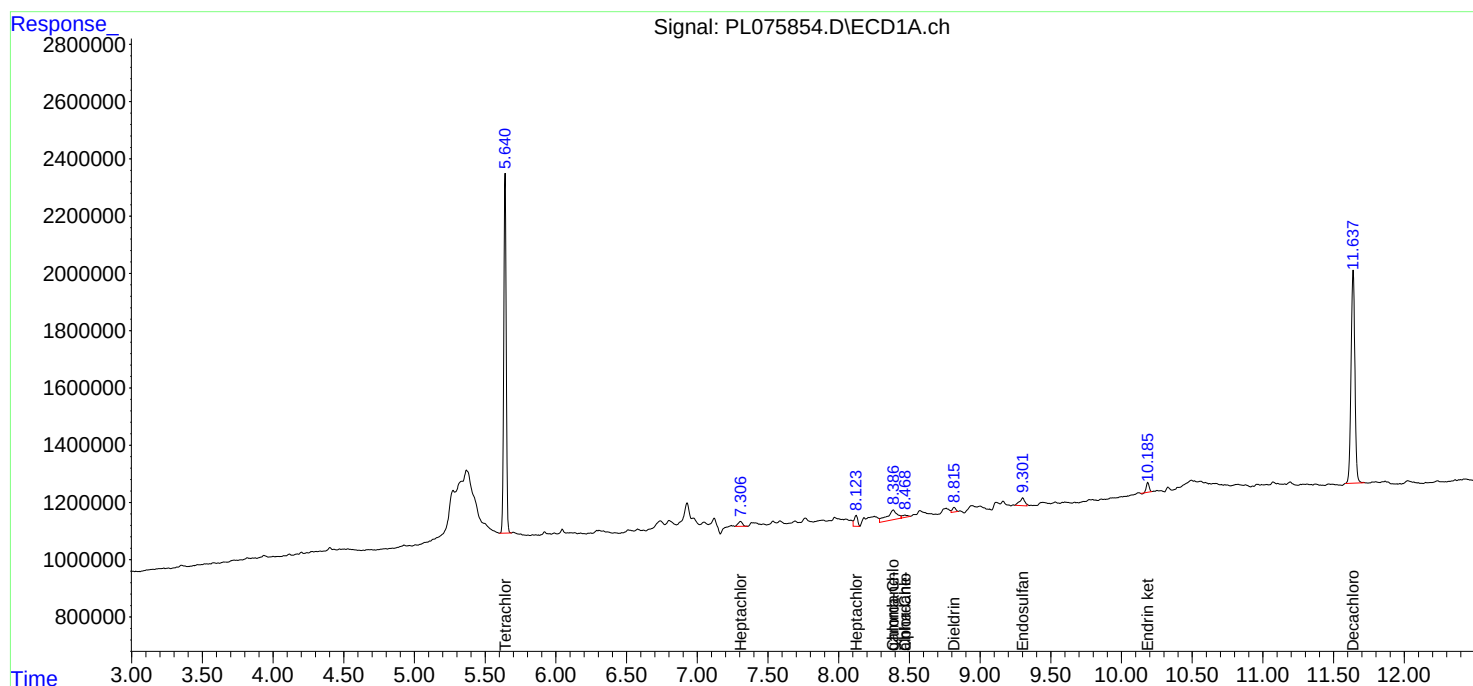


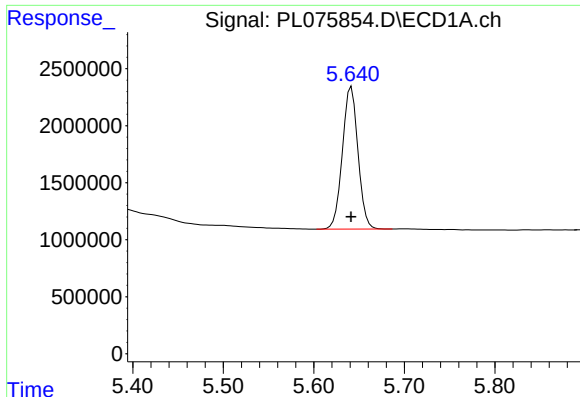

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 14944699
Conc: 22.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

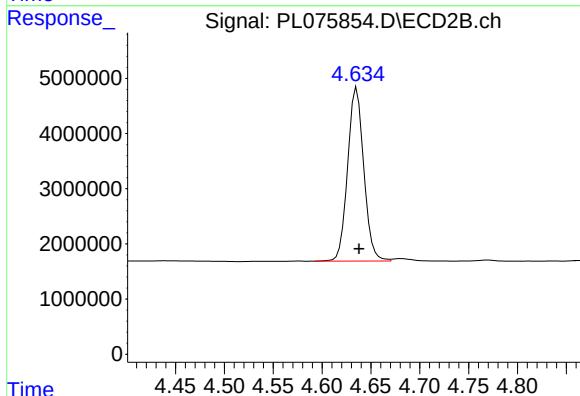


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 36204920
Conc: 21.57 ng/ml

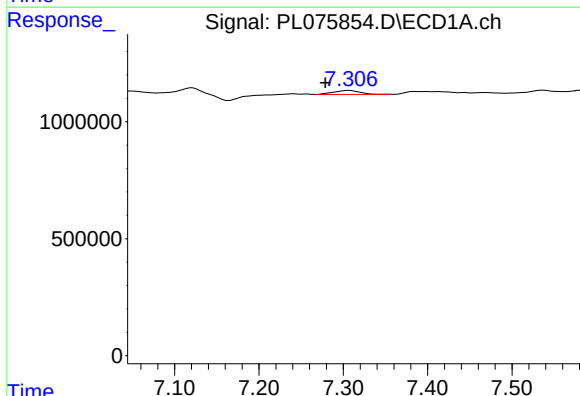


#4 Heptachlor

R.T.: 7.307 min
Delta R.T.: 0.028 min
Response: 362824
Conc: 0.39 ng/ml

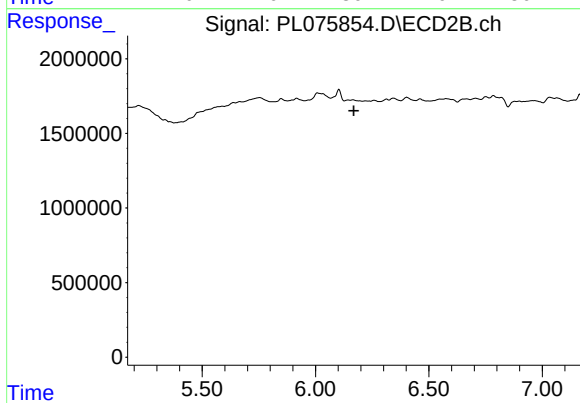

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.169 min
Response: 0
Conc: N.D.

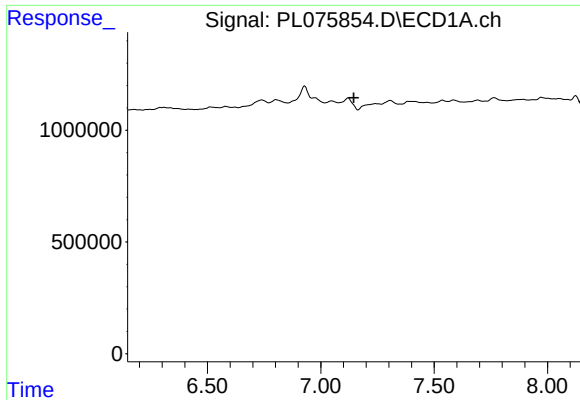

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

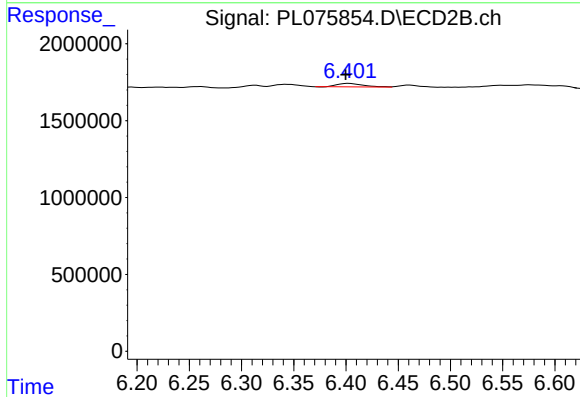


#7 delta-BHC

R.T.: 6.403 min
Delta R.T.: 0.003 min
Response: 383537
Conc: 0.18 ng/ml

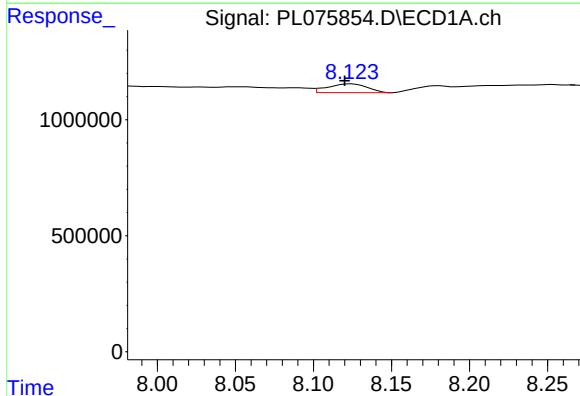


#8 Heptachlor epoxide

R.T.: 8.124 min
Delta R.T.: 0.004 min
Response: 670808
Conc: 0.87 ng/ml

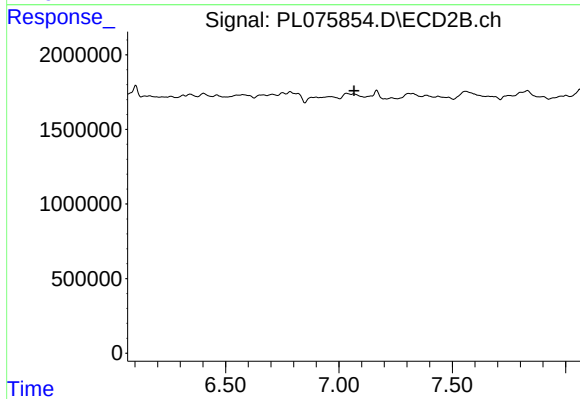

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.067 min
Response: 0
Conc: N.D.

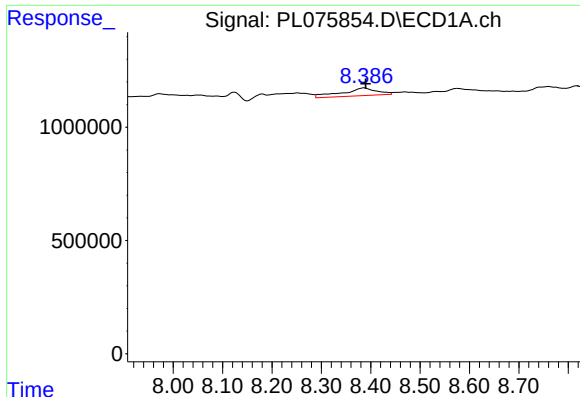

#10 gamma-Chlordane


R.T.: 8.387 min
Delta R.T.: -0.003 min
Response: 1682374
Conc: 2.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

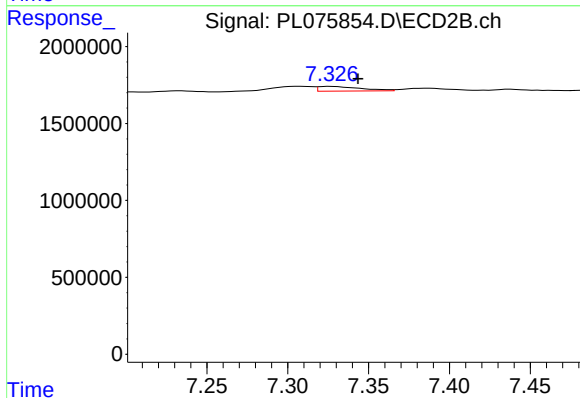


#10 gamma-Chlordane

R.T.: 7.327 min
Delta R.T.: -0.017 min
Response: 572004
Conc: 0.31 ng/ml

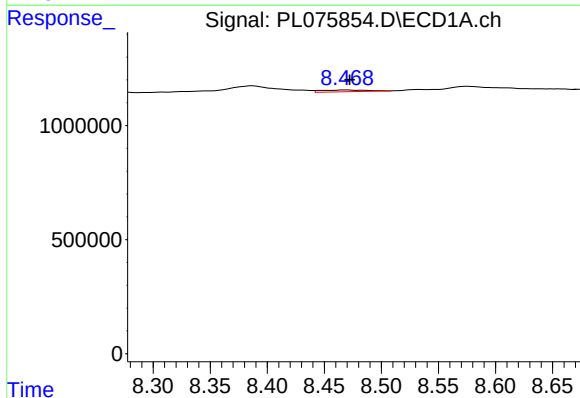


#11 alpha-Chlordane

R.T.: 8.469 min
Delta R.T.: -0.003 min
Response: 216597
Conc: 0.28 ng/ml

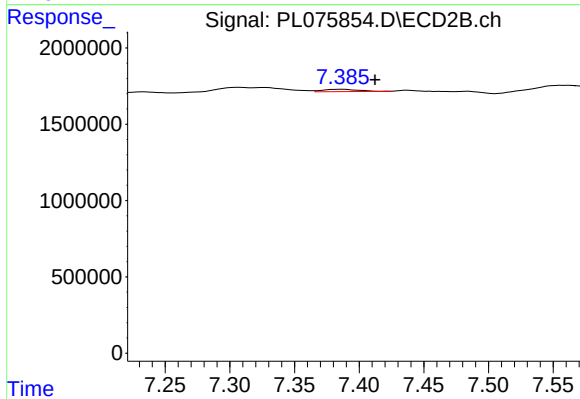

#11 alpha-Chlordane


R.T.: 7.387 min
Delta R.T.: -0.025 min
Response: 293764
Conc: 0.16 ng/ml

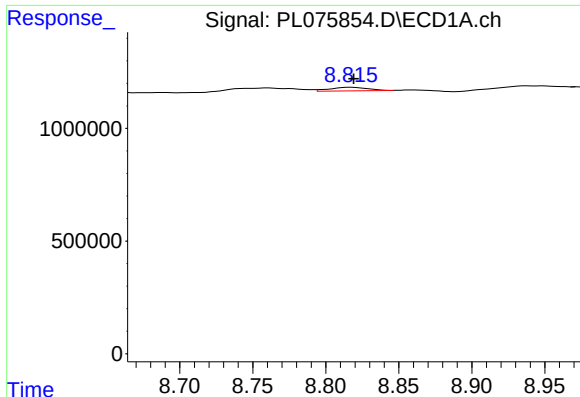

#13 Dieldrin


R.T.: 8.817 min
Delta R.T.: -0.002 min
Response: 284269
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

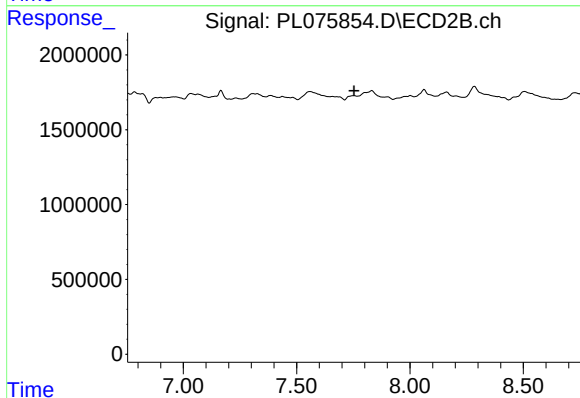


#13 Dieldrin

R.T.: 7.752 min
Delta R.T.: -0.002 min
Response: -170048
Conc: N.D.

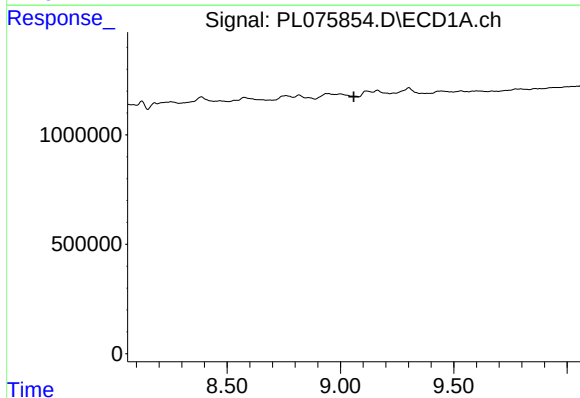


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

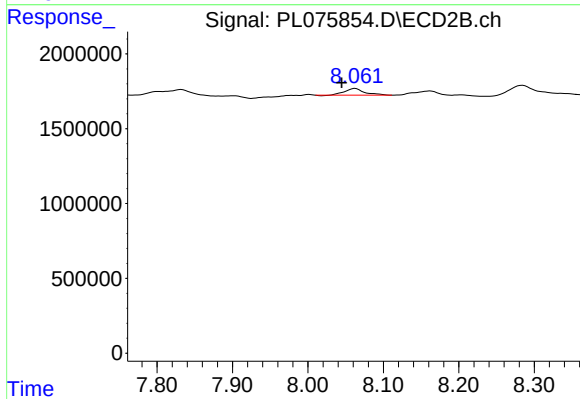

#14 Endrin


R.T.: 8.063 min
Delta R.T.: 0.018 min
Response: 805353
Conc: 0.59 ng/ml

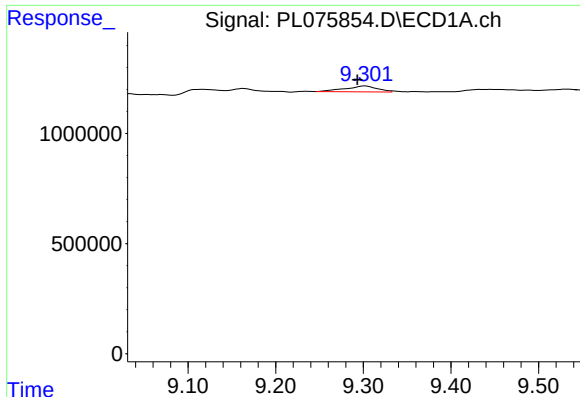

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.009 min
Response: 686979
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

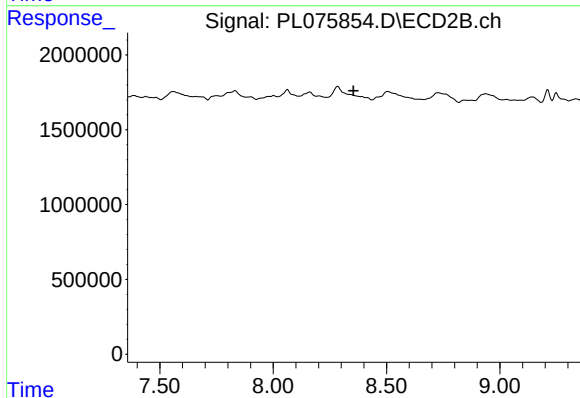


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

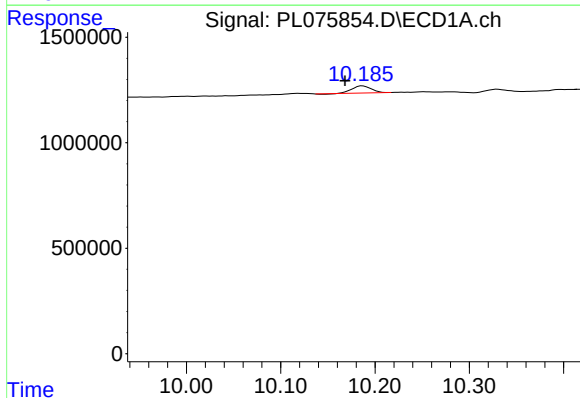


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.019 min
Response: 460000
Conc: 0.65 ng/ml

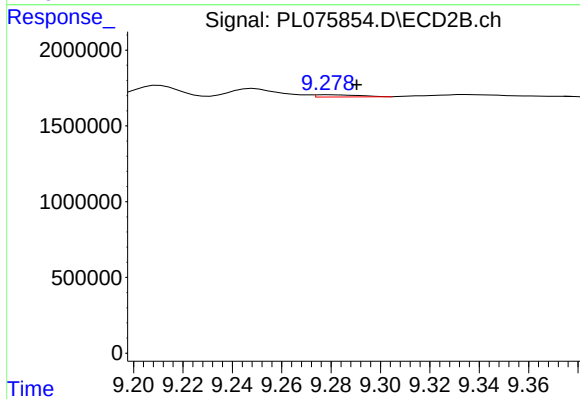

#21 Endrin ketone


R.T.: 9.279 min
Delta R.T.: -0.011 min
Response: 179036
Conc: 0.11 ng/ml

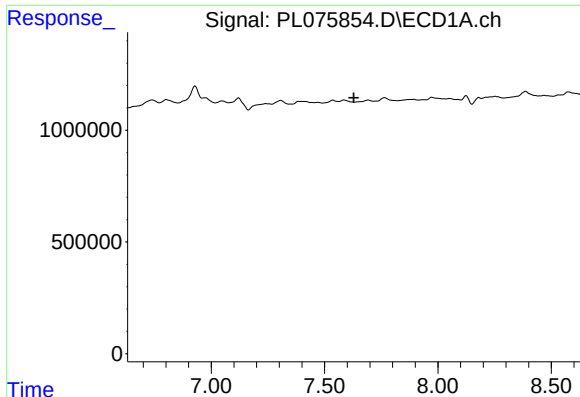

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

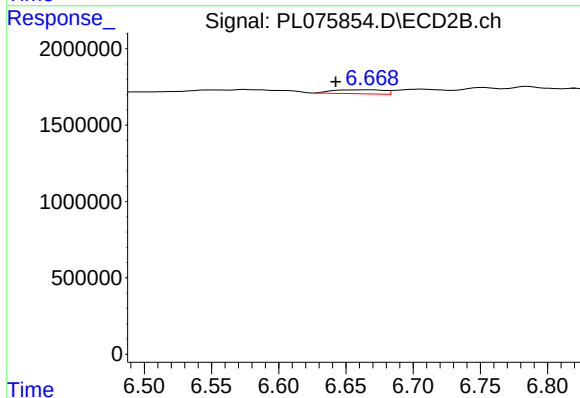


#24 Chlordane-2

R.T.: 6.668 min
Delta R.T.: 0.025 min
Response: 682030
Conc: 10.20 ng/ml

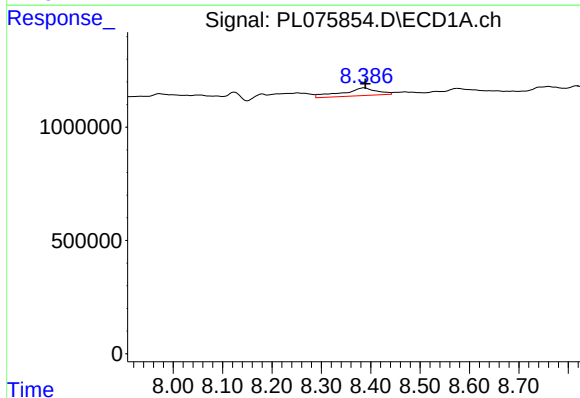


#25 Chlordane-3

R.T.: 8.387 min
Delta R.T.: -0.002 min
Response: 1682374
Conc: 16.29 ng/ml

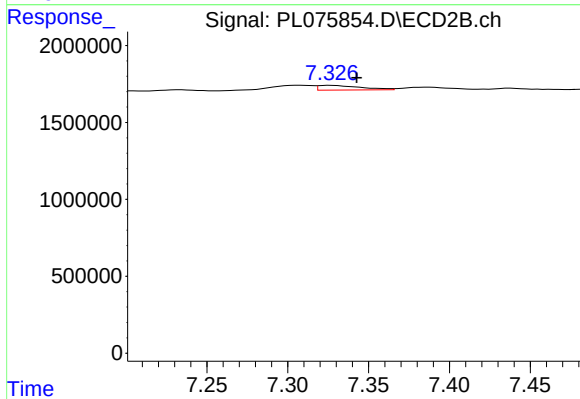

#25 Chlordane-3


R.T.: 7.327 min
Delta R.T.: -0.016 min
Response: 572004
Conc: 3.33 ng/ml

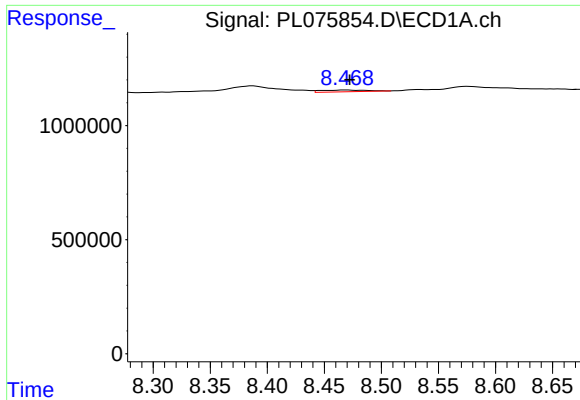

#26 Chlordane-4


R.T.: 8.469 min
Delta R.T.: -0.003 min
Response: 216597
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

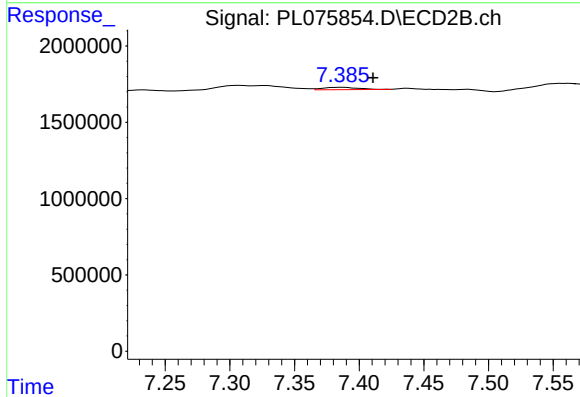


#26 Chlordane-4

R.T.: 7.387 min
Delta R.T.: -0.024 min
Response: 293764
Conc: 1.60 ng/ml

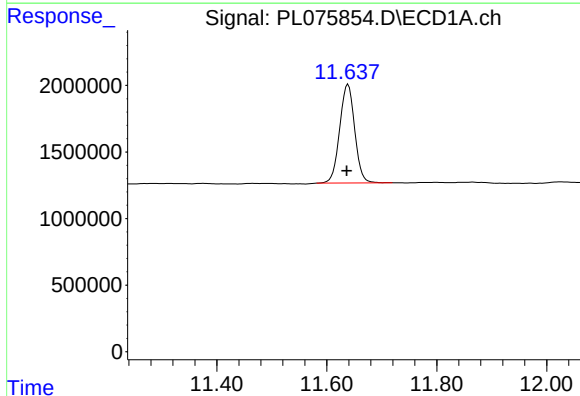

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: 0.003 min
Response: 14072570
Conc: 22.99 ng/ml

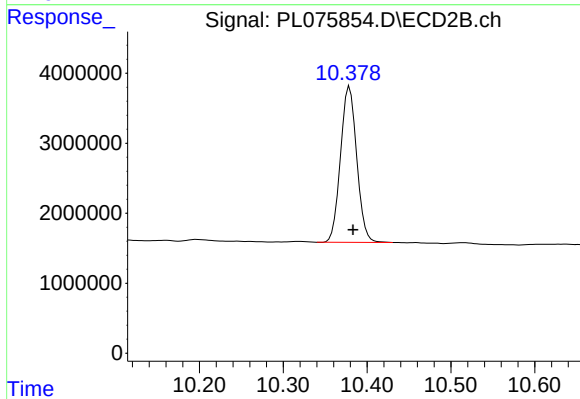

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 29933195
Conc: 21.25 ng/ml