

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
 Data File : PL083519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2023 08:06
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 12:23:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:22:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	2.751	223.9E6	298.8E6	98.701	99.900
28)	SA Decachlor...	8.990	7.964	188.2E6	230.5E6	94.970	93.863
Target Compounds							
23)	Chlordane-1	4.618	3.766	97147510	97747544	986.850	985.939
24)	Chlordane-2	5.150	4.351	101.5E6	115.0E6	937.894	981.935
25)	Chlordane-3	5.863	4.990	390.7E6	340.0E6	1010.412	1026.632
26)	Chlordane-4	5.946	5.053	463.3E6	349.0E6	995.172	1027.417
27)	Chlordane-5	6.795	5.955	80505537	113.6E6	991.621	1022.367



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
Data File : PL083519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2023 08:06
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 12:23:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:22:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

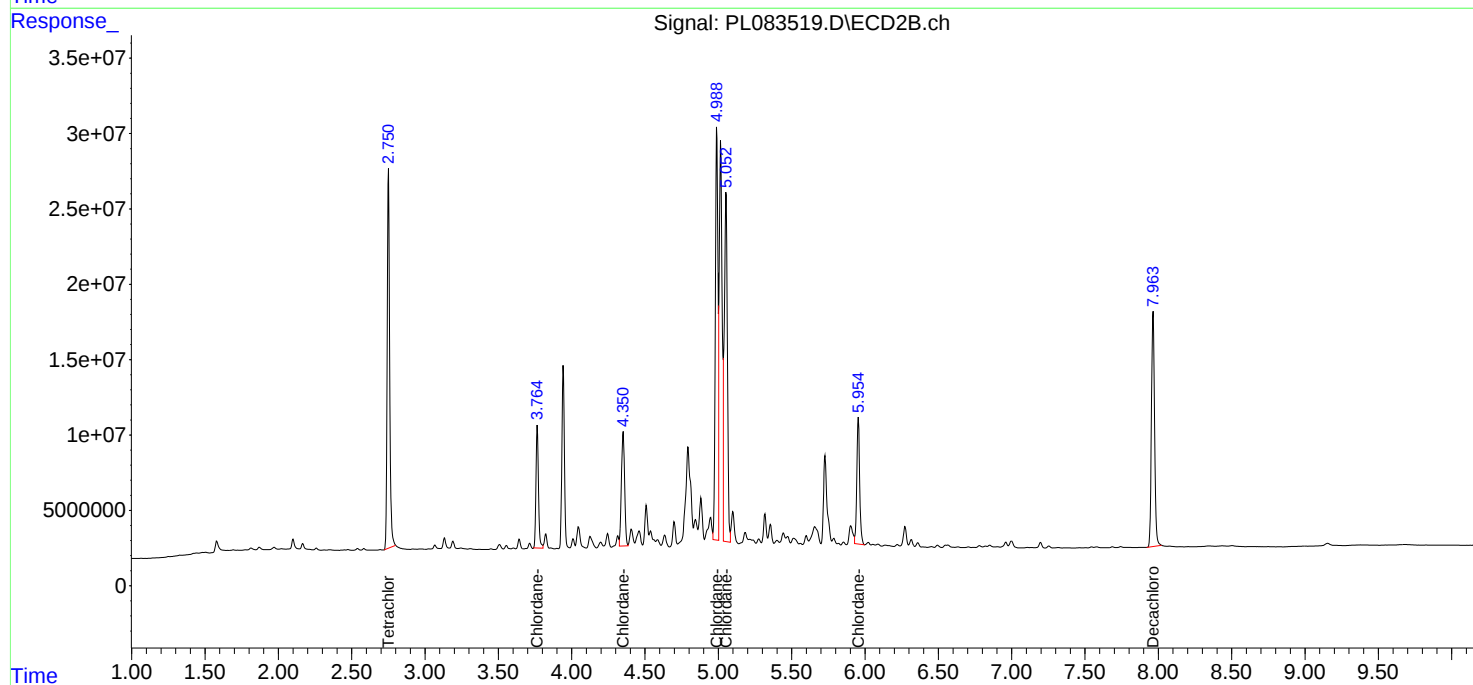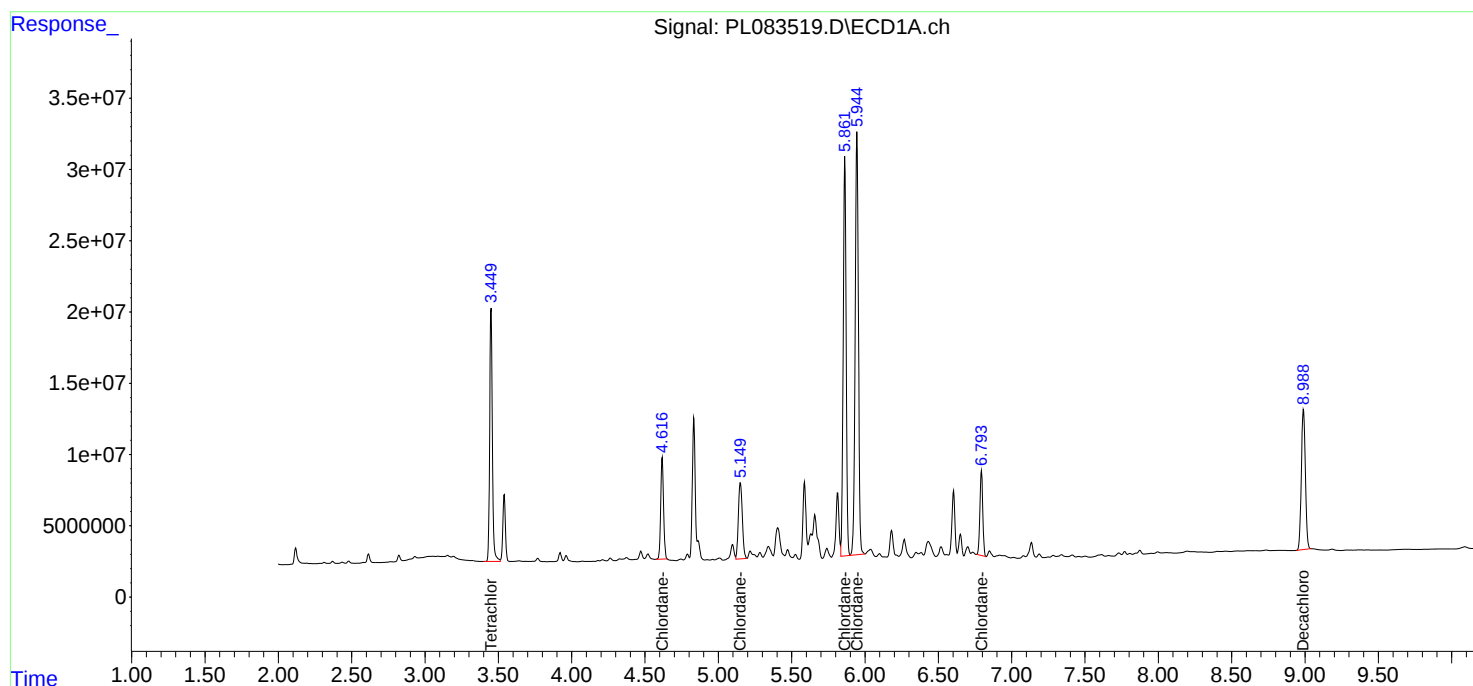


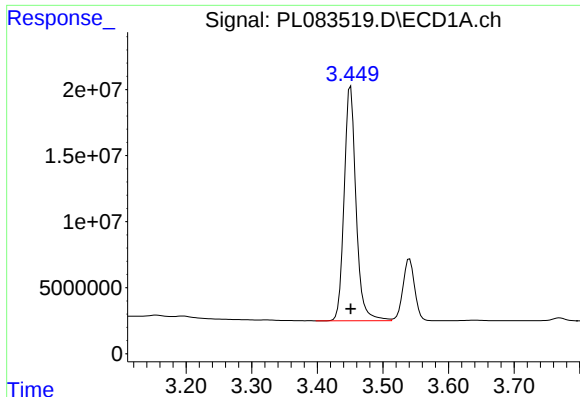

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 223940331
Conc: 98.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

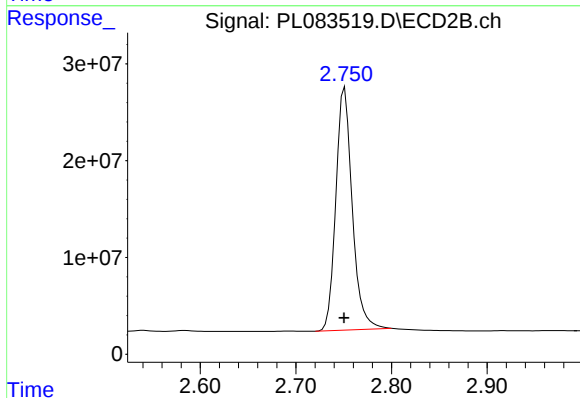


#1 Tetrachloro-m-xylene

R.T.: 2.751 min
Delta R.T.: 0.000 min
Response: 298764618
Conc: 99.90 ng/ml

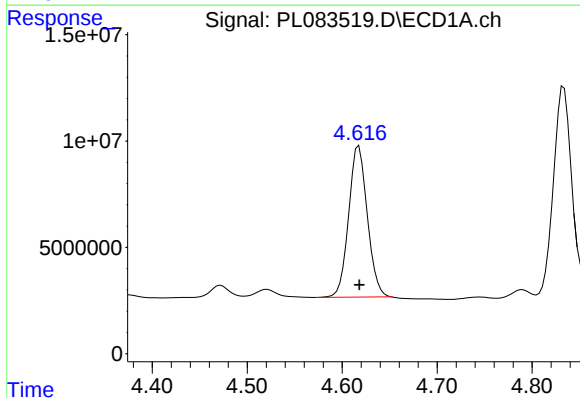


#23 Chlordane-1

R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 97147510
Conc: 986.85 ng/ml

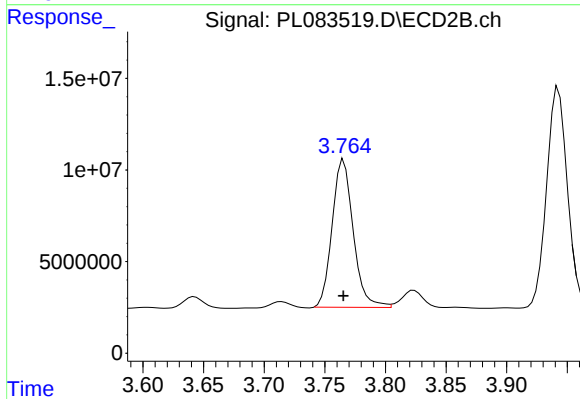

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 97747544
Conc: 985.94 ng/ml

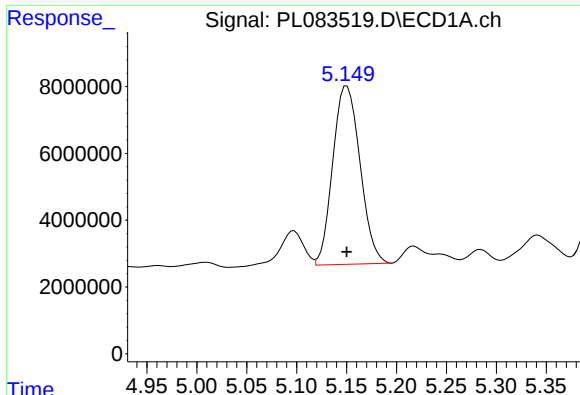

#24 Chlordane-2


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 101485378
Conc: 937.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

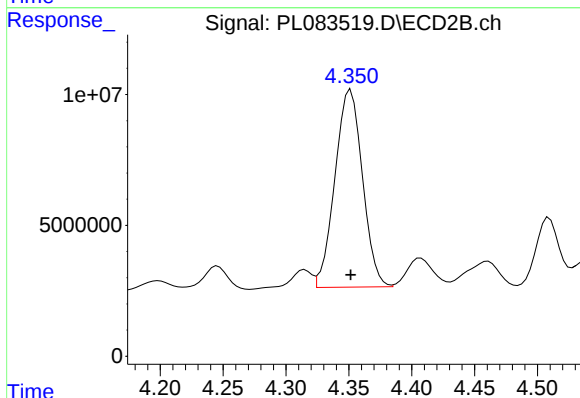


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 115026906
Conc: 981.94 ng/ml

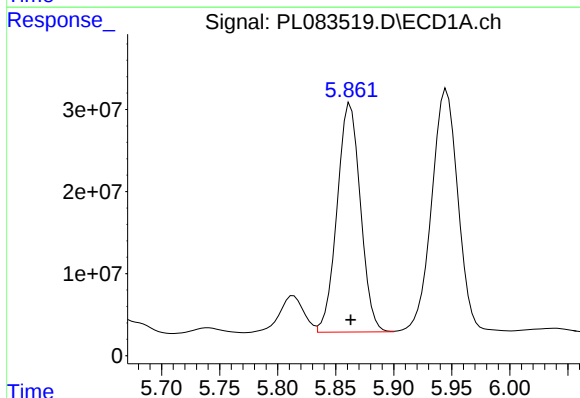


#25 Chlordane-3

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 390662705
Conc: 1010.41 ng/ml

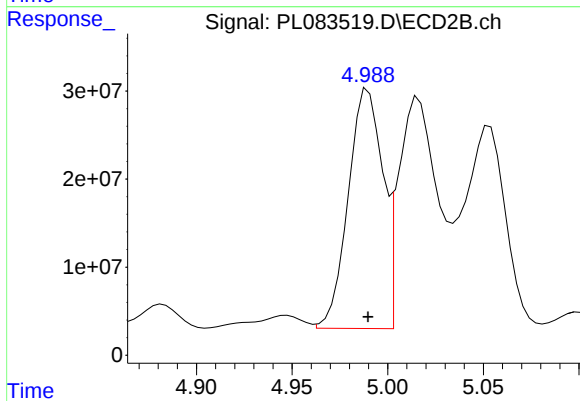

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 339984774
Conc: 1026.63 ng/ml

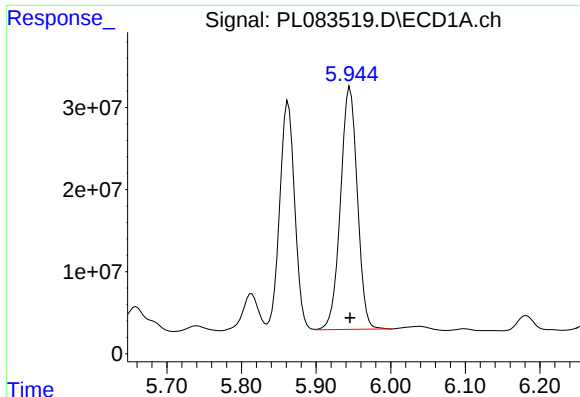

#26 Chlordane-4


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 463343052
Conc: 995.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

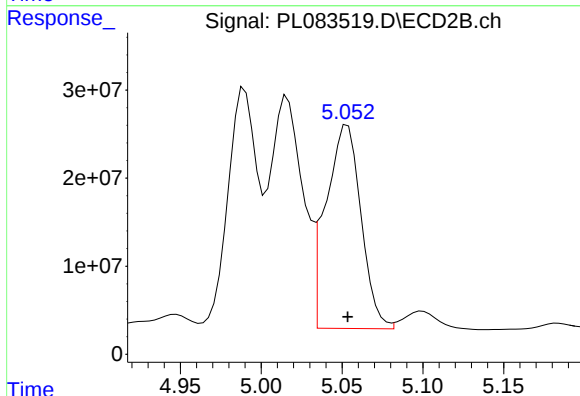


#26 Chlordane-4

R.T.: 5.053 min
Delta R.T.: 0.000 min
Response: 349001832
Conc: 1027.42 ng/ml

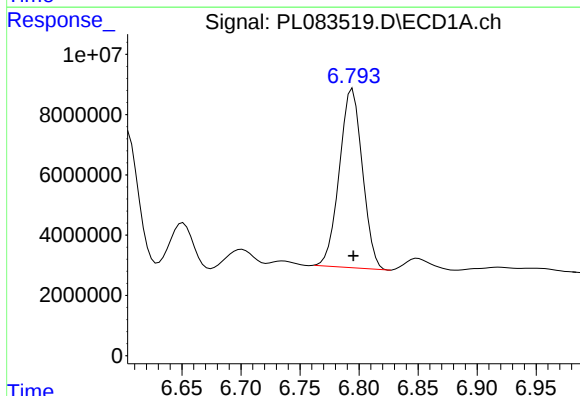


#27 Chlordane-5

R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 80505537
Conc: 991.62 ng/ml

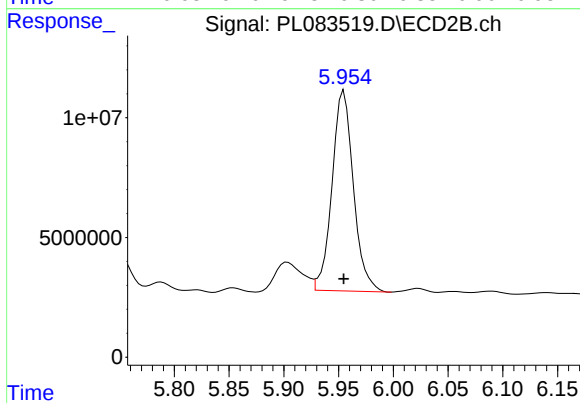

#27 Chlordane-5


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 113649047
Conc: 1022.37 ng/ml

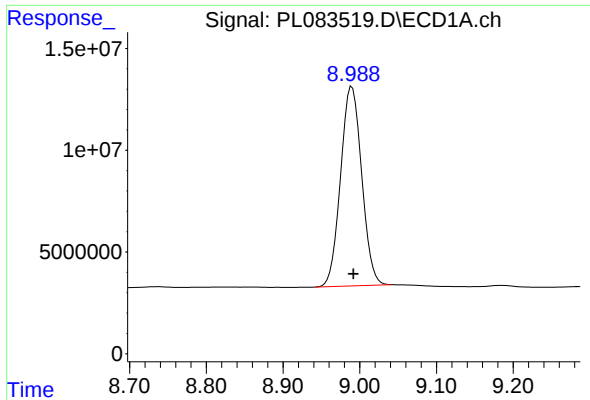

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 188218296
Conc: 94.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

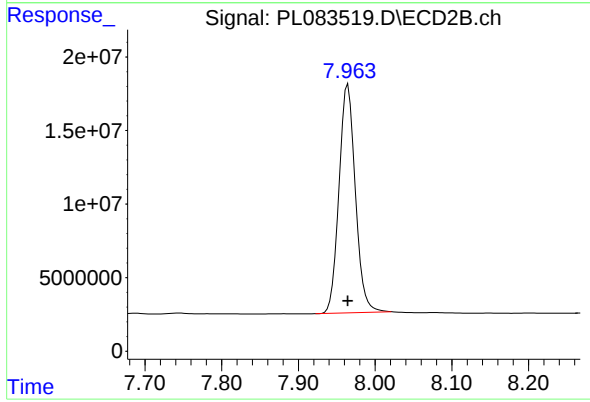

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 230549942
Conc: 93.86 ng/ml