

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
 Data File : PL083520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2023 08:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 12:24:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:22:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	2.751	164.4E6	218.8E6	72.455	73.148
28)	SA Decachlor...	8.991	7.964	139.6E6	172.6E6	70.426	70.268
Target Compounds							
23)	Chlordane-1	4.618	3.765	69908993	71171813	710.154	717.880
24)	Chlordane-2	5.150	4.352	75366499	83654762	696.512	714.125
25)	Chlordane-3	5.862	4.990	280.1E6	245.4E6	724.507	740.948
26)	Chlordane-4	5.945	5.053	334.8E6	251.2E6	718.990	739.366
27)	Chlordane-5	6.794	5.955	57975553	80624463	714.110	725.284



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
Data File : PL083520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2023 08:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 12:24:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:22:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

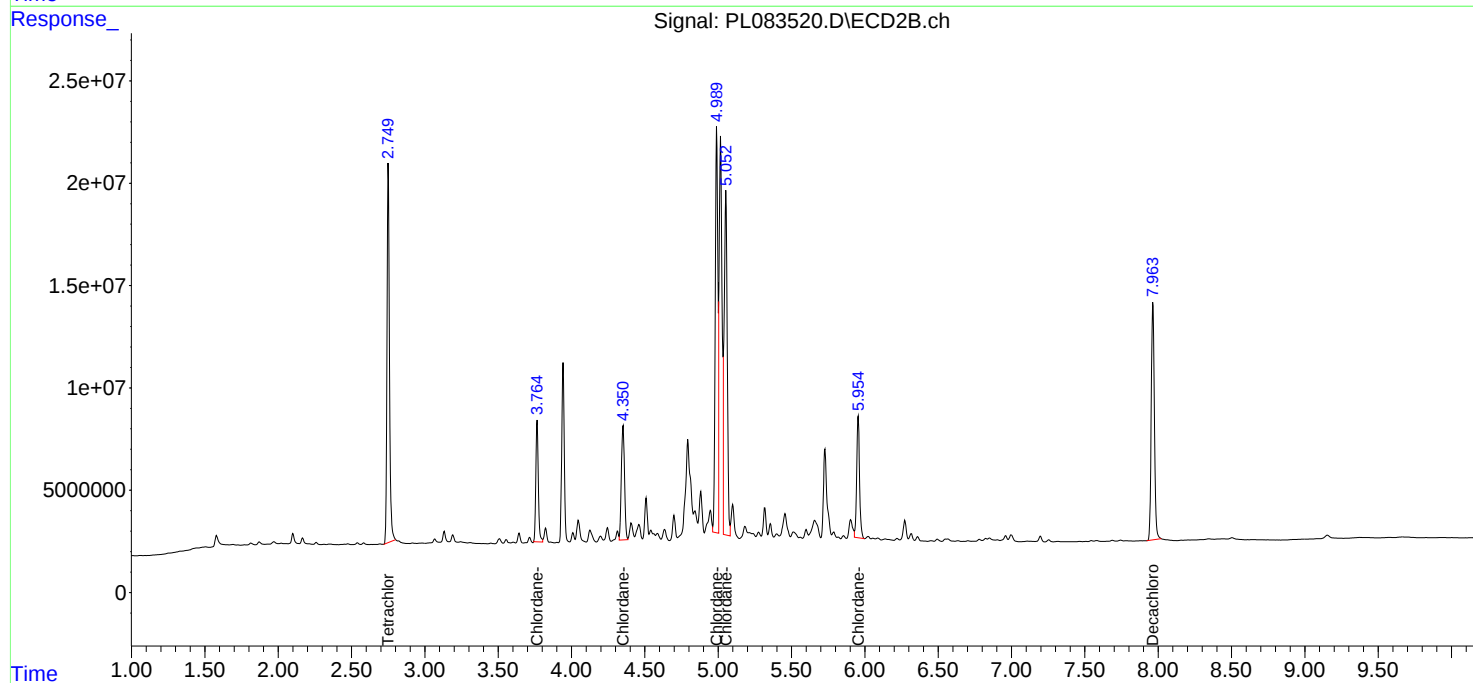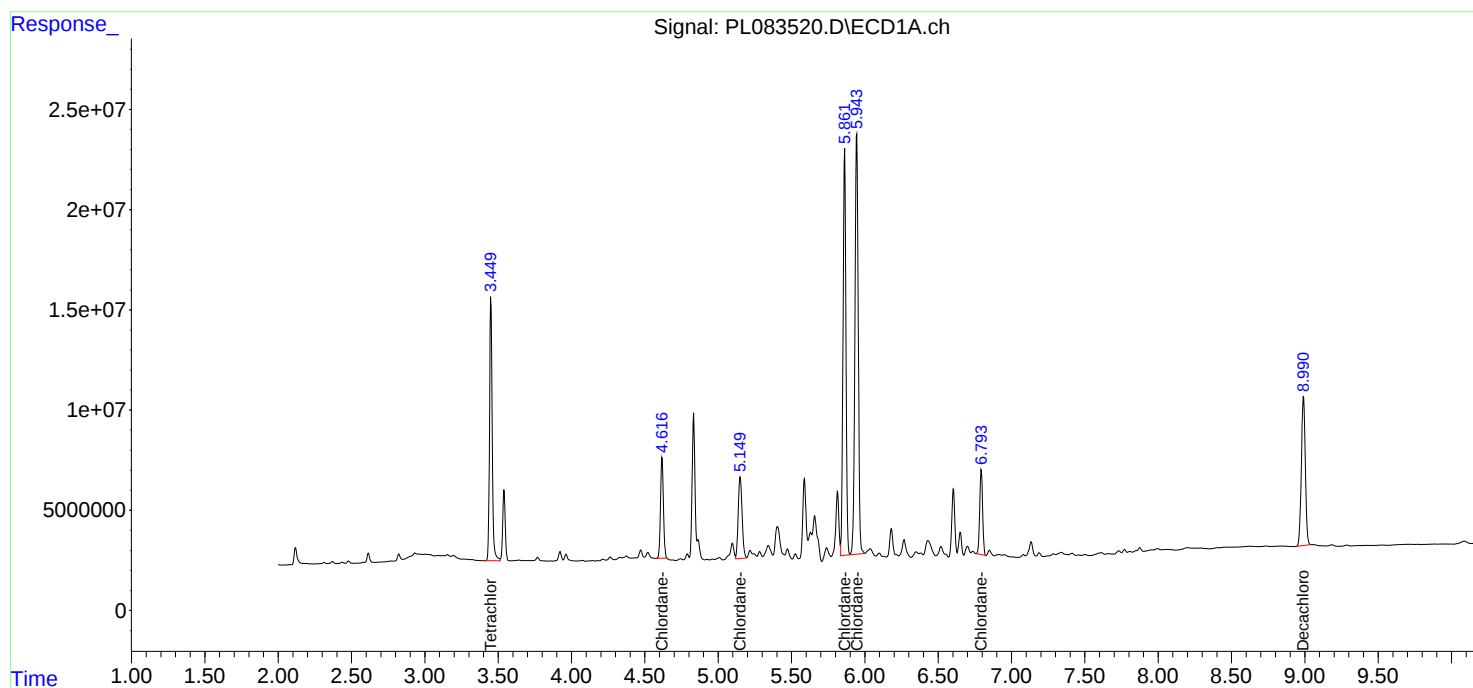


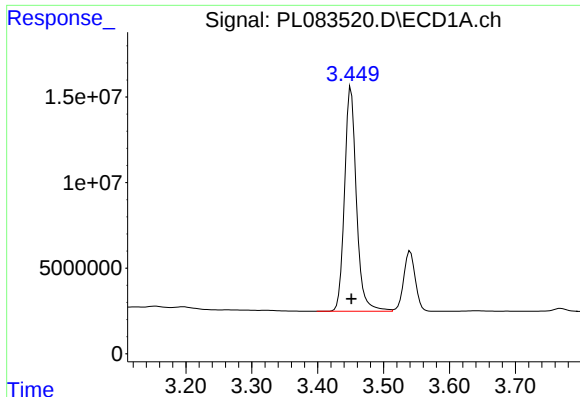

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 164391033
Conc: 72.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

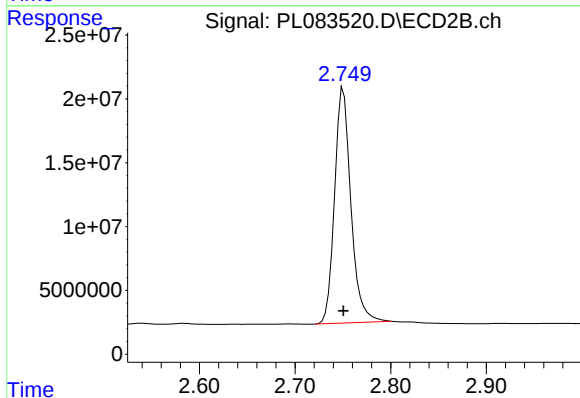


#1 Tetrachloro-m-xylene

R.T.: 2.751 min
Delta R.T.: 0.000 min
Response: 218759267
Conc: 73.15 ng/ml

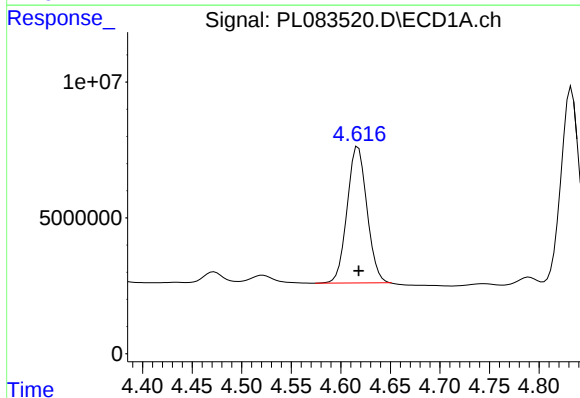


#23 Chlordane-1

R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 69908993
Conc: 710.15 ng/ml

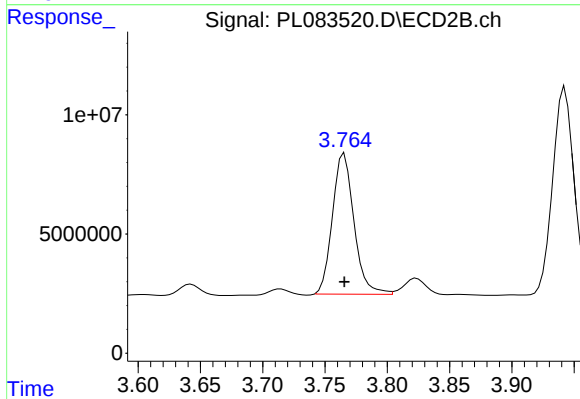

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: 0.000 min
Response: 71171813
Conc: 717.88 ng/ml

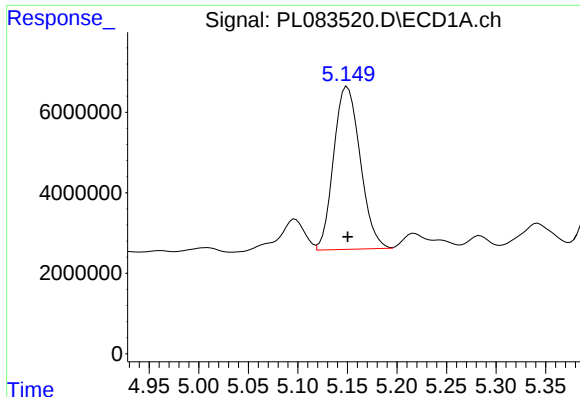

#24 Chlordane-2


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 75366499
Conc: 696.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

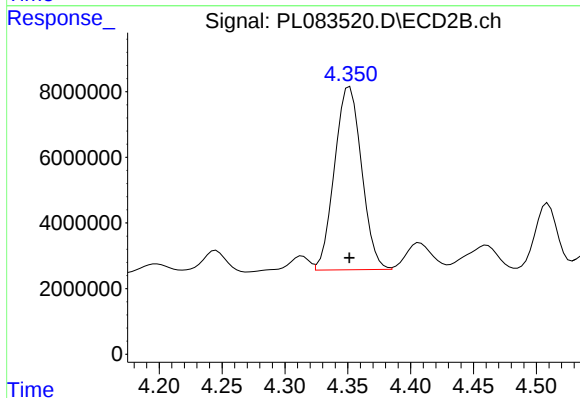


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 83654762
Conc: 714.12 ng/ml

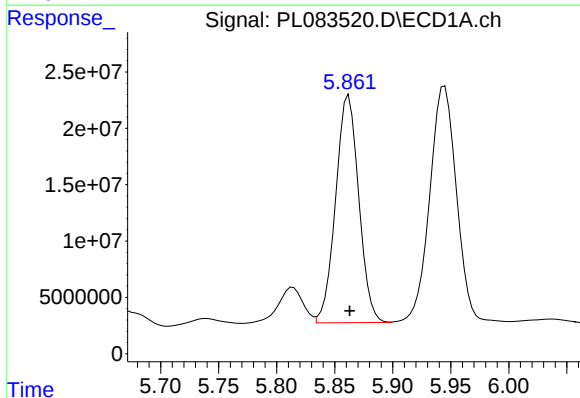


#25 Chlordane-3

R.T.: 5.862 min
Delta R.T.: 0.000 min
Response: 280121128
Conc: 724.51 ng/ml

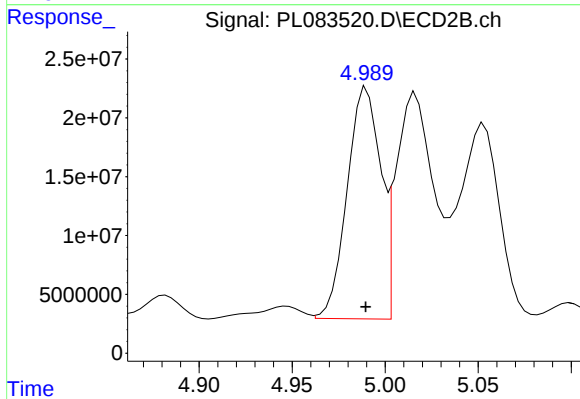

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 245376098
Conc: 740.95 ng/ml

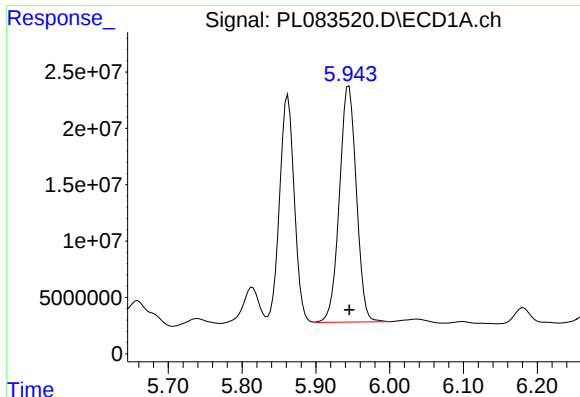

#26 Chlordane-4


R.T.: 5.945 min
Delta R.T.: -0.001 min
Response: 334755499
Conc: 718.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

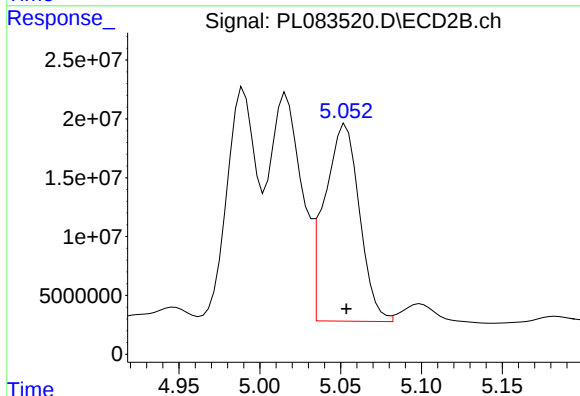


#26 Chlordane-4

R.T.: 5.053 min
Delta R.T.: 0.000 min
Response: 251154058
Conc: 739.37 ng/ml

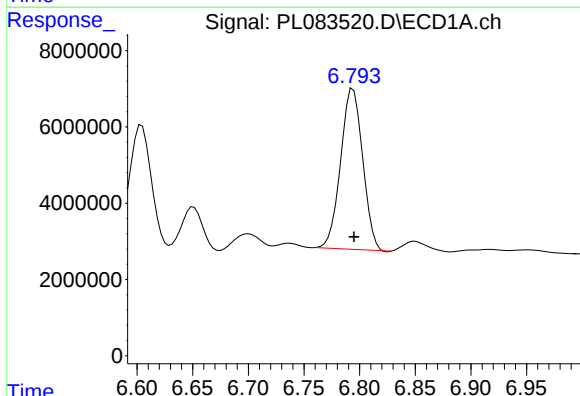


#27 Chlordane-5

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 57975553
Conc: 714.11 ng/ml

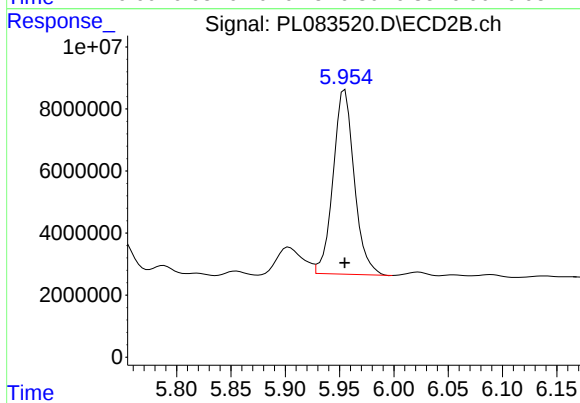

#27 Chlordane-5


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 80624463
Conc: 725.28 ng/ml

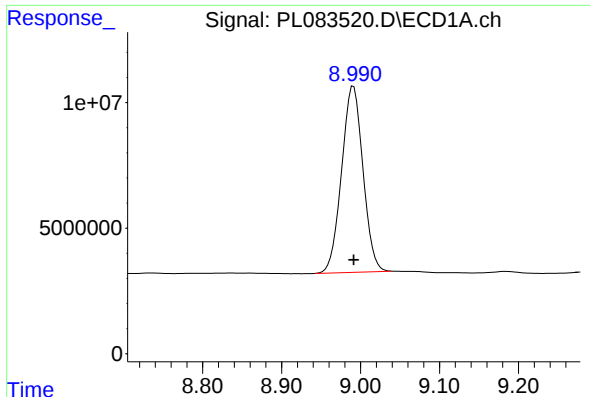

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.000 min
Response: 139575975
Conc: 70.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

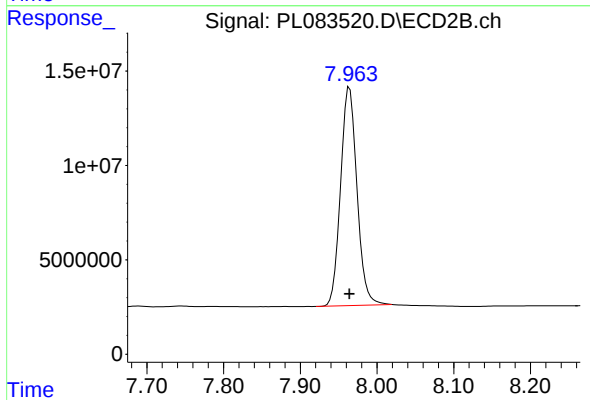

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 172594769
Conc: 70.27 ng/ml