

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
 Data File : PL083513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2023 06:43
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 12:37:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	2.752	52996959	55246149	23.977	23.717
28)	SA Decachlor...	8.990	7.964	45548732	57273061	23.903	23.319
Target Compounds							
9)	A Endosulfan I	5.990	5.108	26331295	30166593	11.817	11.193
10)	B gamma-Chl...	5.862	4.990	28145513	33618228	11.700	11.362
12)	B 4,4'-DDE	6.120	5.251	46209374	56208293	22.891	22.003
13)	MA Dieldrin	6.267	5.376	52240982	62915761	23.265	22.436
19)	B Endosulfa...	7.083	6.357	42740680	51016577	22.256	21.067
20)	A Methoxychlor	7.436	6.650	111.4E6	138.4E6	122.771	114.859
21)	B Endrin ke...	7.567	6.864	47899936	61305272	22.356	21.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
Data File : PL083513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2023 06:43
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 12:37:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

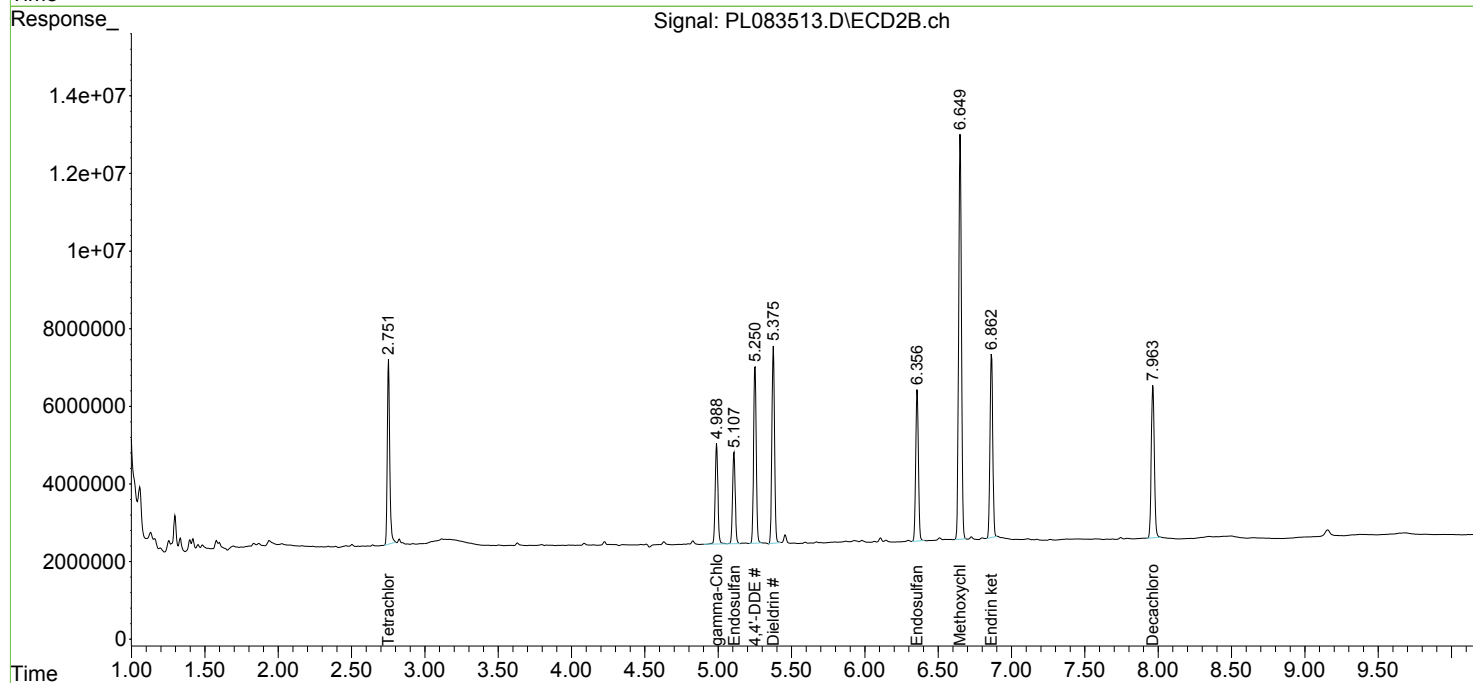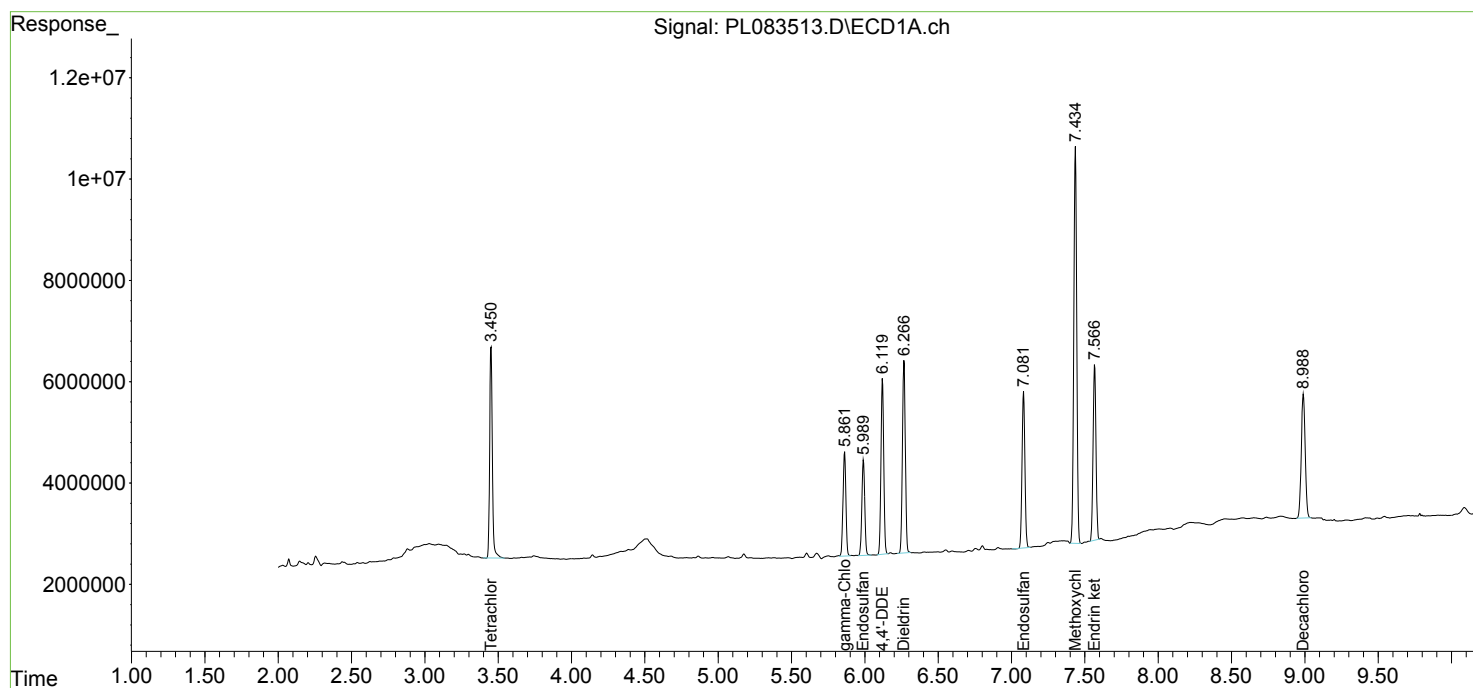


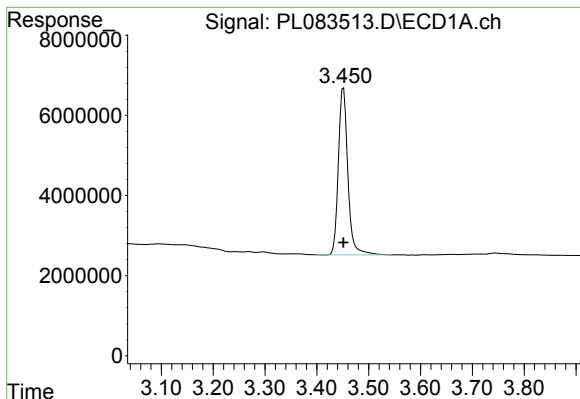

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 52996959
Conc: 23.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

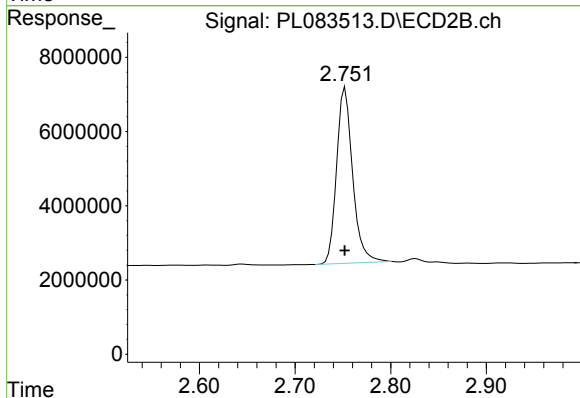


#1 Tetrachloro-m-xylene

R.T.: 2.752 min
Delta R.T.: 0.000 min
Response: 55246149
Conc: 23.72 ng/ml

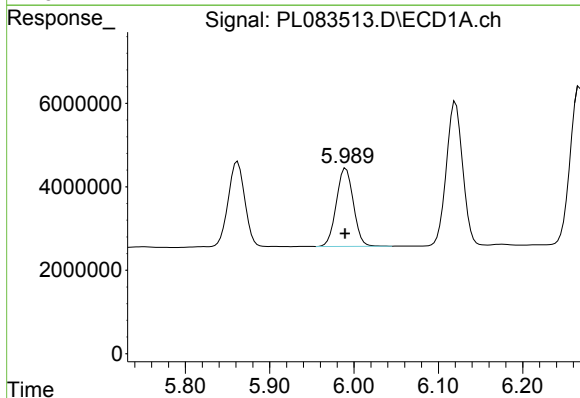


#9 Endosulfan I

R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 26331295
Conc: 11.82 ng/ml

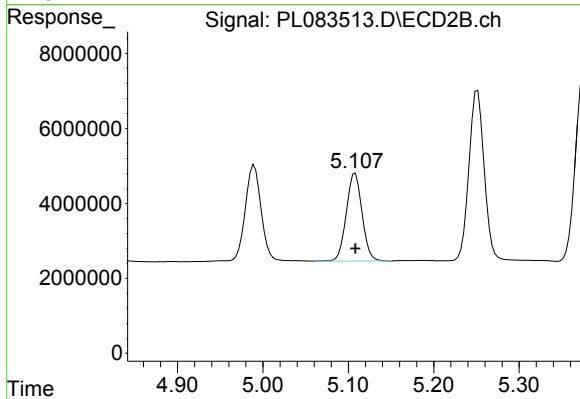

#9 Endosulfan I


R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 30166593
Conc: 11.19 ng/ml

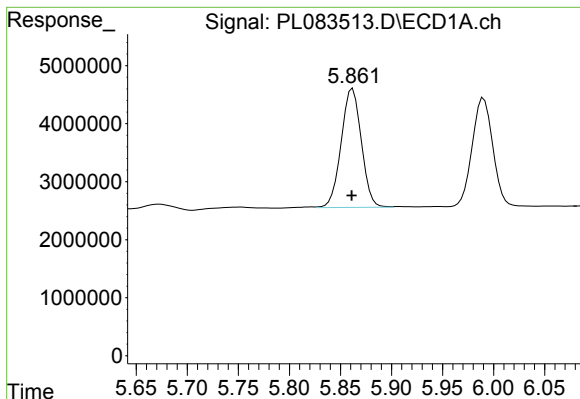

#10 gamma-Chlordane


R.T.: 5.862 min
Delta R.T.: 0.000 min
Response: 28145513
Conc: 11.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

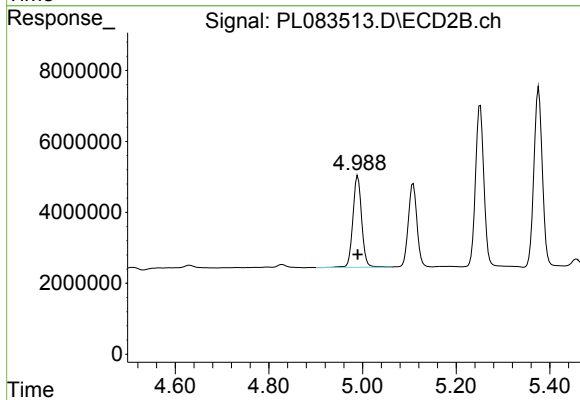


#10 gamma-Chlordane

R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 33618228
Conc: 11.36 ng/ml

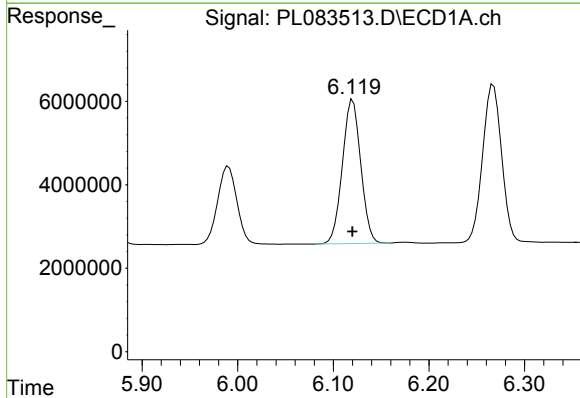


#12 4,4'-DDE

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 46209374
Conc: 22.89 ng/ml

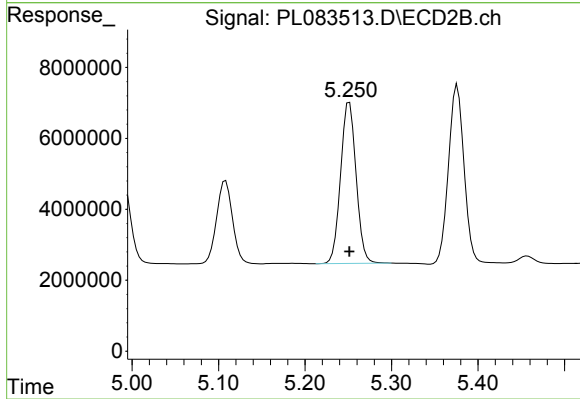

#12 4,4'-DDE


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 56208293
Conc: 22.00 ng/ml

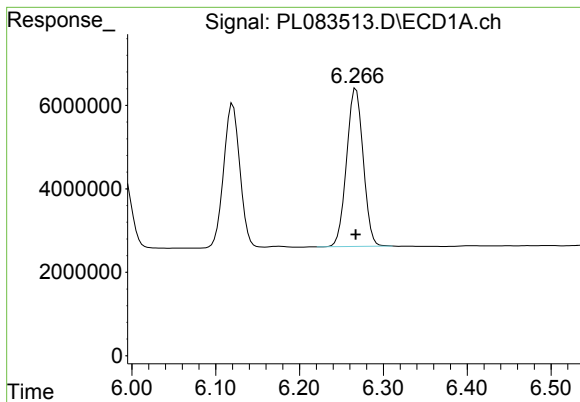

#13 Dieldrin


R.T.: 6.267 min
Delta R.T.: 0.000 min
Response: 52240982
Conc: 23.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

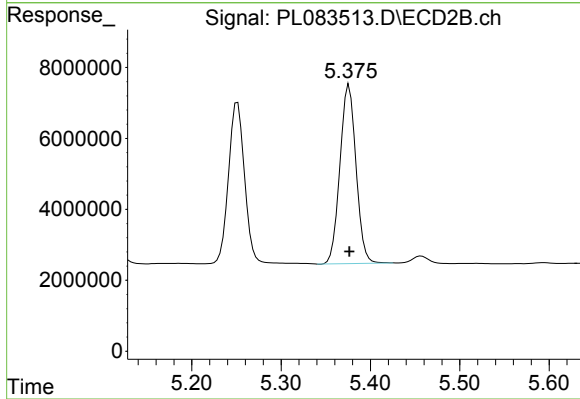


#13 Dieldrin

R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 62915761
Conc: 22.44 ng/ml

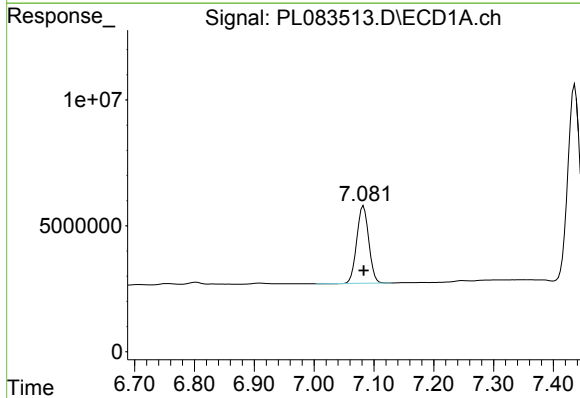


#19 Endosulfan Sulfate

R.T.: 7.083 min
Delta R.T.: 0.000 min
Response: 42740680
Conc: 22.26 ng/ml

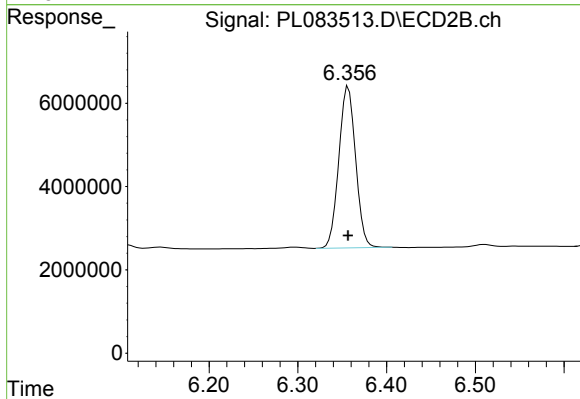

#19 Endosulfan Sulfate


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 51016577
Conc: 21.07 ng/ml

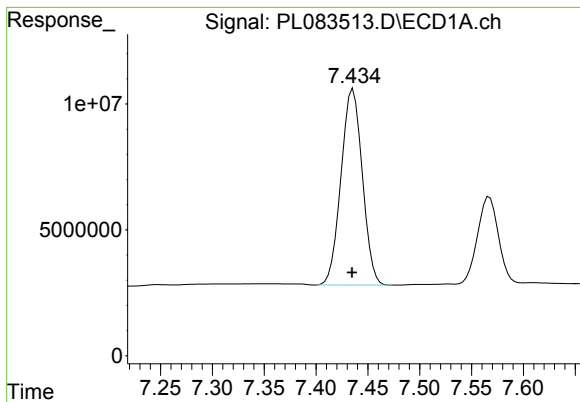

#20 Methoxychlor


R.T.: 7.436 min
Delta R.T.: 0.001 min
Response: 111361264
Conc: 122.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

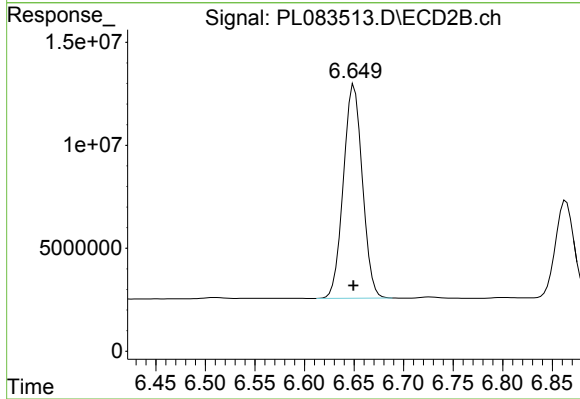


#20 Methoxychlor

R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 138425338
Conc: 114.86 ng/ml

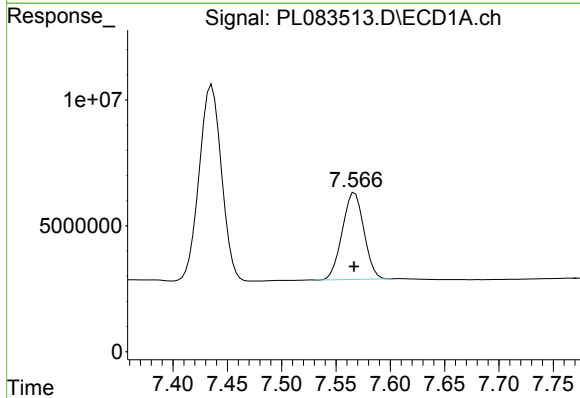


#21 Endrin ketone

R.T.: 7.567 min
Delta R.T.: 0.000 min
Response: 47899936
Conc: 22.36 ng/ml

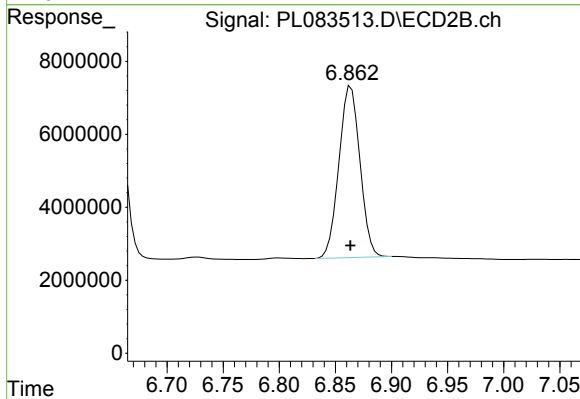

#21 Endrin ketone


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 61305272
Conc: 21.81 ng/ml

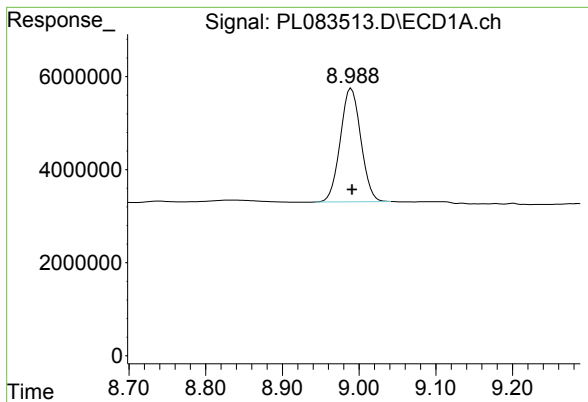

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: -0.001 min
Response: 45548732
Conc: 23.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

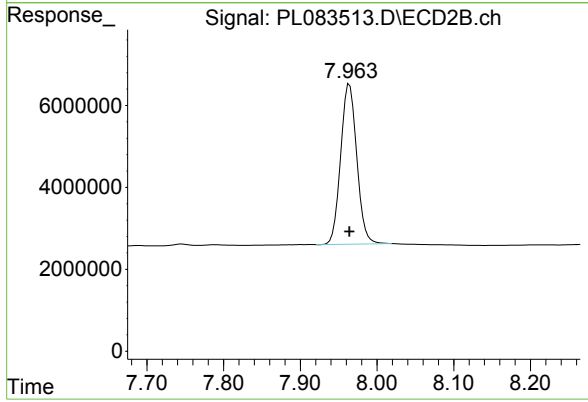

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 57273061
Conc: 23.32 ng/ml