

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
 Data File : PL083521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2023 08:33
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 12:24:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:22:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	2.750	113.4E6	149.5E6	50.000	50.000
28)	SA Decachlor...	8.992	7.964	99093916	122.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.618	3.765	49221007	49570797	500.000	500.000
24)	Chlordane-2	5.150	4.351	54102770	58571545	500.000	500.000
25)	Chlordane-3	5.863	4.990	193.3E6	165.6E6	500.000	500.000
26)	Chlordane-4	5.946	5.054	232.8E6	169.8E6	500.000	500.000
27)	Chlordane-5	6.795	5.955	40592892	55581327	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
Data File : PL083521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2023 08:33
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 12:24:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:22:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

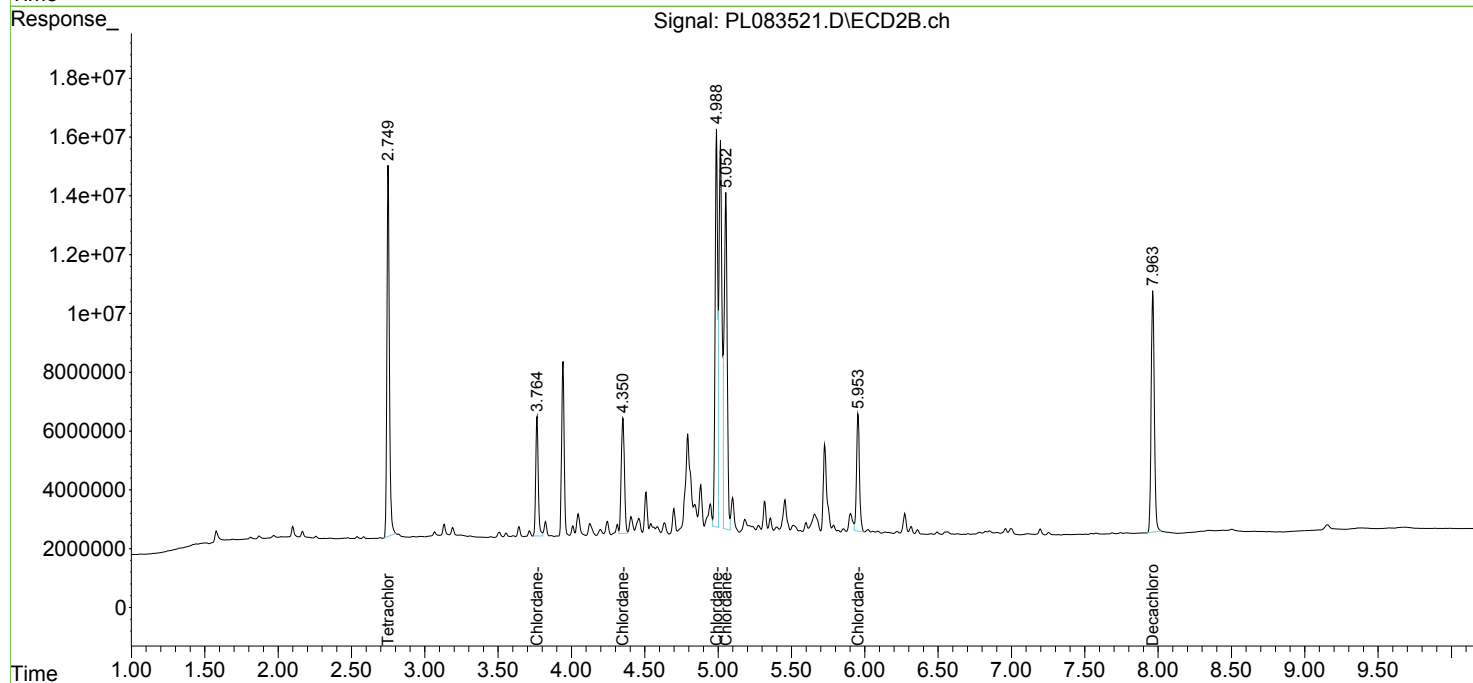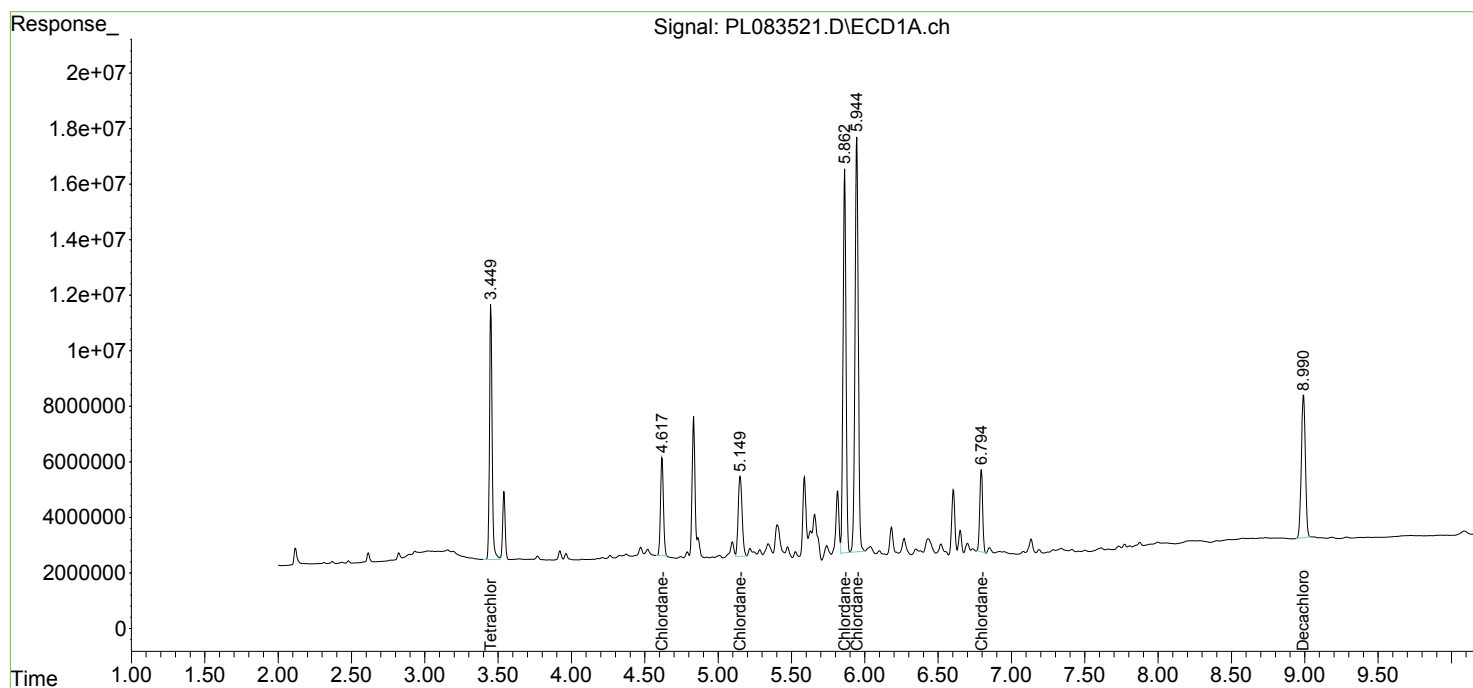


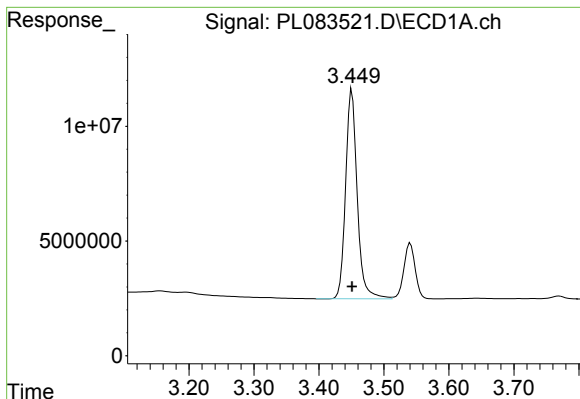

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 113443636
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

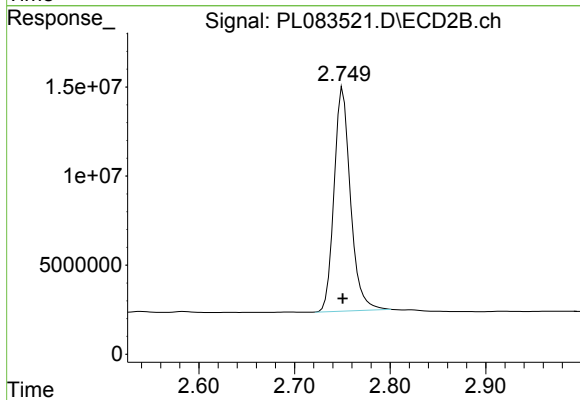


#1 Tetrachloro-m-xylene

R.T.: 2.750 min
Delta R.T.: 0.000 min
Response: 149531879
Conc: 50.00 ng/ml

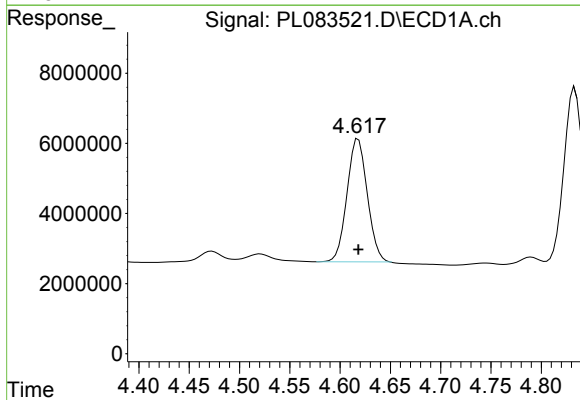


#23 Chlordane-1

R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 49221007
Conc: 500.00 ng/ml

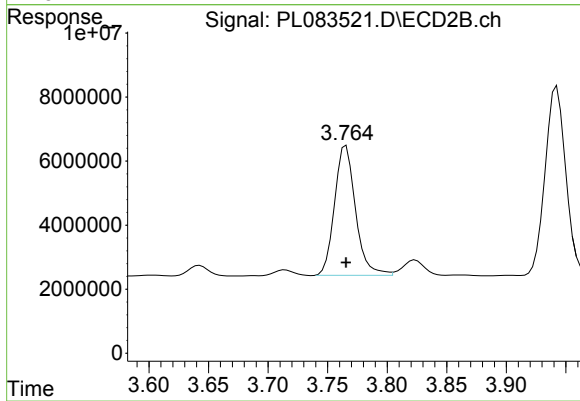

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: 0.000 min
Response: 49570797
Conc: 500.00 ng/ml

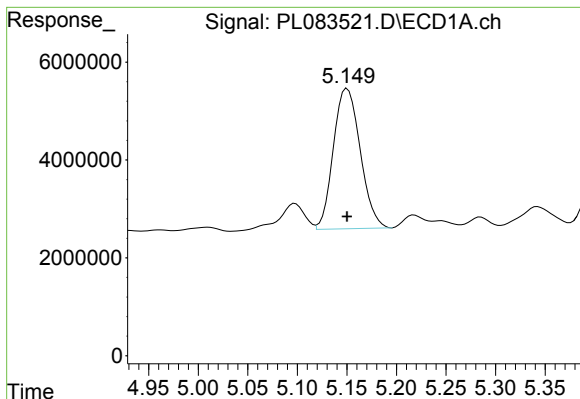

#24 Chlordane-2


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 54102770
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

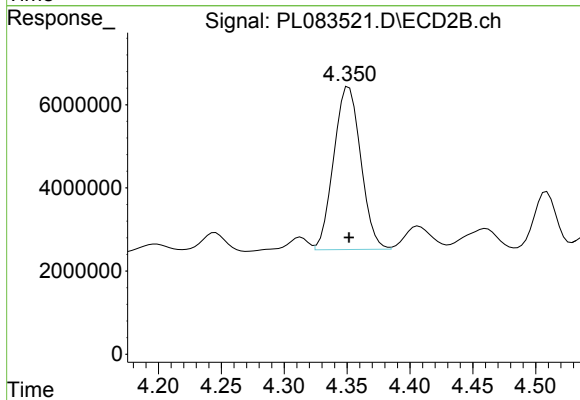


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 58571545
Conc: 500.00 ng/ml

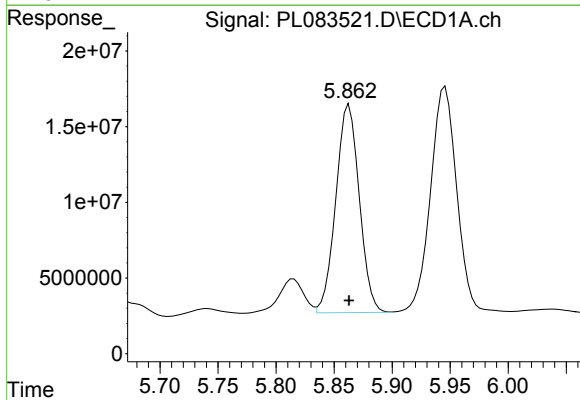


#25 Chlordane-3

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 193318520
Conc: 500.00 ng/ml

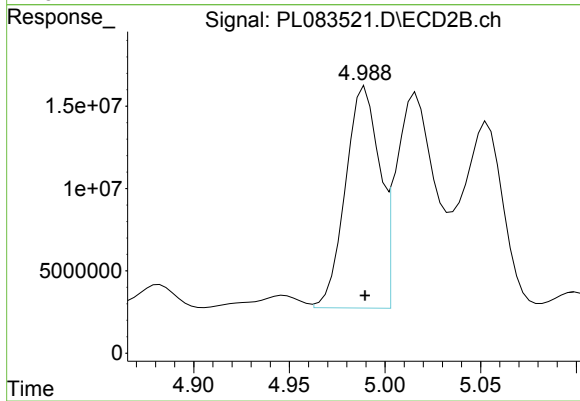

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 165582535
Conc: 500.00 ng/ml

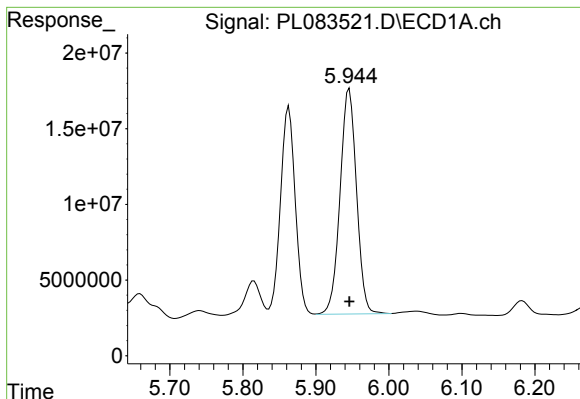

#26 Chlordane-4


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 232795569
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

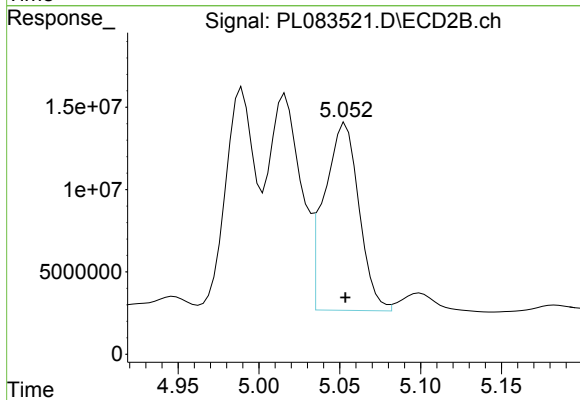


#26 Chlordane-4

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 169844316
Conc: 500.00 ng/ml

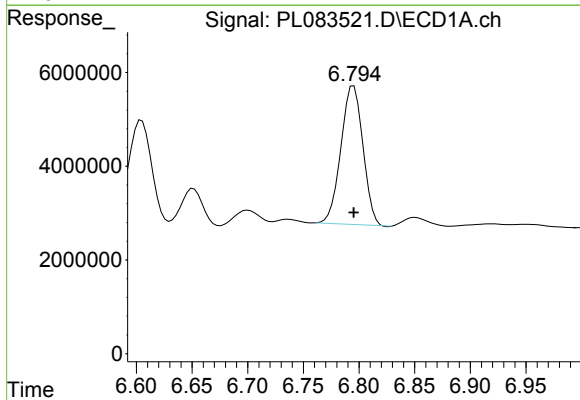


#27 Chlordane-5

R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 40592892
Conc: 500.00 ng/ml

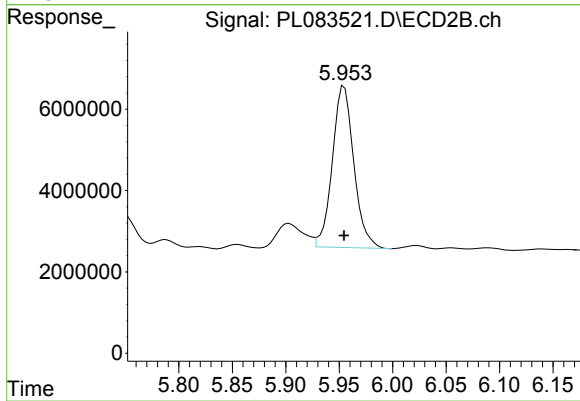

#27 Chlordane-5

R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 55581327
Conc: 500.00 ng/ml

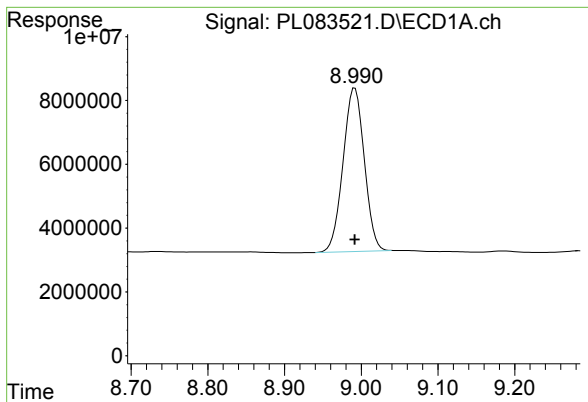

#28 Decachlorobiphenyl


R.T.: 8.992 min

Delta R.T.: 0.000 min

Response: 99093916

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

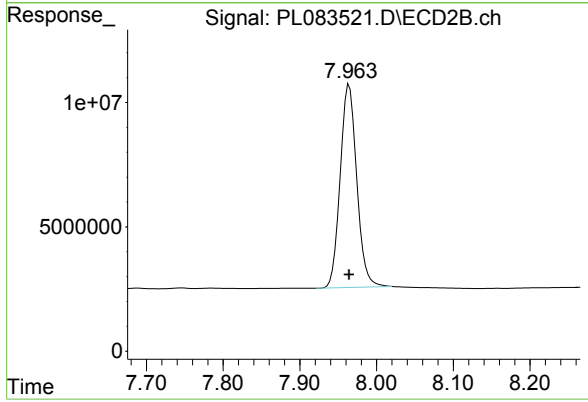

#28 Decachlorobiphenyl

R.T.: 7.964 min

Delta R.T.: 0.000 min

Response: 122812349

Conc: 50.00 ng/ml