

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
 Data File : PL083522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2023 08:47
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 12:30:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:22:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	2.751	55610953	71522650	24.925	24.336
28)	SA Decachlor...	8.990	7.964	50683087	62830634	26.151	26.244
Target Compounds							
23)	Chlordane-1	4.618	3.766	24074536	24214900	250.060	249.224
24)	Chlordane-2	5.151	4.351	27652022	30130493	262.860	259.616
25)	Chlordane-3	5.863	4.990	92593938	78555543	243.481	239.400
26)	Chlordane-4	5.946	5.053	113.2E6	80449205	247.719	239.190
27)	Chlordane-5	6.795	5.955	19937114	27170321	250.199	246.447



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061723\
Data File : PL083522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2023 08:47
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 12:30:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:22:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

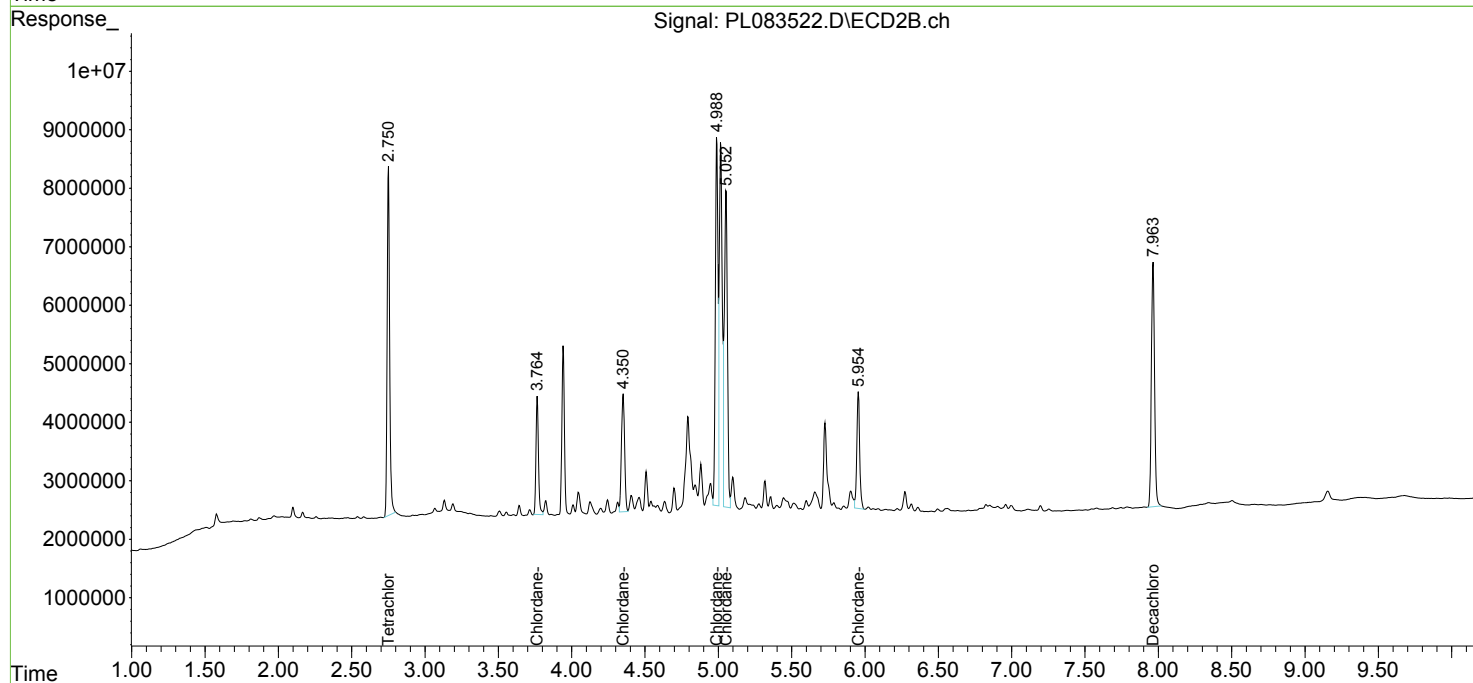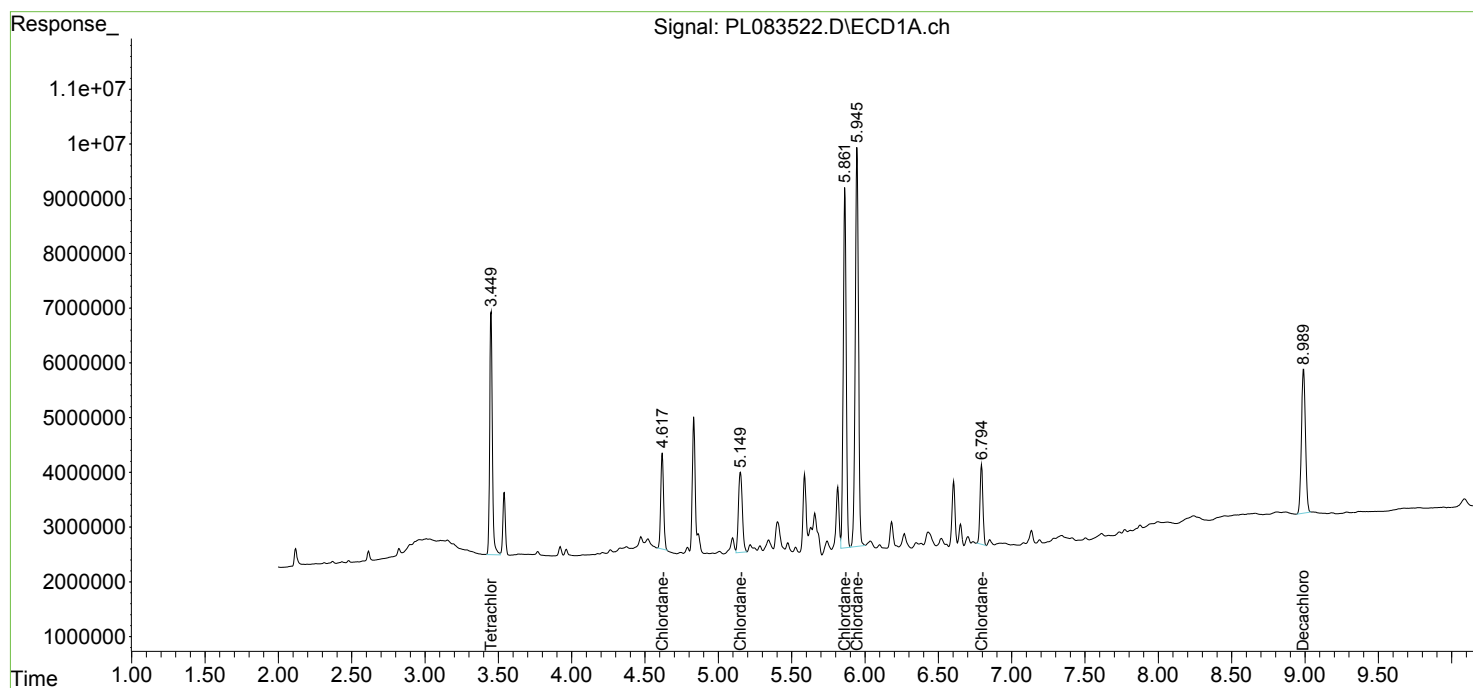


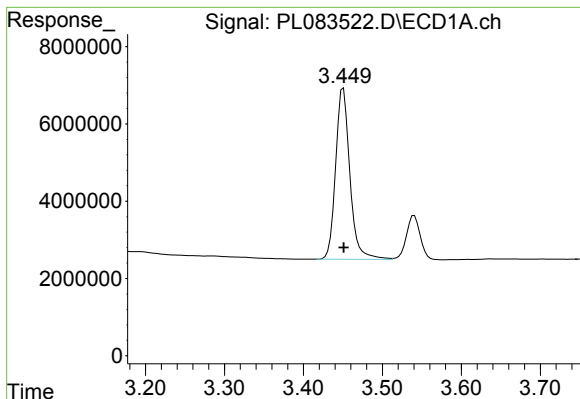

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 55610953
Conc: 24.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

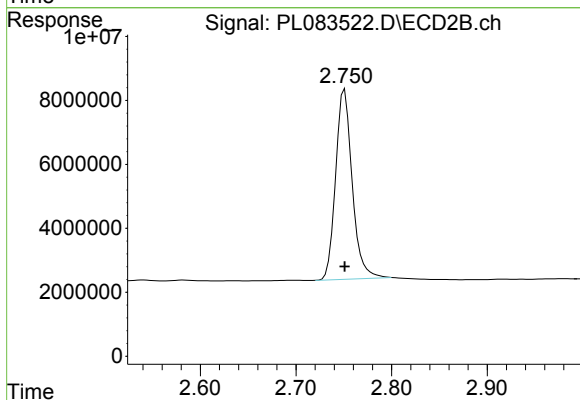


#1 Tetrachloro-m-xylene

R.T.: 2.751 min
Delta R.T.: 0.000 min
Response: 71522650
Conc: 24.34 ng/ml

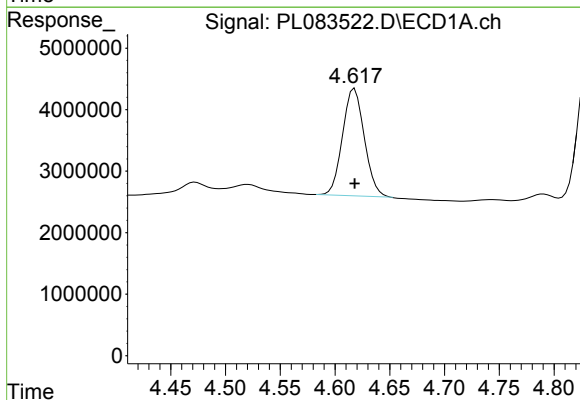


#23 Chlordane-1

R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 24074536
Conc: 250.06 ng/ml

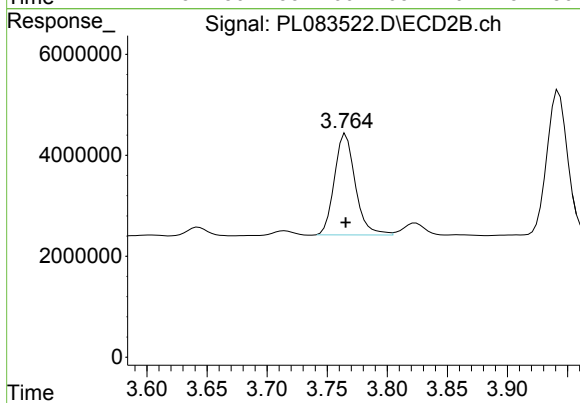

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 24214900
Conc: 249.22 ng/ml

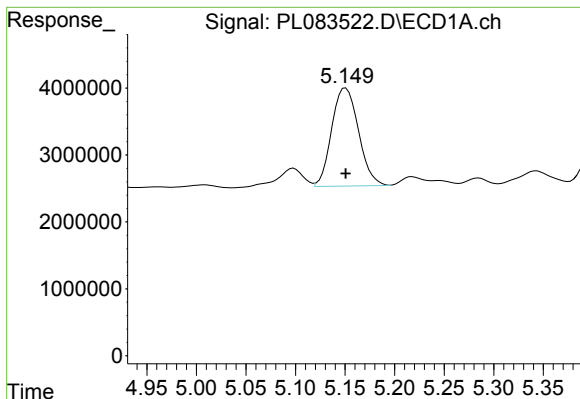

#24 Chlordane-2


R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 27652022
Conc: 262.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

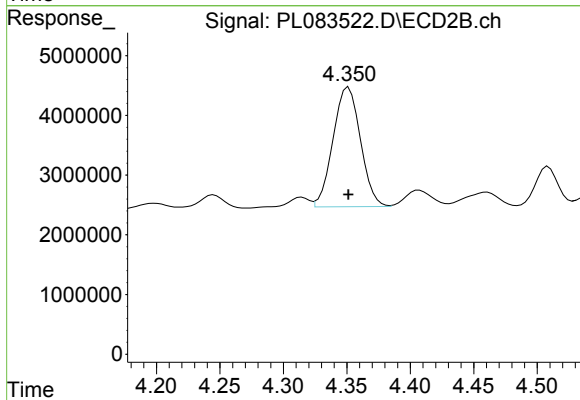


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 30130493
Conc: 259.62 ng/ml

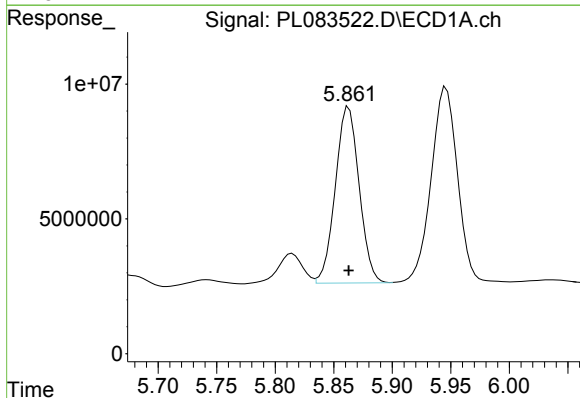


#25 Chlordane-3

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 92593938
Conc: 243.48 ng/ml

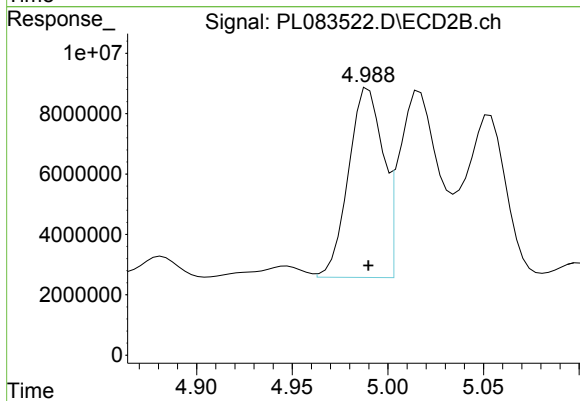

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 78555543
Conc: 239.40 ng/ml

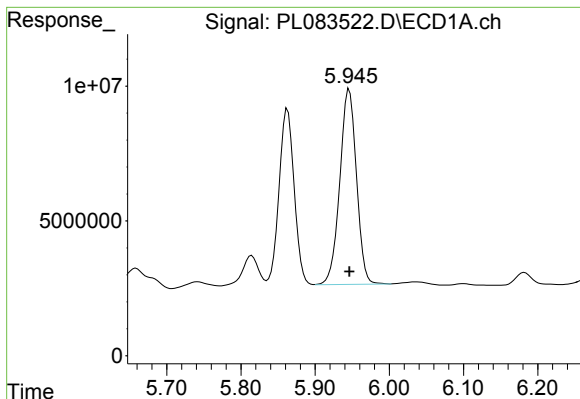

#26 Chlordane-4


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 113216286
Conc: 247.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

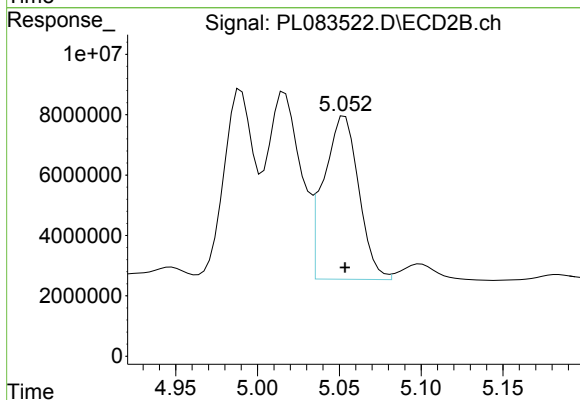


#26 Chlordane-4

R.T.: 5.053 min
Delta R.T.: 0.000 min
Response: 80449205
Conc: 239.19 ng/ml

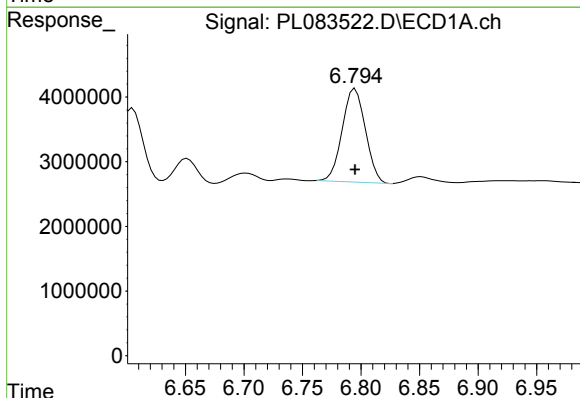


#27 Chlordane-5

R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 19937114
Conc: 250.20 ng/ml

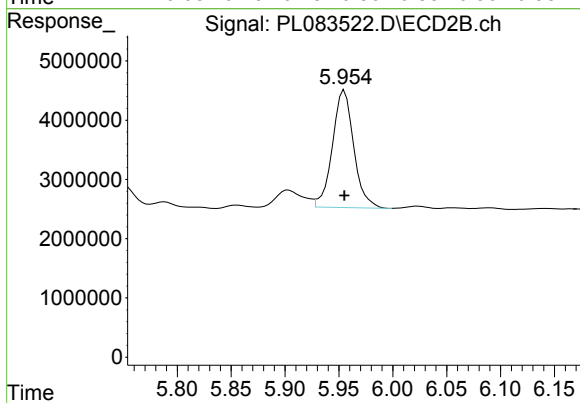

#27 Chlordane-5


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 27170321
Conc: 246.45 ng/ml

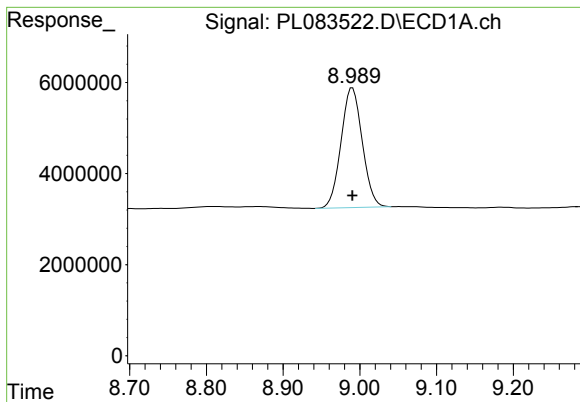

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 50683087
Conc: 26.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

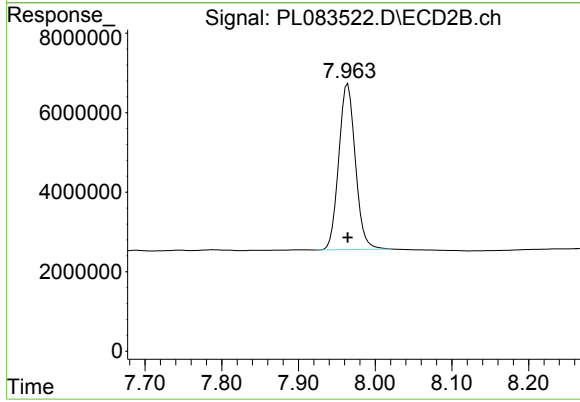

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 62830634
Conc: 26.24 ng/ml