

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061724\
 Data File : PL090205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2024 18:46
 Operator : AR\AJ
 Sample : P2887-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-06132024

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/18/2024
 Supervised By : Ankita Jodhani 06/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:36:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.792	26429090	17411029	12.623m	12.143
28) SA Decachlor...	9.059	7.936	18429911	17253885	12.534	11.611

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061724\
Data File : PL090205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2024 18:46
Operator : AR\AJ
Sample : P2887-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-01-06132024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/18/2024
Supervised By : Ankita Jodhani 06/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:36:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

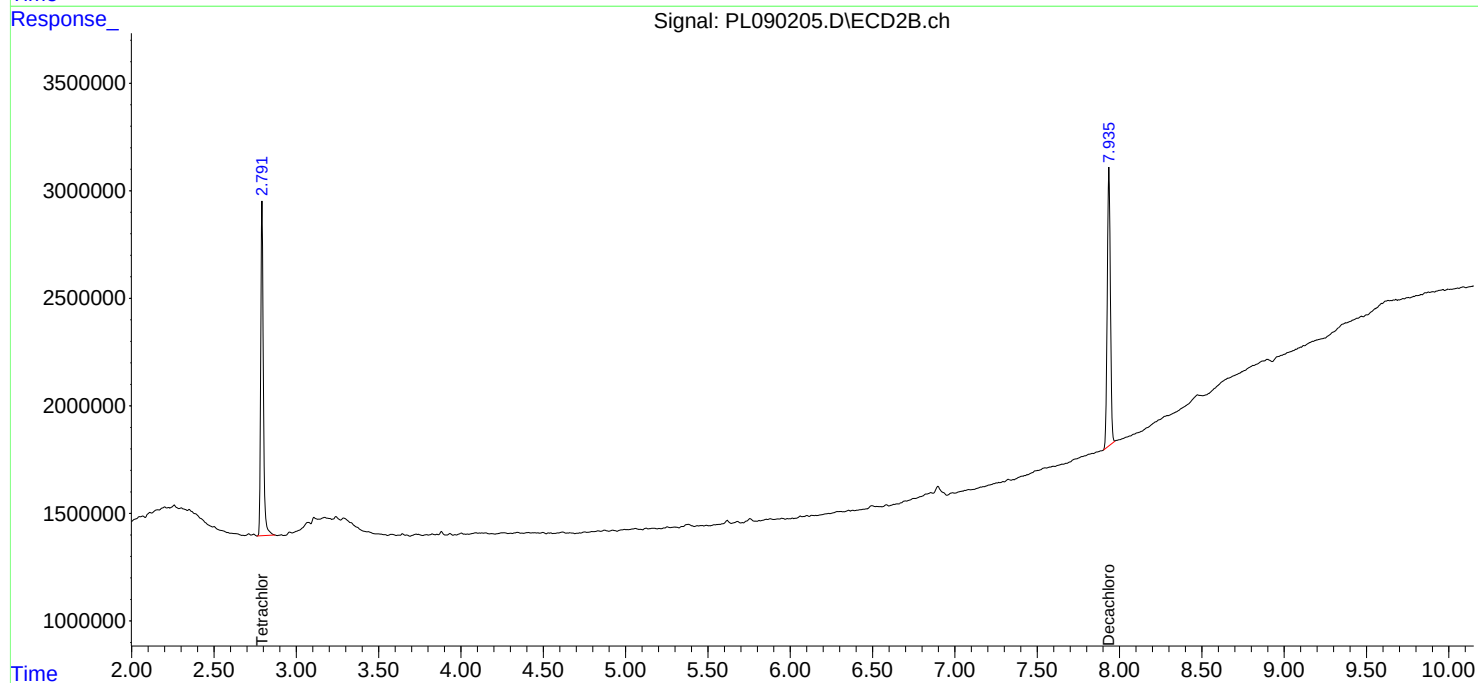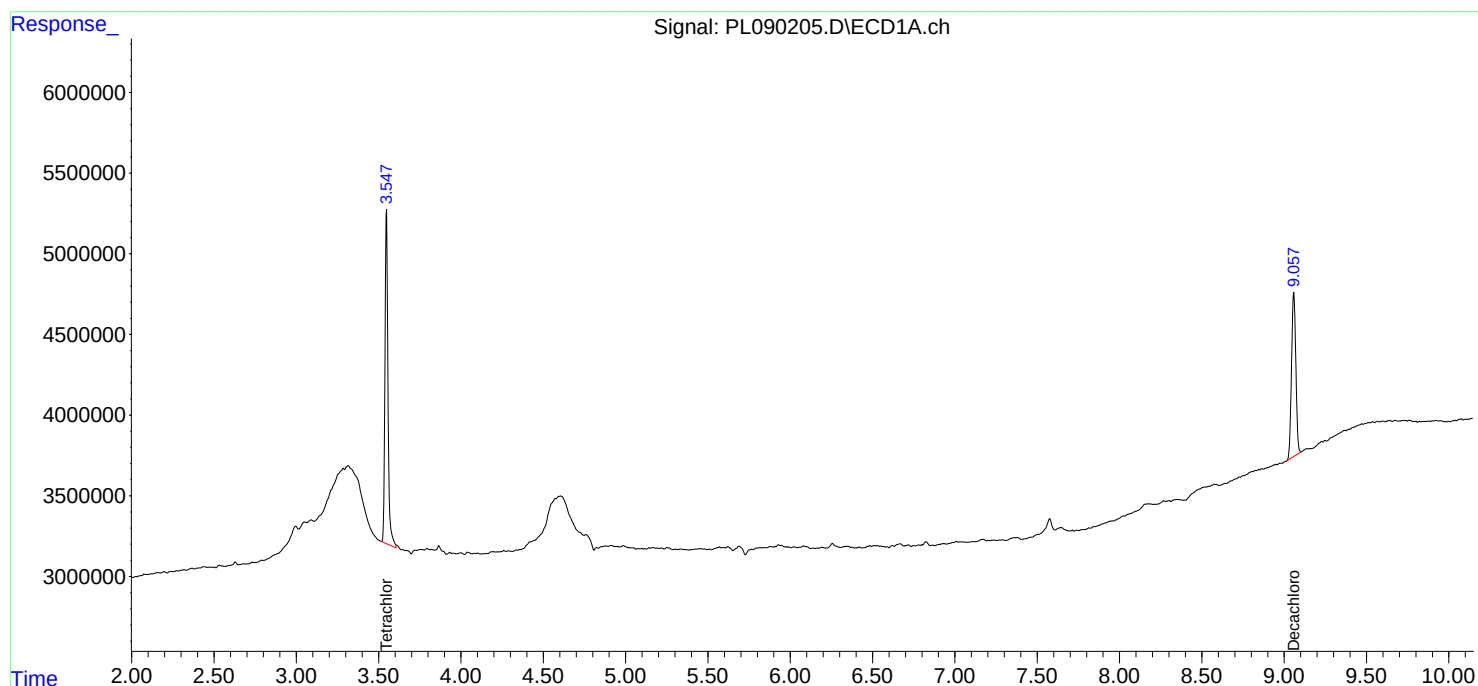

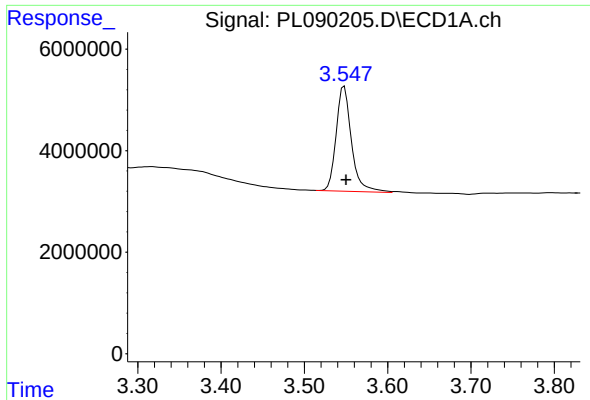


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: -0.003 min
Response: 26429090
Conc: 12.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-06132024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/18/2024
Supervised By :Ankita Jodhani 06/18/2024

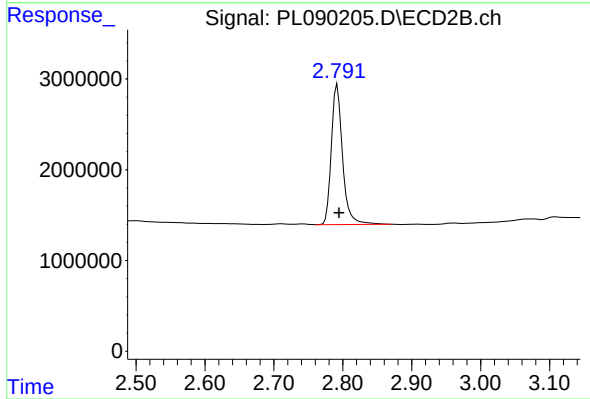


#1 Tetrachloro-m-xylene

R.T.: 2.792 min
Delta R.T.: -0.003 min
Response: 17411029
Conc: 12.14 ng/ml

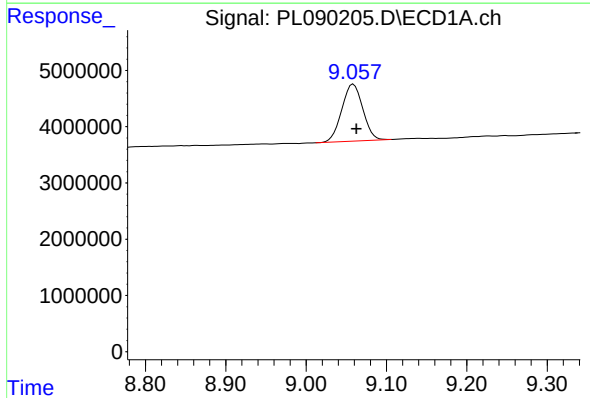

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.004 min
Response: 18429911
Conc: 12.53 ng/ml

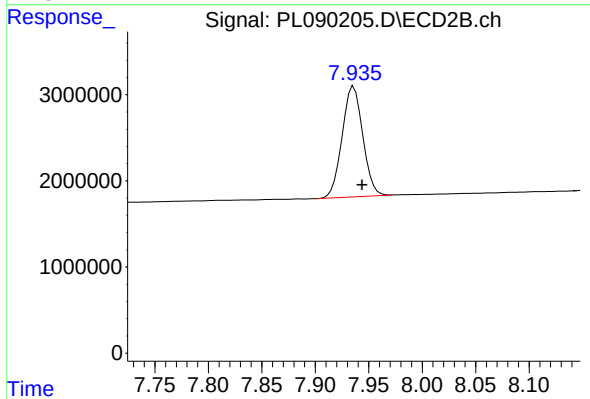

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: -0.008 min
Response: 17253885
Conc: 11.61 ng/ml