

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
 Data File : PL096064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 14:13
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 15:03:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 14:59:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.881	251.6E6	434.8E6	75.099	75.261
28)	SA Decachlor...	9.112	8.064	188.6E6	411.6E6	74.193	74.328
Target Compounds							
23)	Chlordane-1	4.736	3.899	151.5E6	172.8E6	751.142	751.751
24)	Chlordane-2	5.264	4.480	156.6E6	193.2E6	747.671	748.475
25)	Chlordane-3	5.970	5.116	628.1E6	614.5E6	750.404	748.790
26)	Chlordane-4	6.055	5.180	736.2E6	536.8E6	748.835	751.887
27)	Chlordane-5	6.895	6.078	129.1E6	228.2E6	746.642	746.974



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
Data File : PL096064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 14:13
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 15:03:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 14:59:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

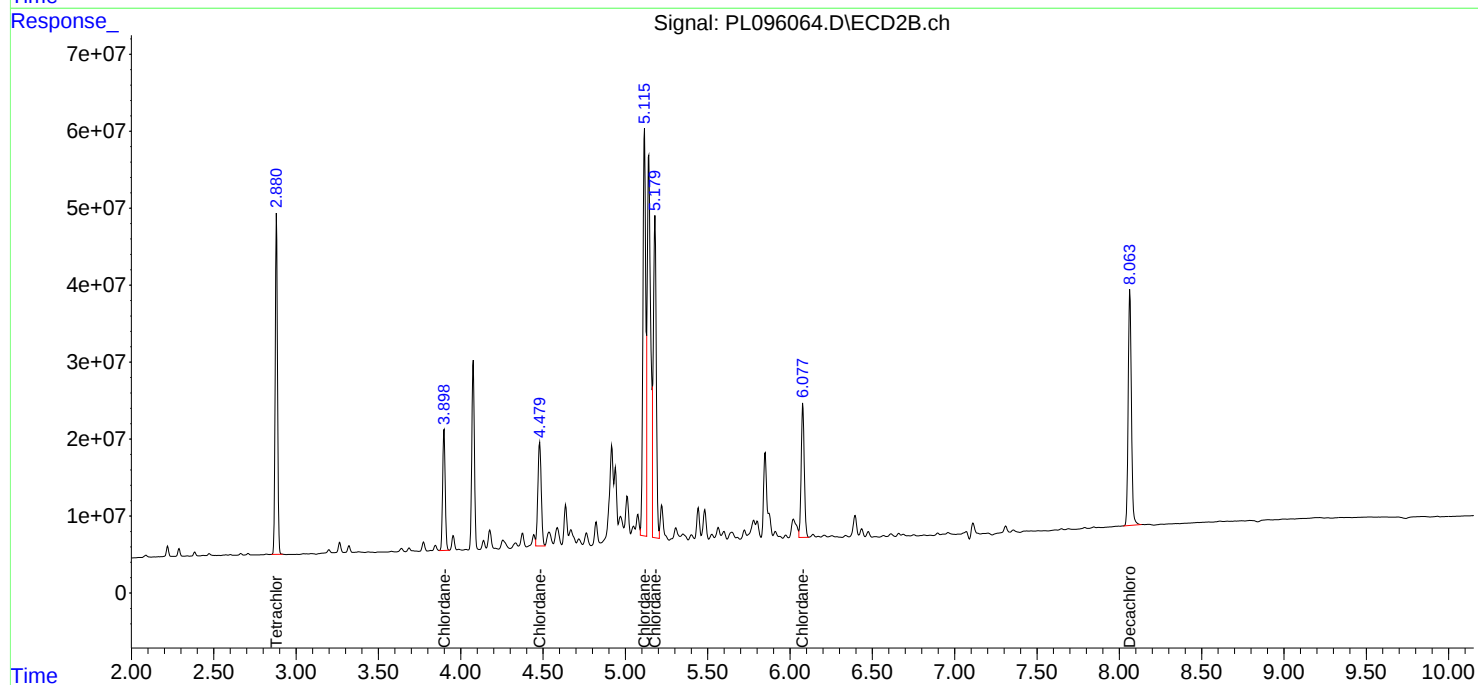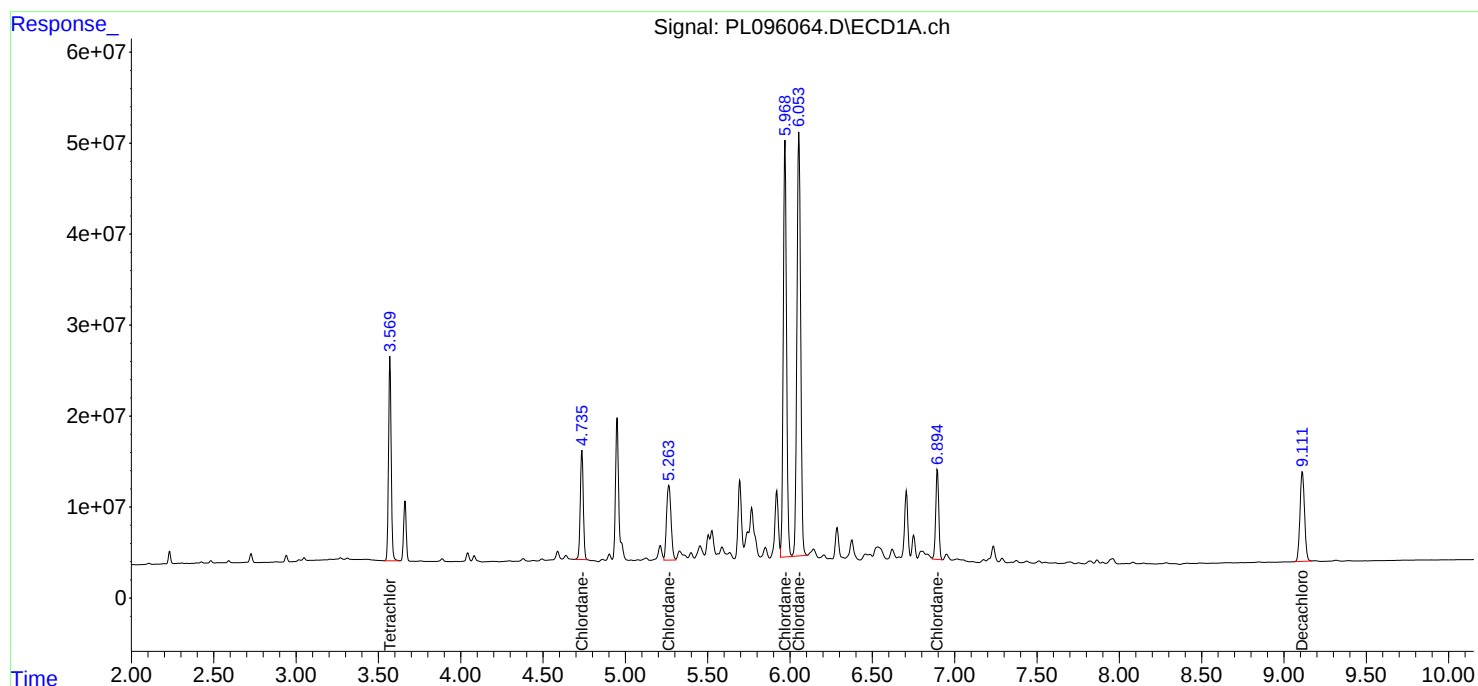


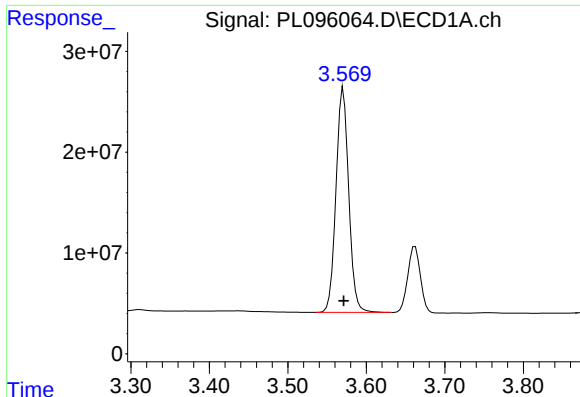

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 251555976
Conc: 75.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

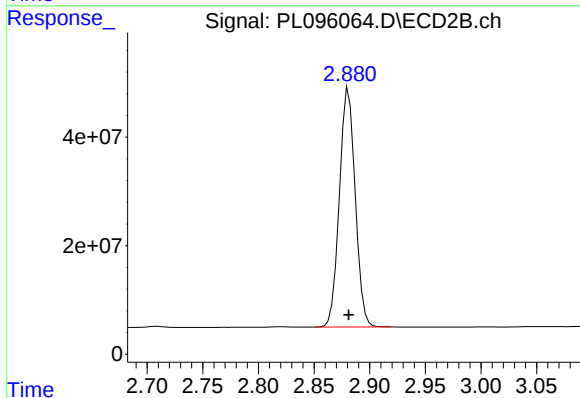


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 434822780
Conc: 75.26 ng/ml

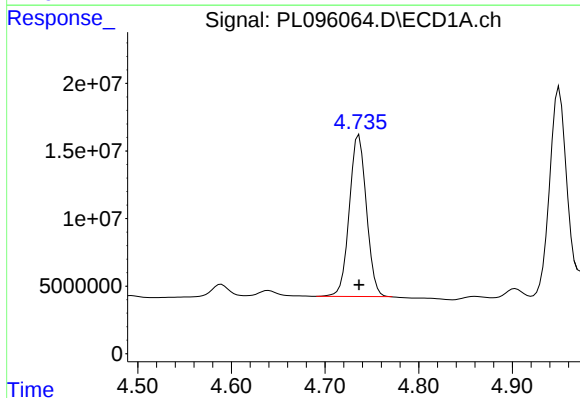


#23 Chlordane-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 151510351
Conc: 751.14 ng/ml

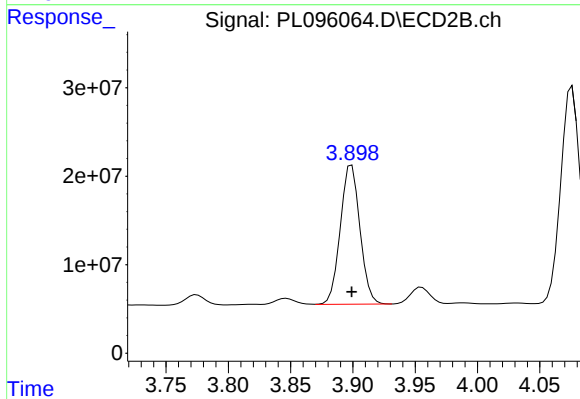

#23 Chlordane-1


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 172818715
Conc: 751.75 ng/ml

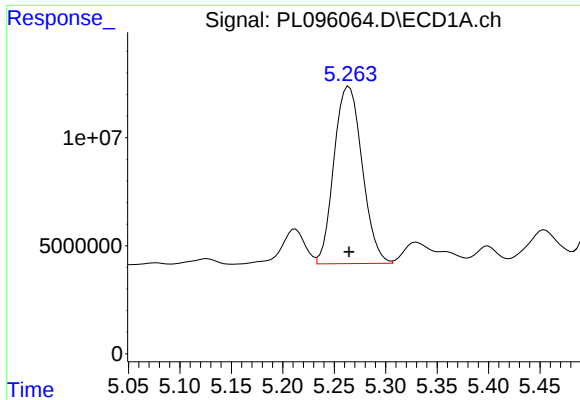

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 156610535
Conc: 747.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

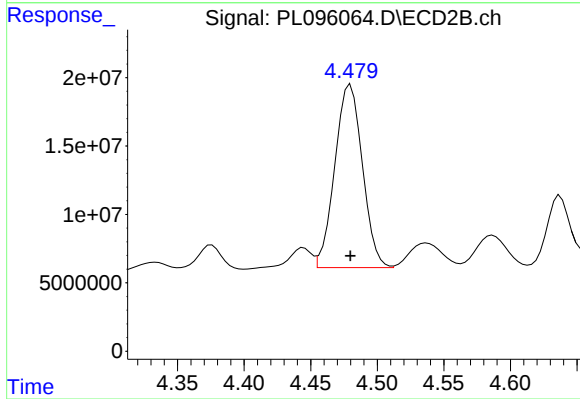


#24 Chlordane-2

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 193198514
Conc: 748.47 ng/ml

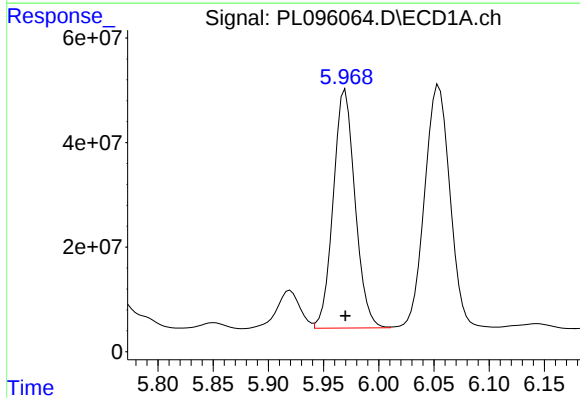


#25 Chlordane-3

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 628050960
Conc: 750.40 ng/ml

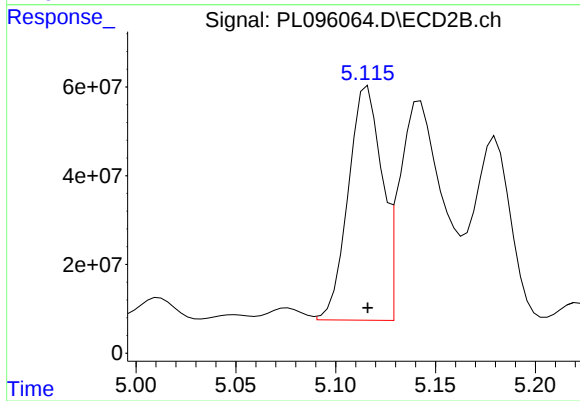

#25 Chlordane-3


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 614465311
Conc: 748.79 ng/ml

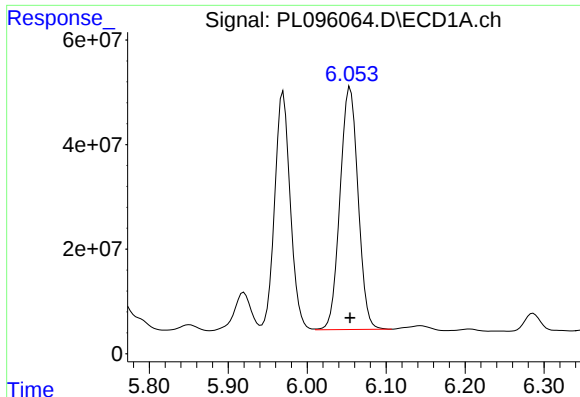

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 736177373
Conc: 748.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

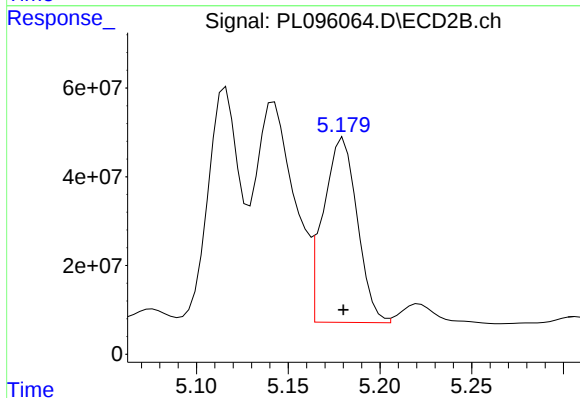


#26 Chlordane-4

R.T.: 5.180 min
Delta R.T.: 0.000 min
Response: 536805329
Conc: 751.89 ng/ml

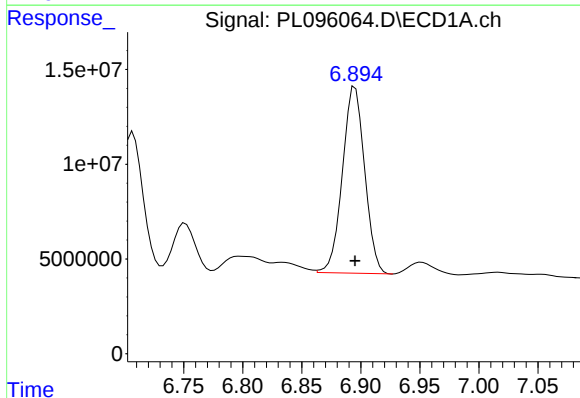


#27 Chlordane-5

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 129053295
Conc: 746.64 ng/ml

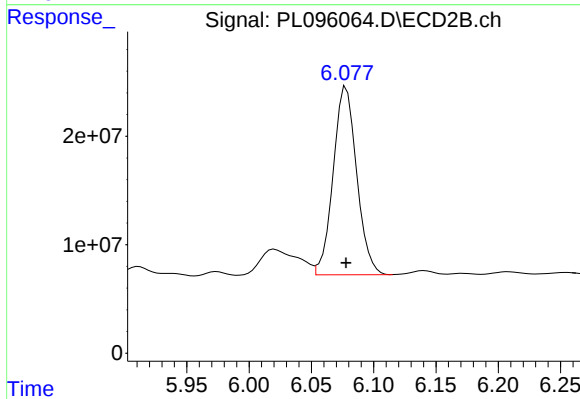

#27 Chlordane-5


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 228185326
Conc: 746.97 ng/ml

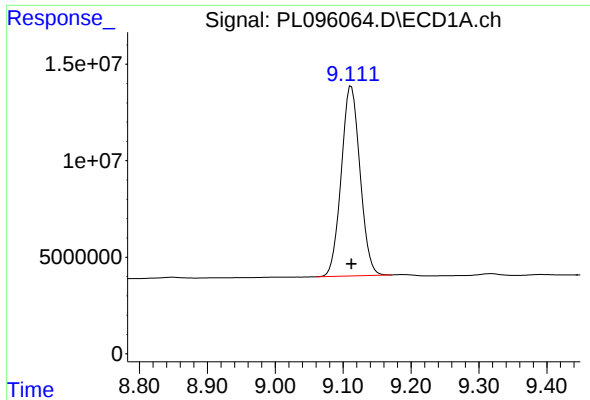

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 188561099
Conc: 74.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

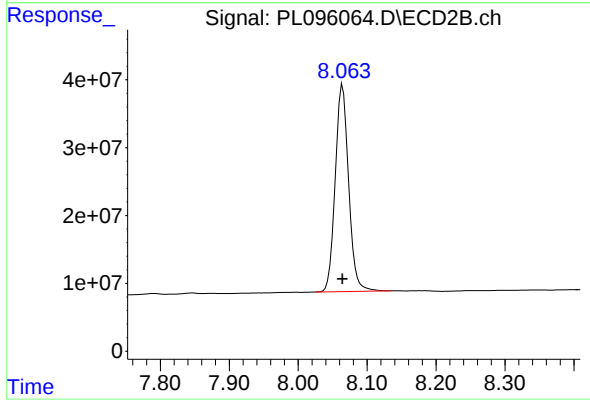

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 411580380
Conc: 74.33 ng/ml