

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
 Data File : PL096066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 14:41
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 15:05:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 14:59:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.881	82077896	138.6E6	24.626	24.230
28)	SA Decachlor...	9.113	8.064	65640074	137.7E6	25.616	24.901
Target Compounds							
23)	Chlordane-1	4.736	3.899	49352215	54986192	245.983	241.801
24)	Chlordane-2	5.263	4.480	52790934	63756414	251.518	247.743
25)	Chlordane-3	5.969	5.116	197.8E6	190.6E6	239.606	236.459
26)	Chlordane-4	6.054	5.180	236.7E6	169.4E6	243.007	240.357
27)	Chlordane-5	6.895	6.078	43228271	72624608	250.074	240.691



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
Data File : PL096066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 14:41
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 15:05:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 14:59:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

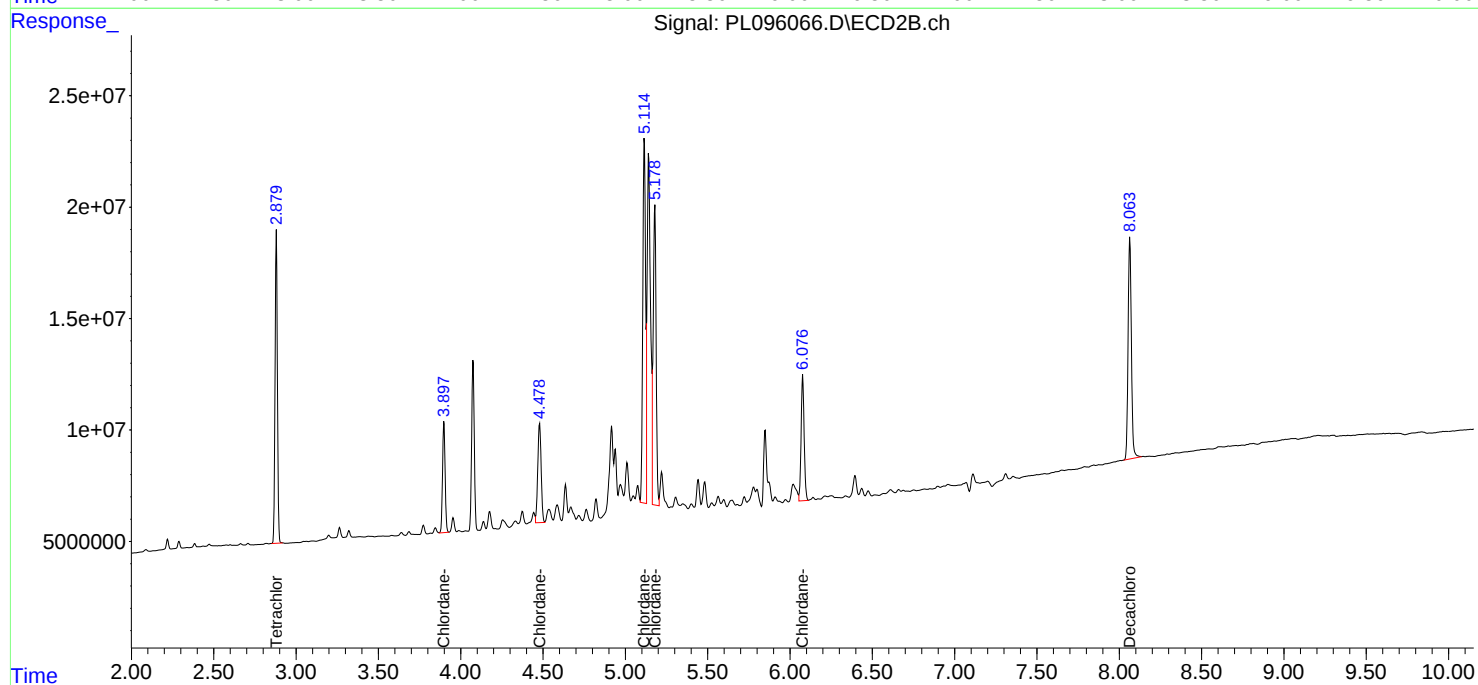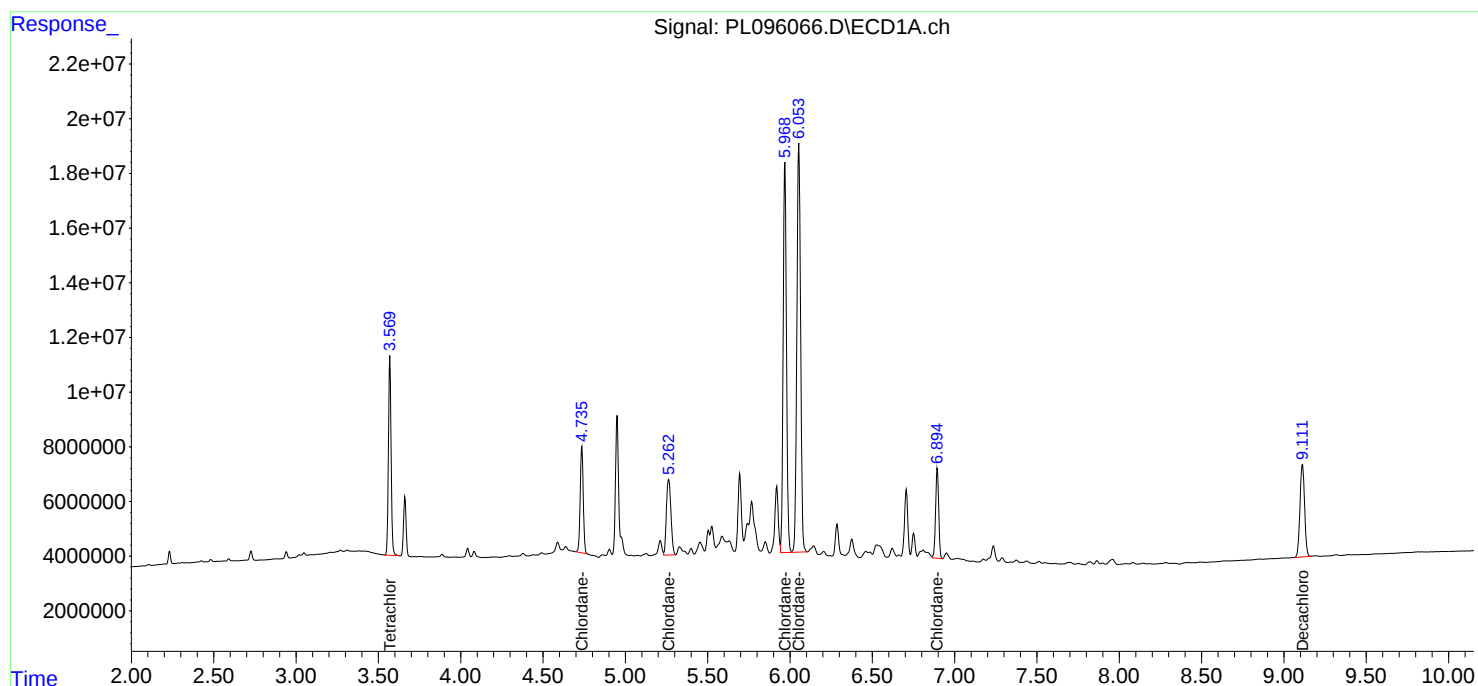


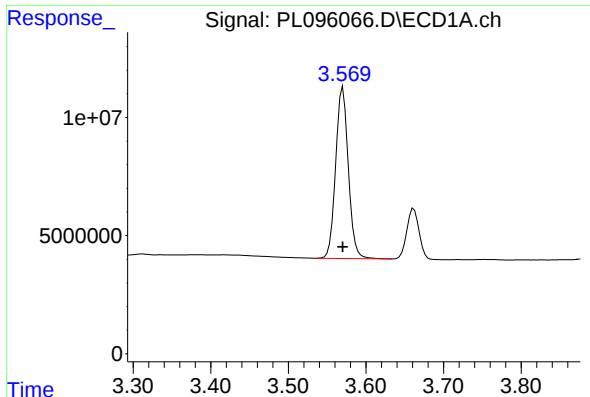

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 82077896
Conc: 24.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

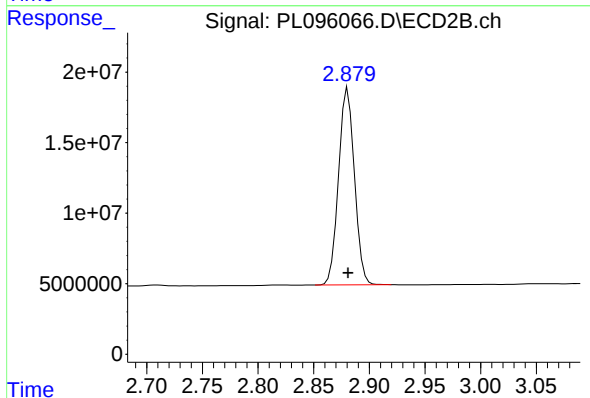


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 138567316
Conc: 24.23 ng/ml

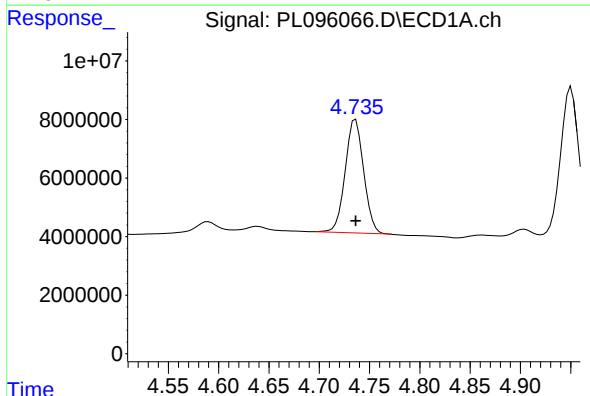


#23 Chlordane-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 49352215
Conc: 245.98 ng/ml

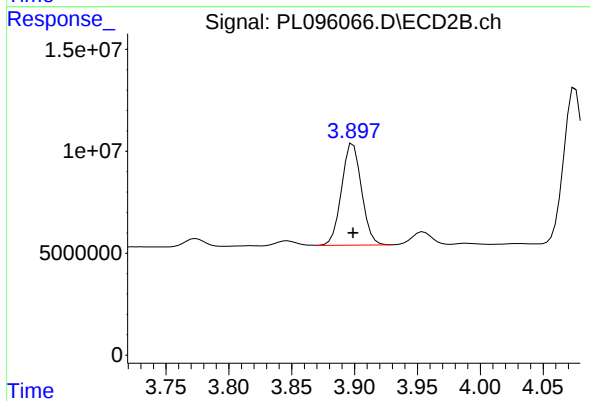

#23 Chlordane-1


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 54986192
Conc: 241.80 ng/ml

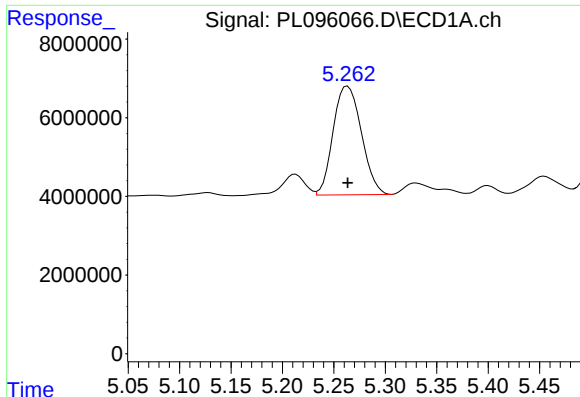

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 52790934
Conc: 251.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

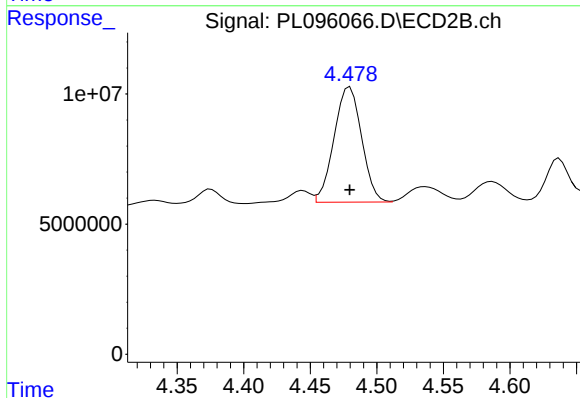


#24 Chlordane-2

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 63756414
Conc: 247.74 ng/ml

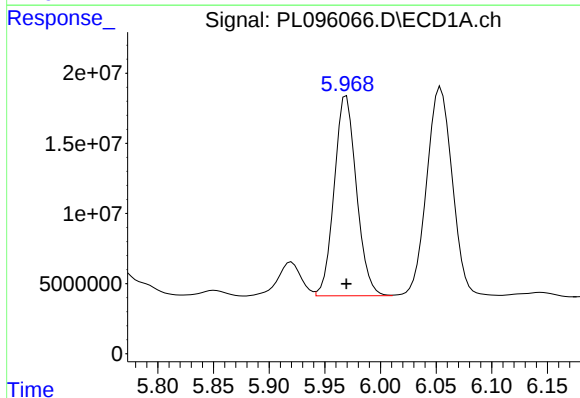


#25 Chlordane-3

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 197796754
Conc: 239.61 ng/ml

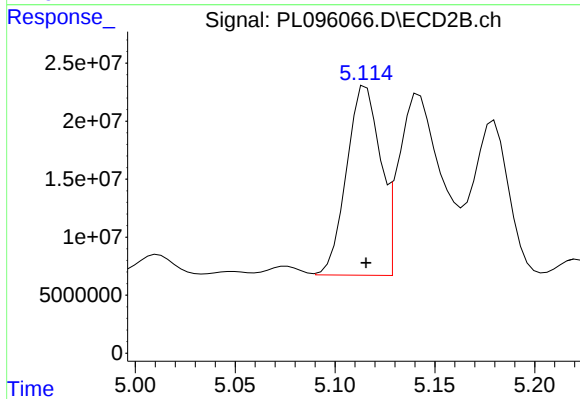

#25 Chlordane-3


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 190599244
Conc: 236.46 ng/ml

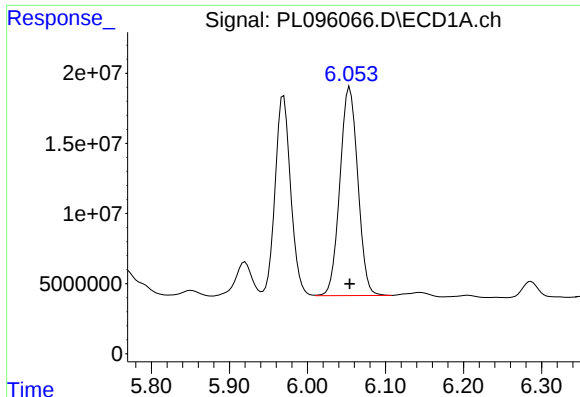

#26 Chlordane-4


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 236692497
Conc: 243.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

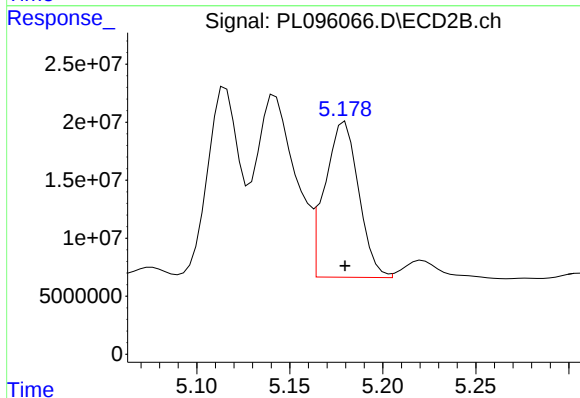


#26 Chlordane-4

R.T.: 5.180 min
Delta R.T.: 0.000 min
Response: 169422900
Conc: 240.36 ng/ml

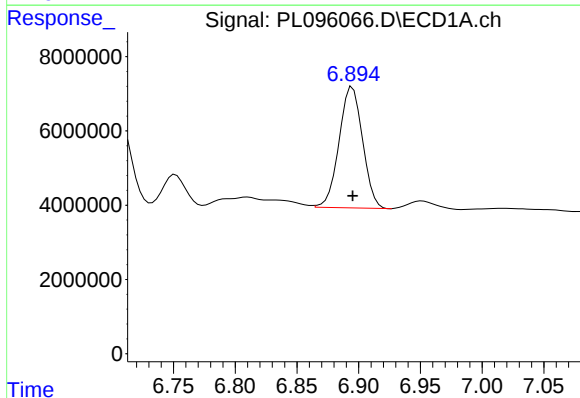


#27 Chlordane-5

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 43228271
Conc: 250.07 ng/ml

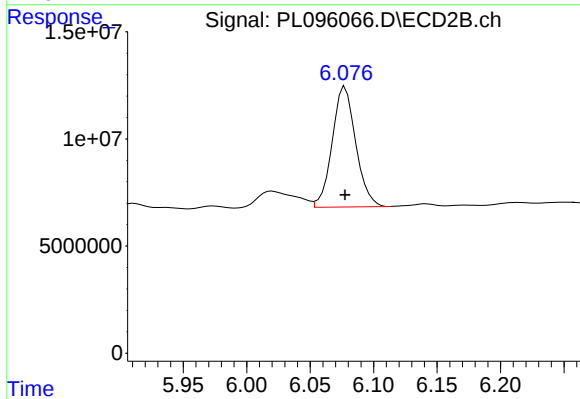

#27 Chlordane-5

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 72624608
Conc: 240.69 ng/ml

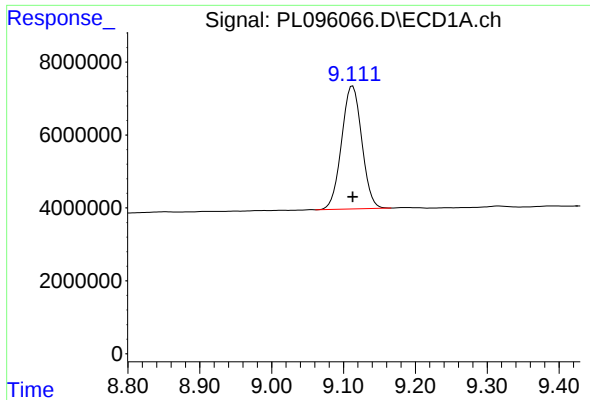

#28 Decachlorobiphenyl


R.T.: 9.113 min

Delta R.T.: 0.000 min

Response: 65640074

Conc: 25.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

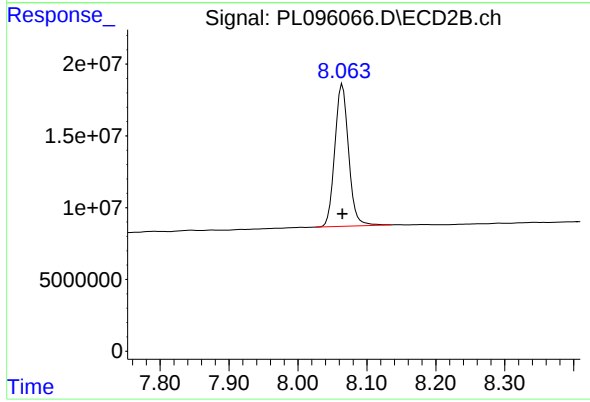

#28 Decachlorobiphenyl

R.T.: 8.064 min

Delta R.T.: 0.000 min

Response: 137703853

Conc: 24.90 ng/ml