

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
 Data File : PL096081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 18:05
 Operator : AR\AJ
 Sample : Q2336-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WBR-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 06:29:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.881	76432092	87375390	21.004	18.422
28)	SA Decachlor...	9.114	8.065	50155646	107.9E6	17.515	17.898
Target Compounds							
9)	A Endosulfan I	6.122f	5.254f	4923957	20965453	1.146	3.270 #
10)	B gamma-Chl...	0.000	5.142f	0	15306934	N.D.	2.301 #
11)	B alpha-Chl...	6.058	0.000	8750733	0	1.890	N.D. #
13)	MA Dieldrin	0.000	5.500	0	16485947	N.D.	2.513 #
15)	B Endosulfa...	0.000	6.072	0	3175771	N.D.	0.534 #
20)	A Methoxychlor	0.000	6.777f	0	5827287	N.D.	1.776 #
23)	Chlordane-1	0.000	3.898	0	7330937	N.D.	31.782 #
25)	Chlordane-3	0.000	5.142f	0	15306934	N.D.	19.107 #
26)	Chlordane-4	6.058	0.000	8750733	0	8.811	N.D. #
27)	Chlordane-5	0.000	6.072	0	3175771	N.D.	10.393 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
Data File : PL096081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 18:05
Operator : AR\AJ
Sample : Q2336-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WBR-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 06:29:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

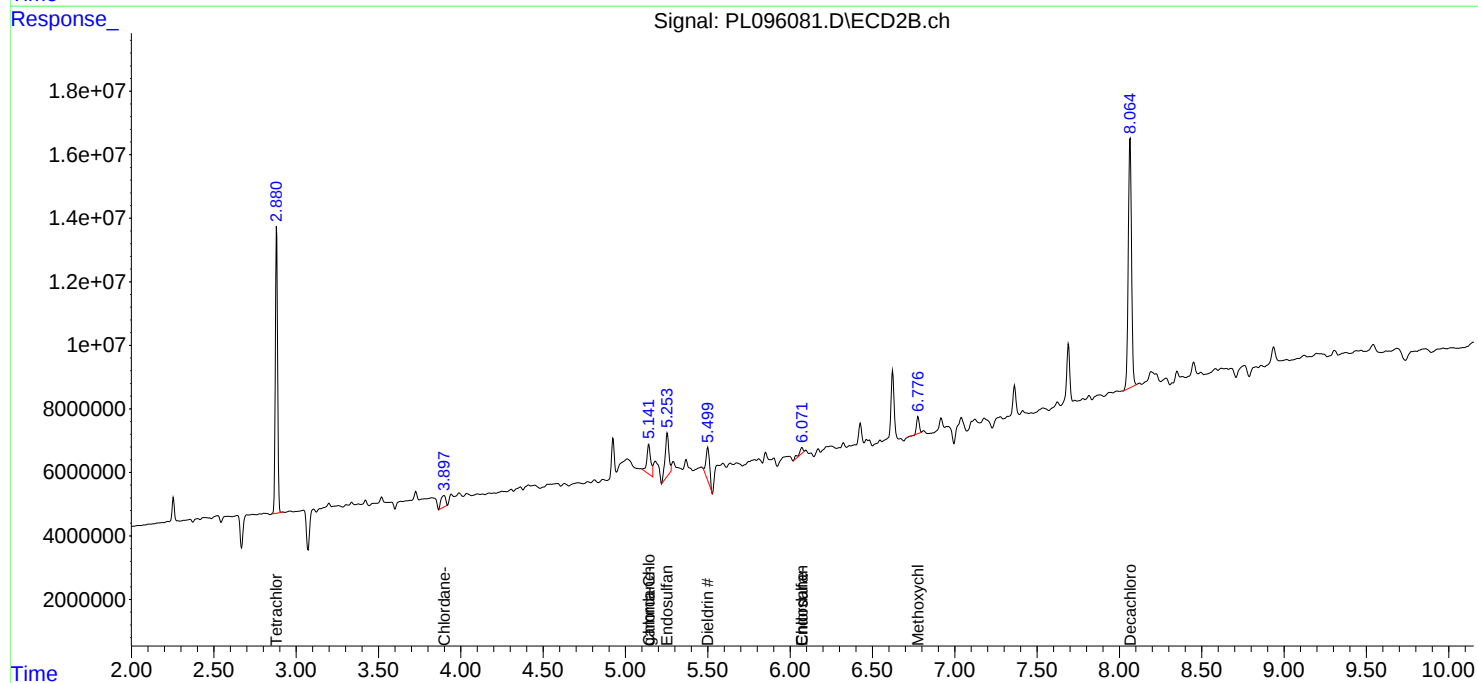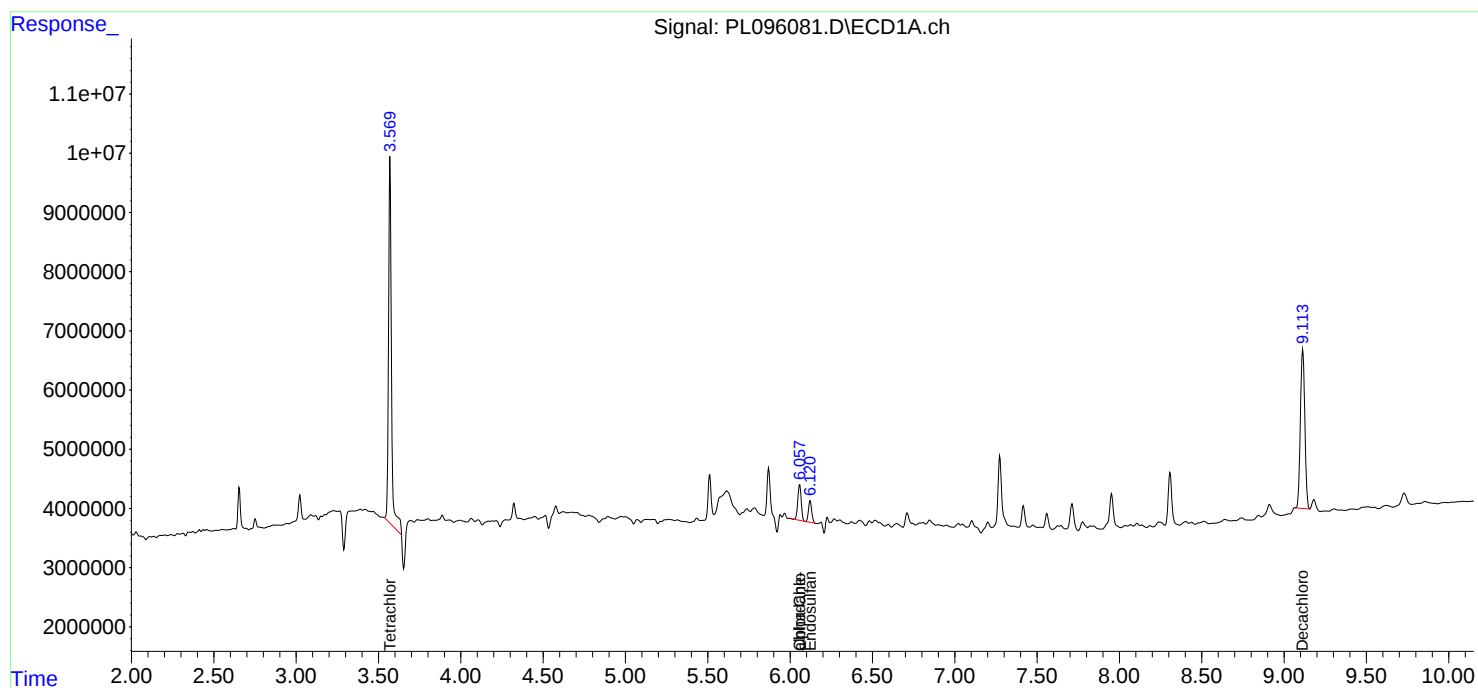


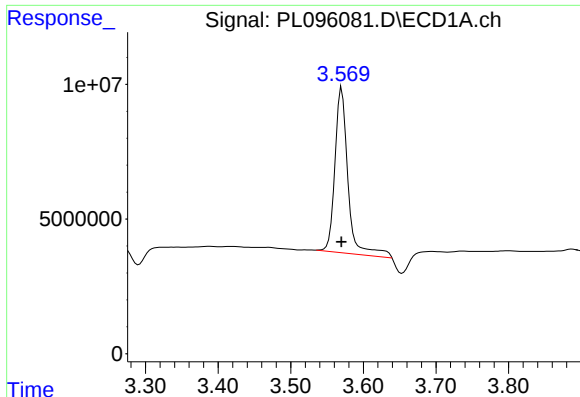

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 76432092
Conc: 21.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
WBR-1

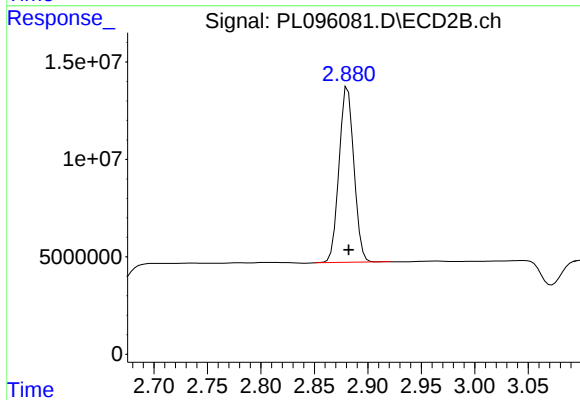


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 87375390
Conc: 18.42 ng/ml

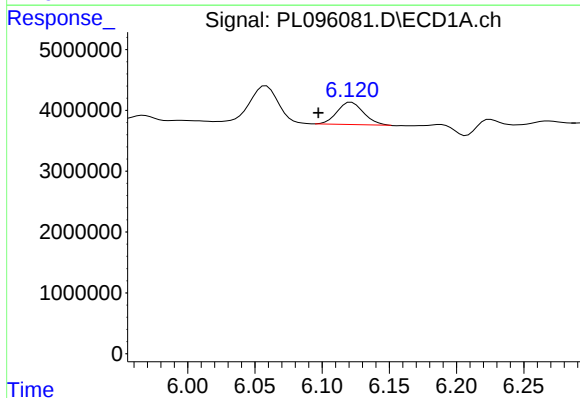


#9 Endosulfan I

R.T.: 6.122 min
Delta R.T.: 0.024 min
Response: 4923957
Conc: 1.15 ng/ml

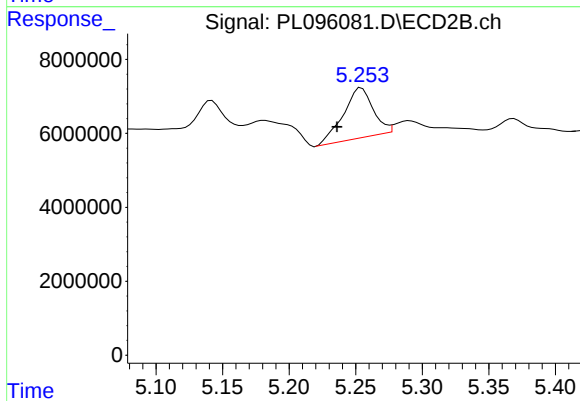

#9 Endosulfan I


R.T.: 5.254 min
Delta R.T.: 0.018 min
Response: 20965453
Conc: 3.27 ng/ml

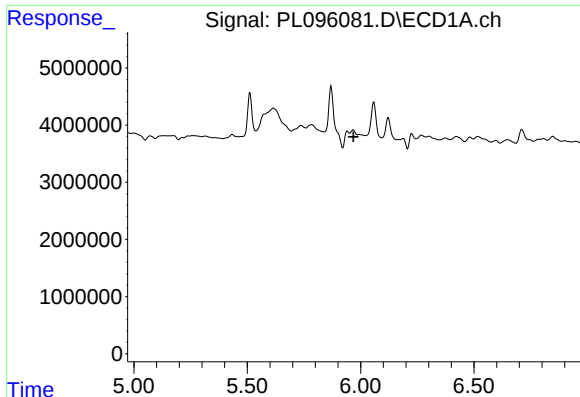

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WBR-1

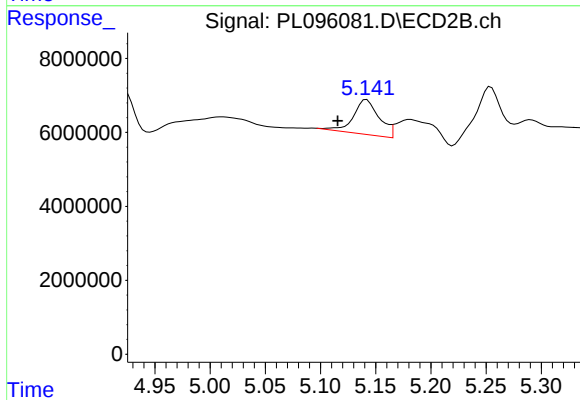


#10 gamma-Chlordane

R.T.: 5.142 min
Delta R.T.: 0.026 min
Response: 15306934
Conc: 2.30 ng/ml

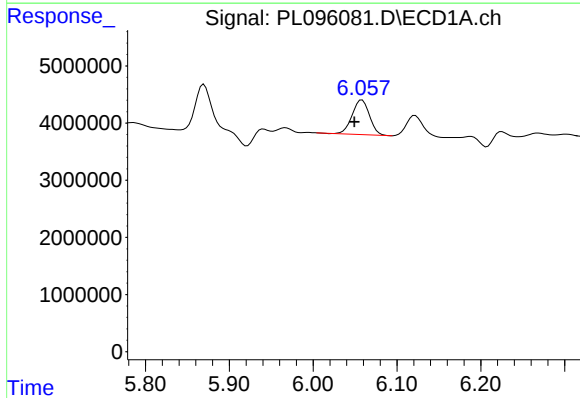


#11 alpha-Chlordane

R.T.: 6.058 min
Delta R.T.: 0.009 min
Response: 8750733
Conc: 1.89 ng/ml

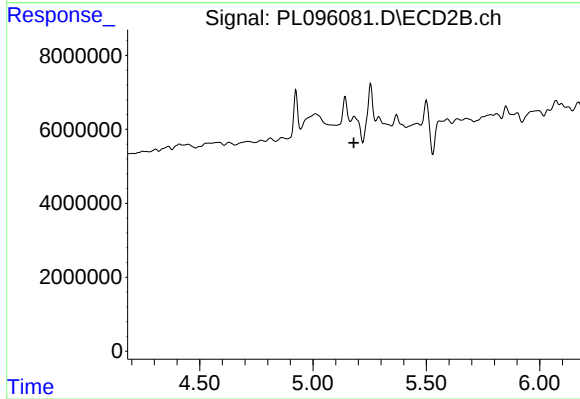

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.180 min
Response: 0
Conc: N.D.

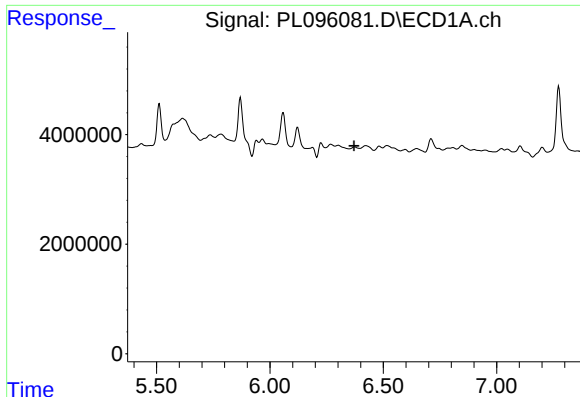

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WBR-1

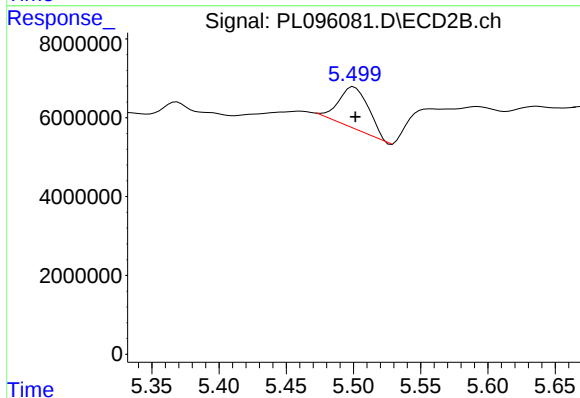


#13 Dieldrin

R.T.: 5.500 min
Delta R.T.: -0.001 min
Response: 16485947
Conc: 2.51 ng/ml

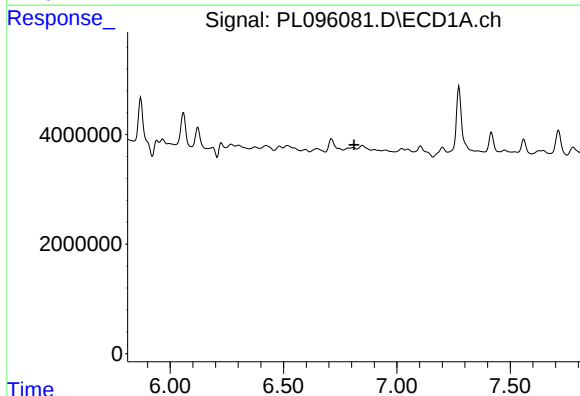


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.812 min
Response: 0
Conc: N.D.

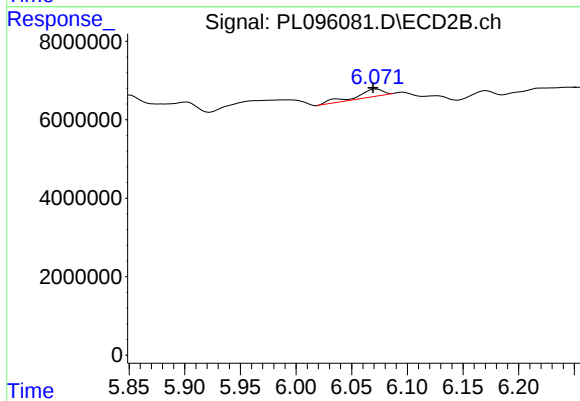

#15 Endosulfan II


R.T.: 6.072 min
Delta R.T.: 0.003 min
Response: 3175771
Conc: 0.53 ng/ml

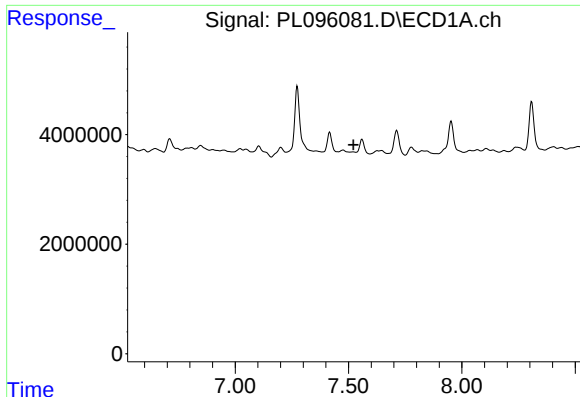

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WBR-1

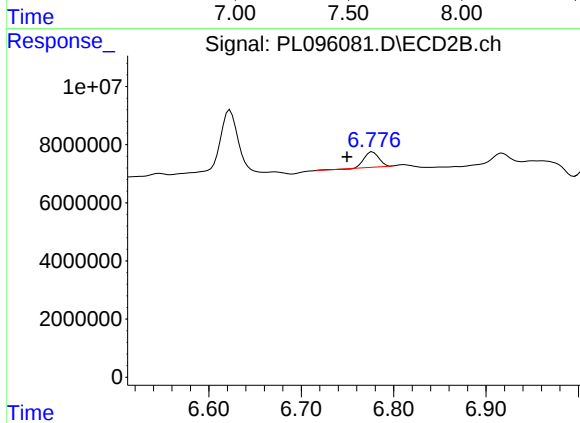


#20 Methoxychlor

R.T.: 6.777 min
Delta R.T.: 0.028 min
Response: 5827287
Conc: 1.78 ng/ml

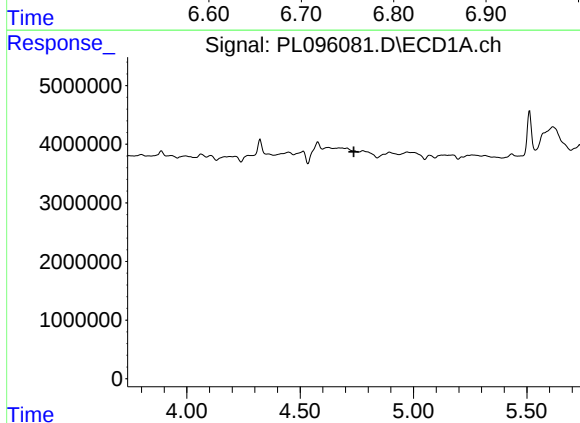


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.737 min
Response: 0
Conc: N.D.

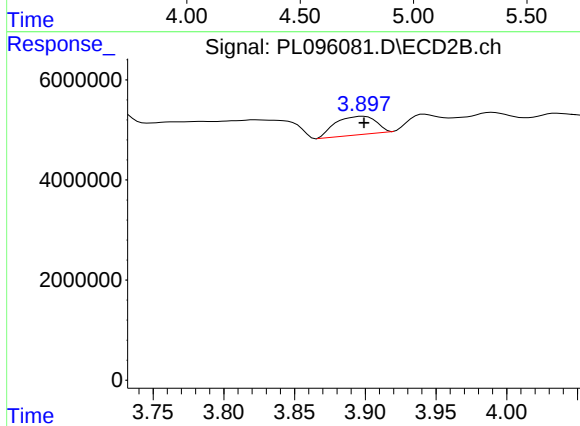

#23 Chlordane-1


R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 7330937
Conc: 31.78 ng/ml

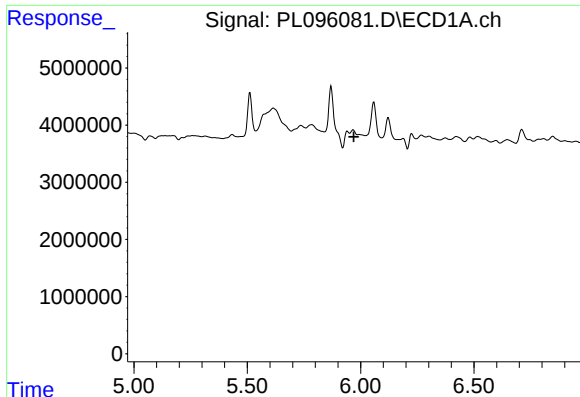

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WBR-1

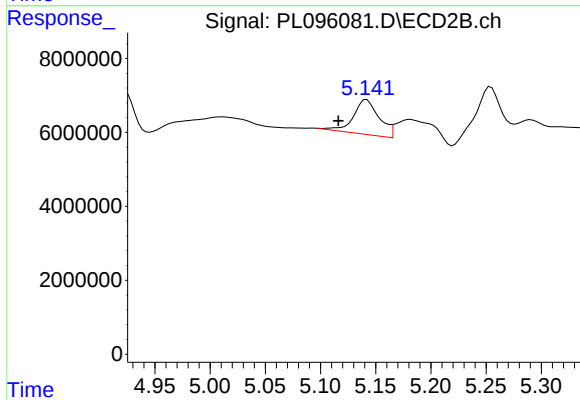


#25 Chlordane-3

R.T.: 5.142 min
Delta R.T.: 0.026 min
Response: 15306934
Conc: 19.11 ng/ml

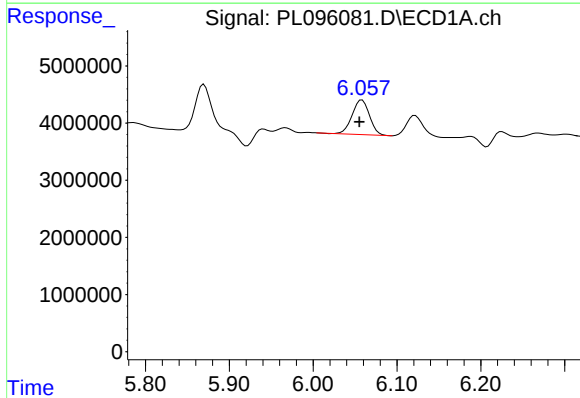


#26 Chlordane-4

R.T.: 6.058 min
Delta R.T.: 0.003 min
Response: 8750733
Conc: 8.81 ng/ml

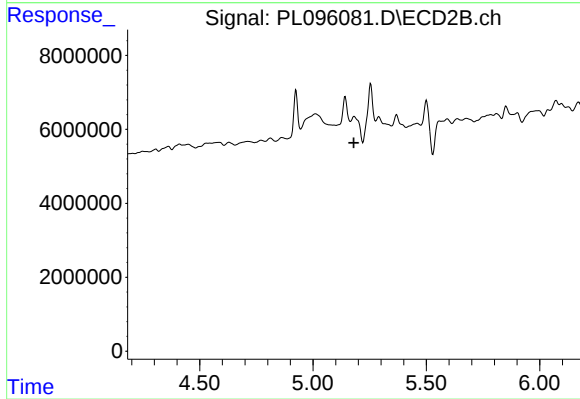

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.180 min
Response: 0
Conc: N.D.

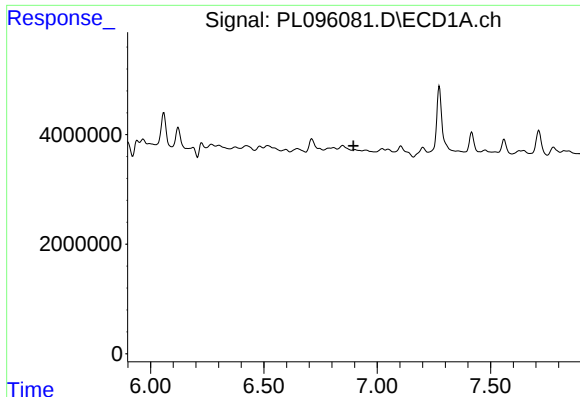

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.896 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WBR-1

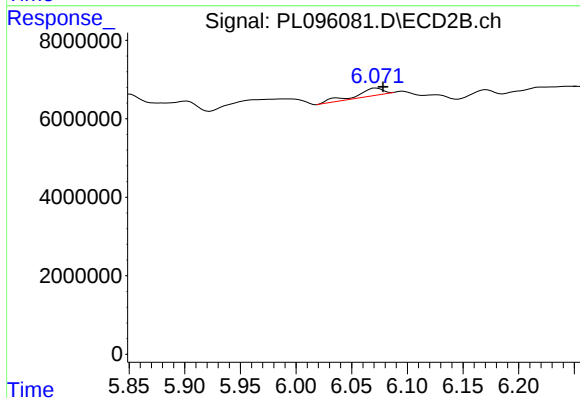


#27 Chlordane-5

R.T.: 6.072 min
Delta R.T.: -0.006 min
Response: 3175771
Conc: 10.39 ng/ml

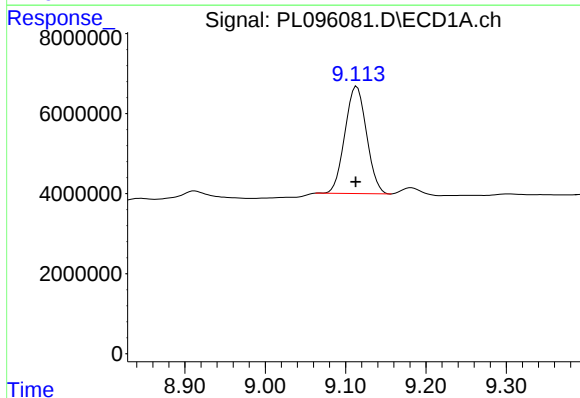

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.001 min
Response: 50155646
Conc: 17.51 ng/ml

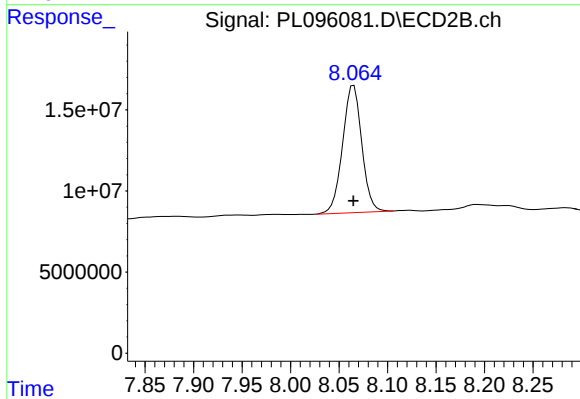

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 107879331
Conc: 17.90 ng/ml