

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
 Data File : PL096092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 20:35
 Operator : AR\AJ
 Sample : Q2341-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 06:31:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.881	74771917	94378106	20.548	19.898
28)	SA Decachlor...	9.113	8.064	40772173	60547916	14.238	10.045 #
Target Compounds							
9)	A Endosulfan I	0.000	5.250	0	6357570	N.D.	0.991 #
23)	Chlordane-1	0.000	3.893	0	14902296	N.D.	64.607 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
Data File : PL096092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 20:35
Operator : AR\AJ
Sample : Q2341-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 06:31:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

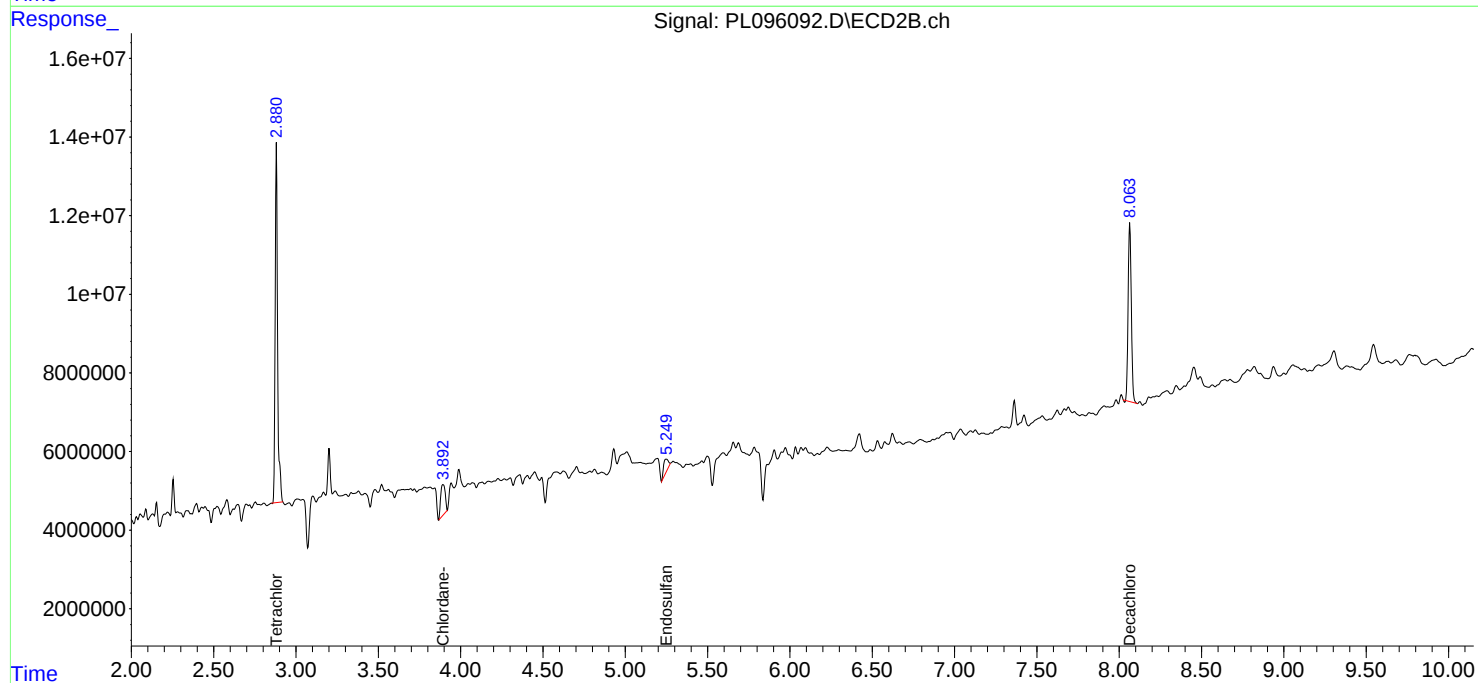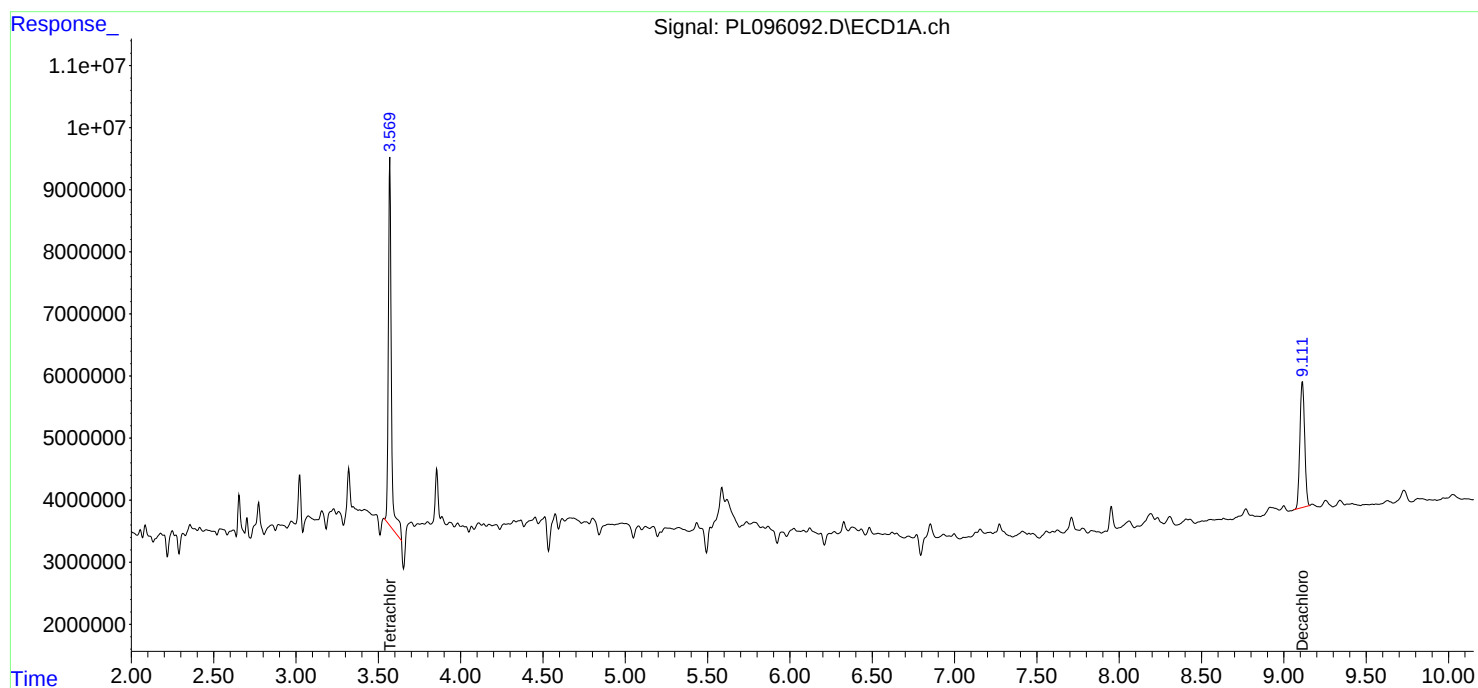


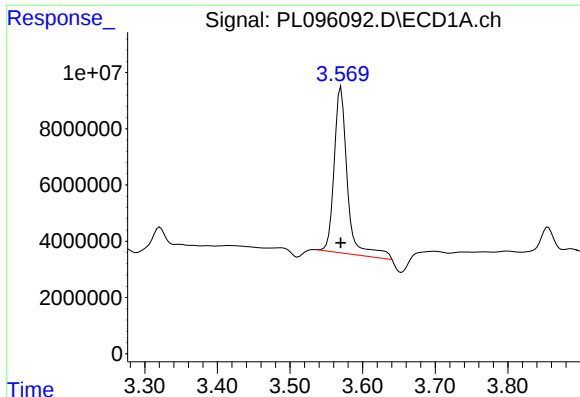

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 74771917
Conc: 20.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
EP-3

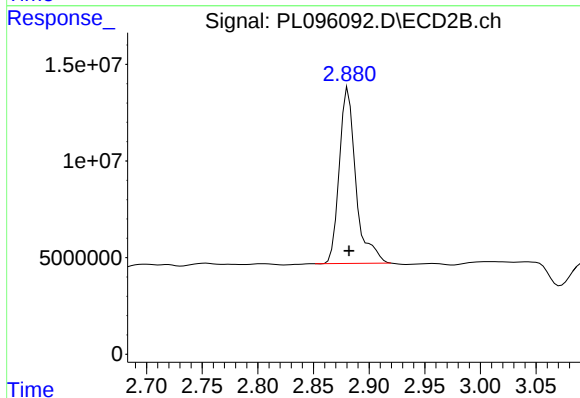


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 94378106
Conc: 19.90 ng/ml

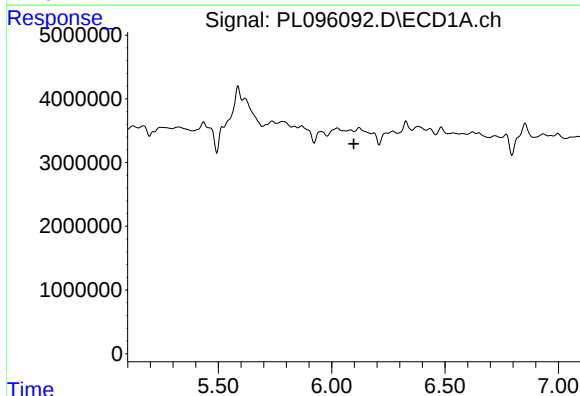


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

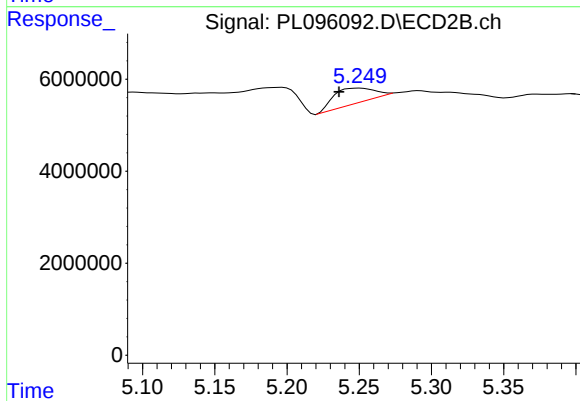

#9 Endosulfan I


R.T.: 5.250 min
Delta R.T.: 0.014 min
Response: 6357570
Conc: 0.99 ng/ml

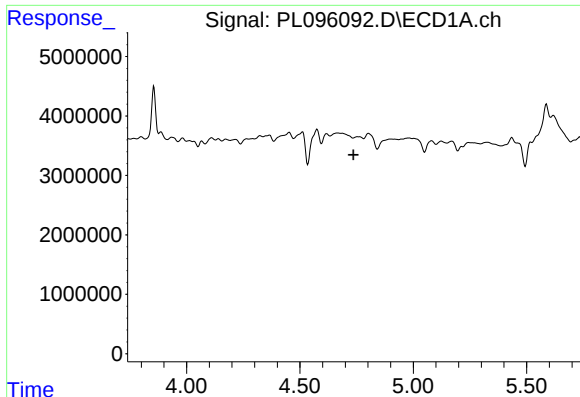

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EP-3

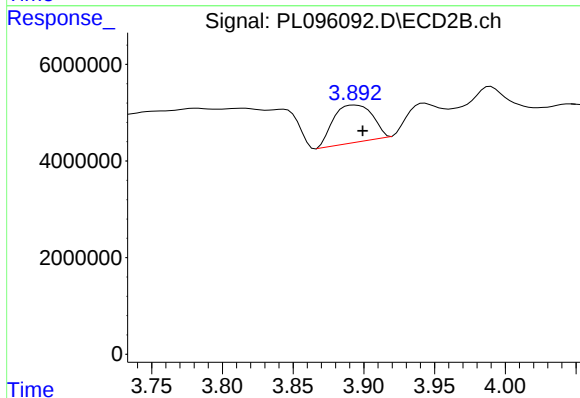


#23 Chlordane-1

R.T.: 3.893 min
Delta R.T.: -0.006 min
Response: 14902296
Conc: 64.61 ng/ml

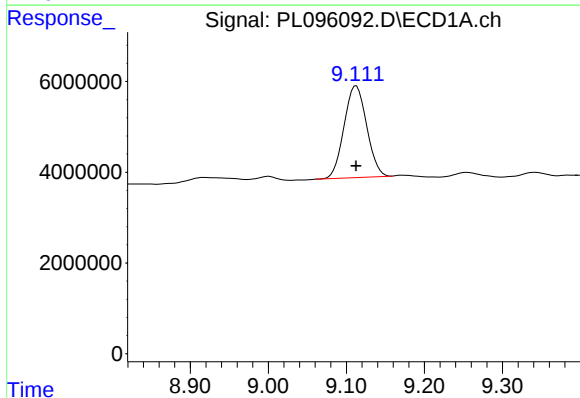

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 40772173
Conc: 14.24 ng/ml

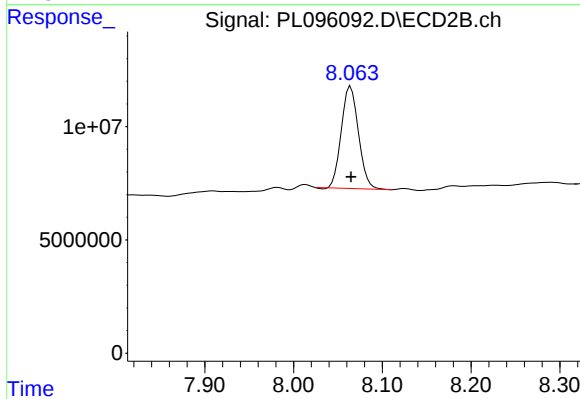

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 60547916
Conc: 10.05 ng/ml