

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
 Data File : PL096063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 14:00
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 15:02:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 14:59:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.881	336.2E6	582.1E6	100.436	100.922
28)	SA Decachlor...	9.112	8.065	253.6E6	556.1E6	99.262	99.970
Target Compounds							
23)	Chlordane-1	4.737	3.899	203.2E6	233.2E6	1008.240	1015.786
24)	Chlordane-2	5.264	4.480	210.0E6	258.9E6	1000.843	1001.900
25)	Chlordane-3	5.970	5.116	848.9E6	835.0E6	1014.545	1016.730
26)	Chlordane-4	6.055	5.180	997.8E6	724.2E6	1014.179	1015.664
27)	Chlordane-5	6.896	6.078	174.1E6	312.0E6	1004.800	1019.351



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
Data File : PL096063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 14:00
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 15:02:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 14:59:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

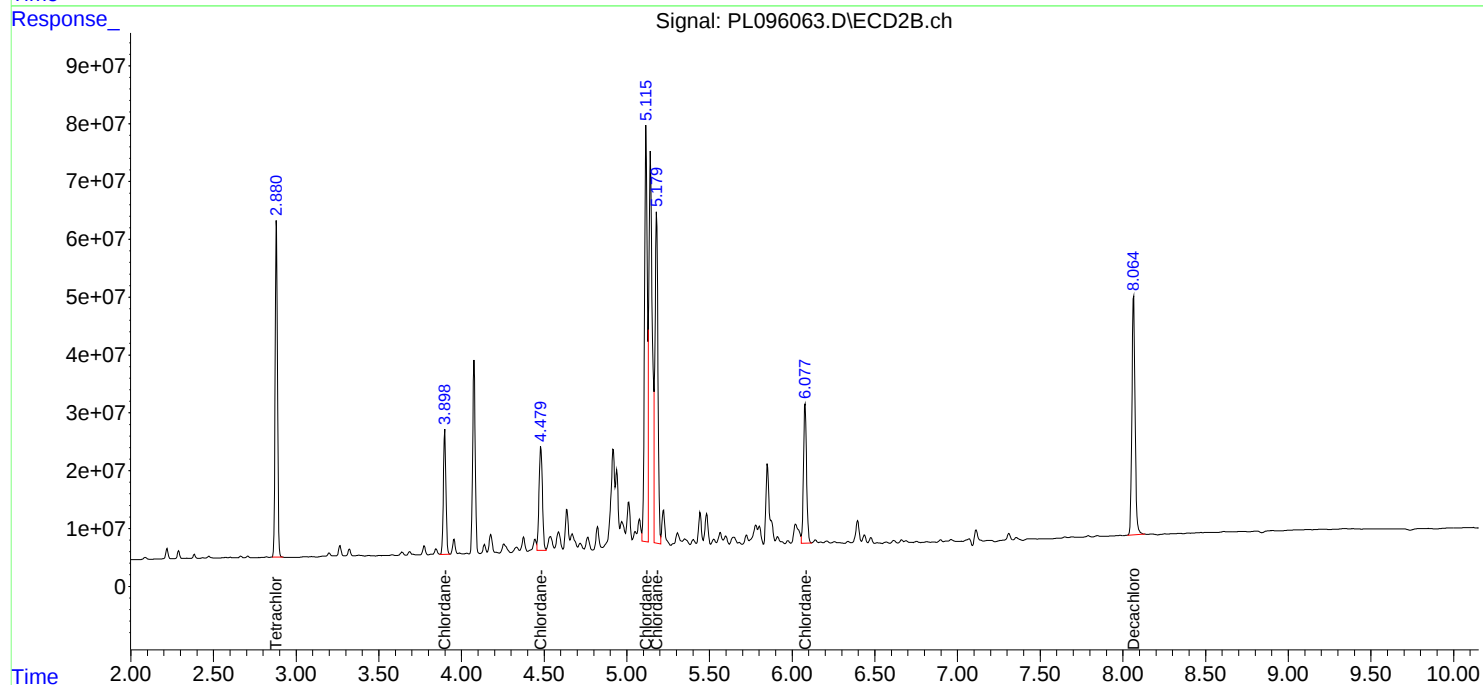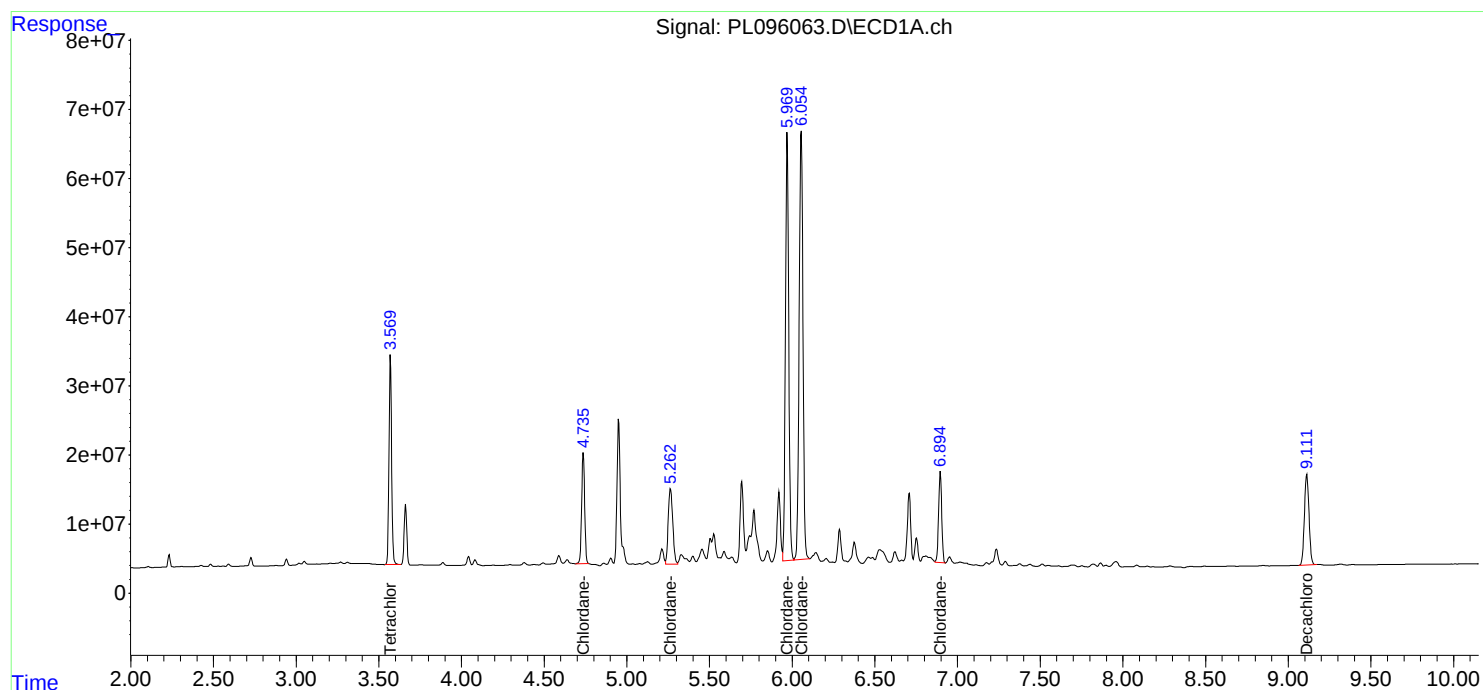


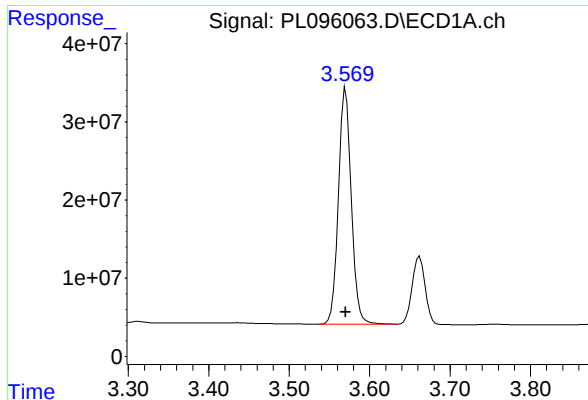

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 336206080
Conc: 100.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

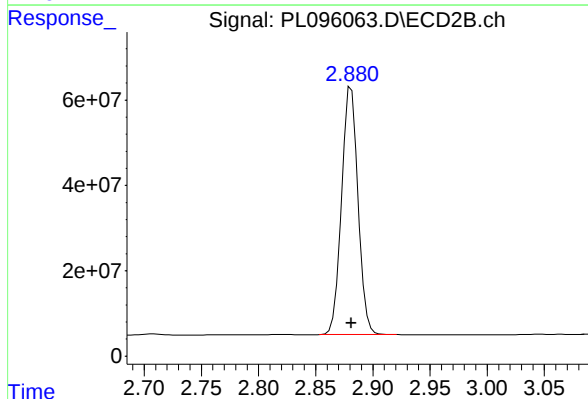


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 582070041
Conc: 100.92 ng/ml

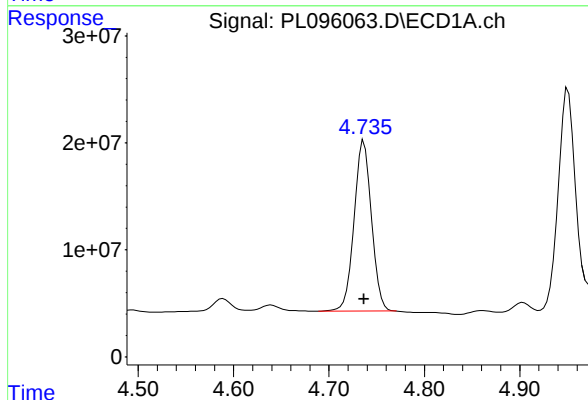


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 203214142
Conc: 1008.24 ng/ml

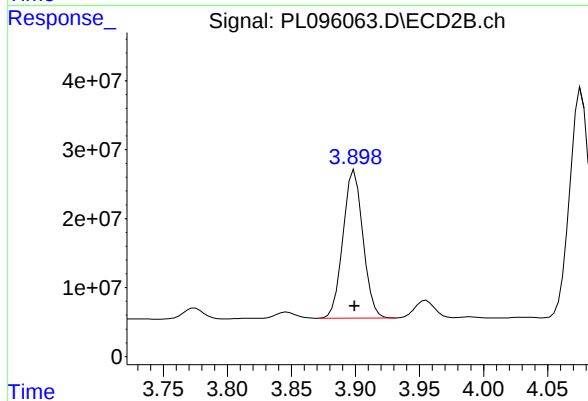

#23 Chlordane-1


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 233244957
Conc: 1015.79 ng/ml

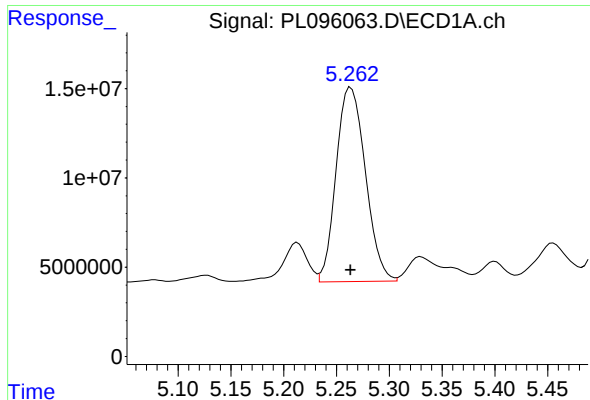

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 209966786
Conc: 1000.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

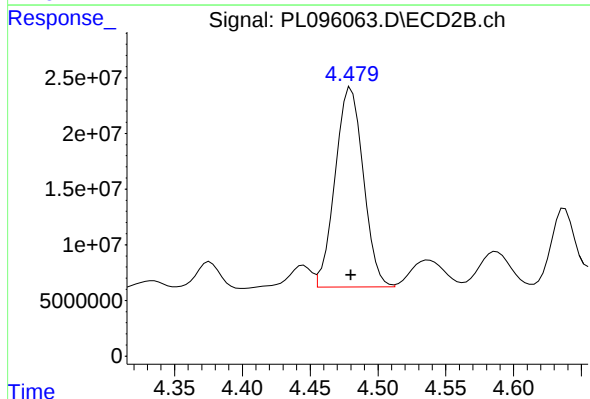


#24 Chlordane-2

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 258876396
Conc: 1001.90 ng/ml

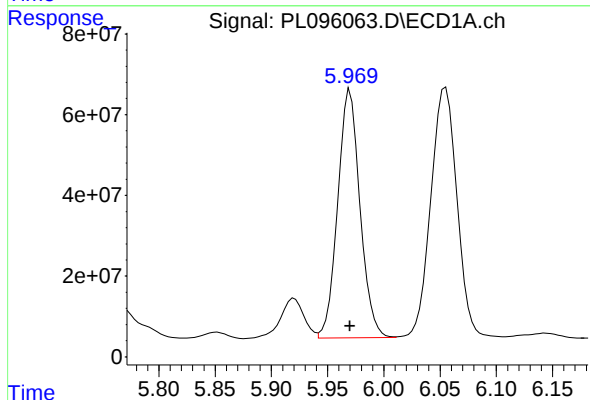


#25 Chlordane-3

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 848894482
Conc: 1014.54 ng/ml

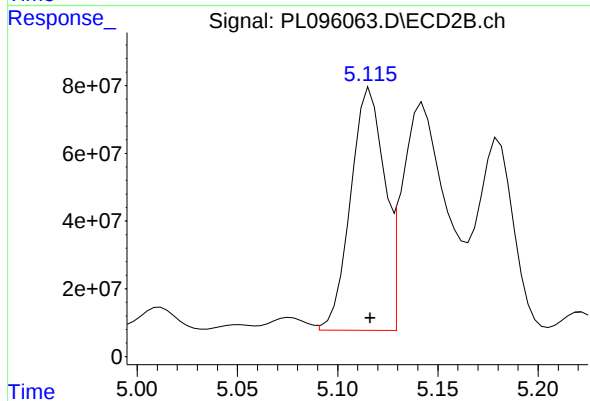

#25 Chlordane-3


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 835013272
Conc: 1016.73 ng/ml

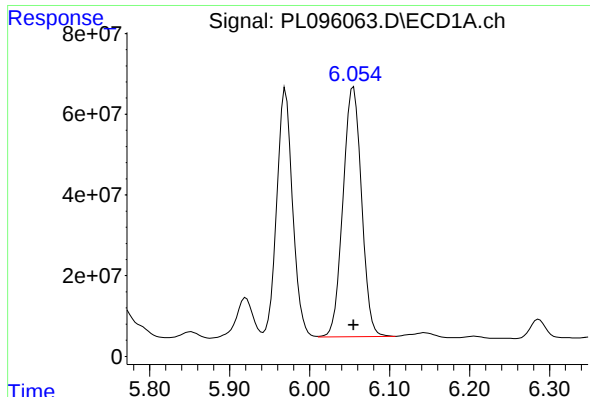

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 997811374
Conc: 1014.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

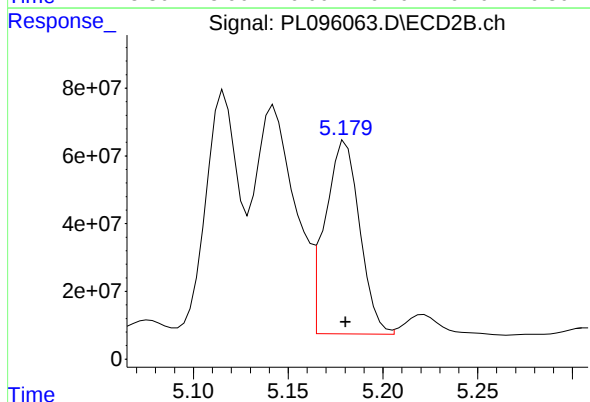


#26 Chlordane-4

R.T.: 5.180 min
Delta R.T.: 0.000 min
Response: 724215085
Conc: 1015.66 ng/ml

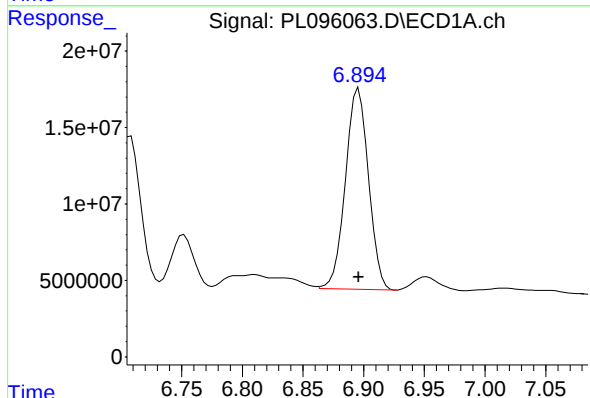


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 174063280
Conc: 1004.80 ng/ml

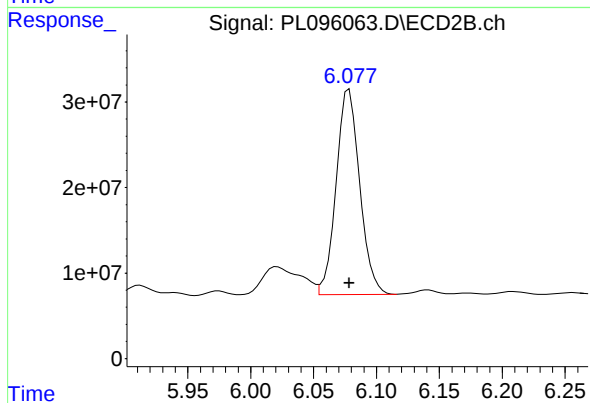

#27 Chlordane-5


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 312019098
Conc: 1019.35 ng/ml

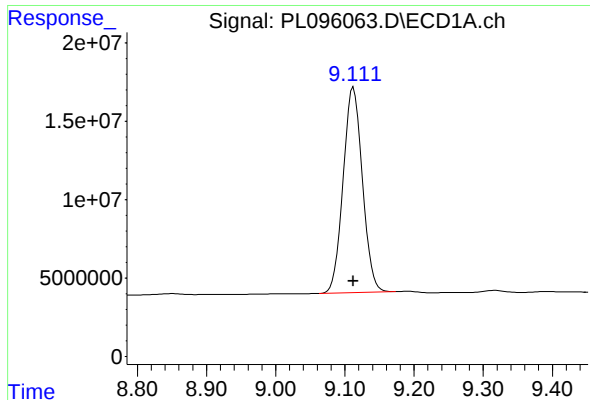

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 253629332
Conc: 99.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

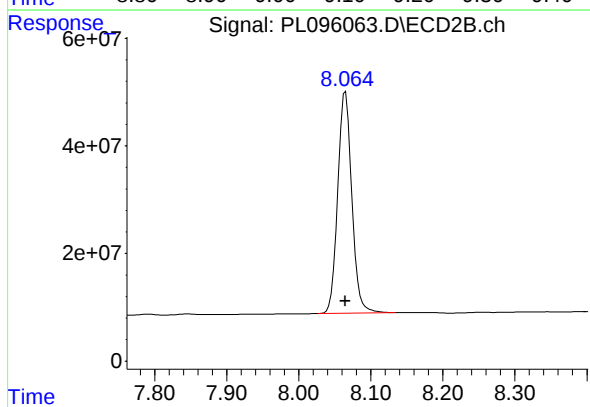

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 556050975
Conc: 99.97 ng/ml